

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061325\
 Data File : PP072909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2025 12:44
 Operator : YP\AJ
 Sample : Q2301-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-URBAN-FILL-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/16/2025
 Supervised By :mohammad ahmed 06/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 15:07:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.495	3.791	28031930	30371696	13.941m	19.002 #
2) SA Decachlor...	10.190	8.802	20628882	17158810	12.663m	16.209m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061325\
Data File : PP072909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2025 12:44
Operator : YP\AJ
Sample : Q2301-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-URBAN-FILL-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/16/2025
Supervised By :mohammad ahmed 06/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 15:07:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

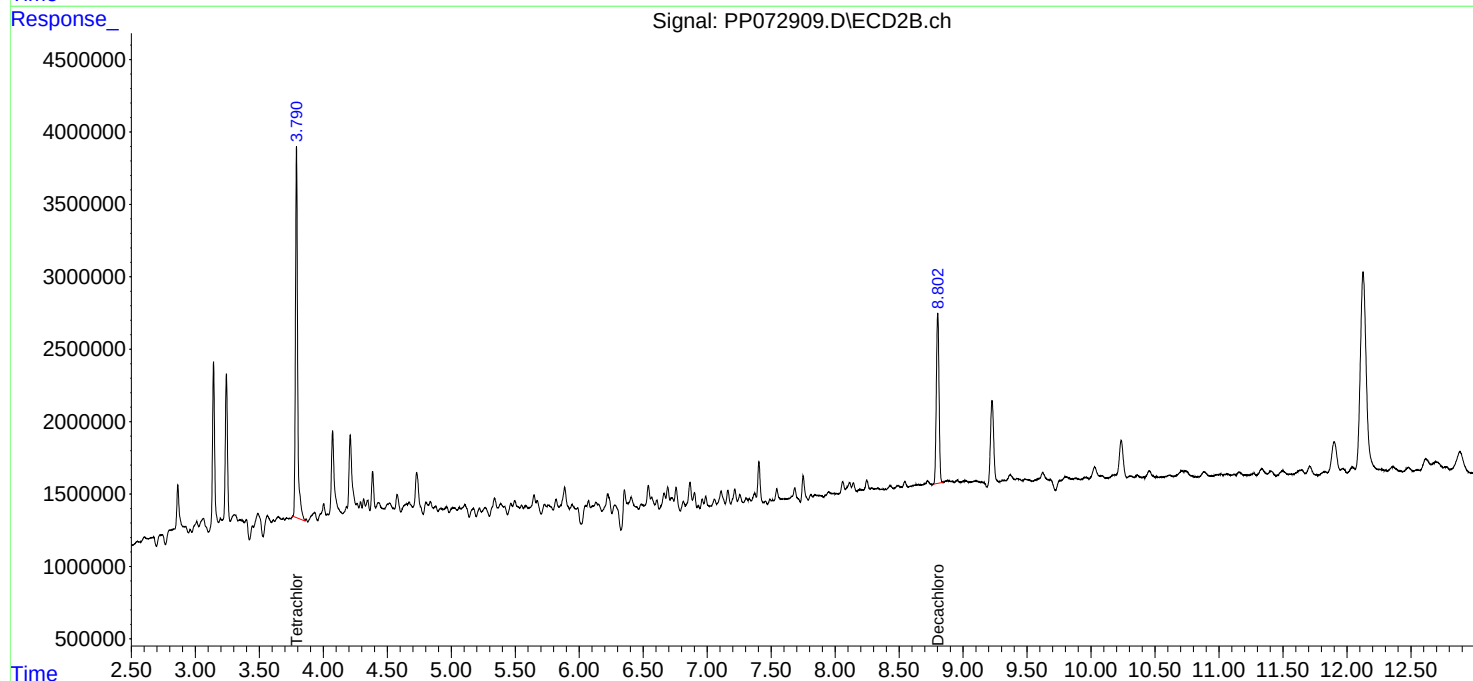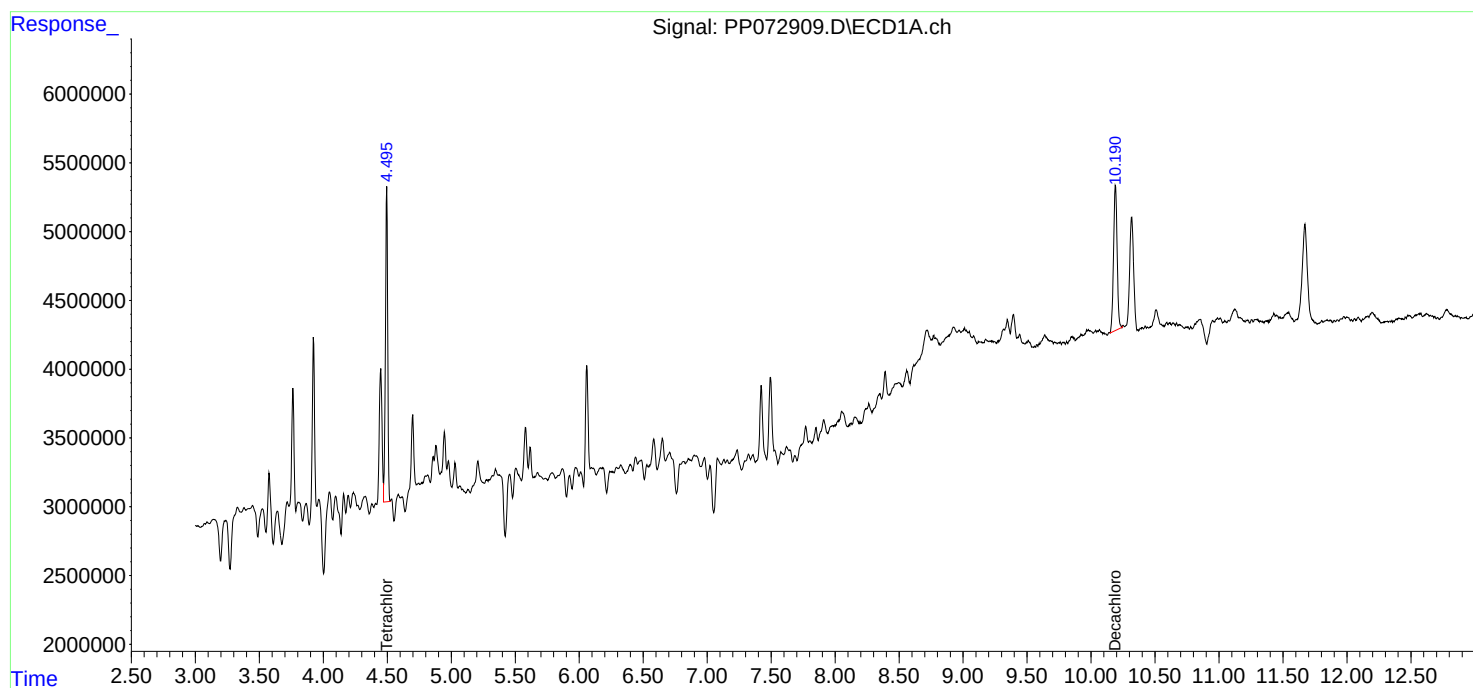

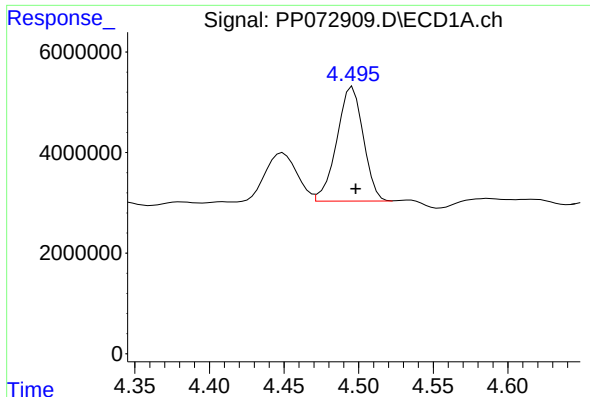


#1 Tetrachloro-m-xylene

R.T.: 4.495 min
Delta R.T.: -0.003 min
Response: 28031930
Conc: 13.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-URBAN-FILL-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/16/2025
Supervised By :mohammad ahmed 06/17/2025

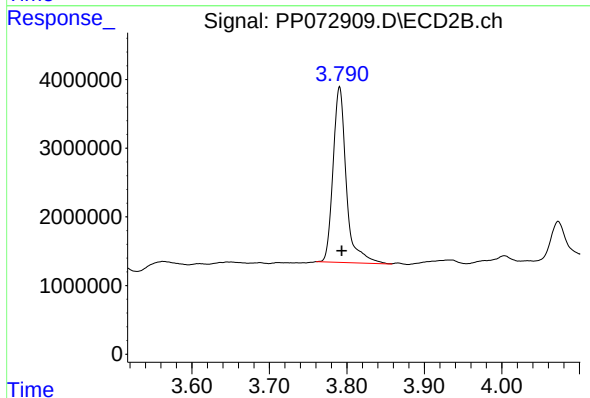


#1 Tetrachloro-m-xylene

R.T.: 3.791 min
Delta R.T.: -0.003 min
Response: 30371696
Conc: 19.00 ng/ml

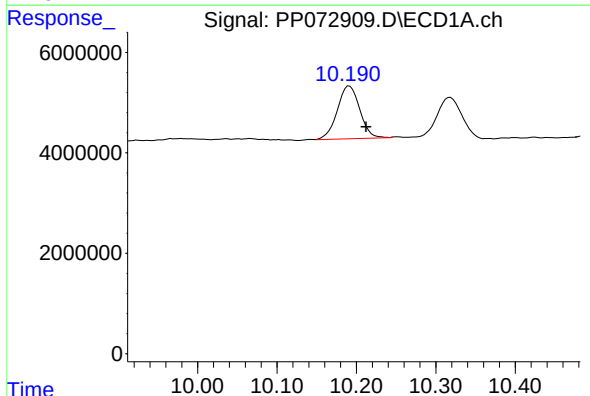

#2 Decachlorobiphenyl

R.T.: 10.190 min
Delta R.T.: -0.022 min
Response: 20628882
Conc: 12.66 ng/ml m

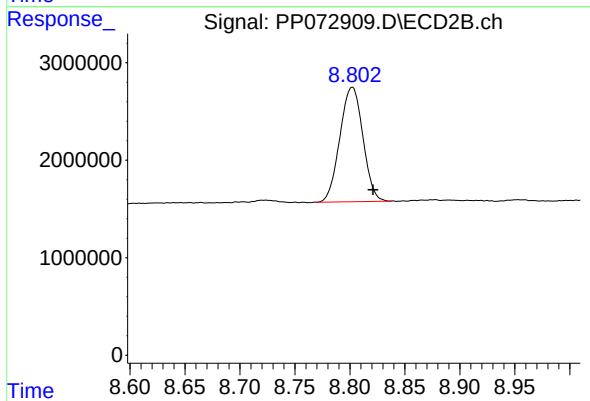

#2 Decachlorobiphenyl

R.T.: 8.802 min
Delta R.T.: -0.019 min
Response: 17158810
Conc: 16.21 ng/ml m