

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061325\
 Data File : PP072938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2025 22:30
 Operator : YP\AJ
 Sample : Q2326-04 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC274770-2-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/16/2025
 Supervised By :mohammad ahmed 06/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 01:20:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.497	3.791	3172051	2721358	1.578	1.703
2) SA Decachlor...	10.192	8.802	2573576	2153333	1.580m	2.034m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061325\
Data File : PP072938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2025 22:30
Operator : YP\AJ
Sample : Q2326-04 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC274770-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/16/2025
Supervised By :mohammad ahmed 06/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 01:20:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

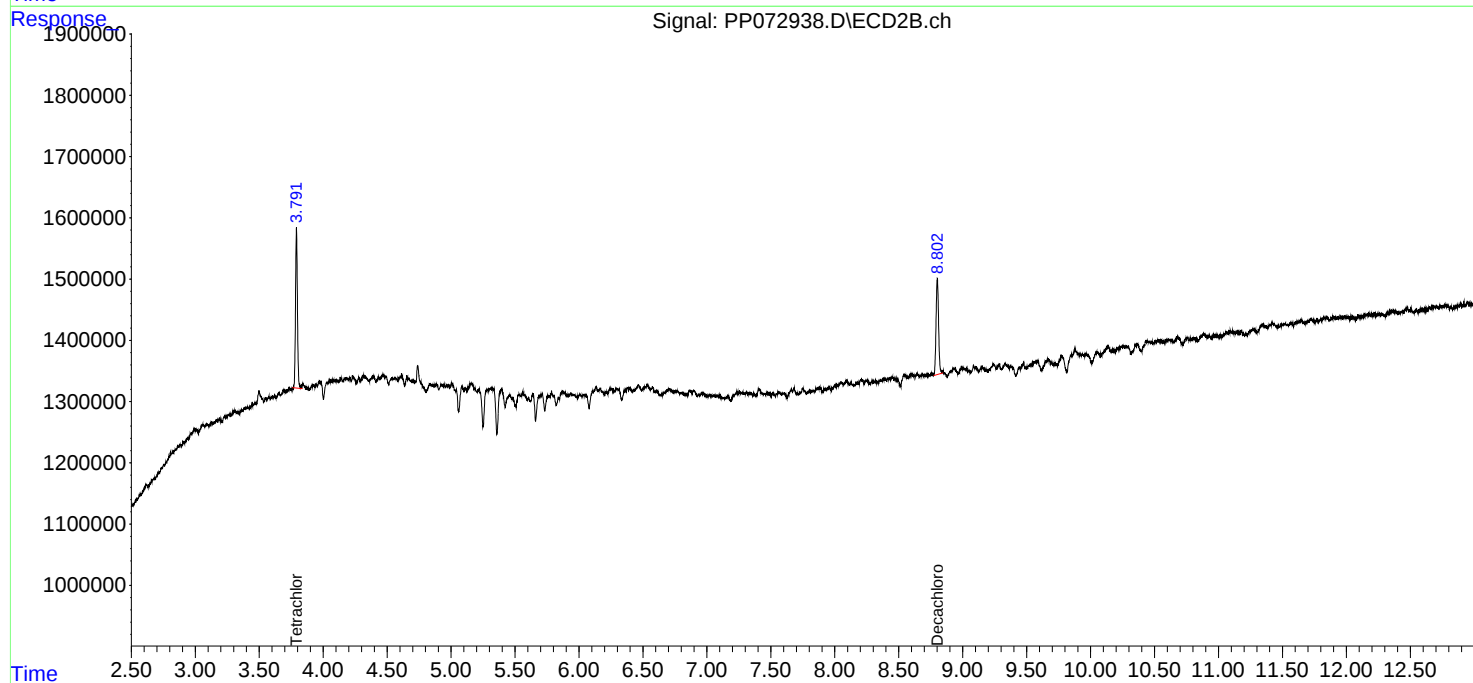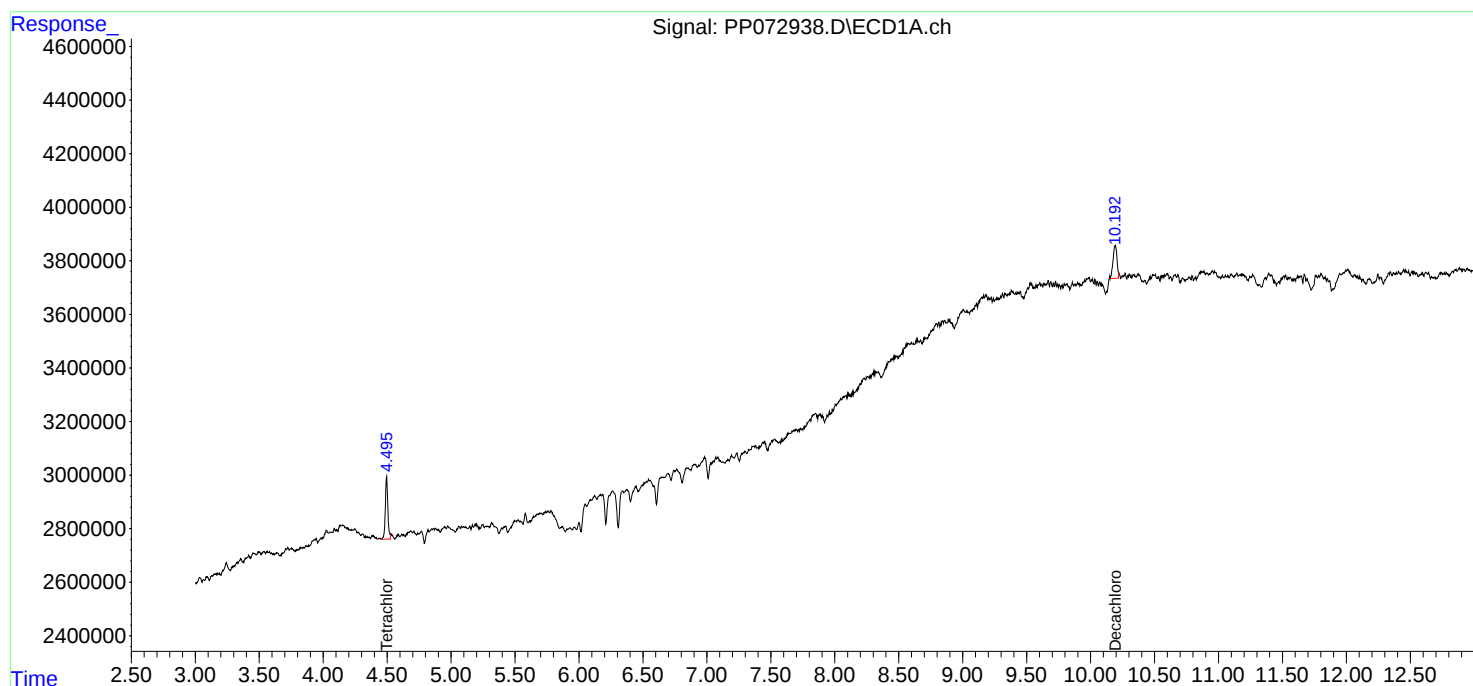

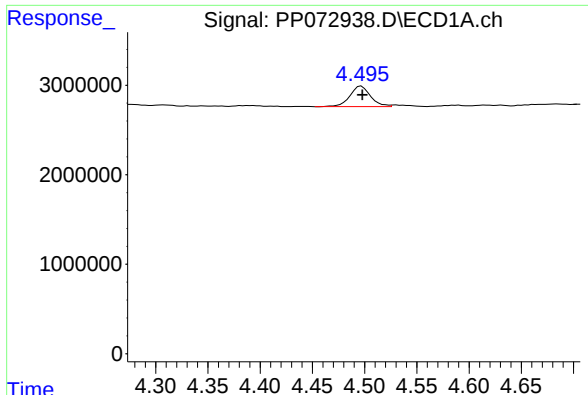

#1 Tetrachloro-m-xylene

R.T.: 4.497 min
Delta R.T.: -0.001 min
Response: 3172051
Conc: 1.58 ng/ml

Instrument :

ECD_P

ClientSampleId :


BC274770-2-2

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 06/16/2025

Supervised By :mohammad ahmed 06/17/2025

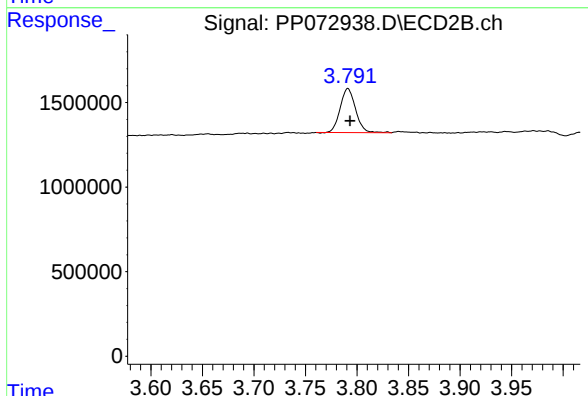


#1 Tetrachloro-m-xylene

R.T.: 3.791 min
Delta R.T.: -0.002 min
Response: 2721358
Conc: 1.70 ng/ml

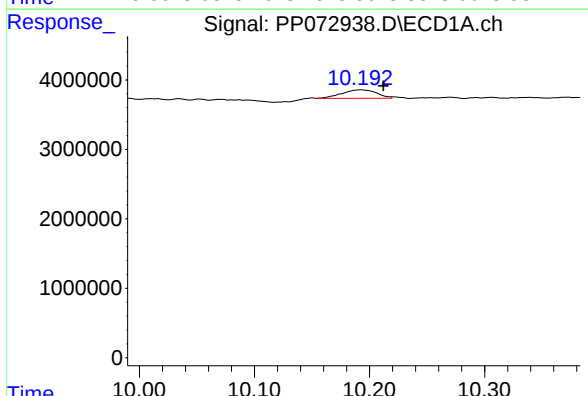

#2 Decachlorobiphenyl

R.T.: 10.192 min
Delta R.T.: -0.020 min
Response: 2573576
Conc: 1.58 ng/ml m

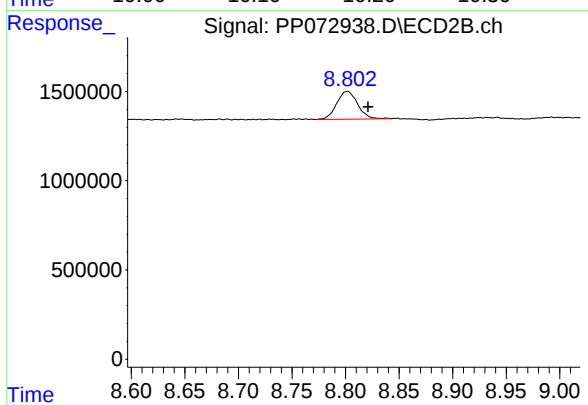

#2 Decachlorobiphenyl

R.T.: 8.802 min
Delta R.T.: -0.019 min
Response: 2153333
Conc: 2.03 ng/ml m