

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061325\
 Data File : PP072949.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2025 04:01
 Operator : YP\AJ
 Sample : Q2327-02 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEH700H-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/16/2025
 Supervised By :mohammad ahmed 06/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 04:43:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.494	3.791	2955648	3052212	1.470	1.910 #
2) SA Decachlor...	10.190	8.802	3445319	2194275	2.115m	2.073m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061325\
Data File : PP072949.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2025 04:01
Operator : YP\AJ
Sample : Q2327-02 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HEH700H-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/16/2025
Supervised By :mohammad ahmed 06/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 04:43:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

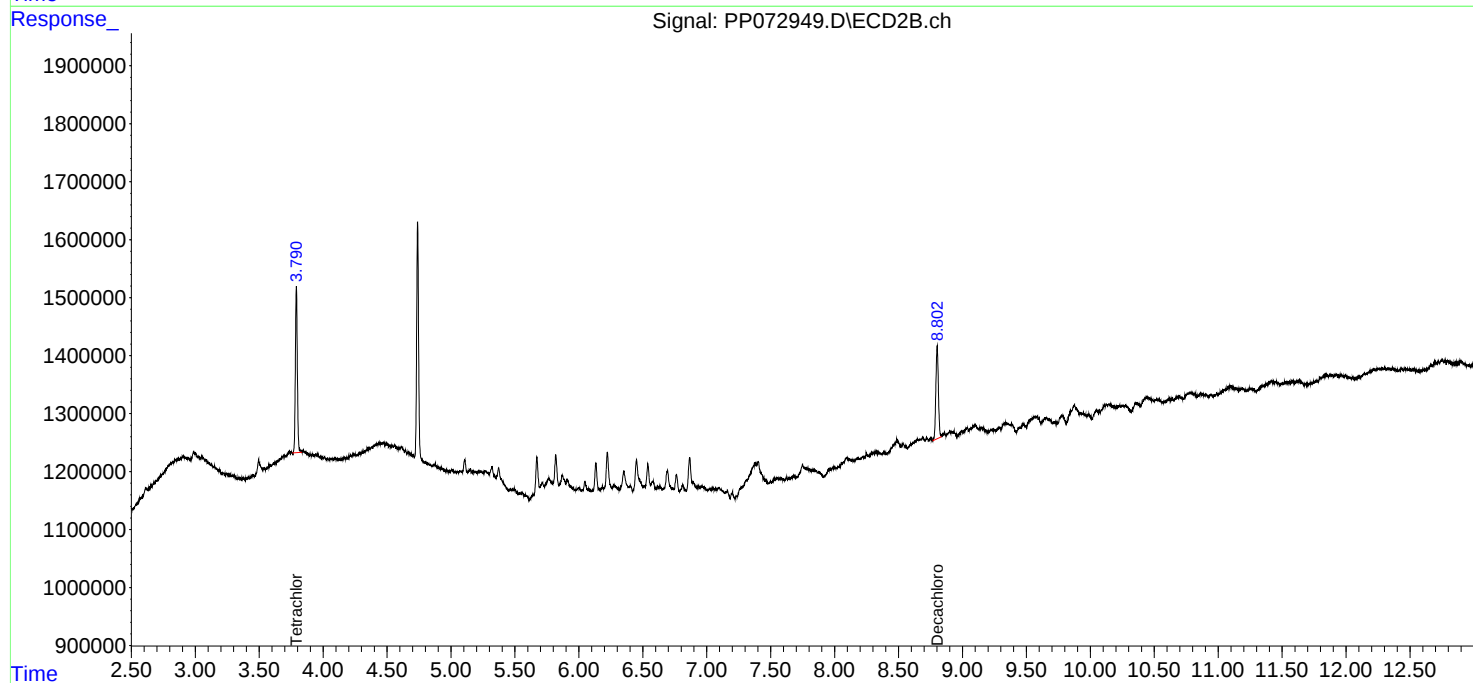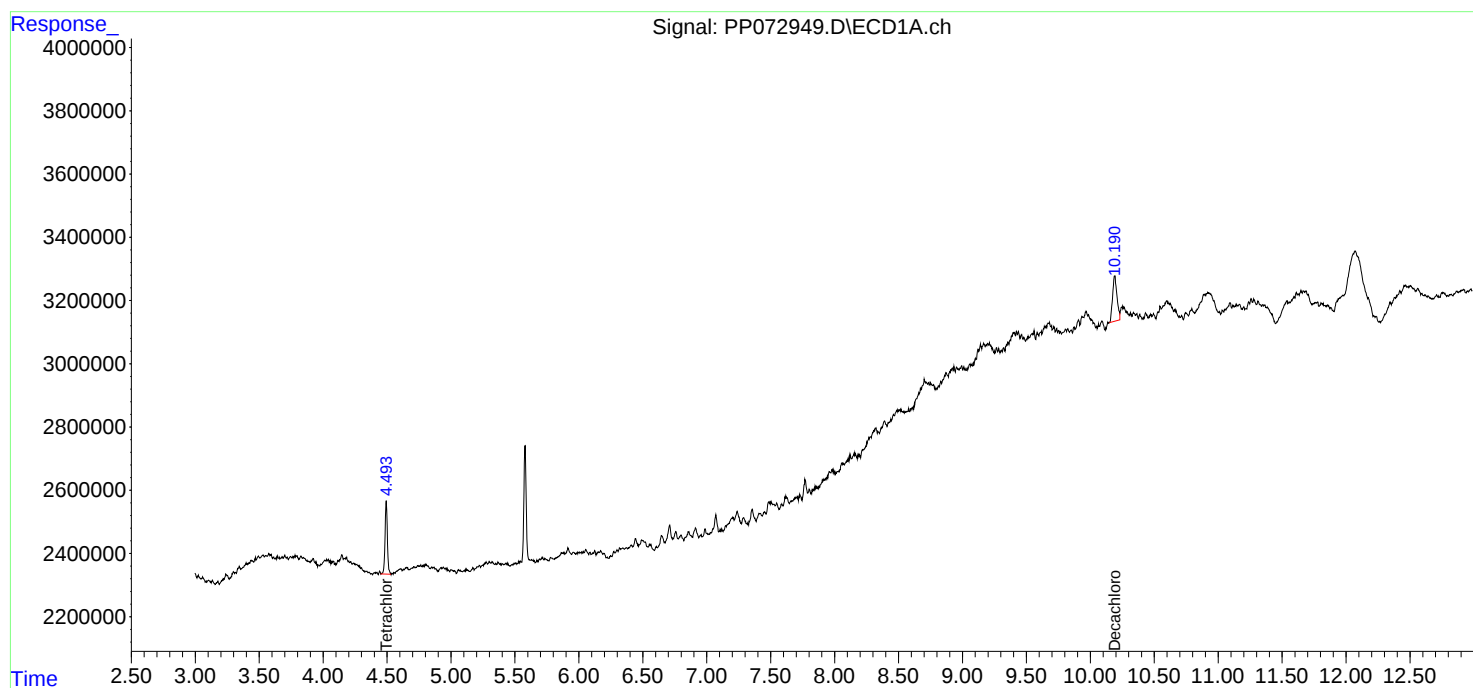

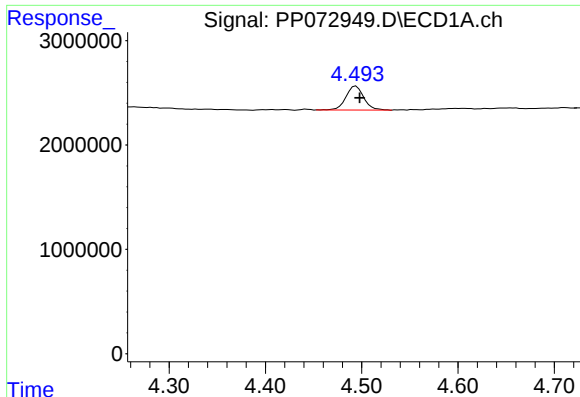


#1 Tetrachloro-m-xylene

R.T.: 4.494 min
Delta R.T.: -0.004 min
Response: 2955648
Conc: 1.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEH700H-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/16/2025
Supervised By :mohammad ahmed 06/17/2025

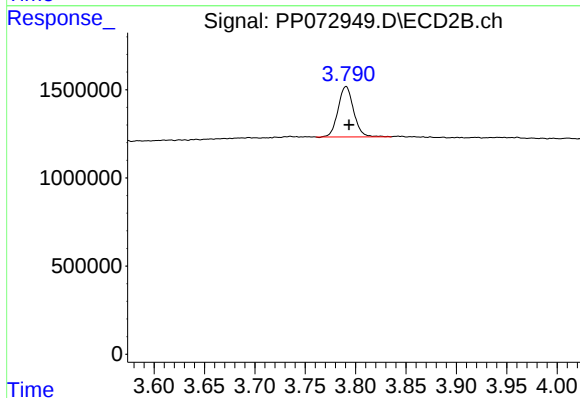


#1 Tetrachloro-m-xylene

R.T.: 3.791 min
Delta R.T.: -0.003 min
Response: 3052212
Conc: 1.91 ng/ml

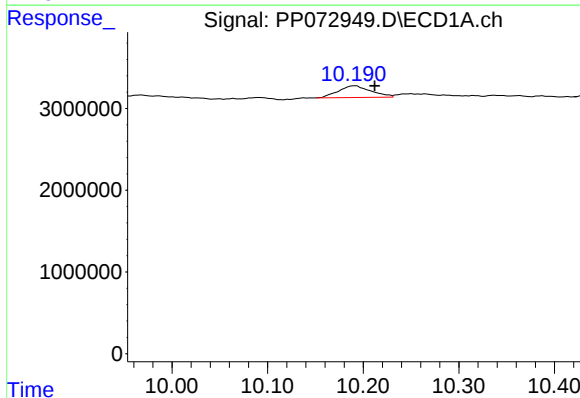

#2 Decachlorobiphenyl

R.T.: 10.190 min
Delta R.T.: -0.022 min
Response: 3445319
Conc: 2.11 ng/ml m

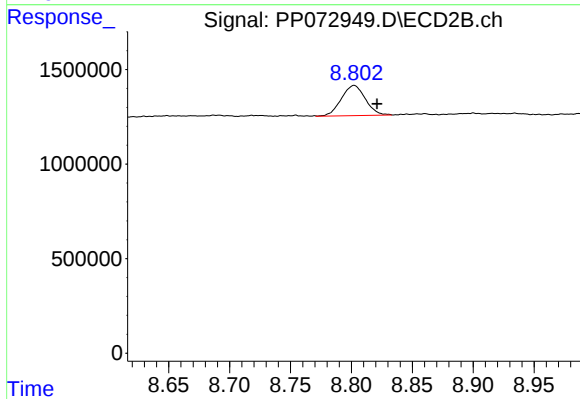

#2 Decachlorobiphenyl

R.T.: 8.802 min
Delta R.T.: -0.019 min
Response: 2194275
Conc: 2.07 ng/ml m