

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
 Data File : PP036432.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2021 9:07
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:34:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
20)	L4	AR-1242-5	7.263	6.115f	36487	37290	39.007 46.839
24)	L5	AR-1248-4	7.211	0.000	144546	0	88.289 N.D. #
25)	L5	AR-1248-5	7.263	6.115	36487	37290	22.900 34.064 #
26)	L6	AR-1254-1	7.211f	6.115f	144546	37290	87.802 22.895 #
28)	L6	AR-1254-3	7.834f	0.000	178000	0	64.132 N.D. #
32)	L7	AR-1260-2	8.266f	0.000	192459	0	82.634 N.D. #
35)	L7	AR-1260-5	9.148	0.000	18712	0	4.986 N.D. #
37)	L8	AR-1262-2	9.148f	0.000	18712	0	3.918 N.D. #
38)	L8	AR-1262-3	0.000	8.200f	0	38958	N.D. 22.739 #
41)	L9	AR-1268-1	0.000	8.200	0	38958	N.D. 8.438 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
Data File : PP036432.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2021 9:07
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:34:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

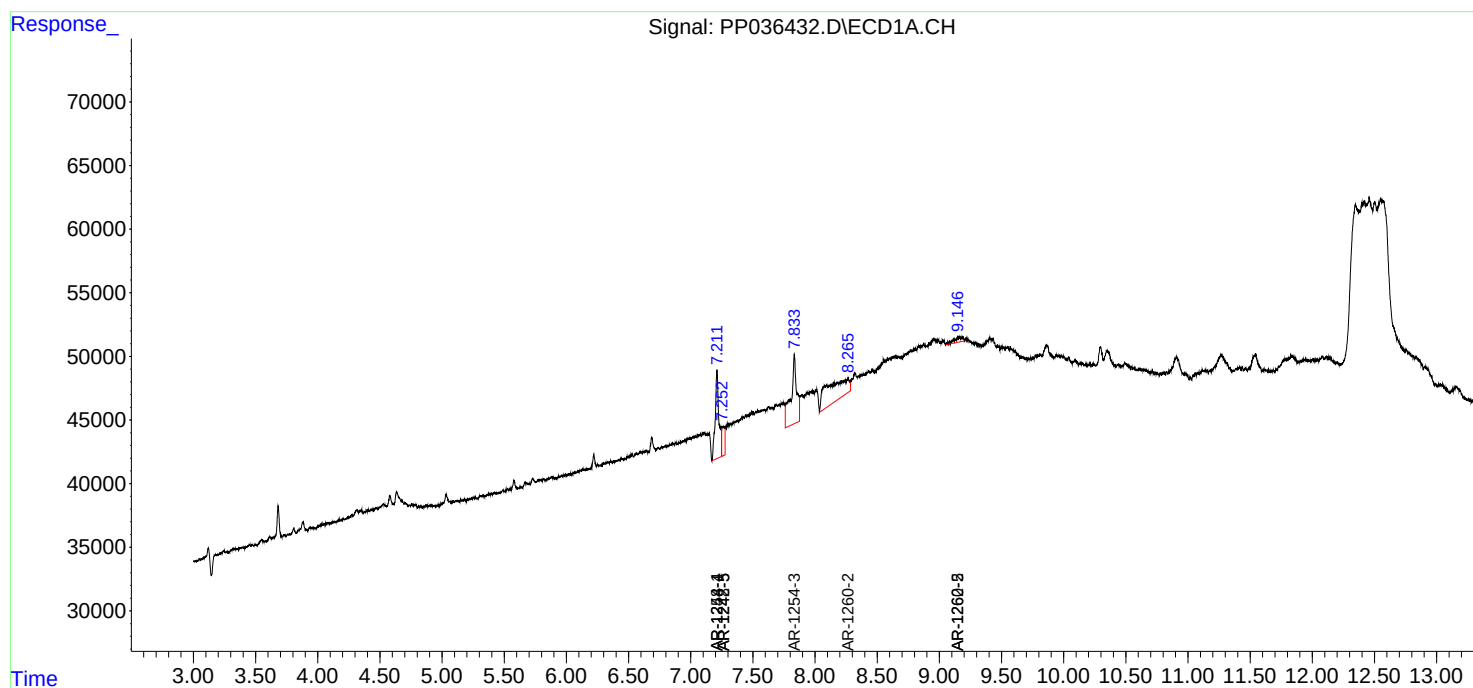


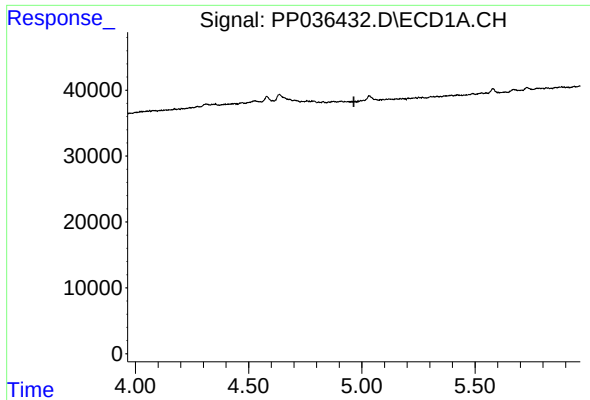

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

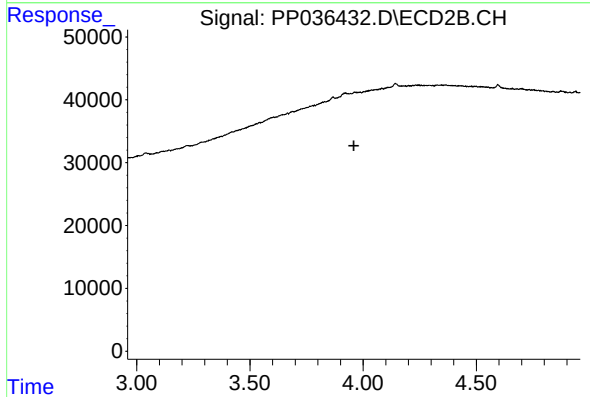


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.959 min
Response: 0
Conc: N.D.

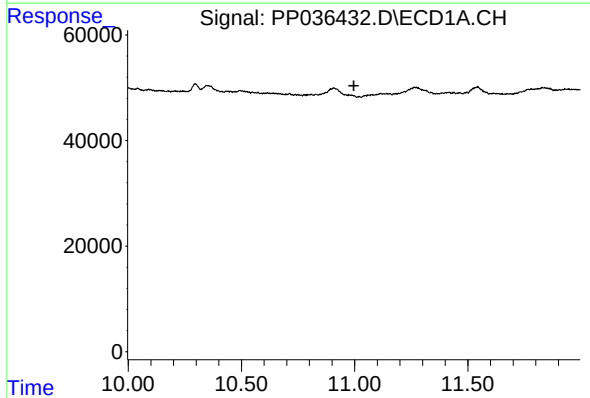


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.997 min
Response: 0
Conc: N.D.

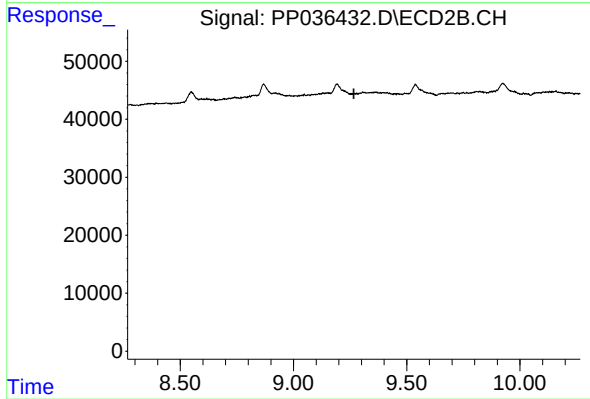

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.267 min
Response: 0
Conc: N.D.

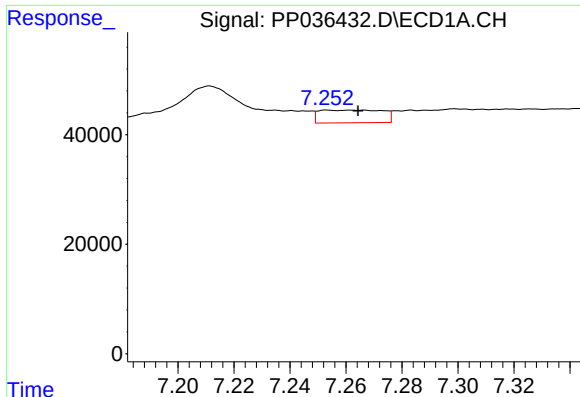

#20 AR-1242-5


R.T.: 7.263 min
Delta R.T.: -0.001 min
Response: 36487
Conc: 39.01 ng/ml

Instrument :
ECD_P
ClientSampleId :

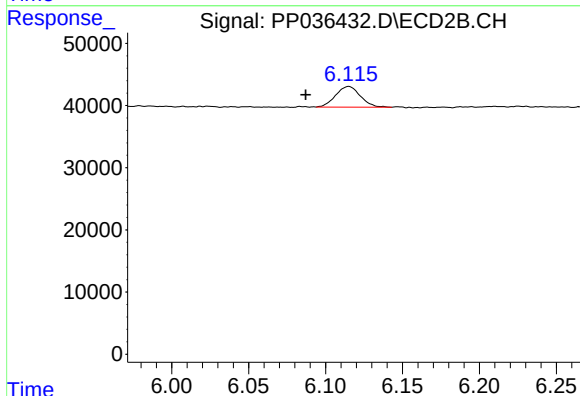


#20 AR-1242-5

R.T.: 6.115 min
Delta R.T.: 0.028 min
Response: 37290
Conc: 46.84 ng/ml

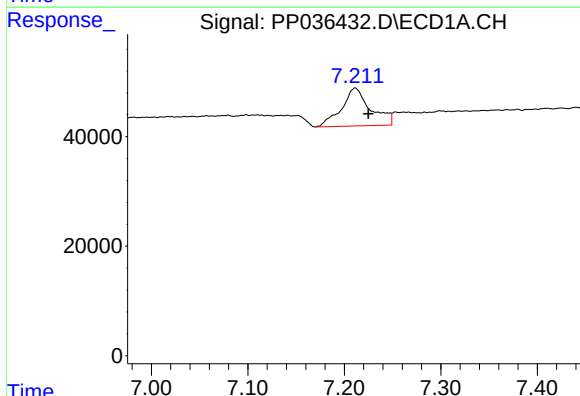


#24 AR-1248-4

R.T.: 7.211 min
Delta R.T.: -0.013 min
Response: 144546
Conc: 88.29 ng/ml

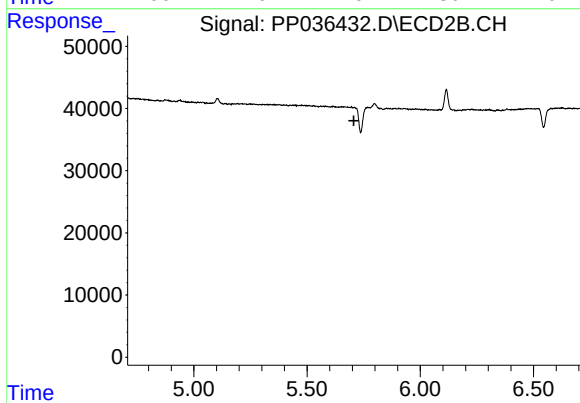

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.706 min
Response: 0
Conc: N.D.

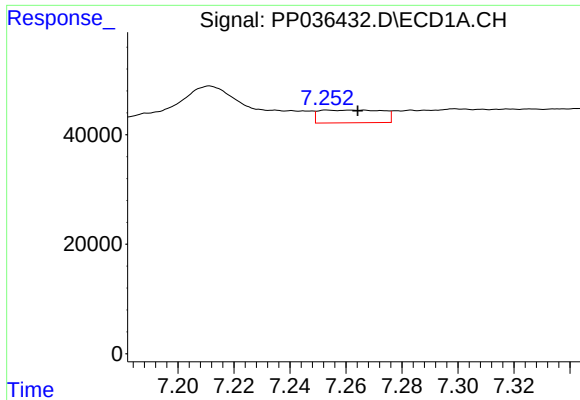

#25 AR-1248-5


R.T.: 7.263 min
Delta R.T.: -0.001 min
Response: 36487
Conc: 22.90 ng/ml

Instrument :
ECD_P
ClientSampleId :

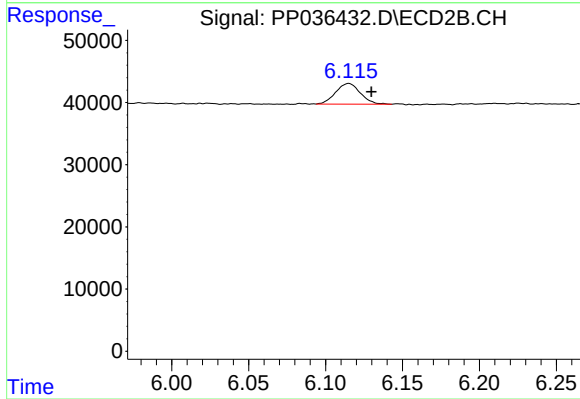


#25 AR-1248-5

R.T.: 6.115 min
Delta R.T.: -0.015 min
Response: 37290
Conc: 34.06 ng/ml

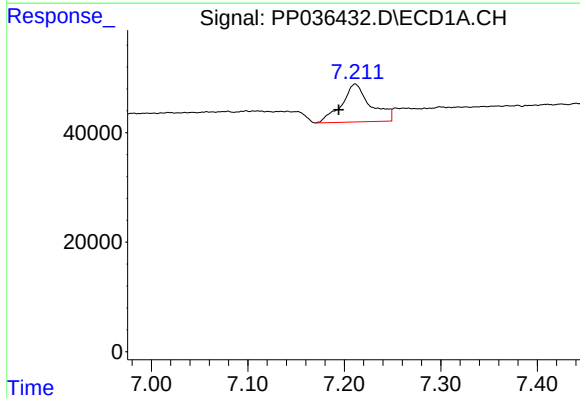


#26 AR-1254-1

R.T.: 7.211 min
Delta R.T.: 0.017 min
Response: 144546
Conc: 87.80 ng/ml

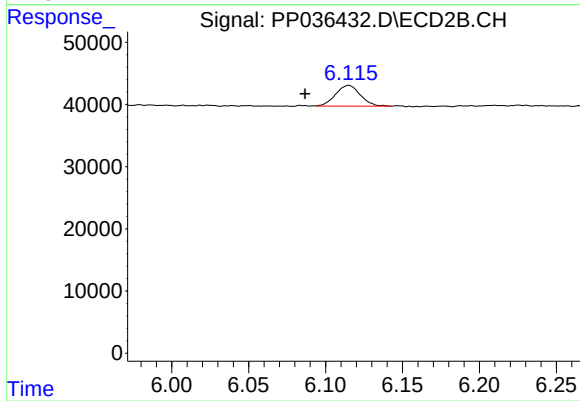

#26 AR-1254-1


R.T.: 6.115 min
Delta R.T.: 0.029 min
Response: 37290
Conc: 22.89 ng/ml

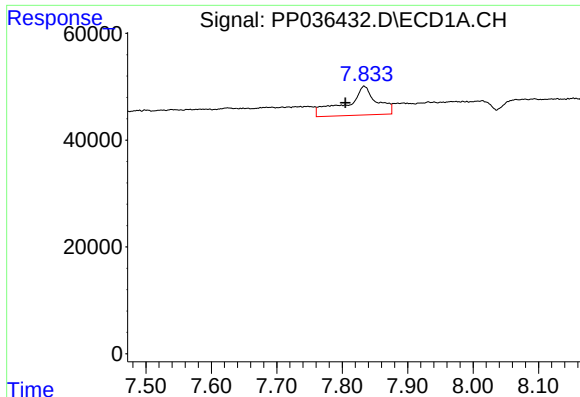

#28 AR-1254-3


R.T.: 7.834 min
Delta R.T.: 0.029 min
Response: 178000
Conc: 64.13 ng/ml

Instrument :
ECD_P
ClientSampleId :

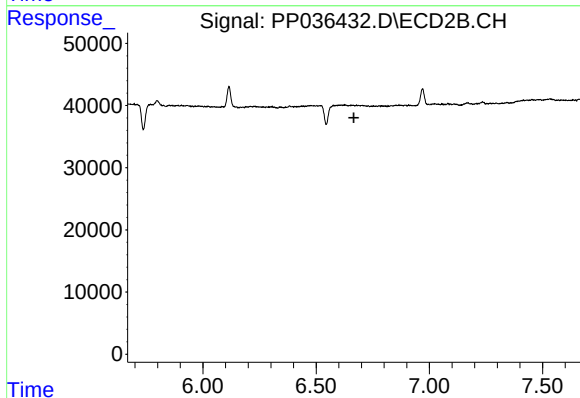


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

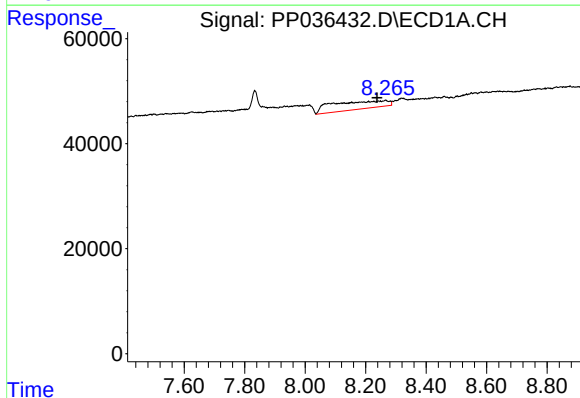


#32 AR-1260-2

R.T.: 8.266 min
Delta R.T.: 0.028 min
Response: 192459
Conc: 82.63 ng/ml

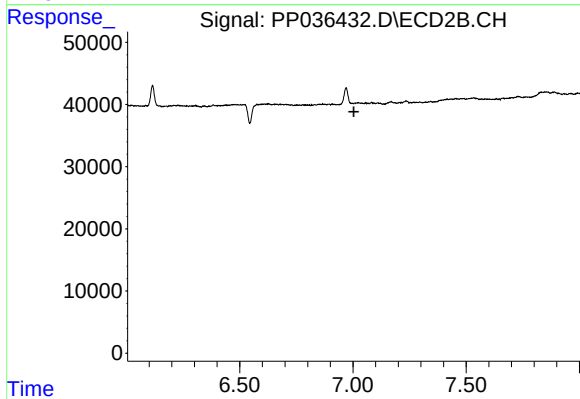

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.004 min
Response: 0
Conc: N.D.

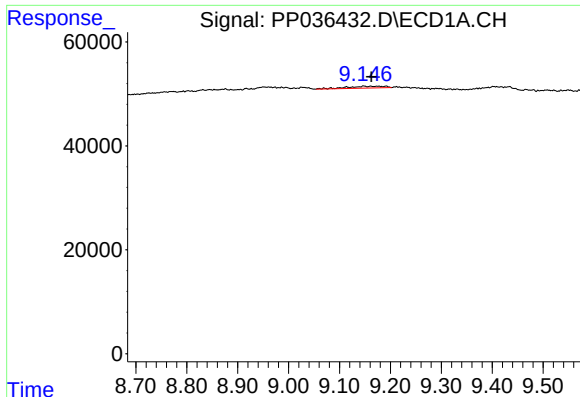

#35 AR-1260-5


R.T.: 9.148 min
Delta R.T.: -0.015 min
Response: 18712
Conc: 4.99 ng/ml

Instrument :
ECD_P
ClientSampleId :

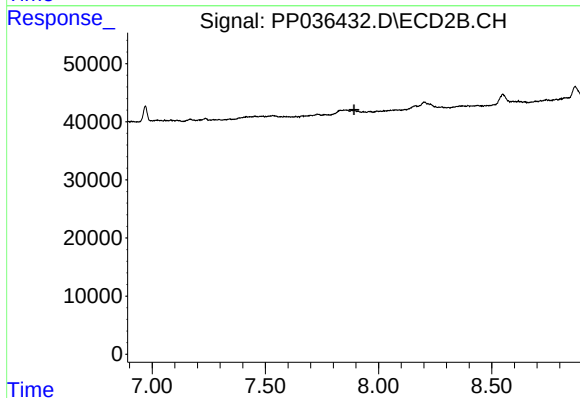


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.891 min
Response: 0
Conc: N.D.

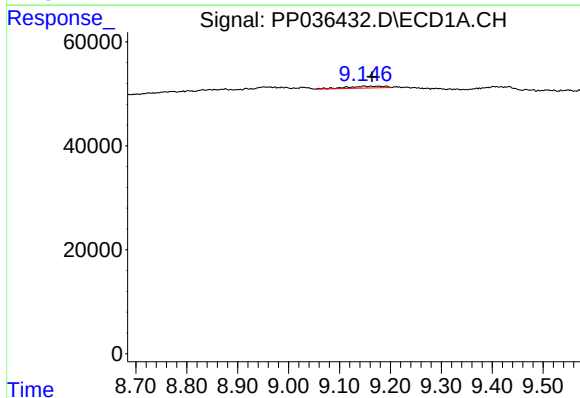


#37 AR-1262-2

R.T.: 9.148 min
Delta R.T.: -0.016 min
Response: 18712
Conc: 3.92 ng/ml

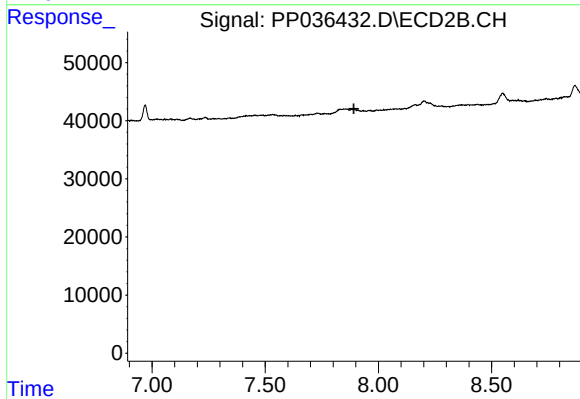

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.892 min
Response: 0
Conc: N.D.

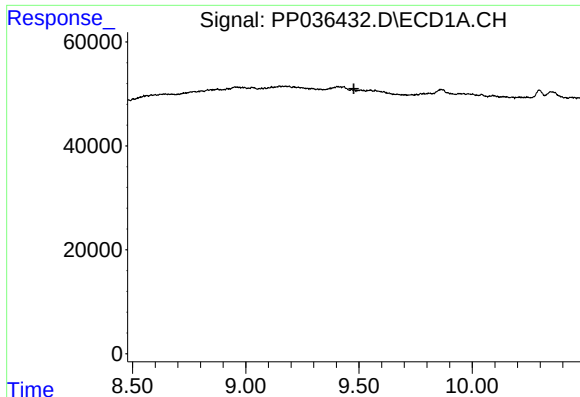

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

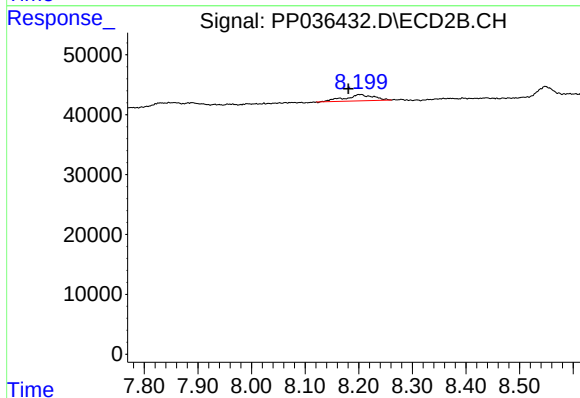


#38 AR-1262-3

R.T.: 8.200 min
Delta R.T.: 0.019 min
Response: 38958
Conc: 22.74 ng/ml

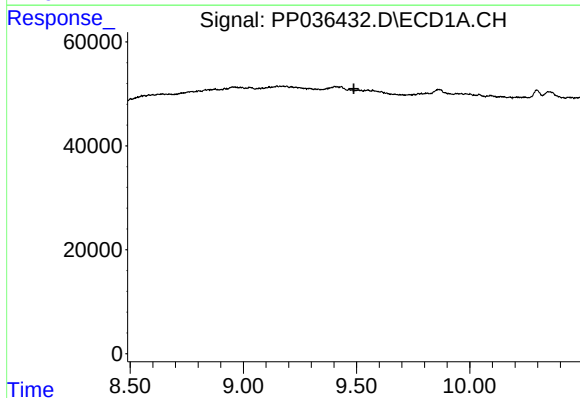

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.488 min
Response: 0
Conc: N.D.

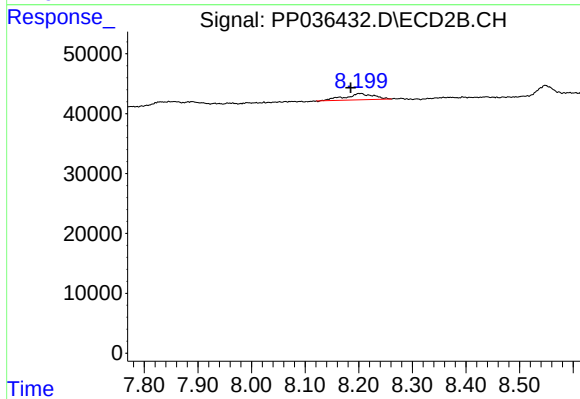

#41 AR-1268-1

R.T.: 8.200 min
Delta R.T.: 0.015 min
Response: 38958
Conc: 8.44 ng/ml