

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
 Data File : PP036443.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2021 12:29
 Operator : DD\AJ
 Sample : M2687-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:39:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.959	814888	573569	19.299	19.095
2)	SA Decachlor...	10.999	9.265	552992	388962	15.314	12.175
Target Compounds							
8)	L2 AR-1221-1	5.219	0.000	81783	0	164.443	N.D. #
9)	L2 AR-1221-2	5.319	0.000	12815	0	33.226	N.D. #
28)	L6 AR-1254-3	7.823f	0.000	38121	0	13.735	N.D. #
30)	L6 AR-1254-5	8.509f	0.000	32467	0	13.942	N.D. #
39)	L8 AR-1262-4	0.000	8.234	0	33810	N.D.	10.777 #
42)	L9 AR-1268-2	0.000	8.234f	0	33810	N.D.	7.860 #
44)	L9 AR-1268-4	10.280f	0.000	29718	0	15.181	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
Data File : PP036443.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2021 12:29
Operator : DD\AJ
Sample : M2687-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:39:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

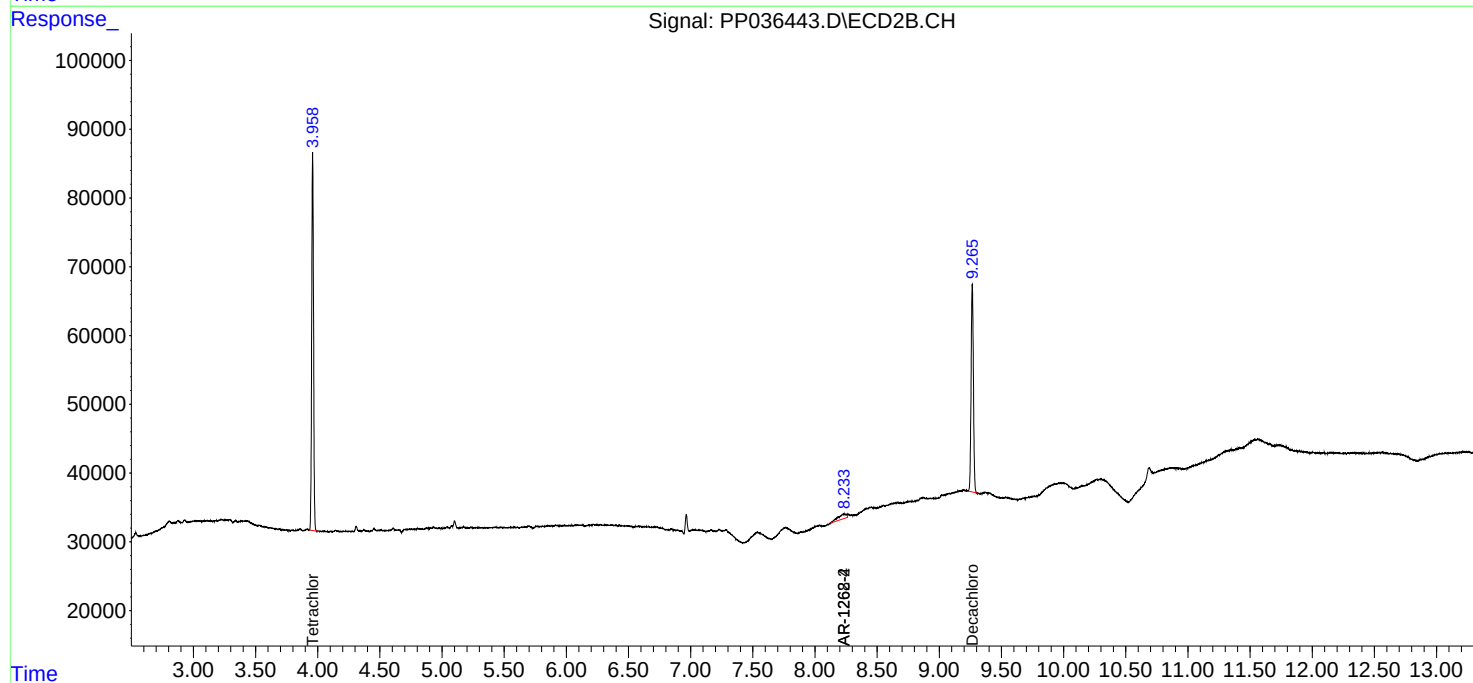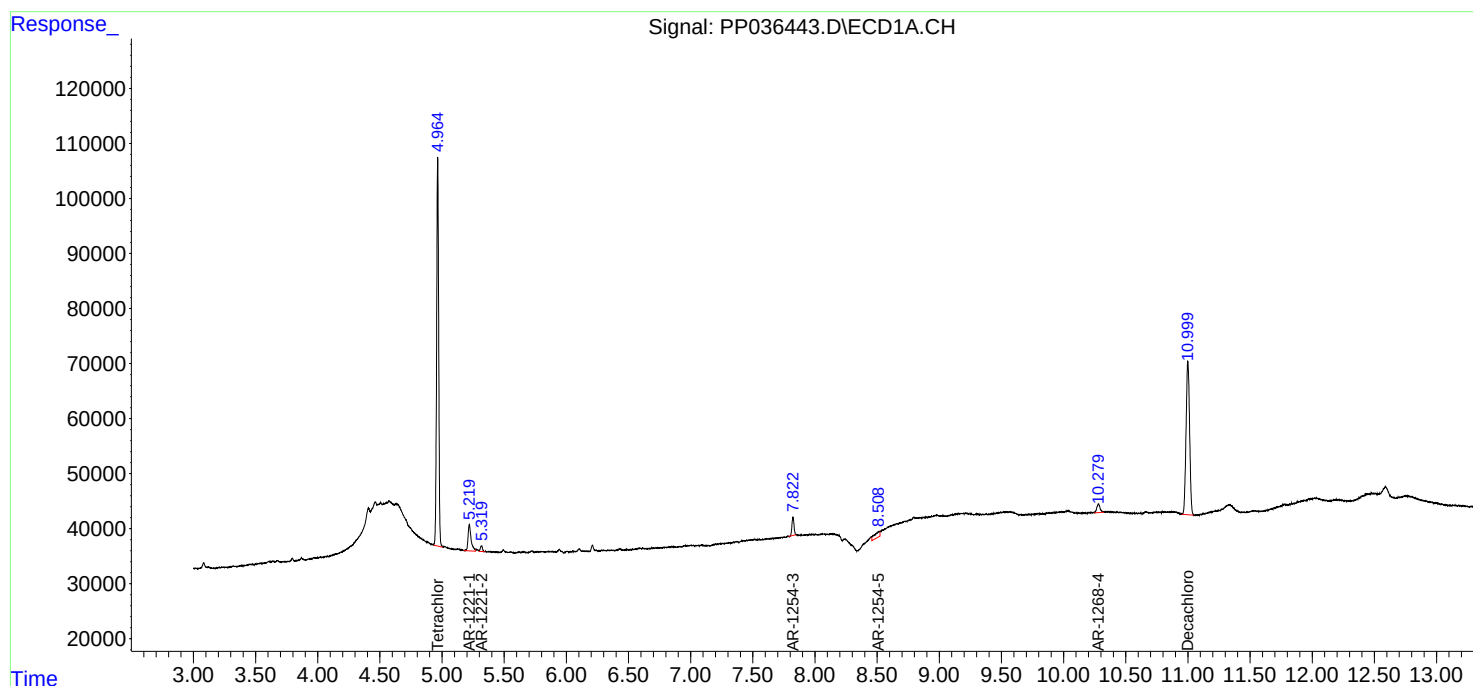


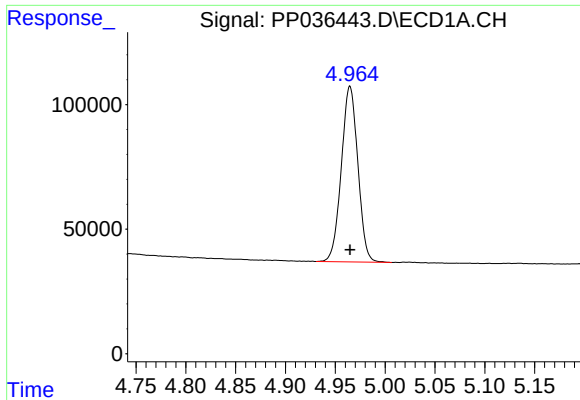

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 814888
Conc: 19.30 ng/ml

Instrument :
ECD_P
ClientSampleId :

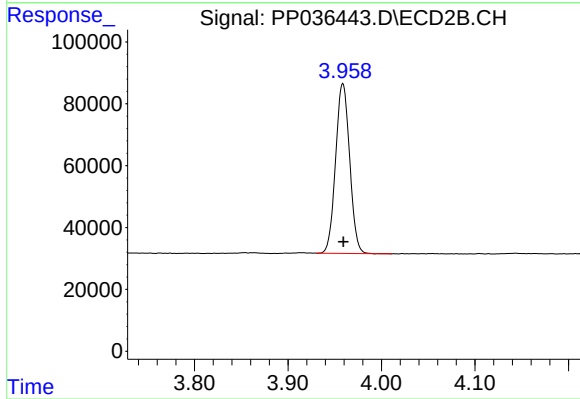


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 573569
Conc: 19.10 ng/ml

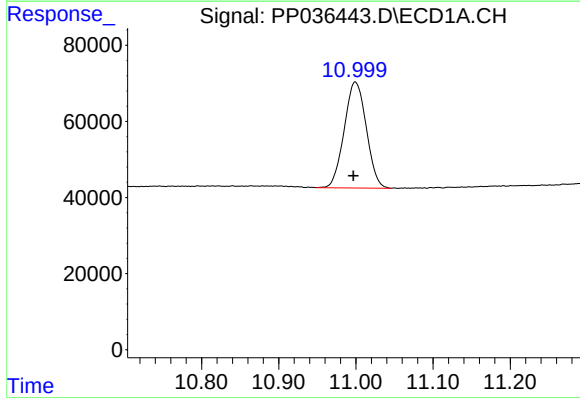


#2 Decachlorobiphenyl

R.T.: 10.999 min
Delta R.T.: 0.002 min
Response: 552992
Conc: 15.31 ng/ml

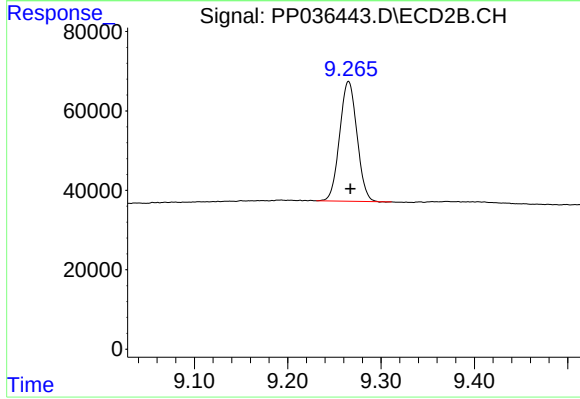

#2 Decachlorobiphenyl


R.T.: 9.265 min
Delta R.T.: -0.002 min
Response: 388962
Conc: 12.18 ng/ml

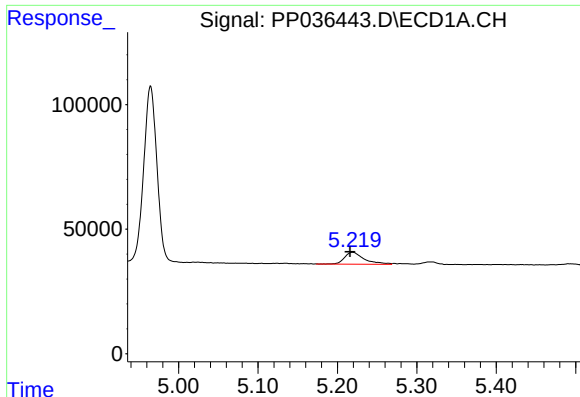

#8 AR-1221-1


R.T.: 5.219 min
Delta R.T.: 0.003 min
Response: 81783
Conc: 164.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

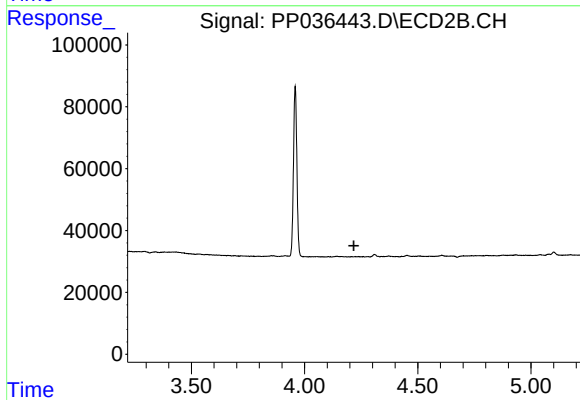


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.218 min
Response: 0
Conc: N.D.

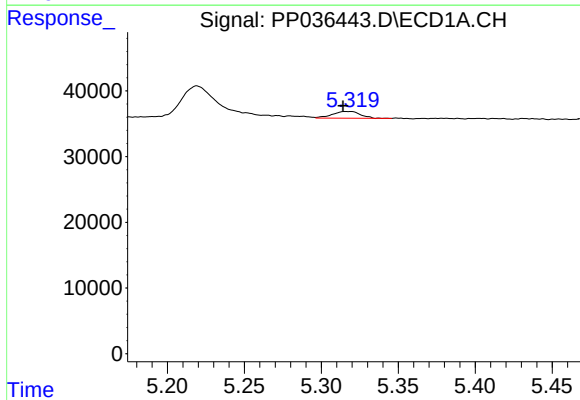


#9 AR-1221-2

R.T.: 5.319 min
Delta R.T.: 0.005 min
Response: 12815
Conc: 33.23 ng/ml

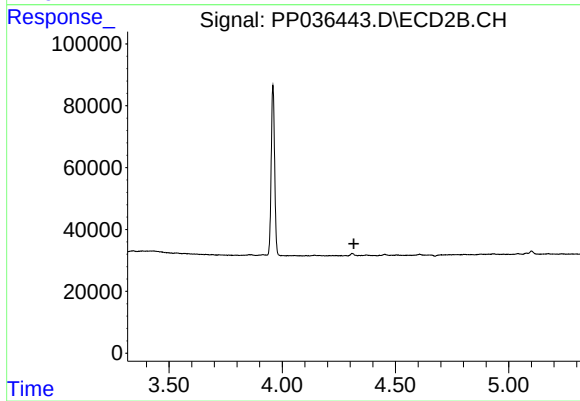

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

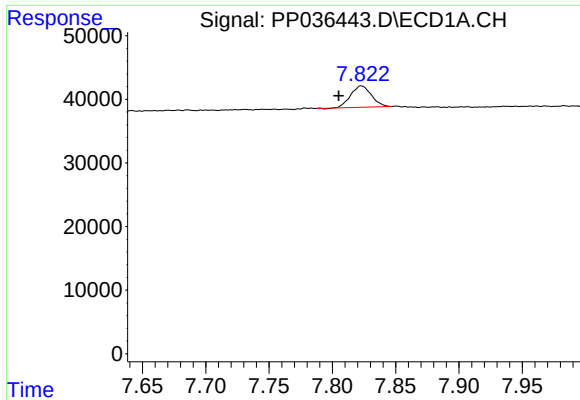

#28 AR-1254-3


R.T.: 7.823 min
Delta R.T.: 0.018 min
Response: 38121
Conc: 13.73 ng/ml

Instrument :
ECD_P
ClientSampleId :

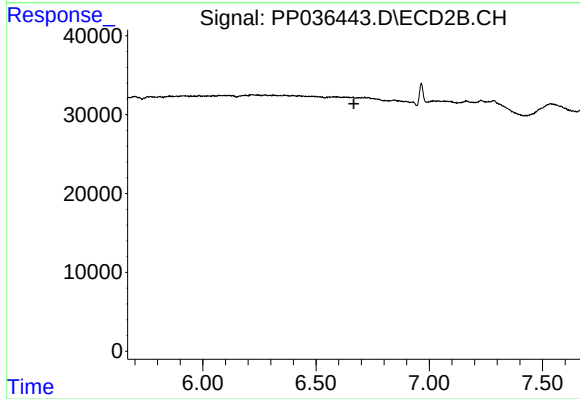


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

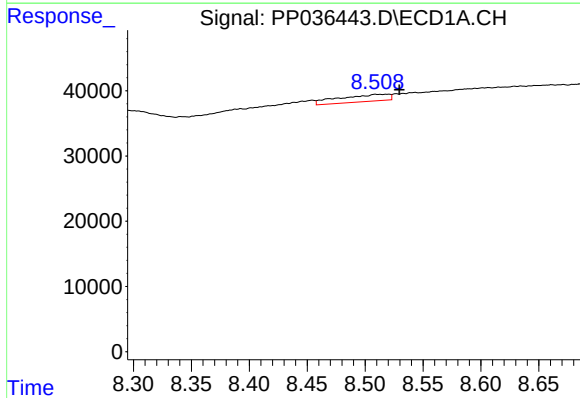


#30 AR-1254-5

R.T.: 8.509 min
Delta R.T.: -0.021 min
Response: 32467
Conc: 13.94 ng/ml

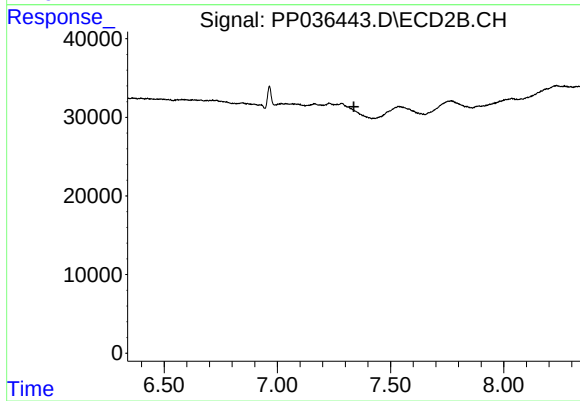

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.338 min
Response: 0
Conc: N.D.

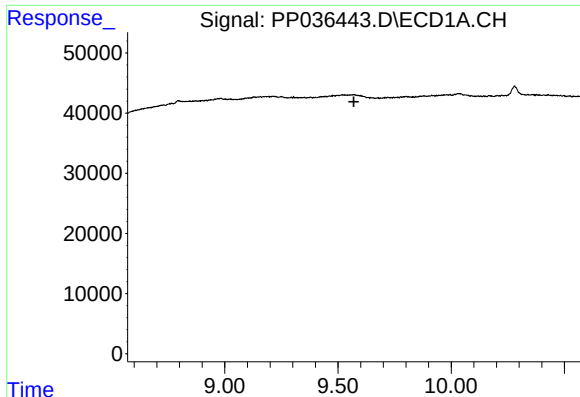

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

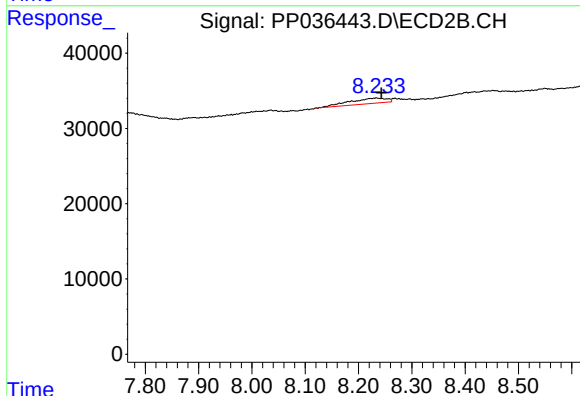


#39 AR-1262-4

R.T.: 8.234 min
Delta R.T.: -0.010 min
Response: 33810
Conc: 10.78 ng/ml

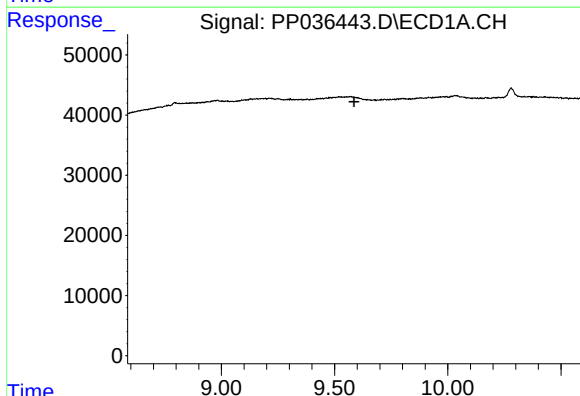


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.586 min
Response: 0
Conc: N.D.

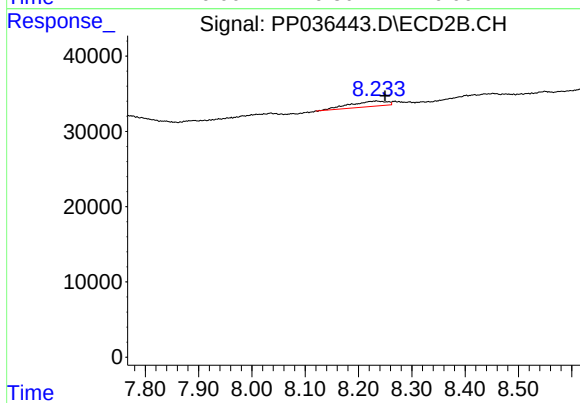

#42 AR-1268-2


R.T.: 8.234 min
Delta R.T.: -0.016 min
Response: 33810
Conc: 7.86 ng/ml

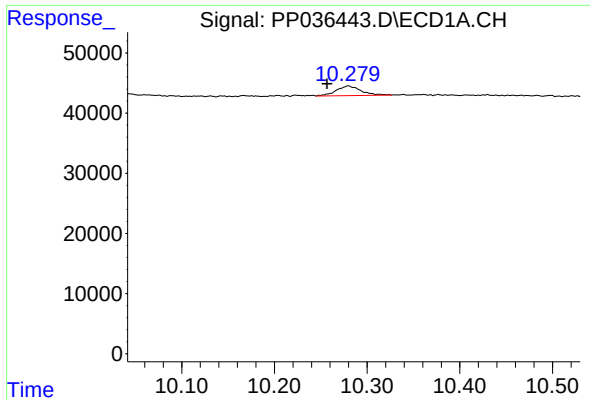

#44 AR-1268-4

R.T.: 10.280 min
Delta R.T.: 0.023 min
Response: 29718
Conc: 15.18 ng/ml

Instrument :
ECD_P
ClientSampleId :

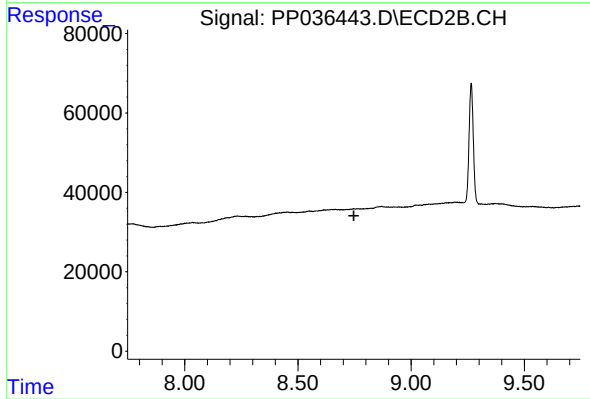

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.747 min
Response: 0
Conc: N.D.