

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
 Data File : PP036450.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2021 14:29
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:42:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.970	3.960	869464	606114	20.592	20.179
2) SA Decachlor...	11.007	9.269	917227	677339	25.401	21.202
Target Compounds						
9) L2 AR-1221-2	5.322	0.000	13154	0	34.106	N.D. #
15) L3 AR-1232-5	6.578	0.000	17375	0	53.689	N.D. #
22) L5 AR-1248-2	6.578	0.000	17375	0	14.403	N.D. #
24) L5 AR-1248-4	7.213	0.000	5854	0	3.576	N.D. #
26) L6 AR-1254-1	7.213f	0.000	5854	0	3.556	N.D. #
28) L6 AR-1254-3	7.827f	0.000	22665	0	8.166	N.D. #
38) L8 AR-1262-3	9.504f	0.000	14194	0	4.142	N.D. #
39) L8 AR-1262-4	9.552f	0.000	328	0	0.123	N.D. #
41) L9 AR-1268-1	9.504f	0.000	14194	0	2.725	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
Data File : PP036450.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2021 14:29
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:42:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

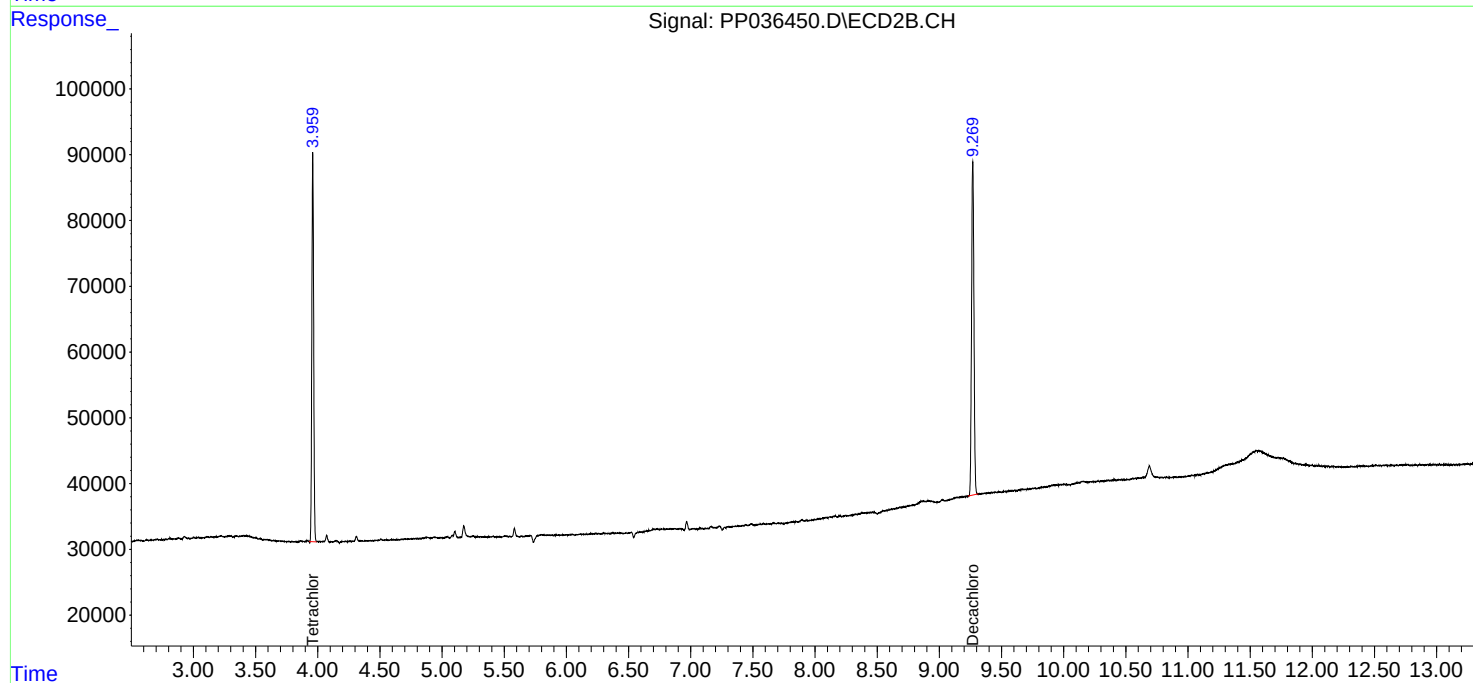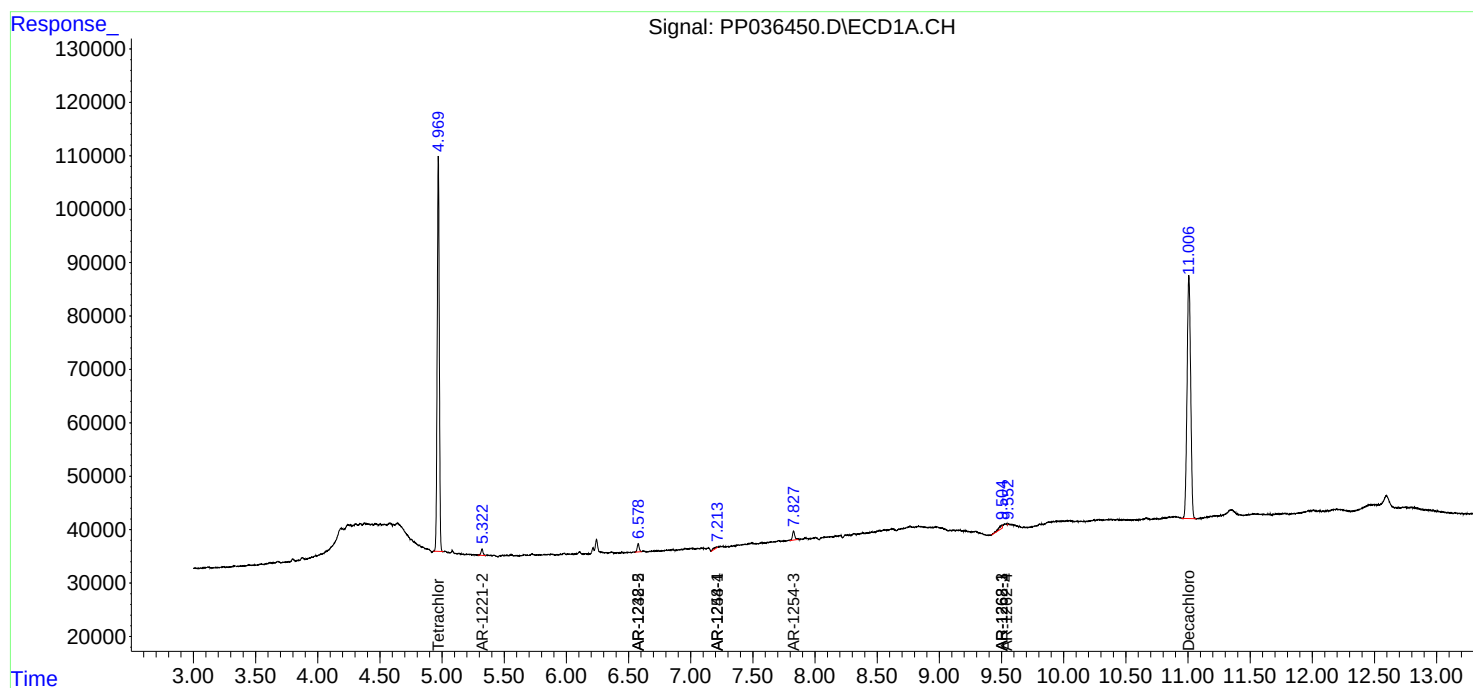


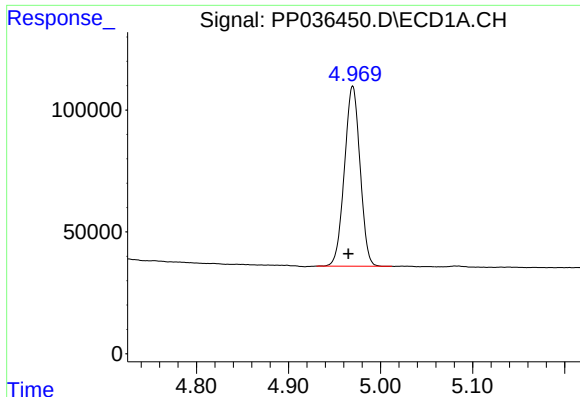

#1 Tetrachloro-m-xylene


R.T.: 4.970 min
Delta R.T.: 0.005 min
Response: 869464
Conc: 20.59 ng/ml

Instrument :
ECD_P
ClientSampleId :

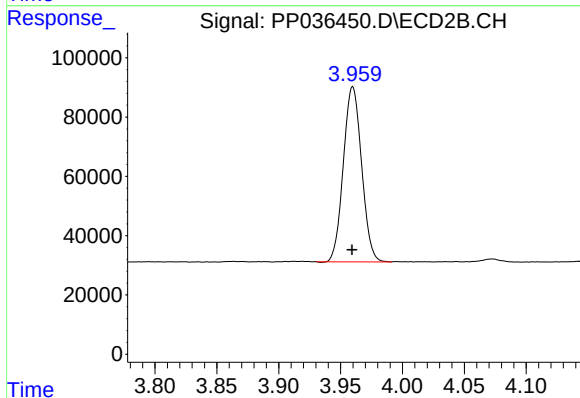


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 606114
Conc: 20.18 ng/ml

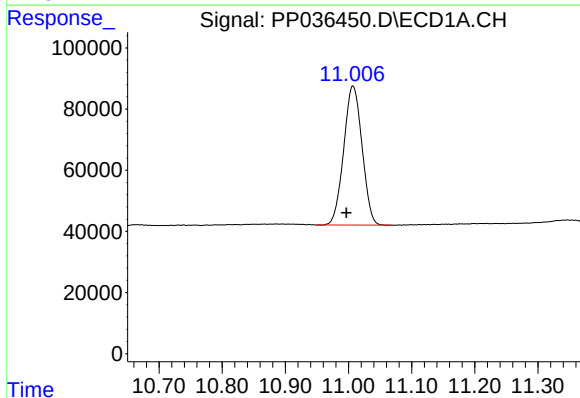


#2 Decachlorobiphenyl

R.T.: 11.007 min
Delta R.T.: 0.010 min
Response: 917227
Conc: 25.40 ng/ml

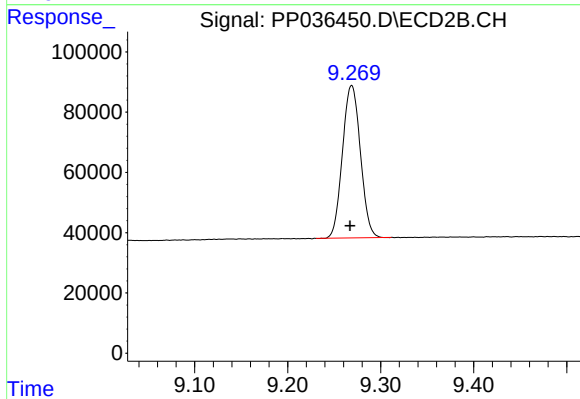

#2 Decachlorobiphenyl


R.T.: 9.269 min
Delta R.T.: 0.002 min
Response: 677339
Conc: 21.20 ng/ml

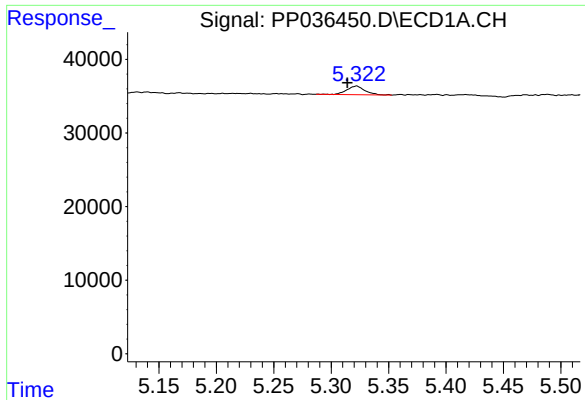

#9 AR-1221-2


R.T.: 5.322 min
Delta R.T.: 0.008 min
Response: 13154
Conc: 34.11 ng/ml

Instrument :
ECD_P
ClientSampleId :

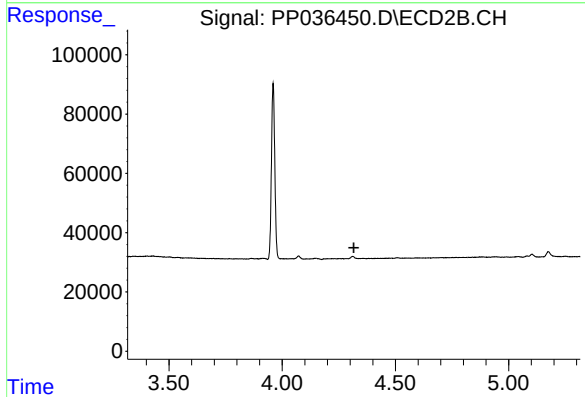


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.316 min
Response: 0
Conc: N.D.

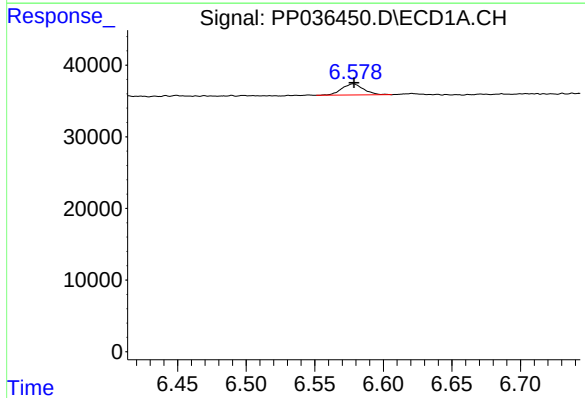


#15 AR-1232-5

R.T.: 6.578 min
Delta R.T.: 0.000 min
Response: 17375
Conc: 53.69 ng/ml

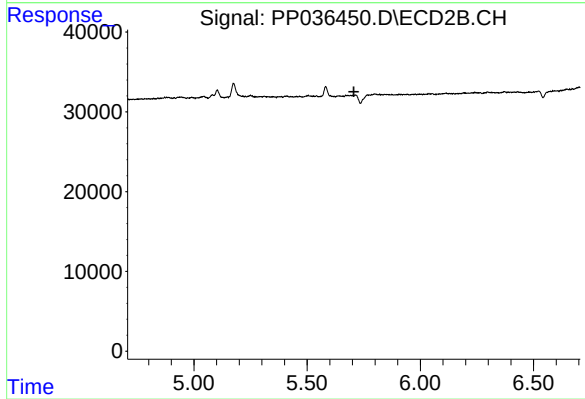

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.707 min
Response: 0
Conc: N.D.

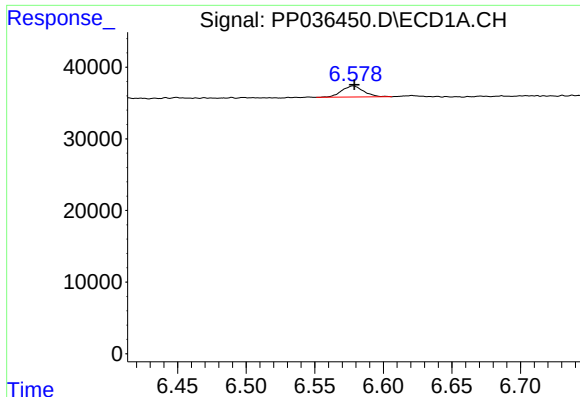

#22 AR-1248-2


R.T.: 6.578 min
Delta R.T.: 0.000 min
Response: 17375
Conc: 14.40 ng/ml

Instrument :
ECD_P
ClientSampleId :

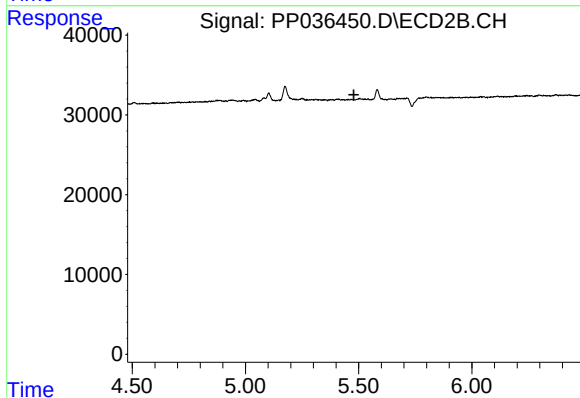


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.479 min
Response: 0
Conc: N.D.

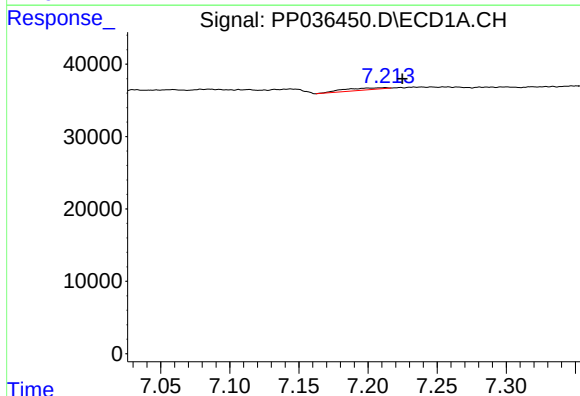


#24 AR-1248-4

R.T.: 7.213 min
Delta R.T.: -0.012 min
Response: 5854
Conc: 3.58 ng/ml

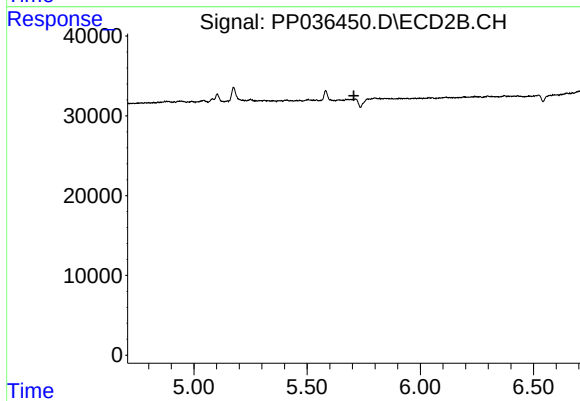

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.706 min
Response: 0
Conc: N.D.

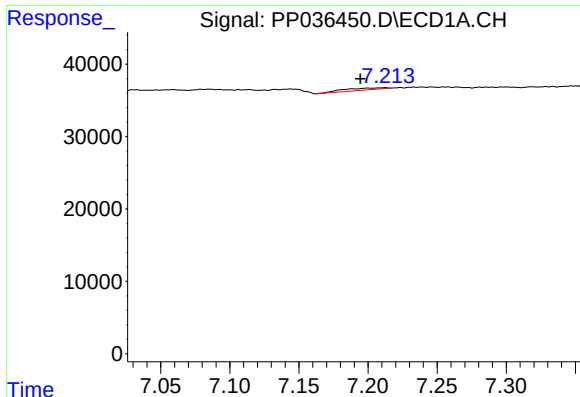

#26 AR-1254-1


R.T.: 7.213 min
Delta R.T.: 0.018 min
Response: 5854
Conc: 3.56 ng/ml

Instrument :
ECD_P
ClientSampleId :

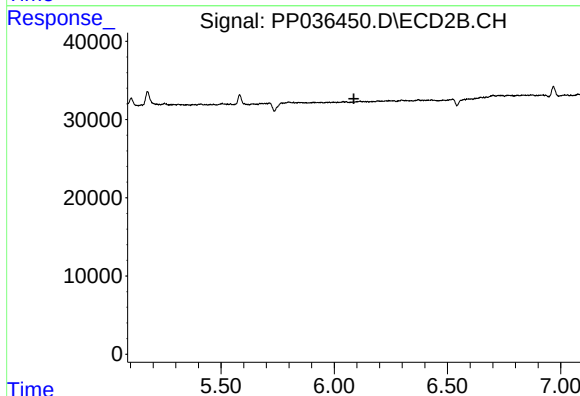


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.087 min
Response: 0
Conc: N.D.

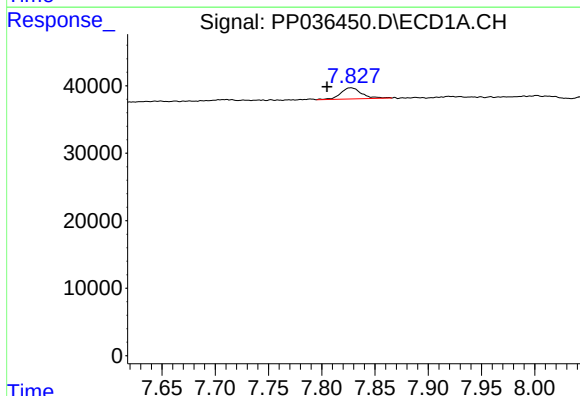


#28 AR-1254-3

R.T.: 7.827 min
Delta R.T.: 0.022 min
Response: 22665
Conc: 8.17 ng/ml

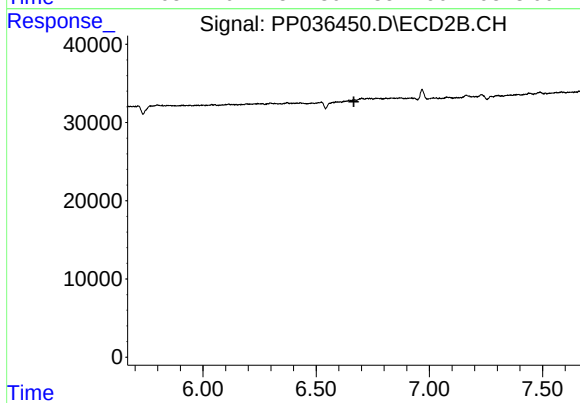

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

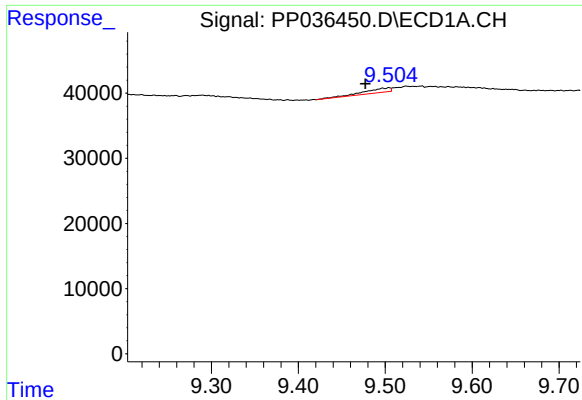

#38 AR-1262-3


R.T.: 9.504 min
Delta R.T.: 0.027 min
Response: 14194
Conc: 4.14 ng/ml

Instrument :
ECD_P
ClientSampleId :

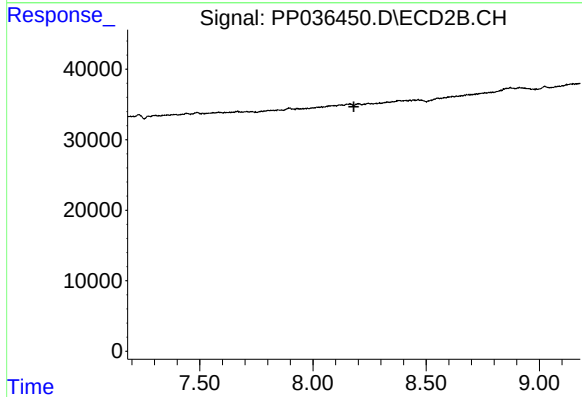


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.181 min
Response: 0
Conc: N.D.

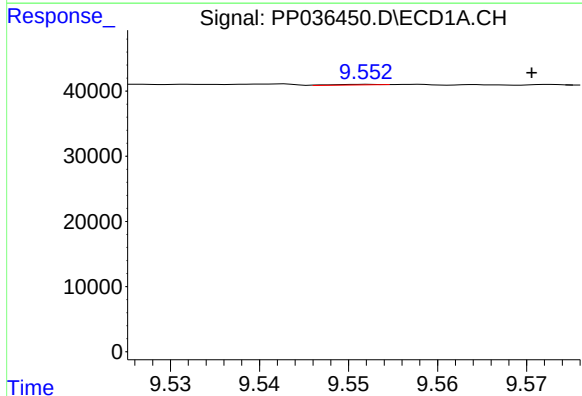


#39 AR-1262-4

R.T.: 9.552 min
Delta R.T.: -0.019 min
Response: 328
Conc: 0.12 ng/ml

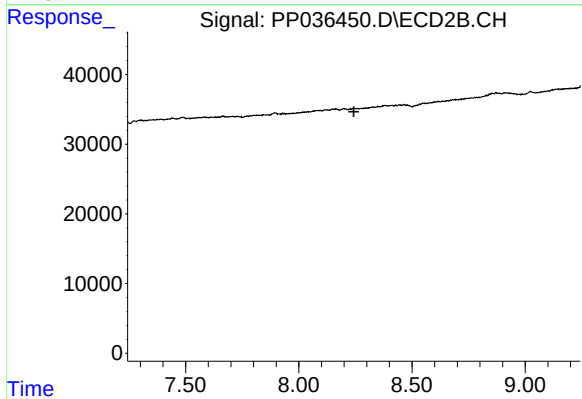

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.243 min
Response: 0
Conc: N.D.

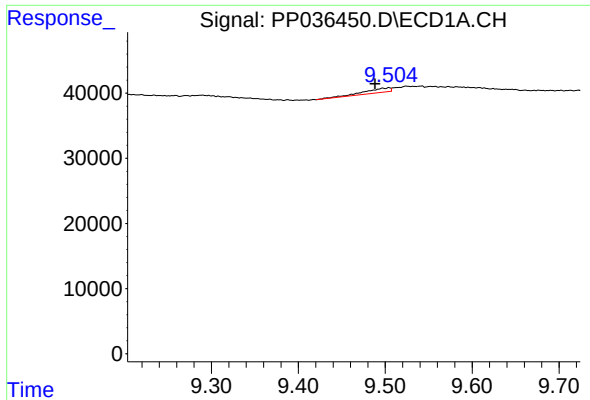

#41 AR-1268-1

R.T.: 9.504 min
Delta R.T.: 0.016 min
Response: 14194
Conc: 2.73 ng/ml

Instrument :
ECD_P
ClientSampleId :

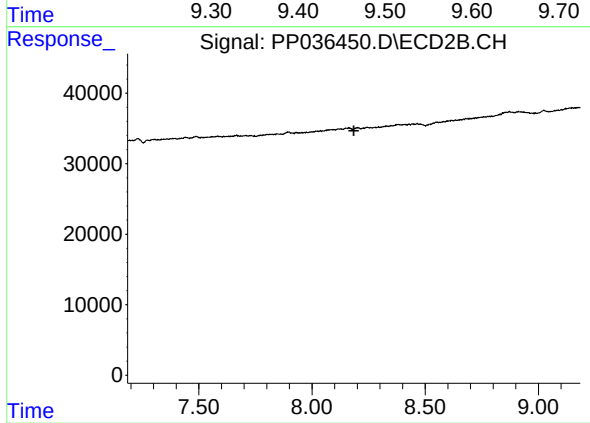

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.185 min
Response: 0
Conc: N.D.