

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
 Data File : PP036446.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2021 13:20 (#1); 14 Jun 2021 13:19 (#2)
 Operator : DD\AJ
 Sample : M2687-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 17-B6(120-124)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:41:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.964	3.958	968069	684086	22.927	22.775
2)	SA Decachlor...	10.997	9.265	915204	656531	25.345	20.550

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
Data File : PP036446.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2021 13:20 (#1); 14 Jun 2021 13:19 (#2)
Operator : DD\AJ
Sample : M2687-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
17-B6(120-124)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:41:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

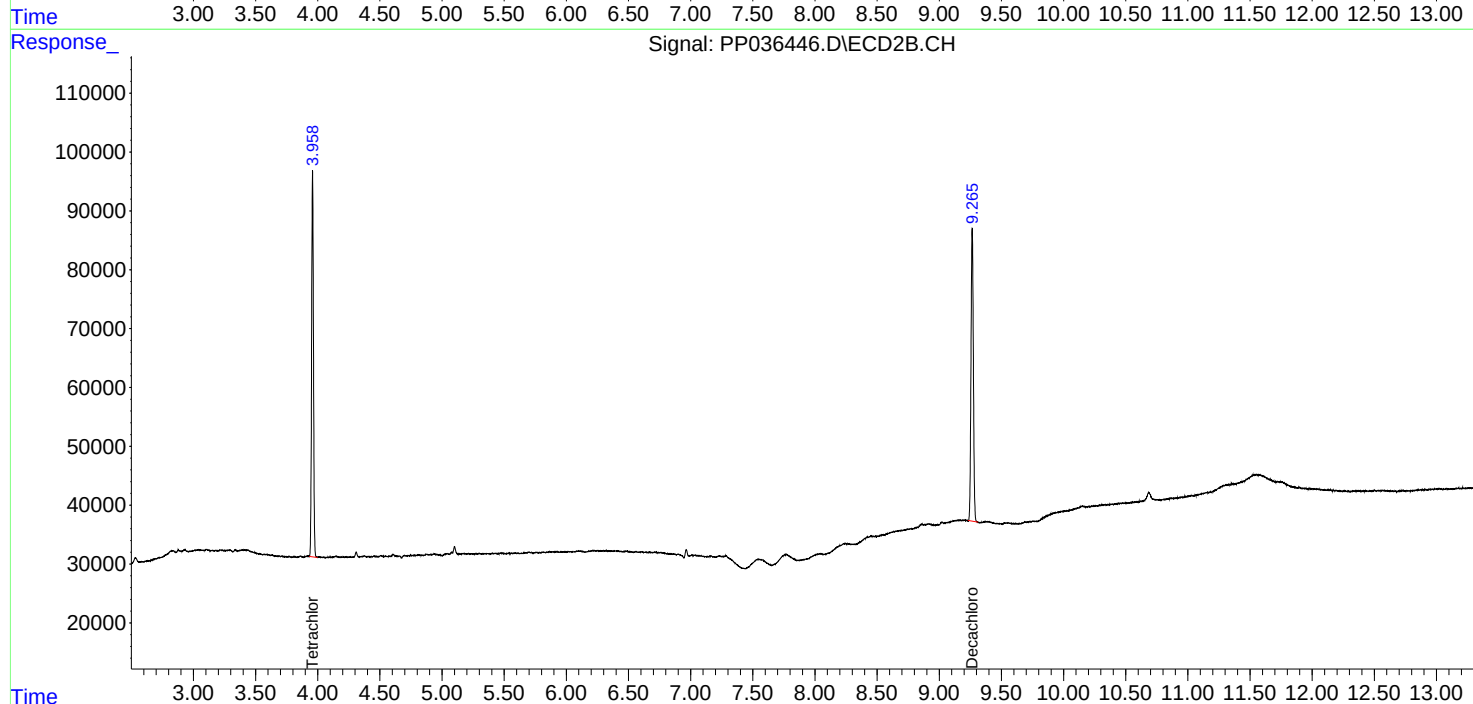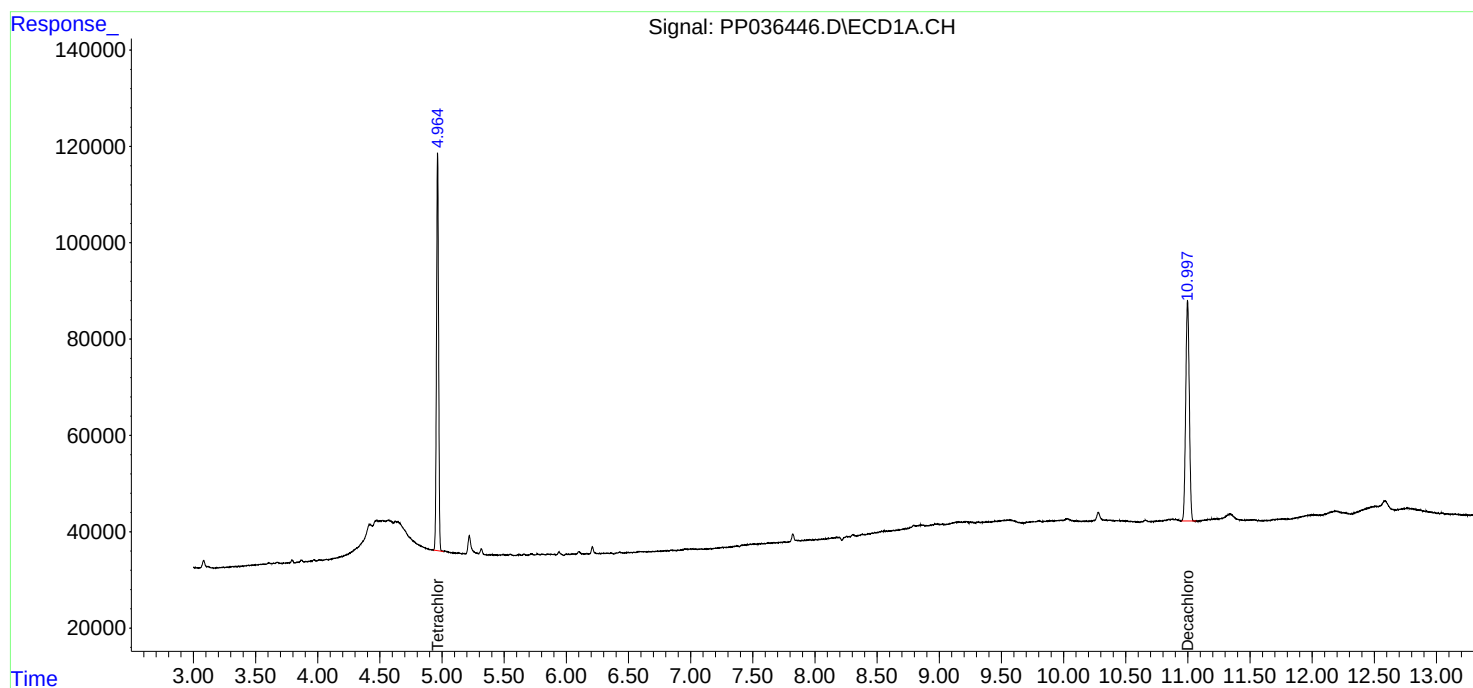


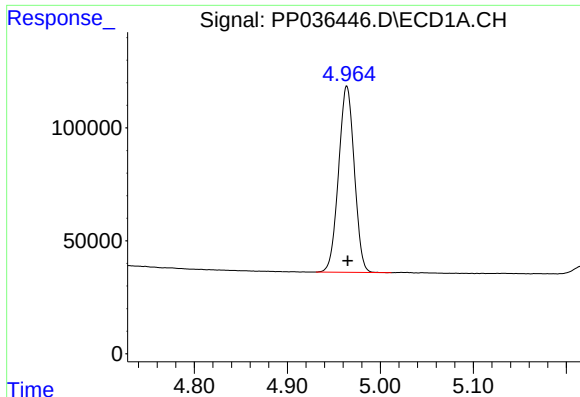

#1 Tetrachloro-m-xylene


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 968069
Conc: 22.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
17-B6(120-124)

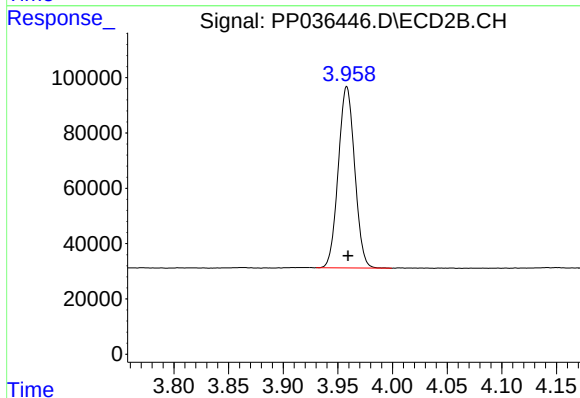


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 684086
Conc: 22.77 ng/ml

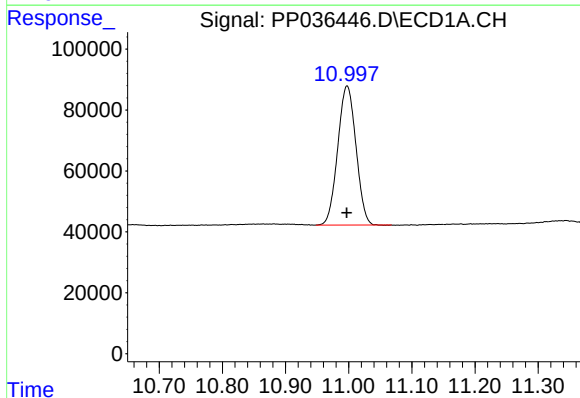

#2 Decachlorobiphenyl

R.T.: 10.997 min
Delta R.T.: 0.000 min
Response: 915204
Conc: 25.34 ng/ml

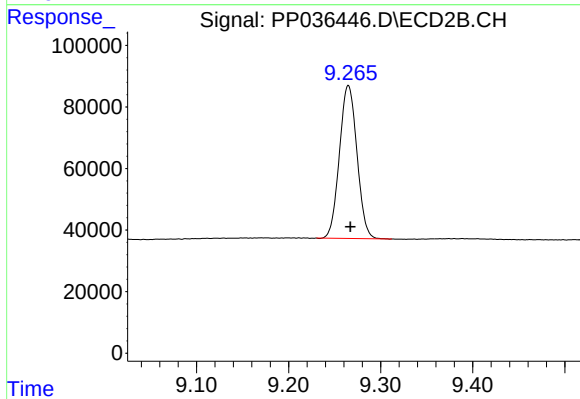

#2 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: -0.002 min
Response: 656531
Conc: 20.55 ng/ml