

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
 Data File : PP036451.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2021 17:10
 Operator : DD\AJ
 Sample : 200 PPB PEST/PCB SURROGATE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 200 PPB PEST/PCB SURROGATE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 05:43:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.977	3.961	6308805	4805725	149.412	159.993
2) SA Decachlor...	11.019f	9.273	5994852	4984080	166.017	156.010

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061421\
Data File : PP036451.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2021 17:10
Operator : DD\AJ
Sample : 200 PPB PEST/PCB SURROGATE
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
200 PPB PEST/PCB SURROGATE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 05:43:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

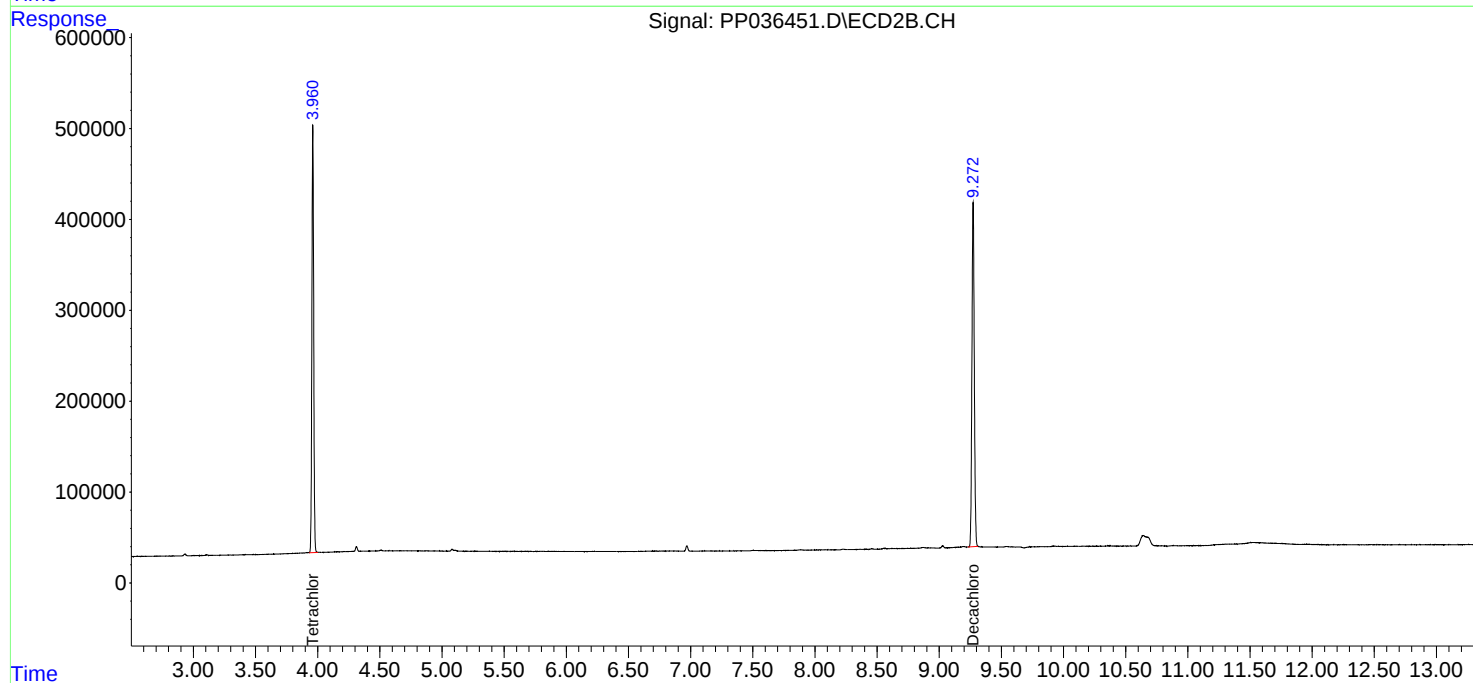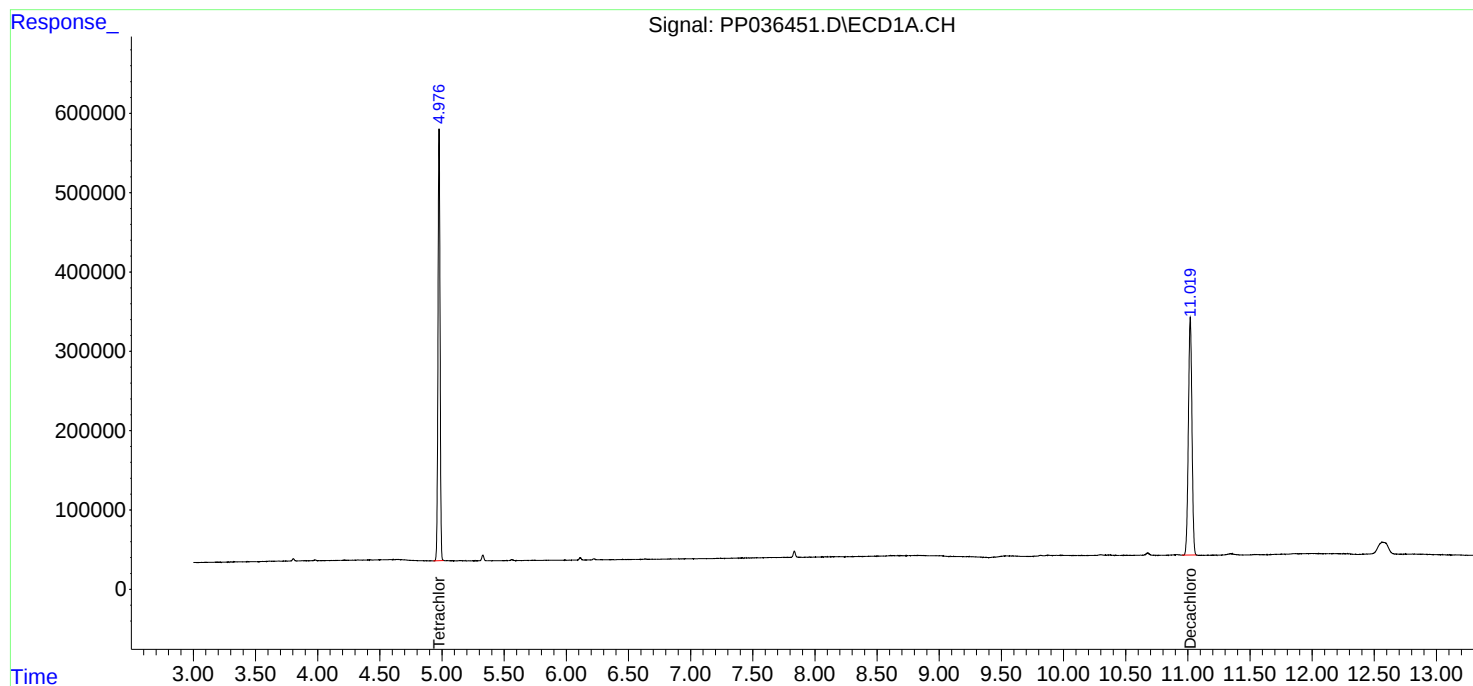


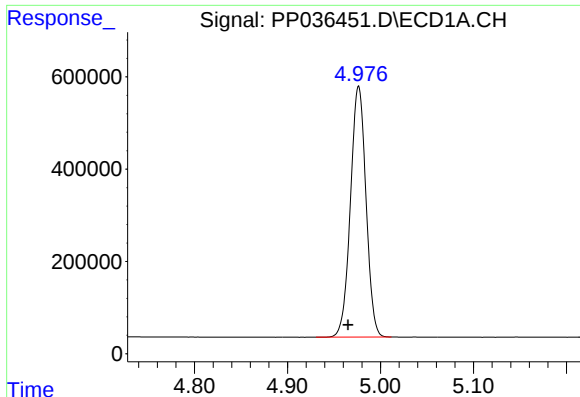

#1 Tetrachloro-m-xylene


R.T.: 4.977 min
Delta R.T.: 0.012 min
Response: 6308805
Conc: 149.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
200 PPB PEST/PCB SURROGATE

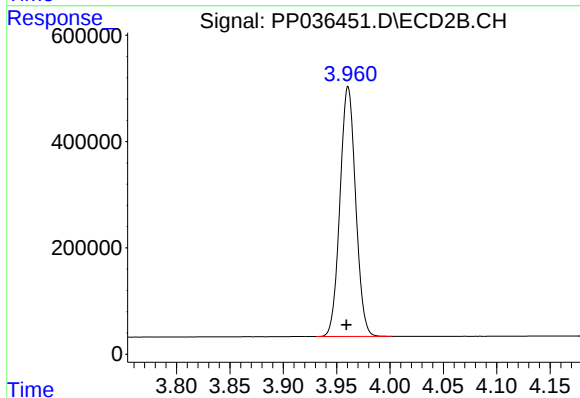


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.002 min
Response: 4805725
Conc: 159.99 ng/ml

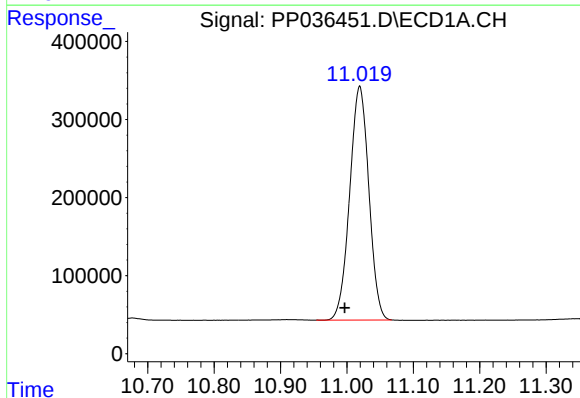

#2 Decachlorobiphenyl

R.T.: 11.019 min
Delta R.T.: 0.023 min
Response: 5994852
Conc: 166.02 ng/ml

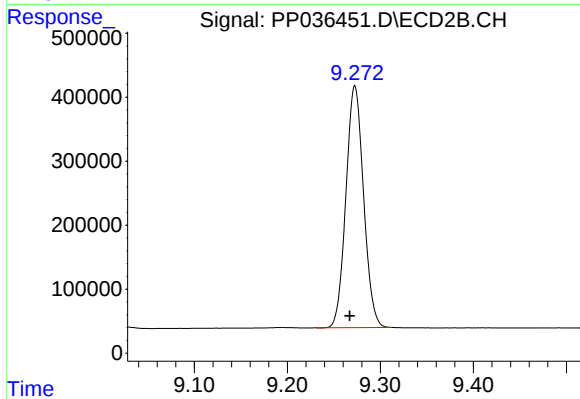

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.006 min
Response: 4984080
Conc: 156.01 ng/ml