

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061621\
 Data File : PP036477.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jun 2021 11:57
 Operator : DD\AJ
 Sample : M2718-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 13:14:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.958	435706	304895	10.319	10.151
2)	SA Decachlor...	11.002	9.265	487670	340418	13.505	10.656
Target Compounds							
8)	L2 AR-1221-1	5.219	0.000	36407	0	73.204	N.D. #
20)	L4 AR-1242-5	7.266	0.000	81185	0	86.790	N.D. #
25)	L5 AR-1248-5	7.266	0.000	81185	0	50.953	N.D. #
27)	L6 AR-1254-2	7.428	0.000	4877	0	1.920	N.D. #
28)	L6 AR-1254-3	7.823f	6.667	86748	24537	31.254	10.207 #
30)	L6 AR-1254-5	8.544	0.000	5290	0	2.272	N.D. #
35)	L7 AR-1260-5	9.157	0.000	21974	0	5.855	N.D. #
37)	L8 AR-1262-2	9.157	0.000	21974	0	4.601	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061621\
Data File : PP036477.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jun 2021 11:57
Operator : DD\AJ
Sample : M2718-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 13:14:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

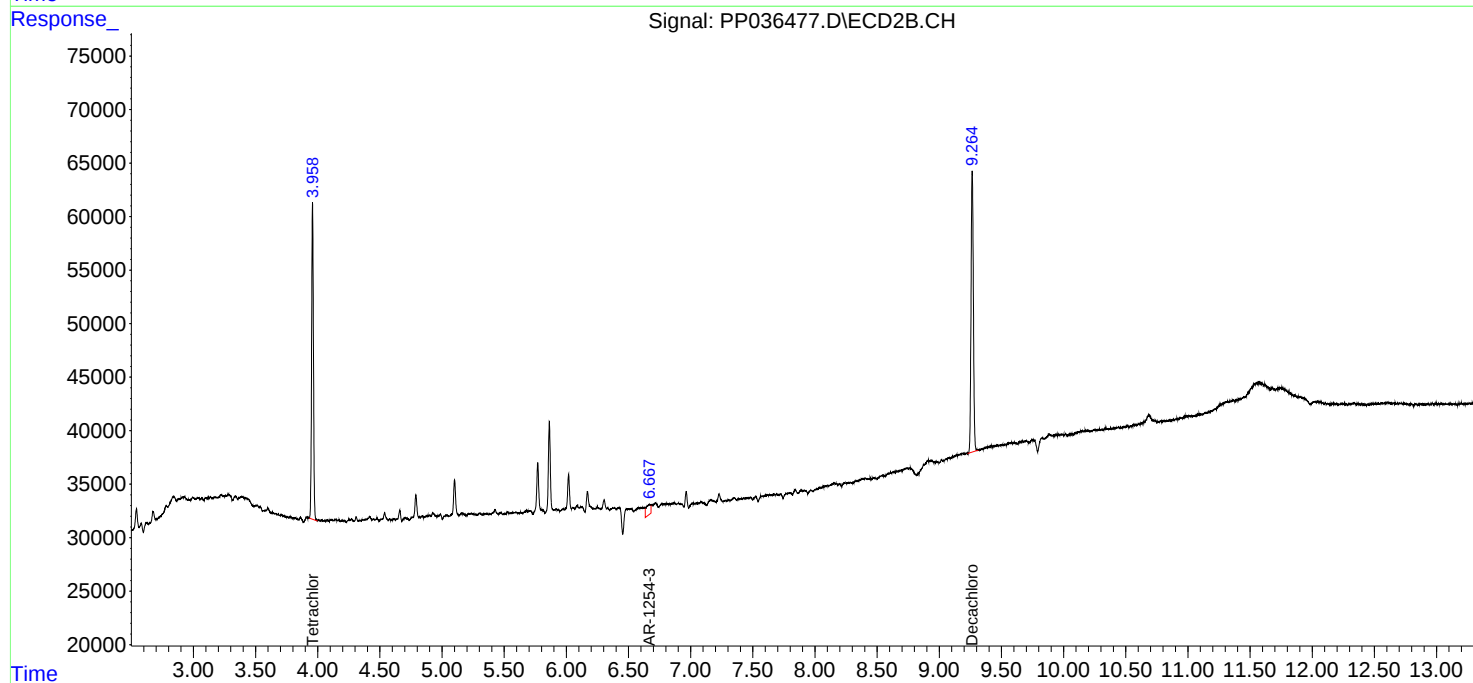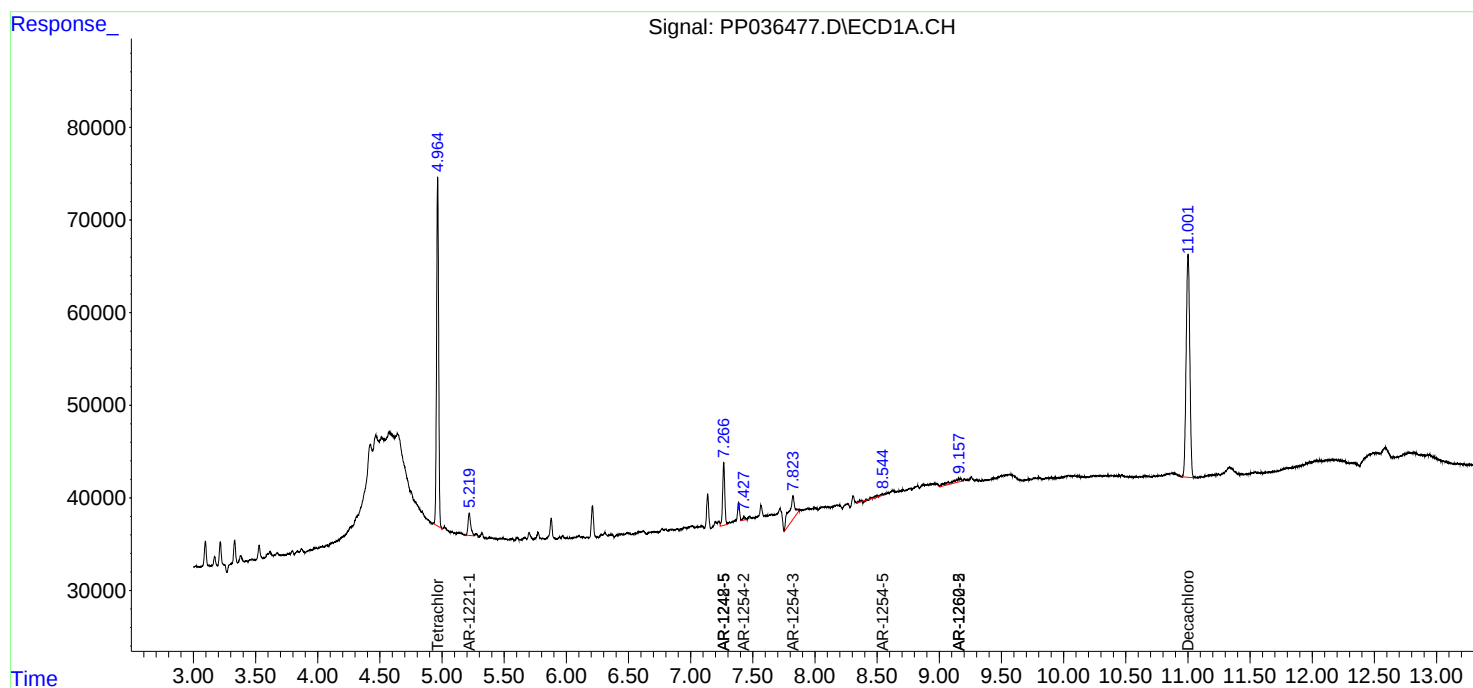


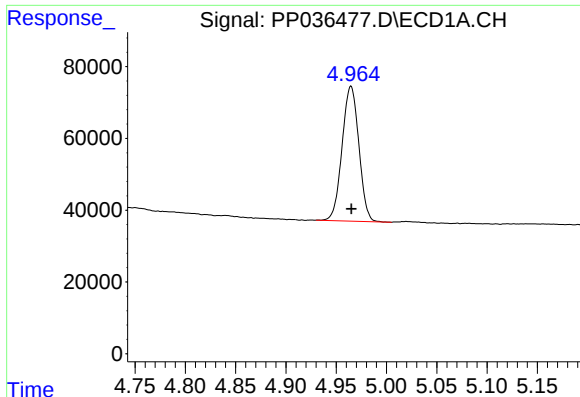

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 435706
Conc: 10.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

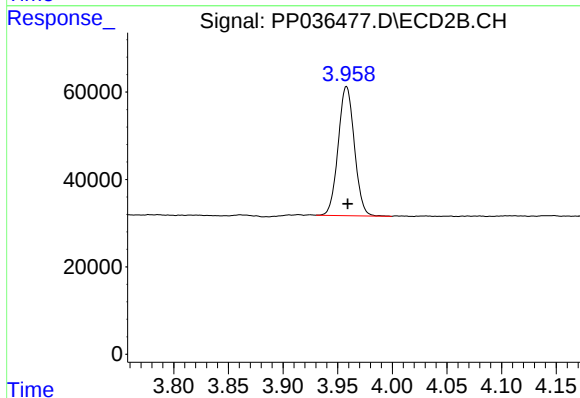


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: -0.001 min
Response: 304895
Conc: 10.15 ng/ml

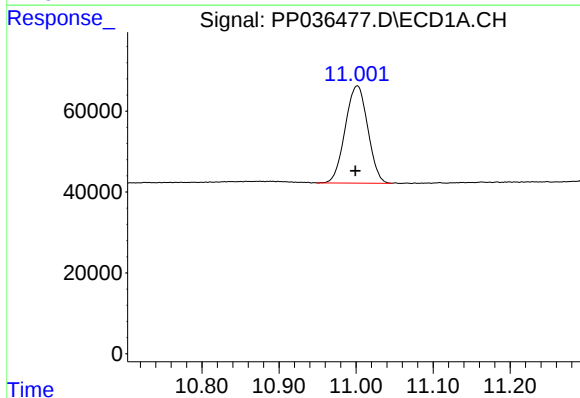


#2 Decachlorobiphenyl

R.T.: 11.002 min
Delta R.T.: 0.003 min
Response: 487670
Conc: 13.51 ng/ml

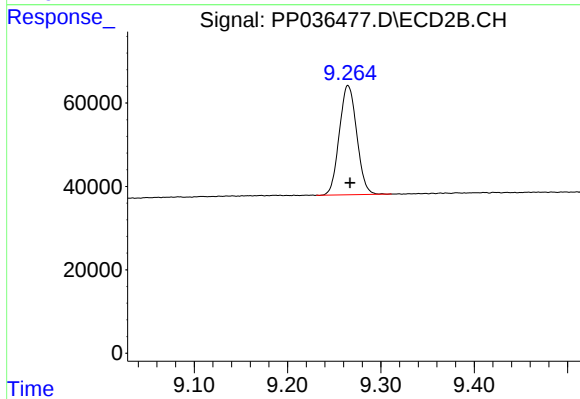

#2 Decachlorobiphenyl


R.T.: 9.265 min
Delta R.T.: -0.002 min
Response: 340418
Conc: 10.66 ng/ml

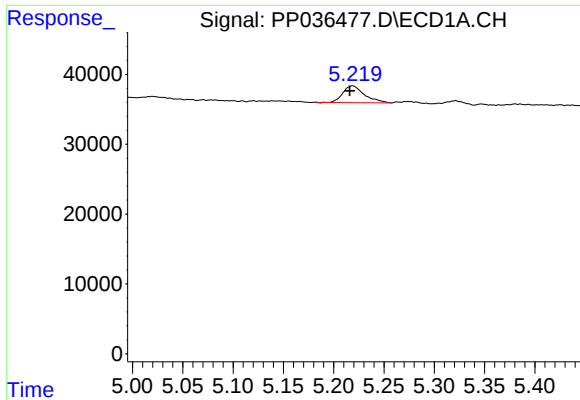

#8 AR-1221-1


R.T.: 5.219 min
Delta R.T.: 0.003 min
Response: 36407
Conc: 73.20 ng/ml

Instrument :
ECD_P
ClientSampleId :

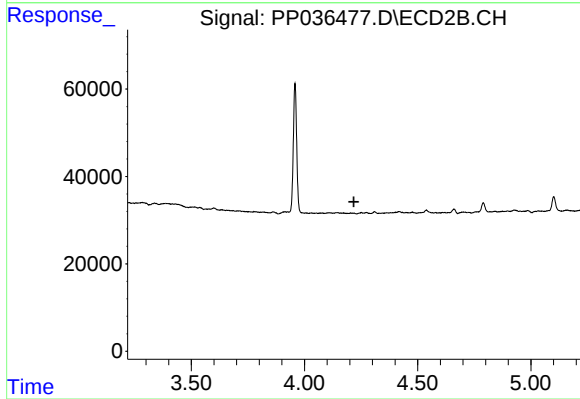


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.218 min
Response: 0
Conc: N.D.

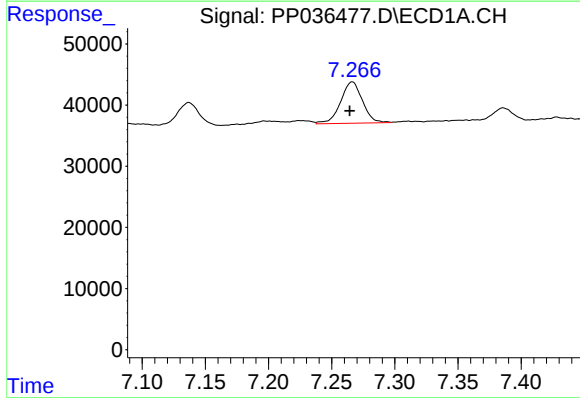


#20 AR-1242-5

R.T.: 7.266 min
Delta R.T.: 0.002 min
Response: 81185
Conc: 86.79 ng/ml

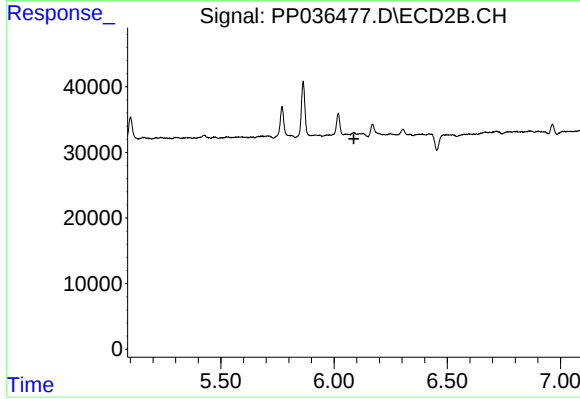

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.087 min
Response: 0
Conc: N.D.

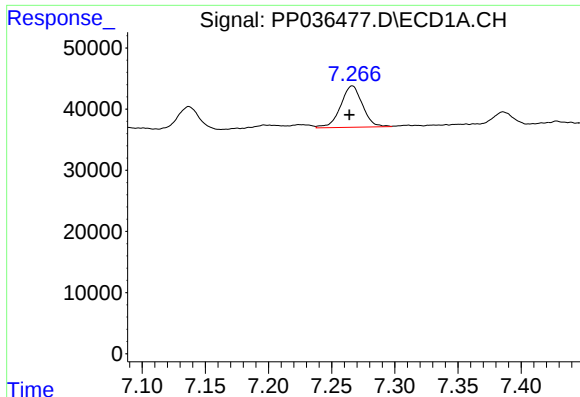

#25 AR-1248-5


R.T.: 7.266 min
Delta R.T.: 0.002 min
Response: 81185
Conc: 50.95 ng/ml

Instrument :
ECD_P
ClientSampleId :

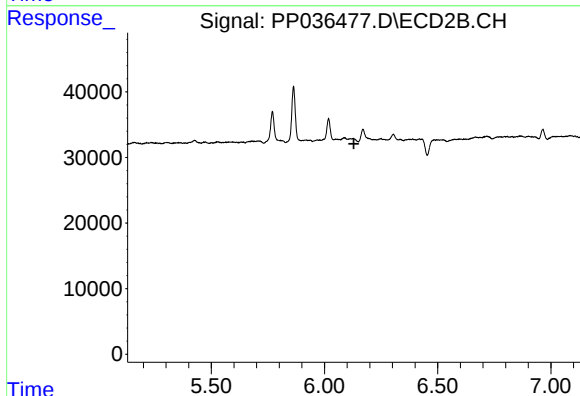


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.130 min
Response: 0
Conc: N.D.

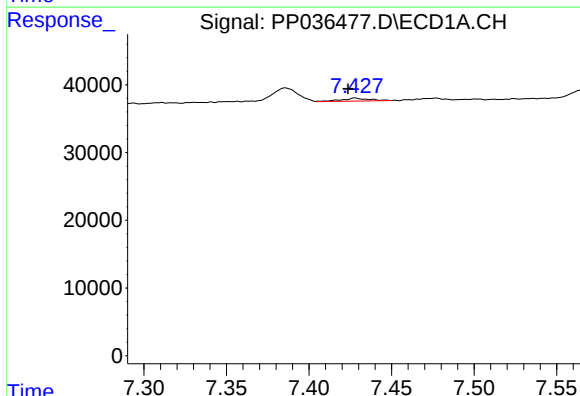


#27 AR-1254-2

R.T.: 7.428 min
Delta R.T.: 0.004 min
Response: 4877
Conc: 1.92 ng/ml

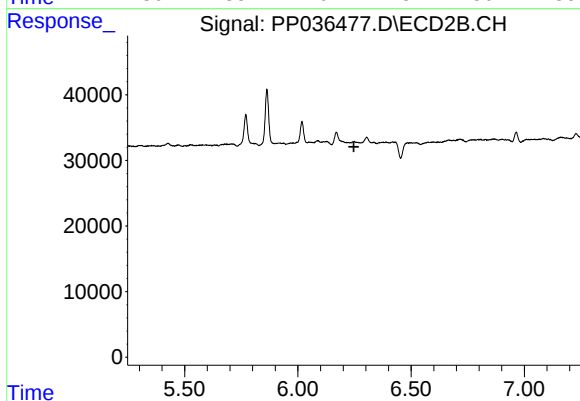

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.247 min
Response: 0
Conc: N.D.

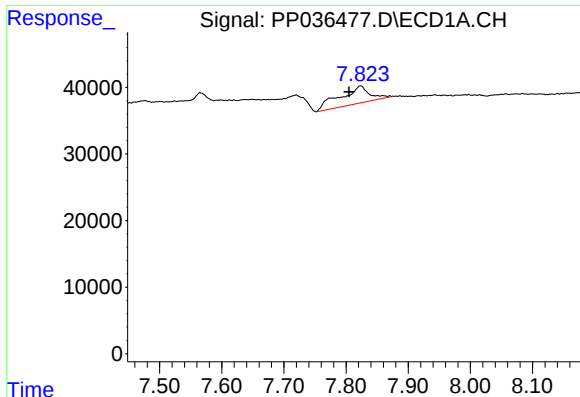

#28 AR-1254-3


R.T.: 7.823 min
Delta R.T.: 0.018 min
Response: 86748
Conc: 31.25 ng/ml

Instrument :
ECD_P
ClientSampleId :

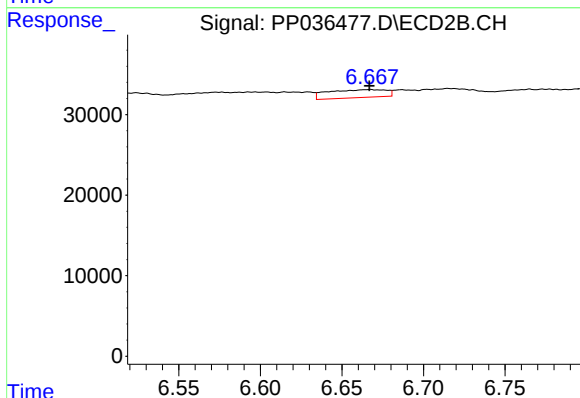


#28 AR-1254-3

R.T.: 6.667 min
Delta R.T.: 0.000 min
Response: 24537
Conc: 10.21 ng/ml

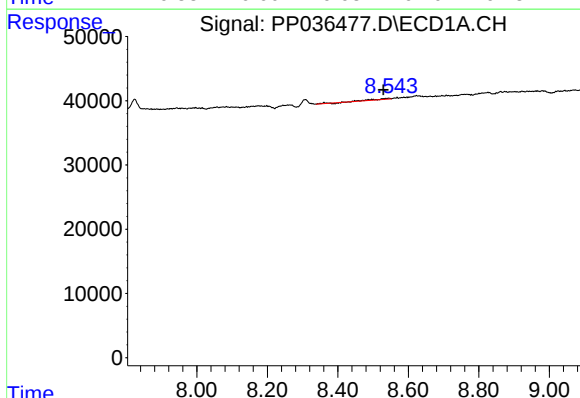


#30 AR-1254-5

R.T.: 8.544 min
Delta R.T.: 0.015 min
Response: 5290
Conc: 2.27 ng/ml

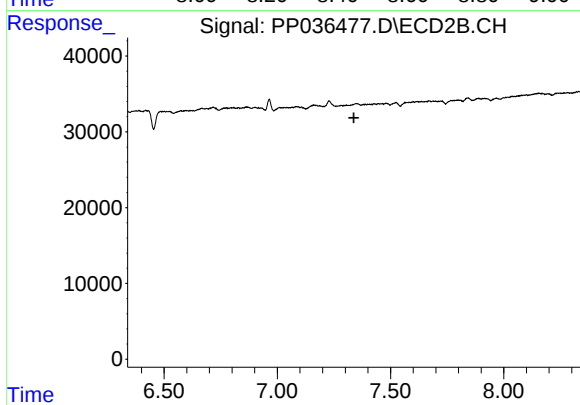

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

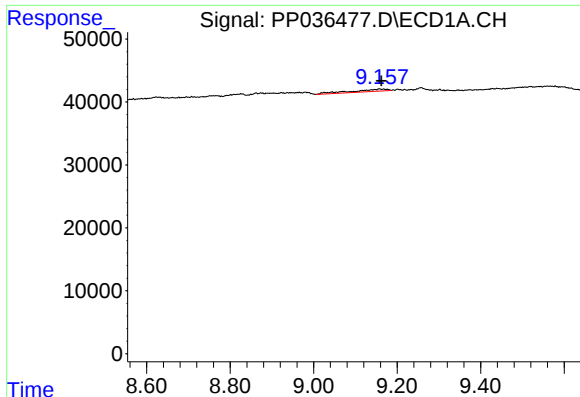

#35 AR-1260-5


R.T.: 9.157 min
Delta R.T.: -0.005 min
Response: 21974
Conc: 5.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

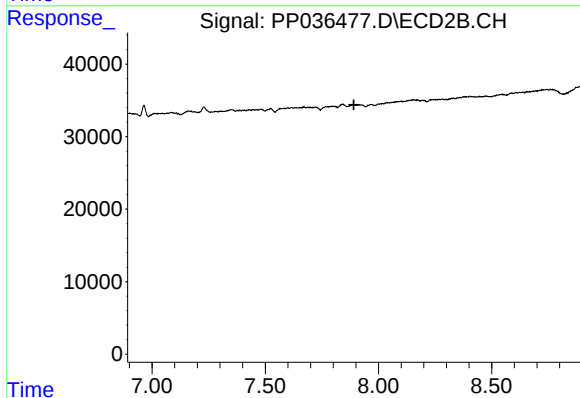


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.891 min
Response: 0
Conc: N.D.

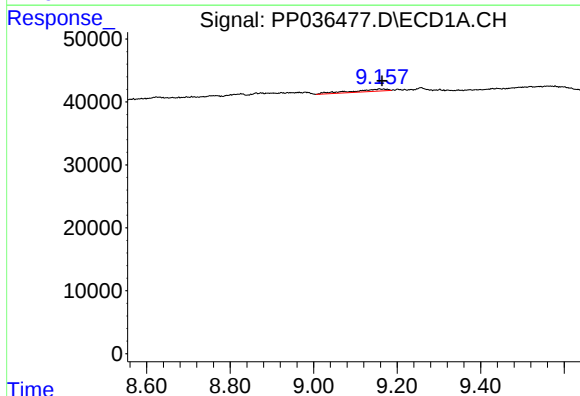

#37 AR-1262-2

R.T.: 9.157 min
Delta R.T.: -0.007 min
Response: 21974
Conc: 4.60 ng/ml

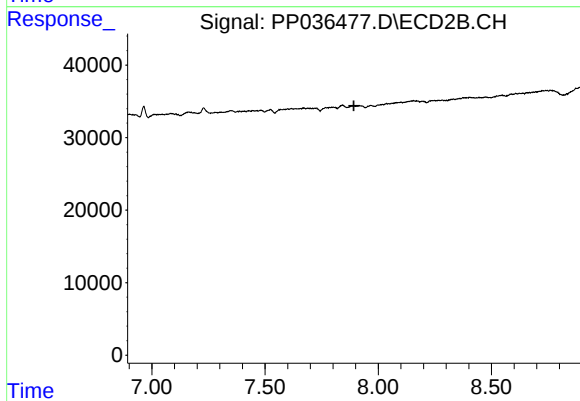

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.892 min
Response: 0
Conc: N.D.