

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061621\
 Data File : PP036478.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jun 2021 12:14
 Operator : DD\AJ
 Sample : M2718-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 13:14:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 12 04:04:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.959	479529	330163	11.357	10.992
2)	SA Decachlor...	11.000	9.265	555669	381007	15.388	11.926
Target Compounds							
7)	L1 AR-1016-5	6.798	0.000	9044	0	8.873	N.D. #
20)	L4 AR-1242-5	7.266	6.086	21778	16312	23.281	20.489
23)	L5 AR-1248-3	6.798	0.000	9044	0	6.335	N.D. #
24)	L5 AR-1248-4	7.227	0.000	23246	0	14.199	N.D. #
25)	L5 AR-1248-5	7.266	6.130	21778	11644	13.668	10.636
26)	L6 AR-1254-1	7.196	6.086	21426	16312	13.015	10.015
27)	L6 AR-1254-2	7.431	0.000	38668	0	15.224	N.D. #
28)	L6 AR-1254-3	7.823f	0.000	90646	0	32.659	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061621\
Data File : PP036478.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jun 2021 12:14
Operator : DD\AJ
Sample : M2718-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 13:14:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061121.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 12 04:04:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

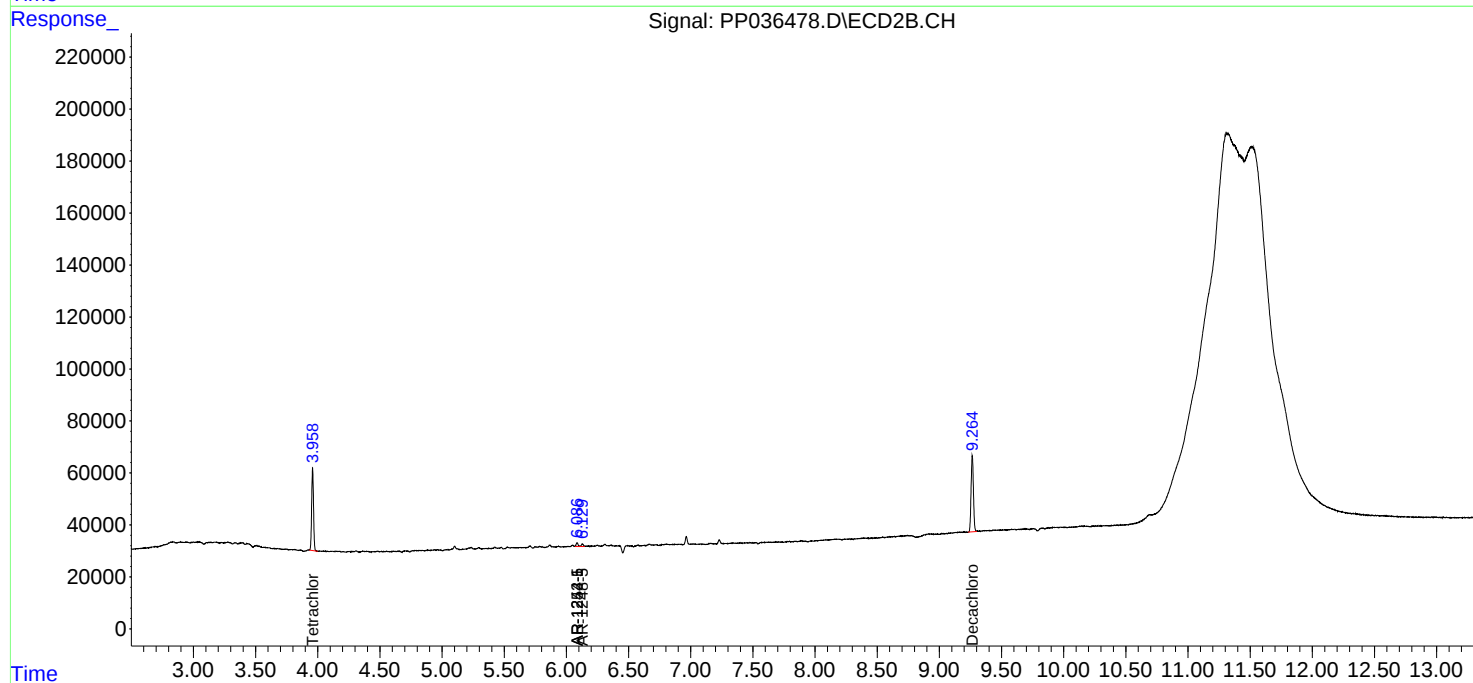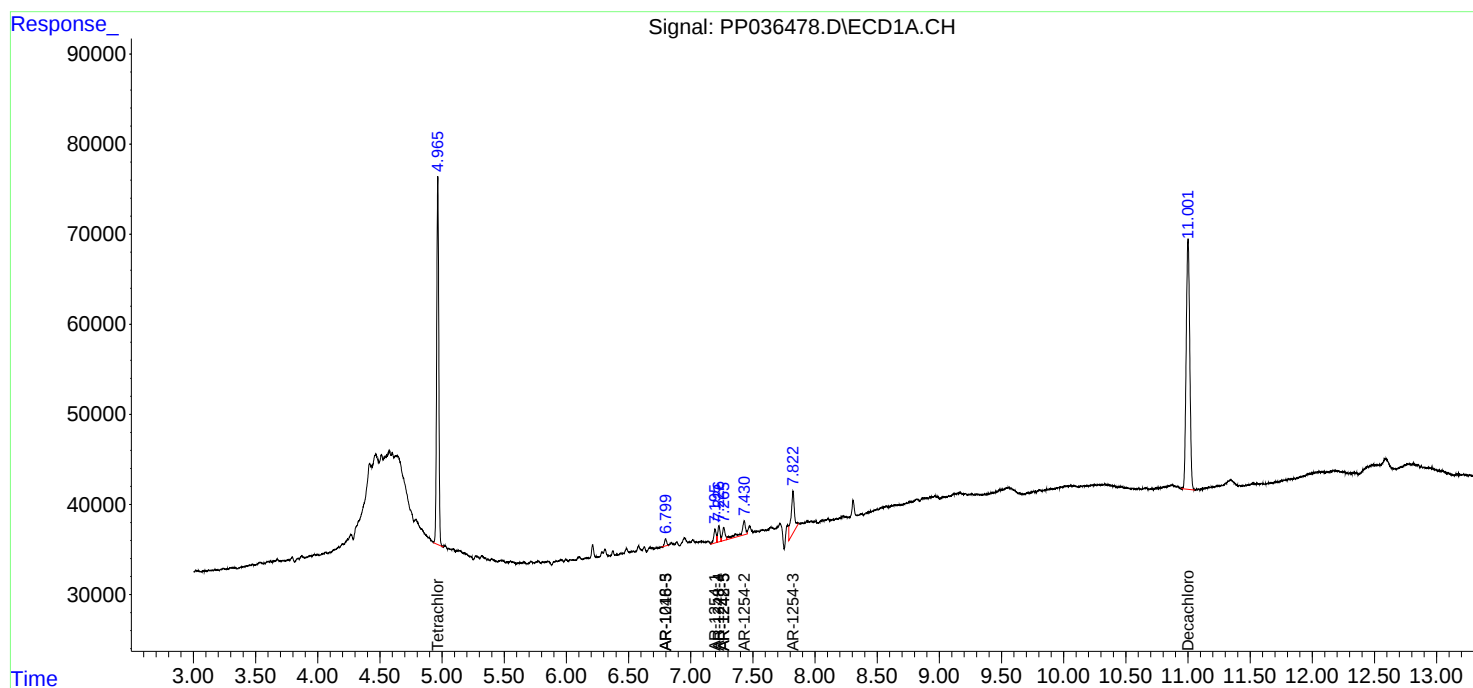


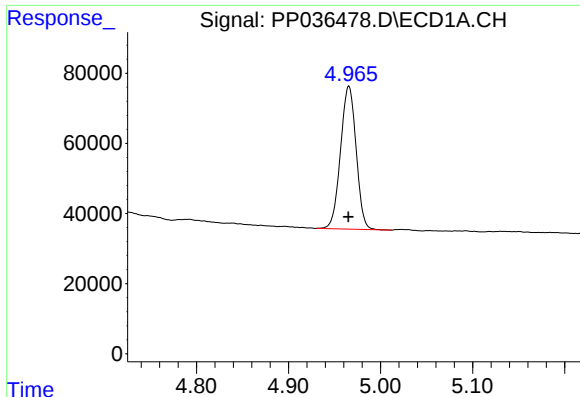

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 479529
Conc: 11.36 ng/ml

Instrument :
ECD_P
ClientSampleId :

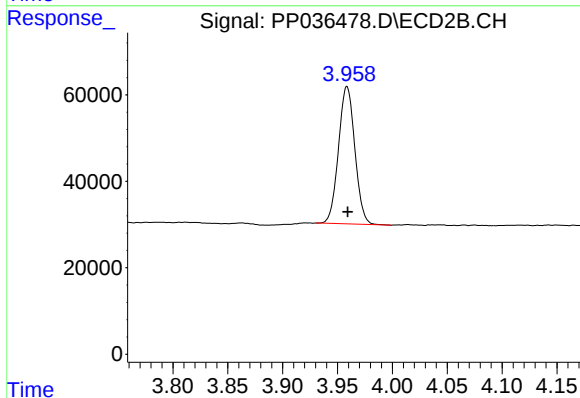


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 330163
Conc: 10.99 ng/ml

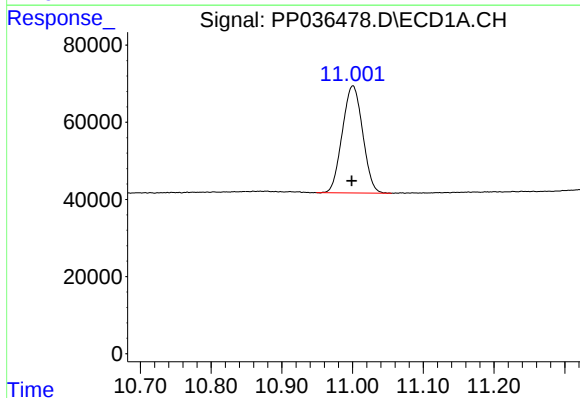


#2 Decachlorobiphenyl

R.T.: 11.000 min
Delta R.T.: 0.001 min
Response: 555669
Conc: 15.39 ng/ml

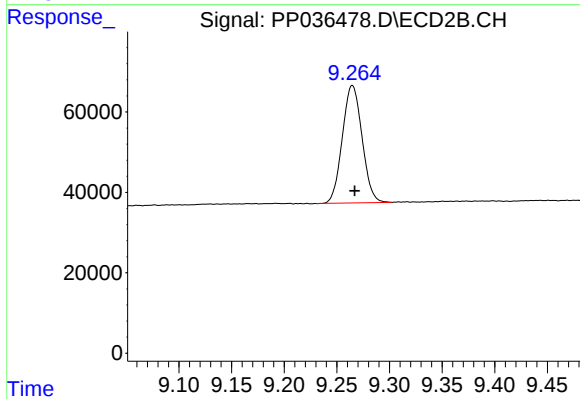

#2 Decachlorobiphenyl


R.T.: 9.265 min
Delta R.T.: -0.002 min
Response: 381007
Conc: 11.93 ng/ml

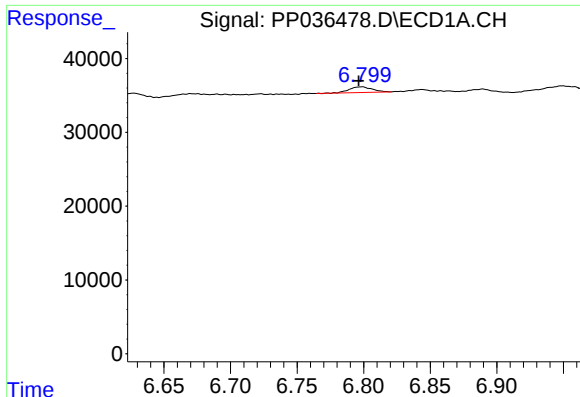

#7 AR-1016-5


R.T.: 6.798 min
Delta R.T.: 0.002 min
Response: 9044
Conc: 8.87 ng/ml

Instrument :
ECD_P
ClientSampleId :

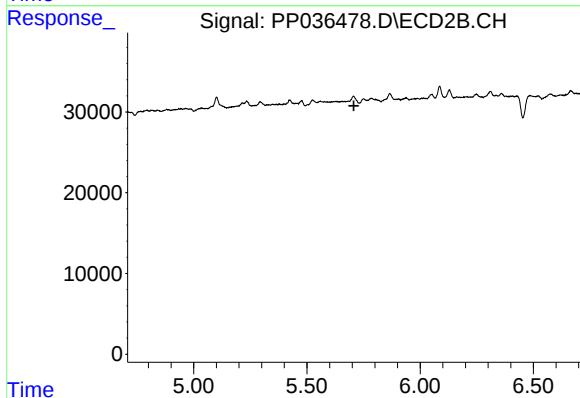


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.707 min
Response: 0
Conc: N.D.

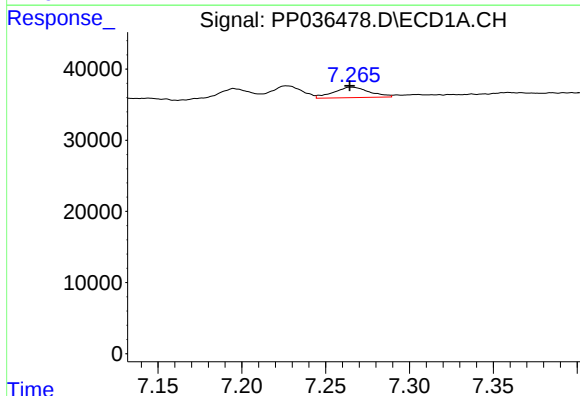


#20 AR-1242-5

R.T.: 7.266 min
Delta R.T.: 0.001 min
Response: 21778
Conc: 23.28 ng/ml

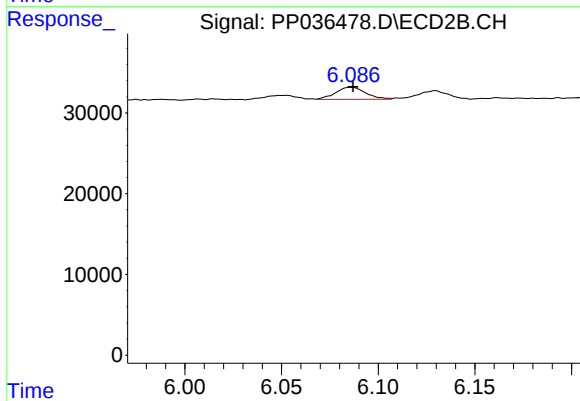

#20 AR-1242-5


R.T.: 6.086 min
Delta R.T.: -0.001 min
Response: 16312
Conc: 20.49 ng/ml

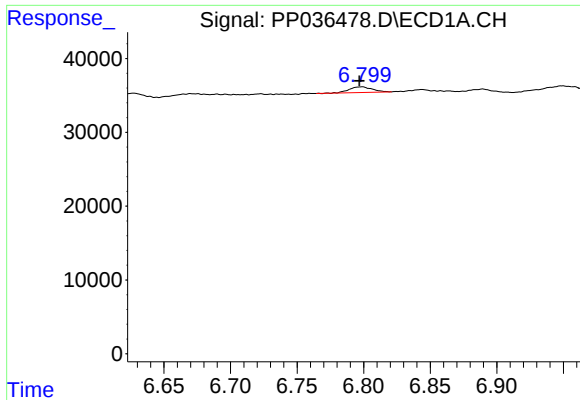

#23 AR-1248-3


R.T.: 6.798 min
Delta R.T.: 0.002 min
Response: 9044
Conc: 6.33 ng/ml

Instrument :
ECD_P
ClientSampleId :

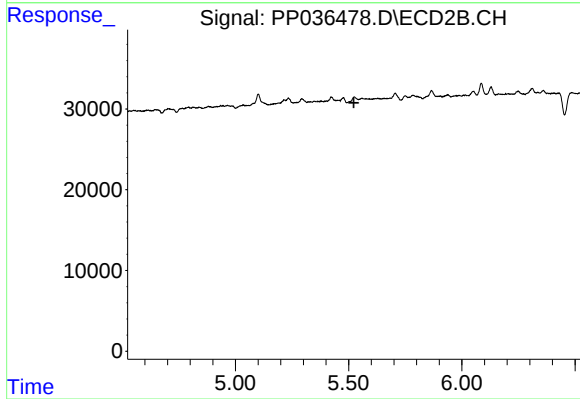


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.523 min
Response: 0
Conc: N.D.

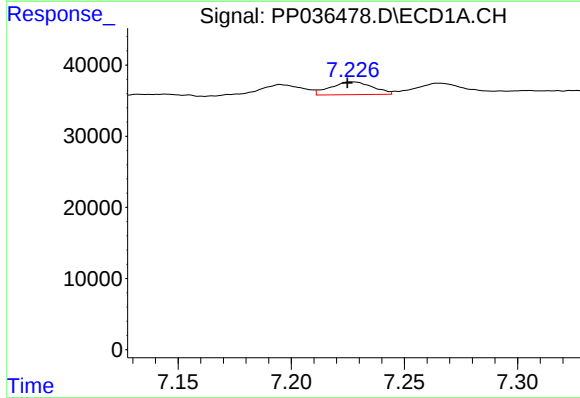


#24 AR-1248-4

R.T.: 7.227 min
Delta R.T.: 0.002 min
Response: 23246
Conc: 14.20 ng/ml

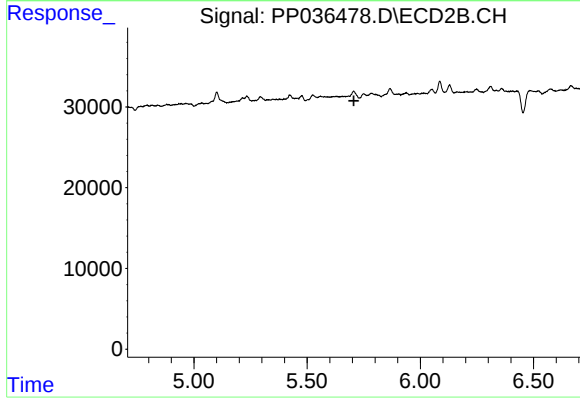

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.706 min
Response: 0
Conc: N.D.

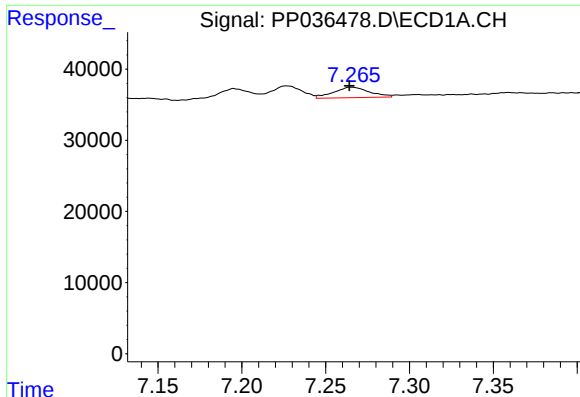

#25 AR-1248-5


R.T.: 7.266 min
Delta R.T.: 0.001 min
Response: 21778
Conc: 13.67 ng/ml

Instrument :
ECD_P
ClientSampleId :

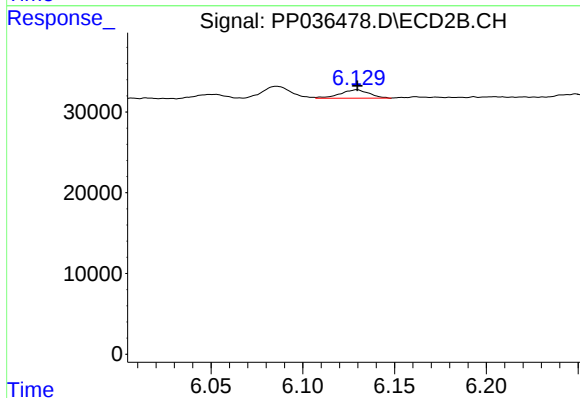


#25 AR-1248-5

R.T.: 6.130 min
Delta R.T.: 0.000 min
Response: 11644
Conc: 10.64 ng/ml

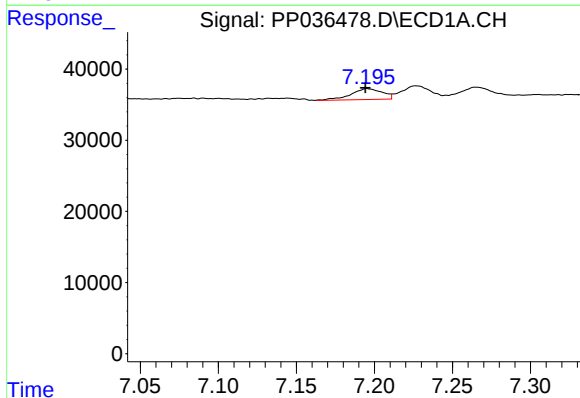


#26 AR-1254-1

R.T.: 7.196 min
Delta R.T.: 0.001 min
Response: 21426
Conc: 13.01 ng/ml

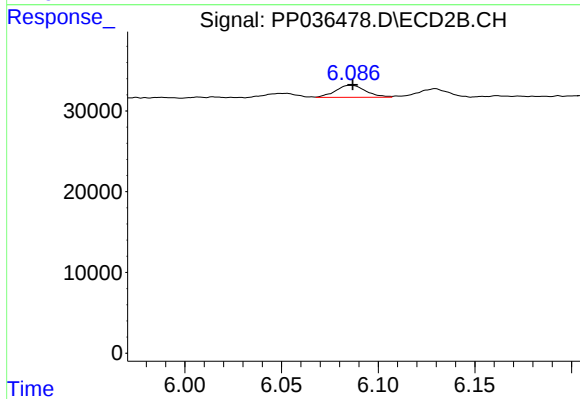

#26 AR-1254-1


R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 16312
Conc: 10.01 ng/ml

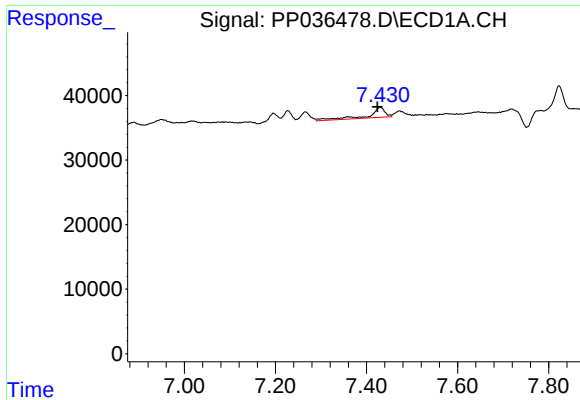

#27 AR-1254-2


R.T.: 7.431 min
Delta R.T.: 0.007 min
Response: 38668
Conc: 15.22 ng/ml

Instrument :
ECD_P
ClientSampleId :

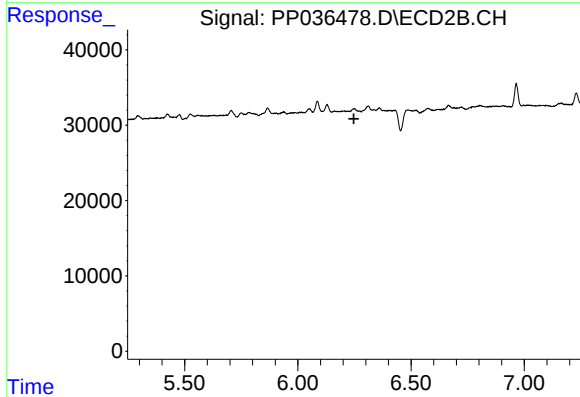


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.247 min
Response: 0
Conc: N.D.

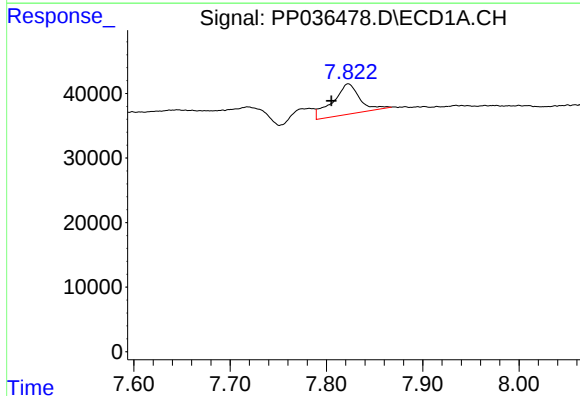

#28 AR-1254-3

R.T.: 7.823 min
Delta R.T.: 0.018 min
Response: 90646
Conc: 32.66 ng/ml

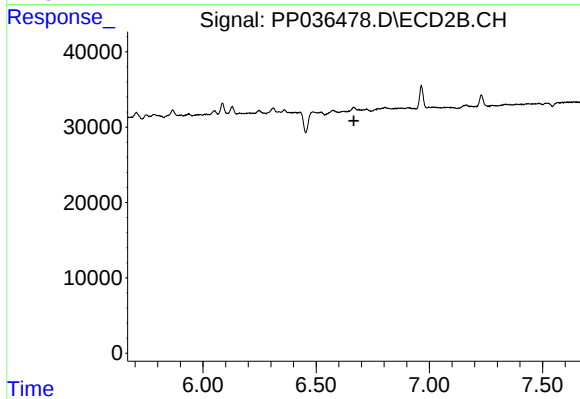

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.