

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061625\
 Data File : PP072971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2025 14:05
 Operator : YP\AJ
 Sample : Q2323-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PL-01-06132025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/17/2025
 Supervised By :mohammad ahmed 06/18/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 01:45:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.790	30289969	30134198	15.064m	18.853 #
2) SA Decachlor...	10.186	8.799	26933024	21497368	16.532m	20.307m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061625\
Data File : PP072971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2025 14:05
Operator : YP\AJ
Sample : Q2323-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleID :
PL-01-06132025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/17/2025
Supervised By :mohammad ahmed 06/18/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 01:45:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

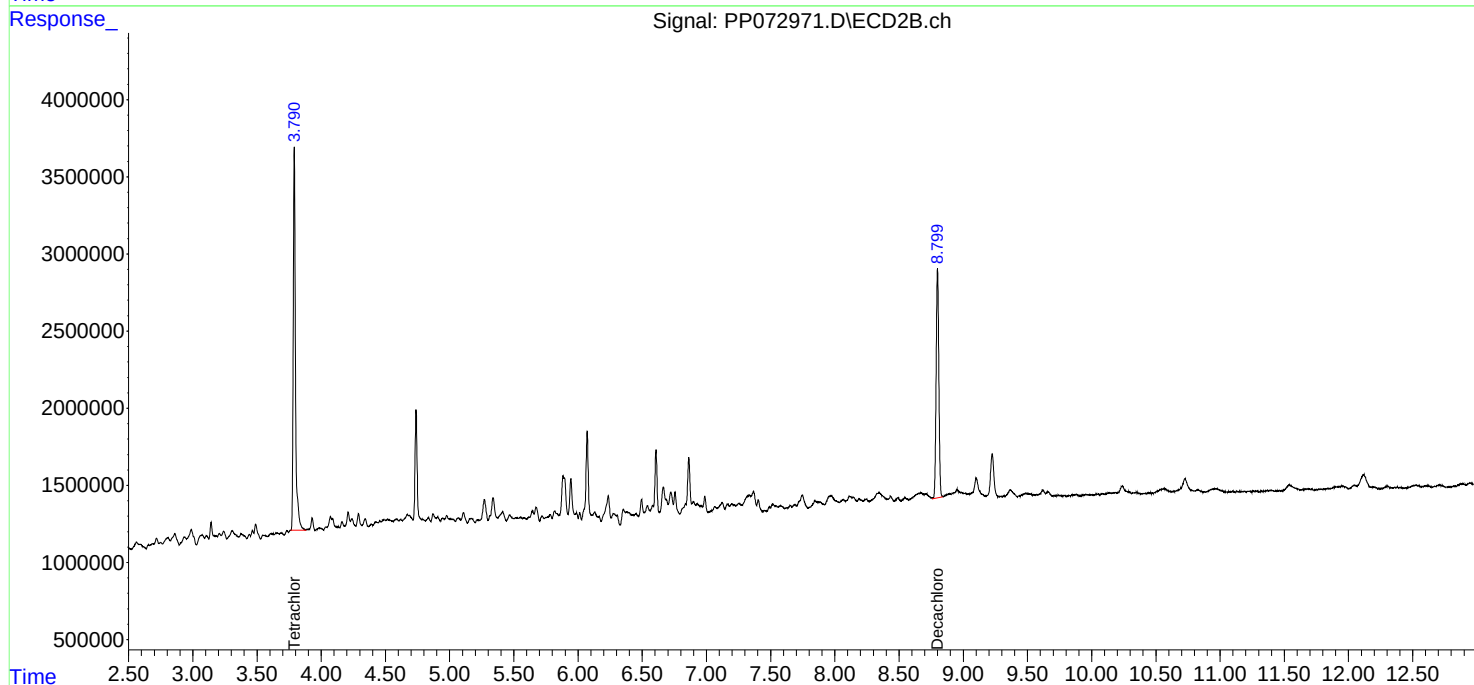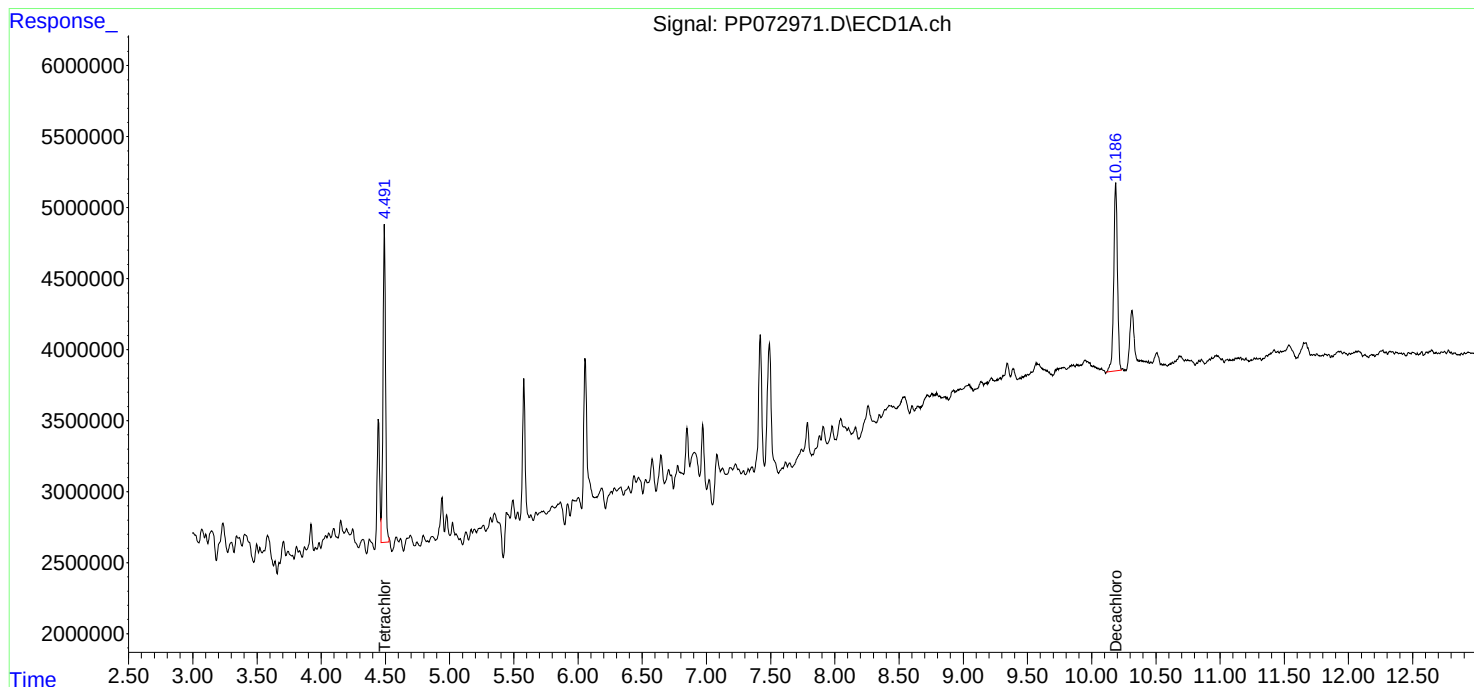

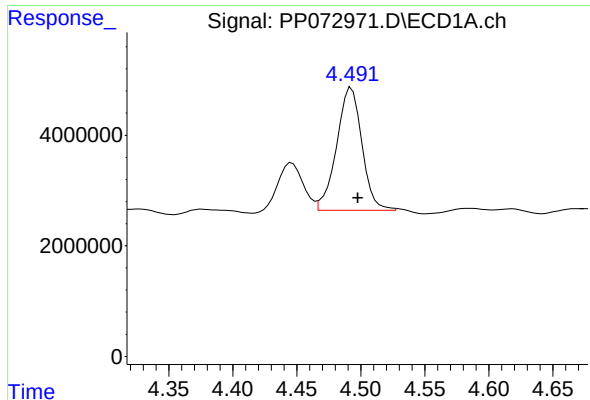


#1 Tetrachloro-m-xylene

R.T.: 4.491 min
Delta R.T.: -0.007 min
Response: 30289969
Conc: 15.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
PL-01-06132025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/17/2025
Supervised By :mohammad ahmed 06/18/2025

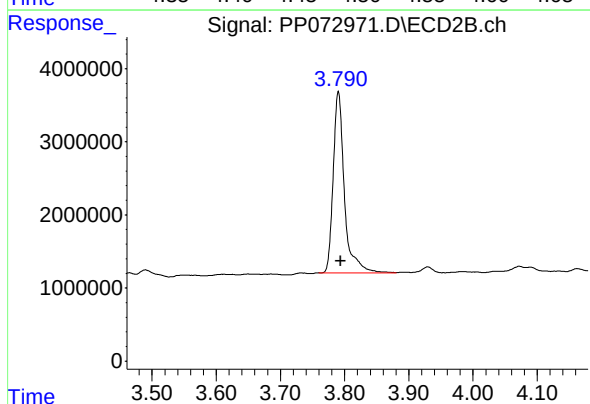


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: -0.003 min
Response: 30134198
Conc: 18.85 ng/ml

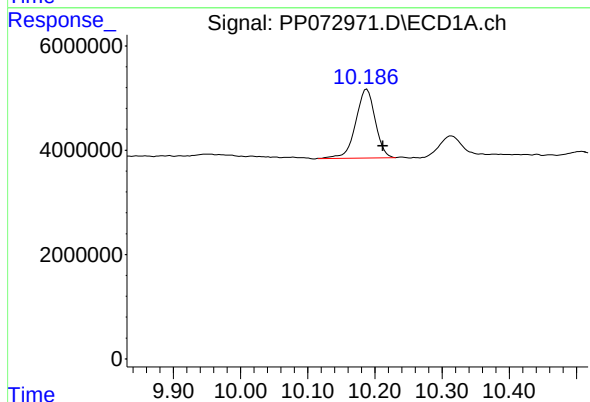

#2 Decachlorobiphenyl

R.T.: 10.186 min
Delta R.T.: -0.026 min
Response: 26933024
Conc: 16.53 ng/ml m

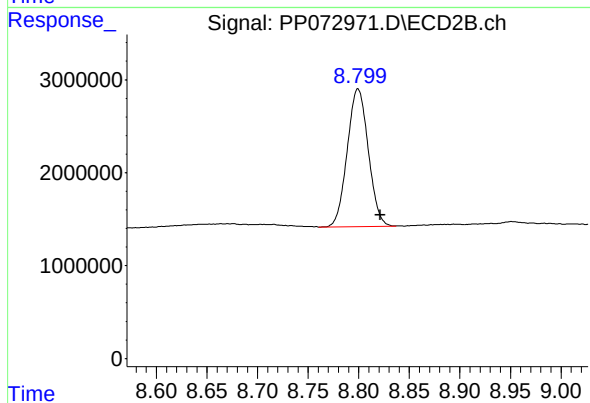

#2 Decachlorobiphenyl

R.T.: 8.799 min
Delta R.T.: -0.022 min
Response: 21497368
Conc: 20.31 ng/ml m