

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061721\
 Data File : PP036497.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jun 2021 17:11
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 06:08:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.959	908495	628885	20.555	20.304
2)	SA Decachlor...	10.998	9.264	967596	681099	22.556	21.297
Target Compounds							
9)	L2 AR-1221-2	0.000	4.308	0	9539	N.D.	31.956 #
15)	L3 AR-1232-5	6.573	0.000	22115	0	60.341	N.D. #
22)	L5 AR-1248-2	6.573	0.000	22115	0	16.284	N.D. #
28)	L6 AR-1254-3	7.823f	0.000	18080	0	6.104	N.D. #
35)	L7 AR-1260-5	9.161	0.000	14344	0	3.215	N.D. #
37)	L8 AR-1262-2	9.161	0.000	14344	0	2.823	N.D. #
39)	L8 AR-1262-4	9.562	0.000	231022	0	80.435	N.D. #
42)	L9 AR-1268-2	9.562	0.000	231022	0	40.528	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061721\
Data File : PP036497.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jun 2021 17:11
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 06:08:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

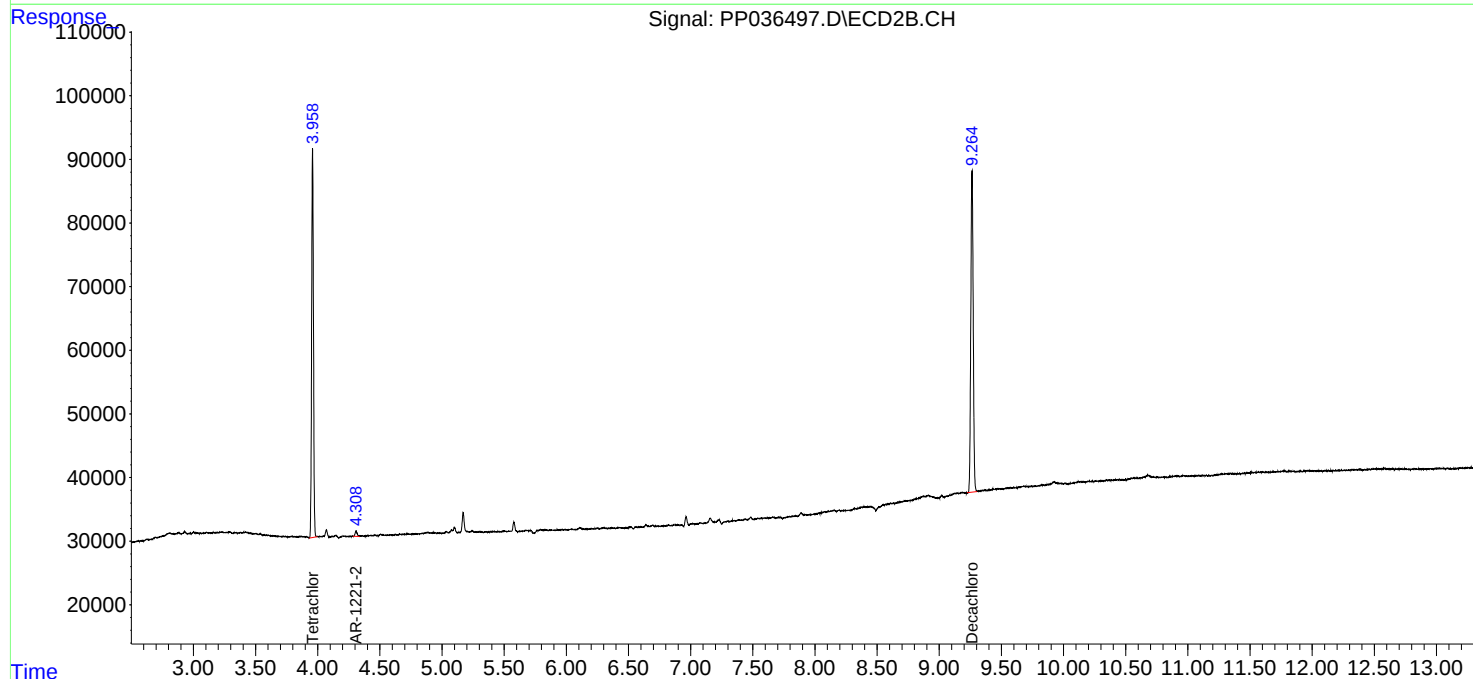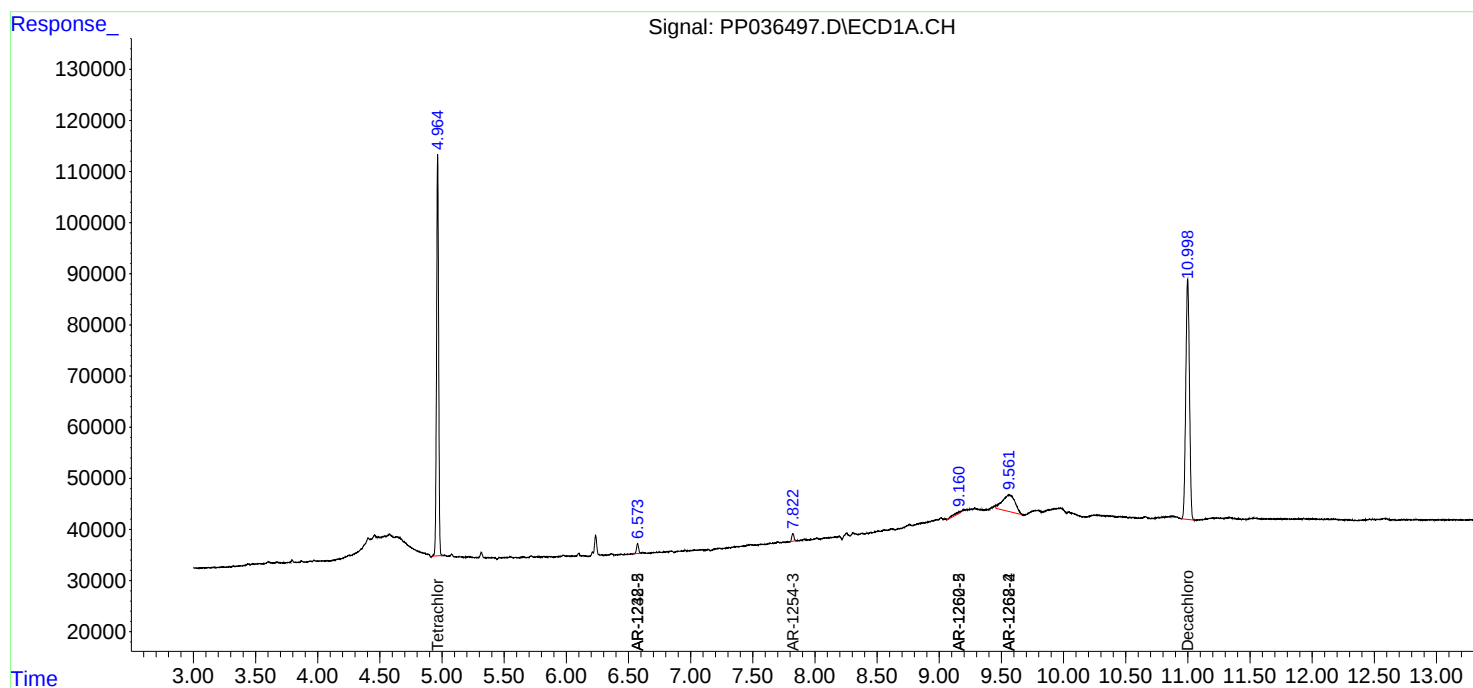


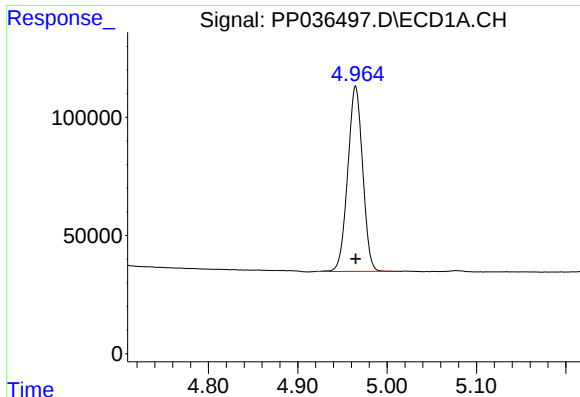

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 908495
Conc: 20.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

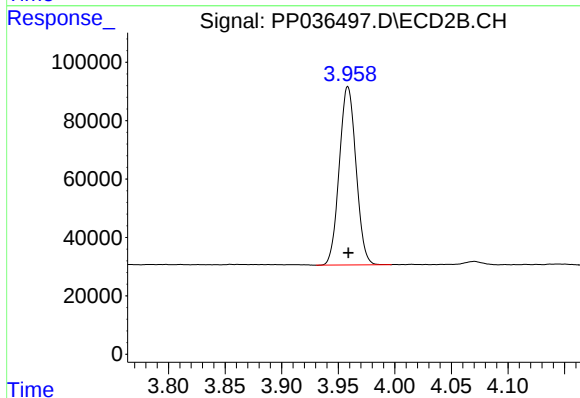


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 628885
Conc: 20.30 ng/ml

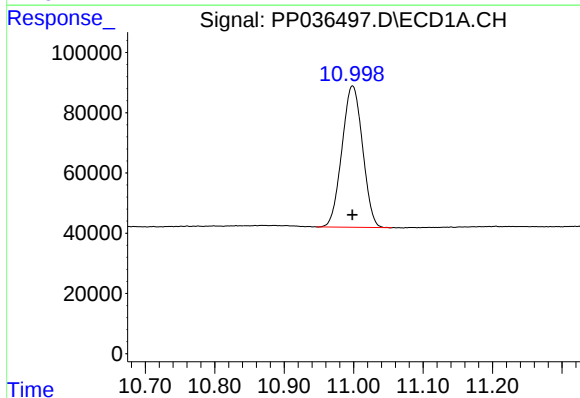


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.000 min
Response: 967596
Conc: 22.56 ng/ml

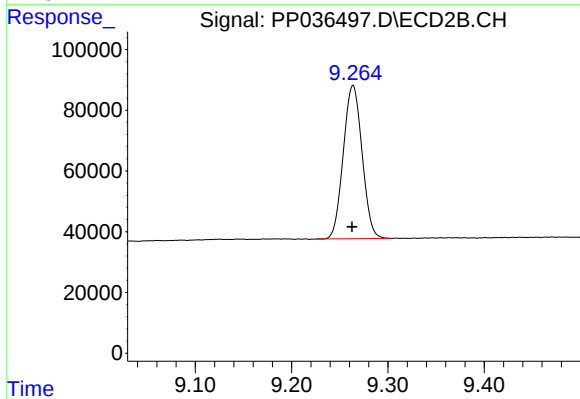

#2 Decachlorobiphenyl


R.T.: 9.264 min
Delta R.T.: 0.000 min
Response: 681099
Conc: 21.30 ng/ml

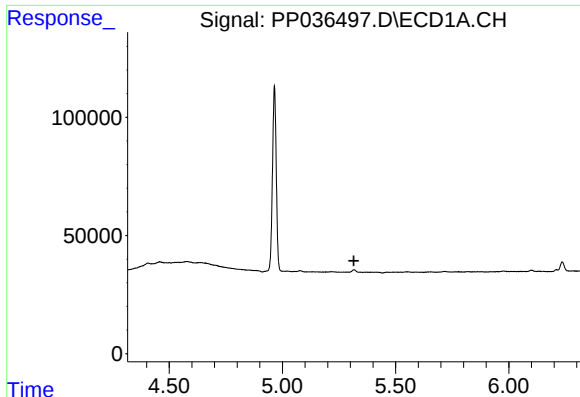

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.315 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

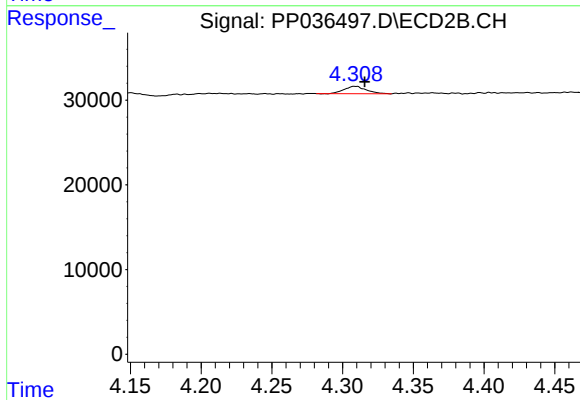


#9 AR-1221-2

R.T.: 4.308 min
Delta R.T.: -0.007 min
Response: 9539
Conc: 31.96 ng/ml

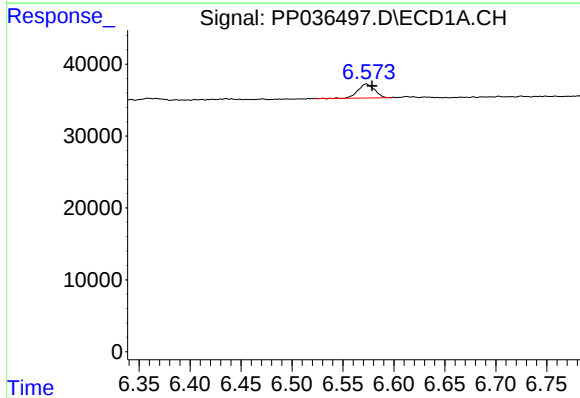


#15 AR-1232-5

R.T.: 6.573 min
Delta R.T.: -0.006 min
Response: 22115
Conc: 60.34 ng/ml

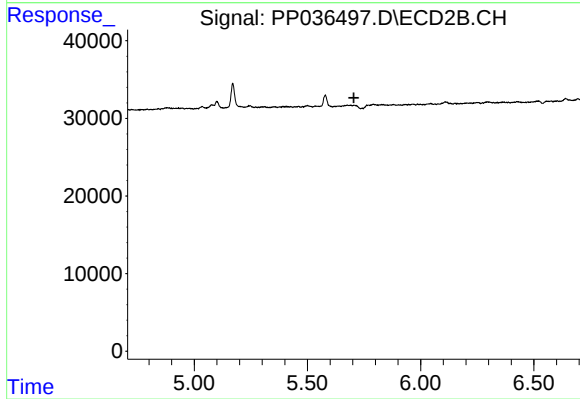

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.705 min
Response: 0
Conc: N.D.

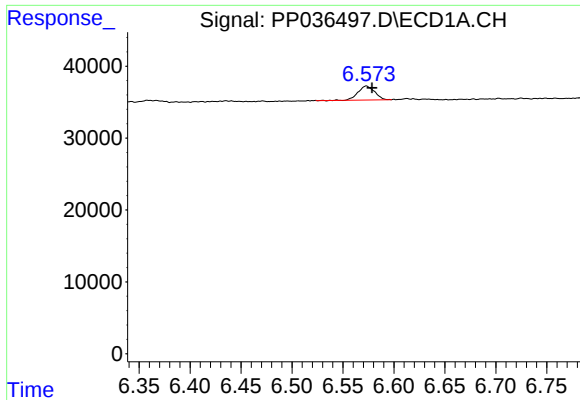

#22 AR-1248-2


R.T.: 6.573 min
Delta R.T.: -0.006 min
Response: 22115
Conc: 16.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

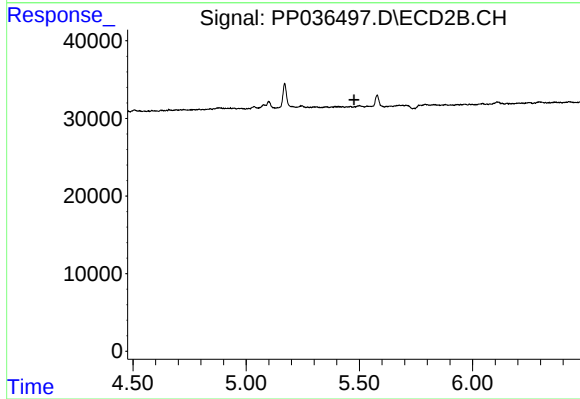


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

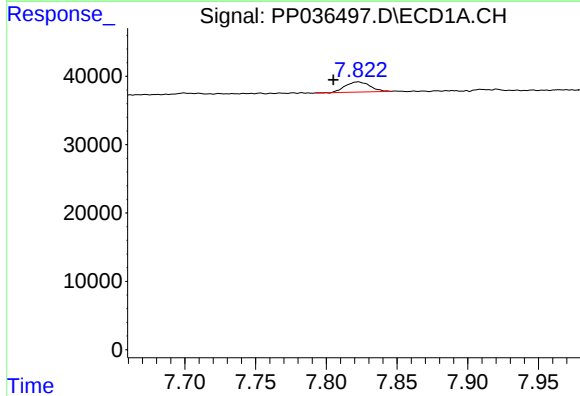


#28 AR-1254-3

R.T.: 7.823 min
Delta R.T.: 0.018 min
Response: 18080
Conc: 6.10 ng/ml

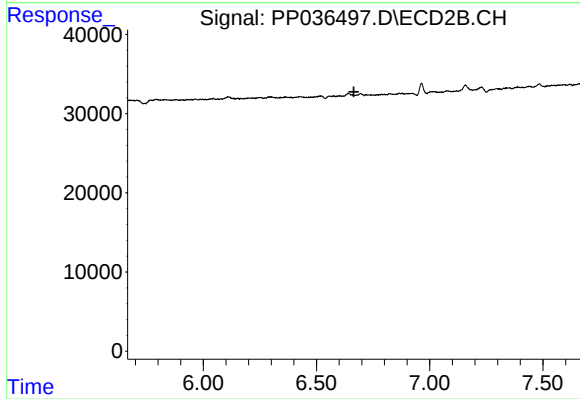

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.

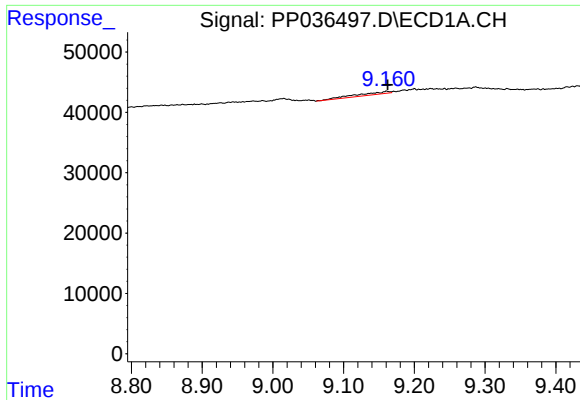

#35 AR-1260-5


R.T.: 9.161 min
Delta R.T.: -0.002 min
Response: 14344
Conc: 3.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

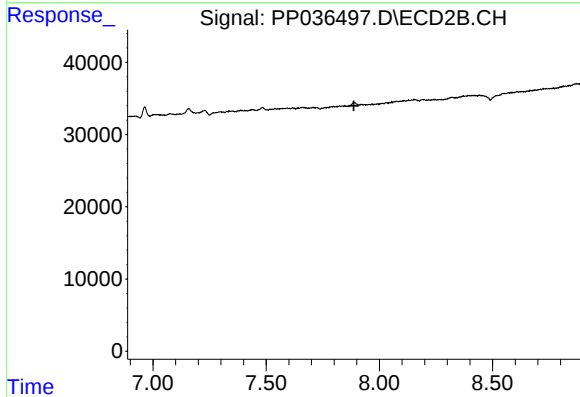


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.888 min
Response: 0
Conc: N.D.

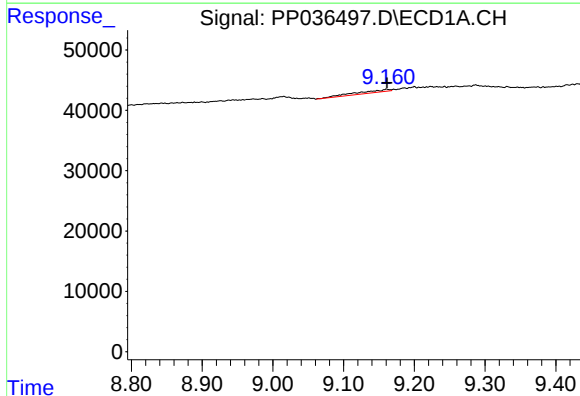


#37 AR-1262-2

R.T.: 9.161 min
Delta R.T.: -0.001 min
Response: 14344
Conc: 2.82 ng/ml

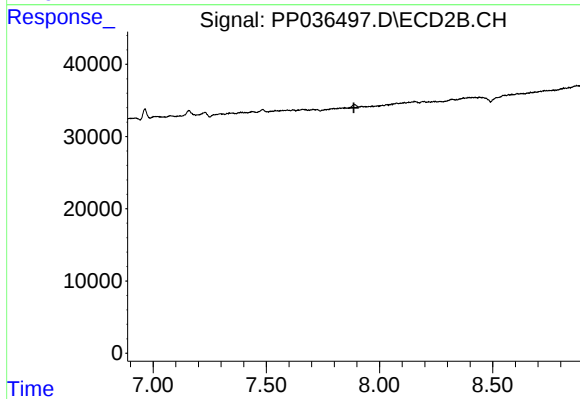

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.887 min
Response: 0
Conc: N.D.

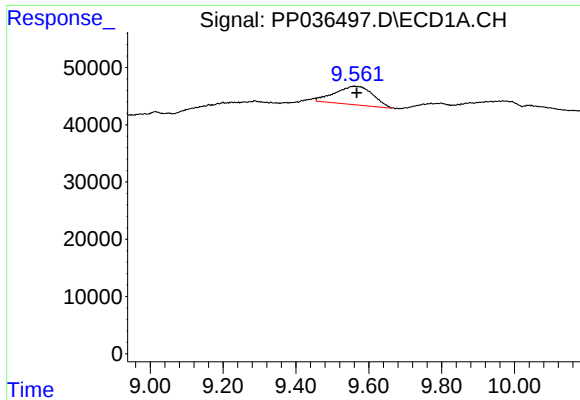

#39 AR-1262-4


R.T.: 9.562 min
Delta R.T.: -0.005 min
Response: 231022
Conc: 80.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

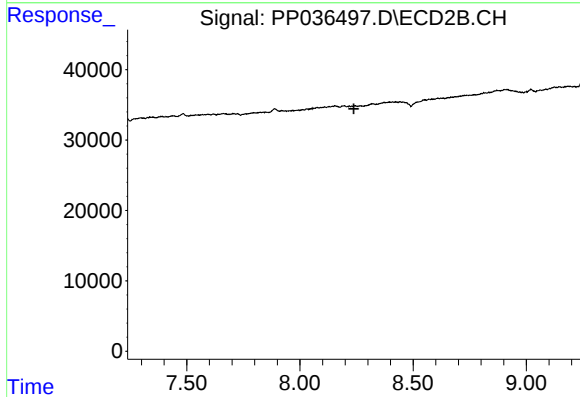


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.238 min
Response: 0
Conc: N.D.

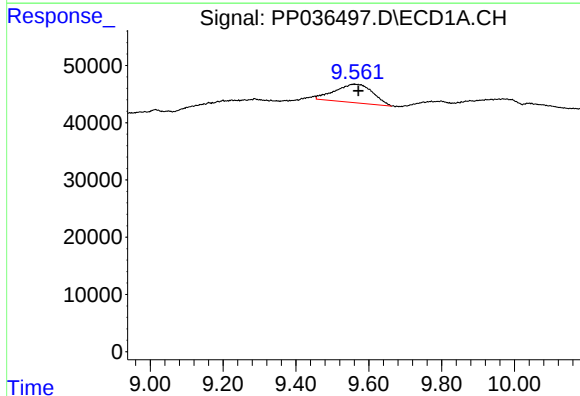

#42 AR-1268-2

R.T.: 9.562 min
Delta R.T.: -0.010 min
Response: 231022
Conc: 40.53 ng/ml

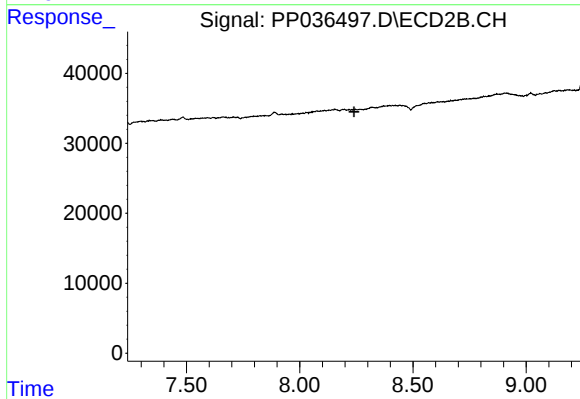

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.240 min
Response: 0
Conc: N.D.