

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036547.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 10:00
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:49:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
20)	L4	AR-1242-5	7.260	6.110f	4412	36599	4.194 44.858 #
24)	L5	AR-1248-4	7.239	0.000	2777	0	1.521 N.D. #
25)	L5	AR-1248-5	7.260	6.110f	4412	36599	2.447 30.855 #
26)	L6	AR-1254-1	7.204	6.110f	51596	36599	29.338 21.601 #
28)	L6	AR-1254-3	7.824f	6.651	33544	5448	11.325 2.241 #
32)	L7	AR-1260-2	8.262f	0.000	36513	0	14.246 N.D. #
38)	L8	AR-1262-3	0.000	8.166	0	44095	N.D. 27.708 #
41)	L9	AR-1268-1	0.000	8.166	0	44095	N.D. 9.469 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036547.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 10:00
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:49:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

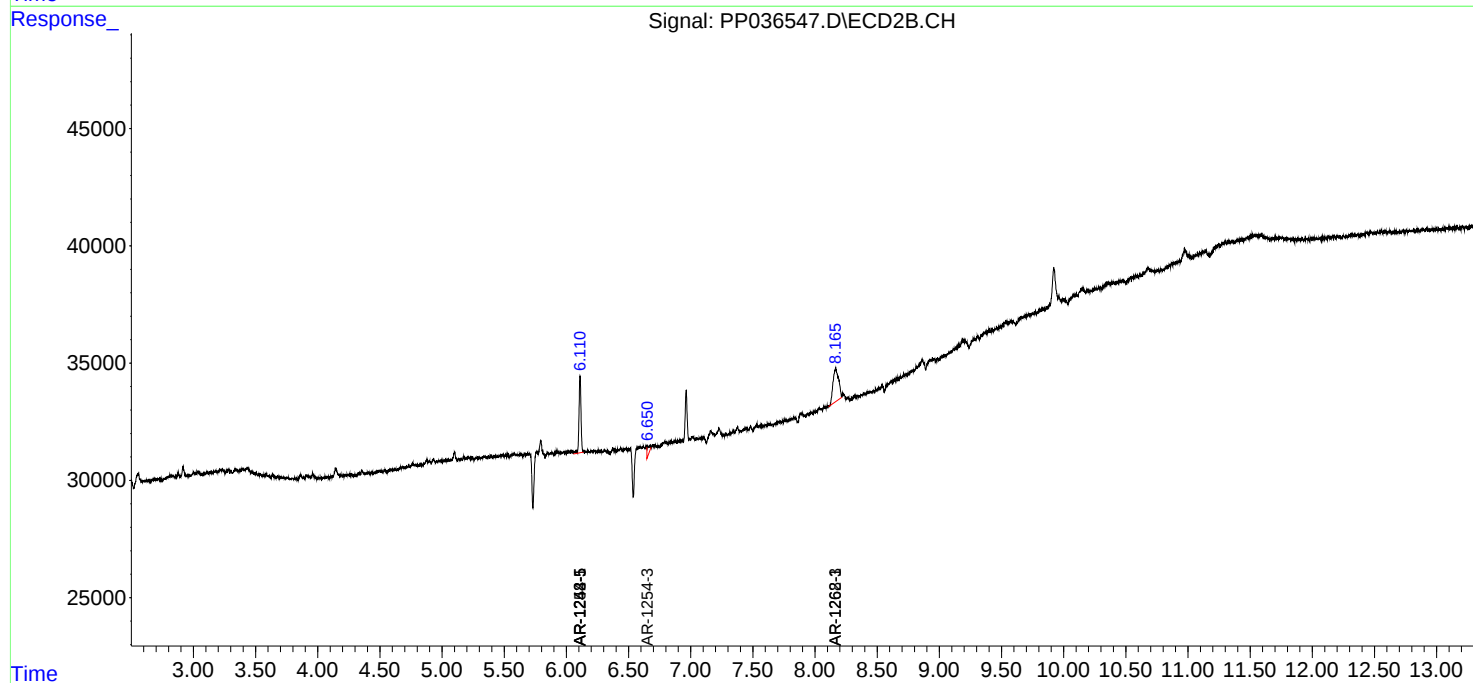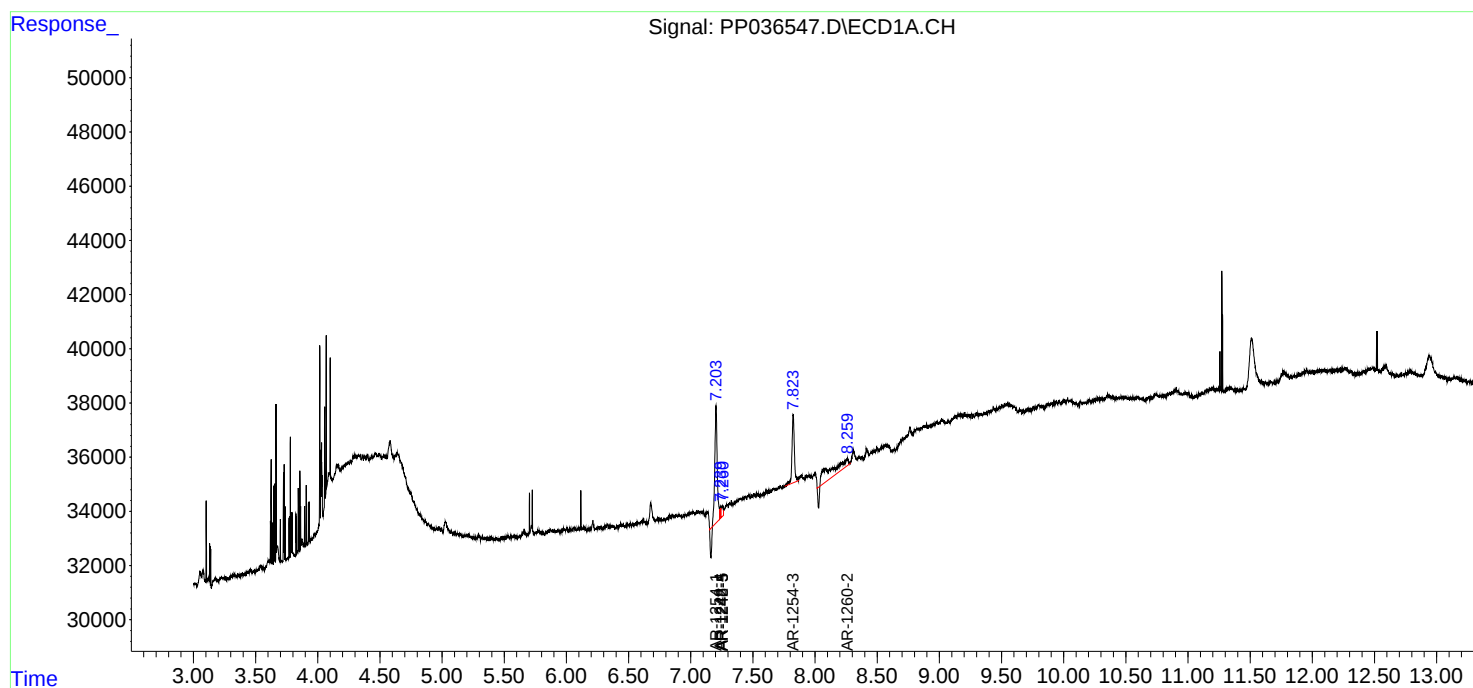


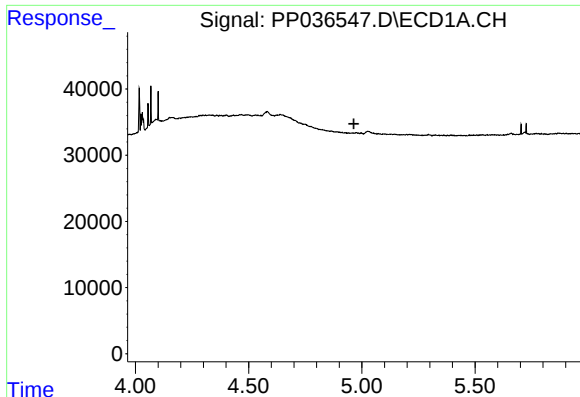

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

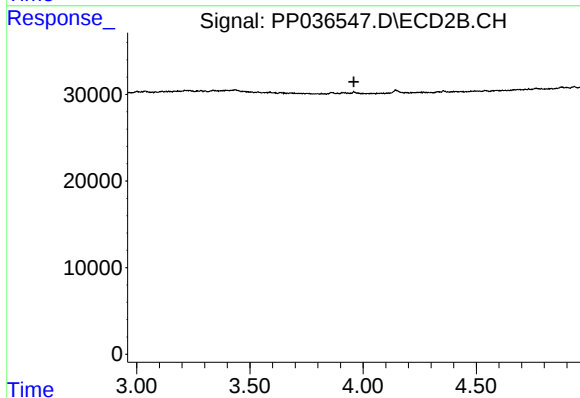


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.959 min
Response: 0
Conc: N.D.

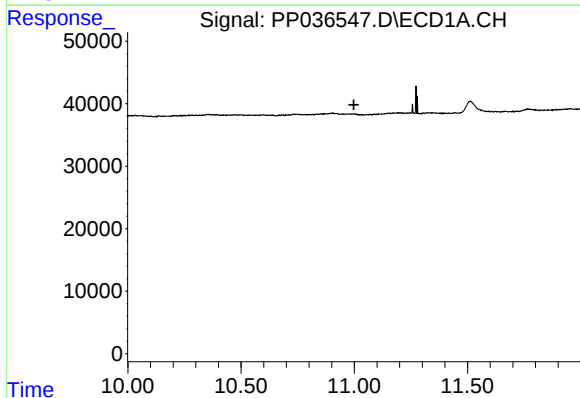


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.998 min
Response: 0
Conc: N.D.

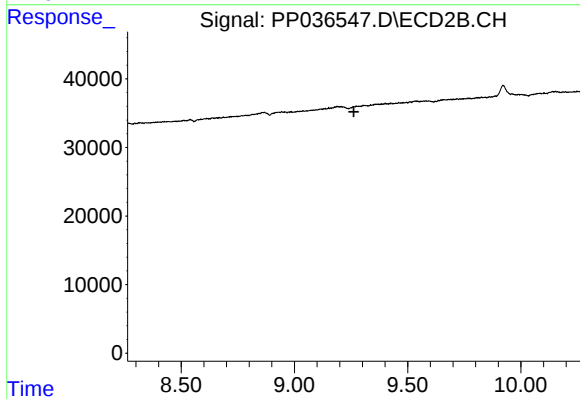

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.263 min
Response: 0
Conc: N.D.

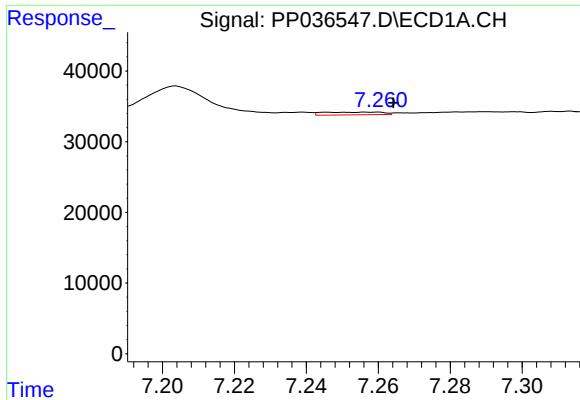

#20 AR-1242-5


R.T.: 7.260 min
Delta R.T.: -0.004 min
Response: 4412
Conc: 4.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

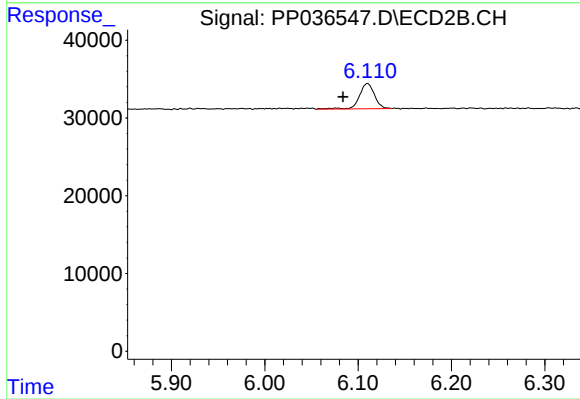


#20 AR-1242-5

R.T.: 6.110 min
Delta R.T.: 0.026 min
Response: 36599
Conc: 44.86 ng/ml

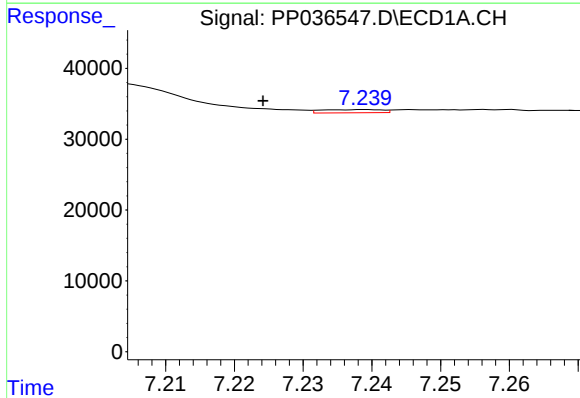


#24 AR-1248-4

R.T.: 7.239 min
Delta R.T.: 0.015 min
Response: 2777
Conc: 1.52 ng/ml

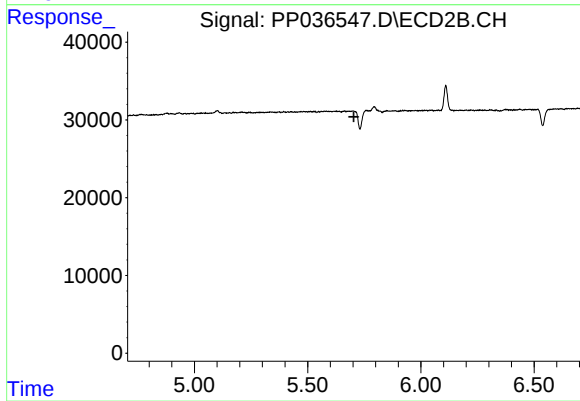

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.704 min
Response: 0
Conc: N.D.

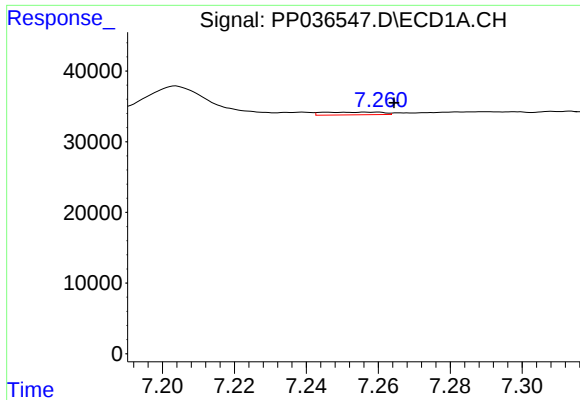

#25 AR-1248-5


R.T.: 7.260 min
Delta R.T.: -0.004 min
Response: 4412
Conc: 2.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

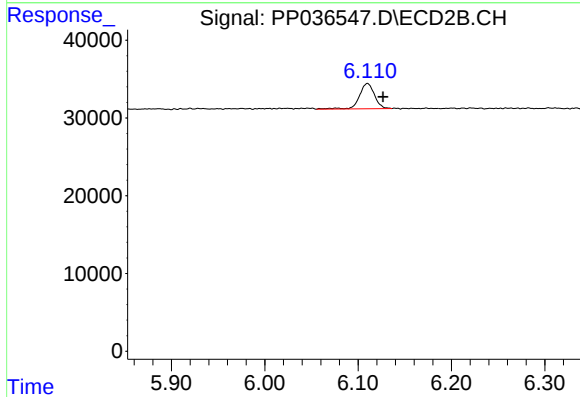


#25 AR-1248-5

R.T.: 6.110 min
Delta R.T.: -0.017 min
Response: 36599
Conc: 30.86 ng/ml

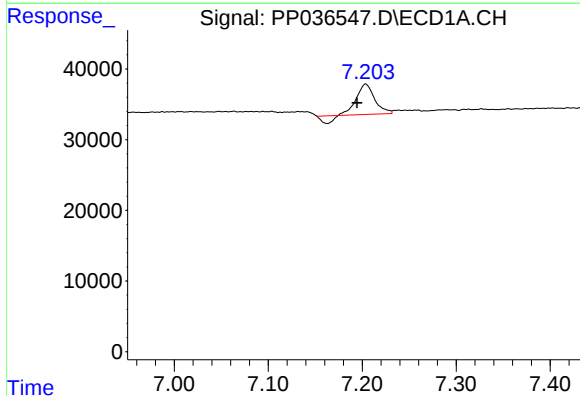


#26 AR-1254-1

R.T.: 7.204 min
Delta R.T.: 0.009 min
Response: 51596
Conc: 29.34 ng/ml

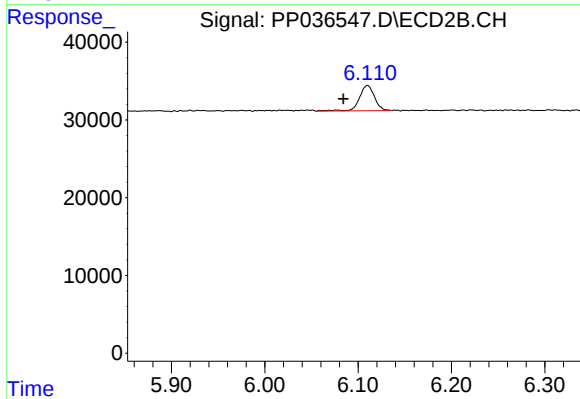

#26 AR-1254-1


R.T.: 6.110 min
Delta R.T.: 0.026 min
Response: 36599
Conc: 21.60 ng/ml

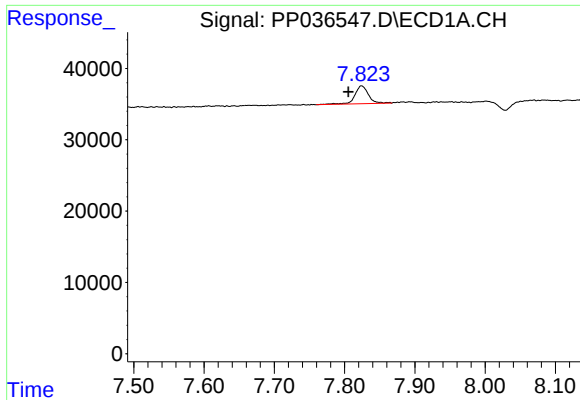

#28 AR-1254-3


R.T.: 7.824 min
Delta R.T.: 0.019 min
Response: 33544
Conc: 11.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

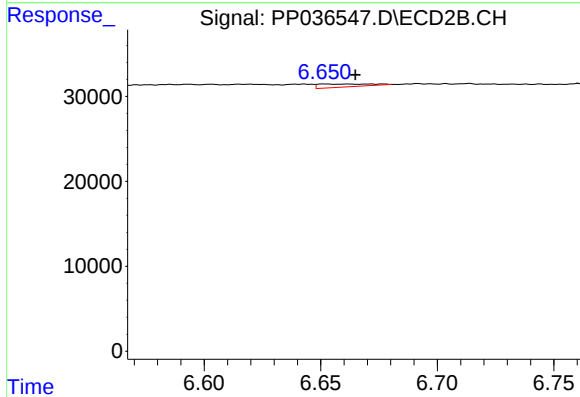


#28 AR-1254-3

R.T.: 6.651 min
Delta R.T.: -0.014 min
Response: 5448
Conc: 2.24 ng/ml

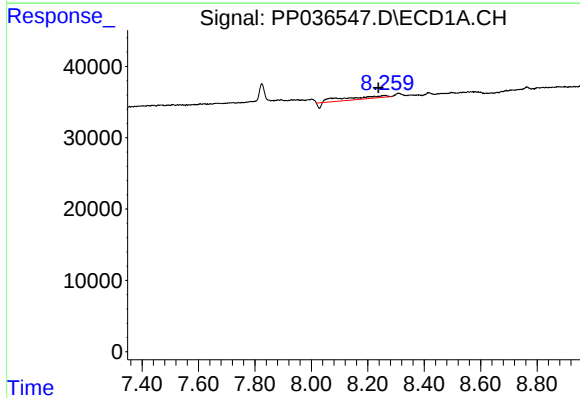


#32 AR-1260-2

R.T.: 8.262 min
Delta R.T.: 0.024 min
Response: 36513
Conc: 14.25 ng/ml

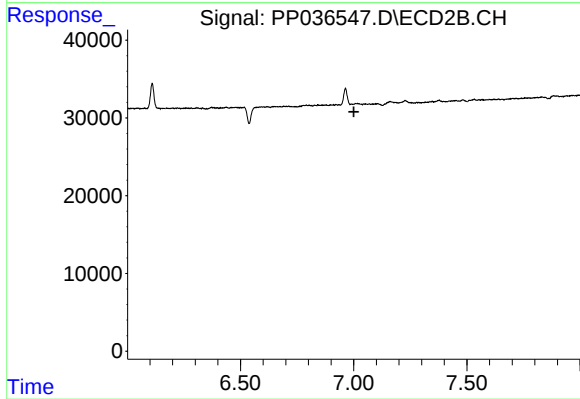

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.001 min
Response: 0
Conc: N.D.

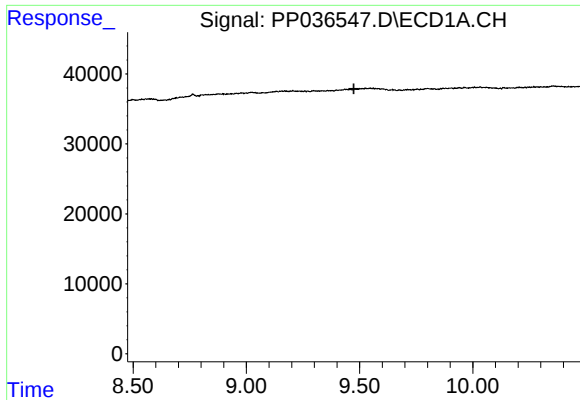

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

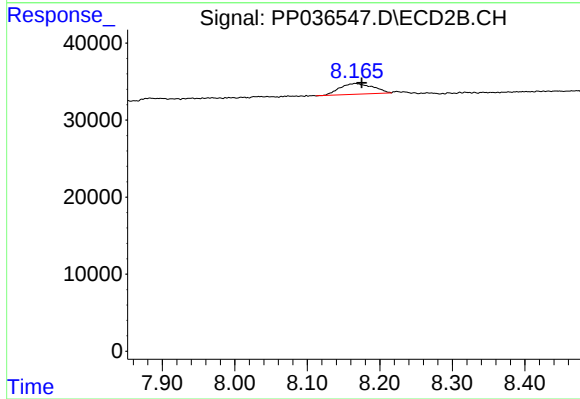


#38 AR-1262-3

R.T.: 8.166 min
Delta R.T.: -0.009 min
Response: 44095
Conc: 27.71 ng/ml

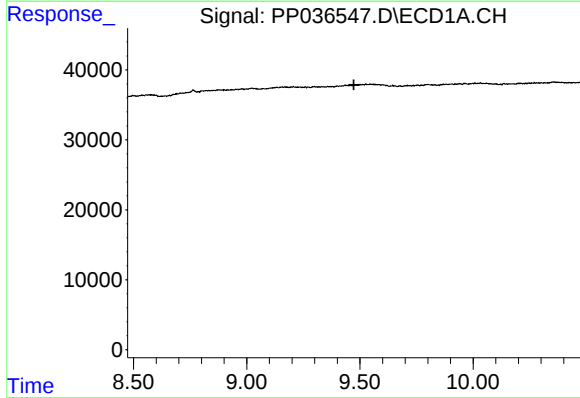

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.473 min
Response: 0
Conc: N.D.

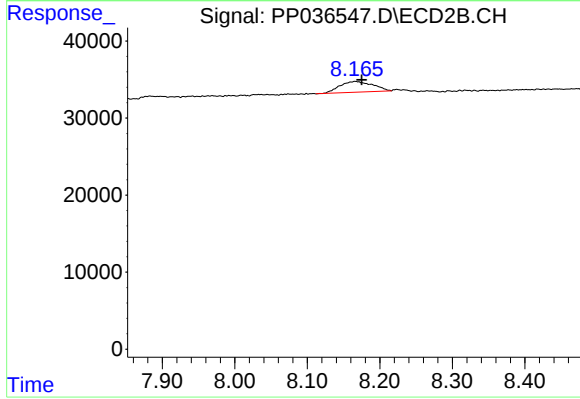

#41 AR-1268-1

R.T.: 8.166 min
Delta R.T.: -0.009 min
Response: 44095
Conc: 9.47 ng/ml