

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036559.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 15:27
 Operator : DD\AJ
 Sample : M2709-06MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 0224-COMP-O(DISCRETE-CL-24)M

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:56:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.958	962384	681036	21.774	21.988
2)	SA Decachlor...	10.998	9.263	818916	568389	19.090	17.773
Target Compounds							
8)	L2 AR-1221-1	5.216	0.000	16648	0	29.654	N.D. #
9)	L2 AR-1221-2	5.317	4.310	14464	8381	33.565	28.078
10)	L2 AR-1221-3	5.426f	0.000	24164	0	18.743	N.D. #
11)	L3 AR-1232-1	5.426f	0.000	24164	0	22.688	N.D. #
28)	L6 AR-1254-3	7.824f	0.000	12438	0	4.199	N.D. #
30)	L6 AR-1254-5	8.508f	0.000	19489	0	8.195	N.D. #
32)	L7 AR-1260-2	8.235	0.000	6841	0	2.669	N.D. #
33)	L7 AR-1260-3	8.591	0.000	574	0	0.287	N.D. #
36)	L8 AR-1262-1	8.591	0.000	574	0	0.202	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036559.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 15:27
Operator : DD\AJ
Sample : M2709-06MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:56:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

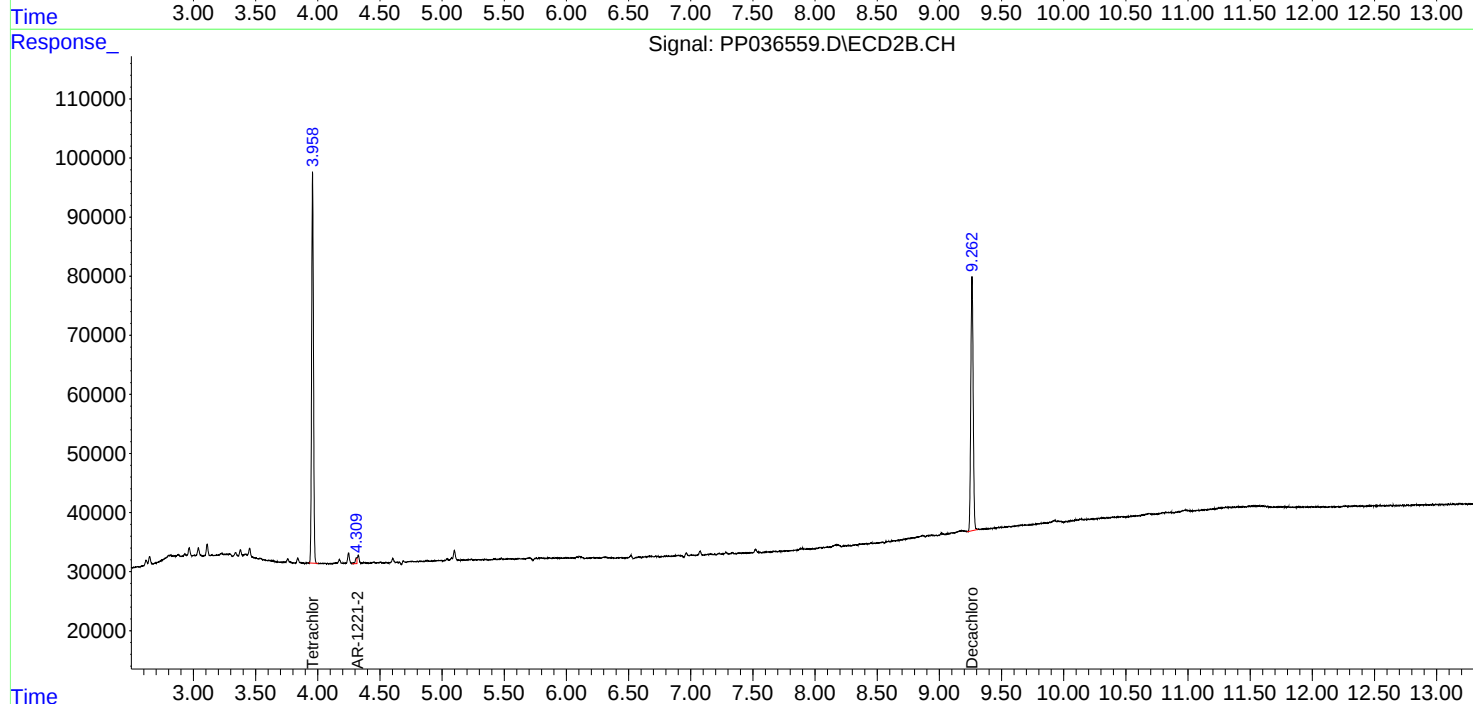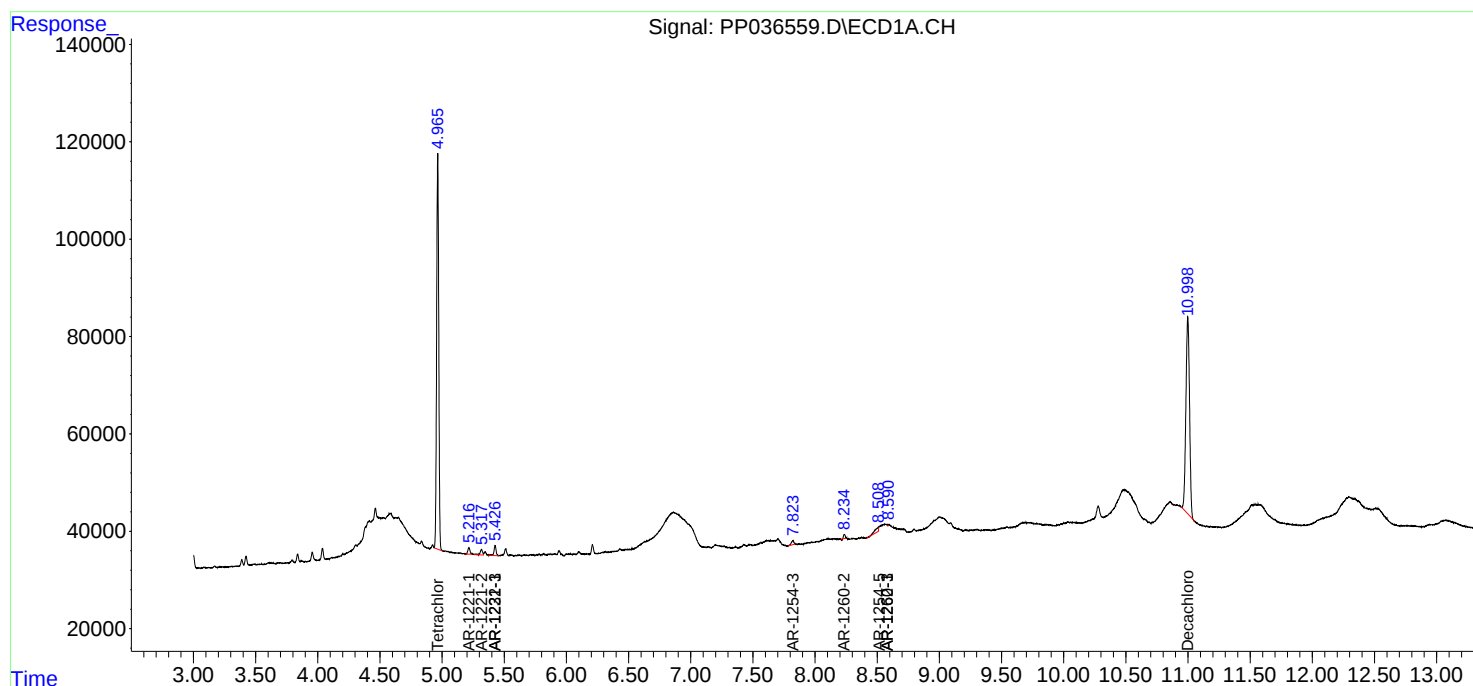


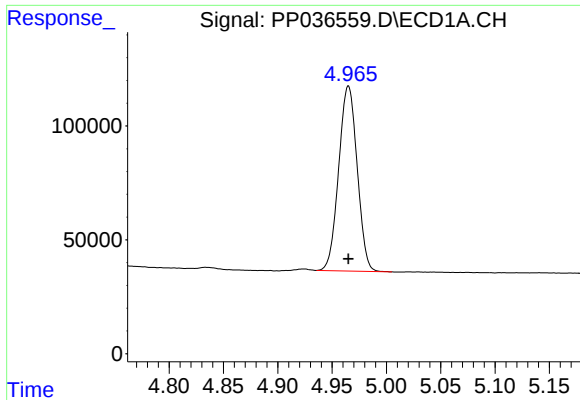

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 962384
Conc: 21.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)M

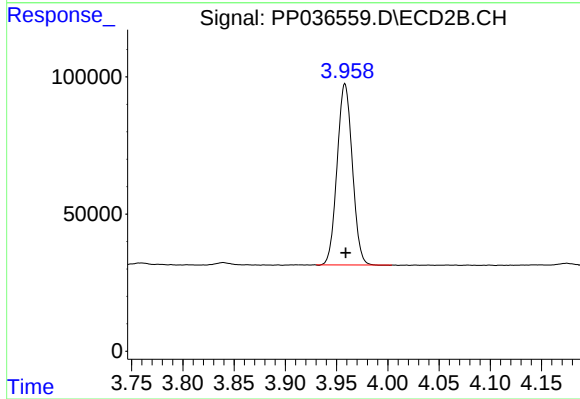


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 681036
Conc: 21.99 ng/ml

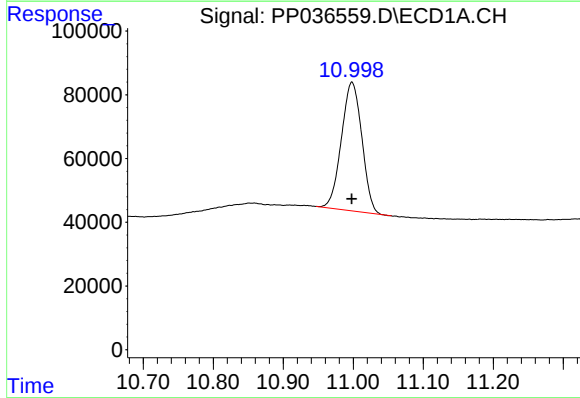


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.000 min
Response: 818916
Conc: 19.09 ng/ml

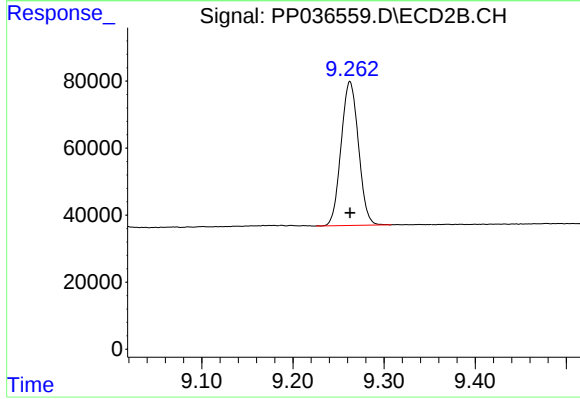

#2 Decachlorobiphenyl


R.T.: 9.263 min
Delta R.T.: 0.000 min
Response: 568389
Conc: 17.77 ng/ml

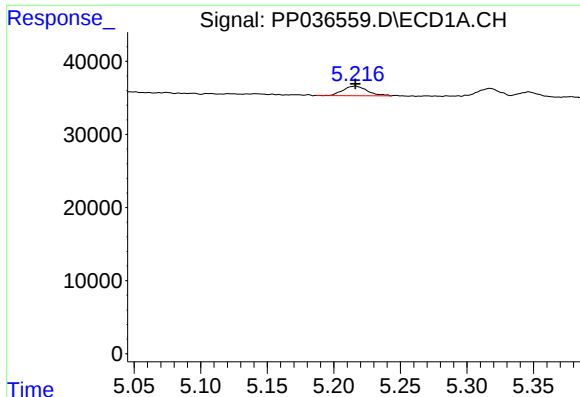

#8 AR-1221-1


R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 16648
Conc: 29.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)M

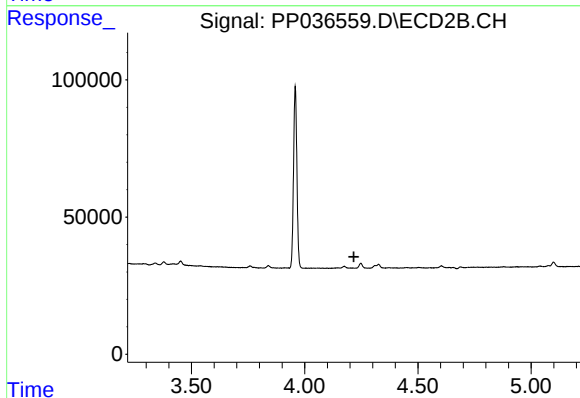


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

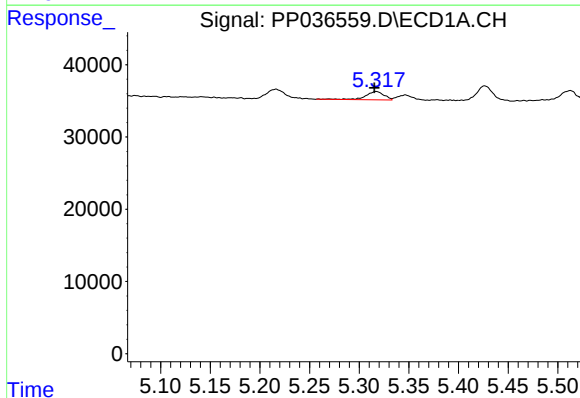


#9 AR-1221-2

R.T.: 5.317 min
Delta R.T.: 0.002 min
Response: 14464
Conc: 33.57 ng/ml

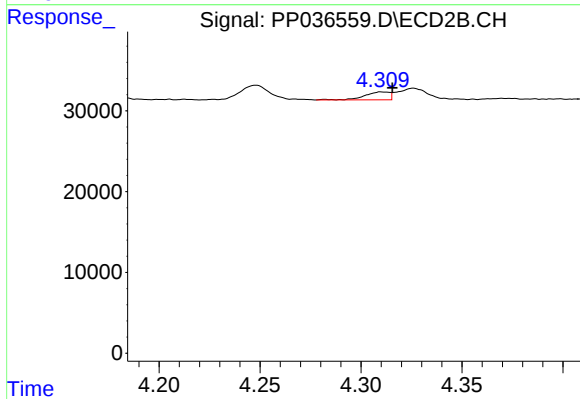

#9 AR-1221-2


R.T.: 4.310 min
Delta R.T.: -0.006 min
Response: 8381
Conc: 28.08 ng/ml

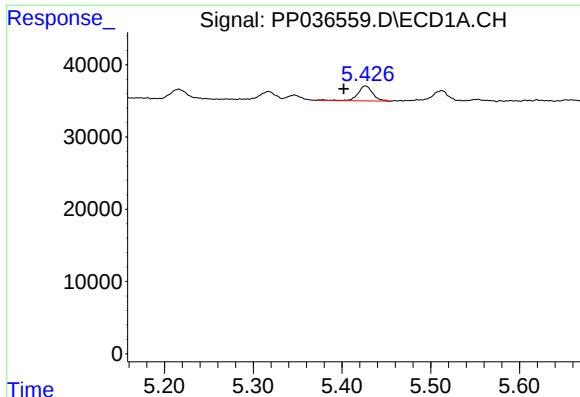

#10 AR-1221-3


R.T.: 5.426 min
Delta R.T.: 0.024 min
Response: 24164
Conc: 18.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)M

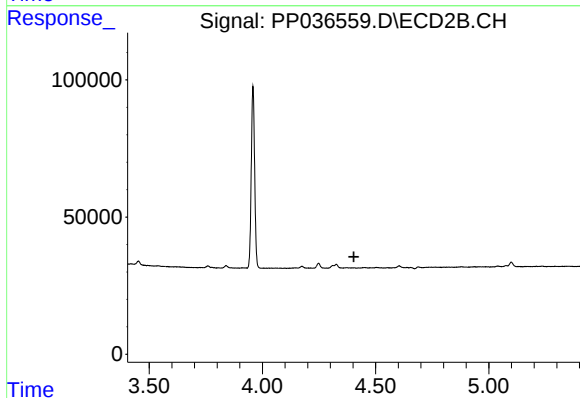


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.404 min
Response: 0
Conc: N.D.

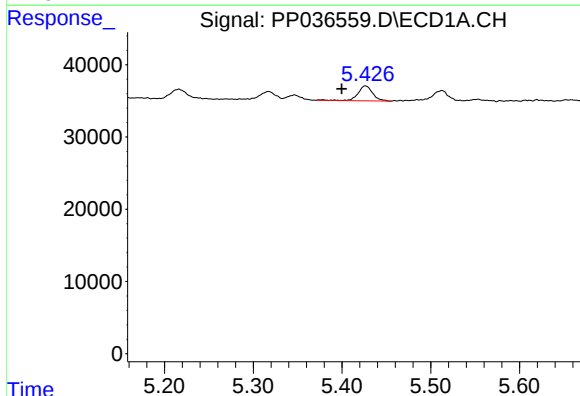


#11 AR-1232-1

R.T.: 5.426 min
Delta R.T.: 0.027 min
Response: 24164
Conc: 22.69 ng/ml

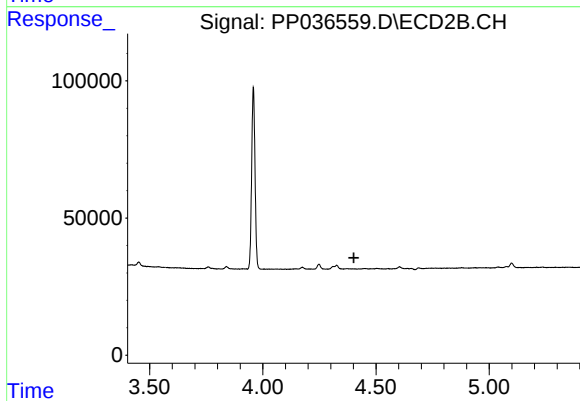

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.402 min
Response: 0
Conc: N.D.

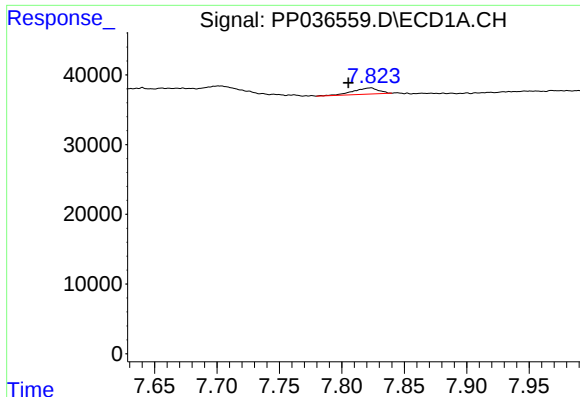

#28 AR-1254-3


R.T.: 7.824 min
Delta R.T.: 0.018 min
Response: 12438
Conc: 4.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)M

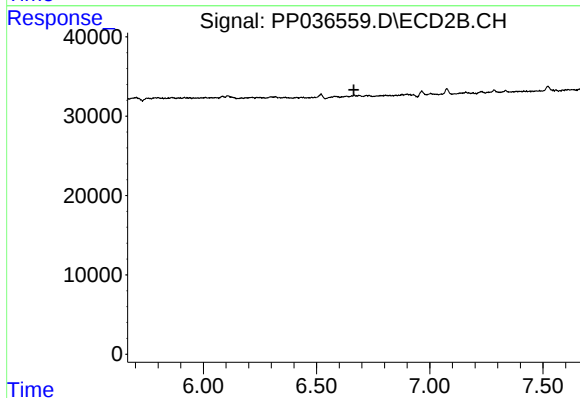


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.

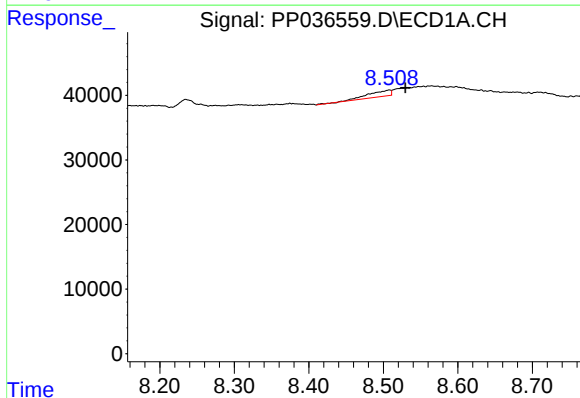


#30 AR-1254-5

R.T.: 8.508 min
Delta R.T.: -0.021 min
Response: 19489
Conc: 8.20 ng/ml

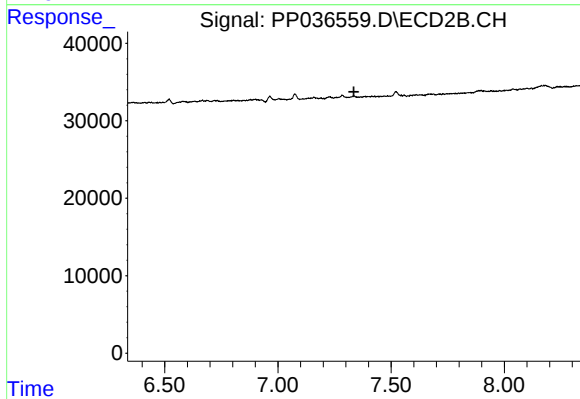

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.335 min
Response: 0
Conc: N.D.

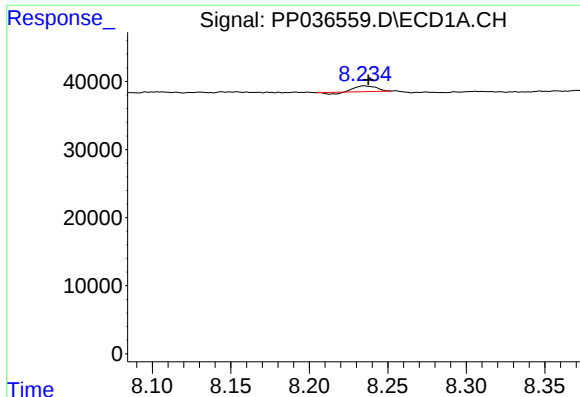

#32 AR-1260-2


R.T.: 8.235 min
Delta R.T.: -0.003 min
Response: 6841
Conc: 2.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)M

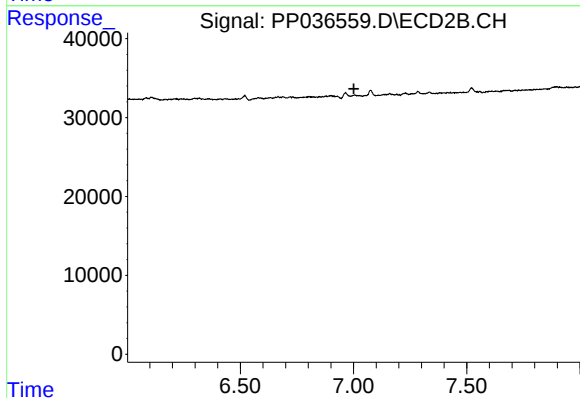


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.001 min
Response: 0
Conc: N.D.

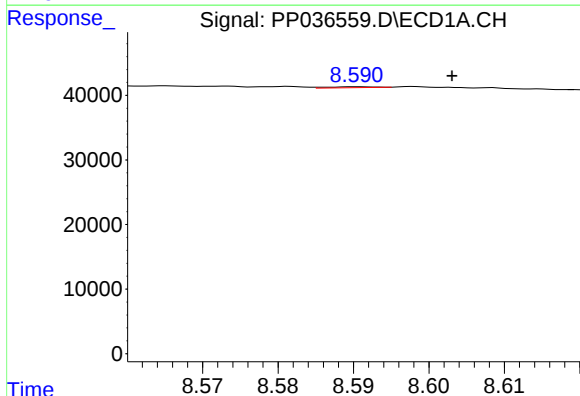


#33 AR-1260-3

R.T.: 8.591 min
Delta R.T.: -0.012 min
Response: 574
Conc: 0.29 ng/ml

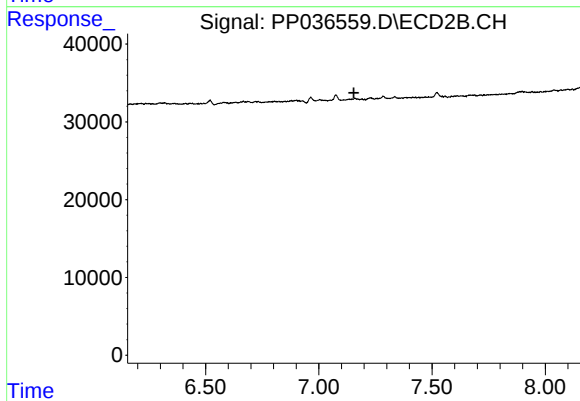

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

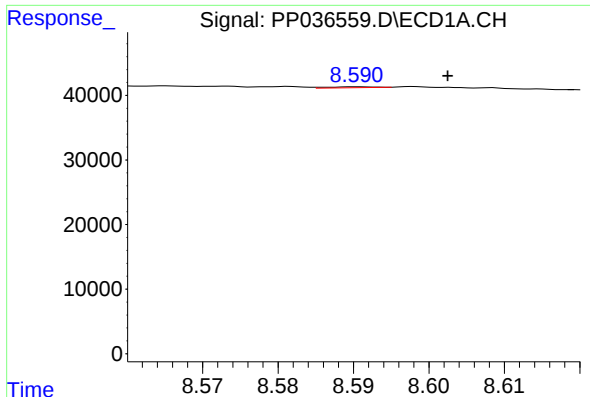

#36 AR-1262-1

R.T.: 8.591 min
Delta R.T.: -0.012 min
Response: 574
Conc: 0.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)M

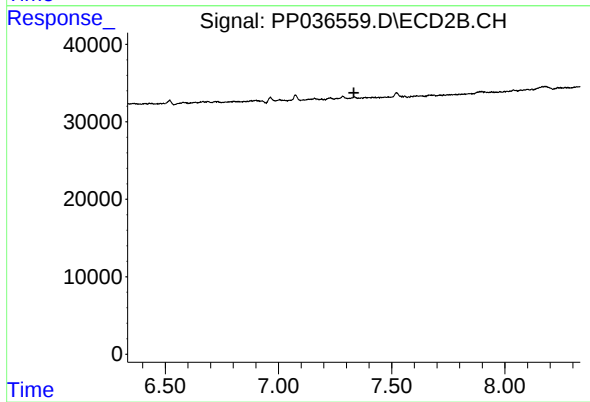

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.333 min
Response: 0
Conc: N.D.