

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036585.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 23:51
 Operator : DD\AJ
 Sample : M2709-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 0344-AMND-COMP-O(CL-24)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:11:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.959	1015418	714512	22.974	23.069
2)	SA Decachlor...	11.000	9.263	965079	656368	22.497	20.524
Target Compounds							
9)	L2 AR-1221-2	5.318	4.309	12659	2127	29.377	7.125 #
10)	L2 AR-1221-3	5.427f	0.000	13540	0	10.503	N.D. #
11)	L3 AR-1232-1	5.427f	0.000	13540	0	12.713	N.D. #
24)	L5 AR-1248-4	7.197f	0.000	5128	0	2.809	N.D. #
26)	L6 AR-1254-1	7.197	0.000	5128	0	2.916	N.D. #
27)	L6 AR-1254-2	7.426	0.000	14811	0	5.474	N.D. #
28)	L6 AR-1254-3	7.823f	0.000	19290	0	6.512	N.D. #
32)	L7 AR-1260-2	8.237	0.000	10237	0	3.994	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036585.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 23:51
Operator : DD\AJ
Sample : M2709-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
0344-AMND-COMP-O(CL-24)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:11:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

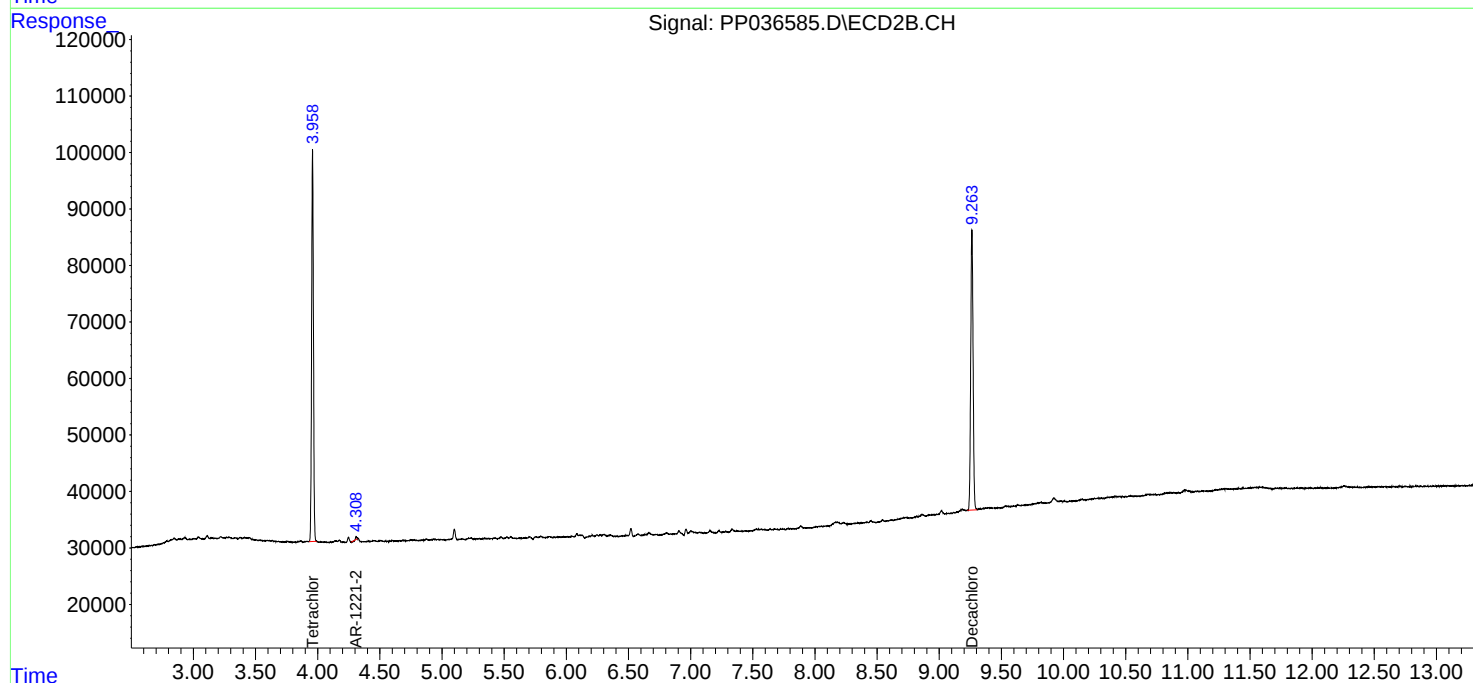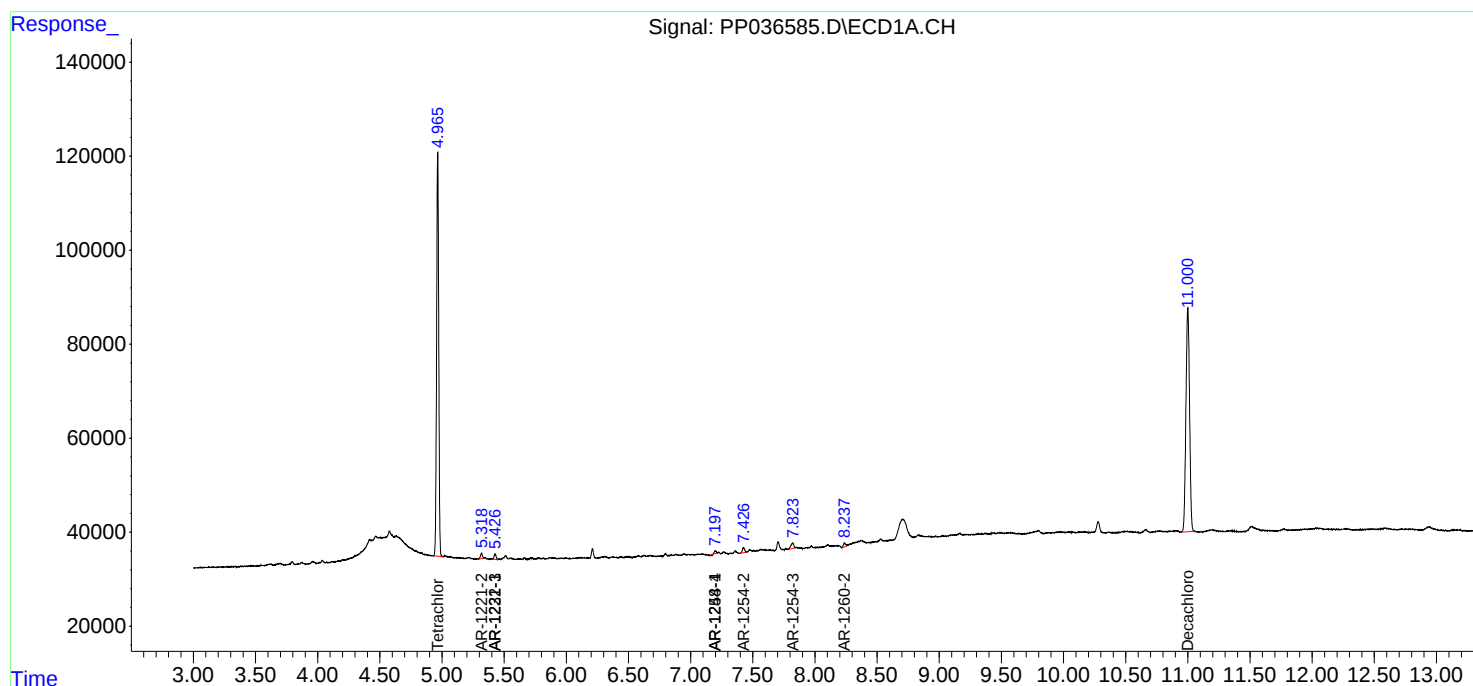


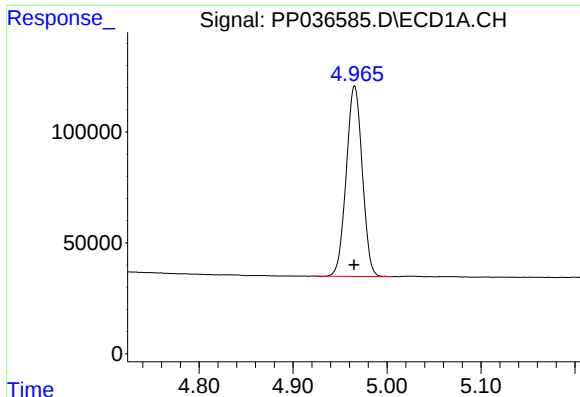

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 1015418
Conc: 22.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
0344-AMND-COMP-O(CL-24)

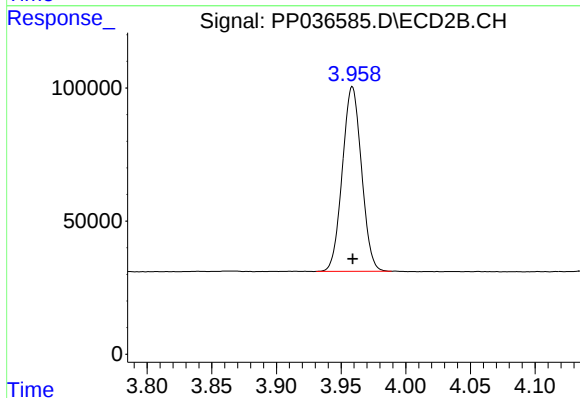


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 714512
Conc: 23.07 ng/ml

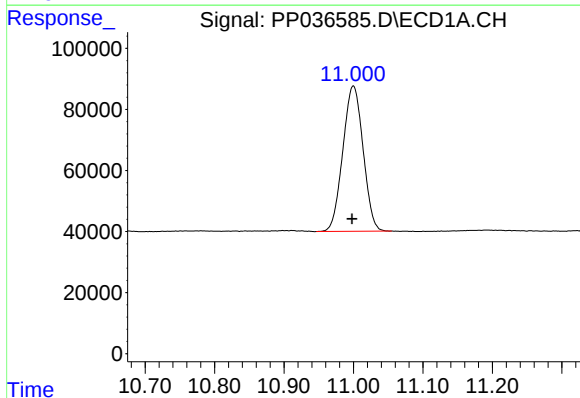


#2 Decachlorobiphenyl

R.T.: 11.000 min
Delta R.T.: 0.002 min
Response: 965079
Conc: 22.50 ng/ml

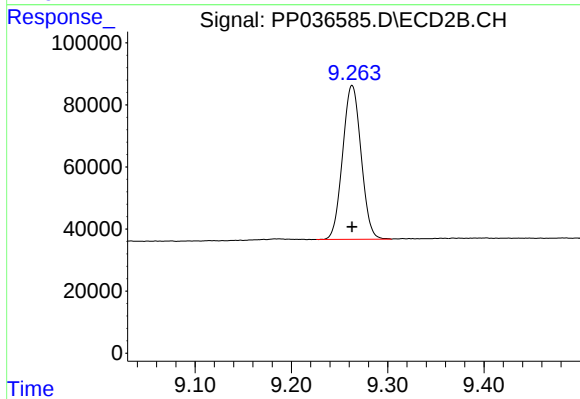

#2 Decachlorobiphenyl


R.T.: 9.263 min
Delta R.T.: 0.000 min
Response: 656368
Conc: 20.52 ng/ml

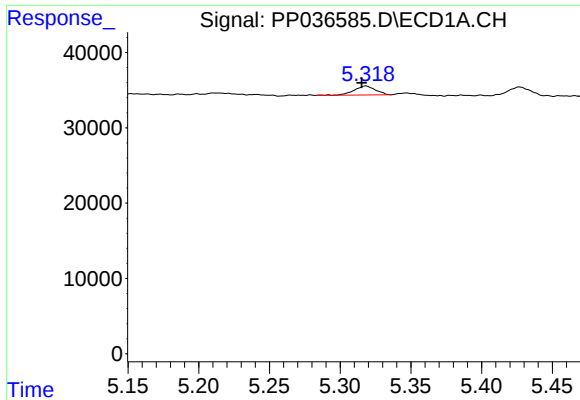

#9 AR-1221-2


R.T.: 5.318 min
Delta R.T.: 0.003 min
Response: 12659
Conc: 29.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
0344-AMND-COMP-O(CL-24)

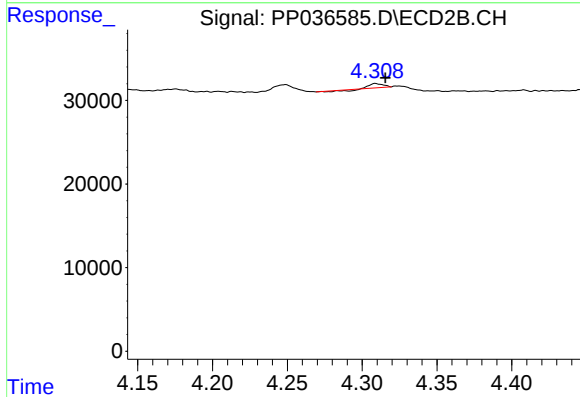


#9 AR-1221-2

R.T.: 4.309 min
Delta R.T.: -0.007 min
Response: 2127
Conc: 7.12 ng/ml

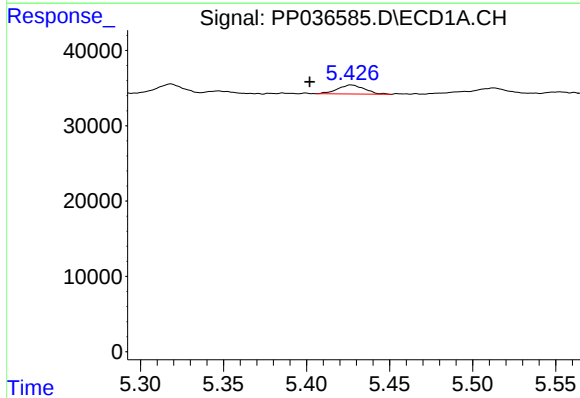


#10 AR-1221-3

R.T.: 5.427 min
Delta R.T.: 0.025 min
Response: 13540
Conc: 10.50 ng/ml

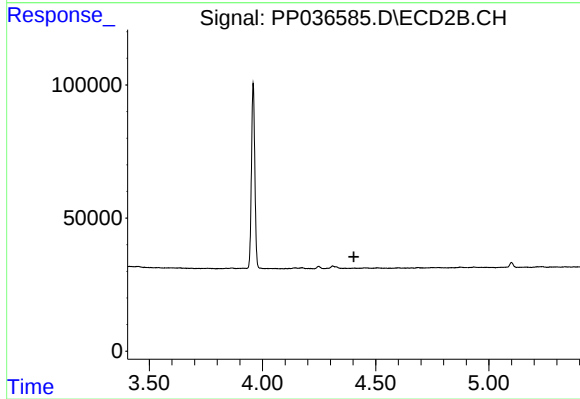

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.404 min
Response: 0
Conc: N.D.

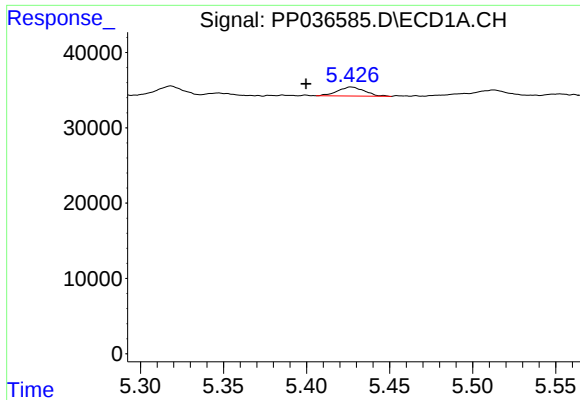

#11 AR-1232-1


R.T.: 5.427 min
Delta R.T.: 0.027 min
Response: 13540
Conc: 12.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
0344-AMND-COMP-O(CL-24)

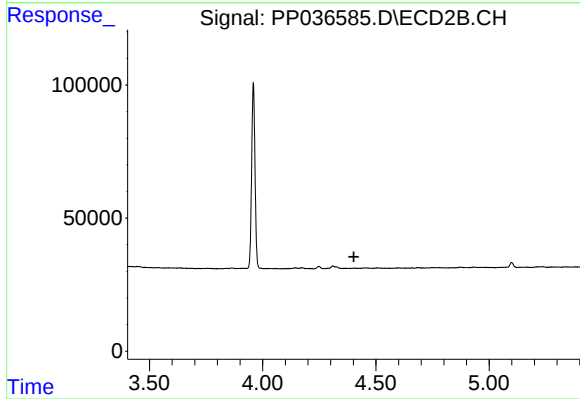


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.402 min
Response: 0
Conc: N.D.

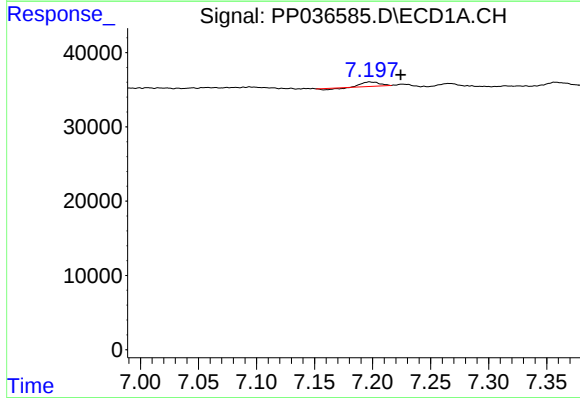


#24 AR-1248-4

R.T.: 7.197 min
Delta R.T.: -0.027 min
Response: 5128
Conc: 2.81 ng/ml

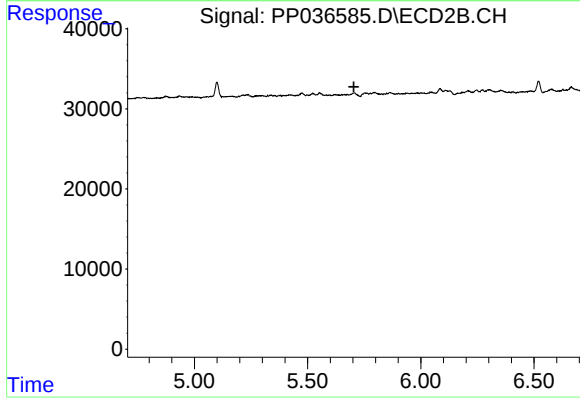

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.704 min
Response: 0
Conc: N.D.

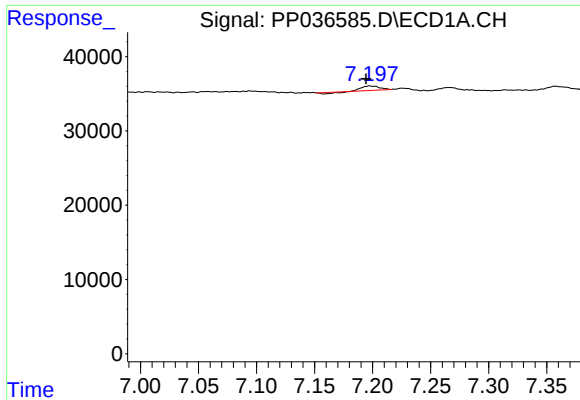

#26 AR-1254-1


R.T.: 7.197 min
Delta R.T.: 0.003 min
Response: 5128
Conc: 2.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
0344-AMND-COMP-O(CL-24)

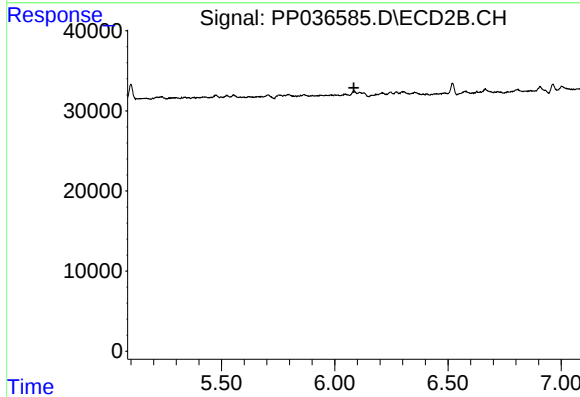


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.084 min
Response: 0
Conc: N.D.

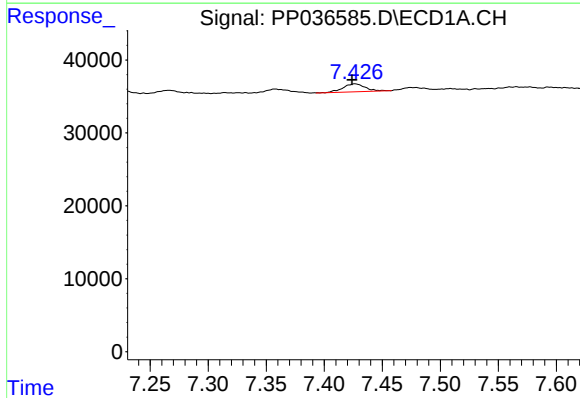


#27 AR-1254-2

R.T.: 7.426 min
Delta R.T.: 0.002 min
Response: 14811
Conc: 5.47 ng/ml

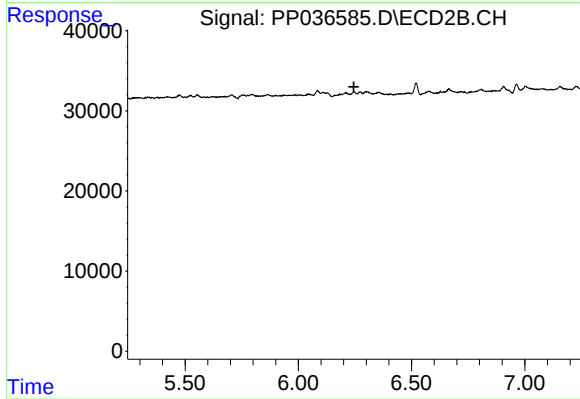

#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

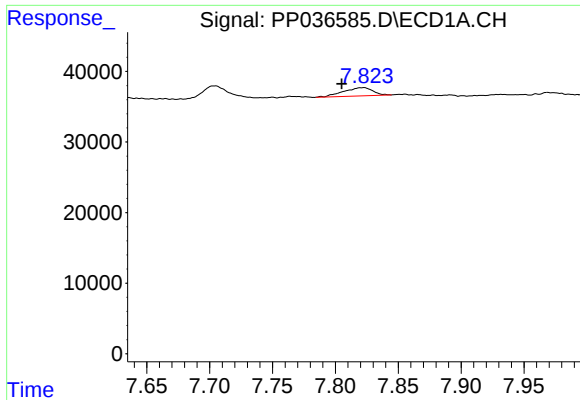


#28 AR-1254-3

```

      R.T.:      7.823 min
Delta R.T.:      0.018 min
  Response:      19290
      Conc:      6.51 ng/ml

```

Instrument :
ECD_P
ClientSampleId :
0344-AMND-COMP-O(CL-24)

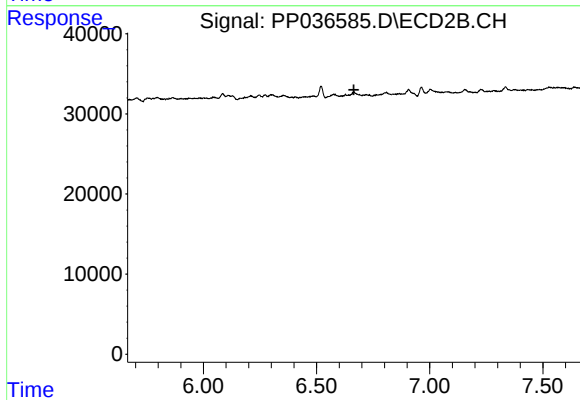


#28 AR-1254-3

```

      R.T.:    0.000 min
Exp R.T.  :    6.665 min
  Response:         0
    Conc:    N.D.

```

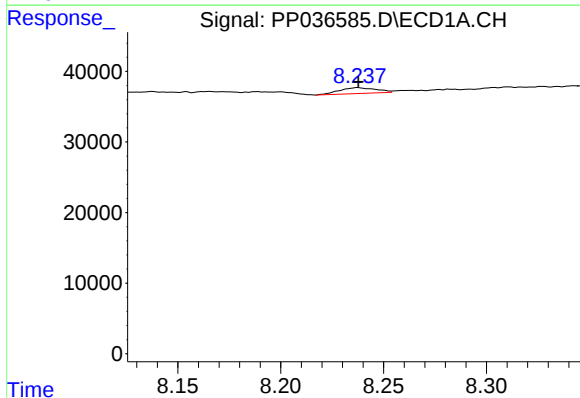


#32 AR-1260-2

```

      R.T.:      8.237 min
Delta R.T.:      0.000 min
  Response:      10237
    Conc:      3.99 ng/ml

```

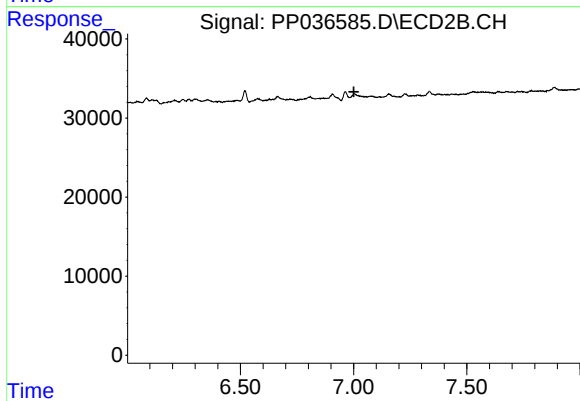

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.001 min
Response: 0
Conc: N.D.