

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036605.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2021 6:00
 Operator : DD\AJ
 Sample : M2741-02
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 0336-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 06:32:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.958	871230	607059	19.712	19.599
2)	SA Decachlor...	11.000	9.262	848232	552615	19.774	17.280
Target Compounds							
8)	L2 AR-1221-1	5.216	0.000	280361	0	499.385	N.D. #
9)	L2 AR-1221-2	5.317	4.309	12251	9054	28.430	30.332
12)	L3 AR-1232-2	6.010f	0.000	12203	0	22.189	N.D. #
15)	L3 AR-1232-5	6.605f	0.000	14671	0	40.031	N.D. #
20)	L4 AR-1242-5	7.291f	0.000	24701	0	23.483	N.D. #
22)	L5 AR-1248-2	6.605f	0.000	14671	0	10.803	N.D. #
25)	L5 AR-1248-5	7.291f	0.000	24701	0	13.700	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036605.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2021 6:00
Operator : DD\AJ
Sample : M2741-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
0336-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 06:32:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

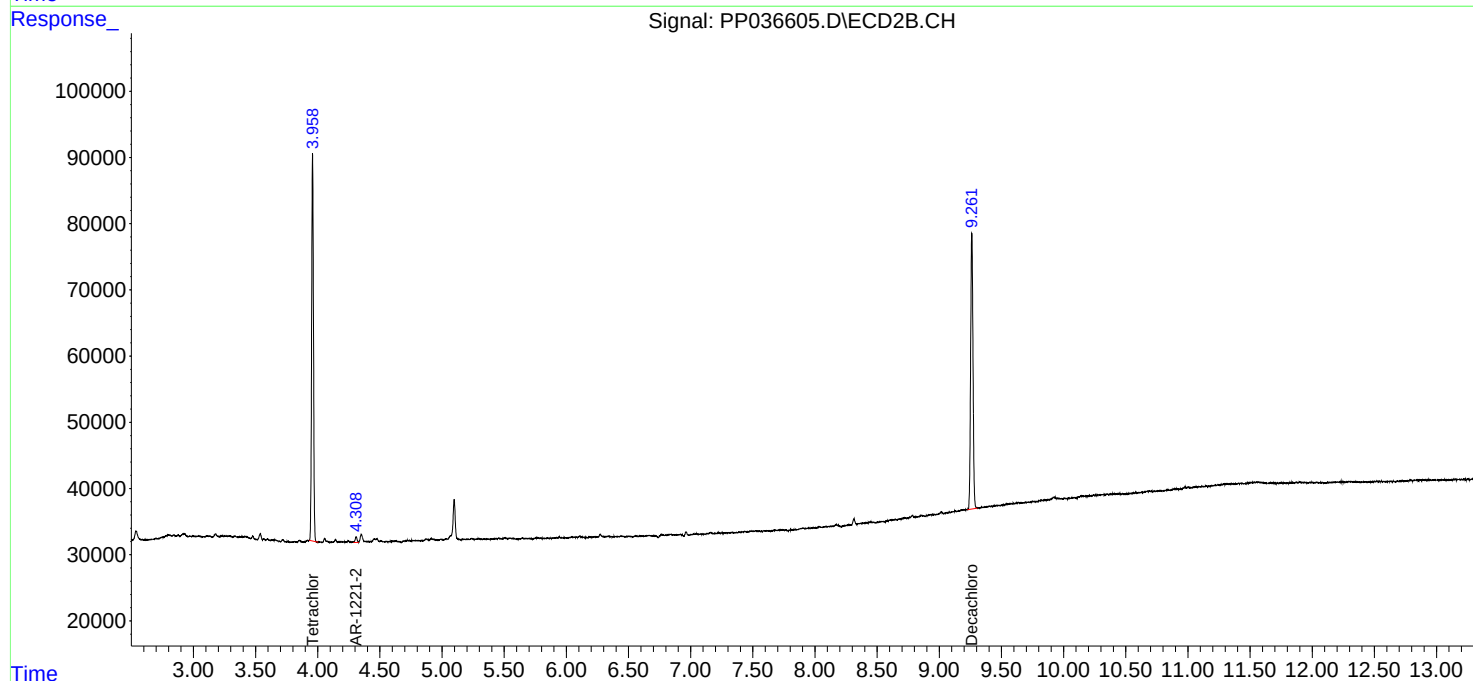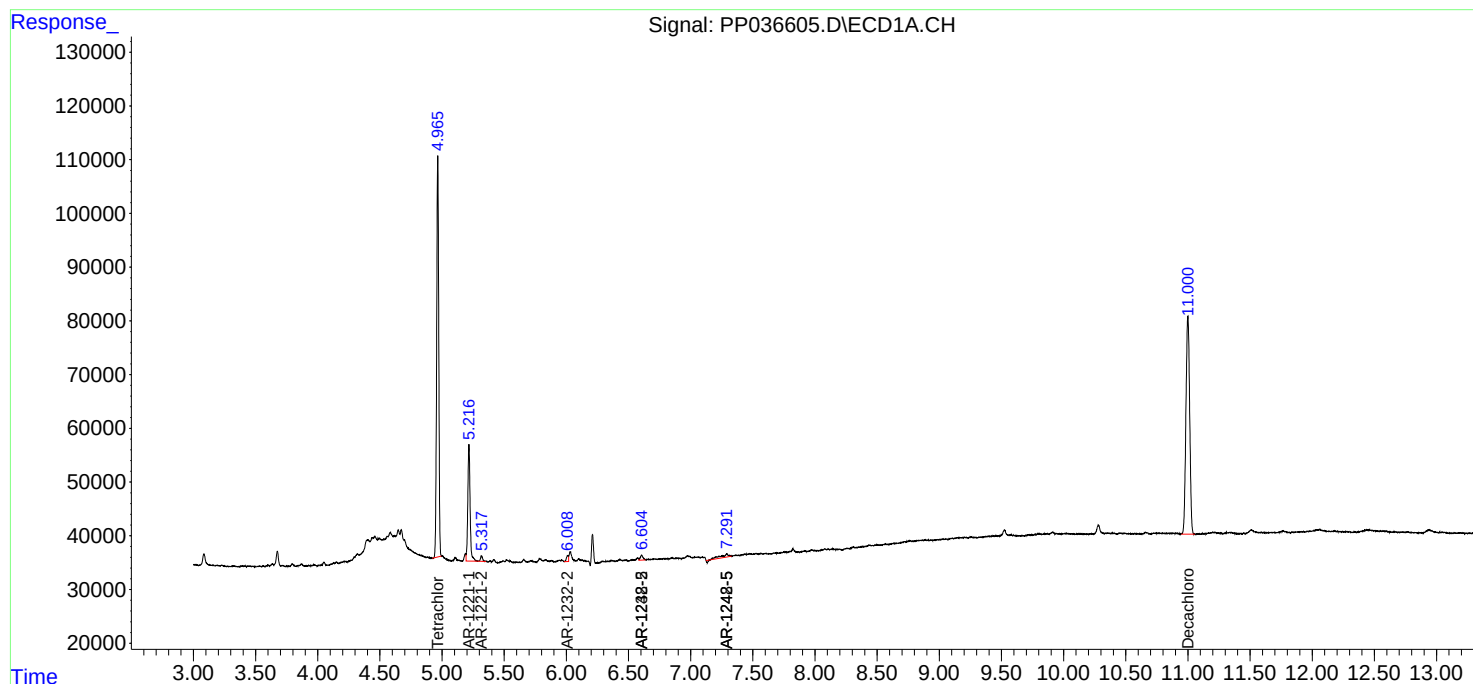


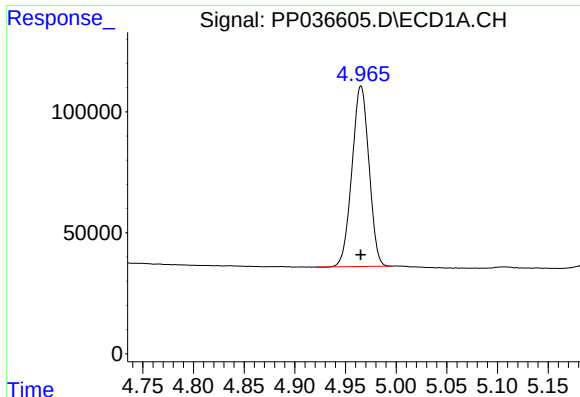

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 871230
Conc: 19.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
0336-SITE-WATER

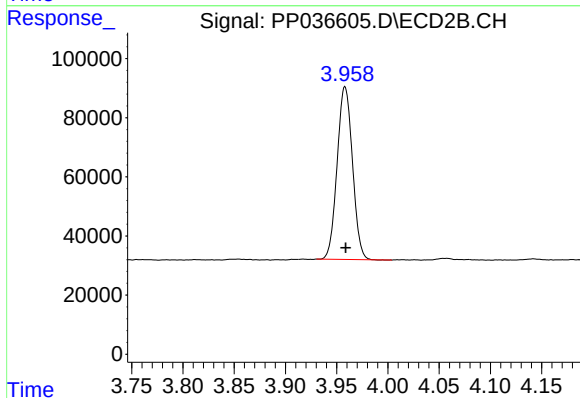


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 607059
Conc: 19.60 ng/ml

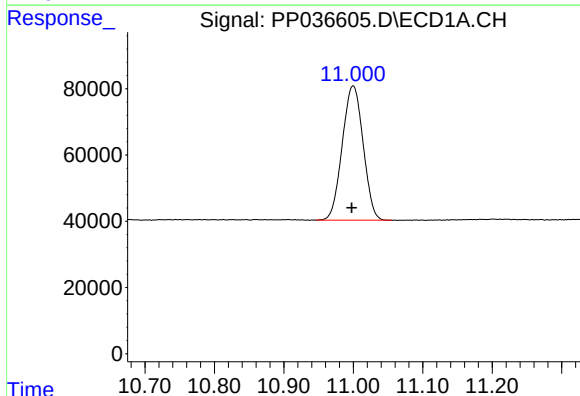


#2 Decachlorobiphenyl

R.T.: 11.000 min
Delta R.T.: 0.002 min
Response: 848232
Conc: 19.77 ng/ml

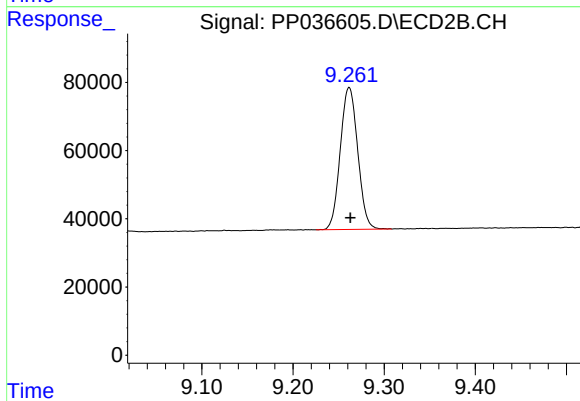

#2 Decachlorobiphenyl


R.T.: 9.262 min
Delta R.T.: -0.001 min
Response: 552615
Conc: 17.28 ng/ml

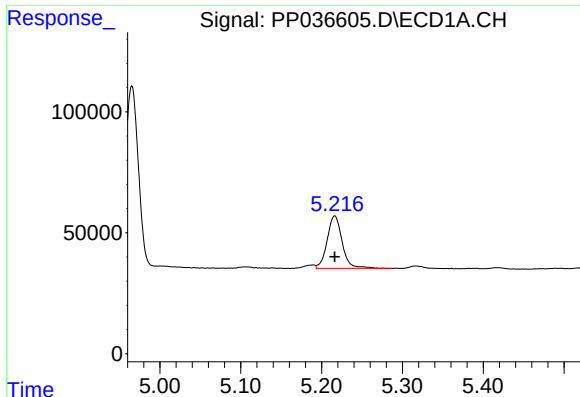

#8 AR-1221-1


R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 280361
Conc: 499.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
0336-SITE-WATER

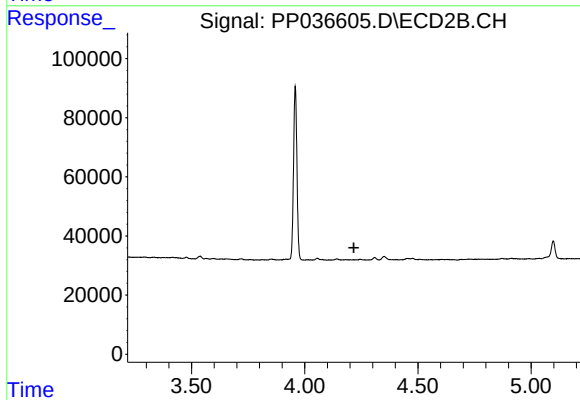


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

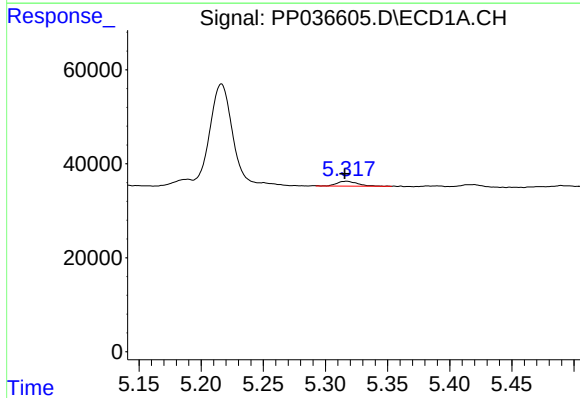


#9 AR-1221-2

R.T.: 5.317 min
Delta R.T.: 0.002 min
Response: 12251
Conc: 28.43 ng/ml

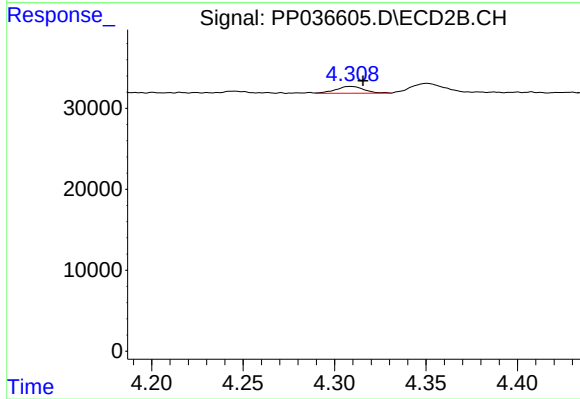

#9 AR-1221-2


R.T.: 4.309 min
Delta R.T.: -0.007 min
Response: 9054
Conc: 30.33 ng/ml

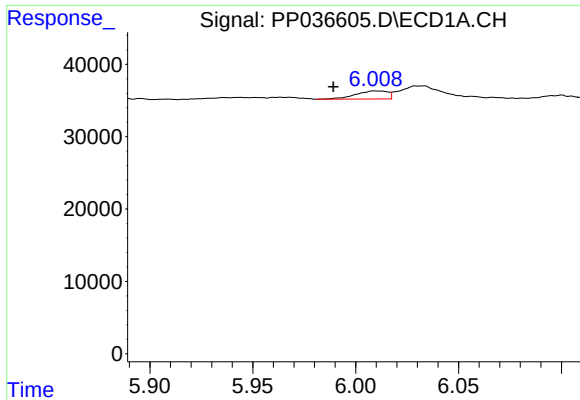

#12 AR-1232-2


R.T.: 6.010 min
Delta R.T.: 0.021 min
Response: 12203
Conc: 22.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
0336-SITE-WATER

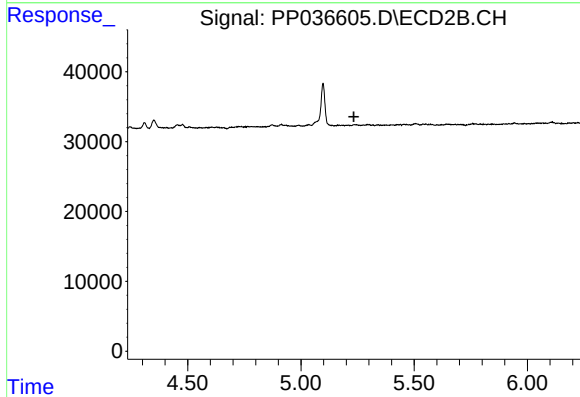


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.234 min
Response: 0
Conc: N.D.

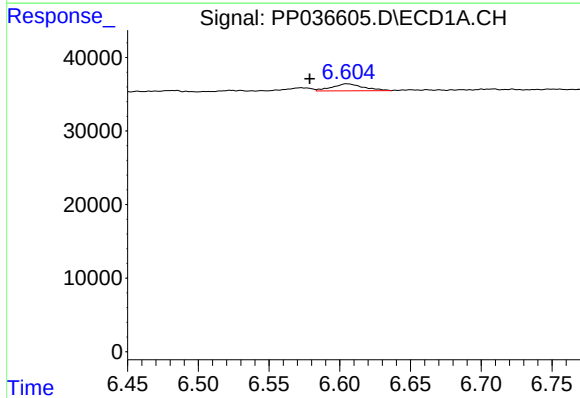


#15 AR-1232-5

R.T.: 6.605 min
Delta R.T.: 0.027 min
Response: 14671
Conc: 40.03 ng/ml

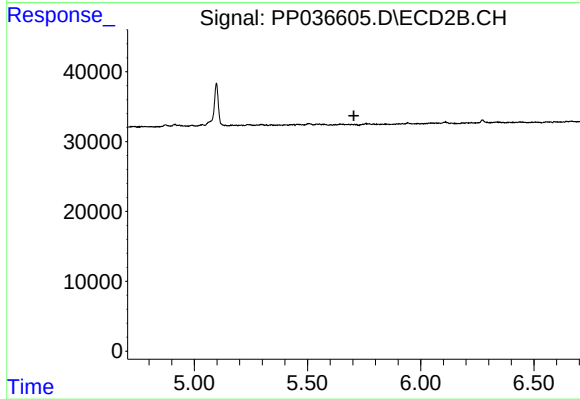

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.705 min
Response: 0
Conc: N.D.

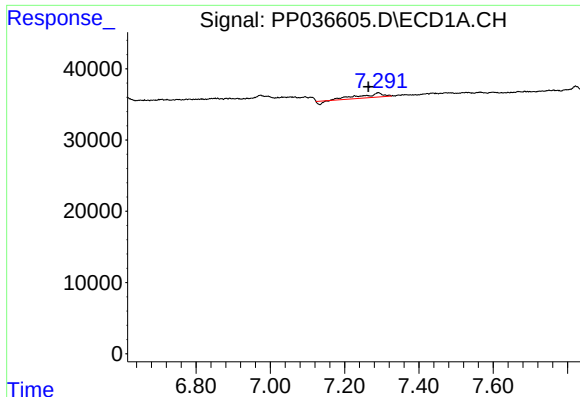

#20 AR-1242-5


R.T.: 7.291 min
Delta R.T.: 0.027 min
Response: 24701
Conc: 23.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
0336-SITE-WATER

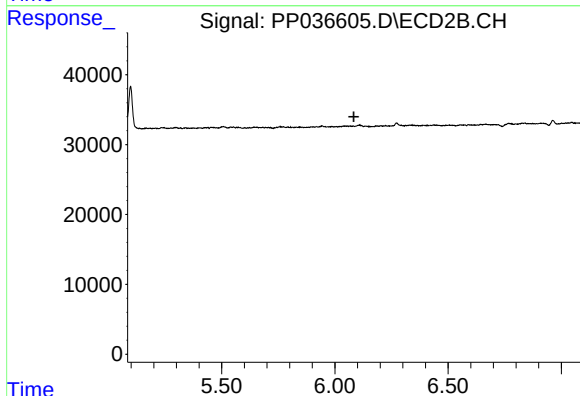


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.084 min
Response: 0
Conc: N.D.

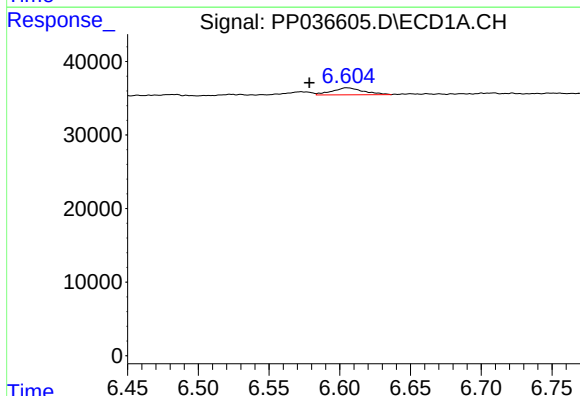


#22 AR-1248-2

R.T.: 6.605 min
Delta R.T.: 0.027 min
Response: 14671
Conc: 10.80 ng/ml

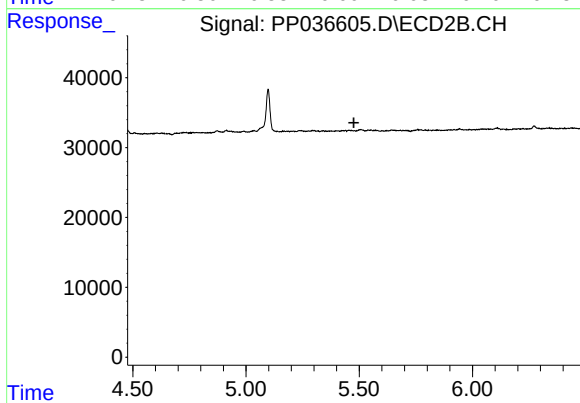

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

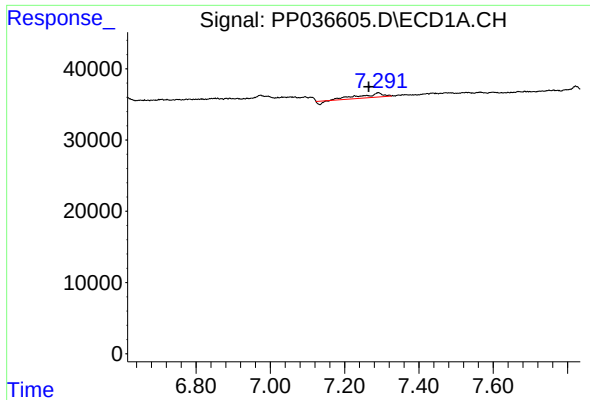

#25 AR-1248-5

R.T.: 7.291 min
Delta R.T.: 0.027 min
Response: 24701
Conc: 13.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
0336-SITE-WATER

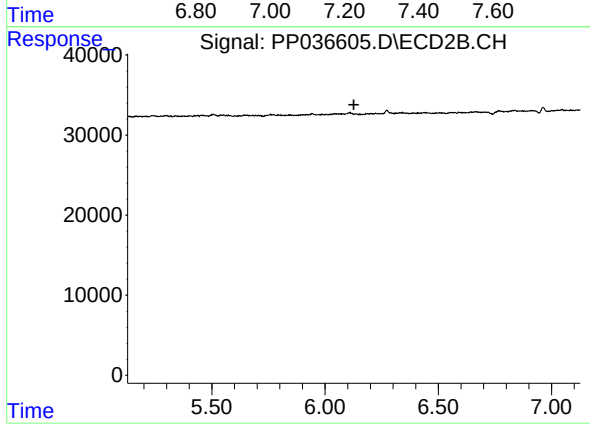

#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.127 min
Response: 0
Conc: N.D.