

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036613.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2021 8:47
 Operator : DD\AJ
 Sample : M2755-02 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEE262Y-N-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:23:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.967	3.960	58914	37004	1.333	1.195
2) SA Decachlor...	11.002	9.263	82265	30940	1.918	0.967 #
Target Compounds						
28) L6 AR-1254-3	7.824f	0.000	7236	0	2.443	N.D. #
33) L7 AR-1260-3	8.614	0.000	7115	0	3.550	N.D. #
35) L7 AR-1260-5	0.000	7.862f	0	2756	N.D.	0.750 #
36) L8 AR-1262-1	8.614	0.000	7115	0	2.497	N.D. #
37) L8 AR-1262-2	0.000	7.862f	0	2756	N.D.	0.703 #
38) L8 AR-1262-3	9.494f	0.000	10809	0	2.918	N.D. #
41) L9 AR-1268-1	9.494f	0.000	10809	0	1.802	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036613.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2021 8:47
Operator : DD\AJ
Sample : M2755-02 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
HEE262Y-N-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:23:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

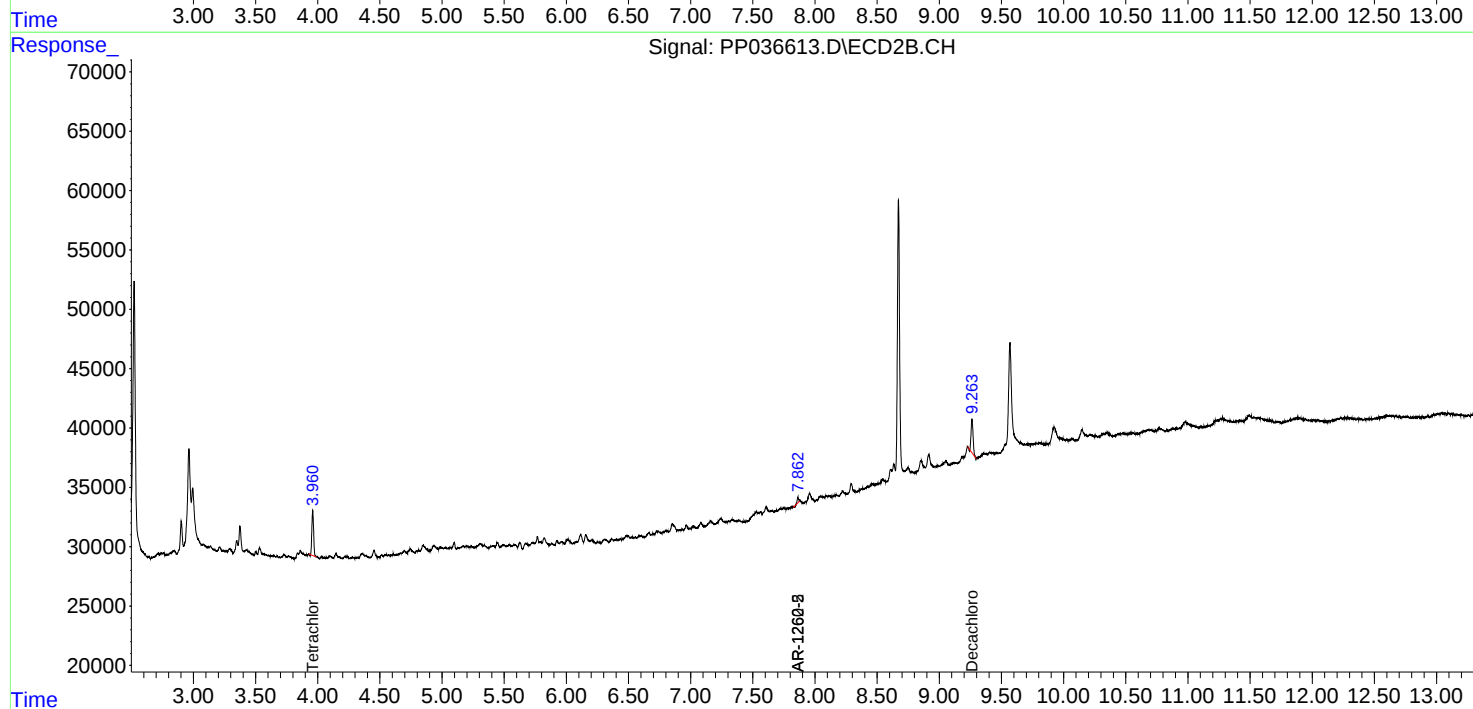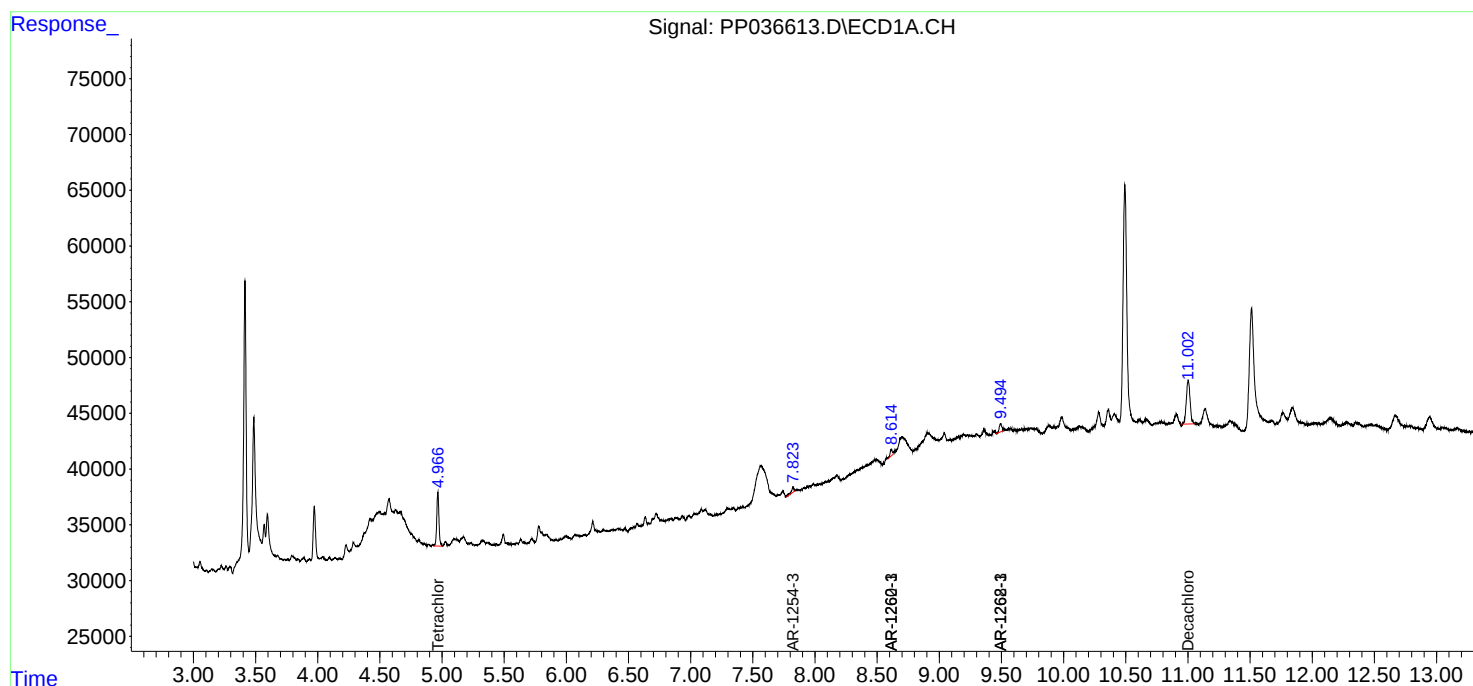


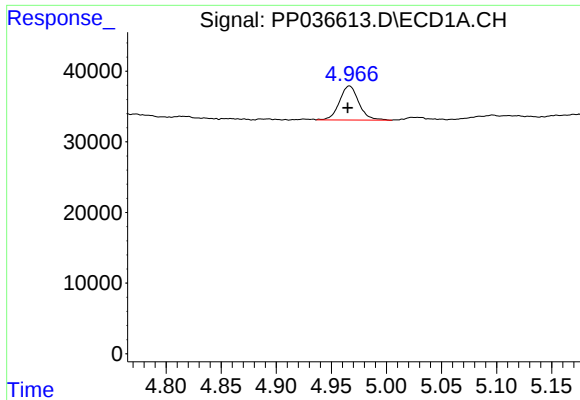

#1 Tetrachloro-m-xylene


R.T.: 4.967 min
Delta R.T.: 0.002 min
Response: 58914
Conc: 1.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE262Y-N-2

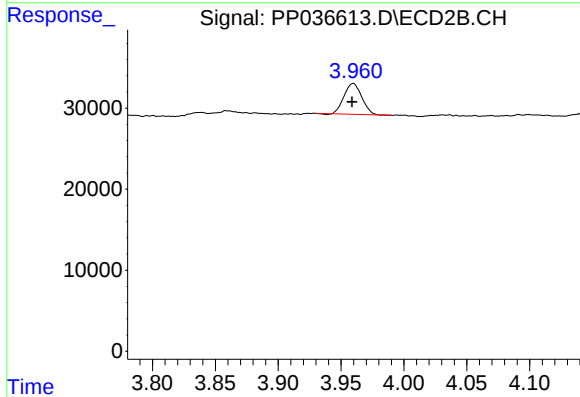


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.001 min
Response: 37004
Conc: 1.19 ng/ml

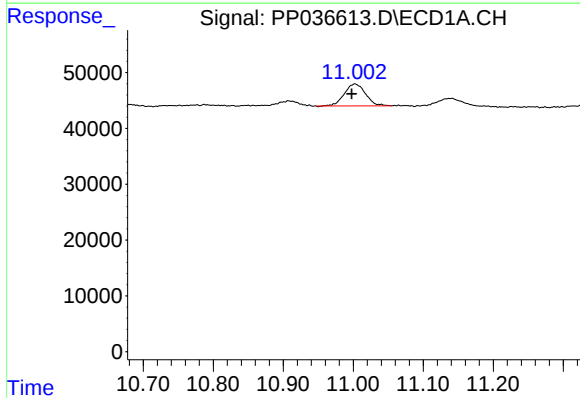


#2 Decachlorobiphenyl

R.T.: 11.002 min
Delta R.T.: 0.005 min
Response: 82265
Conc: 1.92 ng/ml

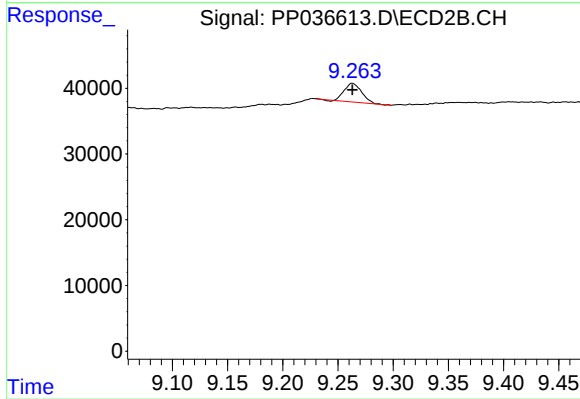

#2 Decachlorobiphenyl


R.T.: 9.263 min
Delta R.T.: 0.000 min
Response: 30940
Conc: 0.97 ng/ml

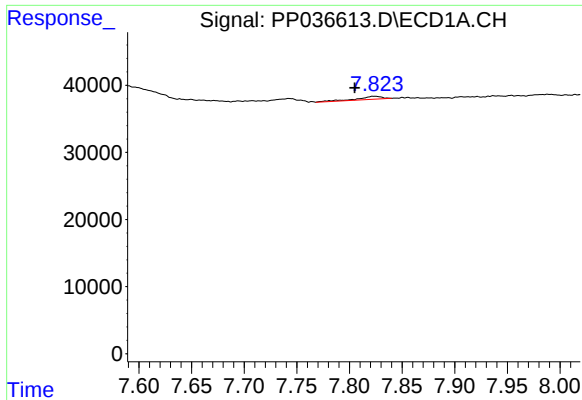

#28 AR-1254-3


R.T.: 7.824 min
Delta R.T.: 0.019 min
Response: 7236
Conc: 2.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE262Y-N-2

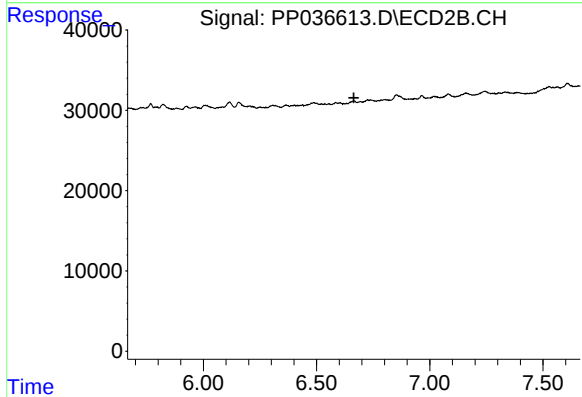


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.665 min
Response: 0
Conc: N.D.

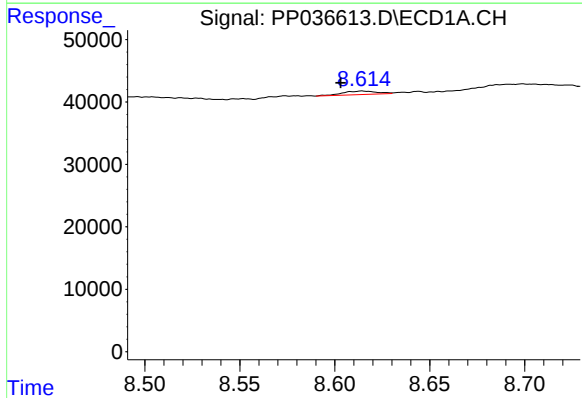


#33 AR-1260-3

R.T.: 8.614 min
Delta R.T.: 0.011 min
Response: 7115
Conc: 3.55 ng/ml

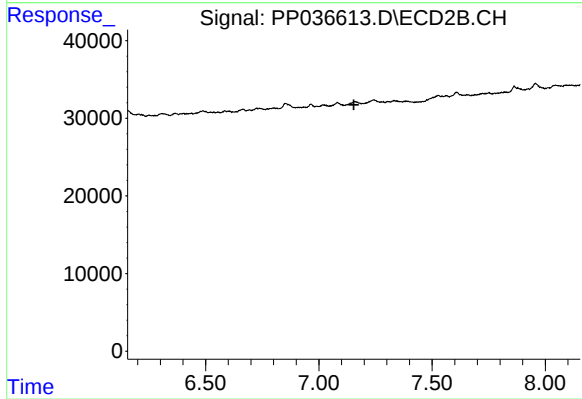

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

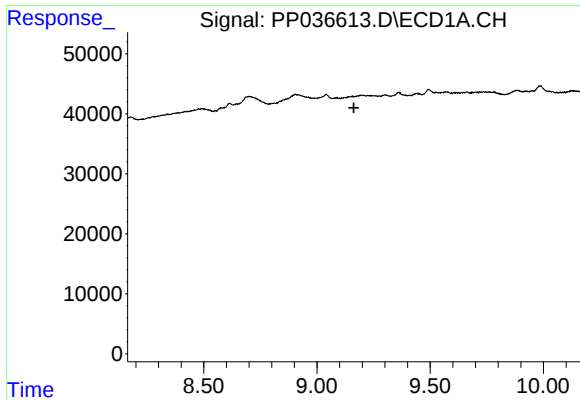

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEE262Y-N-2

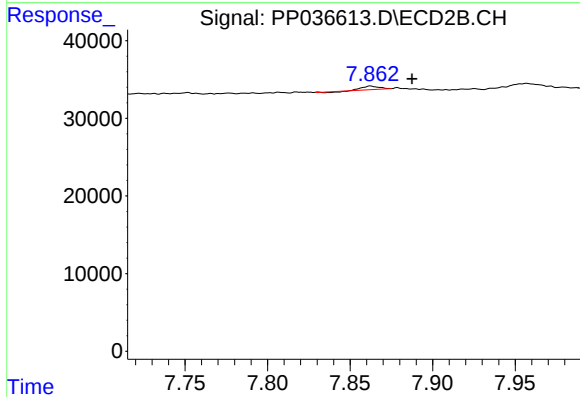


#35 AR-1260-5

R.T.: 7.862 min
Delta R.T.: -0.025 min
Response: 2756
Conc: 0.75 ng/ml

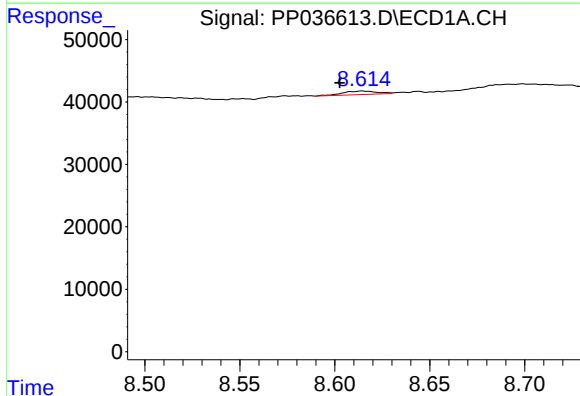


#36 AR-1262-1

R.T.: 8.614 min
Delta R.T.: 0.012 min
Response: 7115
Conc: 2.50 ng/ml

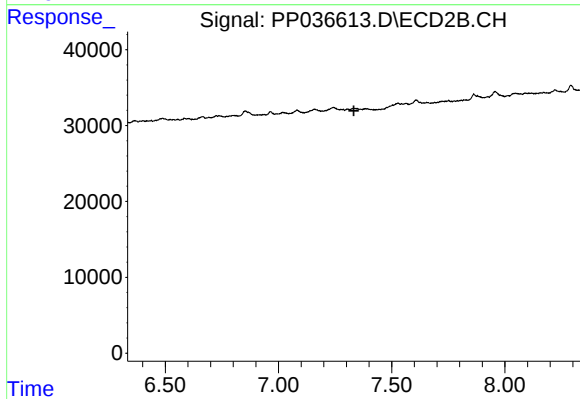

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.333 min
Response: 0
Conc: N.D.

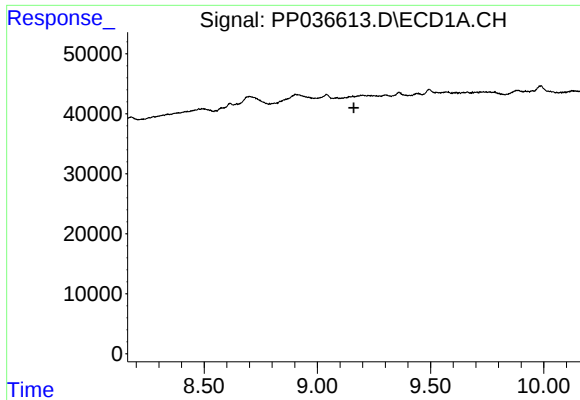

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 9.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEE262Y-N-2

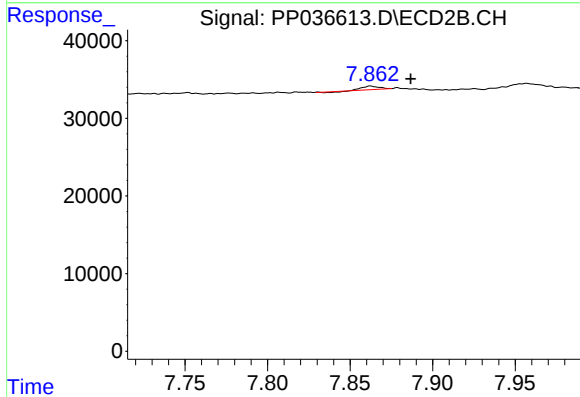


#37 AR-1262-2

R.T.: 7.862 min
Delta R.T.: -0.024 min
Response: 2756
Conc: 0.70 ng/ml

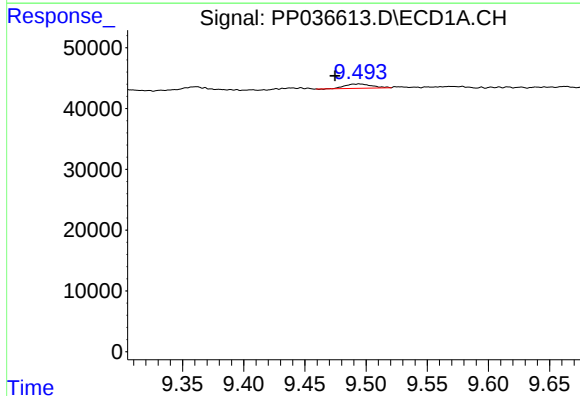


#38 AR-1262-3

R.T.: 9.494 min
Delta R.T.: 0.020 min
Response: 10809
Conc: 2.92 ng/ml

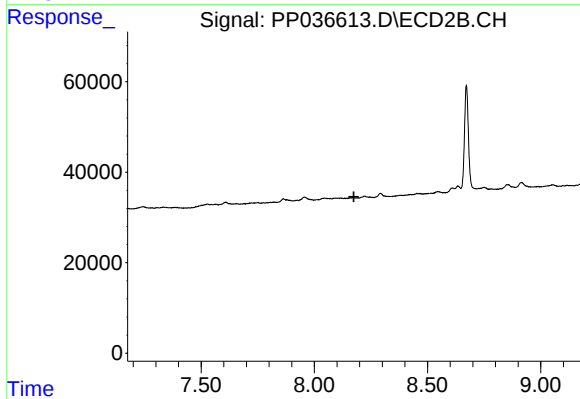

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.175 min
Response: 0
Conc: N.D.

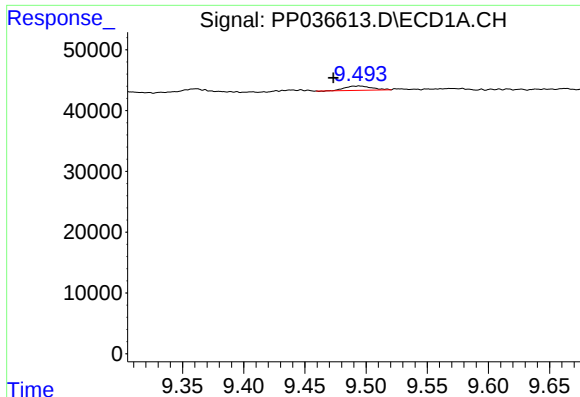

#41 AR-1268-1

R.T.: 9.494 min
Delta R.T.: 0.021 min
Response: 10809
Conc: 1.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE262Y-N-2

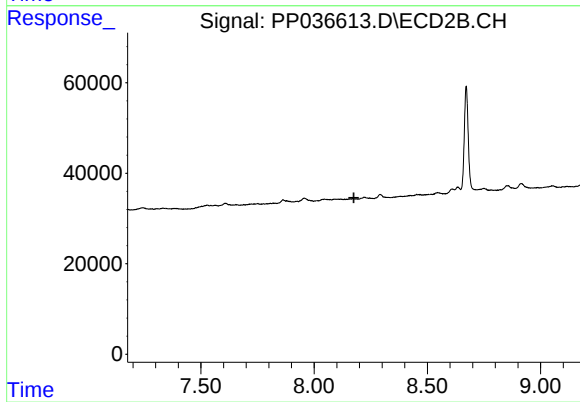

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.175 min
Response: 0
Conc: N.D.