

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036550.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 10:50
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:51:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.962	3.957	2254234	1542337	51.002	49.796
2)	SA Decachlor...	10.998	9.261	2113292	1523274	49.264	47.631
Target Compounds							
21)	L5 AR-1248-1	6.284	5.212	489675	336378	485.392	482.769
22)	L5 AR-1248-2	6.579	5.475	626659	432580	461.437	456.704
23)	L5 AR-1248-3	6.796	5.520	762691	441756	468.750	446.471
24)	L5 AR-1248-4	7.224	5.704	865130	556939	473.850	476.127
25)	L5 AR-1248-5	7.264	6.126	818653	561184	454.039	473.107m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 Client Sample ID :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 6/21/2021 2:24:41 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036550.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 10:50
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:51:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:41 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

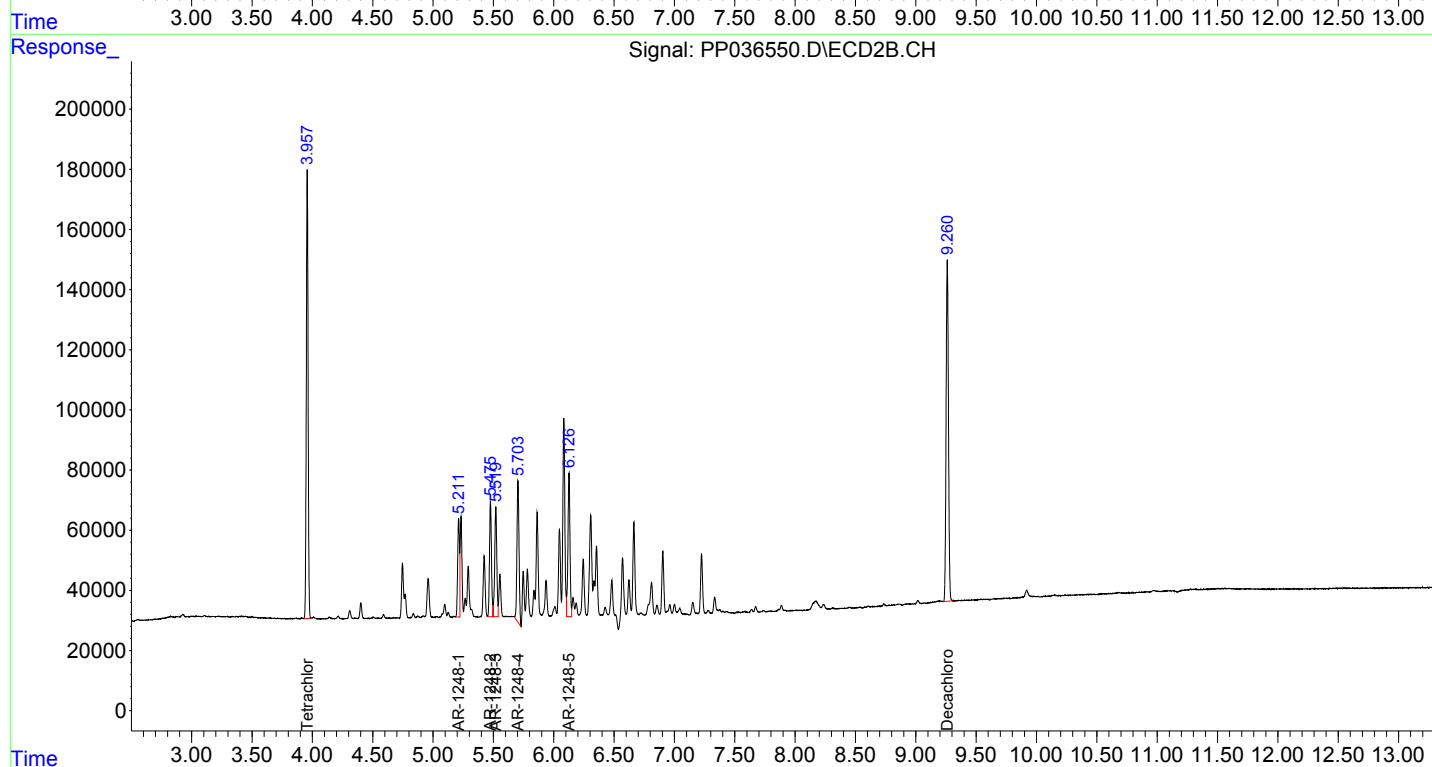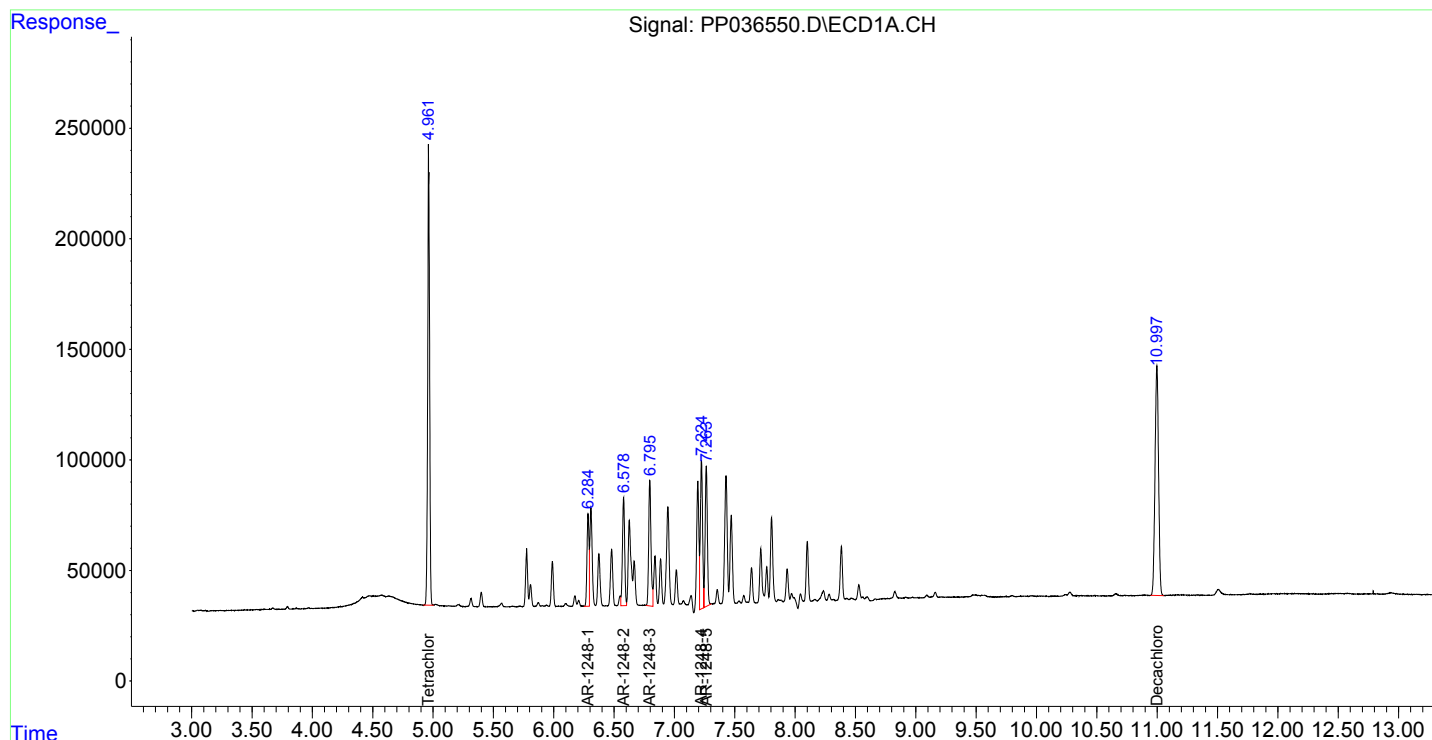

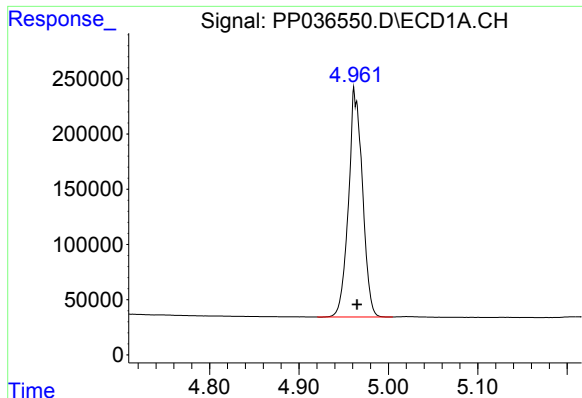


#1 Tetrachloro-m-xylene

R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 2254234
Conc: 51.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:41 PM

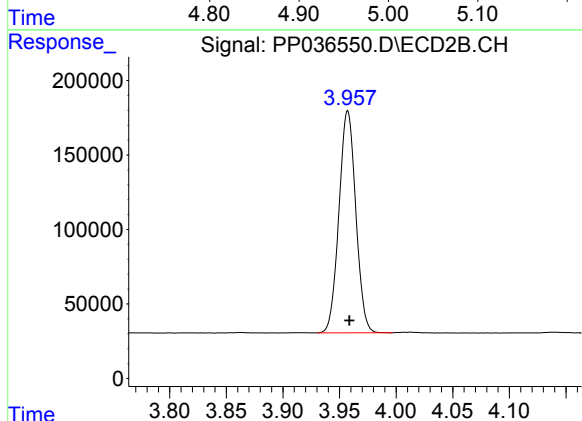


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.002 min
Response: 1542337
Conc: 49.80 ng/ml

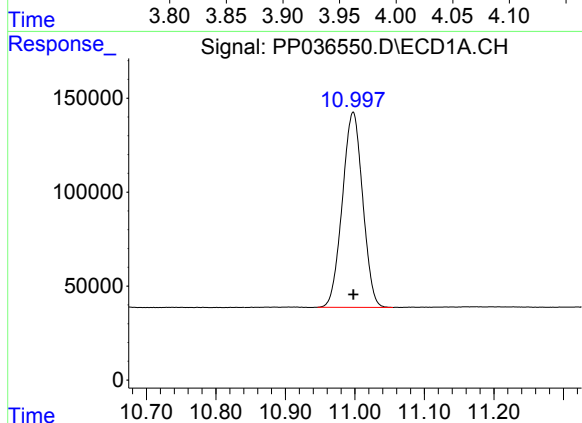


#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.000 min
Response: 2113292
Conc: 49.26 ng/ml

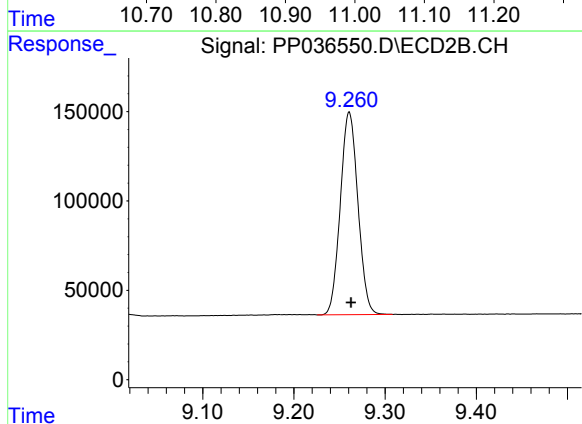

#2 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: -0.002 min
Response: 1523274
Conc: 47.63 ng/ml

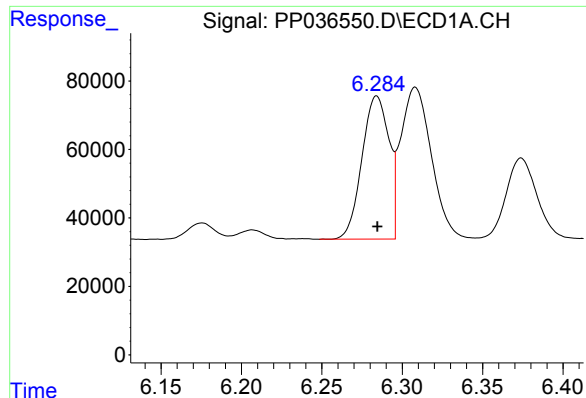


#21 AR-1248-1

R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 489675
Conc: 485.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:41 PM

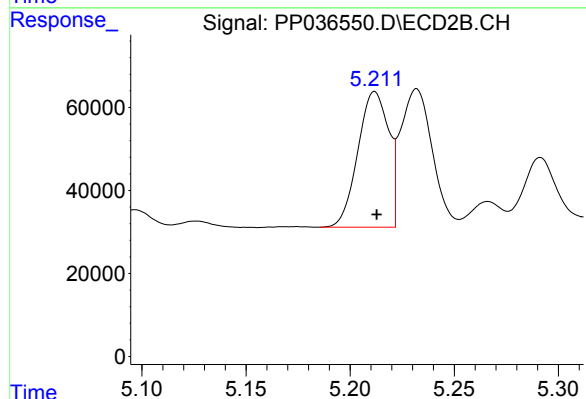


#21 AR-1248-1

R.T.: 5.212 min
Delta R.T.: 0.000 min
Response: 336378
Conc: 482.77 ng/ml

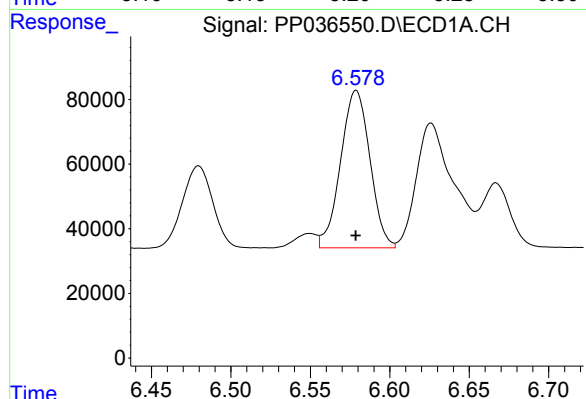


#22 AR-1248-2

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 626659
Conc: 461.44 ng/ml

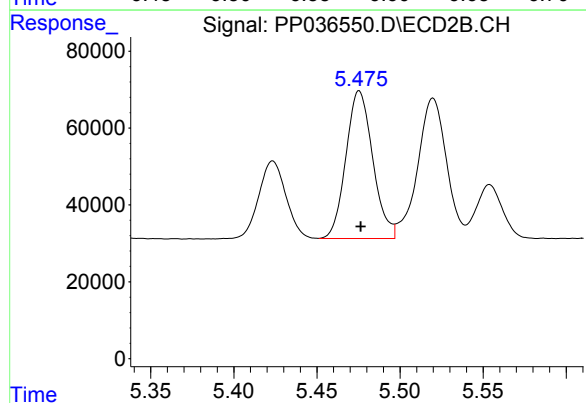

#22 AR-1248-2

R.T.: 5.475 min
Delta R.T.: 0.000 min
Response: 432580
Conc: 456.70 ng/ml

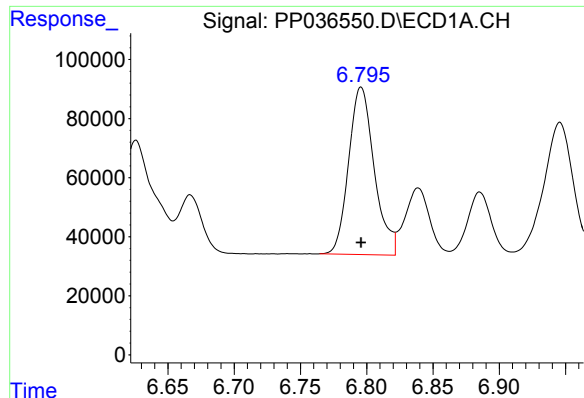


#23 AR-1248-3

R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 762691
Conc: 468.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:41 PM

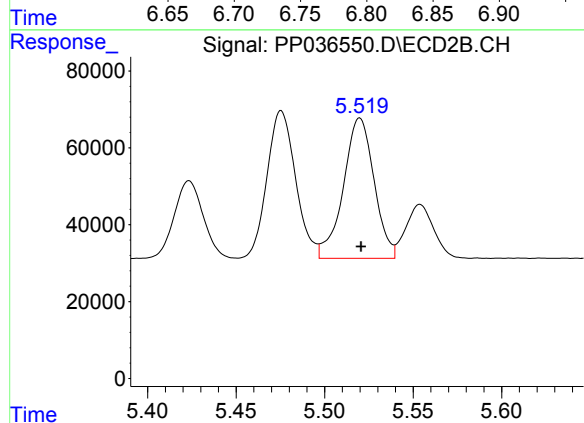


#23 AR-1248-3

R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 441756
Conc: 446.47 ng/ml

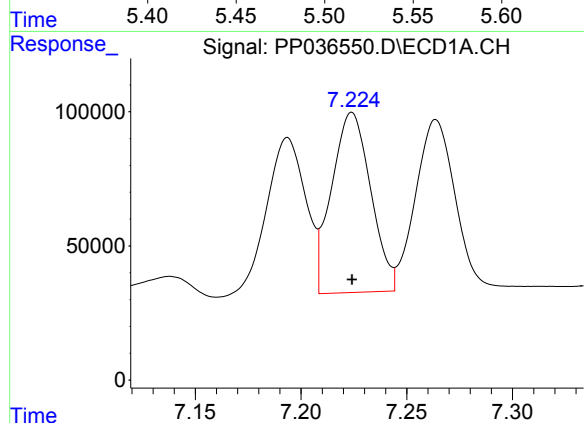


#24 AR-1248-4

R.T.: 7.224 min
Delta R.T.: 0.000 min
Response: 865130
Conc: 473.85 ng/ml

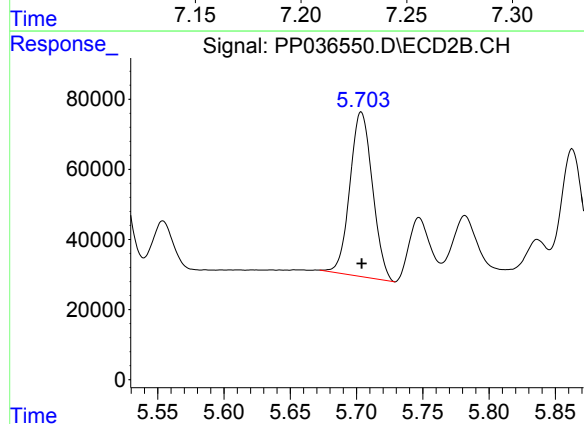

#24 AR-1248-4

R.T.: 5.704 min
Delta R.T.: 0.000 min
Response: 556939
Conc: 476.13 ng/ml

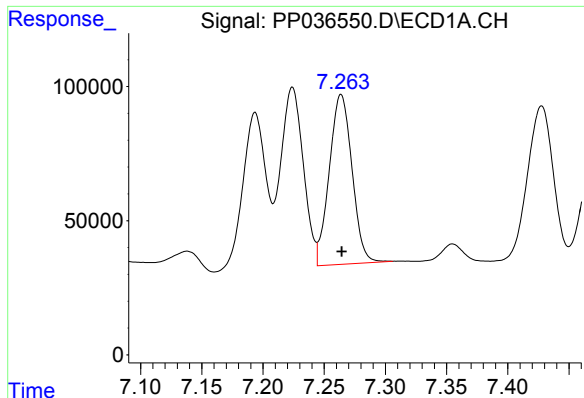


#25 AR-1248-5

R.T.: 7.264 min
Delta R.T.: 0.000 min
Response: 818653
Conc: 454.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:41 PM

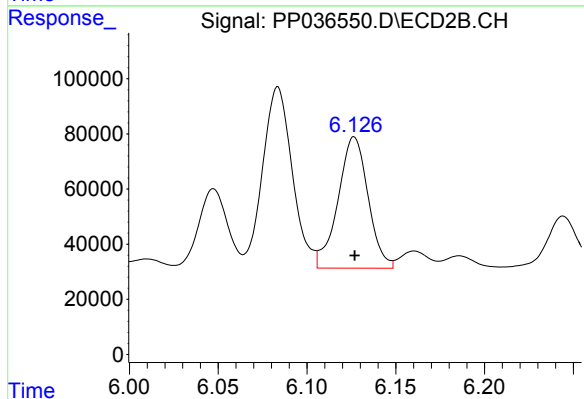

#25 AR-1248-5

R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 561184
Conc: 473.11 ng/ml m