

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036558.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 15:10
 Operator : DD\AJ
 Sample : M2709-06MS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:55:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.964	3.958	964795	687087	21.829m	22.183
2) SA Decachlor...	10.998	9.262	792640	561084	18.478	17.545

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :

ECD_P

ClientSampleId :

0224-COMP-O(DISCRETE-CL-24

Manual Integrations

APPROVED

Ankita

6/21/2021 2:24:44 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036558.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 15:10
Operator : DD\AJ
Sample : M2709-06MS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:55:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Instrument :

ECD_P

ClientSampleId :



0224-COMP-O(DISCRETE-CL-24


Manual Integrations
APPROVED

Ankita

6/21/2021 2:24:44 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

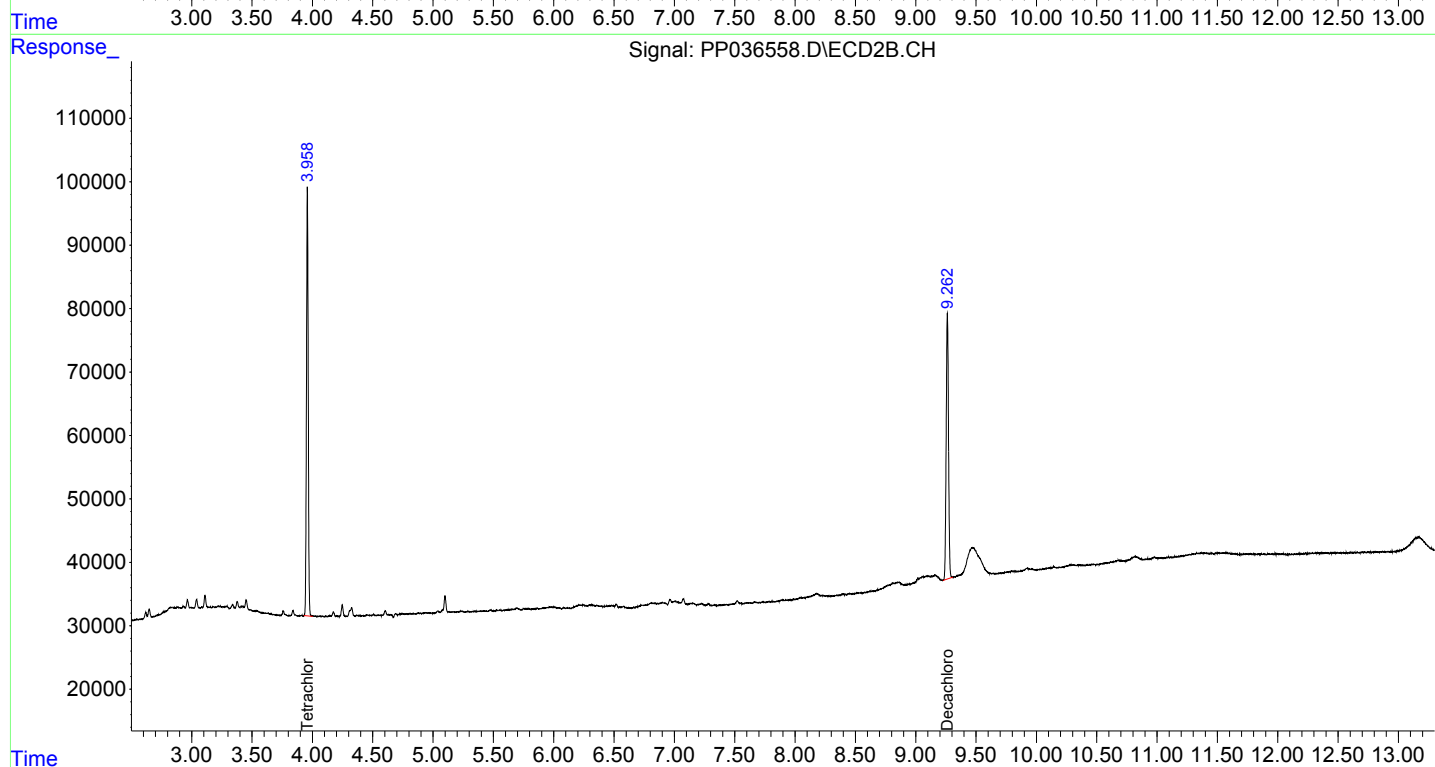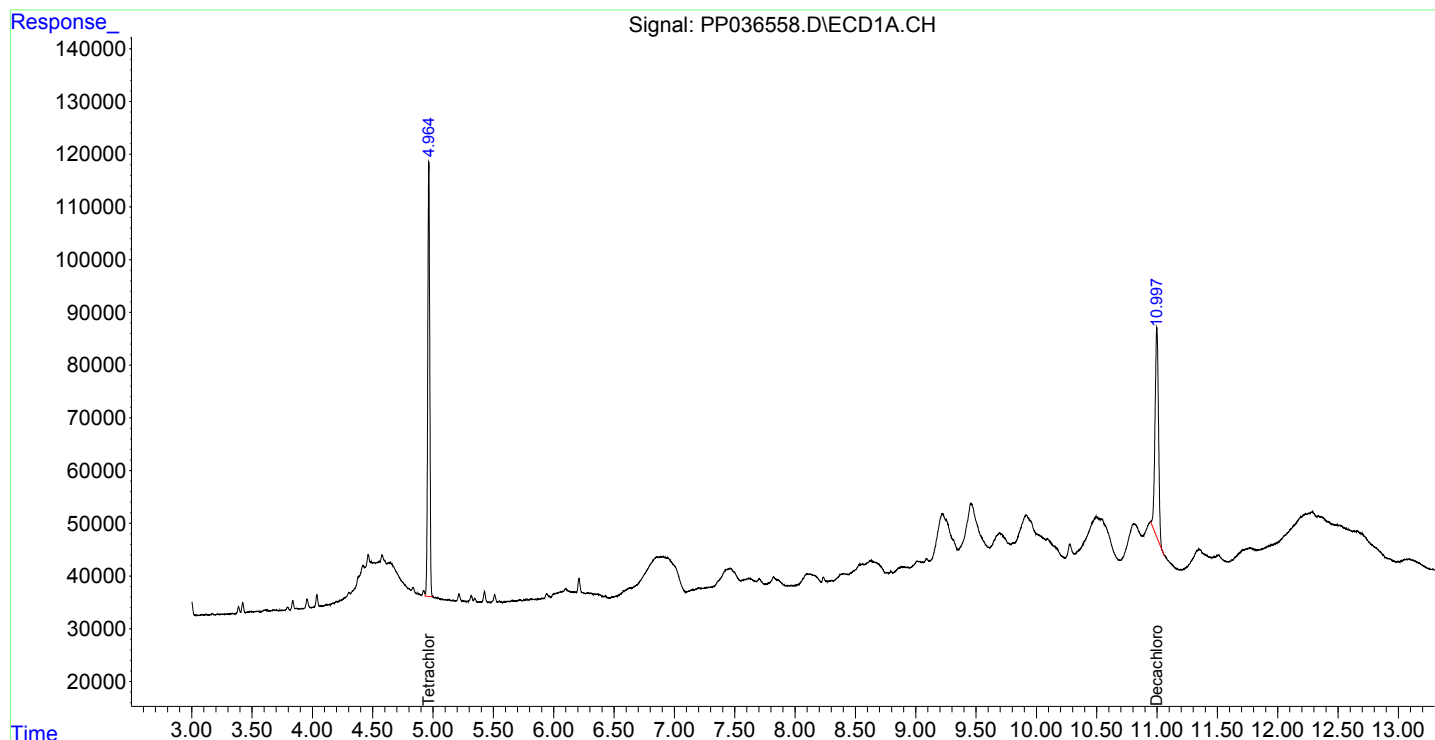

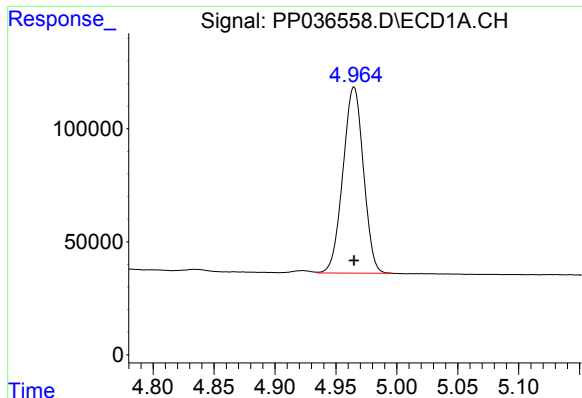


#1 Tetrachloro-m-xylene

R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 964795
Conc: 21.83 ng/ml m

Instrument :
ECD_P
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:44 PM

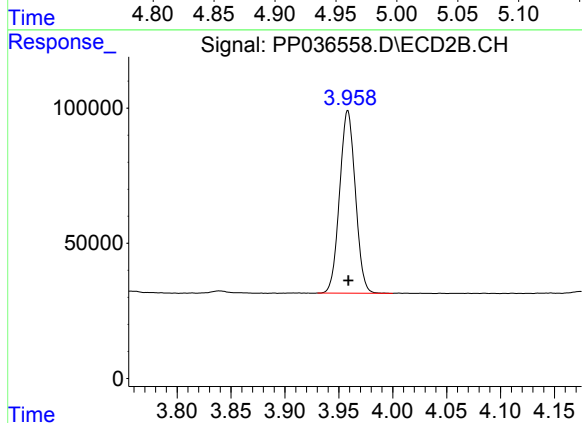


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 687087
Conc: 22.18 ng/ml

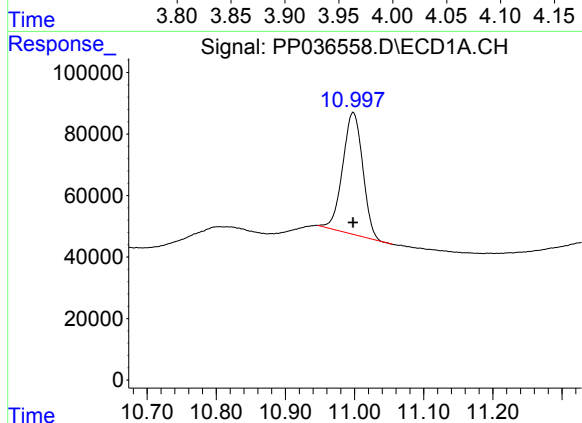

#2 Decachlorobiphenyl

R.T.: 10.998 min
Delta R.T.: 0.000 min
Response: 792640
Conc: 18.48 ng/ml

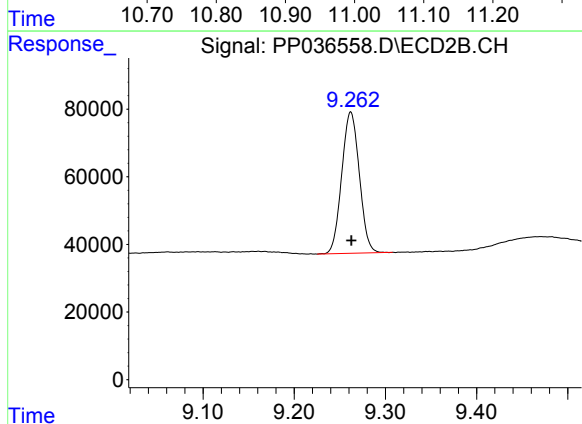

#2 Decachlorobiphenyl

R.T.: 9.262 min
Delta R.T.: 0.000 min
Response: 561084
Conc: 17.54 ng/ml