

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036564.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 16:51
 Operator : DD\AJ
 Sample : AR1262CCC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:59:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.965	3.958	2108331	1498730	47.701	48.388
2) SA Decachlor...	11.000	9.263	2216440	1553188	51.668	48.567
Target Compounds						
36) L8 AR-1262-1	8.604	7.334	1300011	556267	456.232	466.711
37) L8 AR-1262-2	9.163	7.888	2340591	1866274	460.671	476.086
38) L8 AR-1262-3	9.475	8.176	1741349	774833	470.057m	486.873
39) L8 AR-1262-4	9.572	8.239	1370160	1409545	477.049m	473.580
40) L8 AR-1262-5	10.242	8.737	994565	695620	470.747	488.139

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 Client Sample ID :
 AR1262CCC500

Manual Integrations
 APPROVED

Ankita
 6/21/2021 2:24:50 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036564.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 16:51
Operator : DD\AJ
Sample : AR1262CCC500
Misc :
ALS Vial : 7 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:59:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampleId :
AR1262CCC500

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:50 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

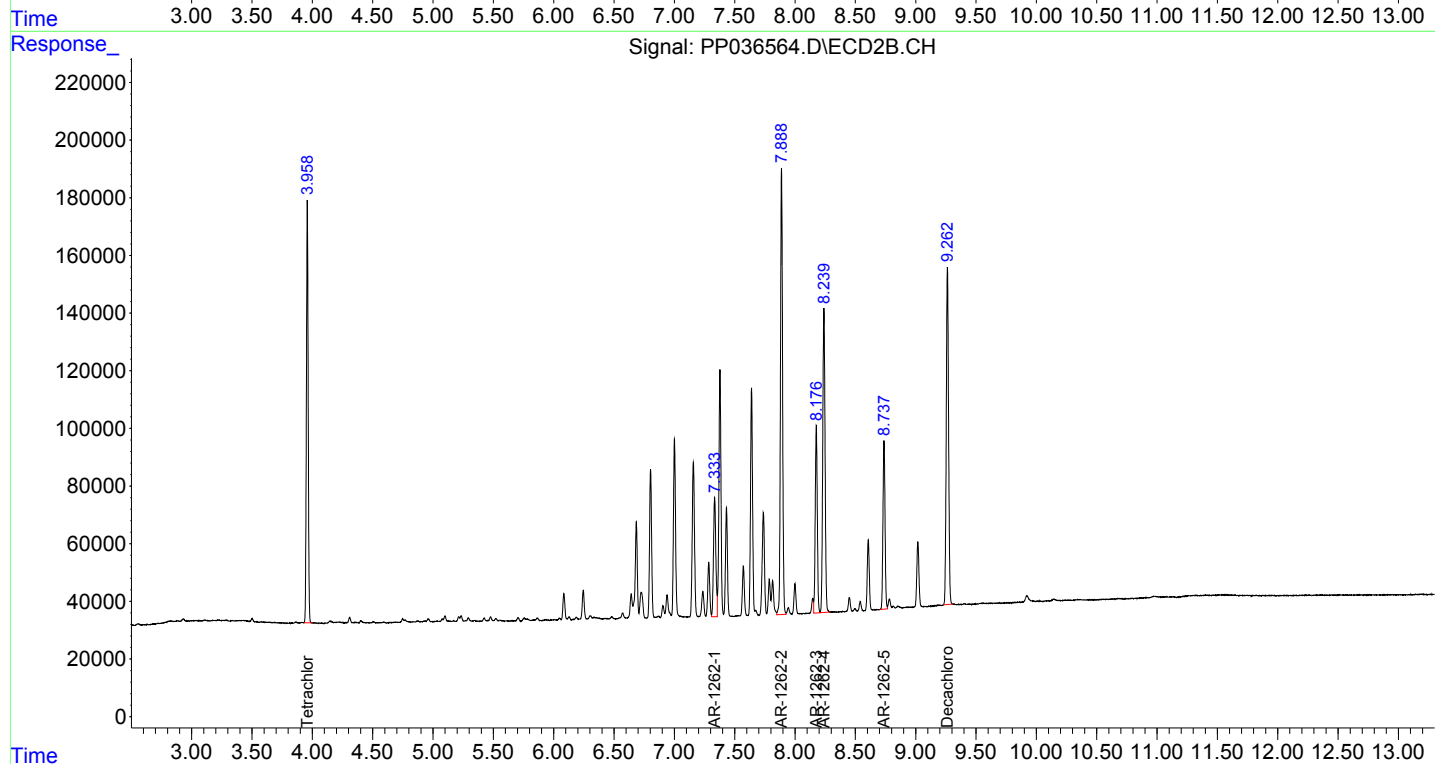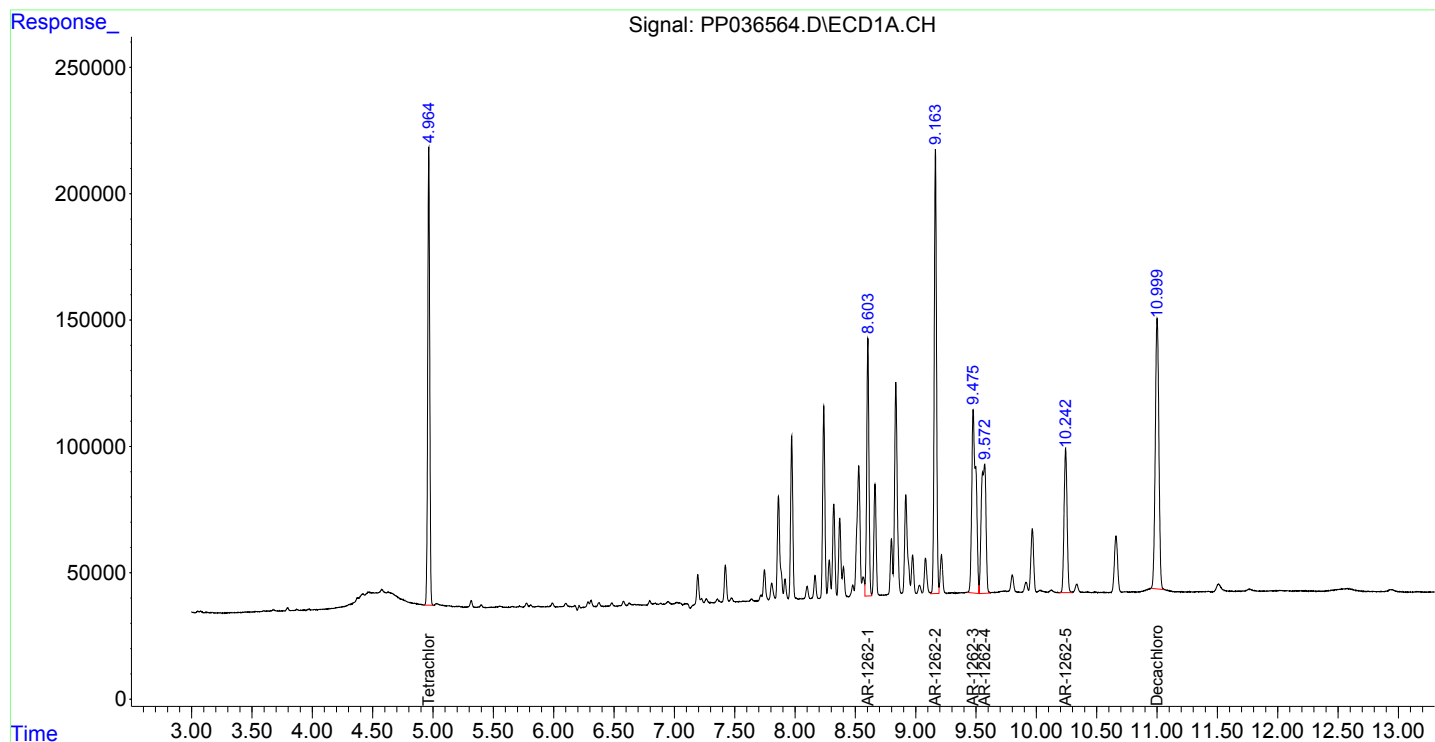

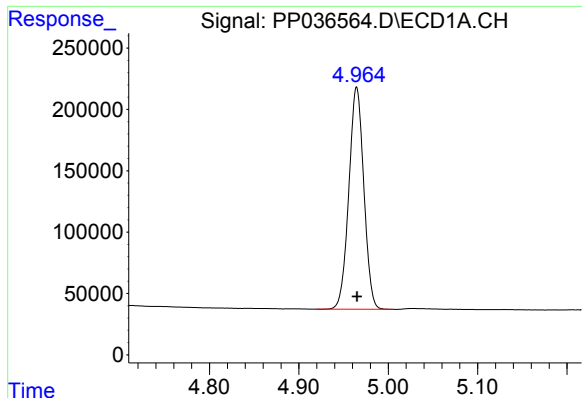


#1 Tetrachloro-m-xylene

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 2108331
Conc: 47.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:50 PM

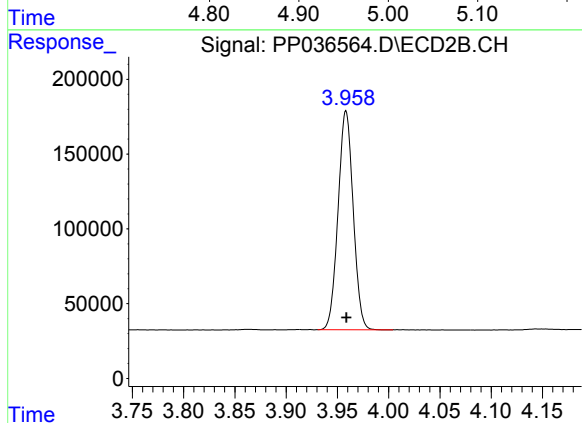


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 1498730
Conc: 48.39 ng/ml

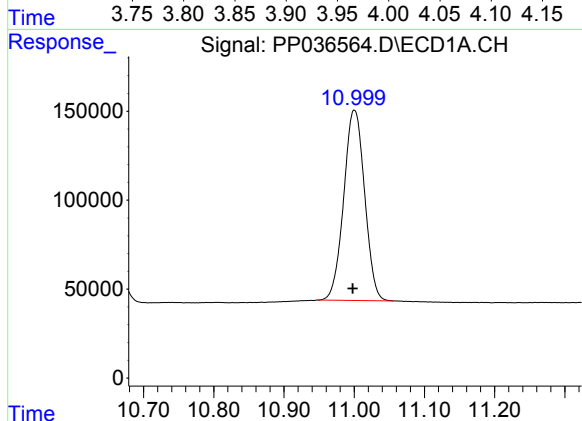


#2 Decachlorobiphenyl

R.T.: 11.000 min
Delta R.T.: 0.002 min
Response: 2216440
Conc: 51.67 ng/ml

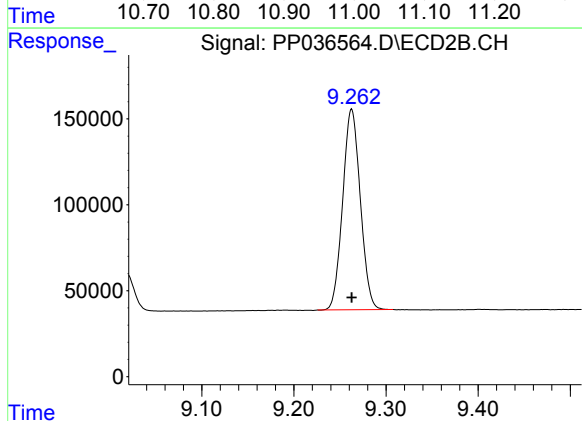

#2 Decachlorobiphenyl

R.T.: 9.263 min
Delta R.T.: 0.000 min
Response: 1553188
Conc: 48.57 ng/ml

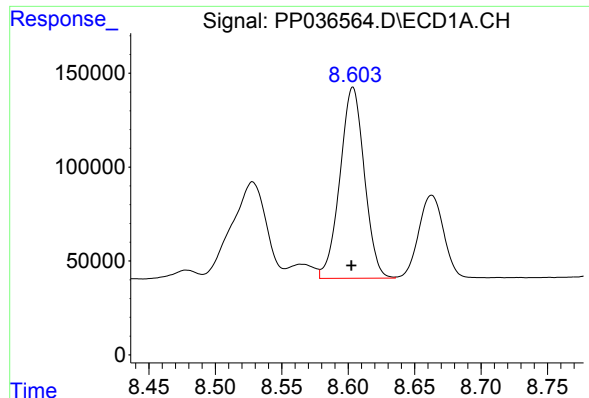


#36 AR-1262-1

R.T.: 8.604 min
Delta R.T.: 0.001 min
Response: 1300011
Conc: 456.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:50 PM

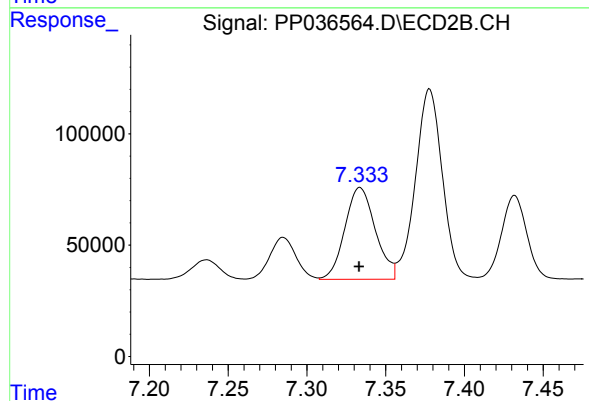


#36 AR-1262-1

R.T.: 7.334 min
Delta R.T.: 0.000 min
Response: 556267
Conc: 466.71 ng/ml

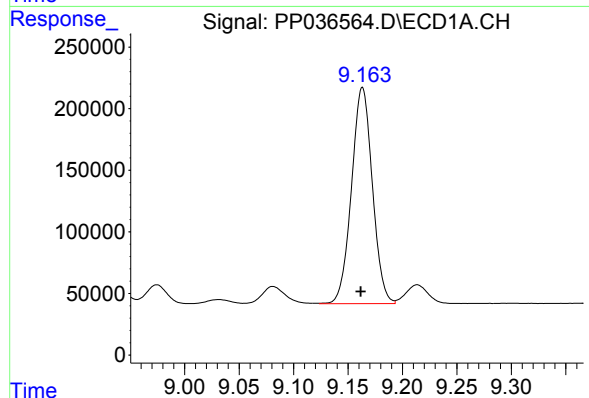


#37 AR-1262-2

R.T.: 9.163 min
Delta R.T.: 0.002 min
Response: 2340591
Conc: 460.67 ng/ml

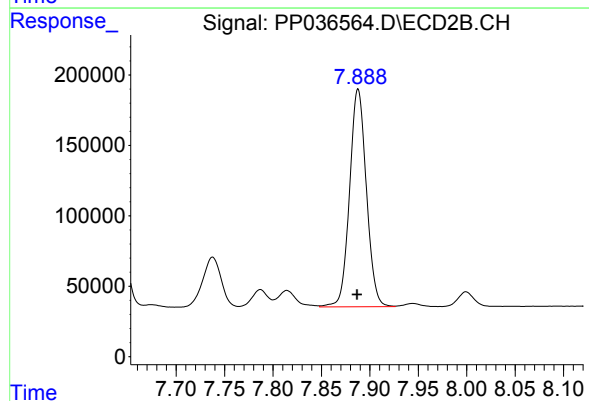

#37 AR-1262-2

R.T.: 7.888 min
Delta R.T.: 0.001 min
Response: 1866274
Conc: 476.09 ng/ml

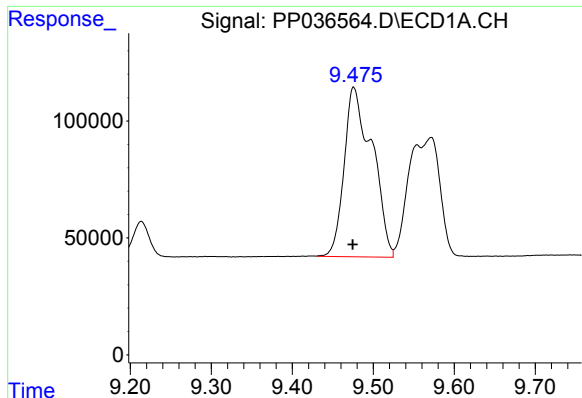


#38 AR-1262-3

R.T.: 9.475 min
Delta R.T.: 0.000 min
Response: 1741349
Conc: 470.06 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:50 PM

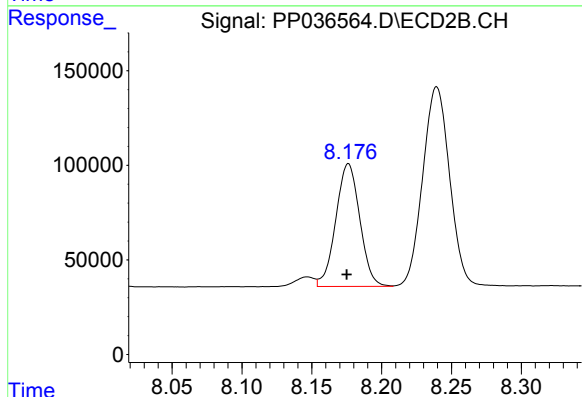


#38 AR-1262-3

R.T.: 8.176 min
Delta R.T.: 0.001 min
Response: 774833
Conc: 486.87 ng/ml

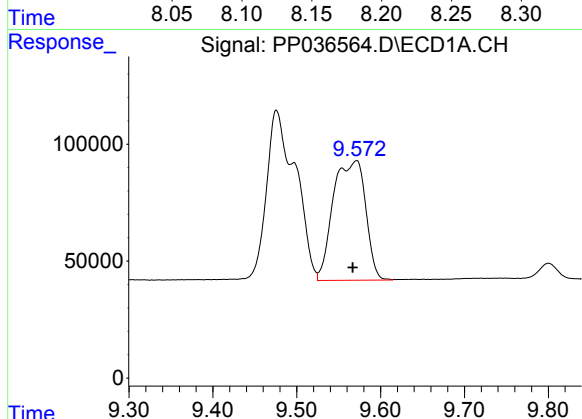


#39 AR-1262-4

R.T.: 9.572 min
Delta R.T.: 0.005 min
Response: 1370160
Conc: 477.05 ng/ml m

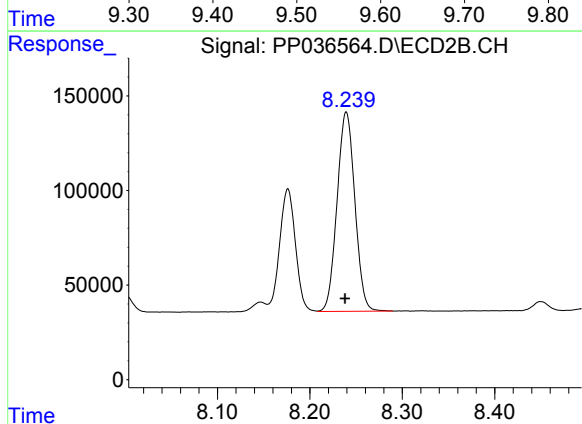

#39 AR-1262-4

R.T.: 8.239 min
Delta R.T.: 0.001 min
Response: 1409545
Conc: 473.58 ng/ml

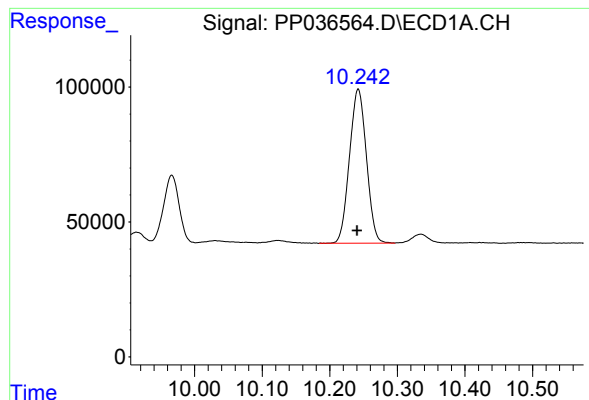


#40 AR-1262-5

R.T.: 10.242 min
Delta R.T.: 0.002 min
Response: 994565
Conc: 470.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1262CCC500

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:50 PM

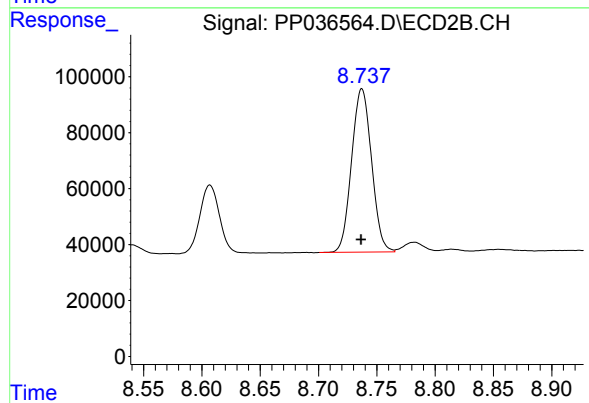

#40 AR-1262-5

R.T.: 8.737 min
Delta R.T.: 0.000 min
Response: 695620
Conc: 488.14 ng/ml