

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036570.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 18:49
 Operator : DD\AJ
 Sample : M2764-03DL 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:02:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.958	91157	65075	2.062	2.101
2)	SA Decachlor...	10.999	9.263	330159	222919	7.696	6.970
Target Compounds							
41)	L9 AR-1268-1	9.475	8.177	1820417	1314265	303.428	282.237
42)	L9 AR-1268-2	9.572	8.242	1993128	1462763	349.650	339.107
43)	L9 AR-1268-3	9.801	8.451	571993	383720	118.974	105.097
44)	L9 AR-1268-4	10.243	8.738	1361005	932033	577.800	585.918
45)	L9 AR-1268-5	10.661	9.018	2629767	1870465	171.005	158.210m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 ClientSampleId :
 PHC-250EM-002DL

Manual Integrations
 APPROVED

Ankita
 6/21/2021 2:24:56 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036570.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 18:49
Operator : DD\AJ
Sample : M2764-03DL 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:02:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampleID :
PHC-250EM-002DL

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:56 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

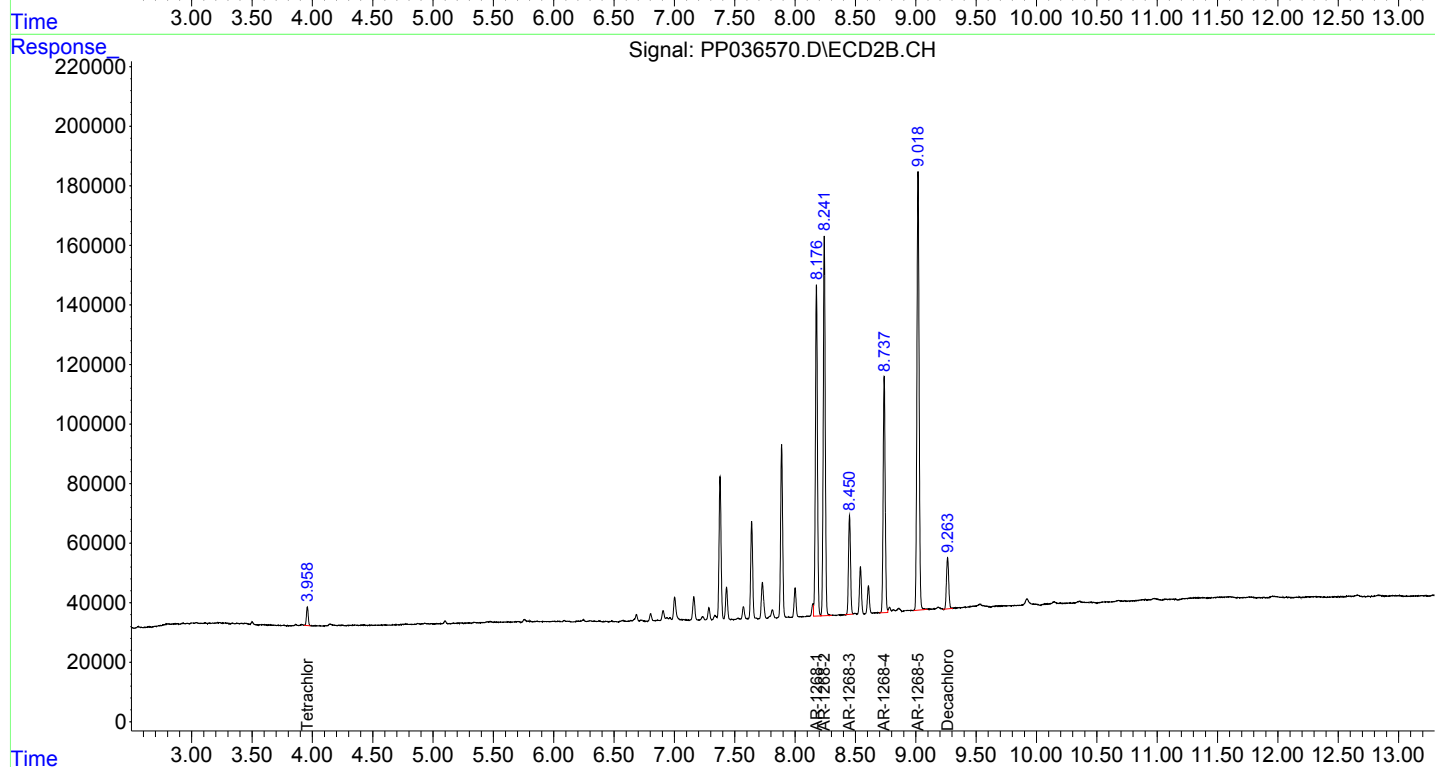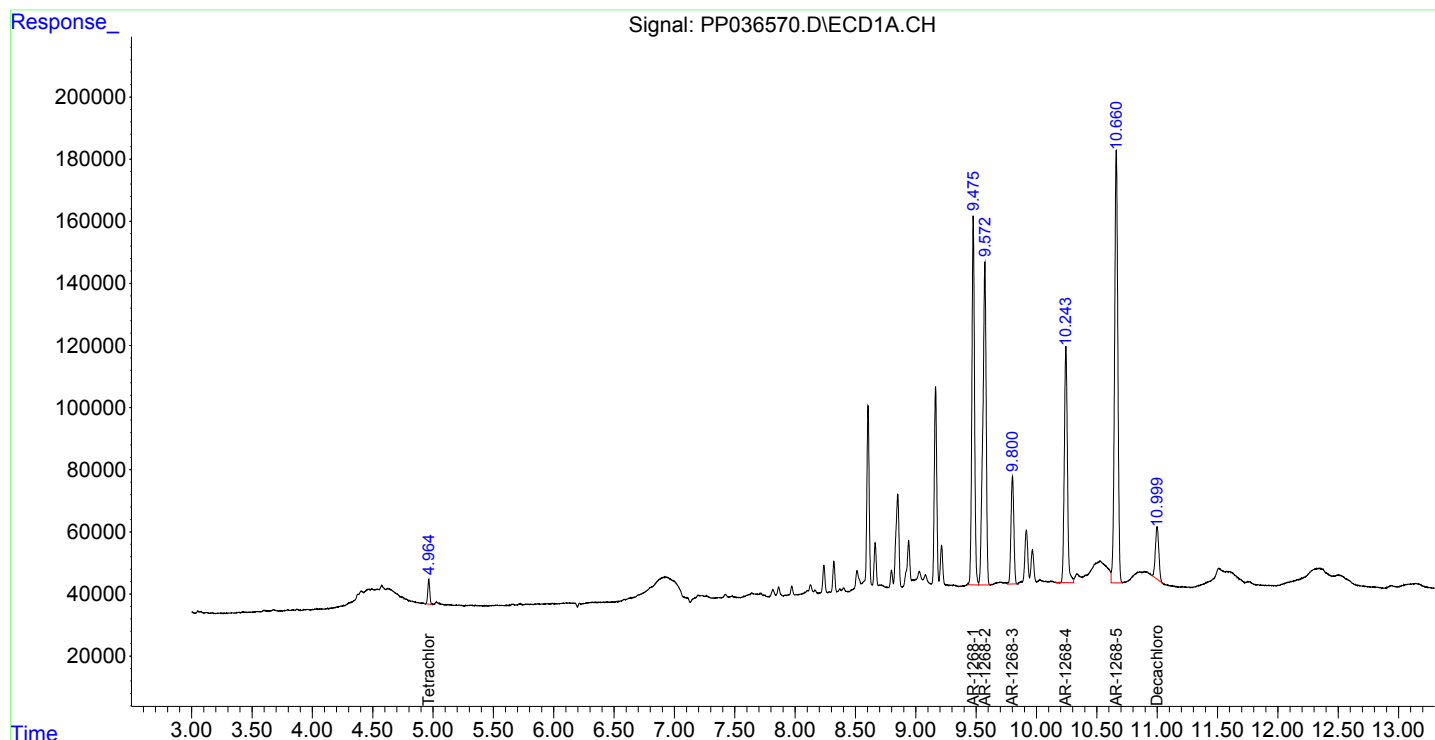

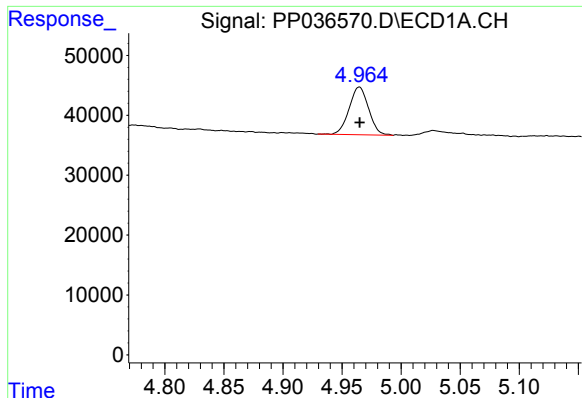


#1 Tetrachloro-m-xylene

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 91157
Conc: 2.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
PHC-250EM-002DL


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:56 PM

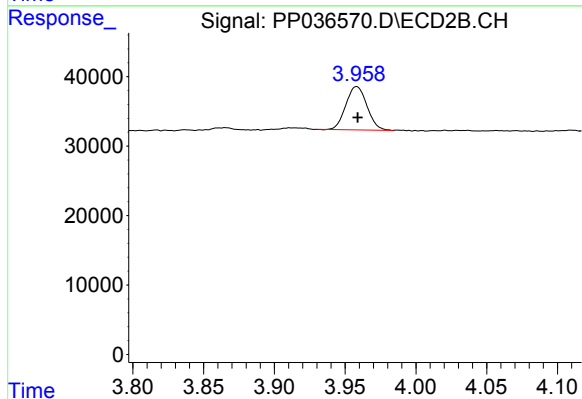


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 65075
Conc: 2.10 ng/ml

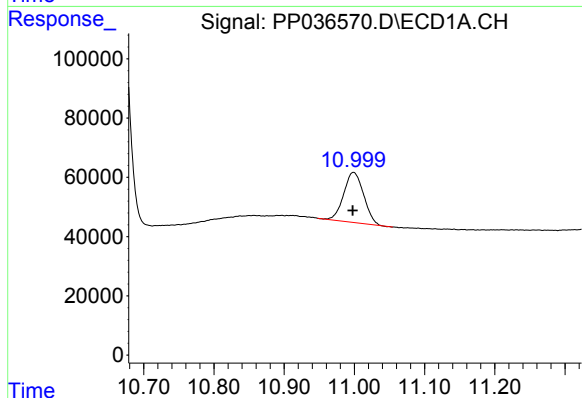


#2 Decachlorobiphenyl

R.T.: 10.999 min
Delta R.T.: 0.000 min
Response: 330159
Conc: 7.70 ng/ml

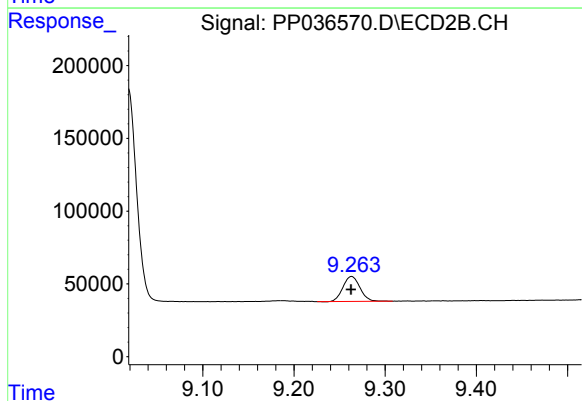

#2 Decachlorobiphenyl

R.T.: 9.263 min
Delta R.T.: 0.000 min
Response: 222919
Conc: 6.97 ng/ml

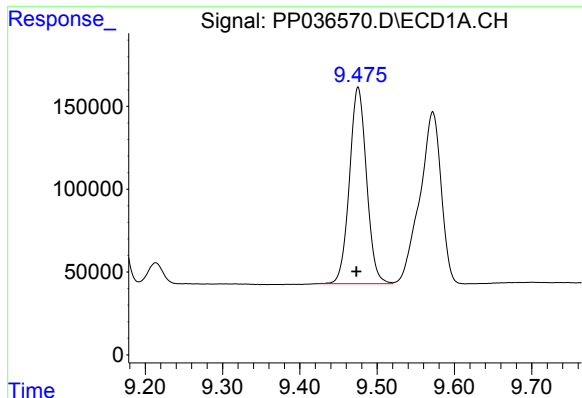


#41 AR-1268-1

R.T.: 9.475 min
Delta R.T.: 0.002 min
Response: 1820417
Conc: 303.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
PHC-250EM-002DL


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:56 PM

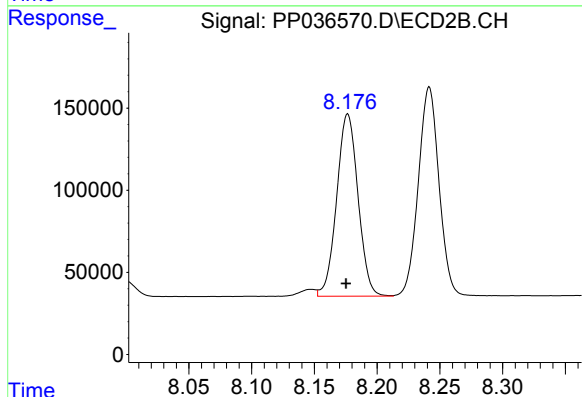


#41 AR-1268-1

R.T.: 8.177 min
Delta R.T.: 0.001 min
Response: 1314265
Conc: 282.24 ng/ml

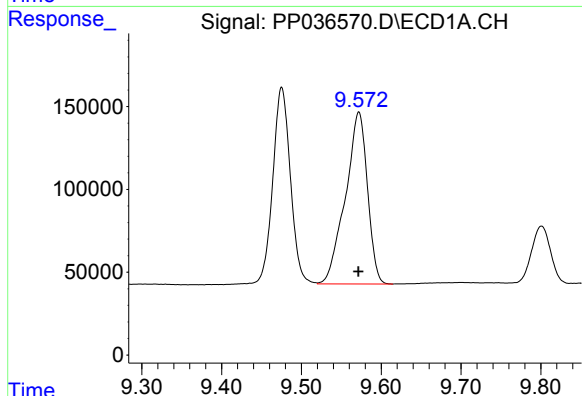


#42 AR-1268-2

R.T.: 9.572 min
Delta R.T.: 0.000 min
Response: 1993128
Conc: 349.65 ng/ml

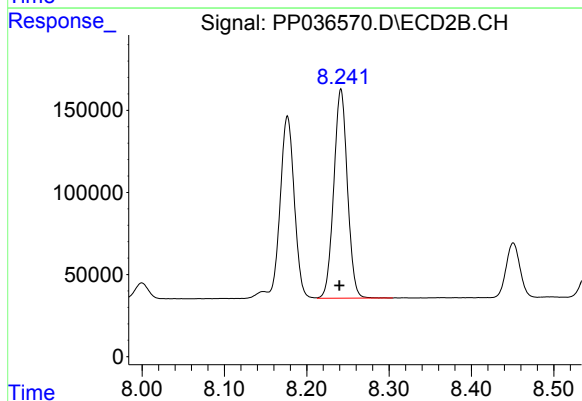

#42 AR-1268-2

R.T.: 8.242 min
Delta R.T.: 0.002 min
Response: 1462763
Conc: 339.11 ng/ml

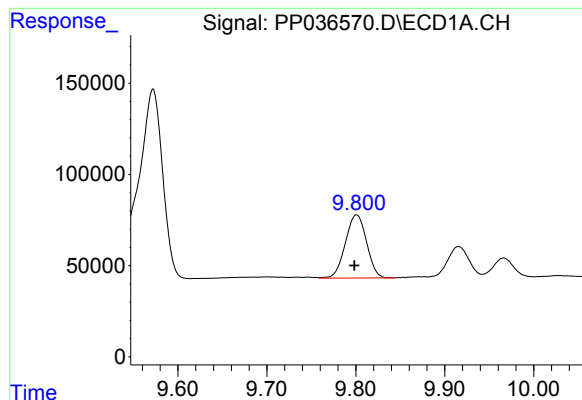


#43 AR-1268-3

R.T.: 9.801 min
Delta R.T.: 0.002 min
Response: 571993
Conc: 118.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
PHC-250EM-002DL


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:56 PM

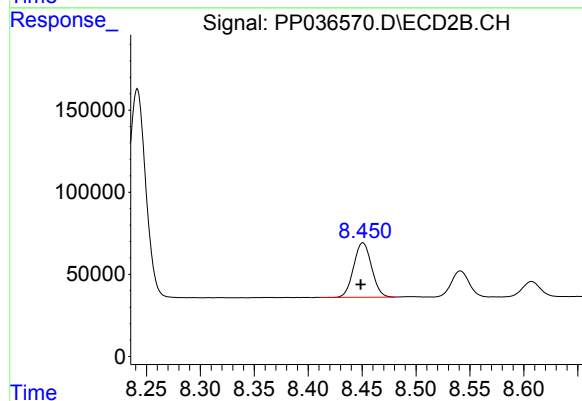


#43 AR-1268-3

R.T.: 8.451 min
Delta R.T.: 0.002 min
Response: 383720
Conc: 105.10 ng/ml

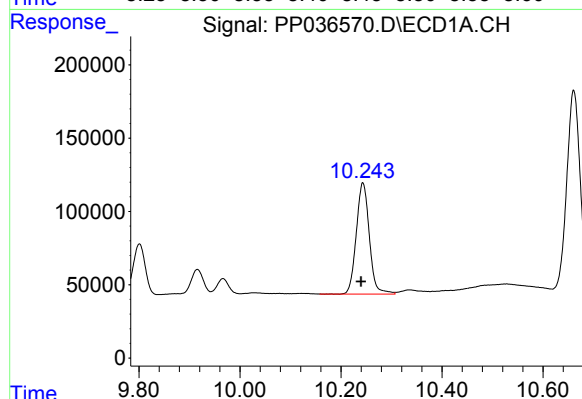


#44 AR-1268-4

R.T.: 10.243 min
Delta R.T.: 0.003 min
Response: 1361005
Conc: 577.80 ng/ml

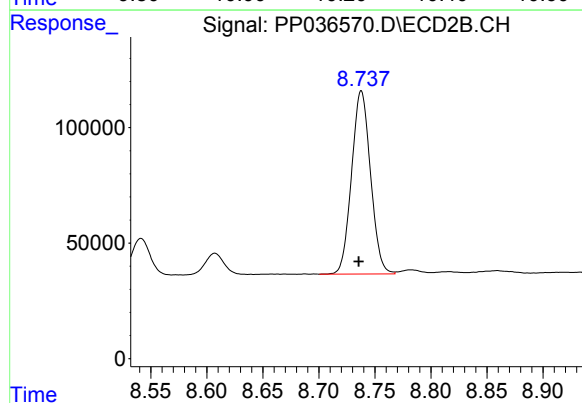

#44 AR-1268-4


R.T.: 8.738 min
Delta R.T.: 0.002 min
Response: 932033
Conc: 585.92 ng/ml

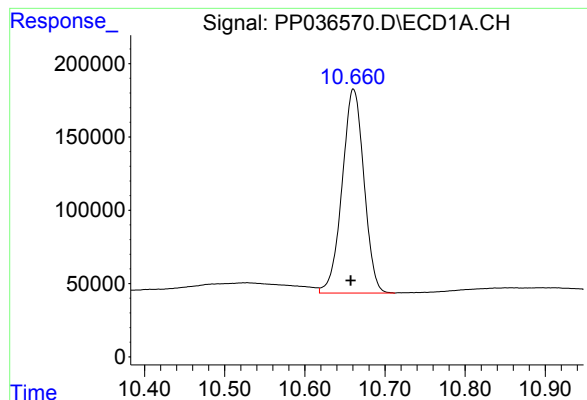

#45 AR-1268-5

R.T.: 10.661 min
Delta R.T.: 0.003 min
Response: 2629767
Conc: 171.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
PHC-250EM-002DL

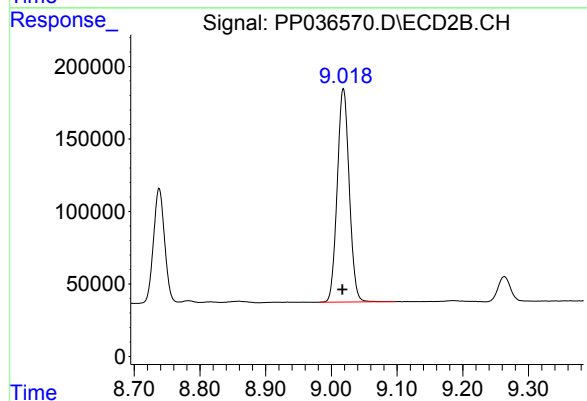

#45 AR-1268-5

R.T.: 9.018 min
Delta R.T.: 0.001 min
Response: 1870465
Conc: 158.21 ng/ml m

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:56 PM