

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036572.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 19:39
 Operator : DD\AJ
 Sample : M2709-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:03:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.967	3.960	805878	568141	18.233	18.343
2)	SA Decachlor...	11.003	9.265	776221	508530	18.095	15.901
Target Compounds							
26)	L6 AR-1254-1	7.197	6.086	71425	61048	40.613	36.030
27)	L6 AR-1254-2	7.426	6.247	106262	48940	39.273	32.903
28)	L6 AR-1254-3	7.808	6.666	104836	79020	35.393	32.503
29)	L6 AR-1254-4	8.104	6.907	74987	41239	34.110	26.649
30)	L6 AR-1254-5	8.532	7.336	73960	55848	31.100	25.972m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :

ECD_P

Client Sample Id :

0223-COMP-O(DISCRETE-CL-23

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:57 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036572.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 19:39
Operator : DD\AJ
Sample : M2709-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:03:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Instrument :



ECD_P


ClientSampleId :

0223-COMP-O(DISCRETE-CL-23

Manual Integrations
APPROVEDAnkita
6/21/2021 2:24:57 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

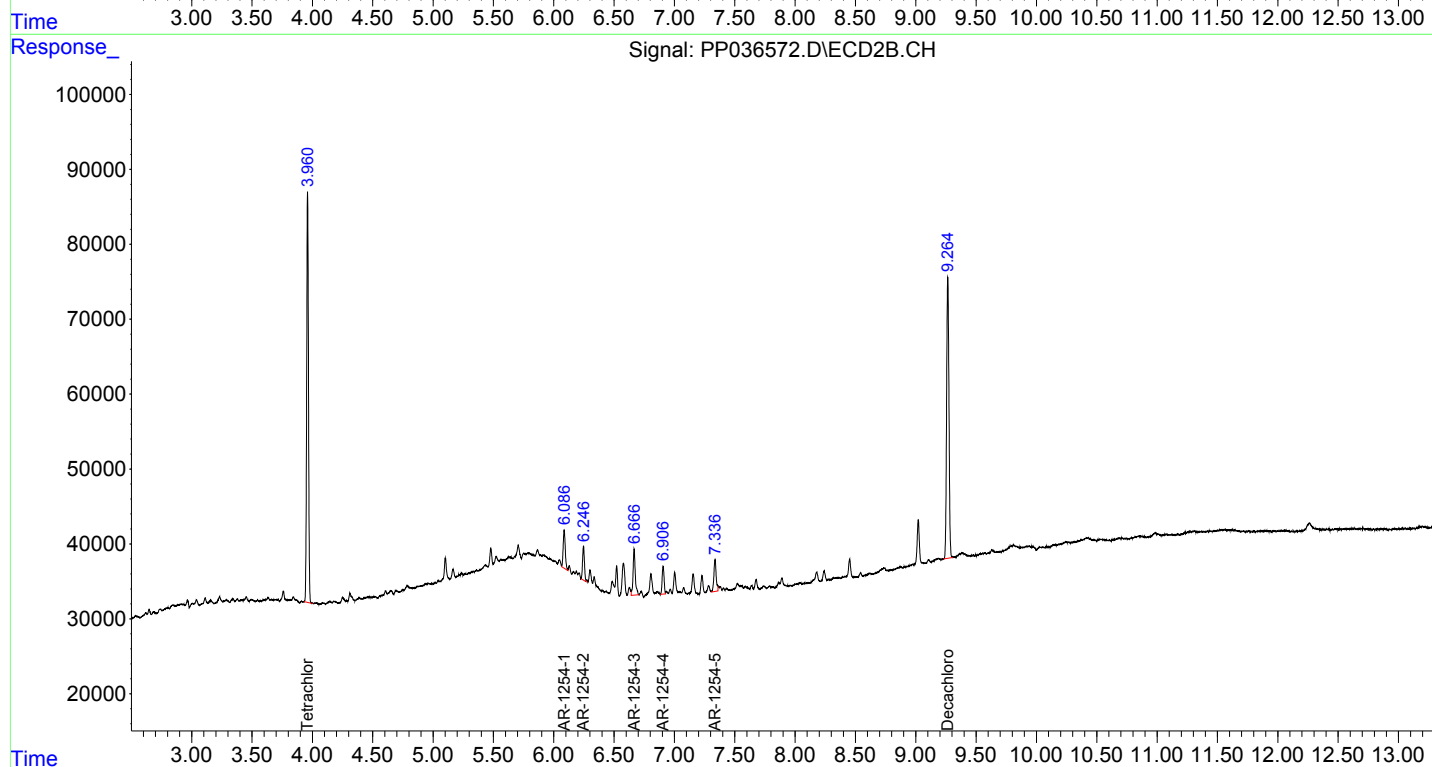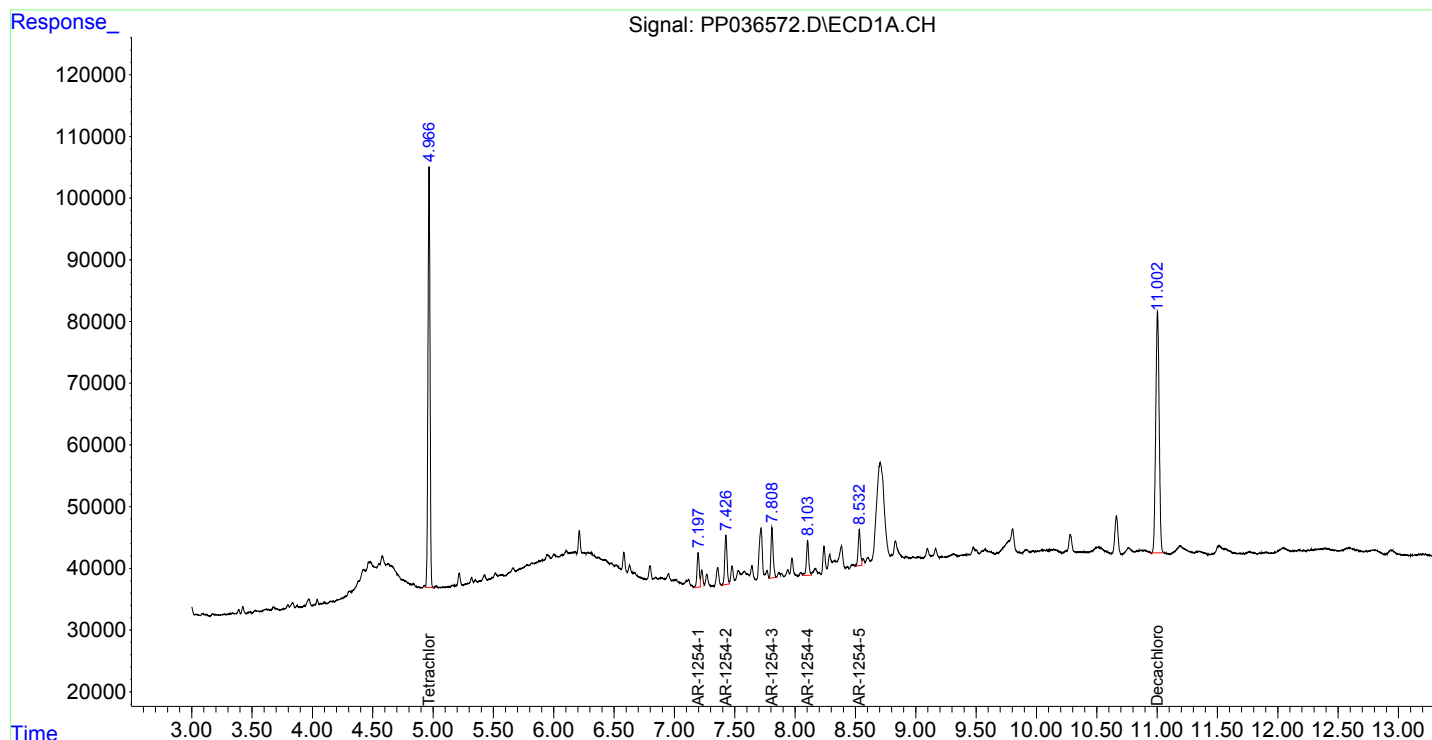

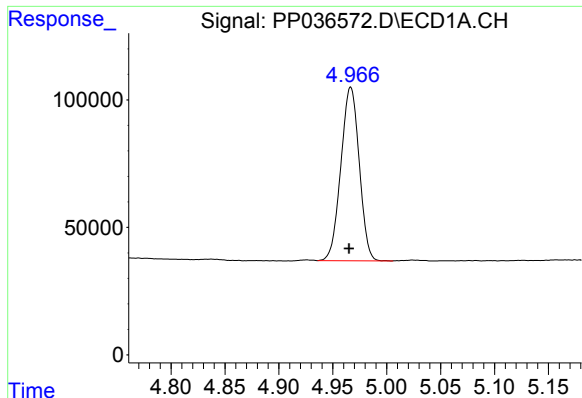


#1 Tetrachloro-m-xylene

R.T.: 4.967 min
Delta R.T.: 0.002 min
Response: 805878
Conc: 18.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
0223-COMP-O(DISCRETE-CL-23


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:57 PM

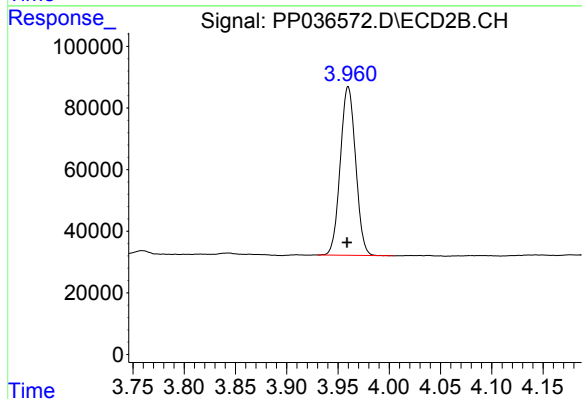


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.001 min
Response: 568141
Conc: 18.34 ng/ml

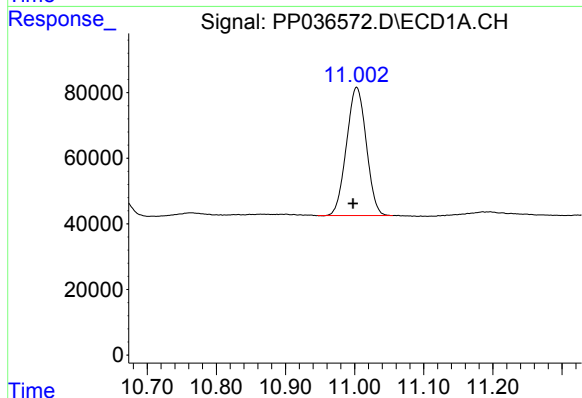


#2 Decachlorobiphenyl

R.T.: 11.003 min
Delta R.T.: 0.005 min
Response: 776221
Conc: 18.09 ng/ml

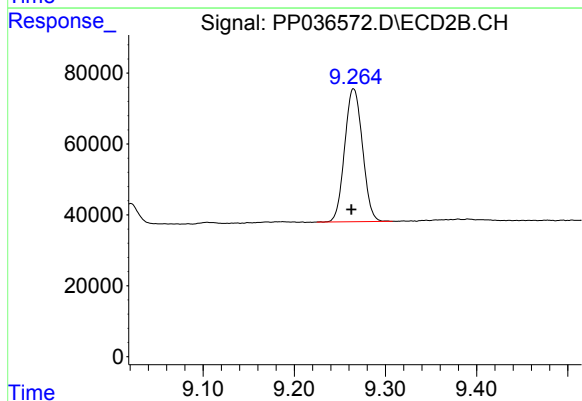

#2 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: 0.002 min
Response: 508530
Conc: 15.90 ng/ml

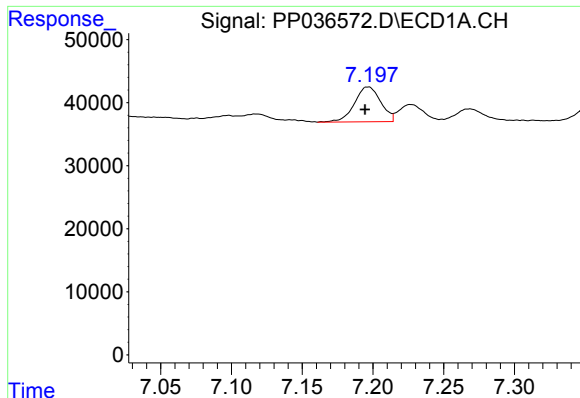


#26 AR-1254-1

R.T.: 7.197 min
Delta R.T.: 0.003 min
Response: 71425
Conc: 40.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
0223-COMP-O(DISCRETE-CL-23


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:57 PM

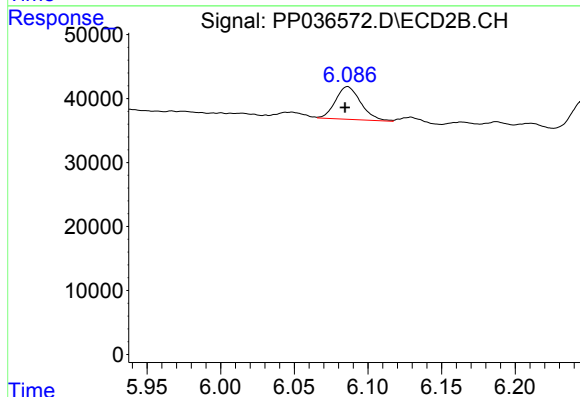


#26 AR-1254-1

R.T.: 6.086 min
Delta R.T.: 0.002 min
Response: 61048
Conc: 36.03 ng/ml

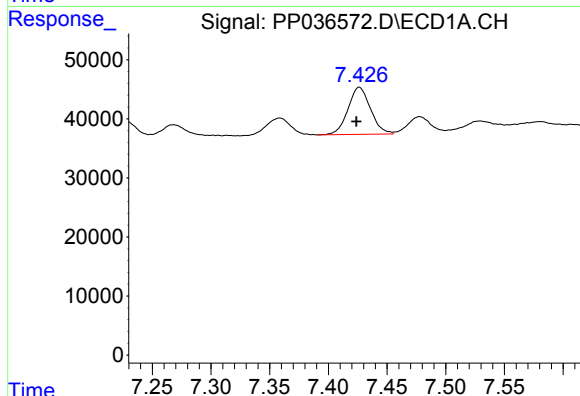


#27 AR-1254-2

R.T.: 7.426 min
Delta R.T.: 0.002 min
Response: 106262
Conc: 39.27 ng/ml

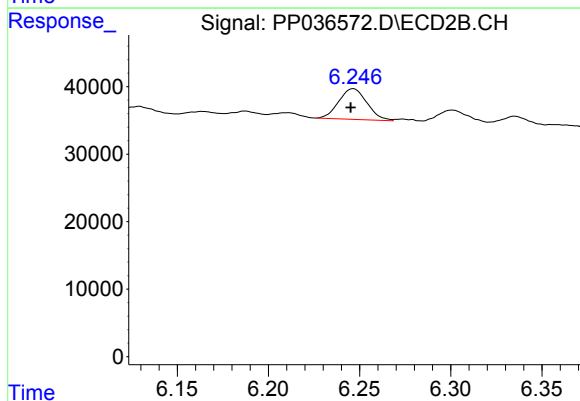

#27 AR-1254-2

R.T.: 6.247 min
Delta R.T.: 0.001 min
Response: 48940
Conc: 32.90 ng/ml

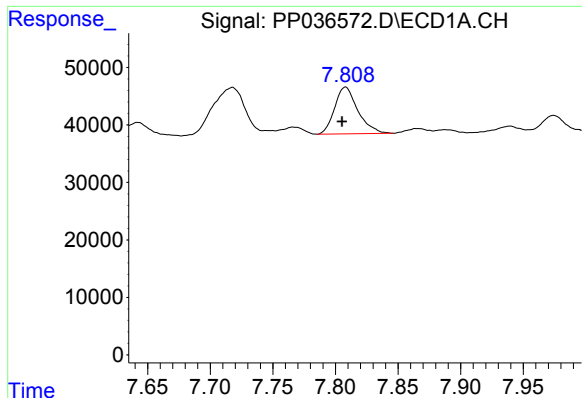


#28 AR-1254-3

R.T.: 7.808 min
Delta R.T.: 0.003 min
Response: 104836
Conc: 35.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
0223-COMP-O(DISCRETE-CL-23


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:57 PM

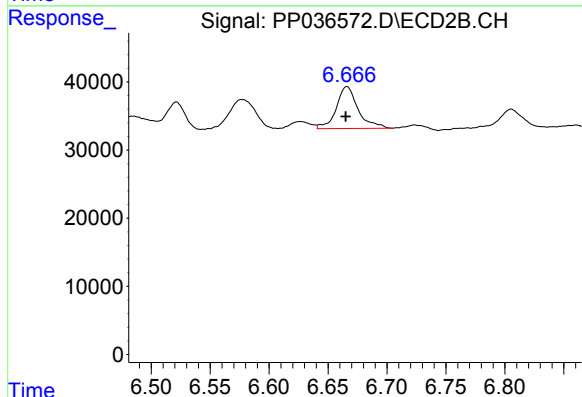


#28 AR-1254-3

R.T.: 6.666 min
Delta R.T.: 0.001 min
Response: 79020
Conc: 32.50 ng/ml

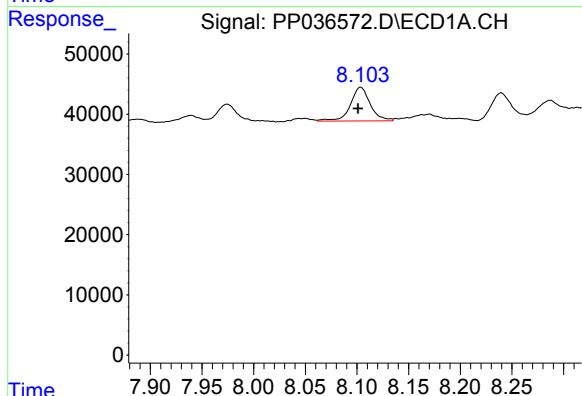


#29 AR-1254-4

R.T.: 8.104 min
Delta R.T.: 0.002 min
Response: 74987
Conc: 34.11 ng/ml

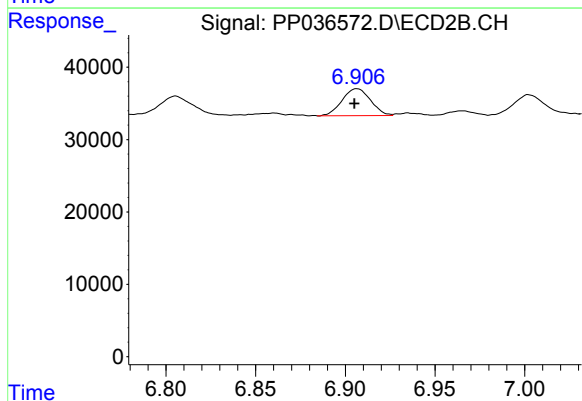


#29 AR-1254-4

R.T.: 6.907 min
Delta R.T.: 0.001 min
Response: 41239
Conc: 26.65 ng/ml

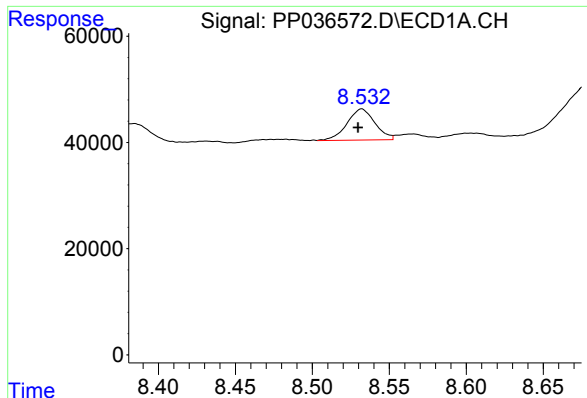

#30 AR-1254-5

R.T.: 8.532 min
Delta R.T.: 0.002 min
Response: 73960
Conc: 31.10 ng/ml

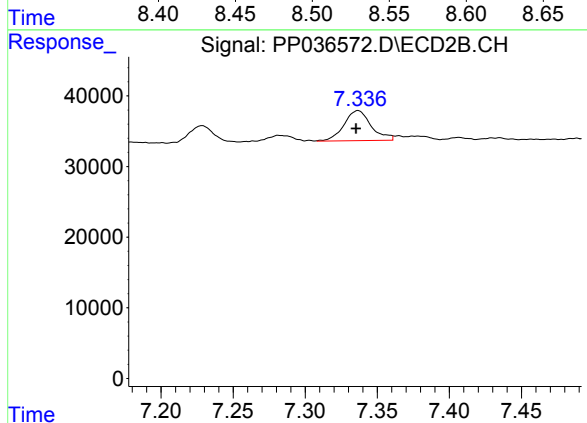

#30 AR-1254-5

R.T.: 7.336 min
Delta R.T.: 0.000 min
Response: 55848
Conc: 25.97 ng/ml m

Instrument :
ECD_P
ClientSampleId :
0223-COMP-O(DISCRETE-CL-23

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:57 PM