

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036573.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 19:56
 Operator : DD\AJ
 Sample : M2709-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:04:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.965	3.959	862479	596186	19.514m	19.248
2) SA Decachlor...	11.000	9.262	687715	446410	16.032	13.959
Target Compounds						
26) L6 AR-1254-1	7.196	6.085	81809	85719	46.518	50.591
27) L6 AR-1254-2	7.426	6.245	133110	54111	49.196	36.380 #
28) L6 AR-1254-3	7.807	6.664	128839	89030	43.497	36.620
29) L6 AR-1254-4	8.103	6.905	74919	46139	34.080	29.816
30) L6 AR-1254-5	8.531	7.334	71513	56108	30.071	26.093m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 Client Sample ID :
 0240-AMND-COMP-E

Manual Integrations
 APPROVED

Ankita
 6/21/2021 2:24:59 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036573.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 19:56
Operator : DD\AJ
Sample : M2709-07
Misc :
ALS Vial : 23 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:04:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampleId :
0240-AMND-COMP-E

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:59 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

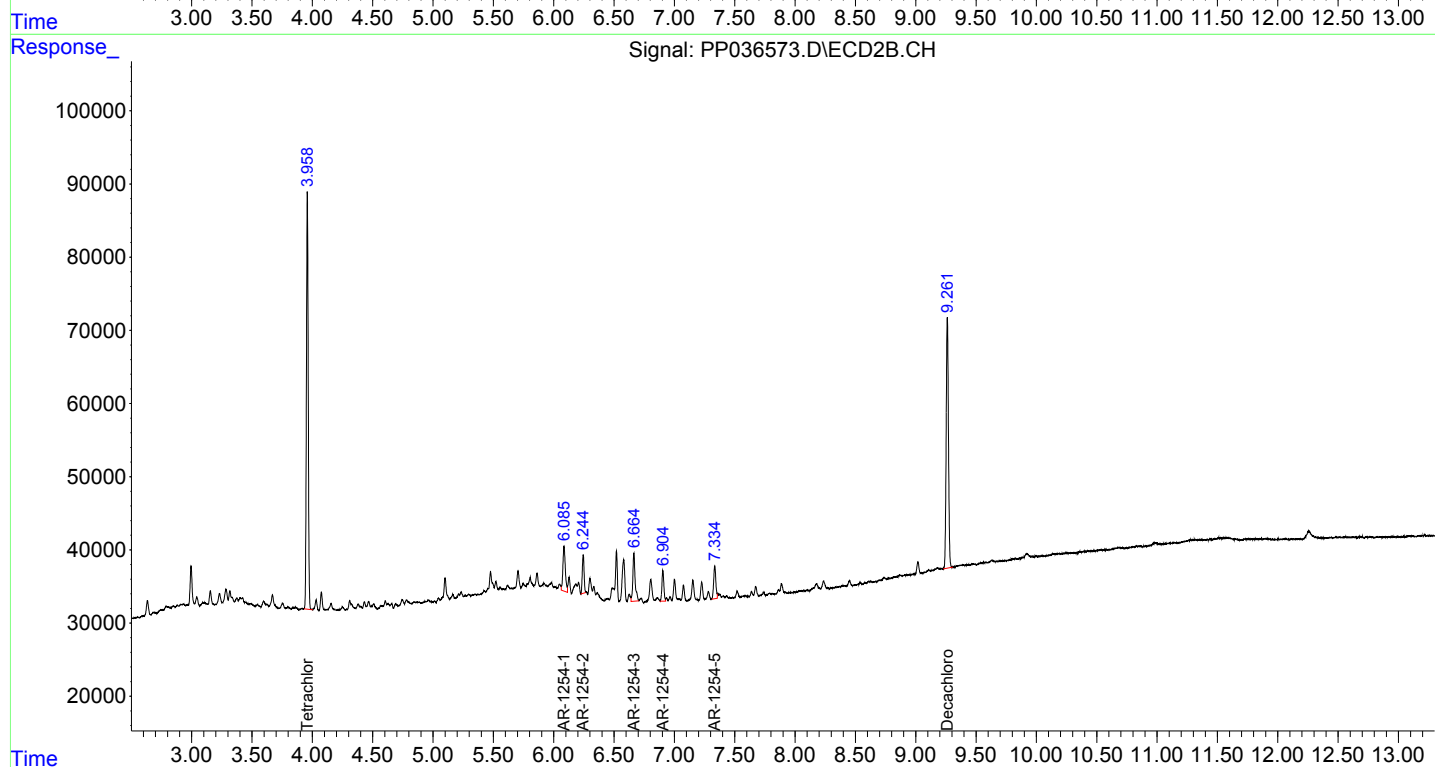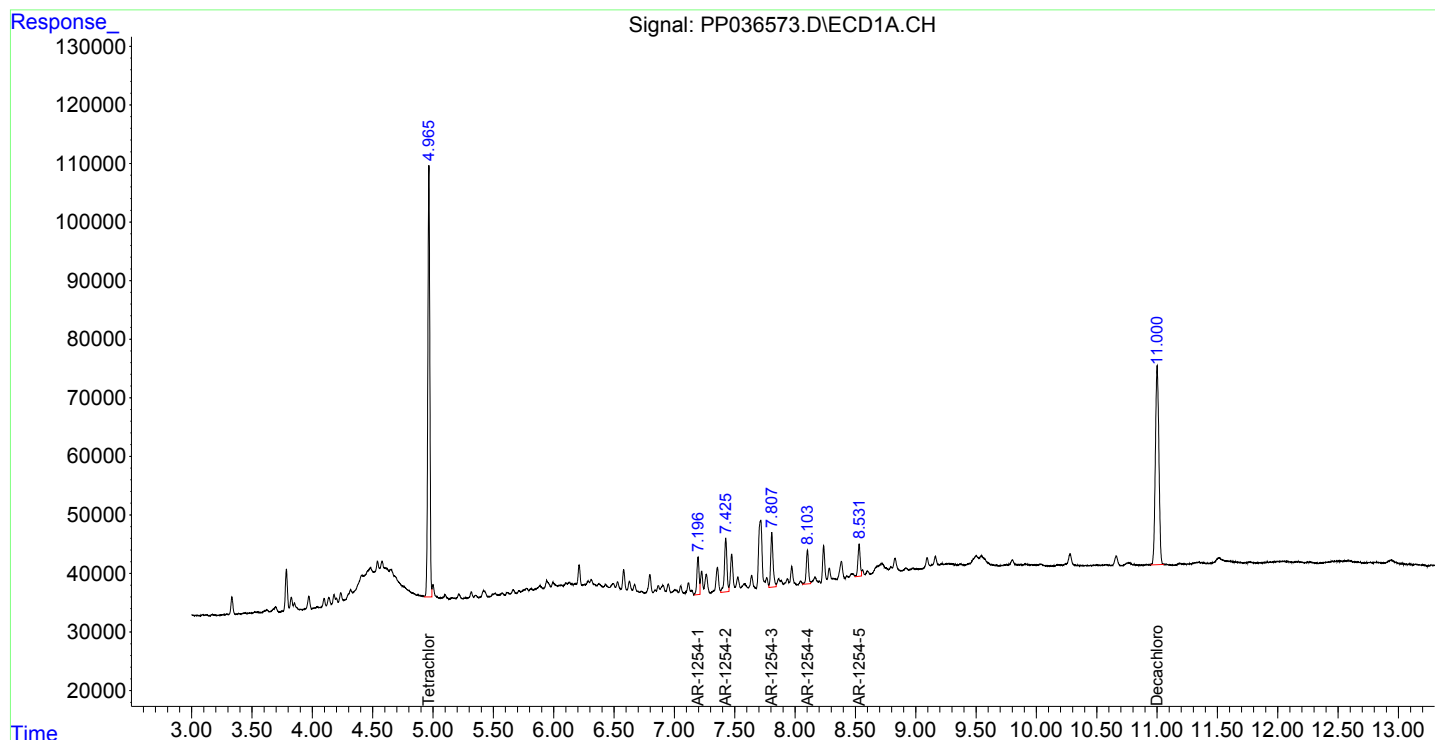

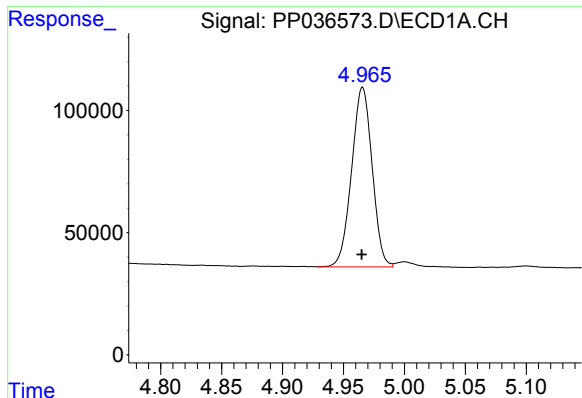


#1 Tetrachloro-m-xylene

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 862479
Conc: 19.51 ng/ml m

Instrument :
ECD_P
ClientSampleId :
0240-AMND-COMP-E


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:59 PM

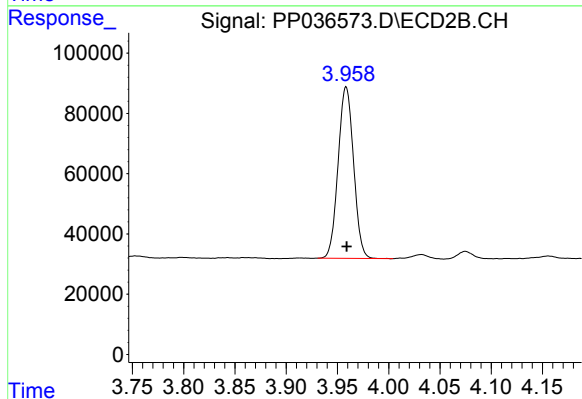


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 596186
Conc: 19.25 ng/ml

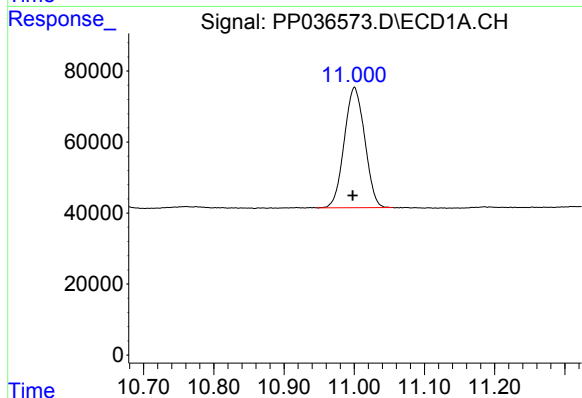


#2 Decachlorobiphenyl

R.T.: 11.000 min
Delta R.T.: 0.002 min
Response: 687715
Conc: 16.03 ng/ml

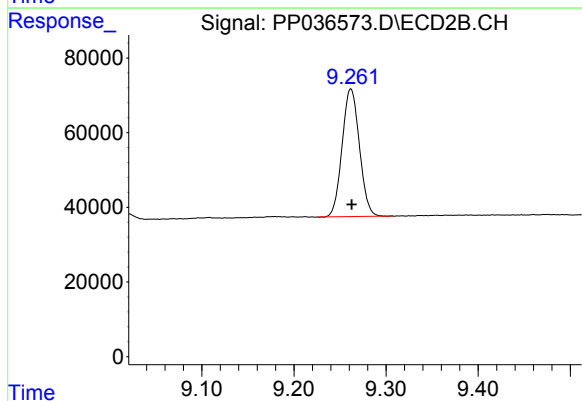

#2 Decachlorobiphenyl

R.T.: 9.262 min
Delta R.T.: -0.001 min
Response: 446410
Conc: 13.96 ng/ml

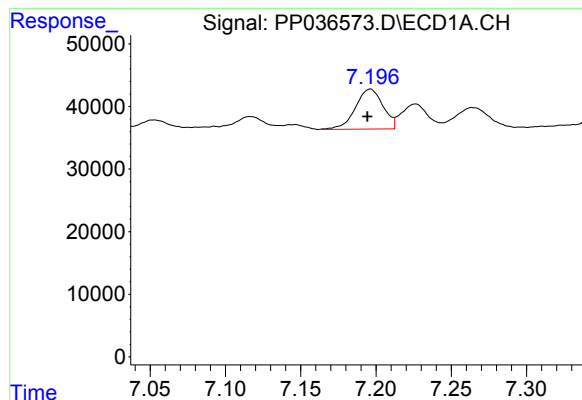


#26 AR-1254-1

R.T.: 7.196 min
Delta R.T.: 0.002 min
Response: 81809
Conc: 46.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
0240-AMND-COMP-E


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:59 PM

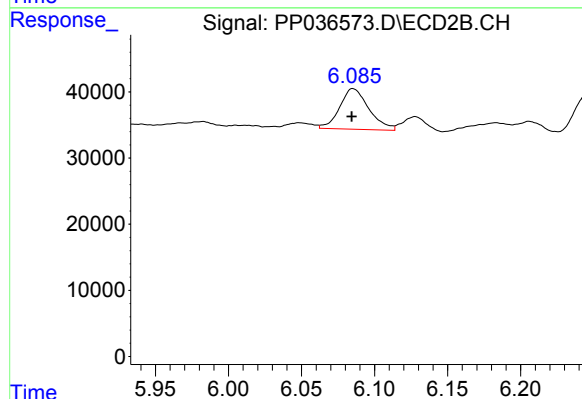


#26 AR-1254-1

R.T.: 6.085 min
Delta R.T.: 0.000 min
Response: 85719
Conc: 50.59 ng/ml

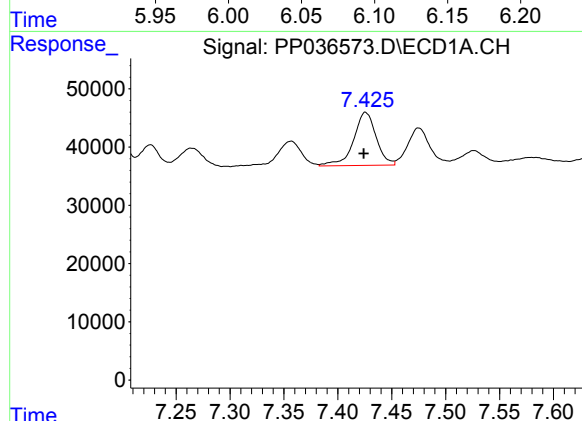


#27 AR-1254-2

R.T.: 7.426 min
Delta R.T.: 0.002 min
Response: 133110
Conc: 49.20 ng/ml

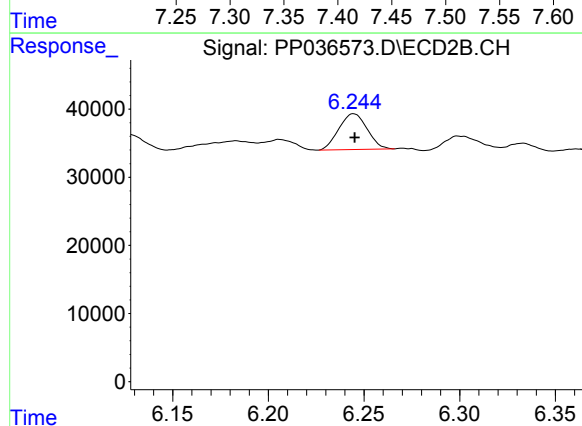

#27 AR-1254-2

R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 54111
Conc: 36.38 ng/ml

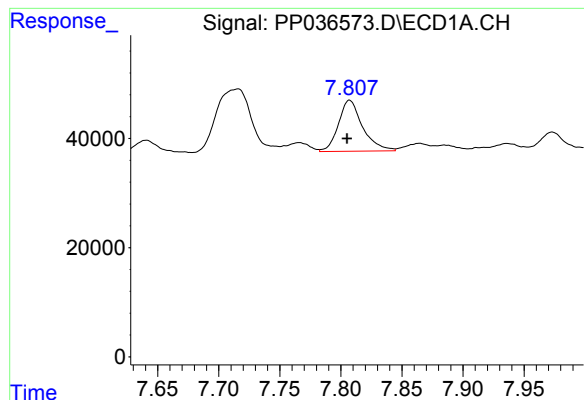


#28 AR-1254-3

R.T.: 7.807 min
Delta R.T.: 0.002 min
Response: 128839
Conc: 43.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
0240-AMND-COMP-E


Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:59 PM

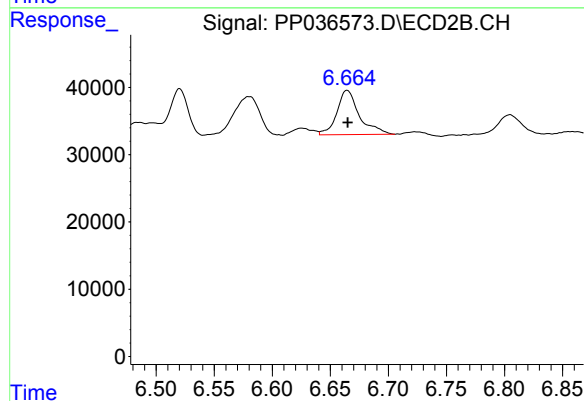


#28 AR-1254-3

R.T.: 6.664 min
Delta R.T.: 0.000 min
Response: 89030
Conc: 36.62 ng/ml

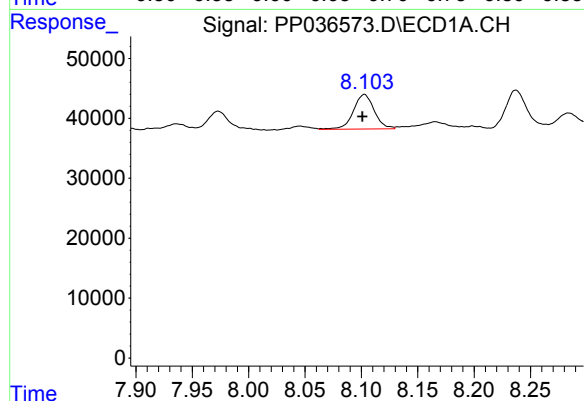


#29 AR-1254-4

R.T.: 8.103 min
Delta R.T.: 0.002 min
Response: 74919
Conc: 34.08 ng/ml

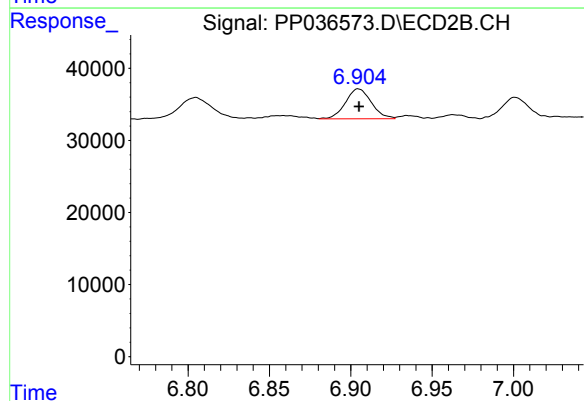


#29 AR-1254-4

R.T.: 6.905 min
Delta R.T.: 0.000 min
Response: 46139
Conc: 29.82 ng/ml

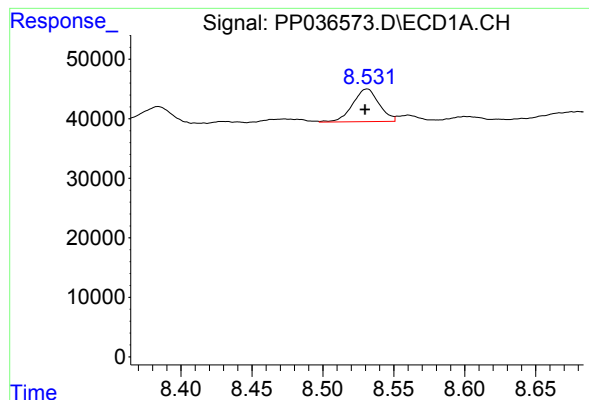

#30 AR-1254-5

R.T.: 8.531 min
Delta R.T.: 0.001 min
Response: 71513
Conc: 30.07 ng/ml

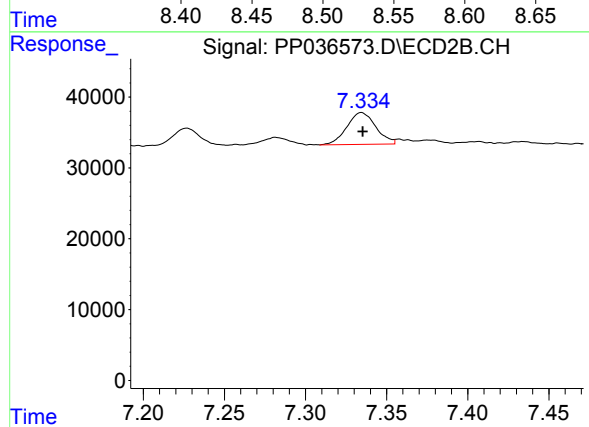

#30 AR-1254-5

R.T.: 7.334 min
Delta R.T.: -0.001 min
Response: 56108
Conc: 26.09 ng/ml m

Instrument :
ECD_P
ClientSampleId :
0240-AMND-COMP-E

Manual Integrations
APPROVED

Ankita
6/21/2021 2:24:59 PM