

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036575.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2021 20:29
 Operator : DD\AJ
 Sample : M2709-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:05:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.959	976005	685357	22.082	22.127
2)	SA Decachlor...	10.999	9.264	955925	638742	22.284	19.973
Target Compounds							
26)	L6 AR-1254-1	7.194	6.085	32886	25051	18.699	14.785
27)	L6 AR-1254-2	7.426	6.245	60138	20914	22.226	14.061 #
28)	L6 AR-1254-3	7.809	6.665	66194	27586	22.347	11.347 #
29)	L6 AR-1254-4	8.101	6.905	30841	16570	14.029m	10.708
30)	L6 AR-1254-5	8.531	7.335	48813	36297	20.526	16.880

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 Client Sample ID :
 0248-AMND-COMP-M

Manual Integrations
 APPROVED

Ankita
 6/21/2021 2:25:02 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036575.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2021 20:29
Operator : DD\AJ
Sample : M2709-09
Misc :
ALS Vial : 25 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:05:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampleId :
0248-AMND-COMP-M

Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:02 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

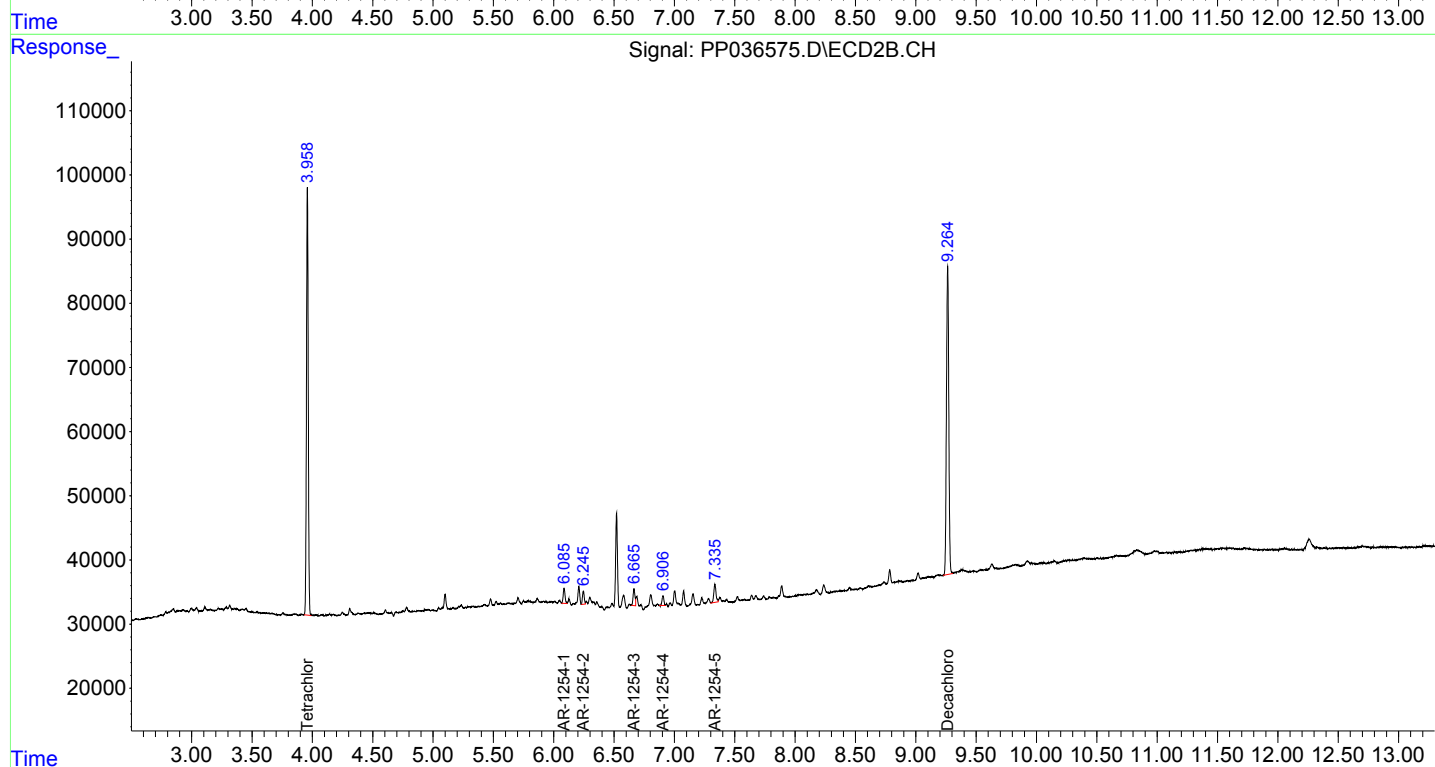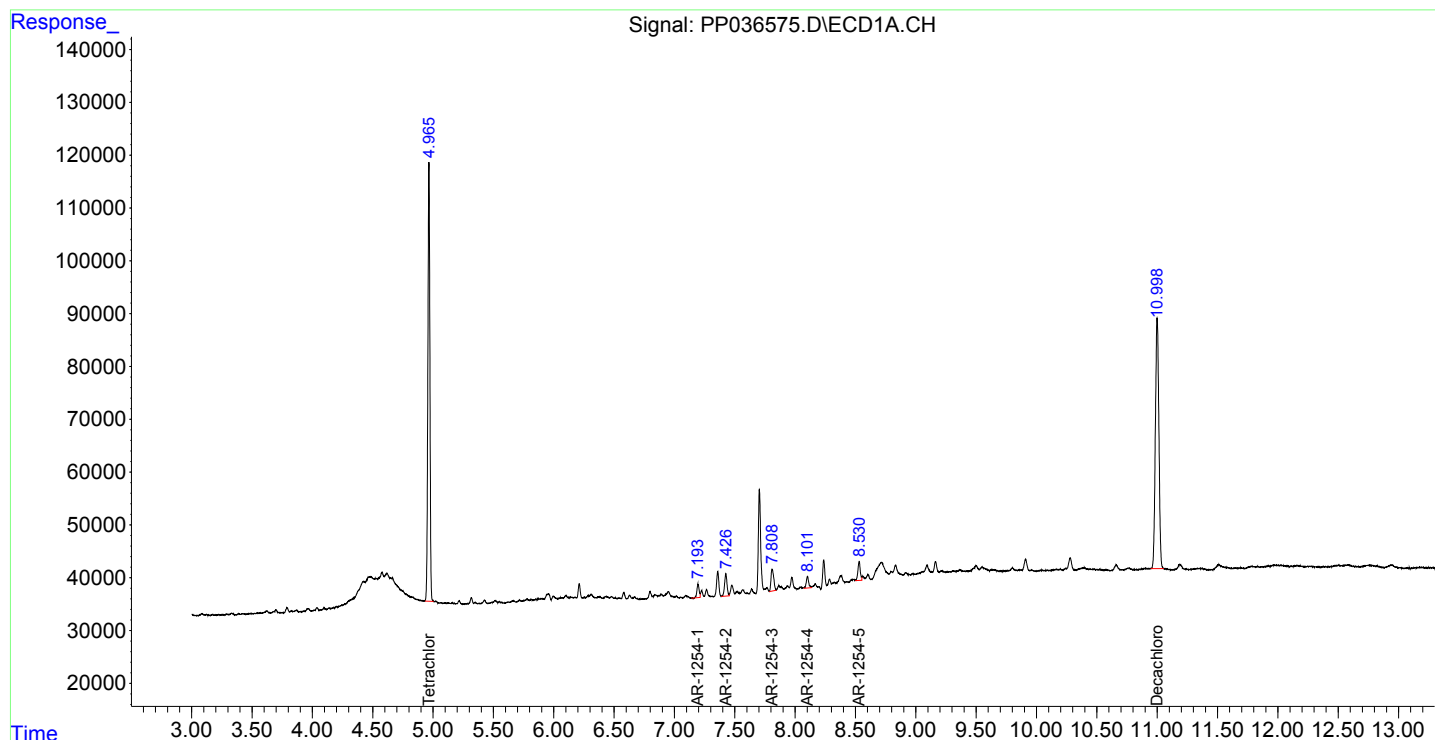

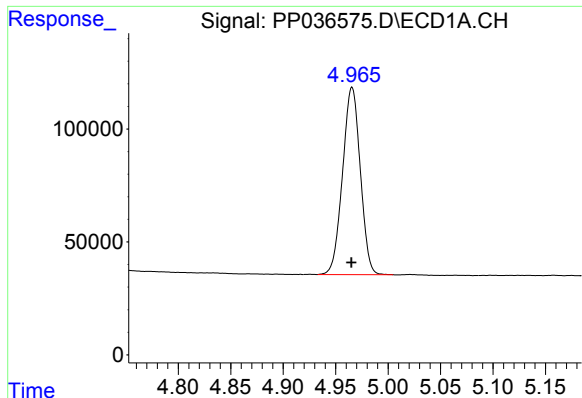


#1 Tetrachloro-m-xylene

R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 976005
Conc: 22.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
0248-AMND-COMP-M


Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:02 PM

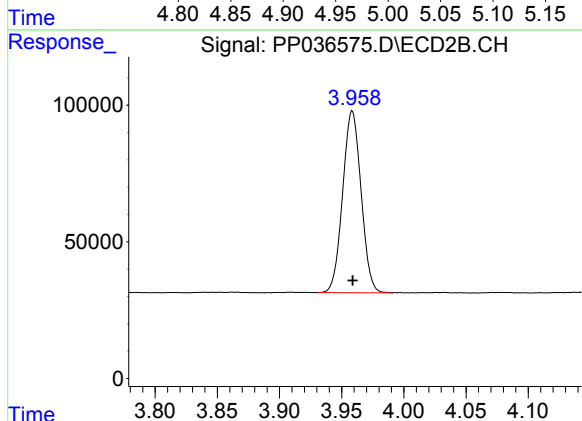


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 685357
Conc: 22.13 ng/ml

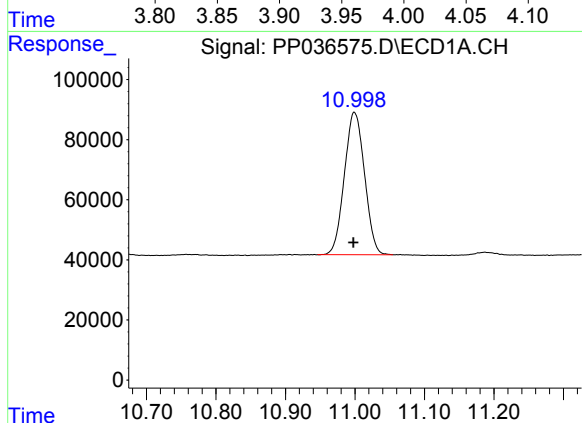


#2 Decachlorobiphenyl

R.T.: 10.999 min
Delta R.T.: 0.001 min
Response: 955925
Conc: 22.28 ng/ml

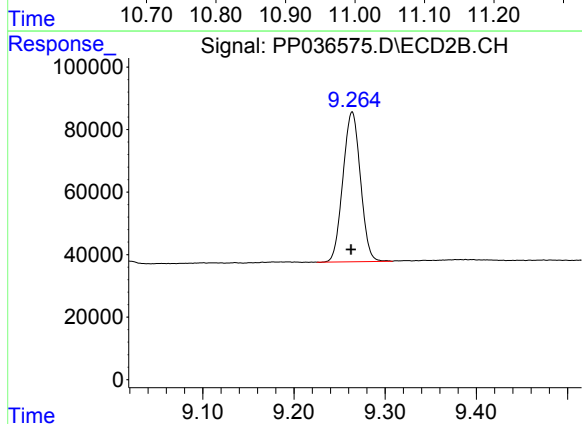

#2 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: 0.001 min
Response: 638742
Conc: 19.97 ng/ml

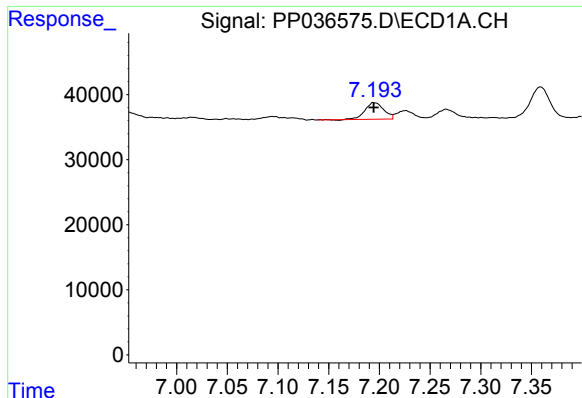


#26 AR-1254-1

R.T.: 7.194 min
Delta R.T.: 0.000 min
Response: 32886
Conc: 18.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
0248-AMND-COMP-M


Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:02 PM

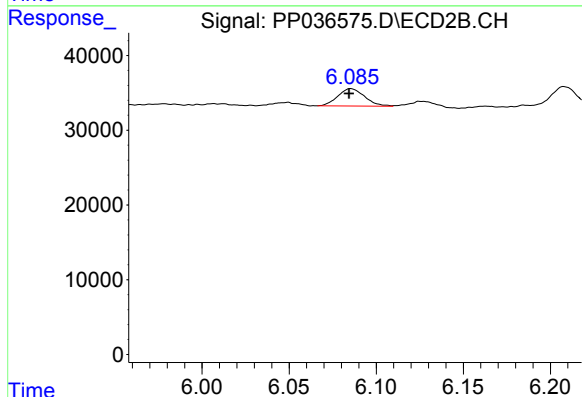


#26 AR-1254-1

R.T.: 6.085 min
Delta R.T.: 0.001 min
Response: 25051
Conc: 14.78 ng/ml

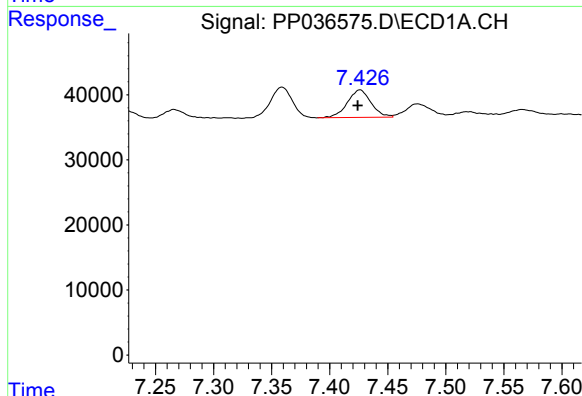


#27 AR-1254-2

R.T.: 7.426 min
Delta R.T.: 0.002 min
Response: 60138
Conc: 22.23 ng/ml

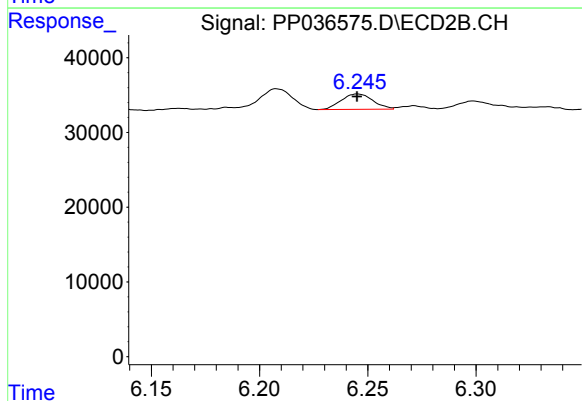

#27 AR-1254-2

R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 20914
Conc: 14.06 ng/ml

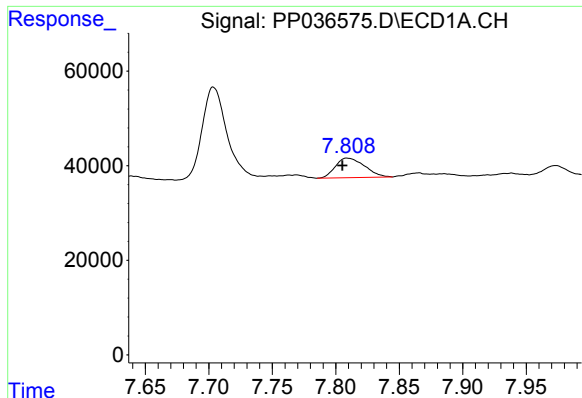


#28 AR-1254-3

R.T.: 7.809 min
Delta R.T.: 0.004 min
Response: 66194
Conc: 22.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
0248-AMND-COMP-M


Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:02 PM

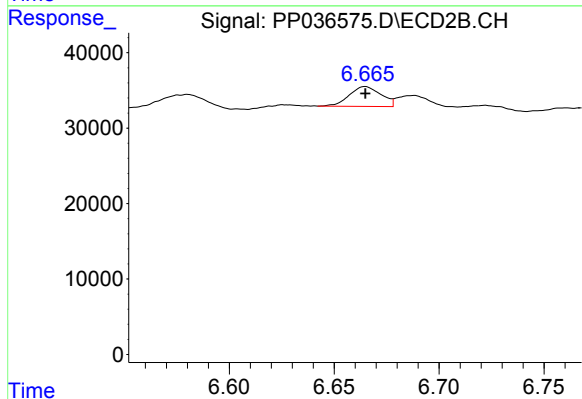


#28 AR-1254-3

R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 27586
Conc: 11.35 ng/ml

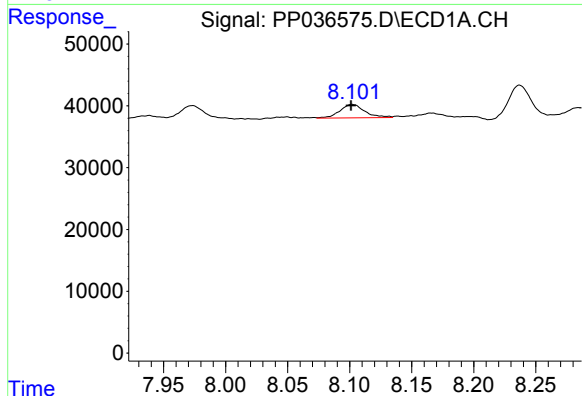


#29 AR-1254-4

R.T.: 8.101 min
Delta R.T.: 0.000 min
Response: 30841
Conc: 14.03 ng/ml m

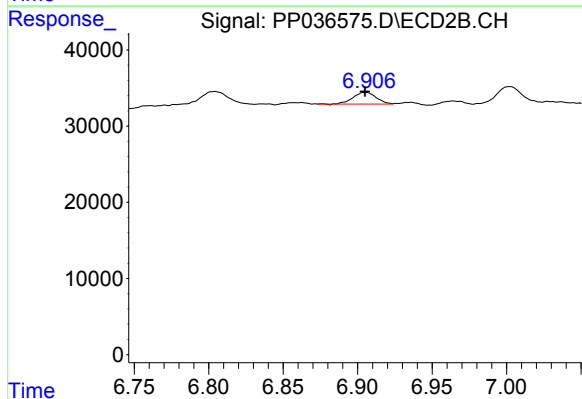

#29 AR-1254-4


R.T.: 6.905 min
Delta R.T.: 0.000 min
Response: 16570
Conc: 10.71 ng/ml

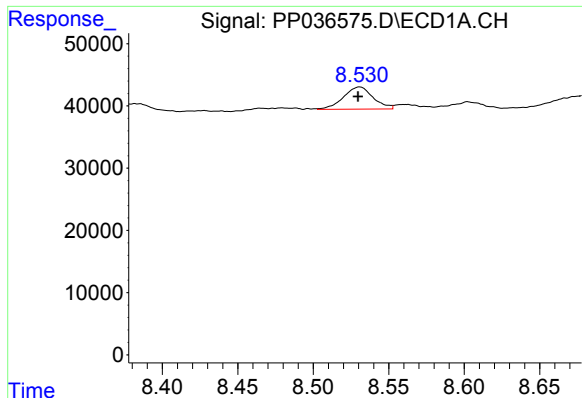

#30 AR-1254-5

R.T.: 8.531 min
Delta R.T.: 0.001 min
Response: 48813
Conc: 20.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
0248-AMND-COMP-M

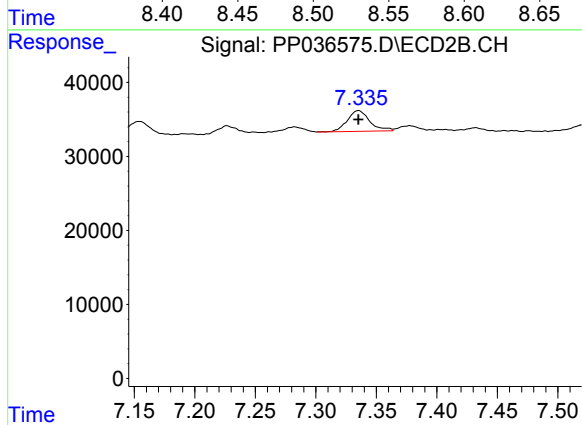

#30 AR-1254-5

R.T.: 7.335 min
Delta R.T.: 0.000 min
Response: 36297
Conc: 16.88 ng/ml

Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:02 PM