

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036593.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2021 2:05
 Operator : DD\AJ
 Sample : M2716-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:15:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.957	725781	476008	16.421m	15.368
2) SA Decachlor...	10.999	9.261	544532	363273	12.694	11.359

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 ClientSampleId :
 33220

Manual Integrations
 APPROVED

Ankita
 6/21/2021 2:25:09 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036593.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2021 2:05
Operator : DD\AJ
Sample : M2716-05
Misc :
ALS Vial : 36 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:15:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampleId :
33220

Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:09 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

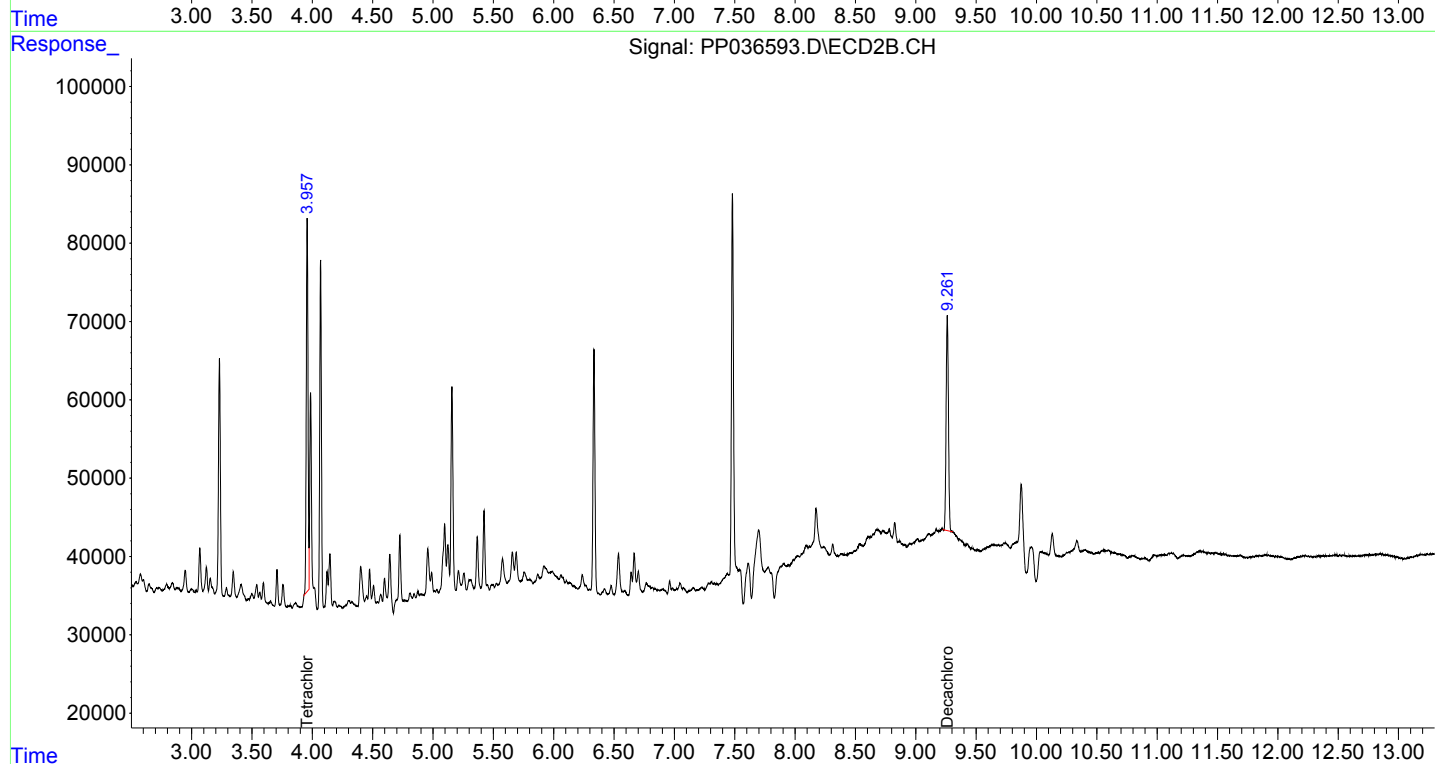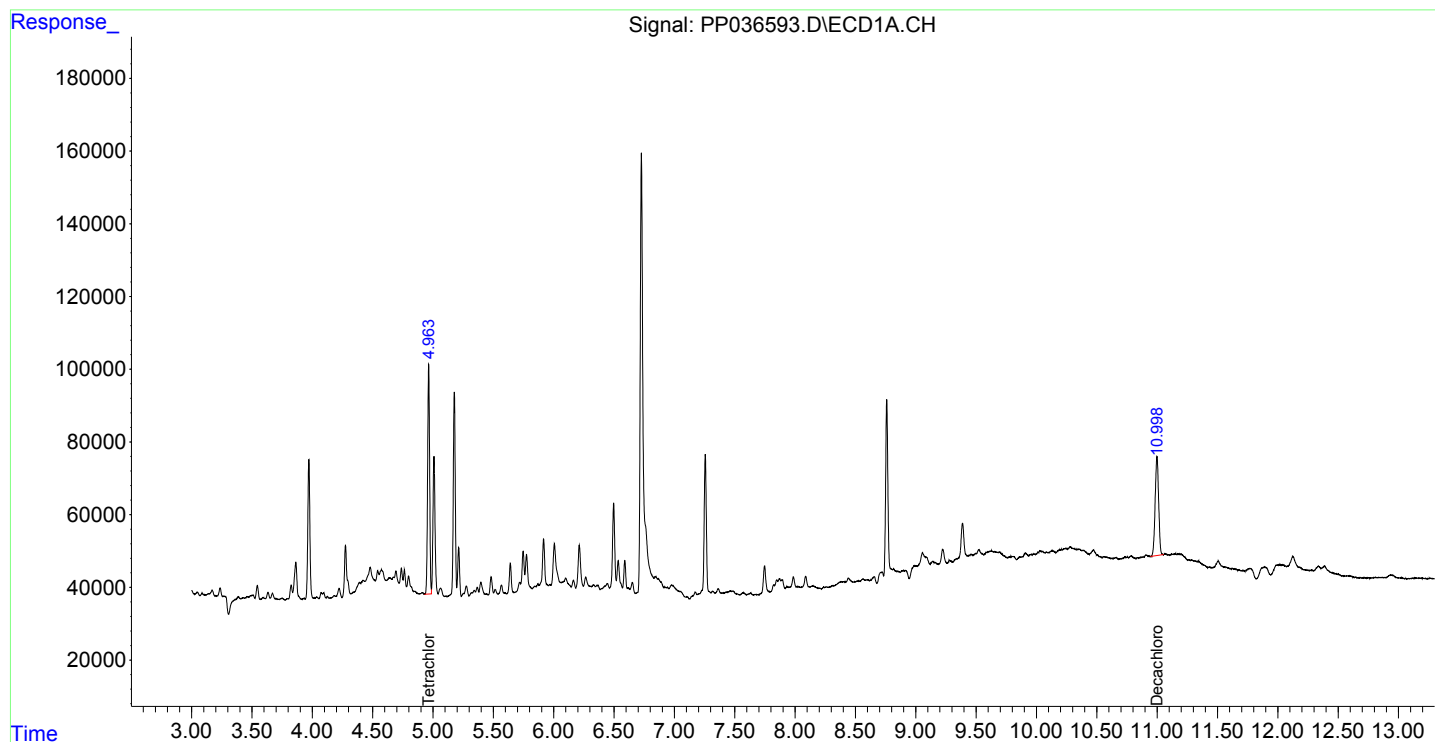

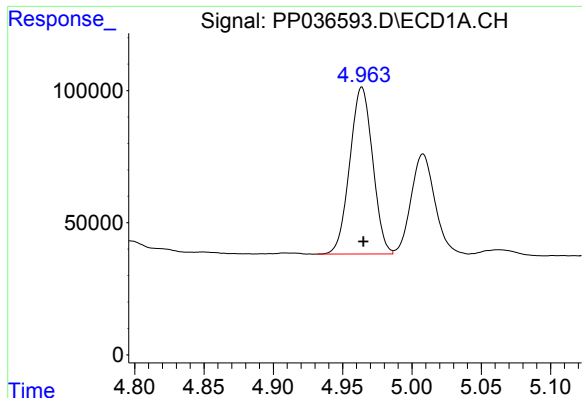

#1 Tetrachloro-m-xylene

R.T.: 4.963 min

Delta R.T.: -0.002 min

Response: 725781

Conc: 16.42 ng/ml m

Instrument :
ECD_P
ClientSampleId :
33220

Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:09 PM

#1 Tetrachloro-m-xylene

R.T.: 3.957 min

Delta R.T.: -0.002 min

Response: 476008

Conc: 15.37 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.999 min

Delta R.T.: 0.000 min

Response: 544532

Conc: 12.69 ng/ml

#2 Decachlorobiphenyl

R.T.: 9.261 min

Delta R.T.: -0.002 min

Response: 363273

Conc: 11.36 ng/ml