

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036597.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2021 3:46
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 05:04:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.965	3.957	2234055	1619440	50.546	52.285
2) SA Decachlor...	10.999	9.261	2078536	1470225	48.454	45.972
Target Compounds						
26) L6 AR-1254-1	7.194	6.083	865342	832733	492.045	491.472m
27) L6 AR-1254-2	7.424	6.243	1263786	724953	467.080	487.395m
28) L6 AR-1254-3	7.806	6.663	1353993	1201925	457.114	494.382
29) L6 AR-1254-4	8.102	6.904	1016779	744516	462.519	481.117
30) L6 AR-1254-5	8.530	7.334	1118873	1031343	470.482	479.631

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 Client Sample Id :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 6/21/2021 2:25:11 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036597.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2021 3:46
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 05:04:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:11 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

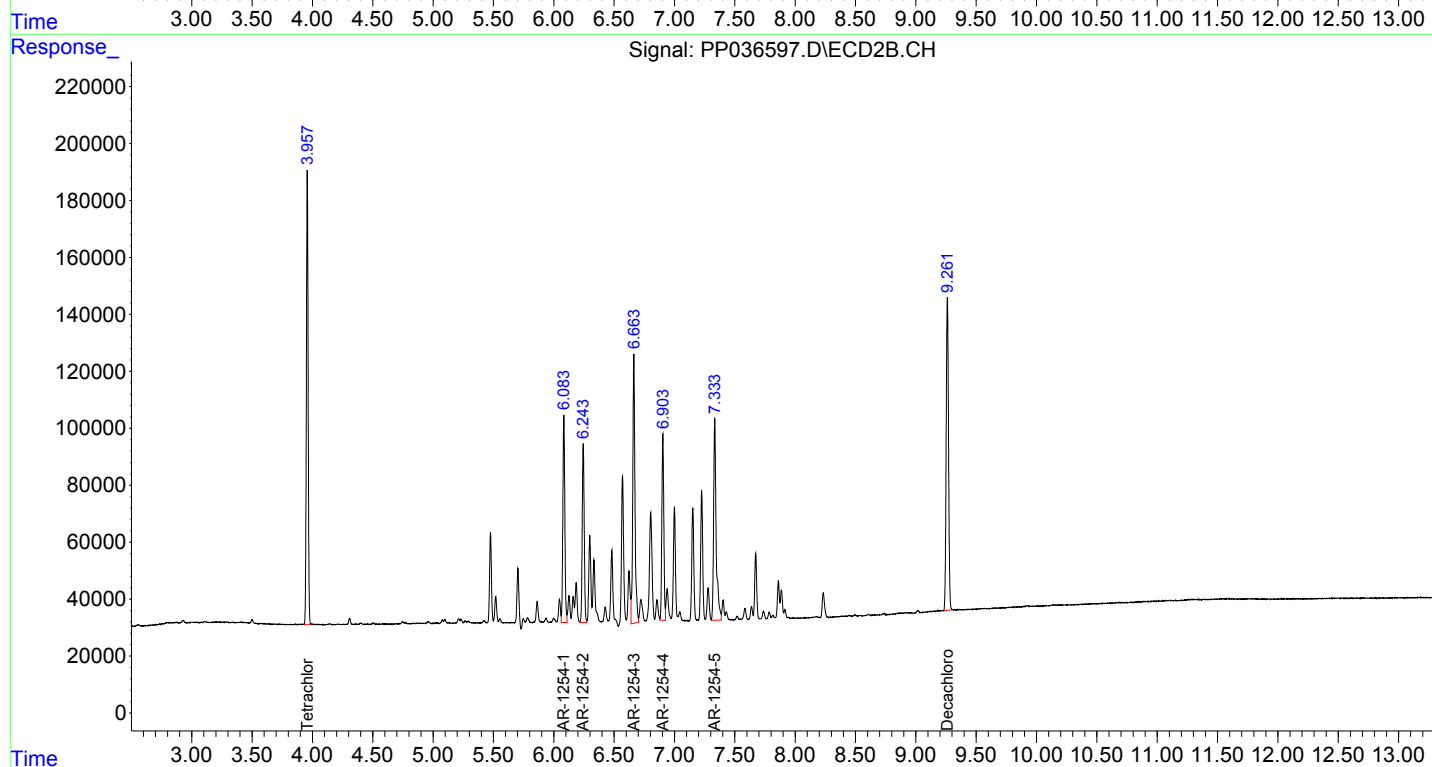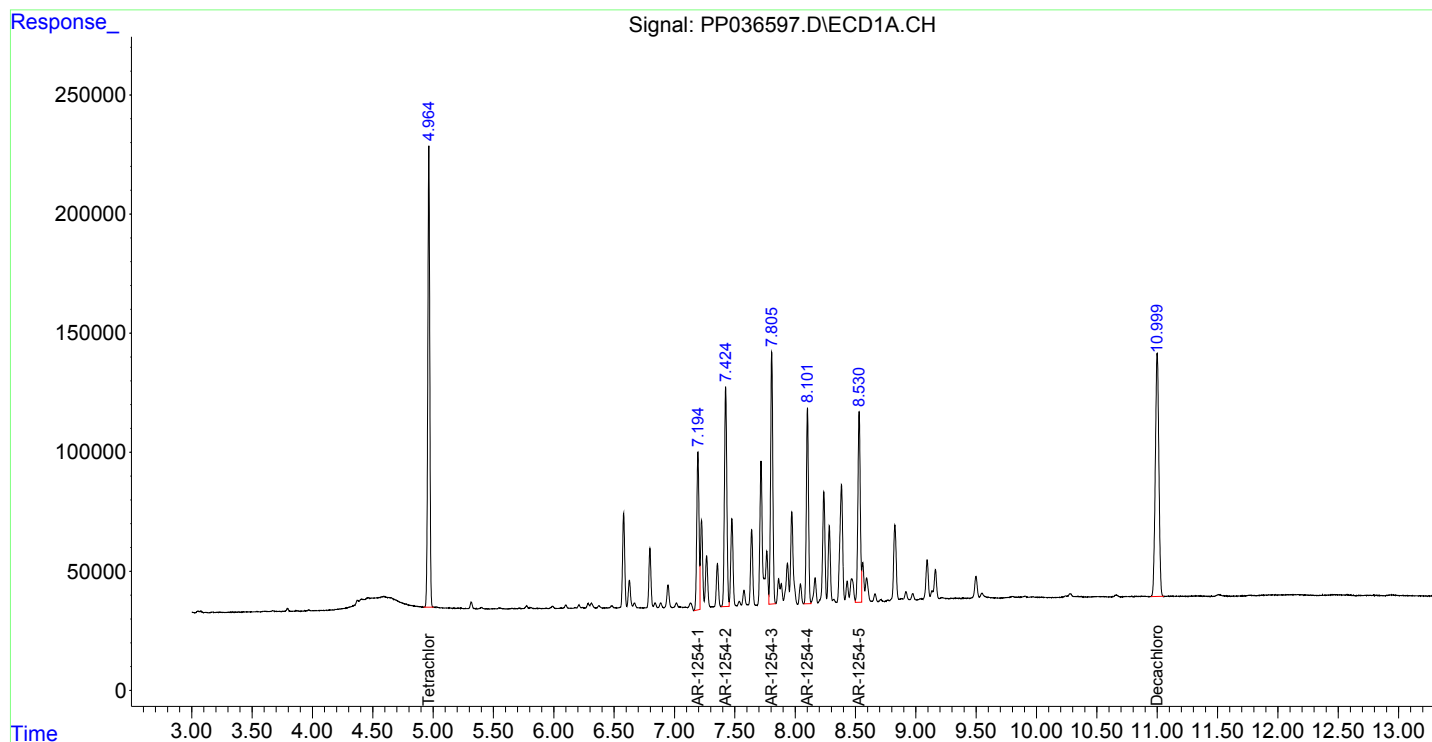

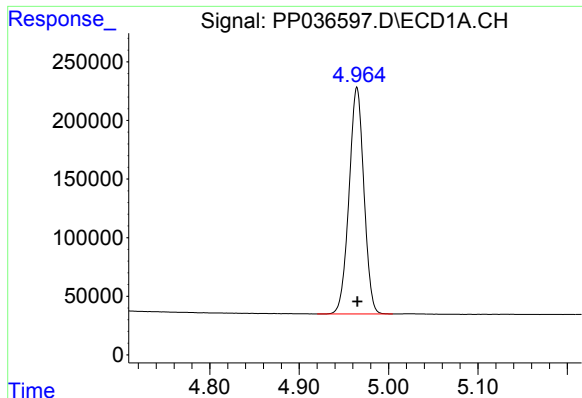


#1 Tetrachloro-m-xylene

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 2234055
Conc: 50.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:11 PM

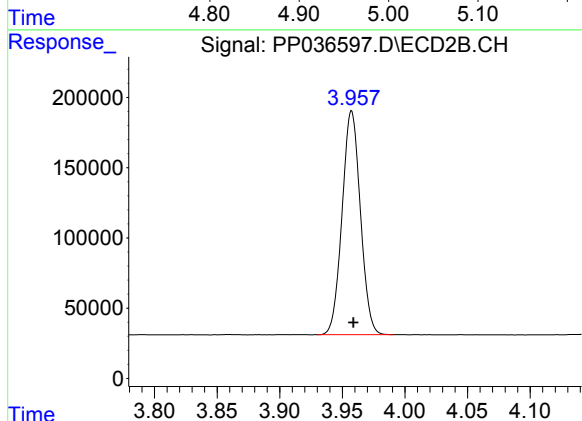


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.001 min
Response: 1619440
Conc: 52.29 ng/ml

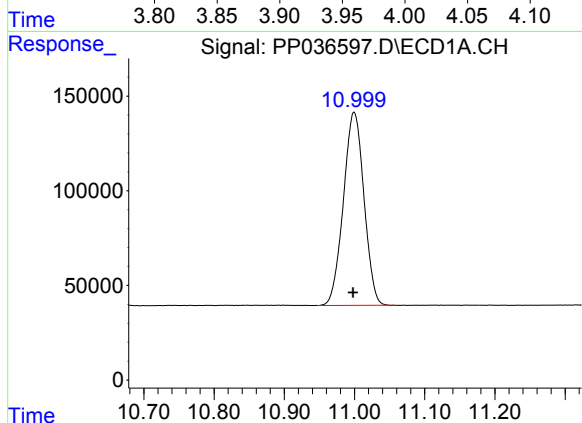


#2 Decachlorobiphenyl

R.T.: 10.999 min
Delta R.T.: 0.001 min
Response: 2078536
Conc: 48.45 ng/ml

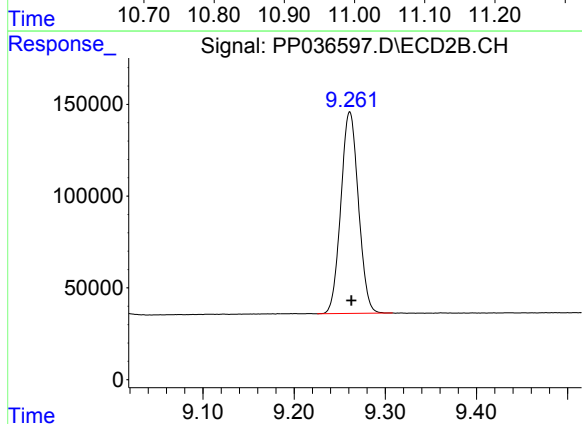

#2 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: -0.002 min
Response: 1470225
Conc: 45.97 ng/ml

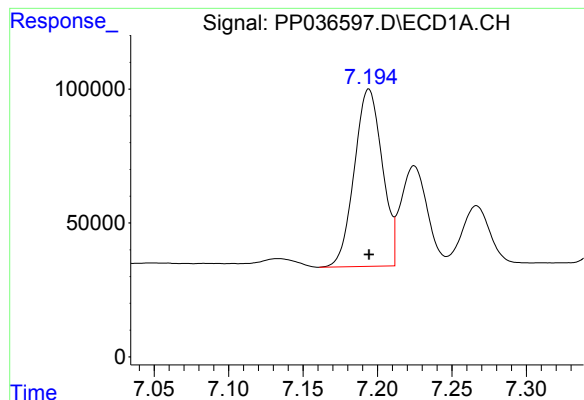


#26 AR-1254-1

R.T.: 7.194 min
Delta R.T.: 0.000 min
Response: 865342
Conc: 492.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:11 PM

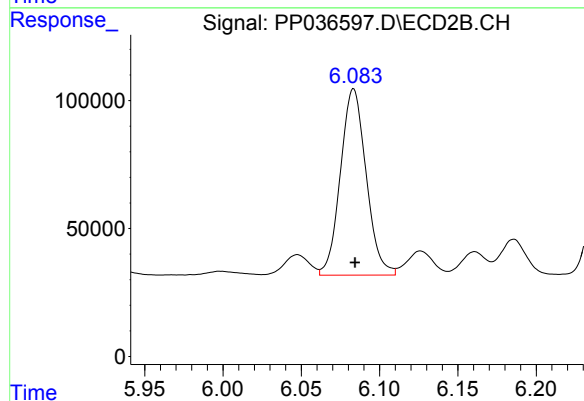


#26 AR-1254-1

R.T.: 6.083 min
Delta R.T.: -0.001 min
Response: 832733
Conc: 491.47 ng/ml m

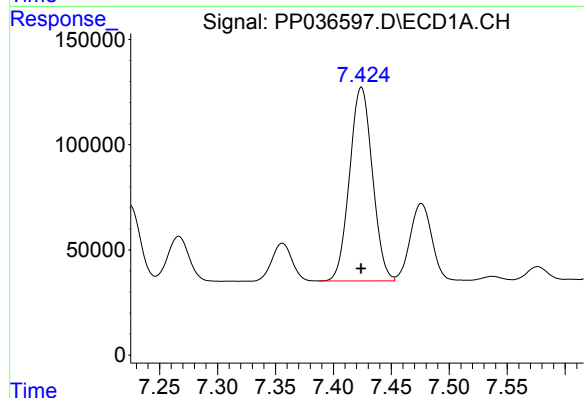


#27 AR-1254-2

R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 1263786
Conc: 467.08 ng/ml

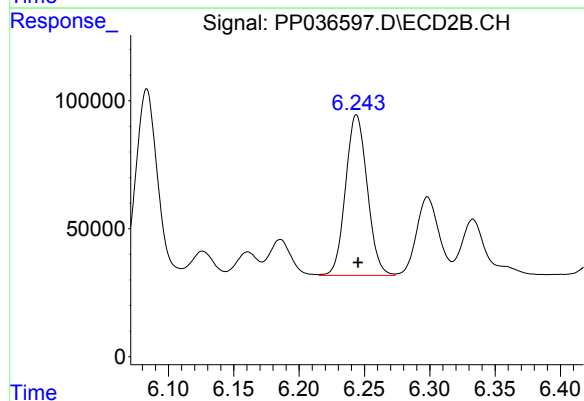

#27 AR-1254-2

R.T.: 6.243 min
Delta R.T.: -0.002 min
Response: 724953
Conc: 487.40 ng/ml m

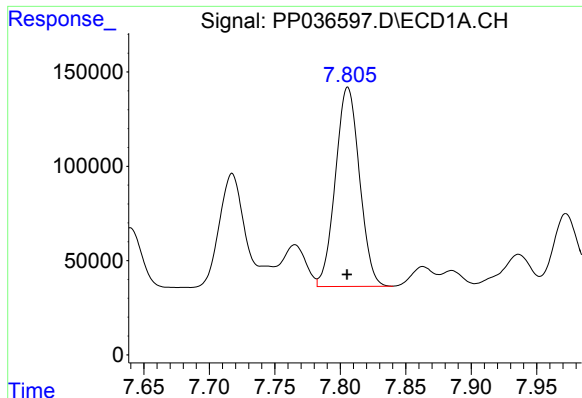


#28 AR-1254-3

R.T.: 7.806 min
Delta R.T.: 0.000 min
Response: 1353993
Conc: 457.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:11 PM

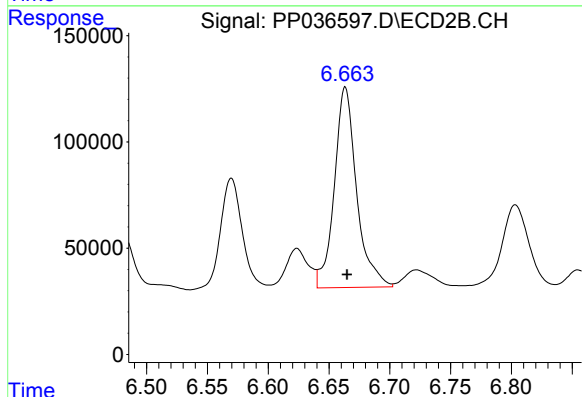


#28 AR-1254-3

R.T.: 6.663 min
Delta R.T.: -0.001 min
Response: 1201925
Conc: 494.38 ng/ml

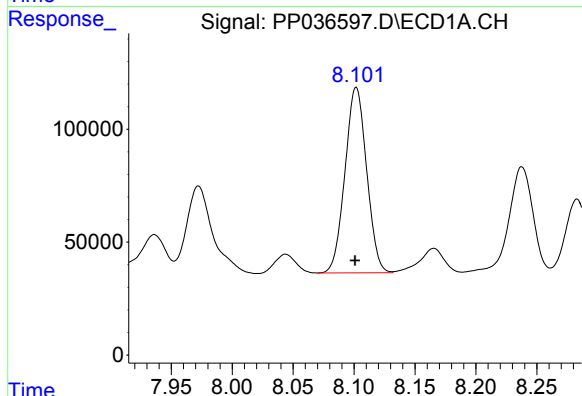


#29 AR-1254-4

R.T.: 8.102 min
Delta R.T.: 0.000 min
Response: 1016779
Conc: 462.52 ng/ml

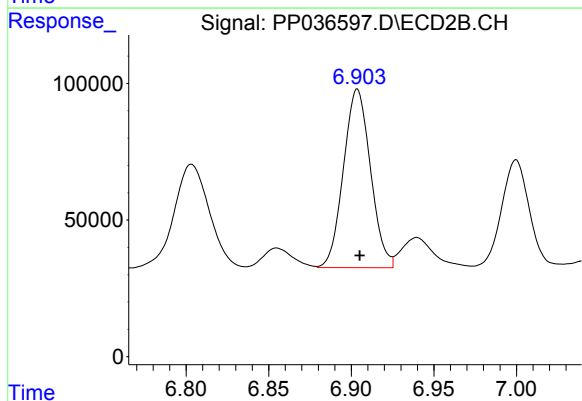

#29 AR-1254-4


R.T.: 6.904 min
Delta R.T.: -0.001 min
Response: 744516
Conc: 481.12 ng/ml

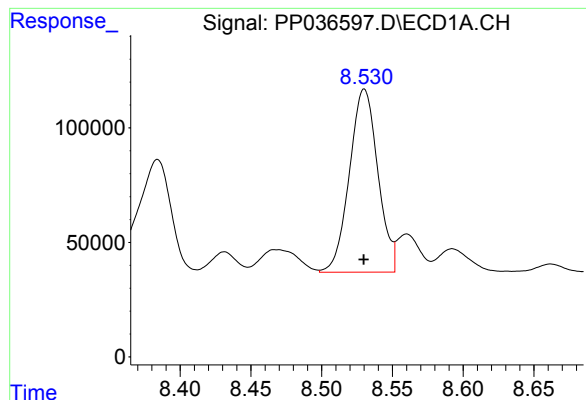

#30 AR-1254-5

R.T.: 8.530 min
Delta R.T.: 0.000 min
Response: 1118873
Conc: 470.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

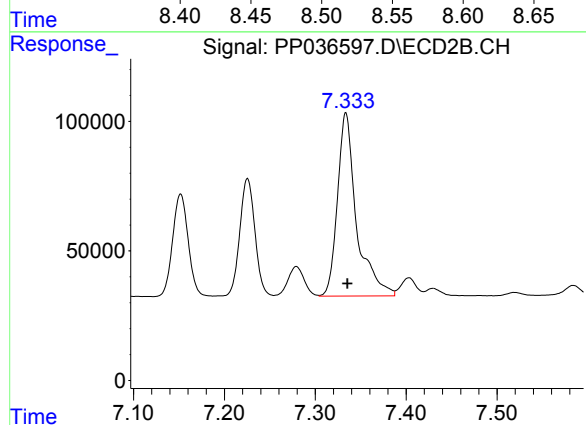

#30 AR-1254-5

R.T.: 7.334 min
Delta R.T.: -0.002 min
Response: 1031343
Conc: 479.63 ng/ml

Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:11 PM