

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
 Data File : PP036613.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2021 8:47
 Operator : DD\AJ
 Sample : M2755-02 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:23:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 18 06:06:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.967	3.960	58914	39403	1.333	1.272m
2) SA Decachlor...	11.002	9.262	82265	43229	1.918	1.352m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_P
 ClientSampleId :
 HEE262Y-N-2

Manual Integrations
 APPROVED

Ankita
 6/21/2021 2:25:23 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061821\
Data File : PP036613.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2021 8:47
Operator : DD\AJ
Sample : M2755-02 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:23:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061721.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 18 06:06:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_P
ClientSampled :
HEE262Y-N-2

Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:23 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

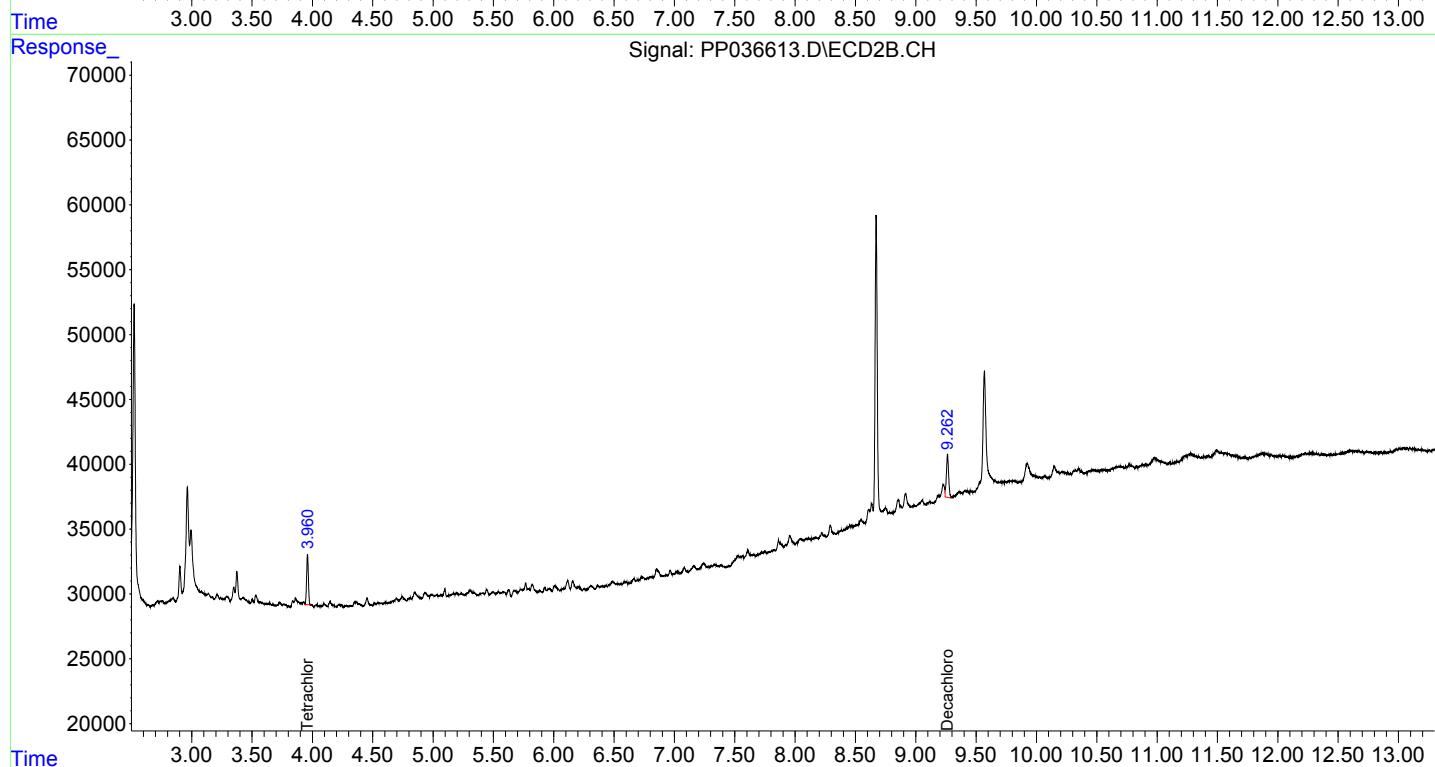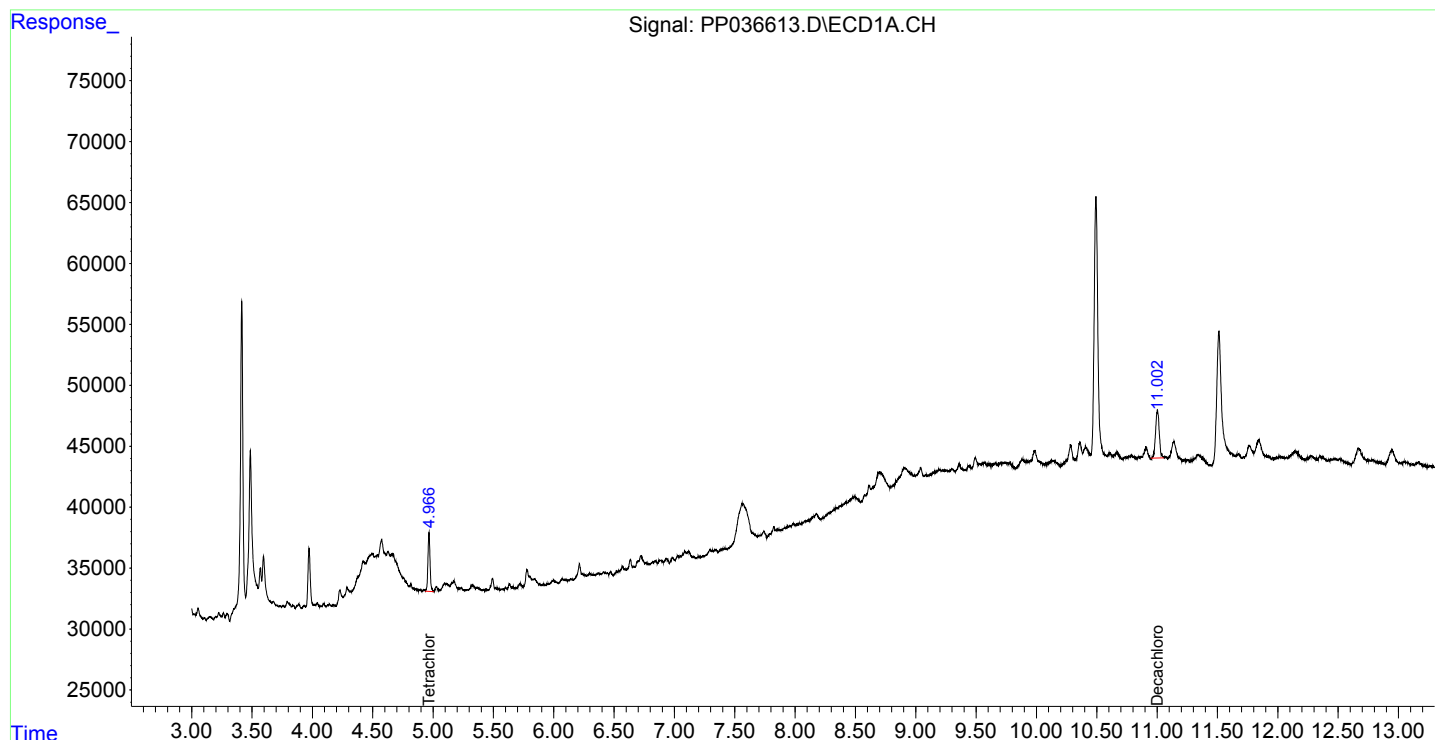

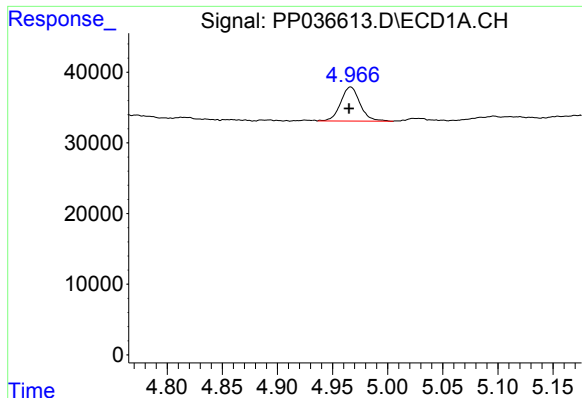


#1 Tetrachloro-m-xylene

R.T.: 4.967 min
Delta R.T.: 0.002 min
Response: 58914
Conc: 1.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE262Y-N-2


Manual Integrations
APPROVED

Ankita
6/21/2021 2:25:23 PM

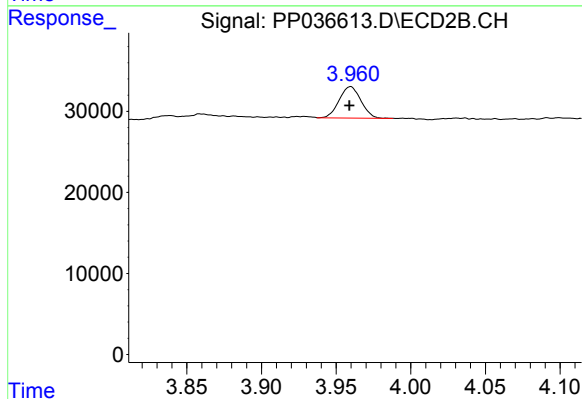


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 39403
Conc: 1.27 ng/ml m

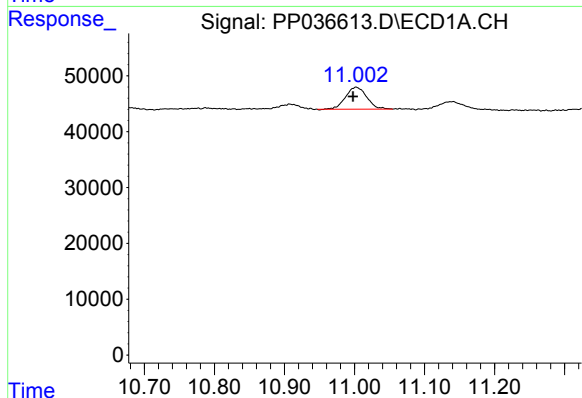

#2 Decachlorobiphenyl

R.T.: 11.002 min
Delta R.T.: 0.005 min
Response: 82265
Conc: 1.92 ng/ml

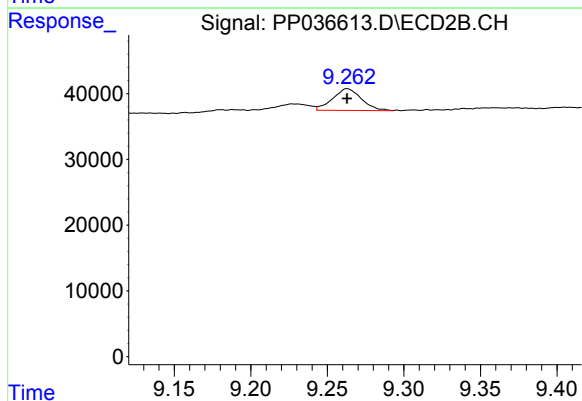

#2 Decachlorobiphenyl

R.T.: 9.262 min
Delta R.T.: 0.000 min
Response: 43229
Conc: 1.35 ng/ml m