

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
 Data File : PP073052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 20:03
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1232 LOD 25 PPB
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:39:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.491	3.788	39469971	32724540	18.699	18.162
2)	SA Decachlor...	10.186	8.797	36702180	27387219	21.477	20.519
Target Compounds							
3)	L1 AR-1016-1	5.640	4.869	2802598	871973	38.565	12.689 #
4)	L1 AR-1016-2	5.663	4.887	2193905	1217297	21.091	12.096 #
5)	L1 AR-1016-3	5.727	5.064	2345220	674648	35.888	12.330 #
6)	L1 AR-1016-4	5.825	5.103	881430	752159	16.860	16.884
7)	L1 AR-1016-5	6.112	5.317	405372	887346	8.107	16.051 #
8)	L2 AR-1221-1	4.688	3.999	610396	764538	24.753	28.451
9)	L2 AR-1221-2	4.790	4.087	953065	1417441	47.230	70.221 #
10)	L2 AR-1221-3	4.854	4.161	1129419	1487593	18.349	25.329 #
11)	L3 AR-1232-1	4.854	4.161	1129419	1487593	24.053	32.648 #
12)	L3 AR-1232-2	5.377	4.887	1061445	1217297	47.450	26.314 #
13)	L3 AR-1232-3	5.663	5.064	2193905	674648	42.520	27.472 #
14)	L3 AR-1232-4	5.825	5.146	881430	600710	34.150	27.778
15)	L3 AR-1232-5	5.912	5.317	740136	887346	20.749	38.818 #
16)	L4 AR-1242-1	5.640	4.869	2802598	871973	47.959	15.791 #
17)	L4 AR-1242-2	5.663	4.887	2193905	1217297	25.347	15.315 #
18)	L4 AR-1242-3	5.727	5.064	2345220	674648	44.495	15.579 #
19)	L4 AR-1242-4	5.825	5.146	881430	600710	20.052	14.474 #
20)	L4 AR-1242-5	6.557	5.671	2403851	738645	48.504	14.046 #
21)	L5 AR-1248-1	5.640	4.869	2802598	871973	58.917	20.004 #
22)	L5 AR-1248-2	5.912	5.103	740136	752159	12.641	12.836
23)	L5 AR-1248-3	6.112	5.146	405372	600710	6.213	9.922 #
24)	L5 AR-1248-4	6.514	5.317	1733838	887346	20.383	12.672 #
25)	L5 AR-1248-5	6.557	5.711	2403851	644842	28.722	9.078 #
26)	L6 AR-1254-1	6.486	5.671	1114884	738645	13.245	6.736 #
27)	L6 AR-1254-2	6.710	5.801	1376629	868941	10.978	9.191
28)	L6 AR-1254-3	7.067	6.224	1420706	315487	10.828	2.138 #
29)	L6 AR-1254-4	7.364	6.435	2442770	439042	20.393	4.521 #
30)	L6 AR-1254-5	7.771	6.864	88827	94293	0.777	0.726
31)	L7 AR-1260-1	7.234	6.340	569147	264326	6.452	2.790 #
32)	L7 AR-1260-2	7.505	6.533	1033862	1463060	7.608	12.565 #
33)	L7 AR-1260-3	7.875	6.698	962157	90083	8.429	0.865 #
34)	L7 AR-1260-4	8.090	7.157	469251	209604	4.554	2.389 #
35)	L7 AR-1260-5	8.416	7.405	702989	312873	2.922	1.466 #
36)	L8 AR-1262-1	8.090	6.906	469251	798677	3.170	5.528 #
37)	L8 AR-1262-2	8.416	7.157	702989	209604	2.221	1.715
38)	L8 AR-1262-3	8.719	7.679	823397	313546	3.848	2.782 #
39)	L8 AR-1262-4	8.804	7.750	775519	602732	4.921	3.287 #
40)	L8 AR-1262-5	9.434	0.000	288421	0	2.578	N.D. #
41)	L9 AR-1268-1	8.719	7.679	823397	313546	2.302	1.091 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
Data File : PP073052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 20:03
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:39:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.804	7.750	775519	602732	2.542	2.344
43) L9	AR-1268-3	9.023	7.953	2028644	590385	7.640	2.734 #
44) L9	AR-1268-4	9.434	0.000	288421	0	2.465	N.D. #
45) L9	AR-1268-5	9.871	8.540	269955	295776	0.365	0.511 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
Data File : PP073052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 20:03
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:39:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

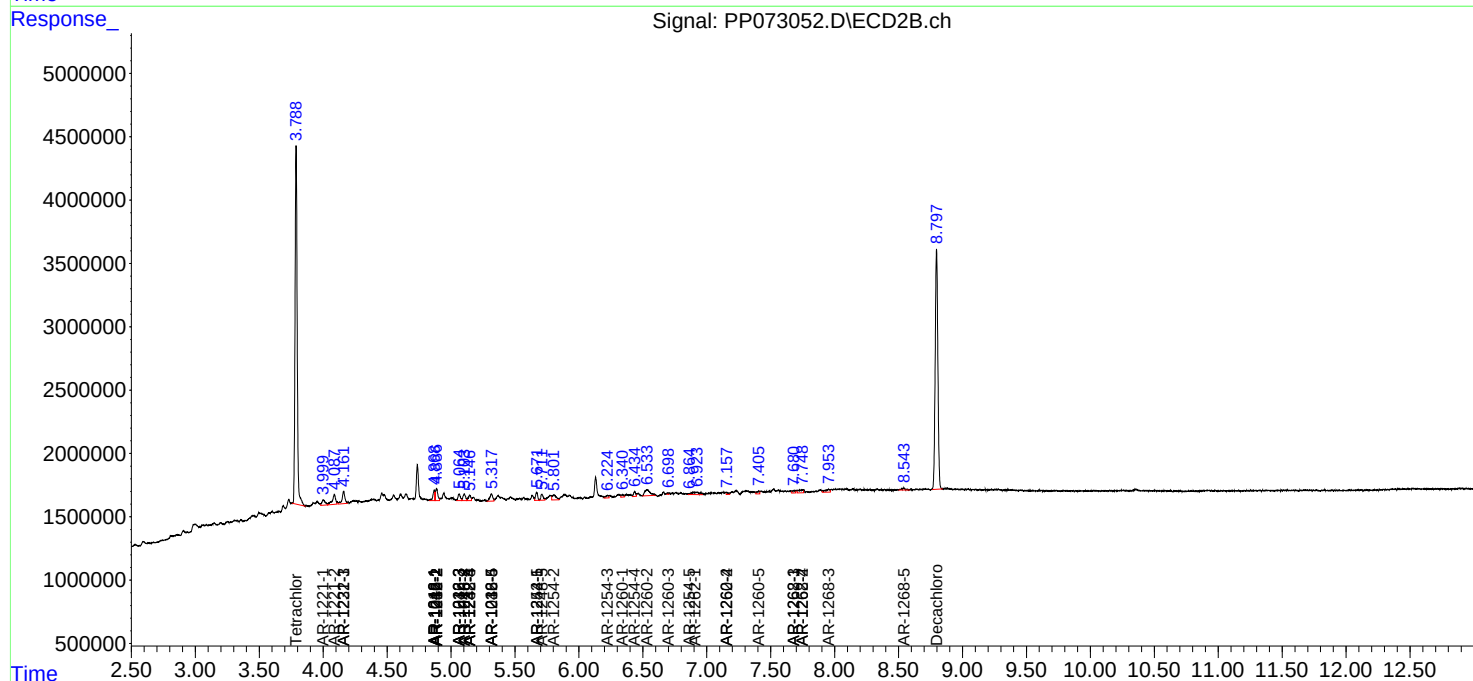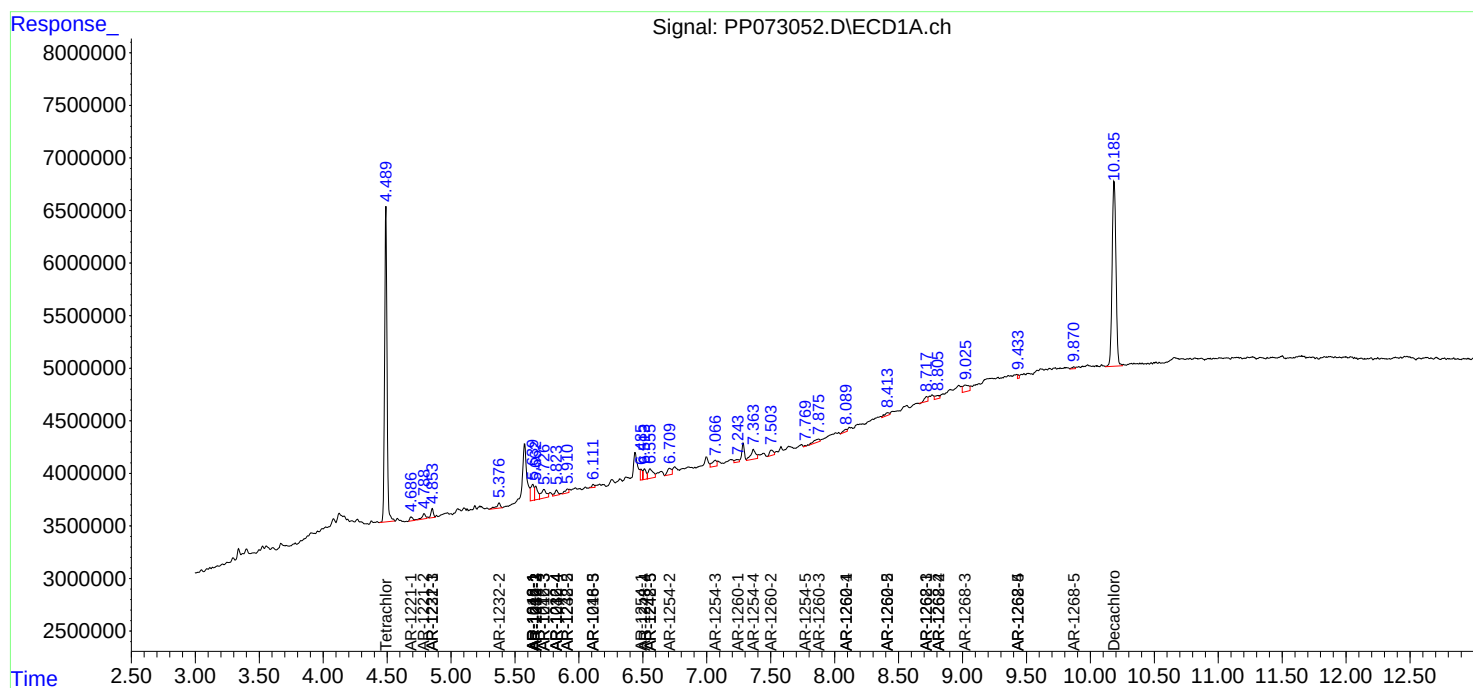


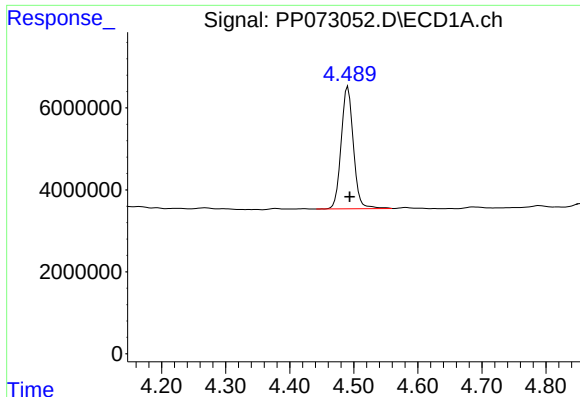

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: -0.003 min
Response: 39469971
Conc: 18.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

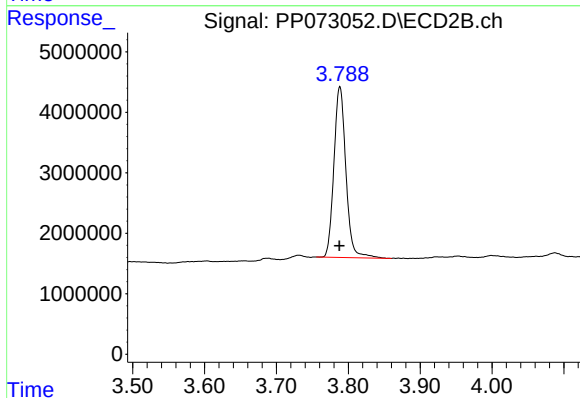


#1 Tetrachloro-m-xylene

R.T.: 3.788 min
Delta R.T.: 0.000 min
Response: 32724540
Conc: 18.16 ng/ml

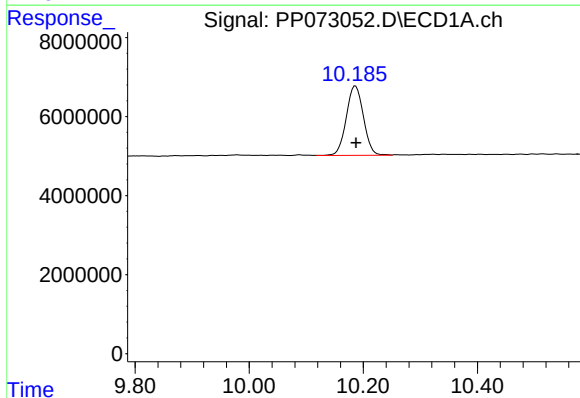


#2 Decachlorobiphenyl

R.T.: 10.186 min
Delta R.T.: 0.000 min
Response: 36702180
Conc: 21.48 ng/ml

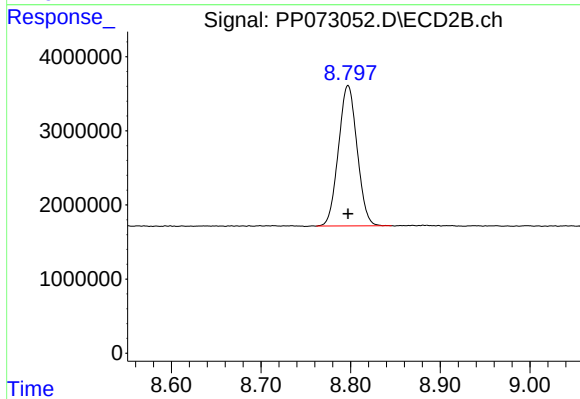

#2 Decachlorobiphenyl


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 27387219
Conc: 20.52 ng/ml

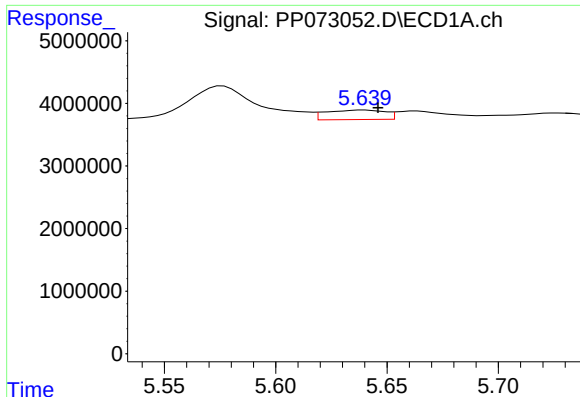

#3 AR-1016-1


R.T.: 5.640 min
Delta R.T.: -0.006 min
Response: 2802598
Conc: 38.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

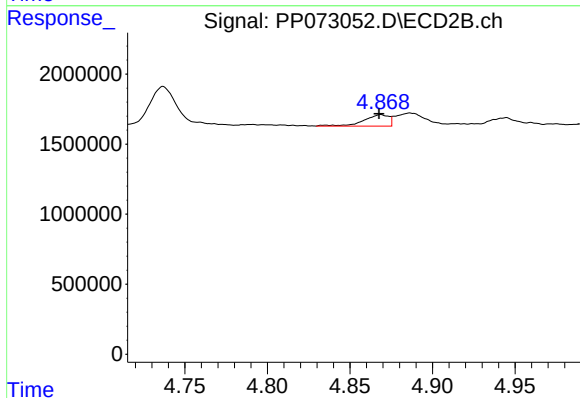


#3 AR-1016-1

R.T.: 4.869 min
Delta R.T.: 0.001 min
Response: 871973
Conc: 12.69 ng/ml

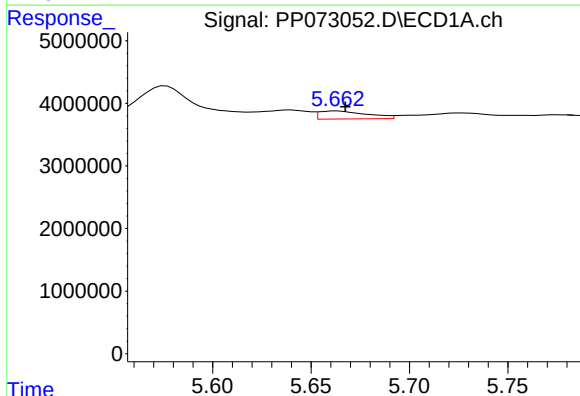


#4 AR-1016-2

R.T.: 5.663 min
Delta R.T.: -0.004 min
Response: 2193905
Conc: 21.09 ng/ml

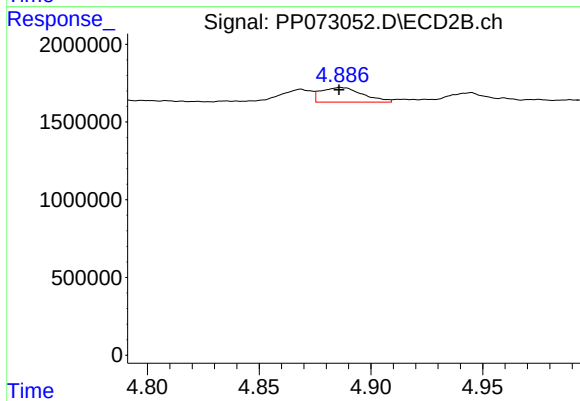

#4 AR-1016-2


R.T.: 4.887 min
Delta R.T.: 0.000 min
Response: 1217297
Conc: 12.10 ng/ml

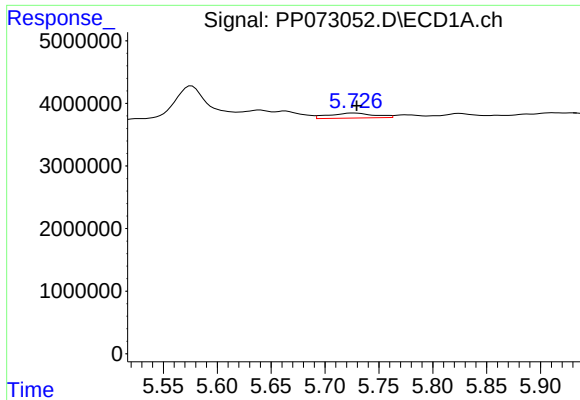

#5 AR-1016-3


R.T.: 5.727 min
Delta R.T.: -0.002 min
Response: 2345220
Conc: 35.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

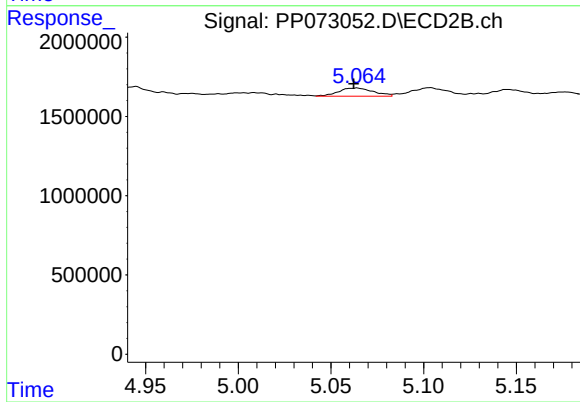


#5 AR-1016-3

R.T.: 5.064 min
Delta R.T.: 0.001 min
Response: 674648
Conc: 12.33 ng/ml

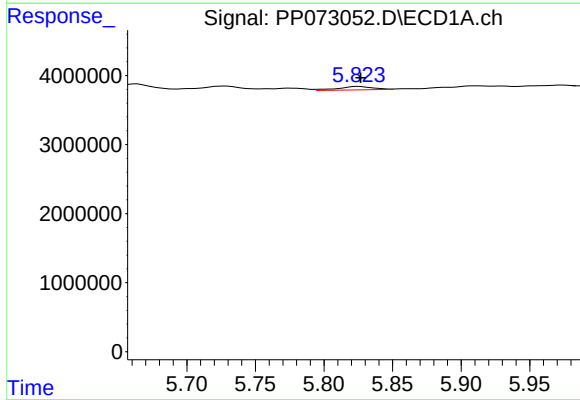


#6 AR-1016-4

R.T.: 5.825 min
Delta R.T.: -0.002 min
Response: 881430
Conc: 16.86 ng/ml

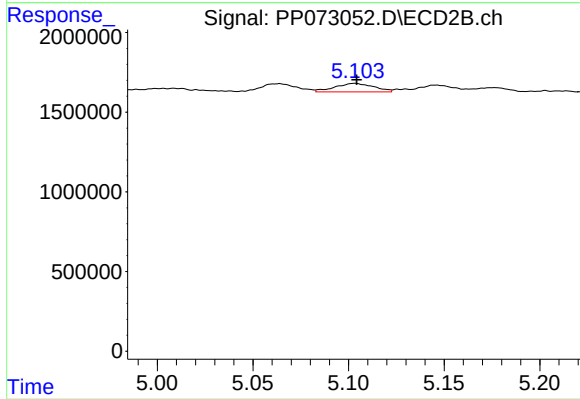

#6 AR-1016-4


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 752159
Conc: 16.88 ng/ml

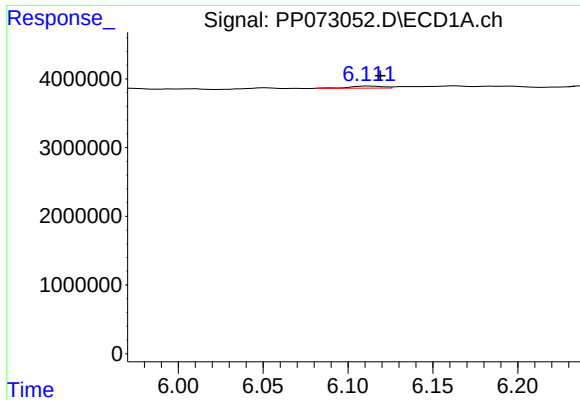

#7 AR-1016-5


R.T.: 6.112 min
Delta R.T.: -0.007 min
Response: 405372
Conc: 8.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

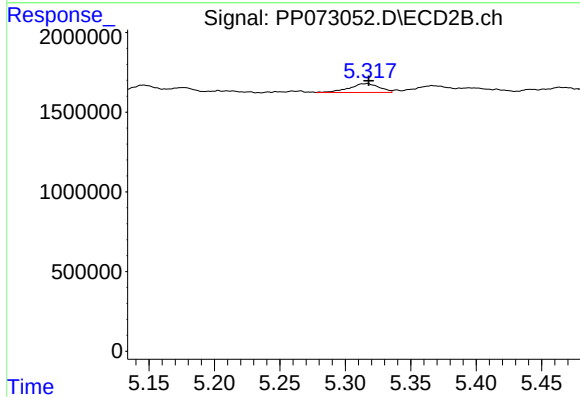


#7 AR-1016-5

R.T.: 5.317 min
Delta R.T.: -0.001 min
Response: 887346
Conc: 16.05 ng/ml

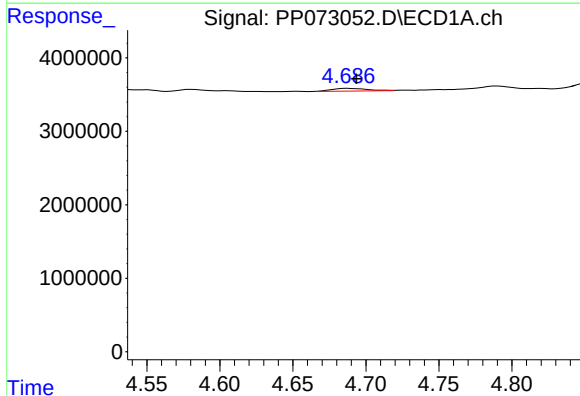


#8 AR-1221-1

R.T.: 4.688 min
Delta R.T.: -0.006 min
Response: 610396
Conc: 24.75 ng/ml

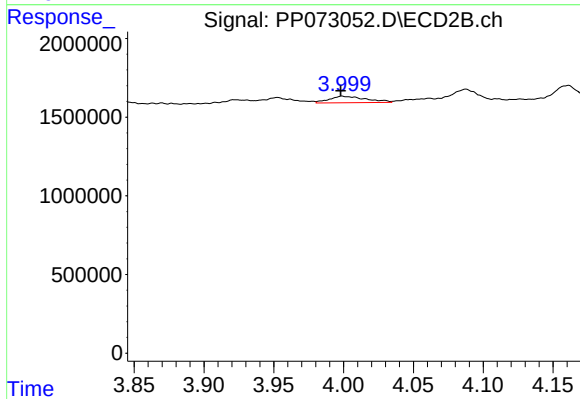

#8 AR-1221-1


R.T.: 3.999 min
Delta R.T.: 0.001 min
Response: 764538
Conc: 28.45 ng/ml

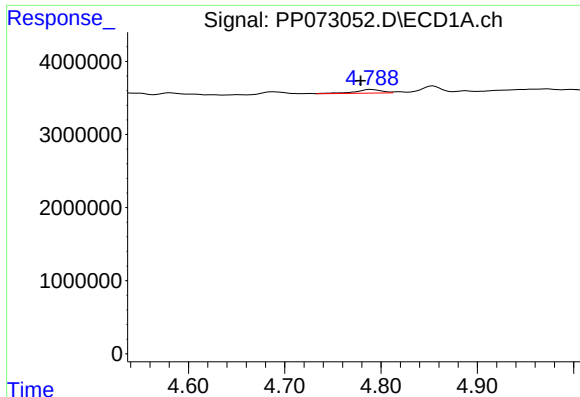

#9 AR-1221-2


R.T.: 4.790 min
Delta R.T.: 0.011 min
Response: 953065
Conc: 47.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

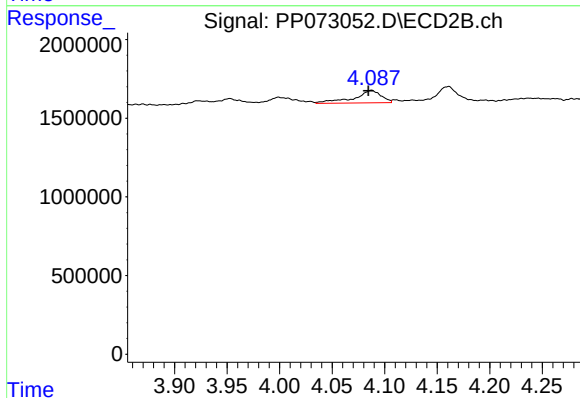


#9 AR-1221-2

R.T.: 4.087 min
Delta R.T.: 0.003 min
Response: 1417441
Conc: 70.22 ng/ml

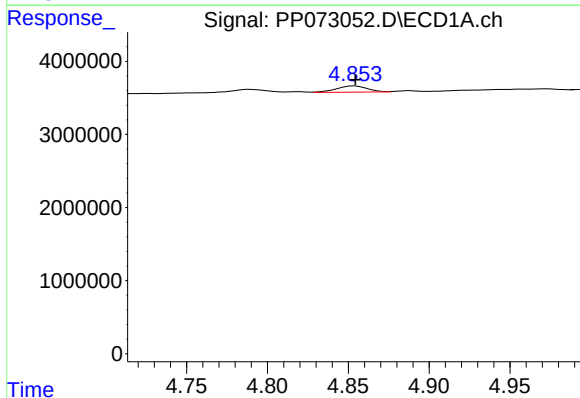


#10 AR-1221-3

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 1129419
Conc: 18.35 ng/ml

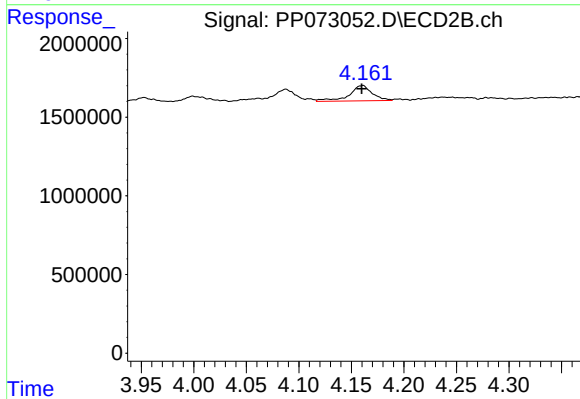

#10 AR-1221-3


R.T.: 4.161 min
Delta R.T.: 0.000 min
Response: 1487593
Conc: 25.33 ng/ml

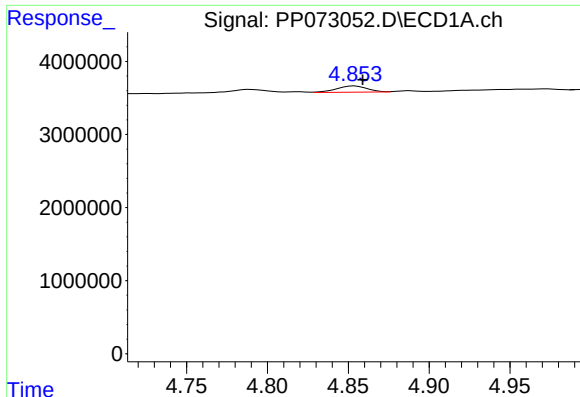

#11 AR-1232-1


R.T.: 4.854 min
Delta R.T.: -0.005 min
Response: 1129419
Conc: 24.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

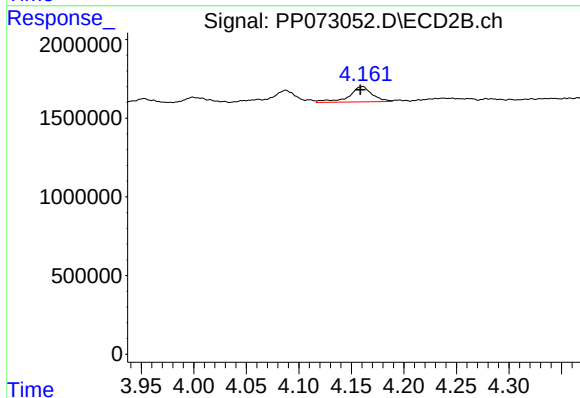


#11 AR-1232-1

R.T.: 4.161 min
Delta R.T.: 0.002 min
Response: 1487593
Conc: 32.65 ng/ml

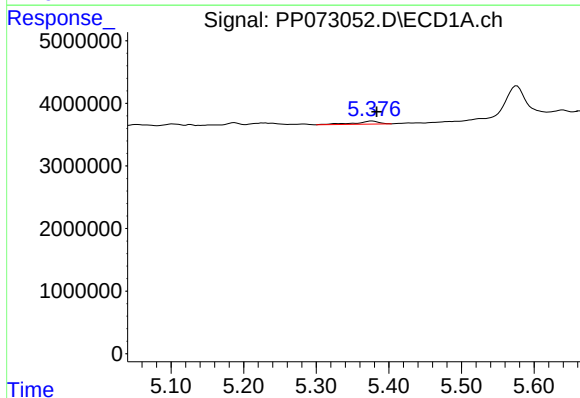


#12 AR-1232-2

R.T.: 5.377 min
Delta R.T.: -0.006 min
Response: 1061445
Conc: 47.45 ng/ml

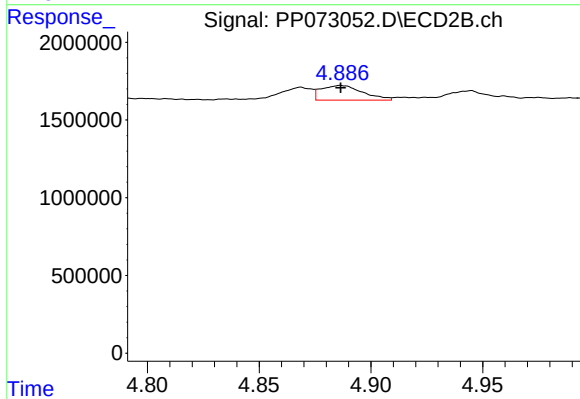

#12 AR-1232-2


R.T.: 4.887 min
Delta R.T.: 0.000 min
Response: 1217297
Conc: 26.31 ng/ml

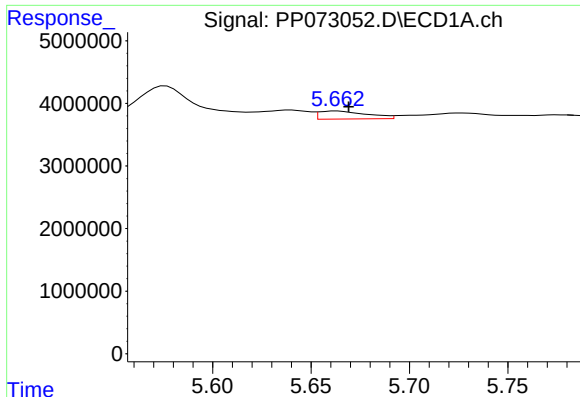

#13 AR-1232-3


R.T.: 5.663 min
Delta R.T.: -0.006 min
Response: 2193905
Conc: 42.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

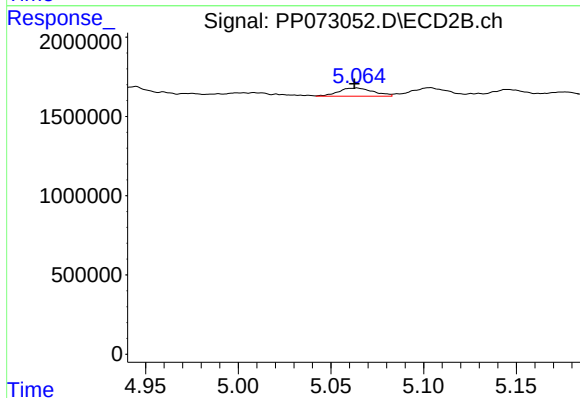


#13 AR-1232-3

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 674648
Conc: 27.47 ng/ml

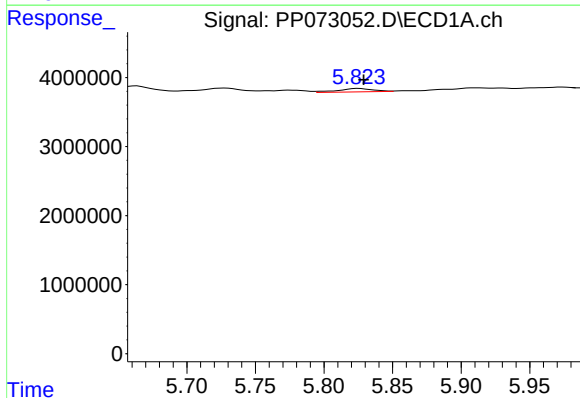


#14 AR-1232-4

R.T.: 5.825 min
Delta R.T.: -0.004 min
Response: 881430
Conc: 34.15 ng/ml

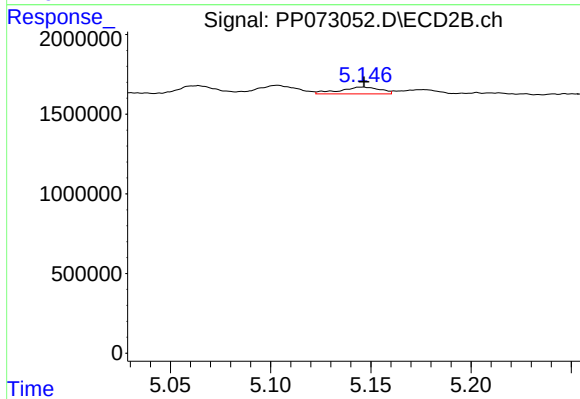

#14 AR-1232-4


R.T.: 5.146 min
Delta R.T.: -0.001 min
Response: 600710
Conc: 27.78 ng/ml

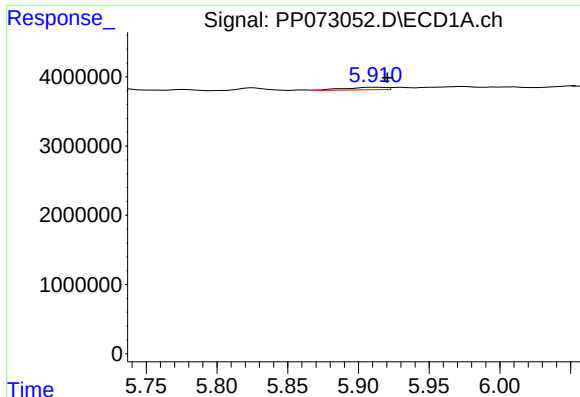

#15 AR-1232-5


R.T.: 5.912 min
Delta R.T.: -0.009 min
Response: 740136
Conc: 20.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

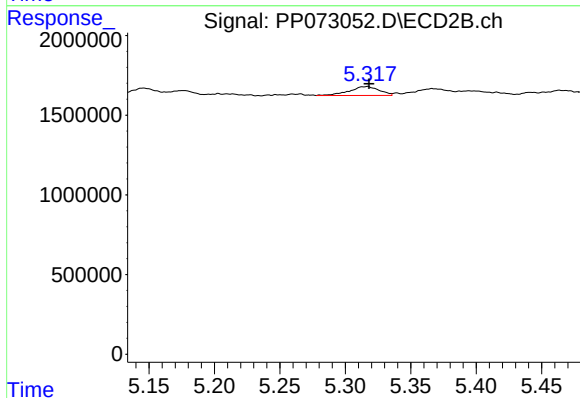


#15 AR-1232-5

R.T.: 5.317 min
Delta R.T.: -0.002 min
Response: 887346
Conc: 38.82 ng/ml

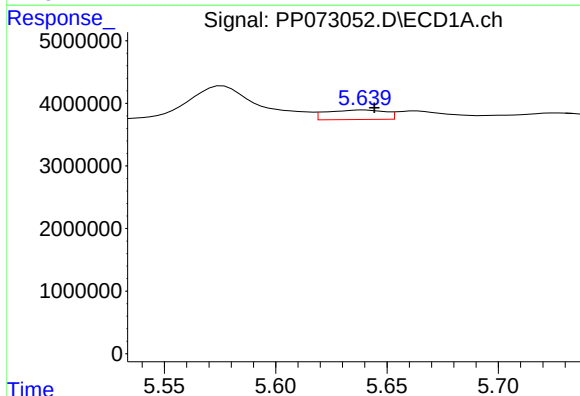


#16 AR-1242-1

R.T.: 5.640 min
Delta R.T.: -0.004 min
Response: 2802598
Conc: 47.96 ng/ml

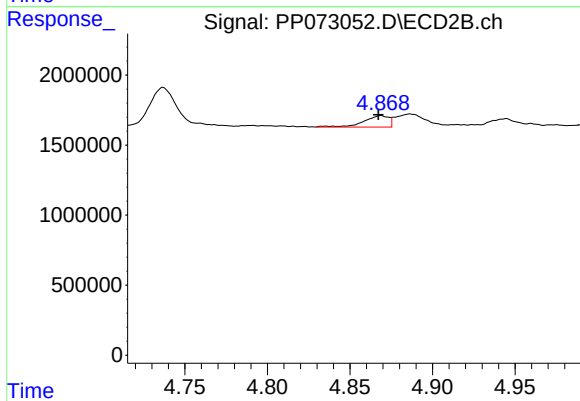

#16 AR-1242-1


R.T.: 4.869 min
Delta R.T.: 0.001 min
Response: 871973
Conc: 15.79 ng/ml

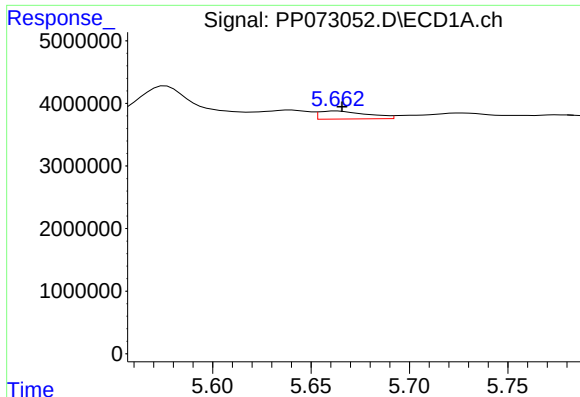

#17 AR-1242-2


R.T.: 5.663 min
Delta R.T.: -0.002 min
Response: 2193905
Conc: 25.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

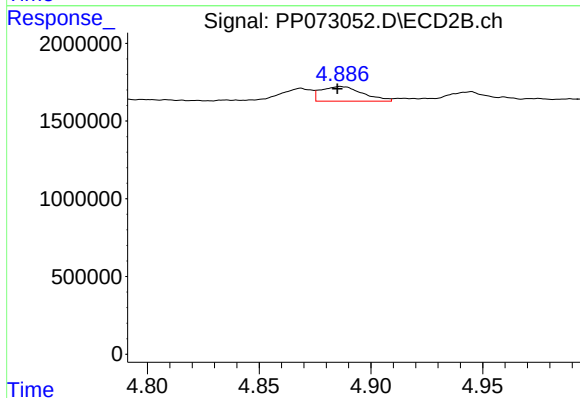


#17 AR-1242-2

R.T.: 4.887 min
Delta R.T.: 0.002 min
Response: 1217297
Conc: 15.31 ng/ml

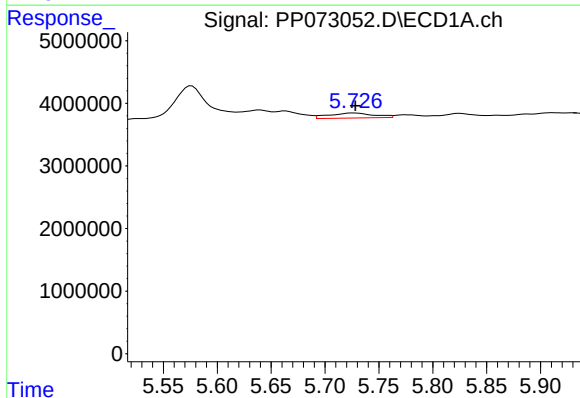


#18 AR-1242-3

R.T.: 5.727 min
Delta R.T.: -0.001 min
Response: 2345220
Conc: 44.49 ng/ml

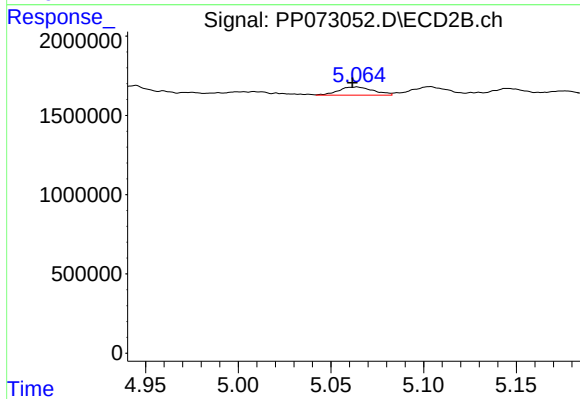

#18 AR-1242-3


R.T.: 5.064 min
Delta R.T.: 0.002 min
Response: 674648
Conc: 15.58 ng/ml

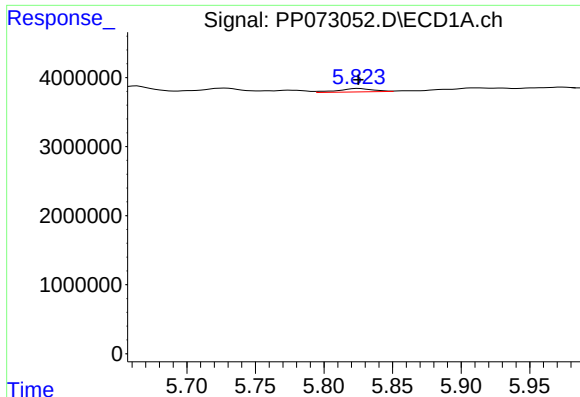

#19 AR-1242-4


R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 881430
Conc: 20.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

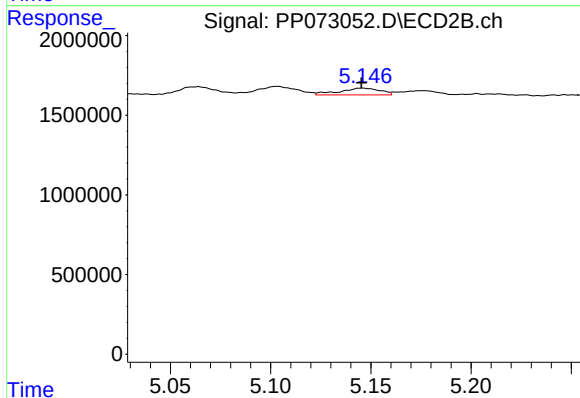


#19 AR-1242-4

R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 600710
Conc: 14.47 ng/ml

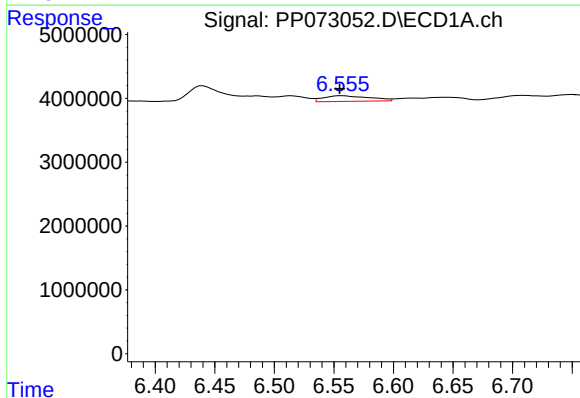


#20 AR-1242-5

R.T.: 6.557 min
Delta R.T.: 0.002 min
Response: 2403851
Conc: 48.50 ng/ml

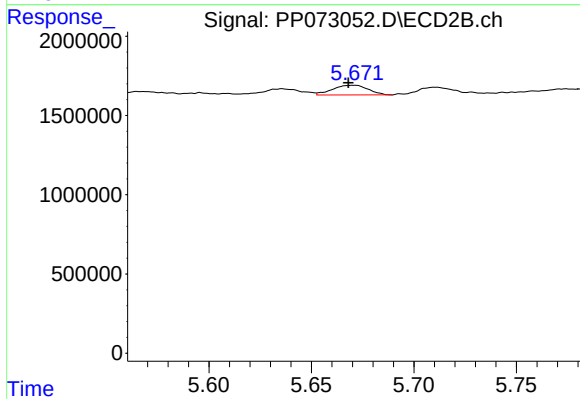

#20 AR-1242-5


R.T.: 5.671 min
Delta R.T.: 0.003 min
Response: 738645
Conc: 14.05 ng/ml

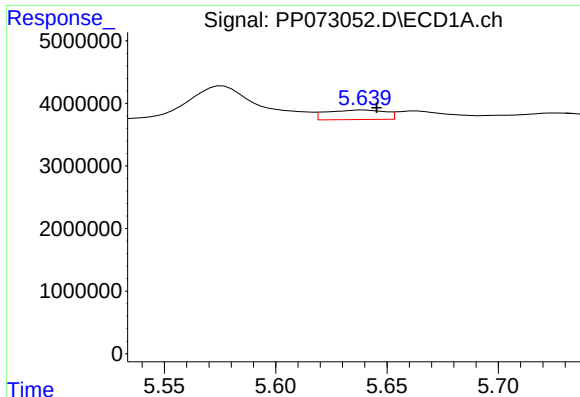

#21 AR-1248-1


R.T.: 5.640 min
Delta R.T.: -0.005 min
Response: 2802598
Conc: 58.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

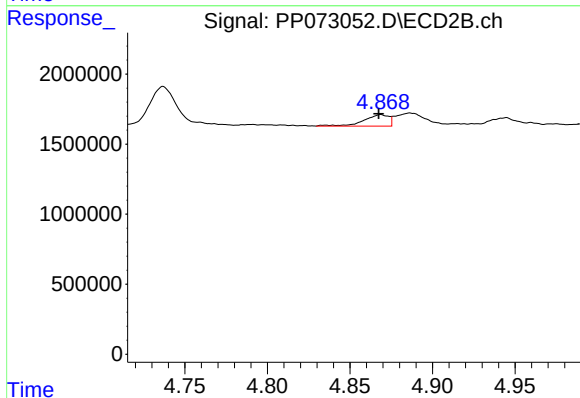


#21 AR-1248-1

R.T.: 4.869 min
Delta R.T.: 0.001 min
Response: 871973
Conc: 20.00 ng/ml

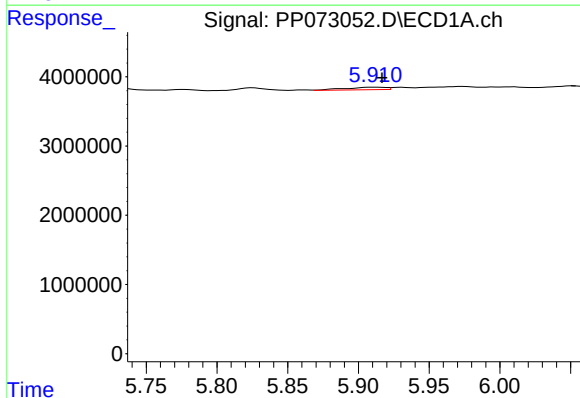


#22 AR-1248-2

R.T.: 5.912 min
Delta R.T.: -0.005 min
Response: 740136
Conc: 12.64 ng/ml

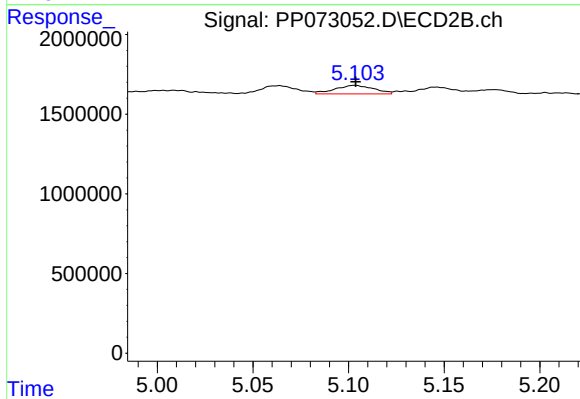

#22 AR-1248-2


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 752159
Conc: 12.84 ng/ml

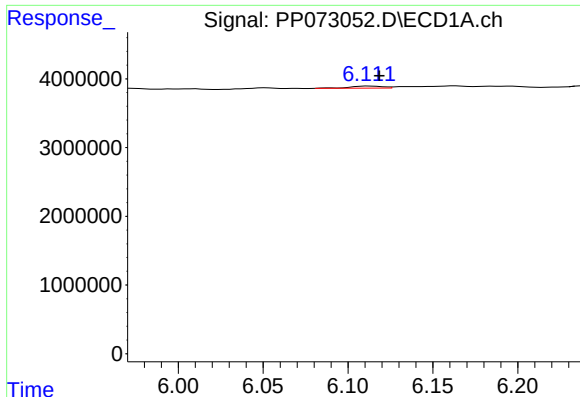

#23 AR-1248-3


R.T.: 6.112 min
Delta R.T.: -0.006 min
Response: 405372
Conc: 6.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

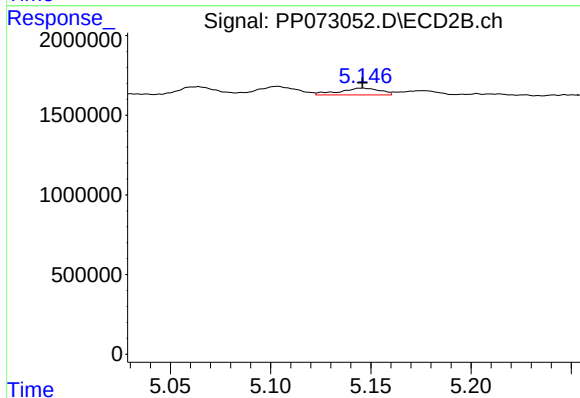


#23 AR-1248-3

R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 600710
Conc: 9.92 ng/ml

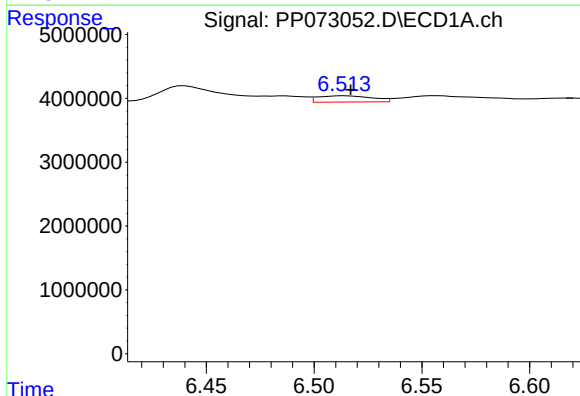


#24 AR-1248-4

R.T.: 6.514 min
Delta R.T.: -0.003 min
Response: 1733838
Conc: 20.38 ng/ml

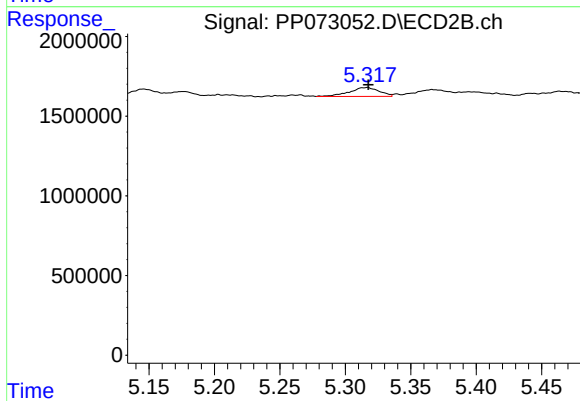

#24 AR-1248-4


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 887346
Conc: 12.67 ng/ml

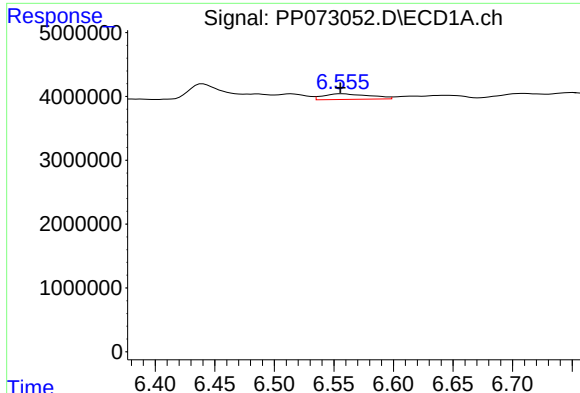

#25 AR-1248-5


R.T.: 6.557 min
Delta R.T.: 0.001 min
Response: 2403851
Conc: 28.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

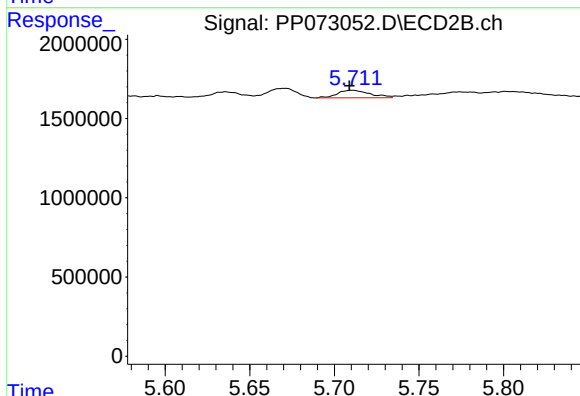


#25 AR-1248-5

R.T.: 5.711 min
Delta R.T.: 0.002 min
Response: 644842
Conc: 9.08 ng/ml

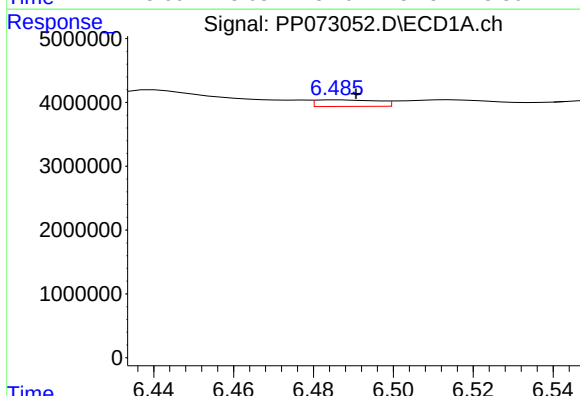


#26 AR-1254-1

R.T.: 6.486 min
Delta R.T.: -0.004 min
Response: 1114884
Conc: 13.25 ng/ml

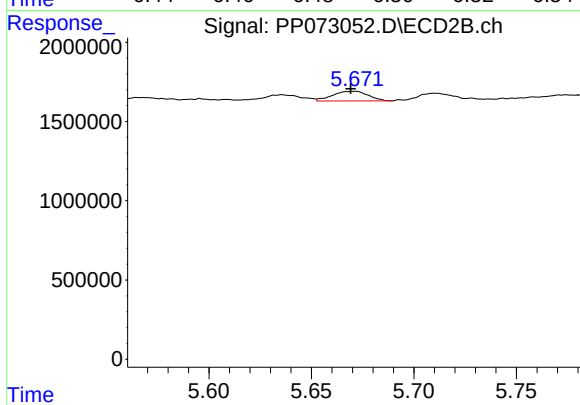

#26 AR-1254-1


R.T.: 5.671 min
Delta R.T.: 0.002 min
Response: 738645
Conc: 6.74 ng/ml

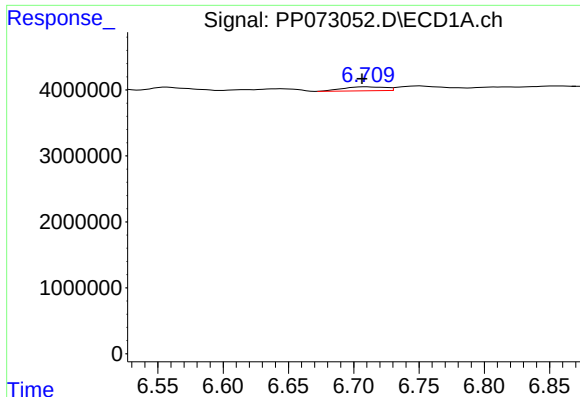

#27 AR-1254-2


R.T.: 6.710 min
Delta R.T.: 0.003 min
Response: 1376629
Conc: 10.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

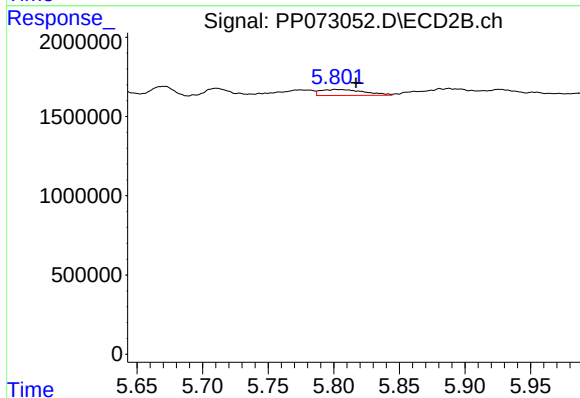


#27 AR-1254-2

R.T.: 5.801 min
Delta R.T.: -0.015 min
Response: 868941
Conc: 9.19 ng/ml

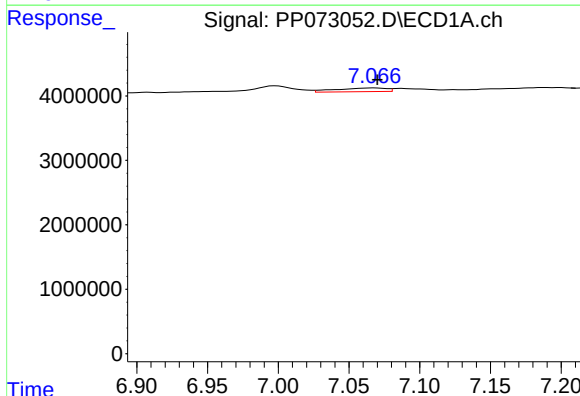


#28 AR-1254-3

R.T.: 7.067 min
Delta R.T.: -0.003 min
Response: 1420706
Conc: 10.83 ng/ml

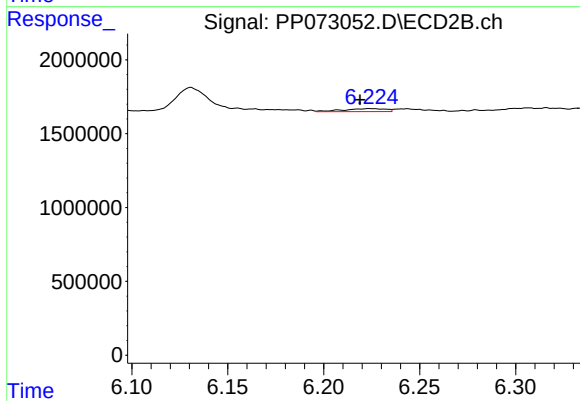

#28 AR-1254-3


R.T.: 6.224 min
Delta R.T.: 0.006 min
Response: 315487
Conc: 2.14 ng/ml

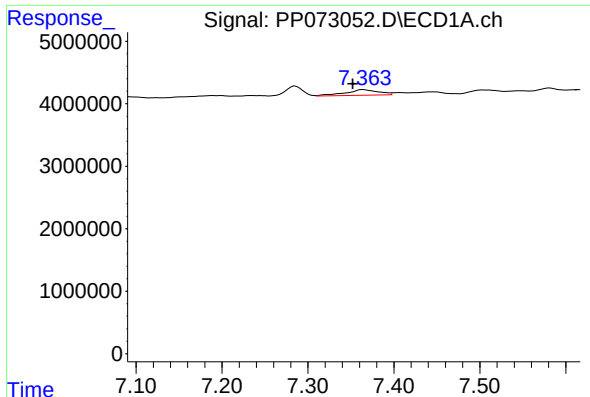

#29 AR-1254-4


R.T.: 7.364 min
Delta R.T.: 0.012 min
Response: 2442770
Conc: 20.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

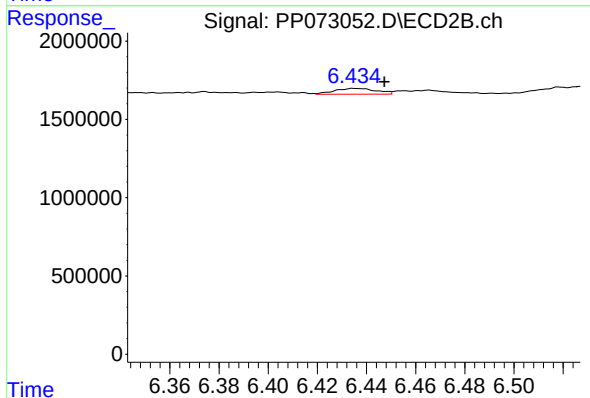


#29 AR-1254-4

R.T.: 6.435 min
Delta R.T.: -0.012 min
Response: 439042
Conc: 4.52 ng/ml

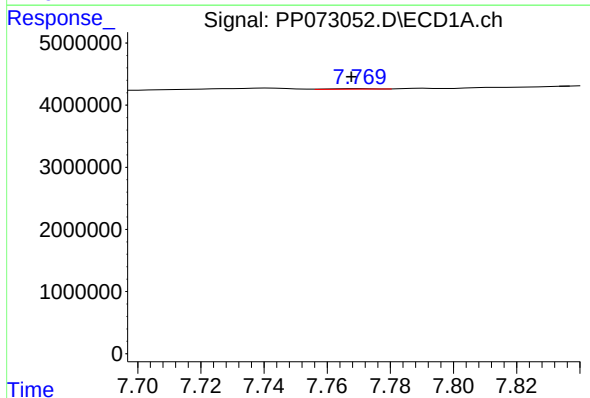


#30 AR-1254-5

R.T.: 7.771 min
Delta R.T.: 0.003 min
Response: 88827
Conc: 0.78 ng/ml

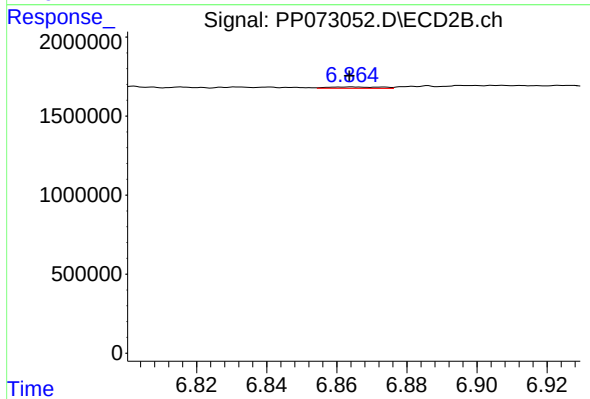

#30 AR-1254-5


R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 94293
Conc: 0.73 ng/ml

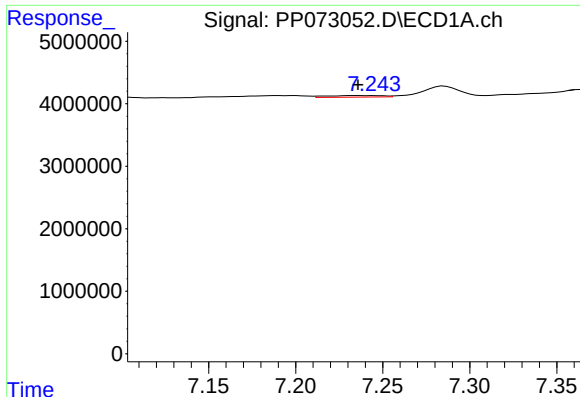

#31 AR-1260-1


R.T.: 7.234 min
Delta R.T.: -0.002 min
Response: 569147
Conc: 6.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

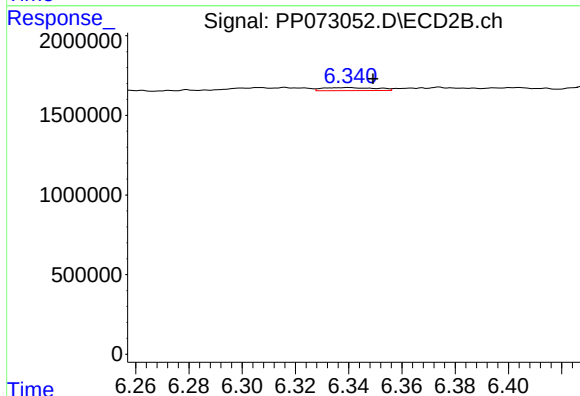


#31 AR-1260-1

R.T.: 6.340 min
Delta R.T.: -0.009 min
Response: 264326
Conc: 2.79 ng/ml

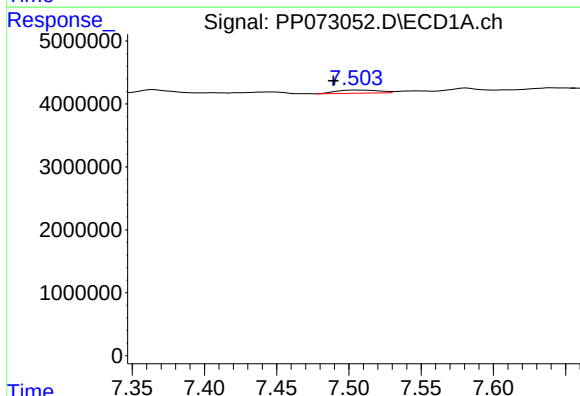


#32 AR-1260-2

R.T.: 7.505 min
Delta R.T.: 0.015 min
Response: 1033862
Conc: 7.61 ng/ml

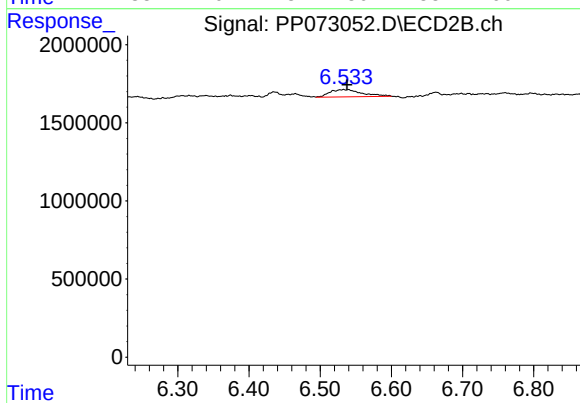

#32 AR-1260-2


R.T.: 6.533 min
Delta R.T.: -0.005 min
Response: 1463060
Conc: 12.57 ng/ml

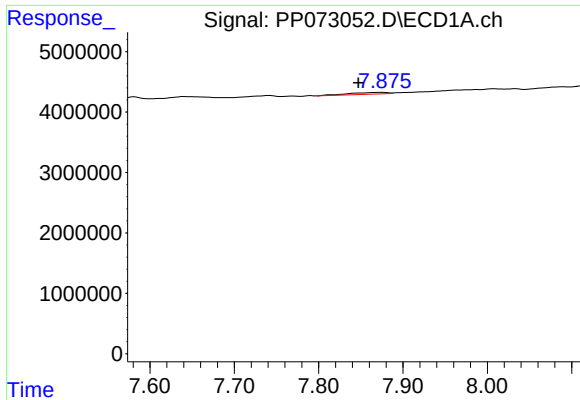

#33 AR-1260-3


R.T.: 7.875 min
Delta R.T.: 0.028 min
Response: 962157
Conc: 8.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

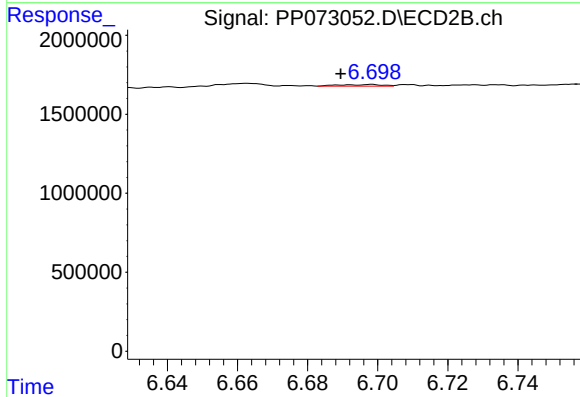


#33 AR-1260-3

R.T.: 6.698 min
Delta R.T.: 0.009 min
Response: 90083
Conc: 0.86 ng/ml

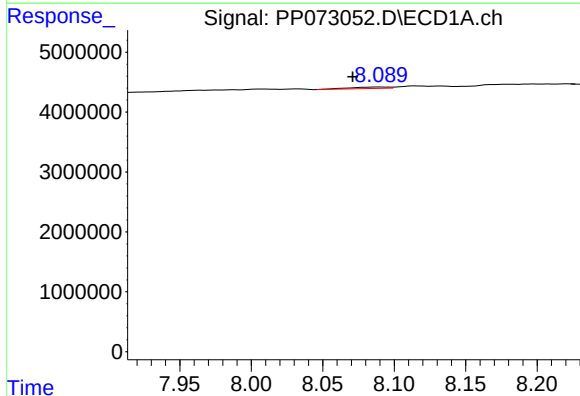


#34 AR-1260-4

R.T.: 8.090 min
Delta R.T.: 0.019 min
Response: 469251
Conc: 4.55 ng/ml

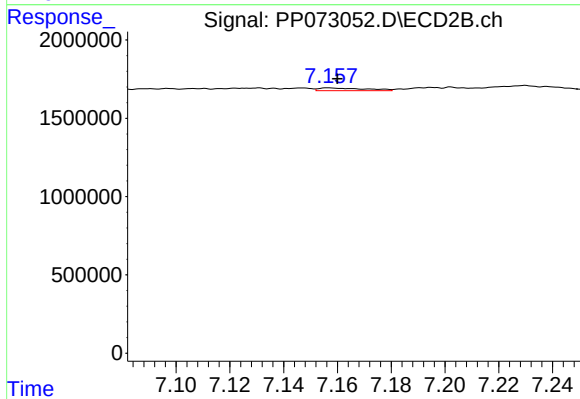

#34 AR-1260-4


R.T.: 7.157 min
Delta R.T.: -0.003 min
Response: 209604
Conc: 2.39 ng/ml

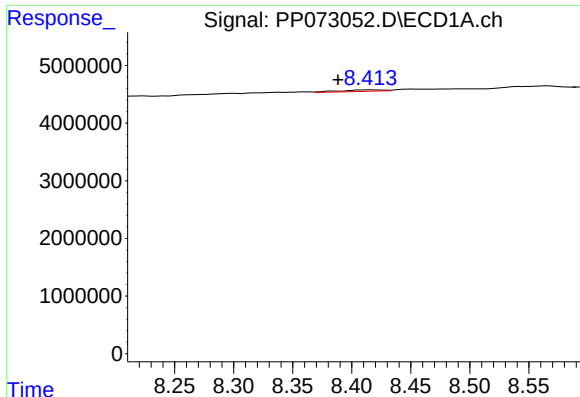

#35 AR-1260-5


R.T.: 8.416 min
Delta R.T.: 0.027 min
Response: 702989
Conc: 2.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

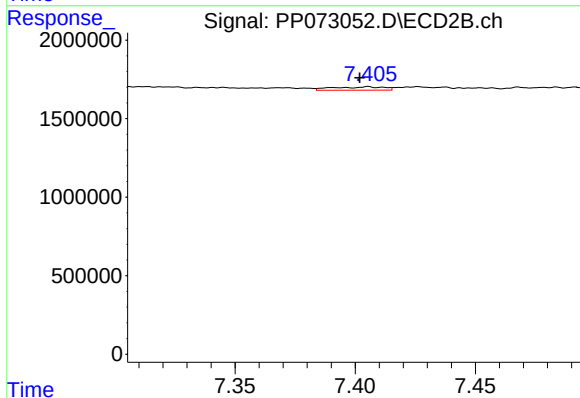


#35 AR-1260-5

R.T.: 7.405 min
Delta R.T.: 0.003 min
Response: 312873
Conc: 1.47 ng/ml

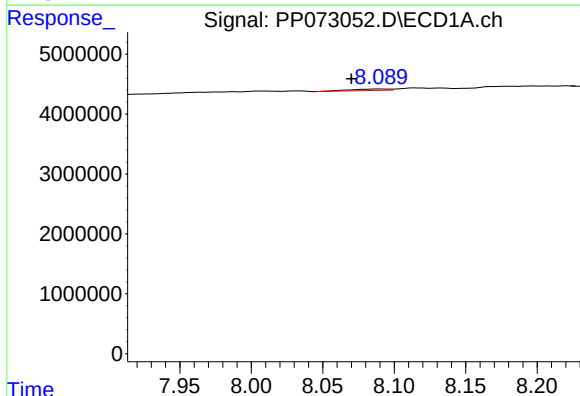


#36 AR-1262-1

R.T.: 8.090 min
Delta R.T.: 0.020 min
Response: 469251
Conc: 3.17 ng/ml

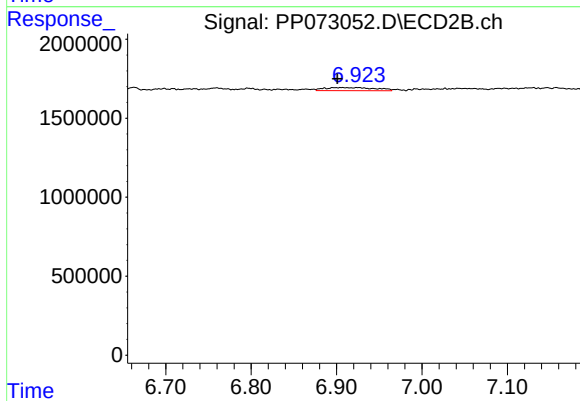

#36 AR-1262-1


R.T.: 6.906 min
Delta R.T.: 0.005 min
Response: 798677
Conc: 5.53 ng/ml

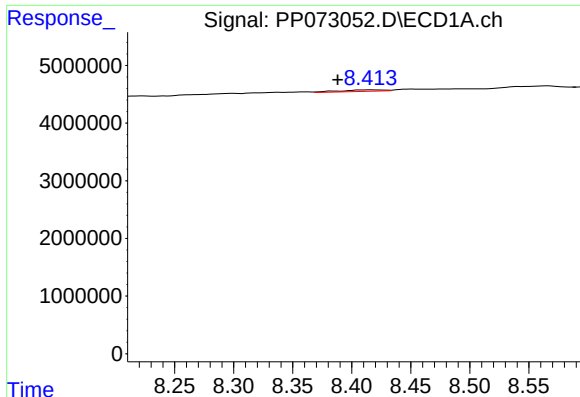

#37 AR-1262-2


R.T.: 8.416 min
Delta R.T.: 0.028 min
Response: 702989
Conc: 2.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

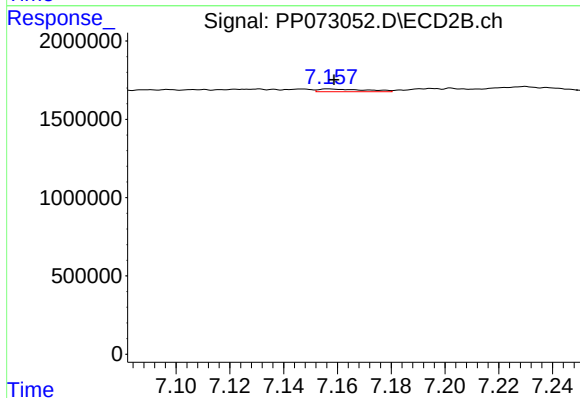


#37 AR-1262-2

R.T.: 7.157 min
Delta R.T.: -0.002 min
Response: 209604
Conc: 1.71 ng/ml

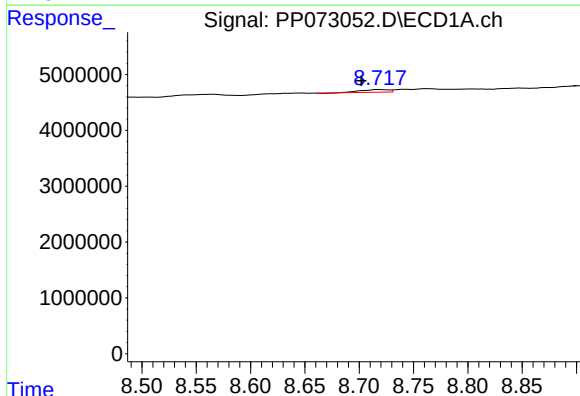


#38 AR-1262-3

R.T.: 8.719 min
Delta R.T.: 0.017 min
Response: 823397
Conc: 3.85 ng/ml

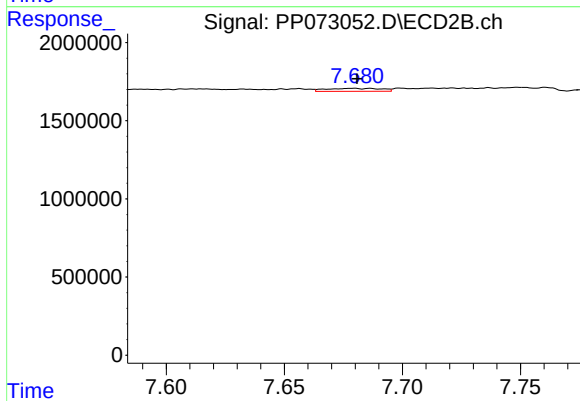

#38 AR-1262-3


R.T.: 7.679 min
Delta R.T.: -0.002 min
Response: 313546
Conc: 2.78 ng/ml

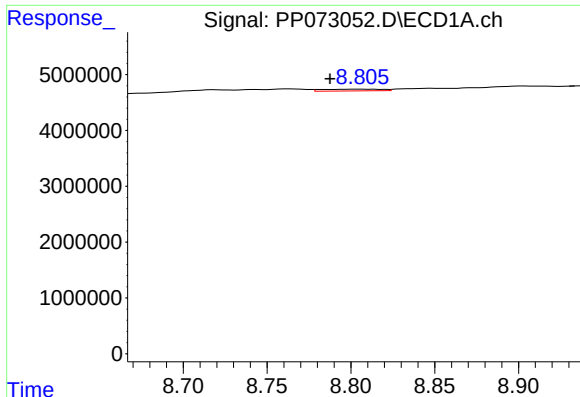

#39 AR-1262-4


R.T.: 8.804 min
Delta R.T.: 0.016 min
Response: 775519
Conc: 4.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

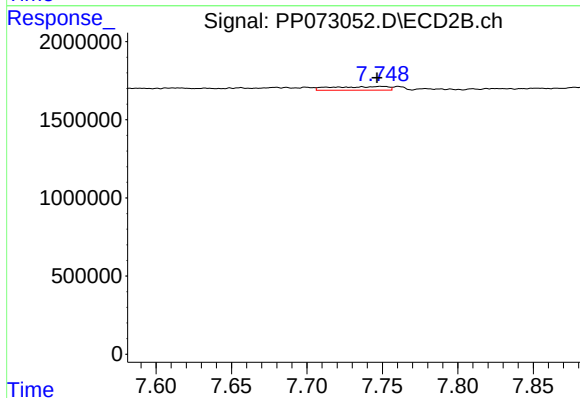


#39 AR-1262-4

R.T.: 7.750 min
Delta R.T.: 0.003 min
Response: 602732
Conc: 3.29 ng/ml

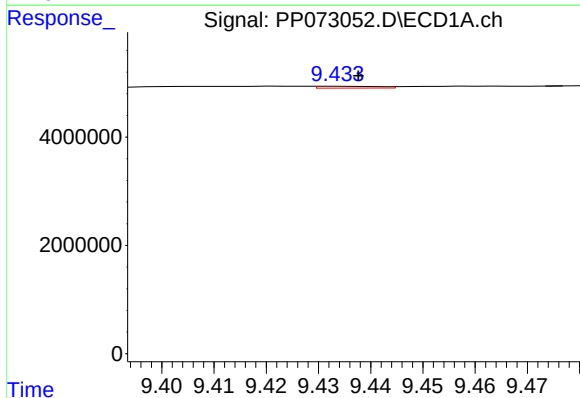


#40 AR-1262-5

R.T.: 9.434 min
Delta R.T.: -0.003 min
Response: 288421
Conc: 2.58 ng/ml

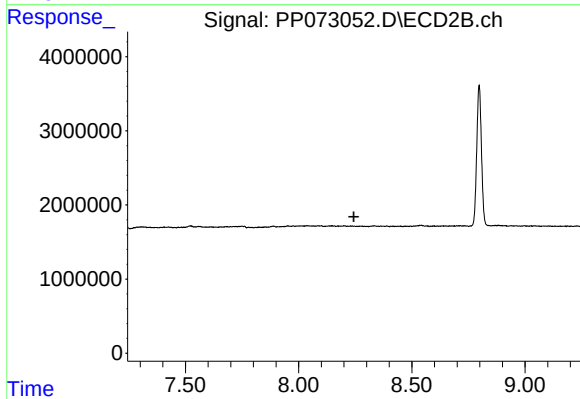

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.244 min
Response: 0
Conc: N.D.

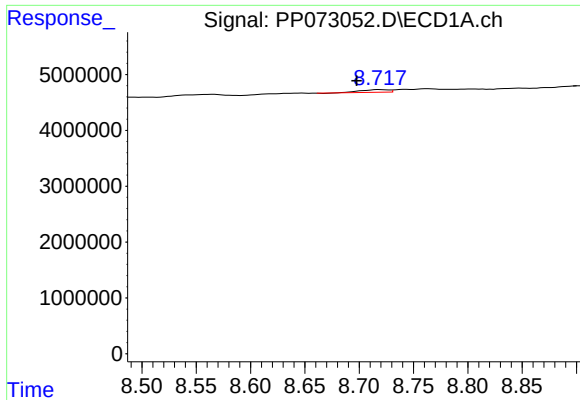

#41 AR-1268-1


R.T.: 8.719 min
Delta R.T.: 0.021 min
Response: 823397
Conc: 2.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

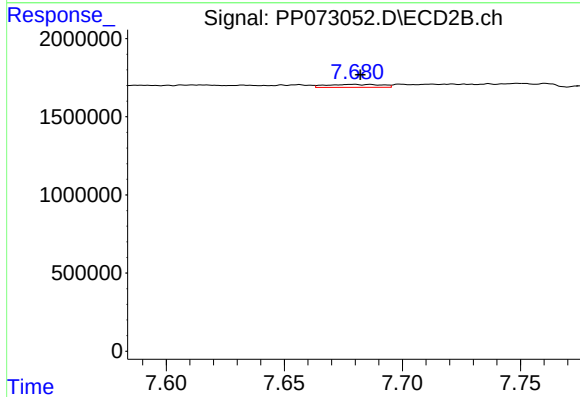


#41 AR-1268-1

R.T.: 7.679 min
Delta R.T.: -0.003 min
Response: 313546
Conc: 1.09 ng/ml

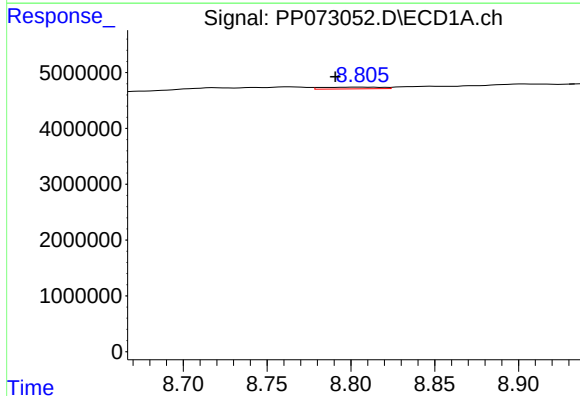


#42 AR-1268-2

R.T.: 8.804 min
Delta R.T.: 0.013 min
Response: 775519
Conc: 2.54 ng/ml

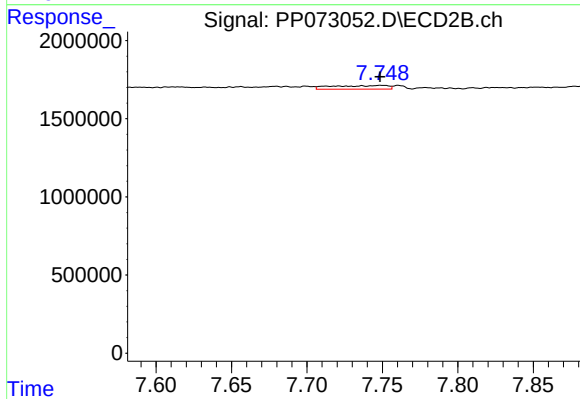

#42 AR-1268-2


R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 602732
Conc: 2.34 ng/ml

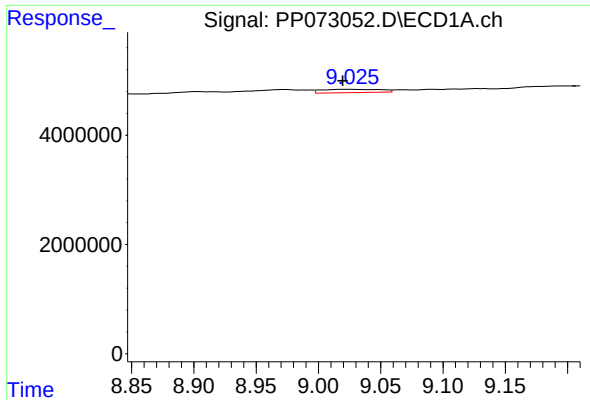

#43 AR-1268-3


R.T.: 9.023 min
Delta R.T.: 0.004 min
Response: 2028644
Conc: 7.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

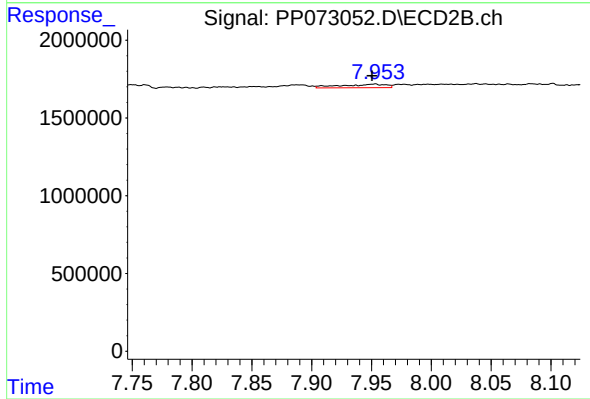


#43 AR-1268-3

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 590385
Conc: 2.73 ng/ml

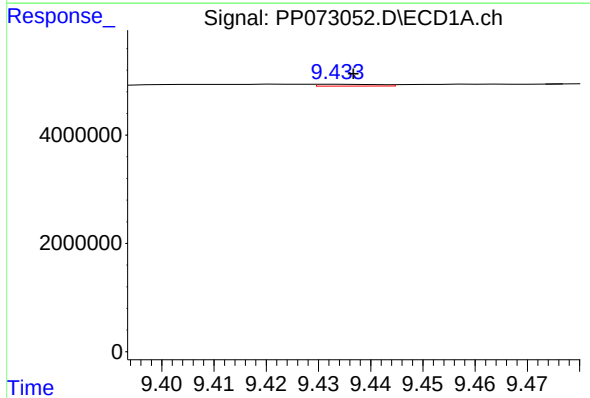


#44 AR-1268-4

R.T.: 9.434 min
Delta R.T.: -0.002 min
Response: 288421
Conc: 2.46 ng/ml

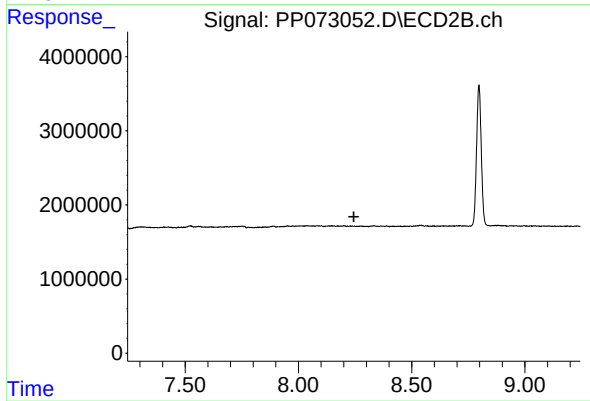

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.245 min
Response: 0
Conc: N.D.

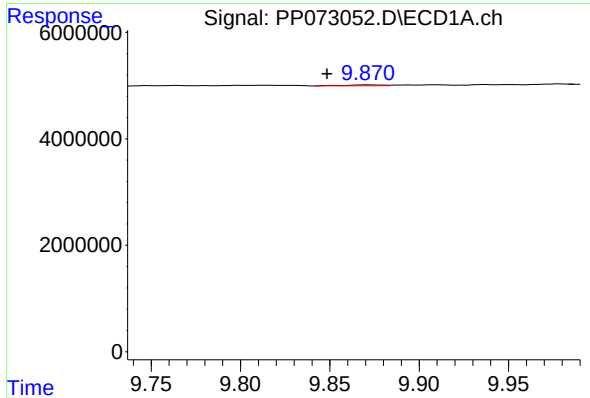

#45 AR-1268-5

R.T.: 9.871 min
Delta R.T.: 0.023 min
Response: 269955
Conc: 0.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

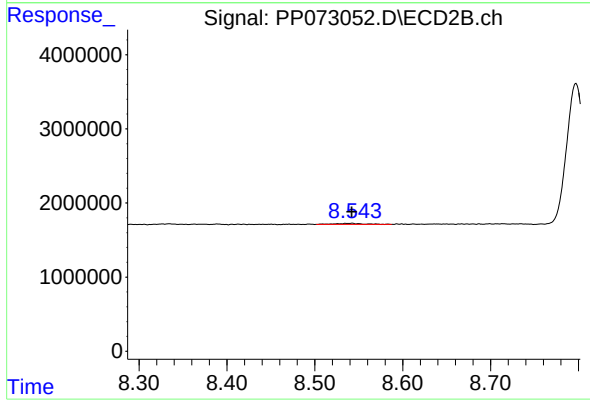

#45 AR-1268-5

R.T.: 8.540 min
Delta R.T.: -0.002 min
Response: 295776
Conc: 0.51 ng/ml