

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
 Data File : PP073060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 22:47
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:42:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.496	3.787	42097683	35958023	19.944	19.957
2)	SA Decachlor...	10.189	8.797	37931524	28517744	22.197	21.366
Target Compounds							
3)	L1 AR-1016-1	5.646	4.868	3274633	2954527	45.061	42.995
4)	L1 AR-1016-2	5.669	4.886	4375765	4212716	42.066	41.860
5)	L1 AR-1016-3	5.731	5.062	2596172	2423103	39.728	44.285
6)	L1 AR-1016-4	5.828	5.104	1976574	2039947	37.807	45.790
7)	L1 AR-1016-5	6.120	5.317	1951632	2188133	39.029	39.581
8)	L2 AR-1221-1	4.700	3.995	3602996	277975	146.111	10.344 #
9)	L2 AR-1221-2	4.796	4.087	1167416	2573590	57.853	127.497 #
10)	L2 AR-1221-3	4.858	4.158	1467068	1612126	23.835	27.449
11)	L3 AR-1232-1	4.858	4.158	1467068	1612126	31.243	35.381
12)	L3 AR-1232-2	5.382	4.886	1796469	4212716	80.307	91.066
13)	L3 AR-1232-3	5.669	5.062	4375765	2423103	84.806	98.669
14)	L3 AR-1232-4	5.828	5.146	1976574	2283088	76.581	105.575 #
15)	L3 AR-1232-5	5.919	5.317	1520245	2188133	42.619	95.724 #
16)	L4 AR-1242-1	5.646	4.868	3274633	2954527	56.037	53.506
17)	L4 AR-1242-2	5.669	4.886	4375765	4212716	50.555	52.999
18)	L4 AR-1242-3	5.731	5.062	2596172	2423103	49.256	55.954
19)	L4 AR-1242-4	5.828	5.146	1976574	2283088	44.965	55.009
20)	L4 AR-1242-5	6.560	5.668	1801915	2203363	36.358	41.900
21)	L5 AR-1248-1	5.646	4.868	3274633	2954527	68.840	67.779
22)	L5 AR-1248-2	5.919	5.104	1520245	2039947	25.964	34.814 #
23)	L5 AR-1248-3	6.120	5.146	1951632	2283088	29.910	37.709 #
24)	L5 AR-1248-4	6.518	5.317	1250635	2188133	14.702	31.249 #
25)	L5 AR-1248-5	6.560	5.709	1801915	509730	21.530	7.176 #
26)	L6 AR-1254-1	6.494	5.668	2726927	2203363	32.396	20.095 #
27)	L6 AR-1254-2	6.711	5.817	2297205	1616668	18.319	17.099
28)	L6 AR-1254-3	7.074	6.233	1753915	2881056	13.367	19.526 #
29)	L6 AR-1254-4	7.358	6.438	2008052	646749	16.764	6.661 #
30)	L6 AR-1254-5	7.770	6.863	5163614	5007390	45.193	38.529
31)	L7 AR-1260-1	7.237	6.349	4573467	3837031	51.846	40.505
32)	L7 AR-1260-2	7.491	6.538	5693038	4880115	41.896	41.912
33)	L7 AR-1260-3	7.849	6.690	4212387	4375961	36.901	42.011
34)	L7 AR-1260-4	8.073	7.160	4105552	3589972	39.842	40.917
35)	L7 AR-1260-5	8.391	7.402	9004036	8264153	37.420	38.726
36)	L8 AR-1262-1	8.073	6.901	4105552	4338348	27.736	30.030
37)	L8 AR-1262-2	8.391	7.160	9004036	3589972	28.452	29.370
38)	L8 AR-1262-3	8.711	7.682	5963152	2080723	27.869	18.462 #
39)	L8 AR-1262-4	8.775	7.745	4742356	6064617	30.092	33.076
40)	L8 AR-1262-5	9.440	8.245	3450909	2209895	30.849	25.523
41)	L9 AR-1268-1	8.711	7.682	5963152	2080723	16.674	7.243 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
 Data File : PP073060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 22:47
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:42:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.775	7.745	4742356	6064617	15.546	23.587 #
43) L9	AR-1268-3	9.036	7.949	2528998	423708	9.525	1.962 #
44) L9	AR-1268-4	9.440	8.245	3450909	2209895	29.489	23.463
45) L9	AR-1268-5	9.851	8.541	589885	600286	0.798	1.037 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
Data File : PP073060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 22:47
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:42:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

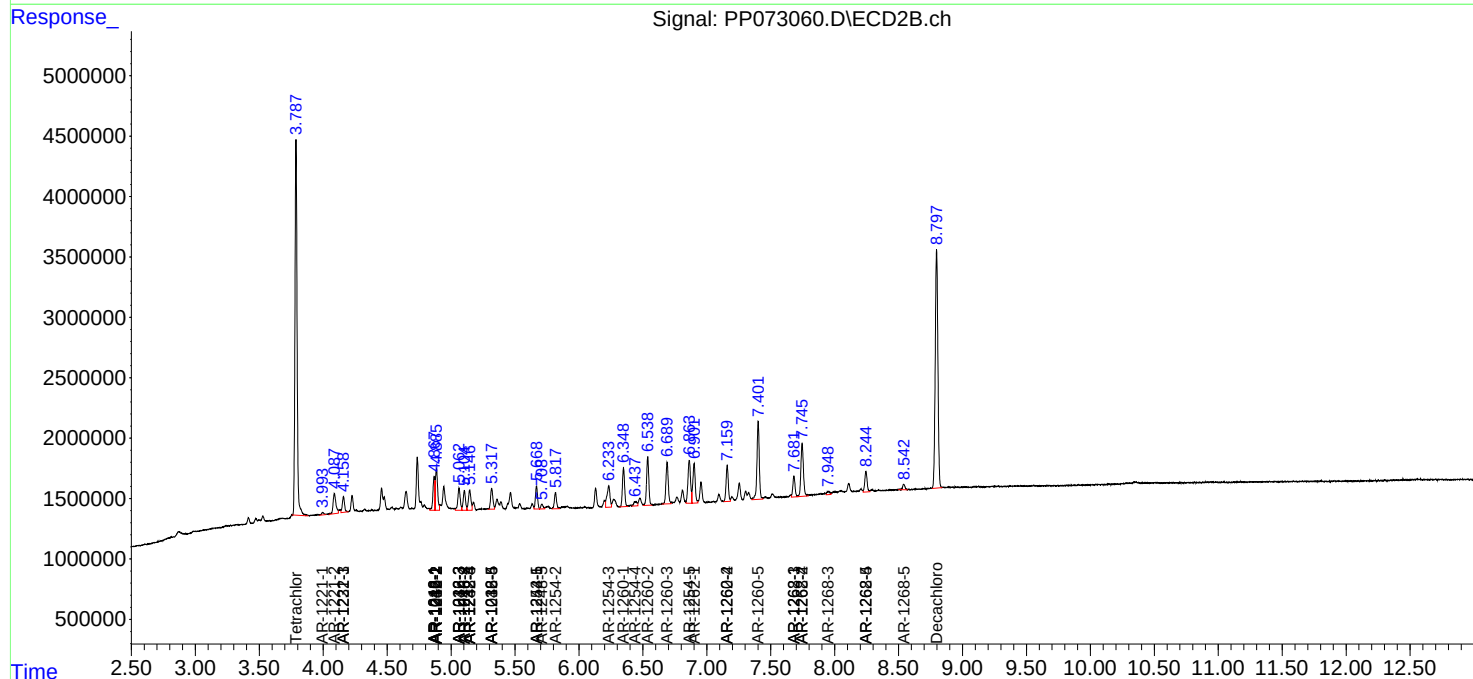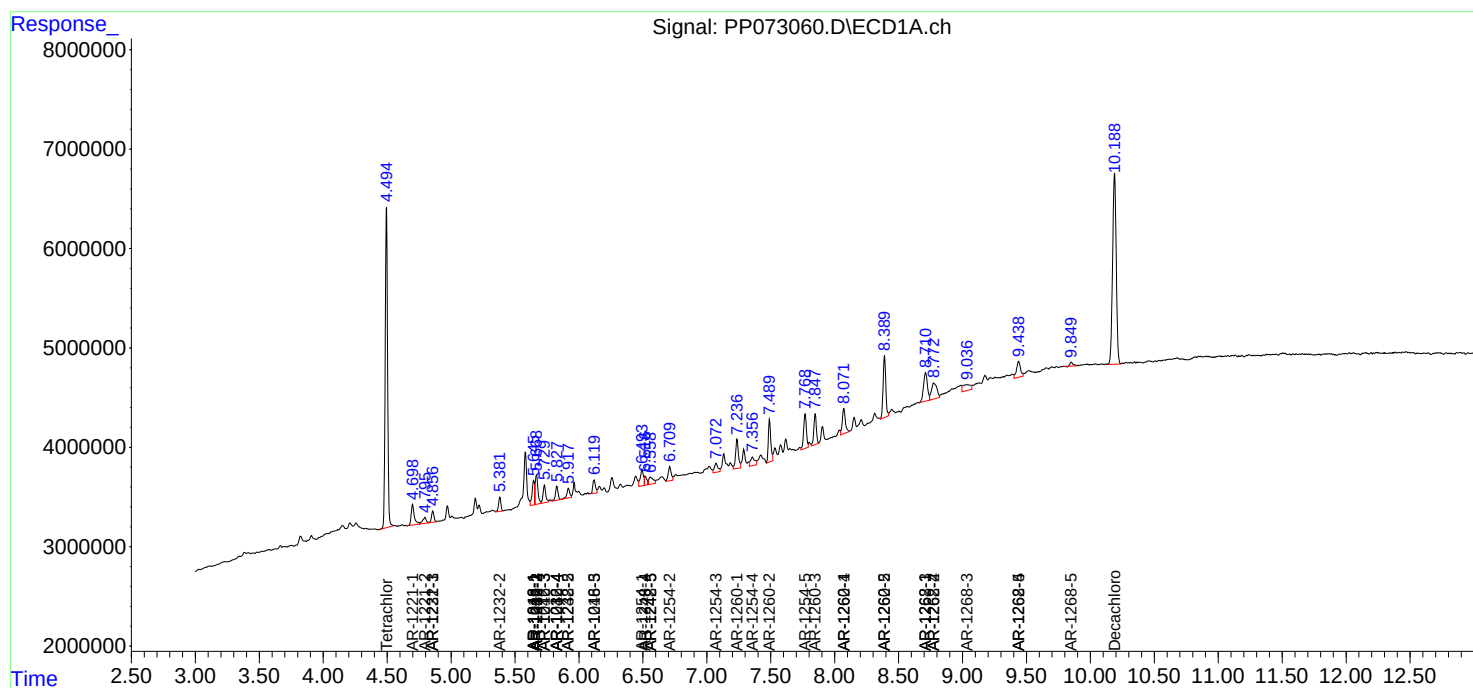


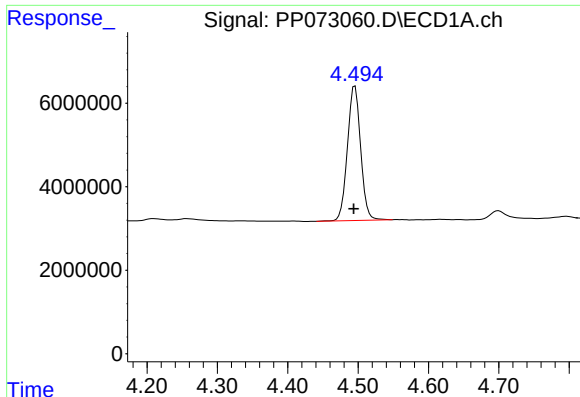

#1 Tetrachloro-m-xylene


R.T.: 4.496 min
Delta R.T.: 0.002 min
Response: 42097683
Conc: 19.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

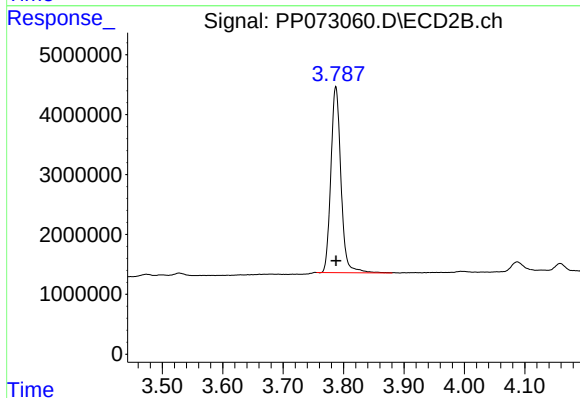


#1 Tetrachloro-m-xylene

R.T.: 3.787 min
Delta R.T.: 0.000 min
Response: 35958023
Conc: 19.96 ng/ml

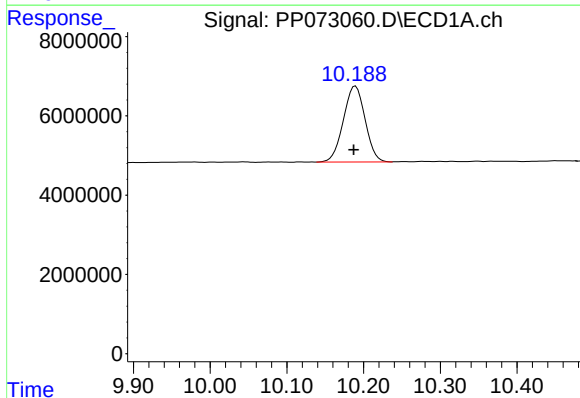


#2 Decachlorobiphenyl

R.T.: 10.189 min
Delta R.T.: 0.002 min
Response: 37931524
Conc: 22.20 ng/ml

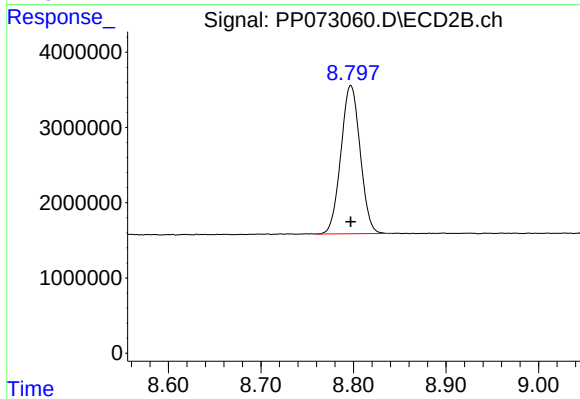

#2 Decachlorobiphenyl


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 28517744
Conc: 21.37 ng/ml

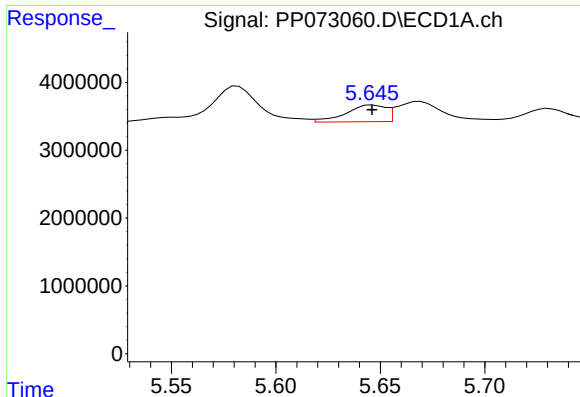

#3 AR-1016-1


R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 3274633
Conc: 45.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

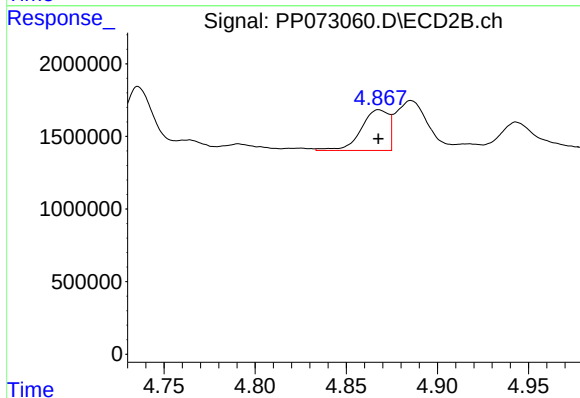


#3 AR-1016-1

R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 2954527
Conc: 43.00 ng/ml

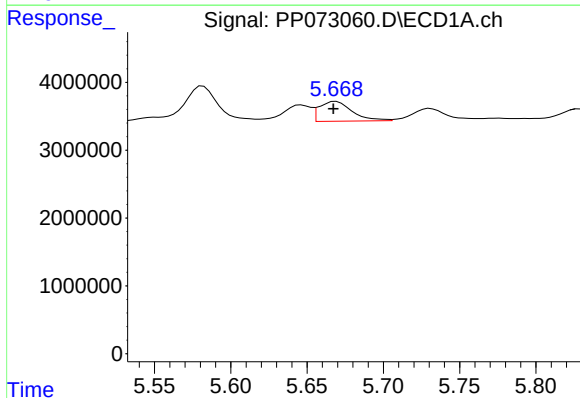


#4 AR-1016-2

R.T.: 5.669 min
Delta R.T.: 0.002 min
Response: 4375765
Conc: 42.07 ng/ml

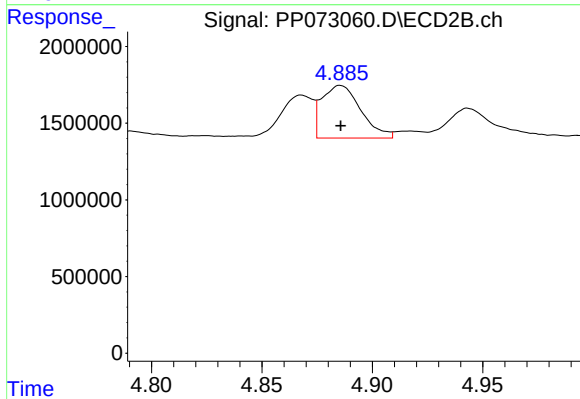

#4 AR-1016-2


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 4212716
Conc: 41.86 ng/ml

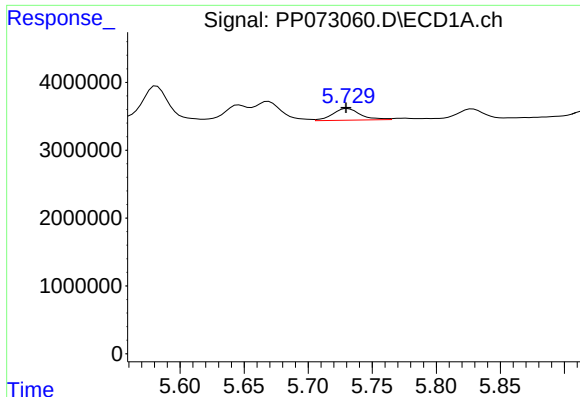

#5 AR-1016-3


R.T.: 5.731 min
Delta R.T.: 0.001 min
Response: 2596172
Conc: 39.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

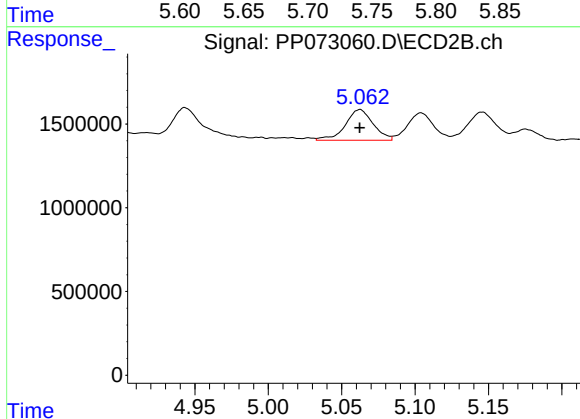


#5 AR-1016-3

R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 2423103
Conc: 44.28 ng/ml

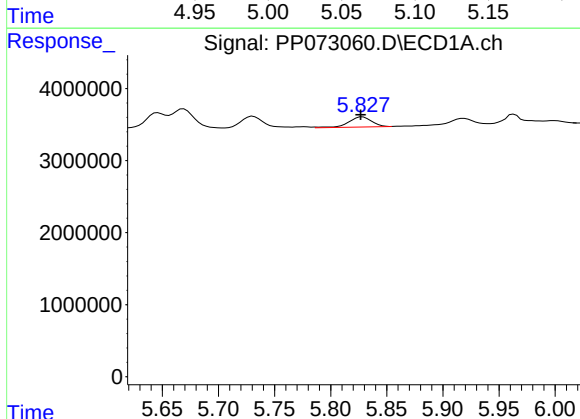


#6 AR-1016-4

R.T.: 5.828 min
Delta R.T.: 0.001 min
Response: 1976574
Conc: 37.81 ng/ml

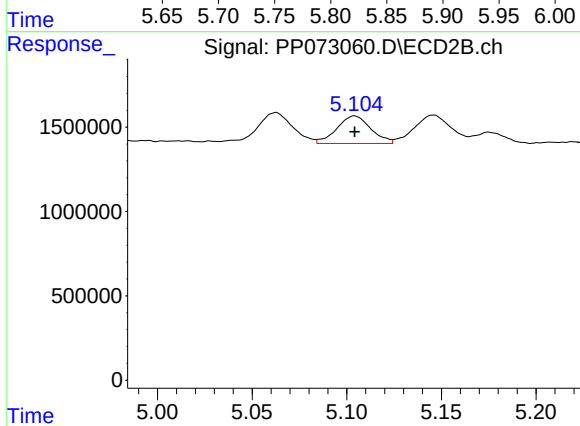

#6 AR-1016-4


R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 2039947
Conc: 45.79 ng/ml

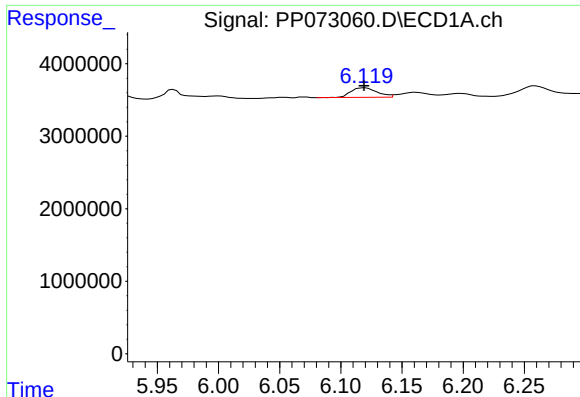

#7 AR-1016-5


R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 1951632
Conc: 39.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

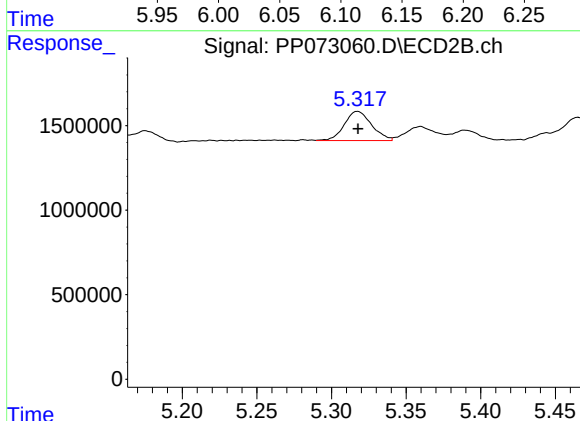


#7 AR-1016-5

R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 2188133
Conc: 39.58 ng/ml

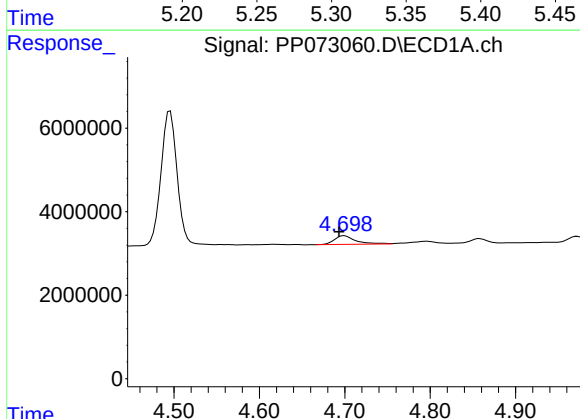


#8 AR-1221-1

R.T.: 4.700 min
Delta R.T.: 0.006 min
Response: 3602996
Conc: 146.11 ng/ml

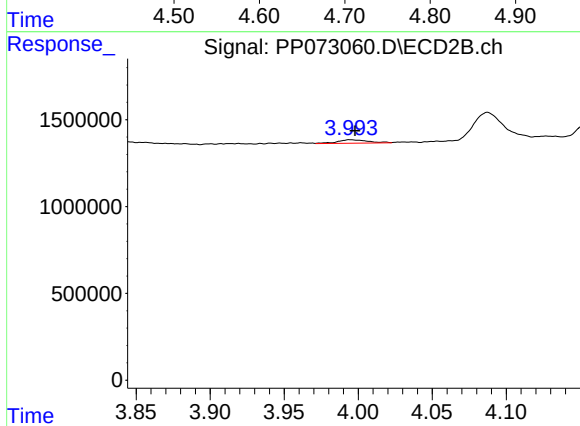

#8 AR-1221-1


R.T.: 3.995 min
Delta R.T.: -0.003 min
Response: 277975
Conc: 10.34 ng/ml

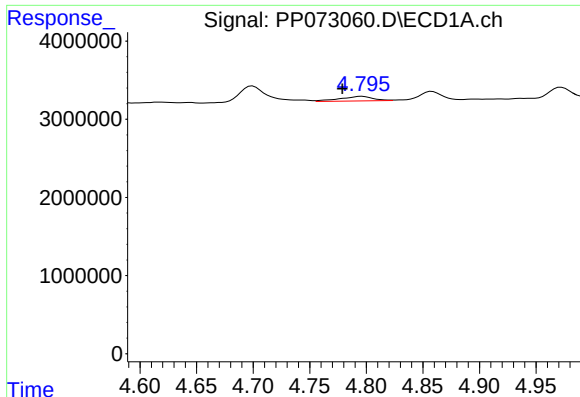

#9 AR-1221-2


R.T.: 4.796 min
Delta R.T.: 0.018 min
Response: 1167416
Conc: 57.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

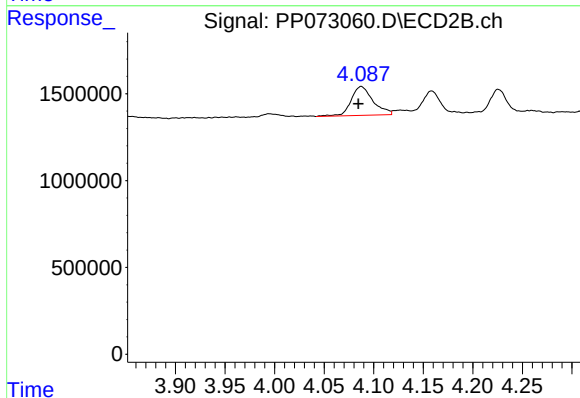


#9 AR-1221-2

R.T.: 4.087 min
Delta R.T.: 0.003 min
Response: 2573590
Conc: 127.50 ng/ml

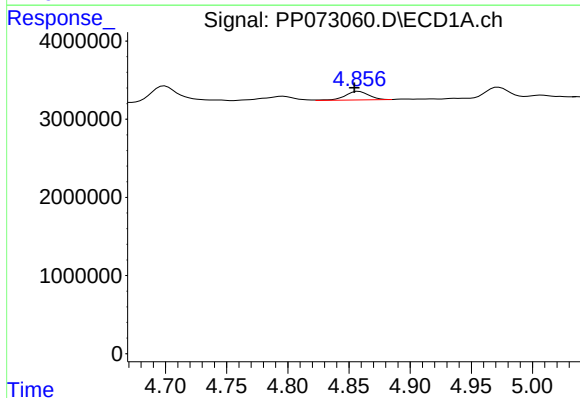


#10 AR-1221-3

R.T.: 4.858 min
Delta R.T.: 0.004 min
Response: 1467068
Conc: 23.83 ng/ml

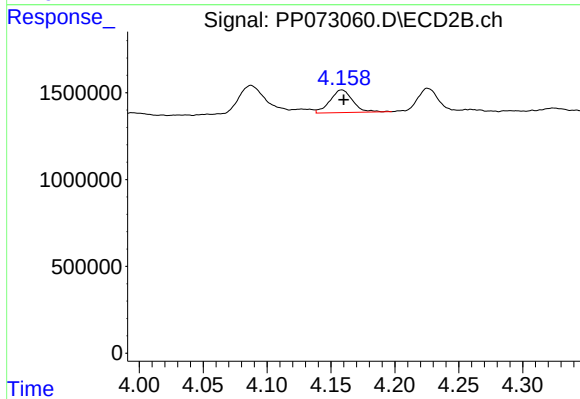

#10 AR-1221-3


R.T.: 4.158 min
Delta R.T.: -0.001 min
Response: 1612126
Conc: 27.45 ng/ml

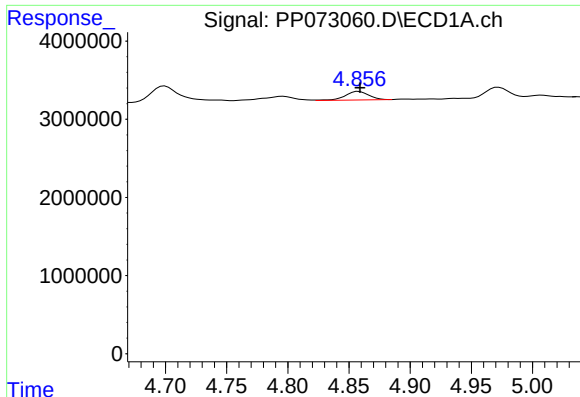

#11 AR-1232-1


R.T.: 4.858 min
Delta R.T.: -0.001 min
Response: 1467068
Conc: 31.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

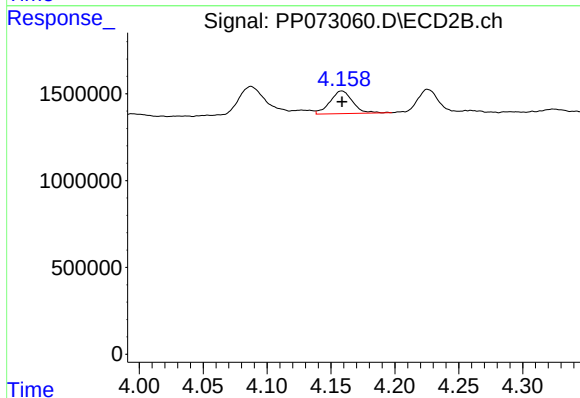


#11 AR-1232-1

R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 1612126
Conc: 35.38 ng/ml

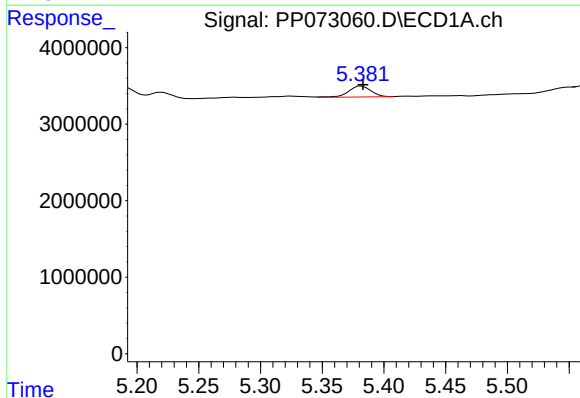


#12 AR-1232-2

R.T.: 5.382 min
Delta R.T.: -0.001 min
Response: 1796469
Conc: 80.31 ng/ml

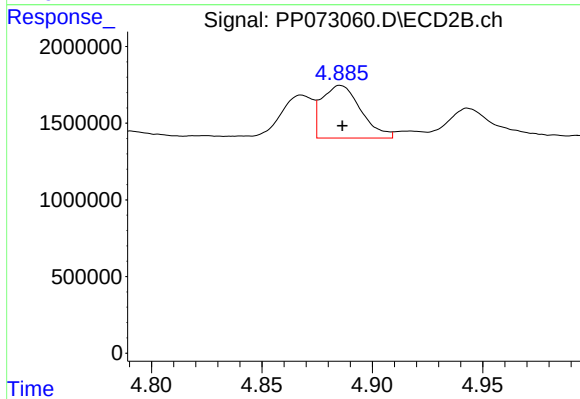

#12 AR-1232-2


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 4212716
Conc: 91.07 ng/ml

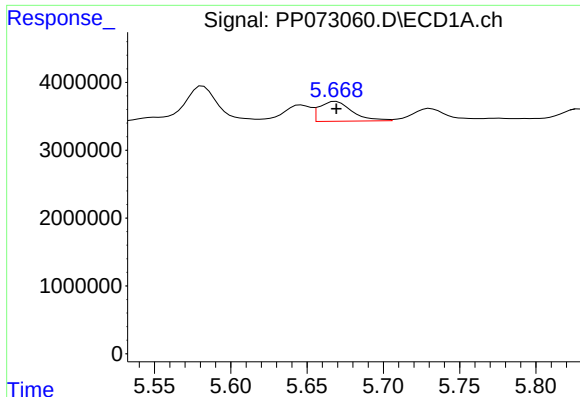

#13 AR-1232-3


R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 4375765
Conc: 84.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

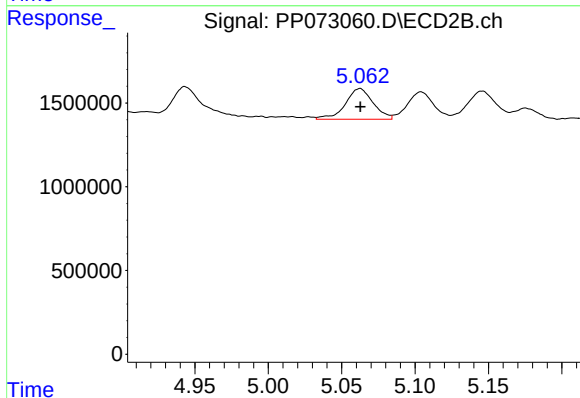


#13 AR-1232-3

R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 2423103
Conc: 98.67 ng/ml

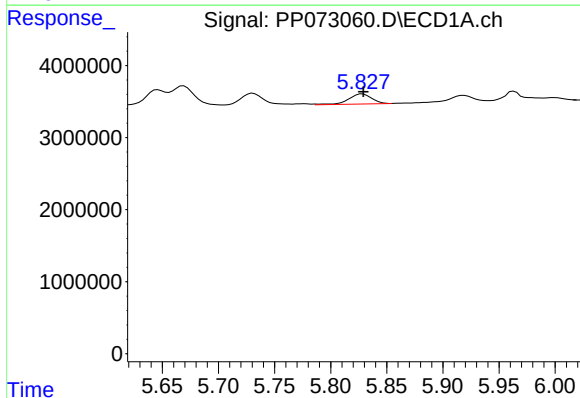


#14 AR-1232-4

R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 1976574
Conc: 76.58 ng/ml

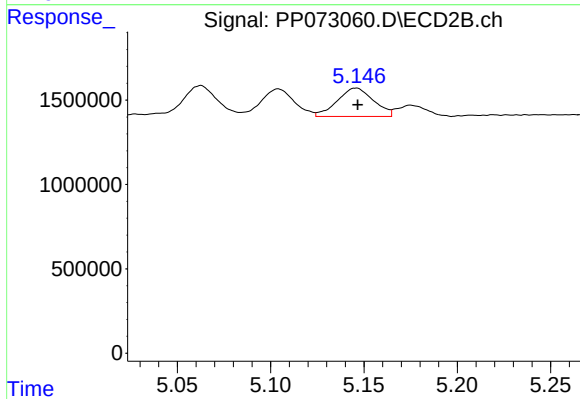

#14 AR-1232-4


R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 2283088
Conc: 105.58 ng/ml

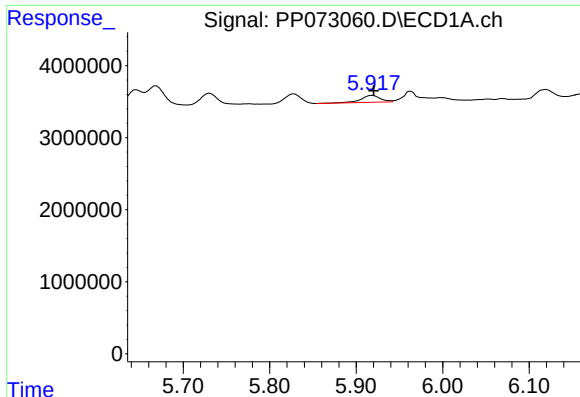

#15 AR-1232-5


R.T.: 5.919 min
Delta R.T.: -0.002 min
Response: 1520245
Conc: 42.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

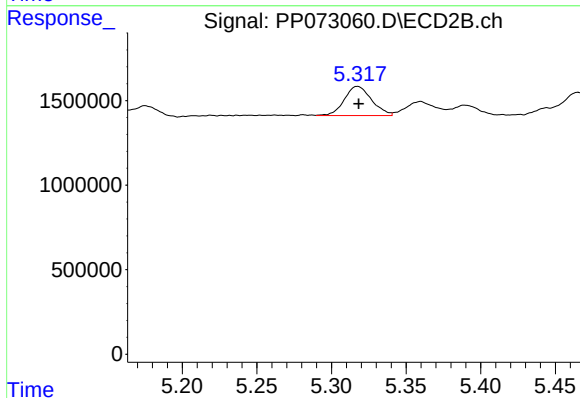


#15 AR-1232-5

R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 2188133
Conc: 95.72 ng/ml

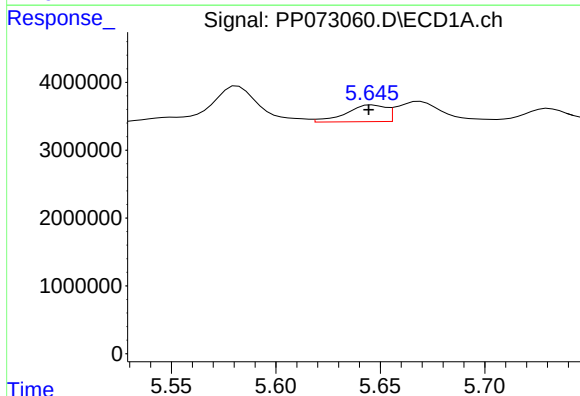


#16 AR-1242-1

R.T.: 5.646 min
Delta R.T.: 0.002 min
Response: 3274633
Conc: 56.04 ng/ml

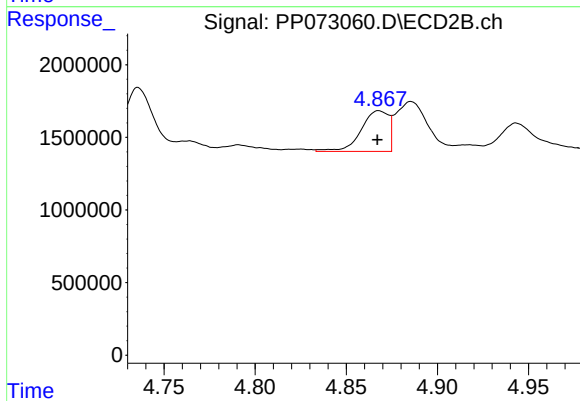

#16 AR-1242-1


R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 2954527
Conc: 53.51 ng/ml

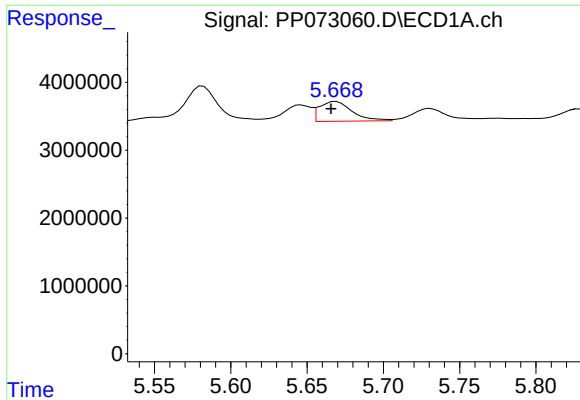

#17 AR-1242-2


R.T.: 5.669 min
Delta R.T.: 0.003 min
Response: 4375765
Conc: 50.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

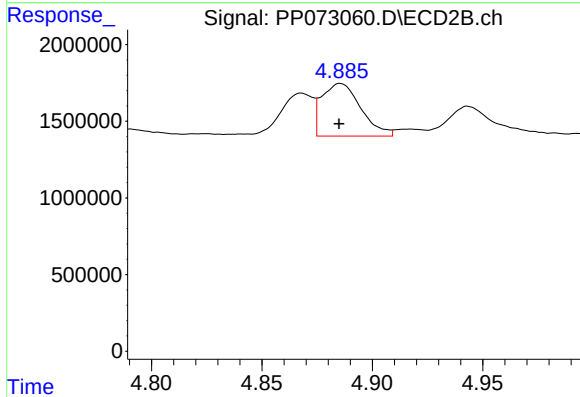


#17 AR-1242-2

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 4212716
Conc: 53.00 ng/ml

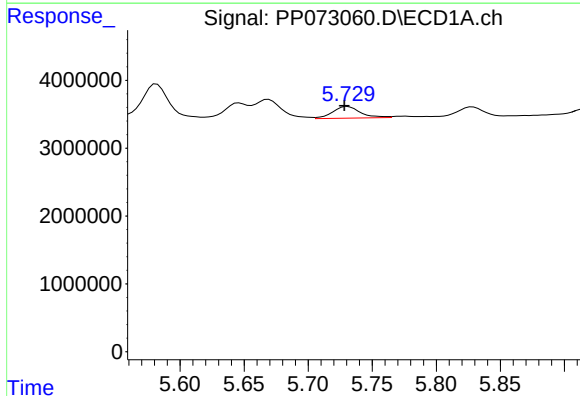


#18 AR-1242-3

R.T.: 5.731 min
Delta R.T.: 0.002 min
Response: 2596172
Conc: 49.26 ng/ml

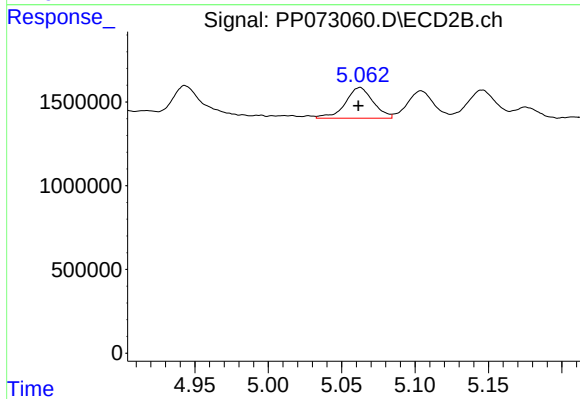

#18 AR-1242-3


R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 2423103
Conc: 55.95 ng/ml

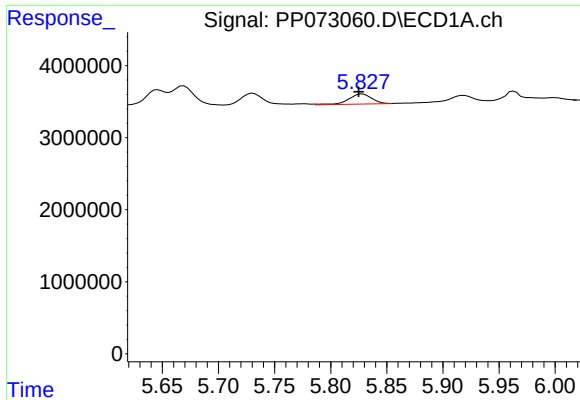

#19 AR-1242-4


R.T.: 5.828 min
Delta R.T.: 0.003 min
Response: 1976574
Conc: 44.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

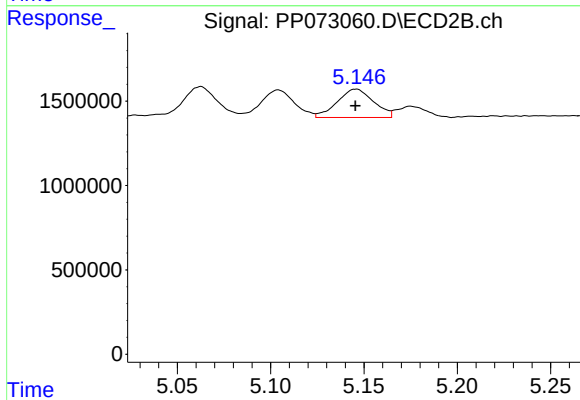


#19 AR-1242-4

R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 2283088
Conc: 55.01 ng/ml

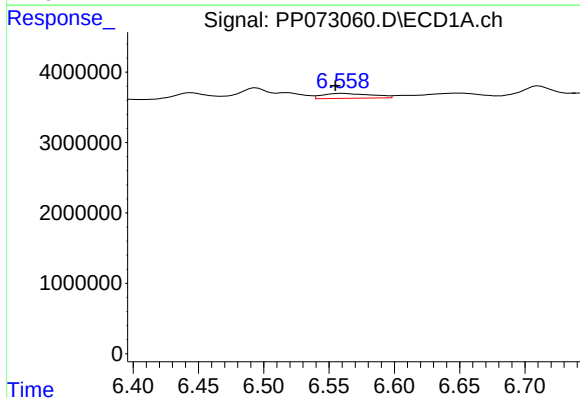


#20 AR-1242-5

R.T.: 6.560 min
Delta R.T.: 0.005 min
Response: 1801915
Conc: 36.36 ng/ml

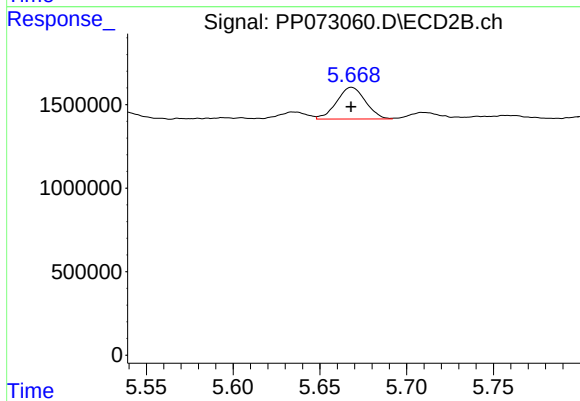

#20 AR-1242-5


R.T.: 5.668 min
Delta R.T.: 0.000 min
Response: 2203363
Conc: 41.90 ng/ml

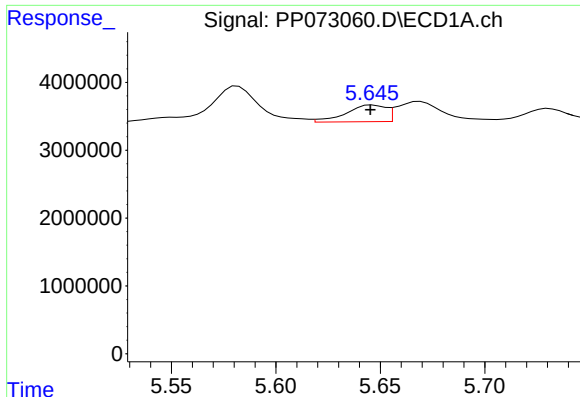

#21 AR-1248-1


R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 3274633
Conc: 68.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

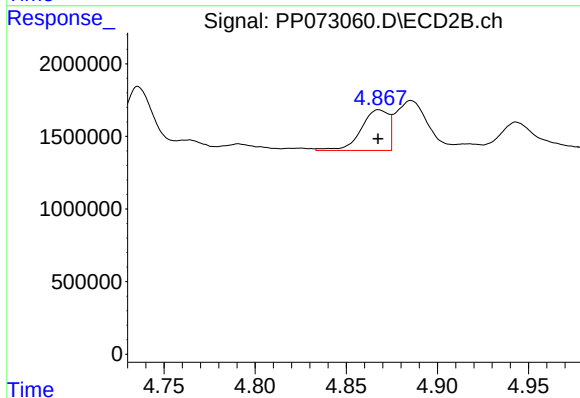


#21 AR-1248-1

R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 2954527
Conc: 67.78 ng/ml

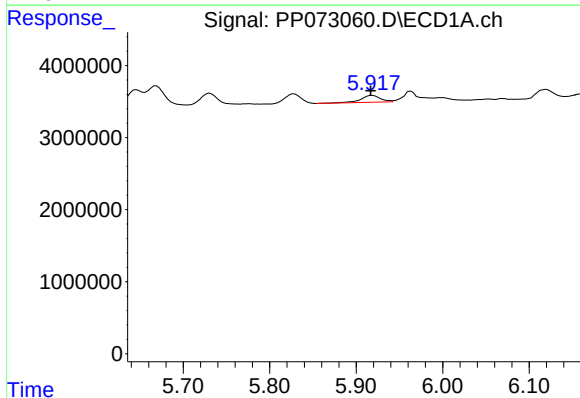


#22 AR-1248-2

R.T.: 5.919 min
Delta R.T.: 0.002 min
Response: 1520245
Conc: 25.96 ng/ml

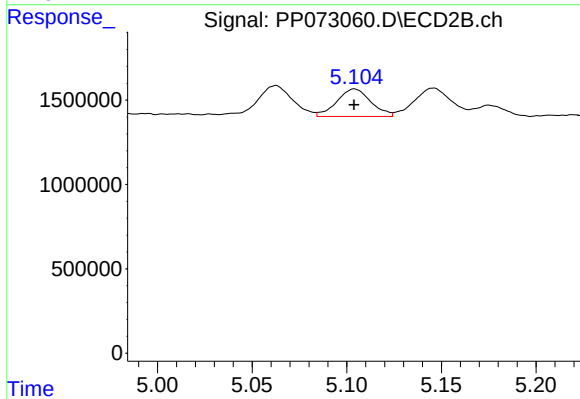

#22 AR-1248-2


R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 2039947
Conc: 34.81 ng/ml

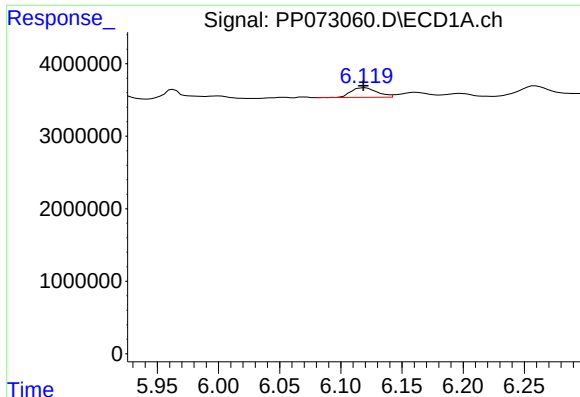

#23 AR-1248-3


R.T.: 6.120 min
Delta R.T.: 0.001 min
Response: 1951632
Conc: 29.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

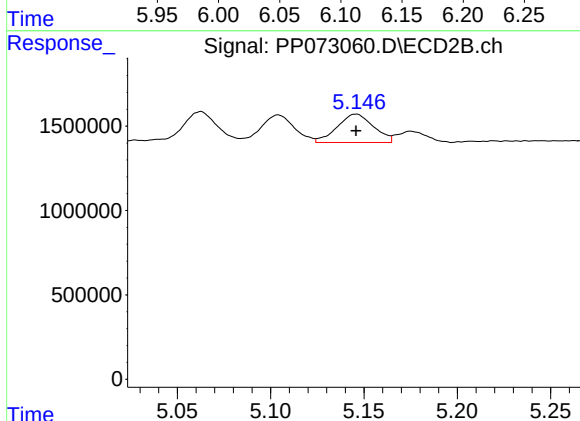


#23 AR-1248-3

R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 2283088
Conc: 37.71 ng/ml

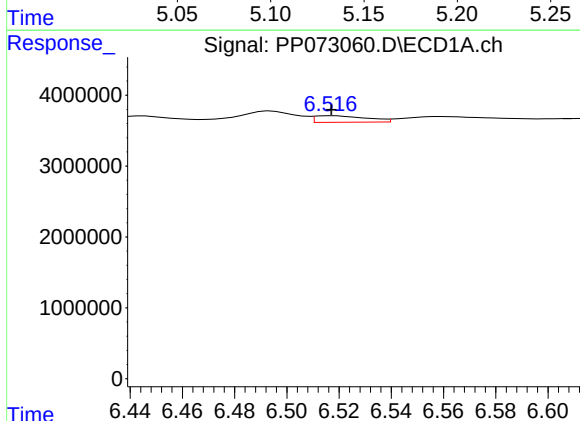


#24 AR-1248-4

R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 1250635
Conc: 14.70 ng/ml

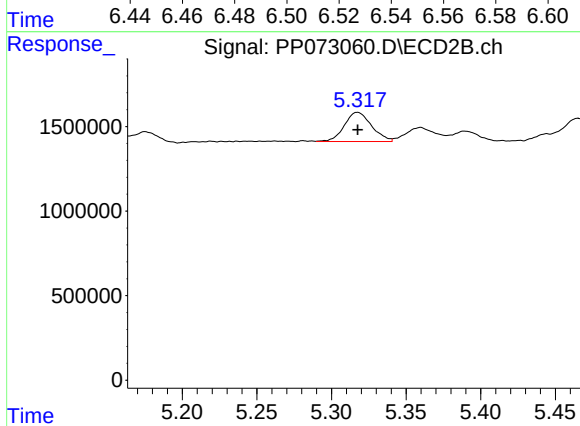

#24 AR-1248-4


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 2188133
Conc: 31.25 ng/ml

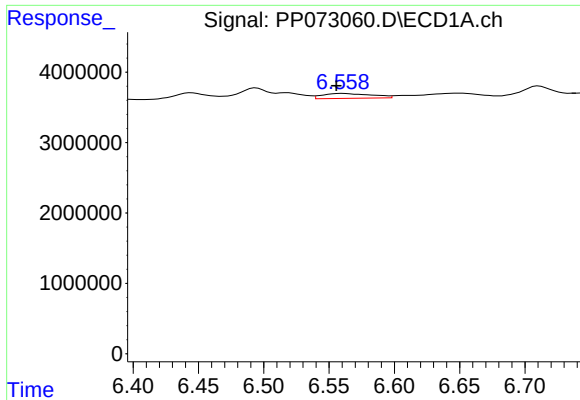

#25 AR-1248-5


R.T.: 6.560 min
Delta R.T.: 0.004 min
Response: 1801915
Conc: 21.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

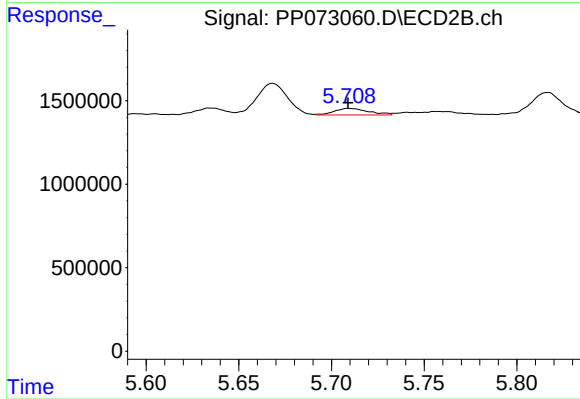


#25 AR-1248-5

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 509730
Conc: 7.18 ng/ml

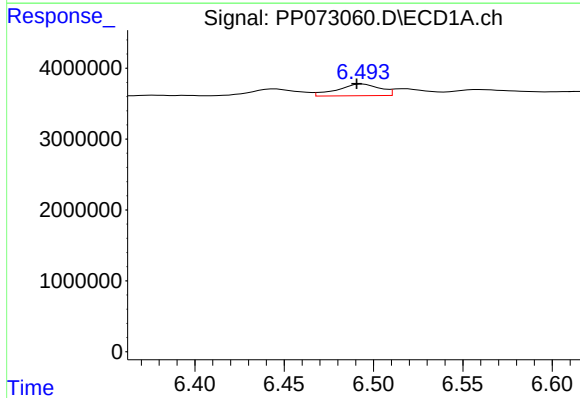


#26 AR-1254-1

R.T.: 6.494 min
Delta R.T.: 0.003 min
Response: 2726927
Conc: 32.40 ng/ml

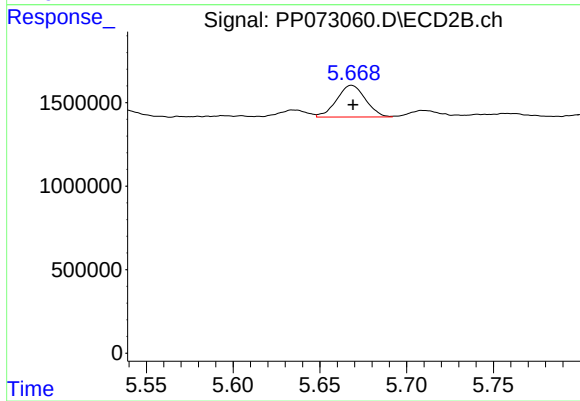

#26 AR-1254-1


R.T.: 5.668 min
Delta R.T.: 0.000 min
Response: 2203363
Conc: 20.09 ng/ml

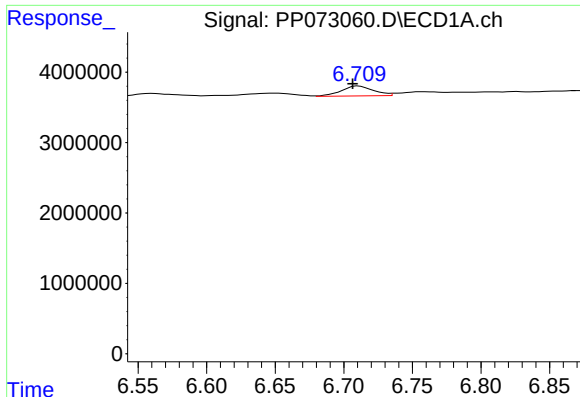

#27 AR-1254-2


R.T.: 6.711 min
Delta R.T.: 0.004 min
Response: 2297205
Conc: 18.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

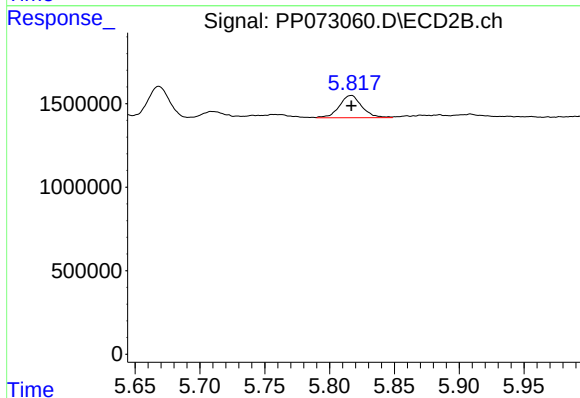


#27 AR-1254-2

R.T.: 5.817 min
Delta R.T.: 0.000 min
Response: 1616668
Conc: 17.10 ng/ml

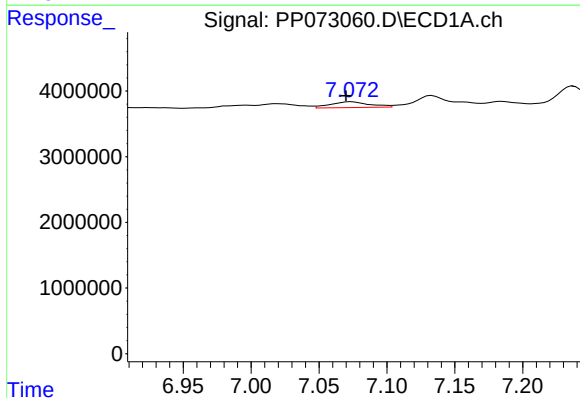


#28 AR-1254-3

R.T.: 7.074 min
Delta R.T.: 0.004 min
Response: 1753915
Conc: 13.37 ng/ml

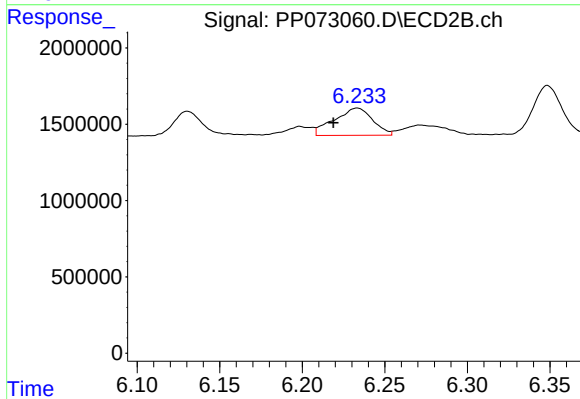

#28 AR-1254-3


R.T.: 6.233 min
Delta R.T.: 0.014 min
Response: 2881056
Conc: 19.53 ng/ml

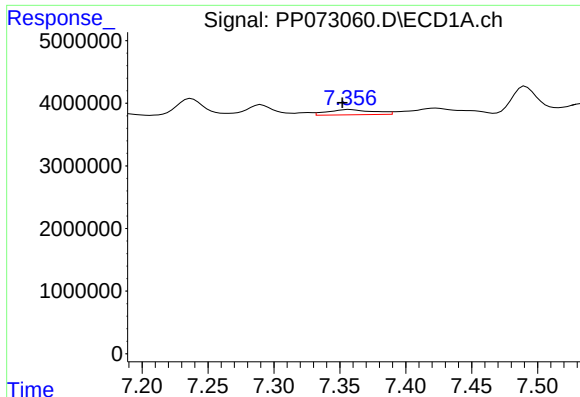

#29 AR-1254-4


R.T.: 7.358 min
Delta R.T.: 0.005 min
Response: 2008052
Conc: 16.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

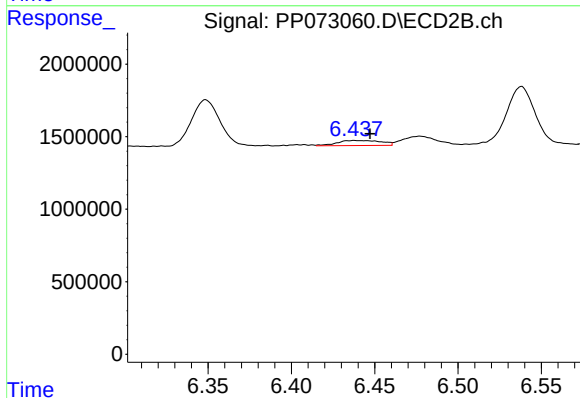


#29 AR-1254-4

R.T.: 6.438 min
Delta R.T.: -0.009 min
Response: 646749
Conc: 6.66 ng/ml

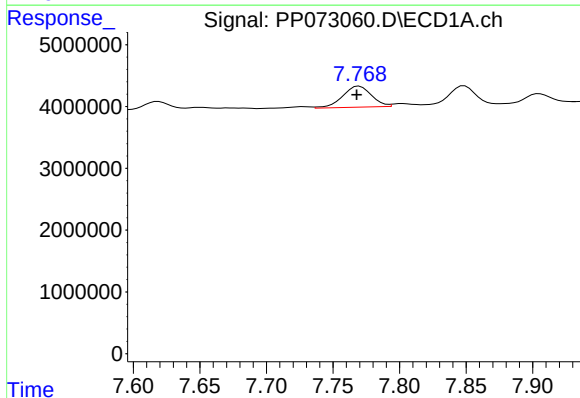


#30 AR-1254-5

R.T.: 7.770 min
Delta R.T.: 0.002 min
Response: 5163614
Conc: 45.19 ng/ml

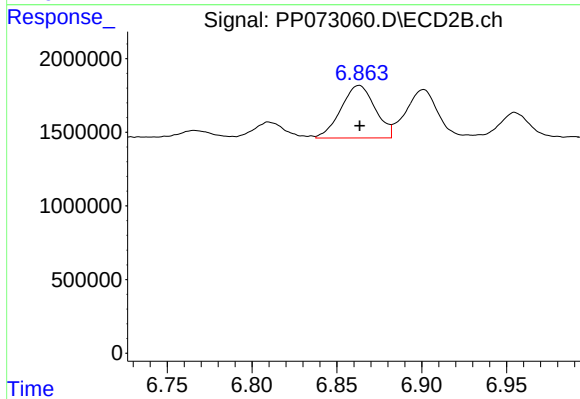

#30 AR-1254-5


R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 5007390
Conc: 38.53 ng/ml

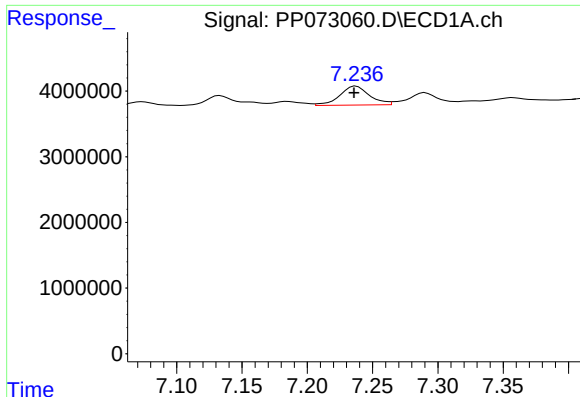

#31 AR-1260-1


R.T.: 7.237 min
Delta R.T.: 0.001 min
Response: 4573467
Conc: 51.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

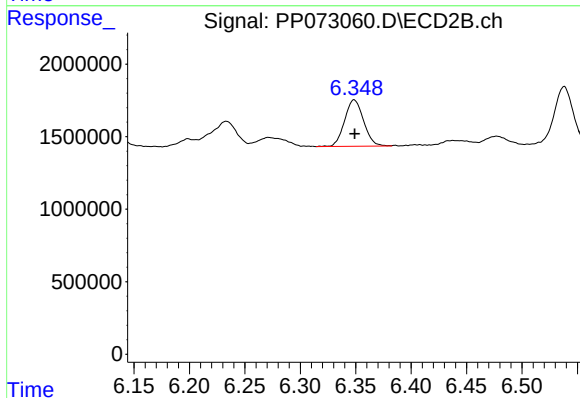


#31 AR-1260-1

R.T.: 6.349 min
Delta R.T.: 0.000 min
Response: 3837031
Conc: 40.50 ng/ml

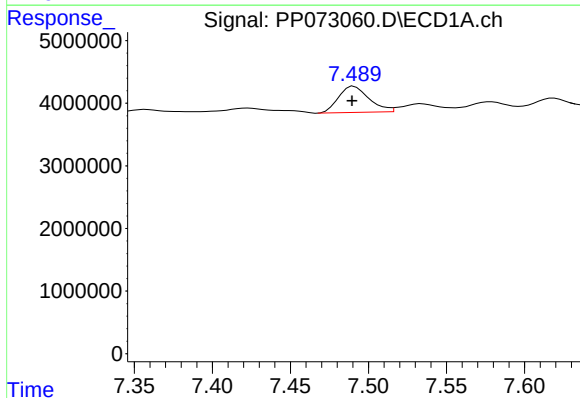


#32 AR-1260-2

R.T.: 7.491 min
Delta R.T.: 0.002 min
Response: 5693038
Conc: 41.90 ng/ml

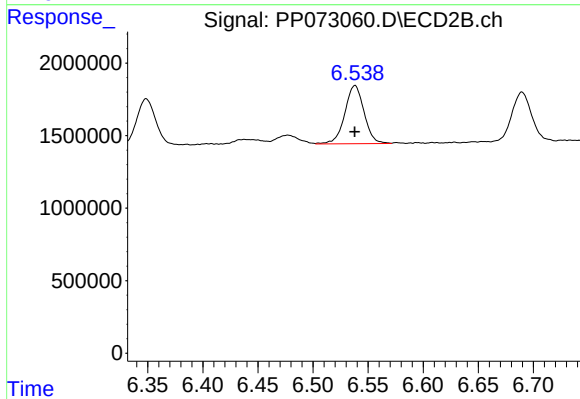

#32 AR-1260-2


R.T.: 6.538 min
Delta R.T.: 0.000 min
Response: 4880115
Conc: 41.91 ng/ml

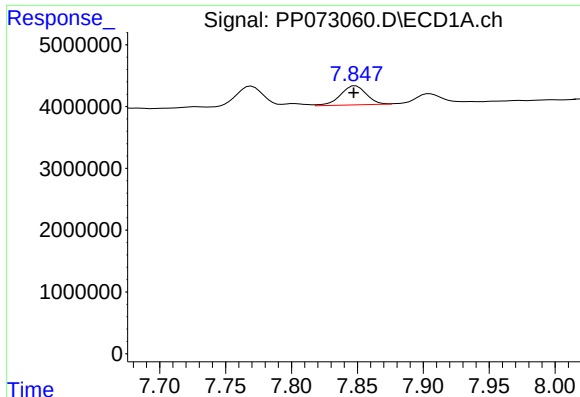

#33 AR-1260-3


R.T.: 7.849 min
Delta R.T.: 0.001 min
Response: 4212387
Conc: 36.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

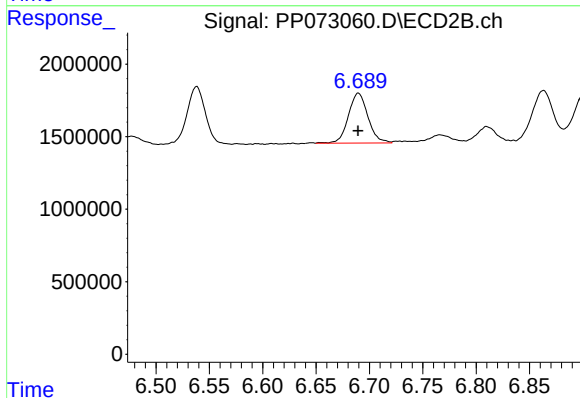


#33 AR-1260-3

R.T.: 6.690 min
Delta R.T.: 0.000 min
Response: 4375961
Conc: 42.01 ng/ml

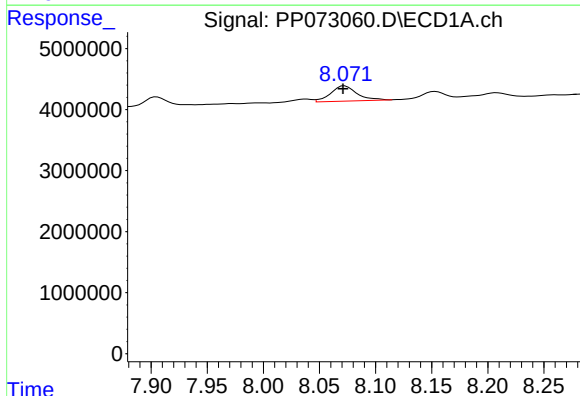


#34 AR-1260-4

R.T.: 8.073 min
Delta R.T.: 0.002 min
Response: 4105552
Conc: 39.84 ng/ml

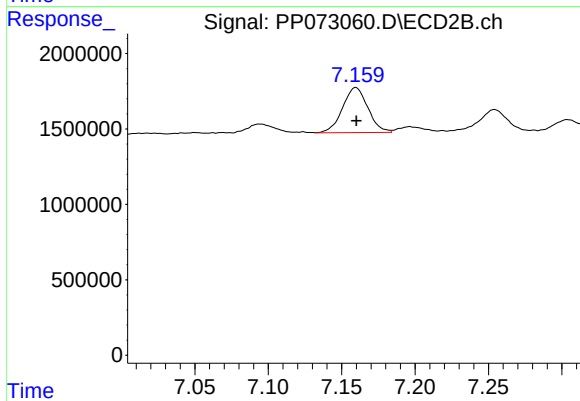

#34 AR-1260-4


R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 3589972
Conc: 40.92 ng/ml

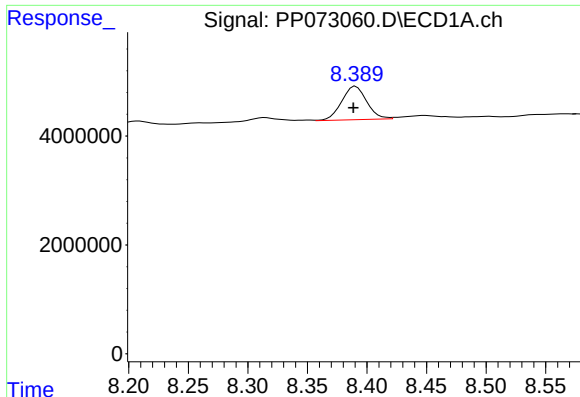

#35 AR-1260-5


R.T.: 8.391 min
Delta R.T.: 0.002 min
Response: 9004036
Conc: 37.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

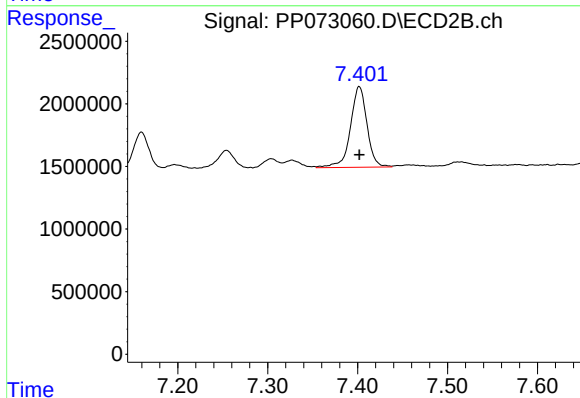


#35 AR-1260-5

R.T.: 7.402 min
Delta R.T.: 0.000 min
Response: 8264153
Conc: 38.73 ng/ml

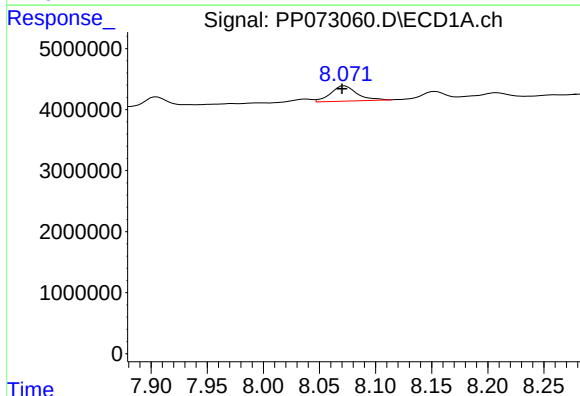


#36 AR-1262-1

R.T.: 8.073 min
Delta R.T.: 0.002 min
Response: 4105552
Conc: 27.74 ng/ml

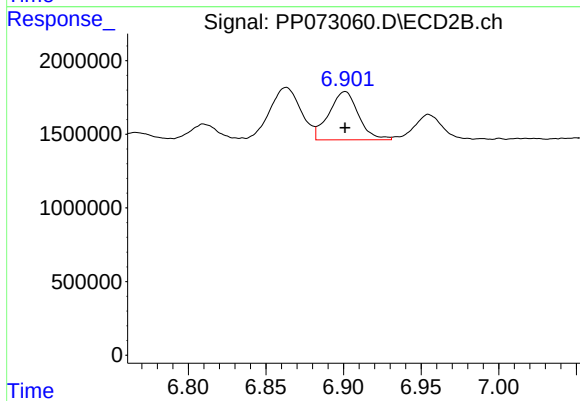

#36 AR-1262-1


R.T.: 6.901 min
Delta R.T.: 0.000 min
Response: 4338348
Conc: 30.03 ng/ml

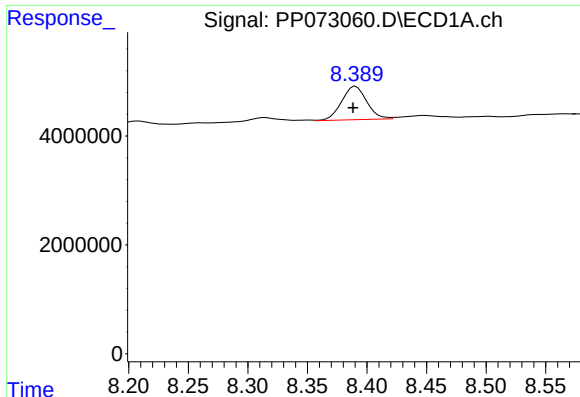

#37 AR-1262-2


R.T.: 8.391 min
Delta R.T.: 0.002 min
Response: 9004036
Conc: 28.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

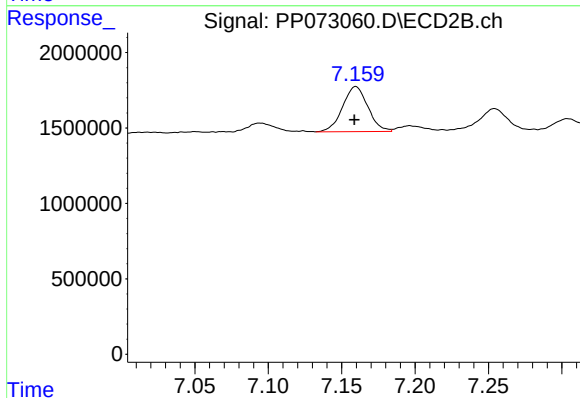


#37 AR-1262-2

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 3589972
Conc: 29.37 ng/ml

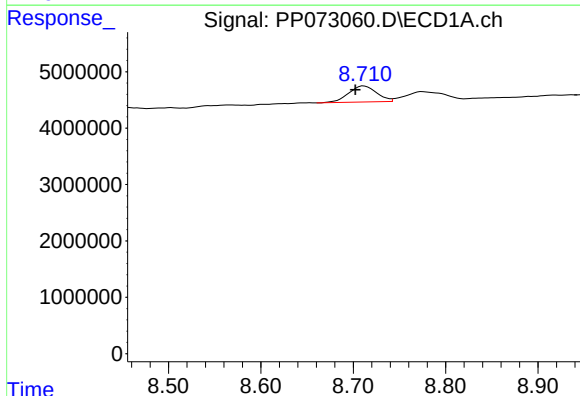


#38 AR-1262-3

R.T.: 8.711 min
Delta R.T.: 0.009 min
Response: 5963152
Conc: 27.87 ng/ml

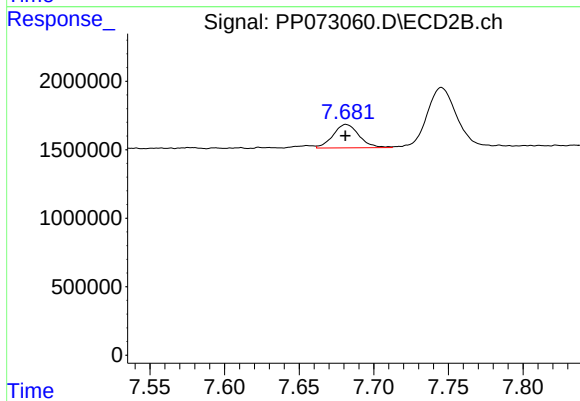

#38 AR-1262-3


R.T.: 7.682 min
Delta R.T.: 0.000 min
Response: 2080723
Conc: 18.46 ng/ml

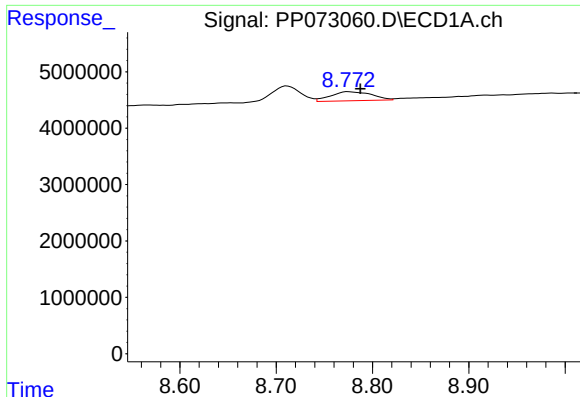

#39 AR-1262-4


R.T.: 8.775 min
Delta R.T.: -0.013 min
Response: 4742356
Conc: 30.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

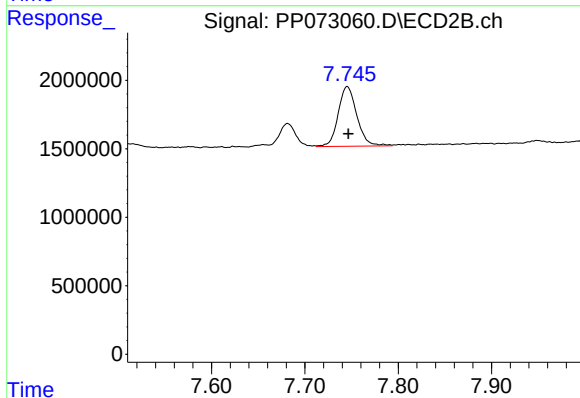


#39 AR-1262-4

R.T.: 7.745 min
Delta R.T.: -0.001 min
Response: 6064617
Conc: 33.08 ng/ml

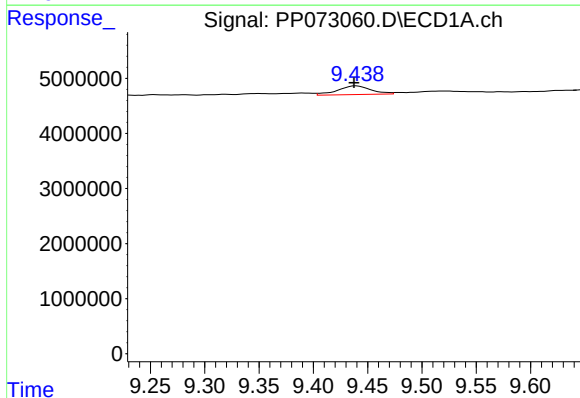


#40 AR-1262-5

R.T.: 9.440 min
Delta R.T.: 0.002 min
Response: 3450909
Conc: 30.85 ng/ml

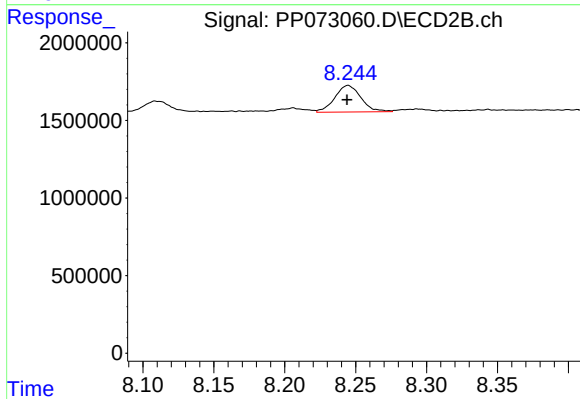

#40 AR-1262-5


R.T.: 8.245 min
Delta R.T.: 0.000 min
Response: 2209895
Conc: 25.52 ng/ml

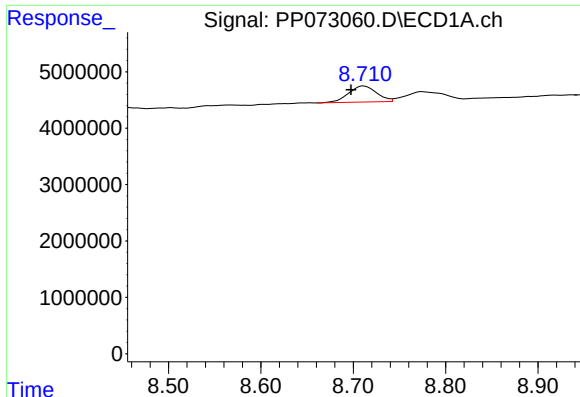

#41 AR-1268-1


R.T.: 8.711 min
Delta R.T.: 0.014 min
Response: 5963152
Conc: 16.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

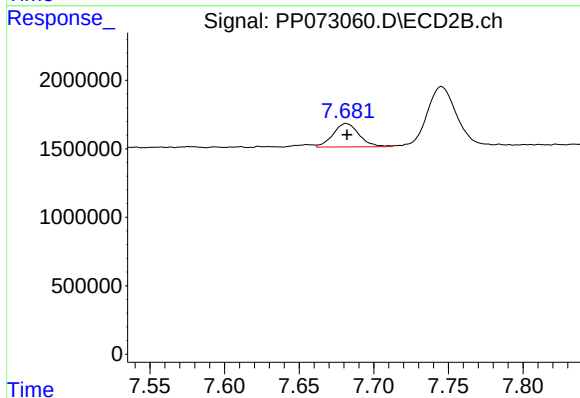


#41 AR-1268-1

R.T.: 7.682 min
Delta R.T.: 0.000 min
Response: 2080723
Conc: 7.24 ng/ml

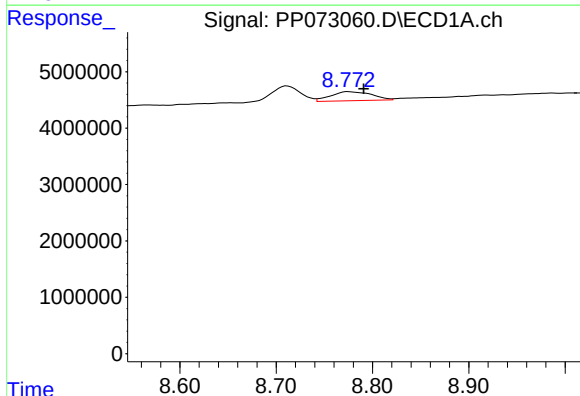


#42 AR-1268-2

R.T.: 8.775 min
Delta R.T.: -0.016 min
Response: 4742356
Conc: 15.55 ng/ml

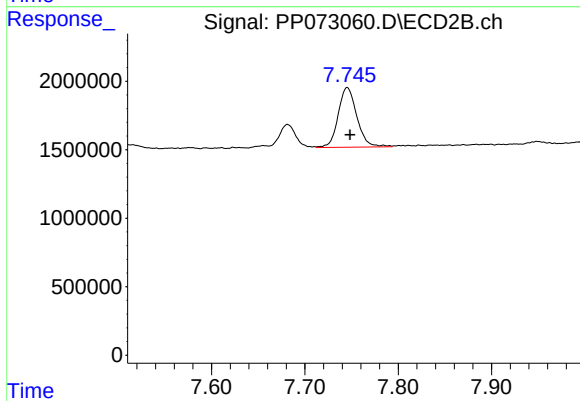

#42 AR-1268-2


R.T.: 7.745 min
Delta R.T.: -0.003 min
Response: 6064617
Conc: 23.59 ng/ml

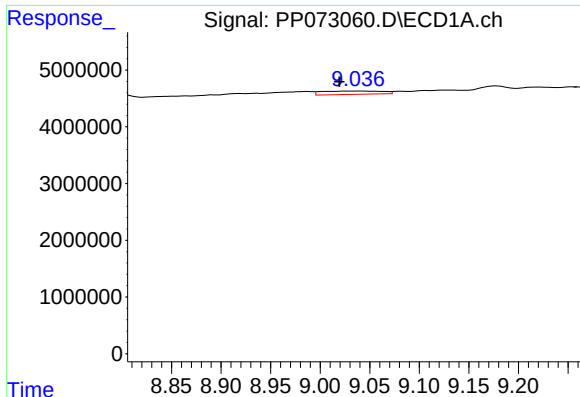

#43 AR-1268-3


R.T.: 9.036 min
Delta R.T.: 0.017 min
Response: 2528998
Conc: 9.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

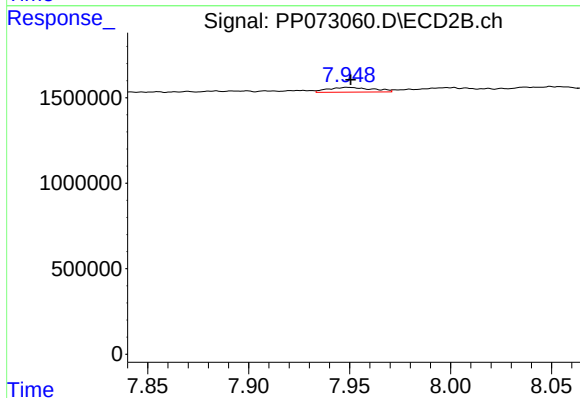


#43 AR-1268-3

R.T.: 7.949 min
Delta R.T.: -0.001 min
Response: 423708
Conc: 1.96 ng/ml

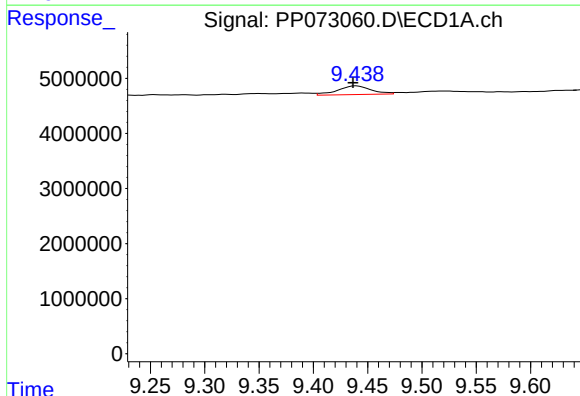


#44 AR-1268-4

R.T.: 9.440 min
Delta R.T.: 0.003 min
Response: 3450909
Conc: 29.49 ng/ml

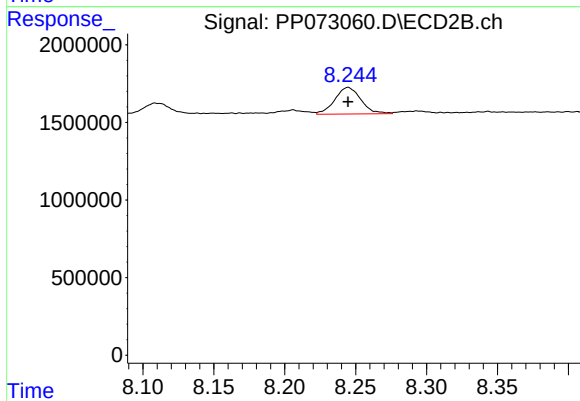

#44 AR-1268-4


R.T.: 8.245 min
Delta R.T.: 0.000 min
Response: 2209895
Conc: 23.46 ng/ml

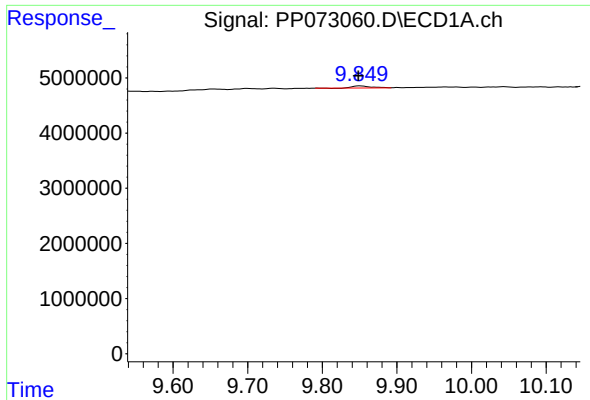

#45 AR-1268-5

R.T.: 9.851 min
Delta R.T.: 0.002 min
Response: 589885
Conc: 0.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

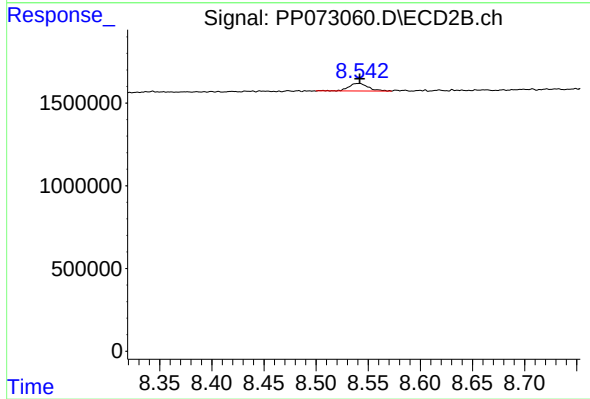

#45 AR-1268-5

R.T.: 8.541 min
Delta R.T.: 0.000 min
Response: 600286
Conc: 1.04 ng/ml