

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
 Data File : PP073061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 23:03
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:42:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.491	3.789	42284667	36016729	20.032	19.989
2)	SA Decachlor...	10.185	8.798	38364343	30488714	22.450	22.843
Target Compounds							
3)	L1 AR-1016-1	5.665	4.869	1390324	258662	19.132	3.764 #
4)	L1 AR-1016-2	5.665	4.887	1390324	319751	13.366	3.177 #
5)	L1 AR-1016-3	5.722	5.061	433613	300554	6.635	5.493
6)	L1 AR-1016-4	5.830	5.106	371079	351336	7.098	7.886
7)	L1 AR-1016-5	6.125	5.316	185582	328547	3.711	5.943 #
8)	L2 AR-1221-1	4.694	3.998	1008127	948086	40.882	35.281
9)	L2 AR-1221-2	4.790	4.087	1697303	1247264	84.112	61.790 #
10)	L2 AR-1221-3	4.854	4.160	2294164	2348982	37.272	39.995
11)	L3 AR-1232-1	4.854	4.160	2294164	2348982	48.858	51.553
12)	L3 AR-1232-2	5.377	4.887	331133	319751	14.803	6.912 #
13)	L3 AR-1232-3	5.665	5.061	1390324	300554	26.946	12.239 #
14)	L3 AR-1232-4	5.830	5.147	371079	302054	14.377	13.968
15)	L3 AR-1232-5	5.942	5.316	313177	328547	8.780	14.373 #
16)	L4 AR-1242-1	5.665	4.869	1390324	258662	23.792	4.684 #
17)	L4 AR-1242-2	5.665	4.887	1390324	319751	16.063	4.023 #
18)	L4 AR-1242-3	5.722	5.061	433613	300554	8.227	6.940
19)	L4 AR-1242-4	5.830	5.147	371079	302054	8.442	7.278
20)	L4 AR-1242-5	6.574	5.668	2758026	247285	55.651	4.702 #
21)	L5 AR-1248-1	5.665	4.869	1390324	258662	29.228	5.934 #
22)	L5 AR-1248-2	5.892	5.106	256731	351336	4.385	5.996 #
23)	L5 AR-1248-3	6.125	5.147	185582	302054	2.844	4.989 #
24)	L5 AR-1248-4	6.516	5.316	1638251	328547	19.259	4.692 #
25)	L5 AR-1248-5	6.574	5.731	2758026	198249	32.954	2.791 #
26)	L6 AR-1254-1	6.482	5.668	1341370	247285	15.936	2.255 #
27)	L6 AR-1254-2	6.754f	5.814	4851005	156327	38.684	1.653 #
28)	L6 AR-1254-3	7.068	6.233	4930904	160666	37.580	1.089 #
29)	L6 AR-1254-4	7.357	6.433	3537310	496289	29.531	5.111 #
30)	L6 AR-1254-5	7.767	6.883	736437	140128	6.445	1.078 #
31)	L7 AR-1260-1	7.255	6.333	2555685	94803	28.972	1.001 #
32)	L7 AR-1260-2	7.523	6.520	3191556	794371	23.487	6.822 #
33)	L7 AR-1260-3	7.819	6.693	1025707	193707	8.985	1.860 #
34)	L7 AR-1260-4	8.027f	7.164	374011	110849	3.630	1.263 #
35)	L7 AR-1260-5	8.360	7.416	56990	279667	0.237	1.311 #
36)	L8 AR-1262-1	8.027f	6.913	374011	207327	2.527	1.435 #
37)	L8 AR-1262-2	8.360	7.164	56990	110849	0.180	0.907 #
38)	L8 AR-1262-3	8.714	7.695	399885	199984	1.869	1.774
39)	L8 AR-1262-4	8.762	7.771	994791	278749	6.312	1.520 #
40)	L8 AR-1262-5	9.441	8.238	350036	167985	3.129	1.940 #
41)	L9 AR-1268-1	8.714	7.695	399885	199984	1.118	0.696 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
 Data File : PP073061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 23:03
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:42:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.762	7.771	994791	278749	3.261	1.084 #
43) L9	AR-1268-3	9.022	7.959	719300	452521	2.709	2.096
44) L9	AR-1268-4	9.441	8.238	350036	167985	2.991	1.784 #
45) L9	AR-1268-5	9.856	8.541	119726	202392	0.162	0.350 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
Data File : PP073061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 23:03
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:42:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

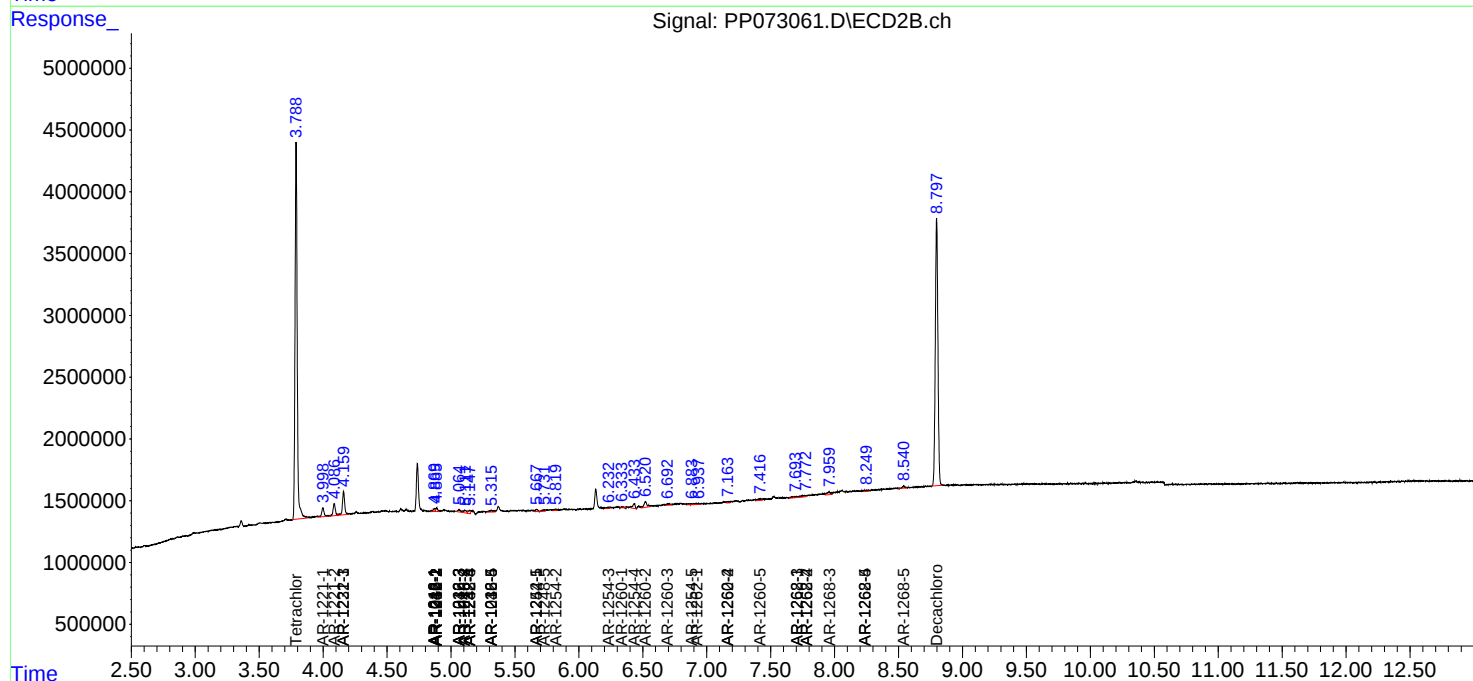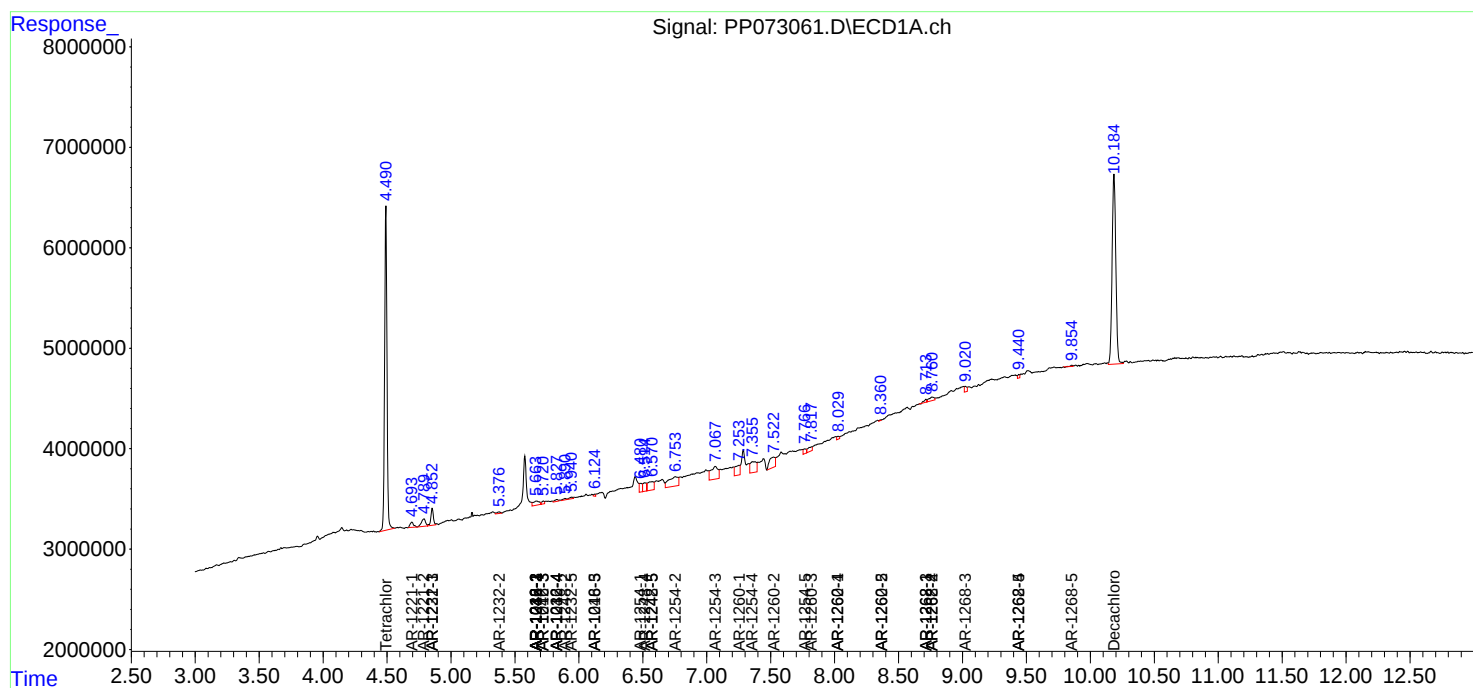


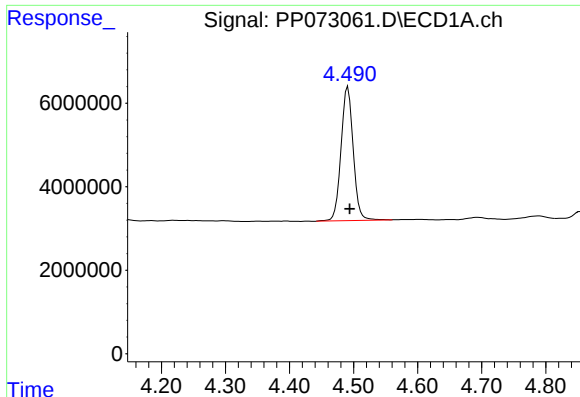

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: -0.003 min
Response: 42284667
Conc: 20.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

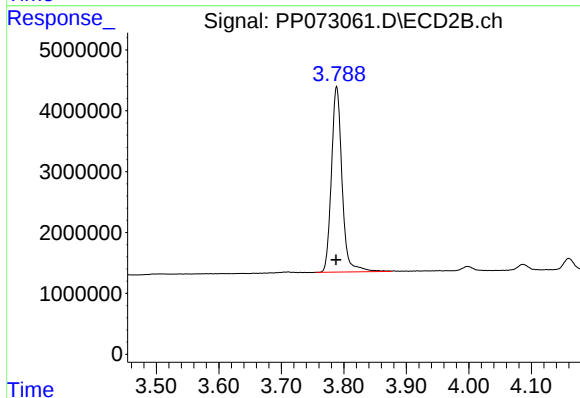


#1 Tetrachloro-m-xylene

R.T.: 3.789 min
Delta R.T.: 0.000 min
Response: 36016729
Conc: 19.99 ng/ml

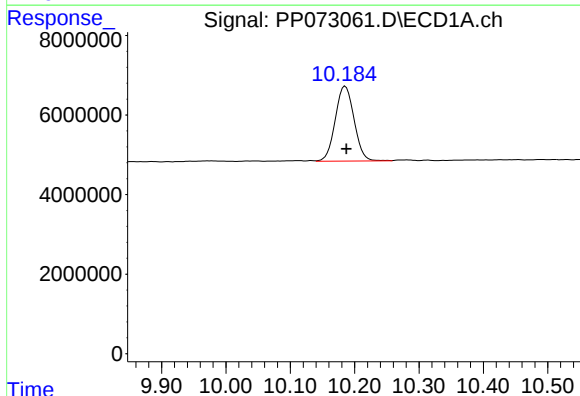


#2 Decachlorobiphenyl

R.T.: 10.185 min
Delta R.T.: -0.002 min
Response: 38364343
Conc: 22.45 ng/ml

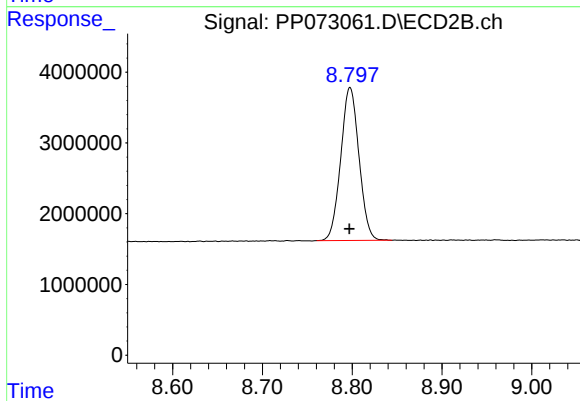

#2 Decachlorobiphenyl


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 30488714
Conc: 22.84 ng/ml

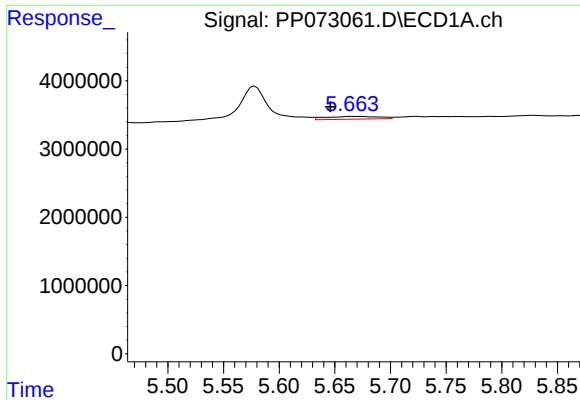

#3 AR-1016-1


R.T.: 5.665 min
Delta R.T.: 0.019 min
Response: 1390324
Conc: 19.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

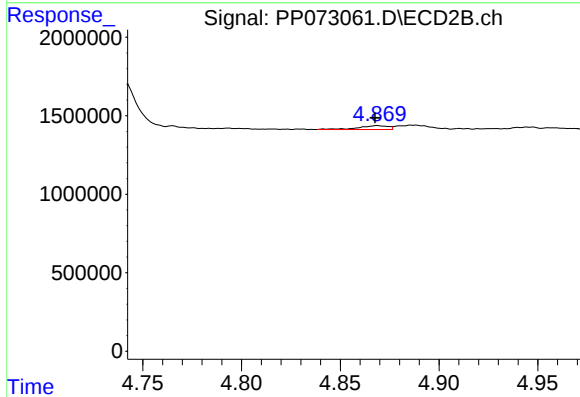


#3 AR-1016-1

R.T.: 4.869 min
Delta R.T.: 0.001 min
Response: 258662
Conc: 3.76 ng/ml

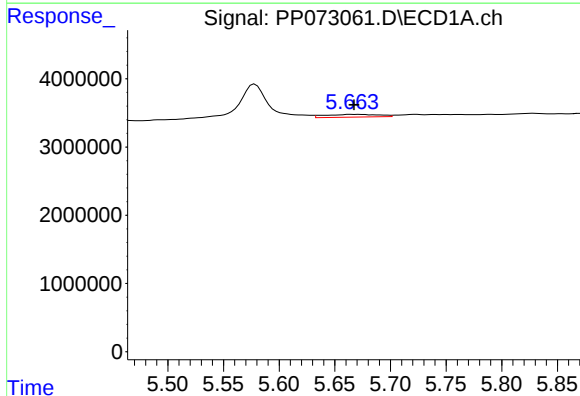


#4 AR-1016-2

R.T.: 5.665 min
Delta R.T.: -0.003 min
Response: 1390324
Conc: 13.37 ng/ml

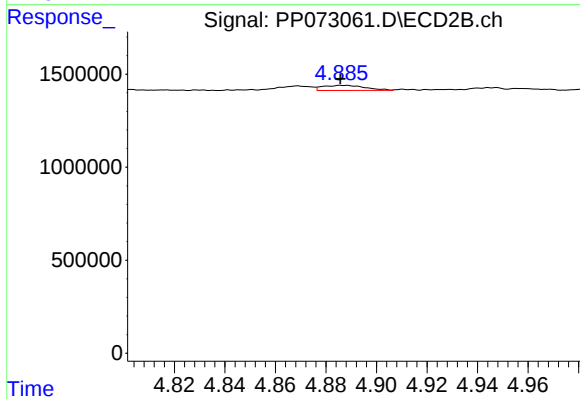

#4 AR-1016-2


R.T.: 4.887 min
Delta R.T.: 0.001 min
Response: 319751
Conc: 3.18 ng/ml

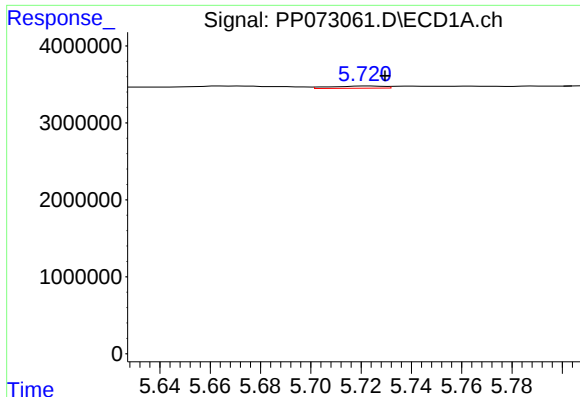

#5 AR-1016-3


R.T.: 5.722 min
Delta R.T.: -0.007 min
Response: 433613
Conc: 6.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

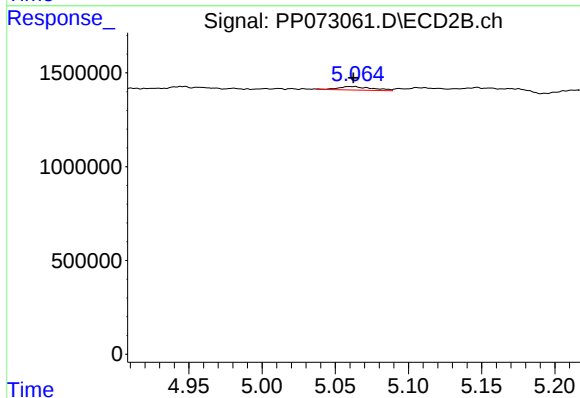


#5 AR-1016-3

R.T.: 5.061 min
Delta R.T.: -0.002 min
Response: 300554
Conc: 5.49 ng/ml

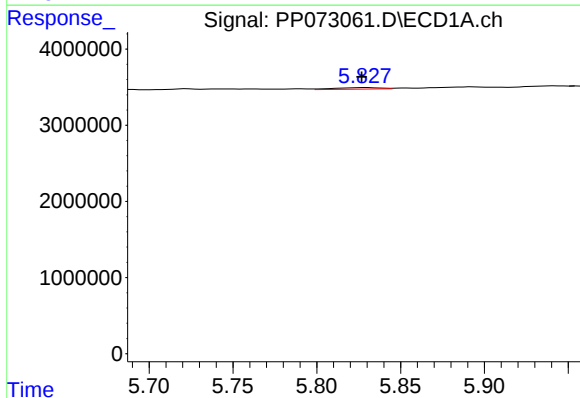


#6 AR-1016-4

R.T.: 5.830 min
Delta R.T.: 0.003 min
Response: 371079
Conc: 7.10 ng/ml

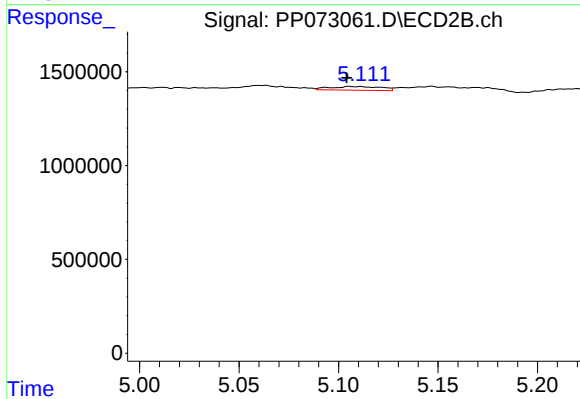

#6 AR-1016-4


R.T.: 5.106 min
Delta R.T.: 0.002 min
Response: 351336
Conc: 7.89 ng/ml

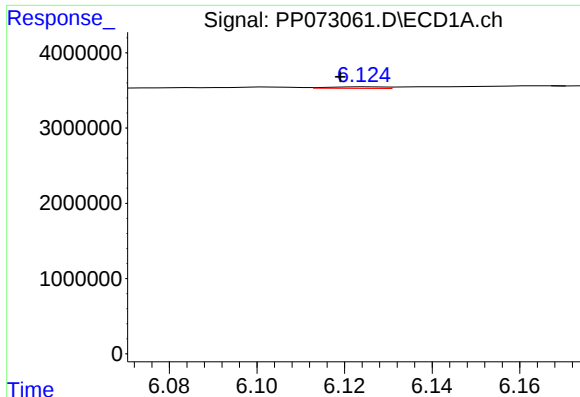

#7 AR-1016-5


R.T.: 6.125 min
Delta R.T.: 0.006 min
Response: 185582
Conc: 3.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

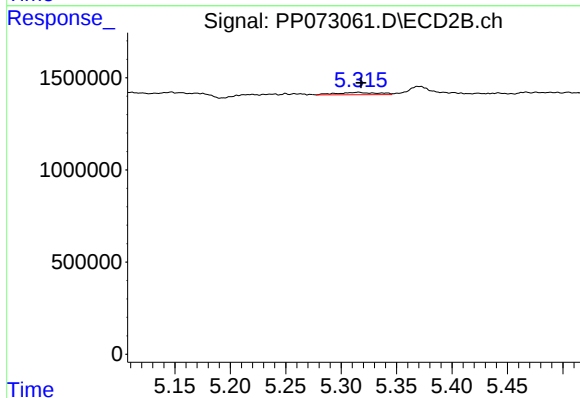


#7 AR-1016-5

R.T.: 5.316 min
Delta R.T.: -0.002 min
Response: 328547
Conc: 5.94 ng/ml

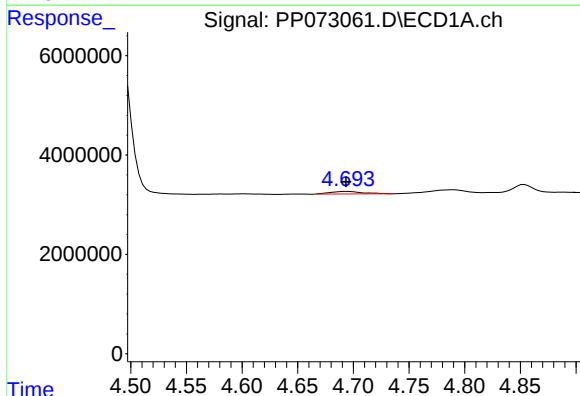


#8 AR-1221-1

R.T.: 4.694 min
Delta R.T.: 0.001 min
Response: 1008127
Conc: 40.88 ng/ml

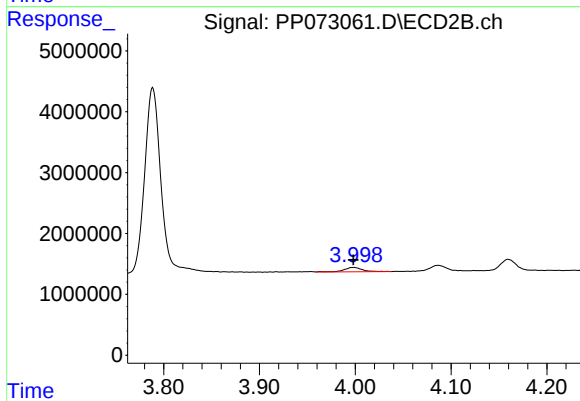

#8 AR-1221-1


R.T.: 3.998 min
Delta R.T.: 0.000 min
Response: 948086
Conc: 35.28 ng/ml

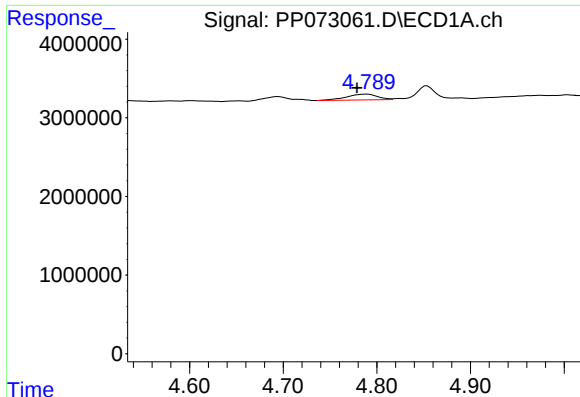

#9 AR-1221-2


R.T.: 4.790 min
Delta R.T.: 0.011 min
Response: 1697303
Conc: 84.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

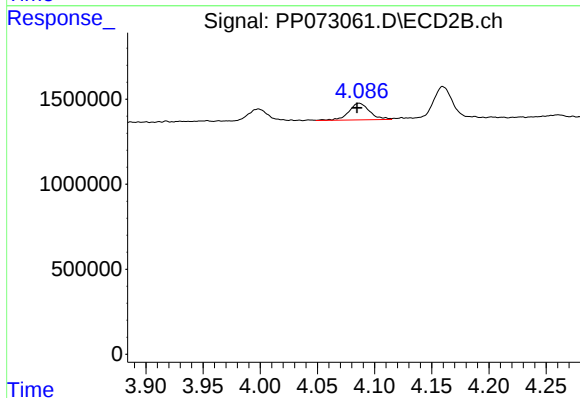


#9 AR-1221-2

R.T.: 4.087 min
Delta R.T.: 0.002 min
Response: 1247264
Conc: 61.79 ng/ml

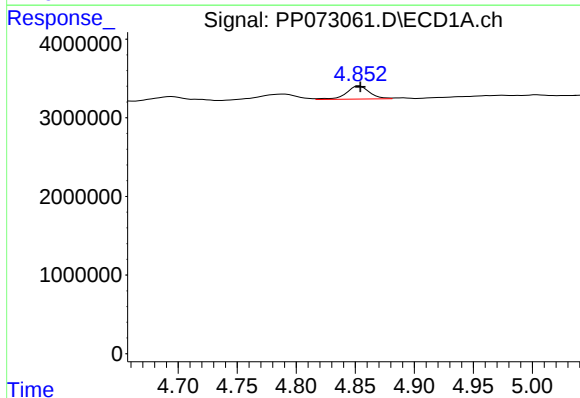


#10 AR-1221-3

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 2294164
Conc: 37.27 ng/ml

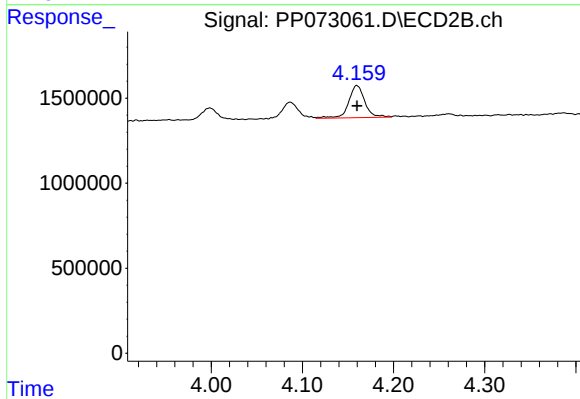

#10 AR-1221-3


R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 2348982
Conc: 39.99 ng/ml

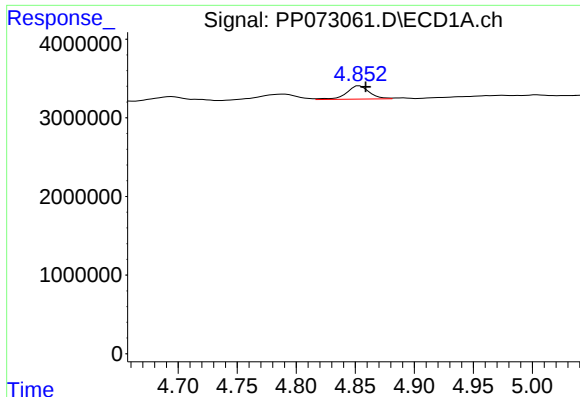

#11 AR-1232-1


R.T.: 4.854 min
Delta R.T.: -0.005 min
Response: 2294164
Conc: 48.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

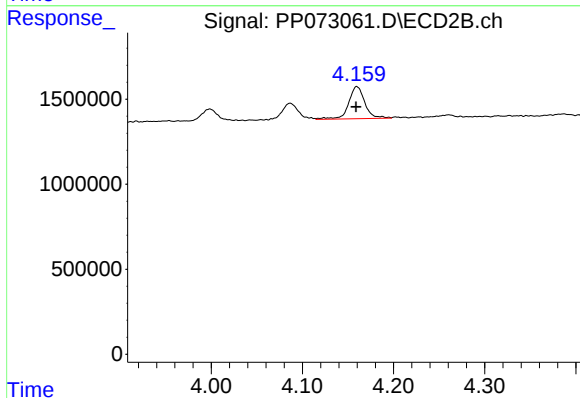


#11 AR-1232-1

R.T.: 4.160 min
Delta R.T.: 0.001 min
Response: 2348982
Conc: 51.55 ng/ml

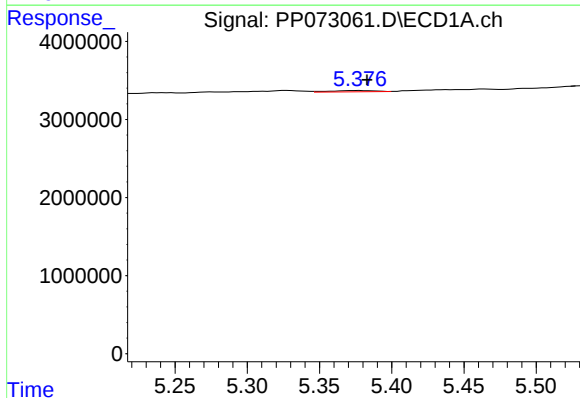


#12 AR-1232-2

R.T.: 5.377 min
Delta R.T.: -0.006 min
Response: 331133
Conc: 14.80 ng/ml

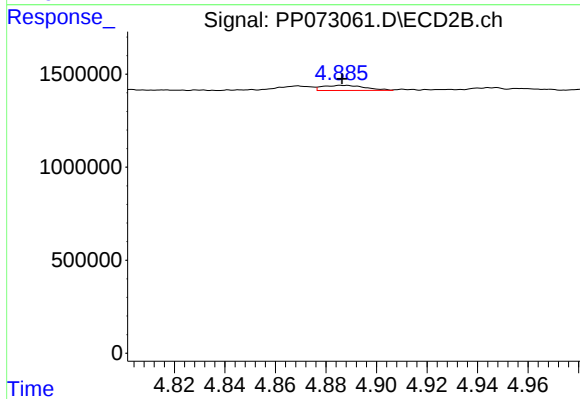

#12 AR-1232-2


R.T.: 4.887 min
Delta R.T.: 0.000 min
Response: 319751
Conc: 6.91 ng/ml

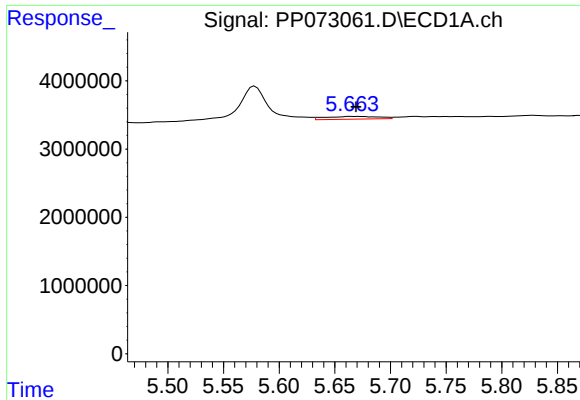

#13 AR-1232-3


R.T.: 5.665 min
Delta R.T.: -0.005 min
Response: 1390324
Conc: 26.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

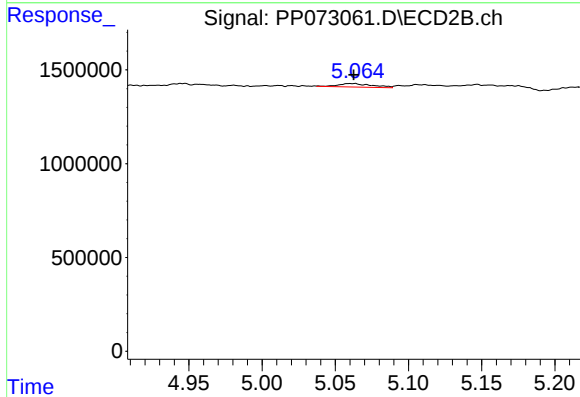


#13 AR-1232-3

R.T.: 5.061 min
Delta R.T.: -0.002 min
Response: 300554
Conc: 12.24 ng/ml

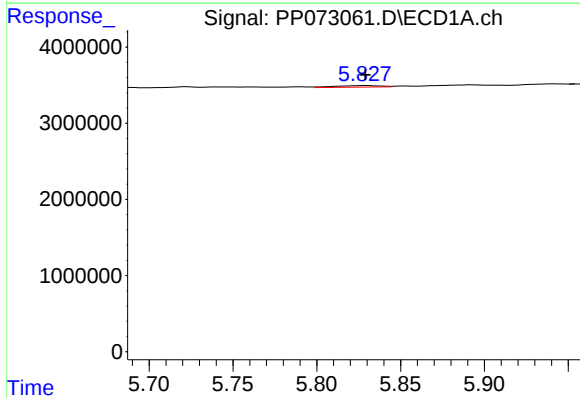


#14 AR-1232-4

R.T.: 5.830 min
Delta R.T.: 0.000 min
Response: 371079
Conc: 14.38 ng/ml

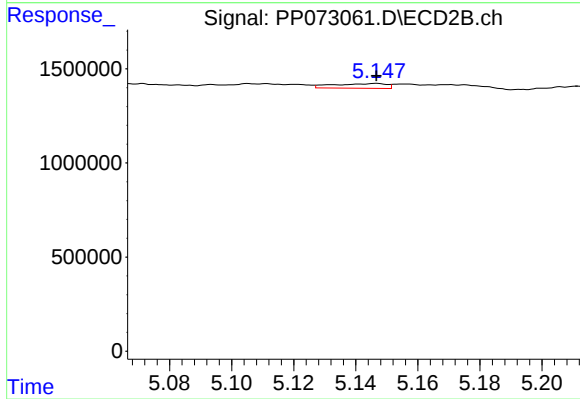

#14 AR-1232-4


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 302054
Conc: 13.97 ng/ml

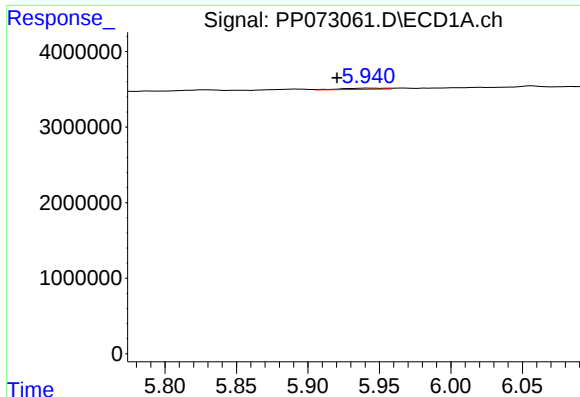

#15 AR-1232-5


R.T.: 5.942 min
Delta R.T.: 0.022 min
Response: 313177
Conc: 8.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

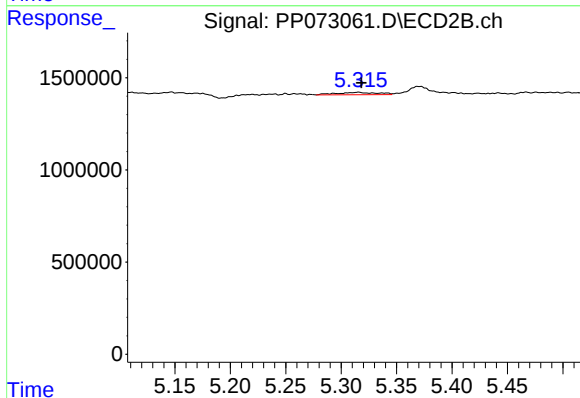


#15 AR-1232-5

R.T.: 5.316 min
Delta R.T.: -0.002 min
Response: 328547
Conc: 14.37 ng/ml

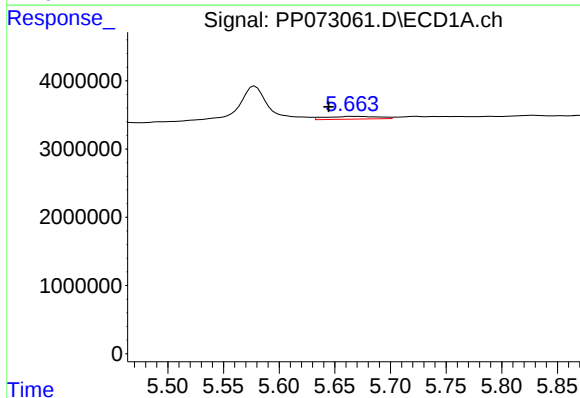


#16 AR-1242-1

R.T.: 5.665 min
Delta R.T.: 0.020 min
Response: 1390324
Conc: 23.79 ng/ml

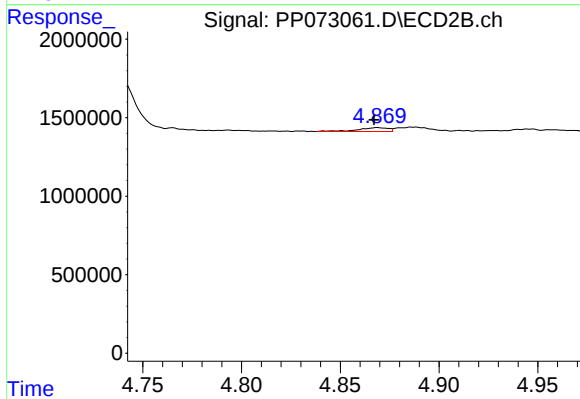

#16 AR-1242-1


R.T.: 4.869 min
Delta R.T.: 0.002 min
Response: 258662
Conc: 4.68 ng/ml

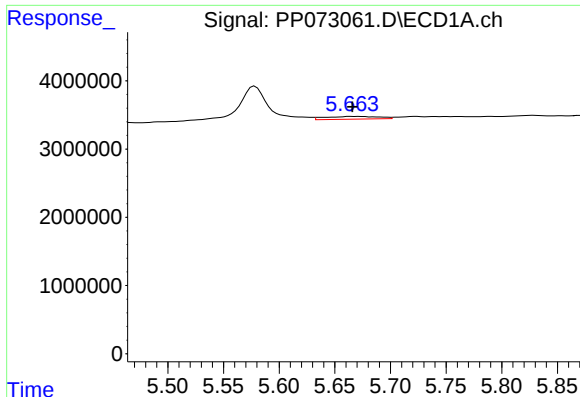

#17 AR-1242-2


R.T.: 5.665 min
Delta R.T.: -0.001 min
Response: 1390324
Conc: 16.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

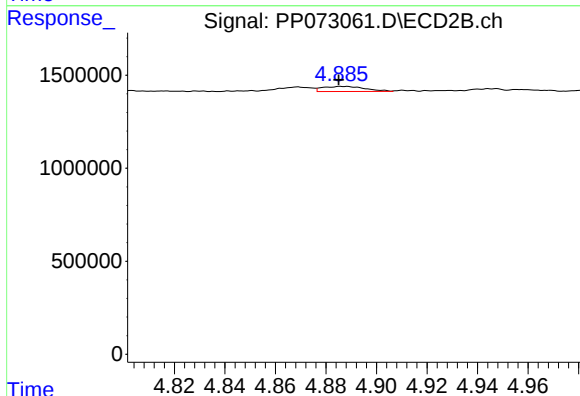


#17 AR-1242-2

R.T.: 4.887 min
Delta R.T.: 0.002 min
Response: 319751
Conc: 4.02 ng/ml

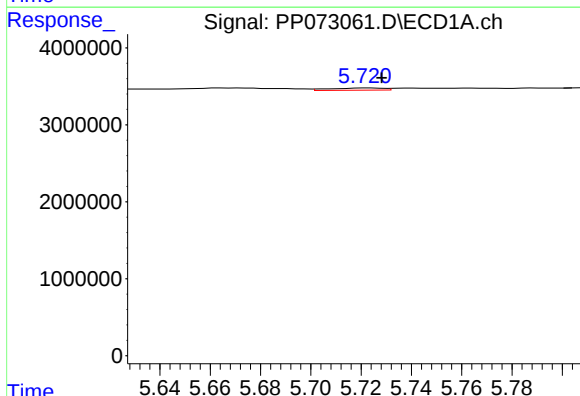


#18 AR-1242-3

R.T.: 5.722 min
Delta R.T.: -0.006 min
Response: 433613
Conc: 8.23 ng/ml

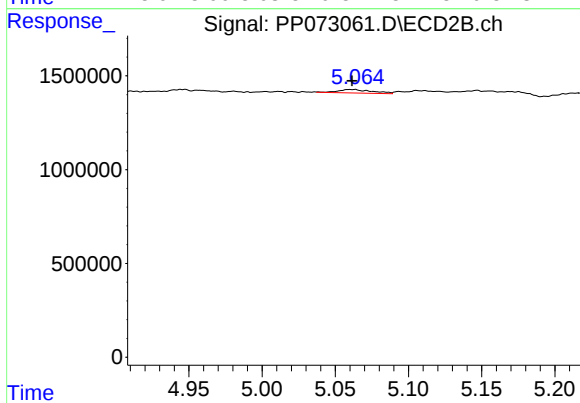

#18 AR-1242-3


R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 300554
Conc: 6.94 ng/ml

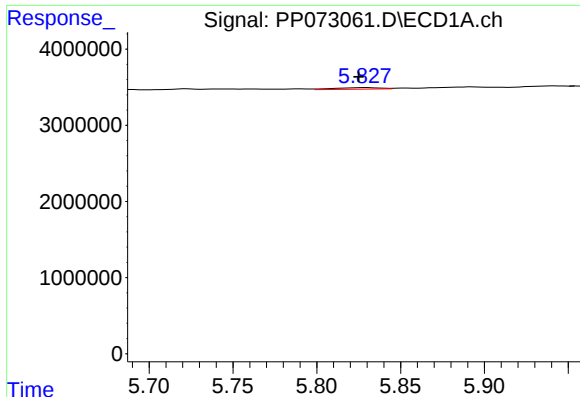

#19 AR-1242-4


R.T.: 5.830 min
Delta R.T.: 0.004 min
Response: 371079
Conc: 8.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

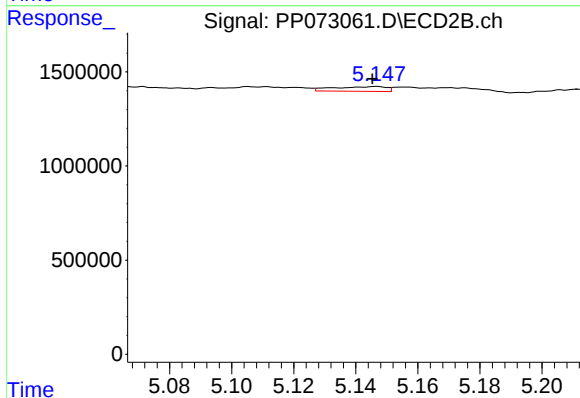


#19 AR-1242-4

R.T.: 5.147 min
Delta R.T.: 0.001 min
Response: 302054
Conc: 7.28 ng/ml

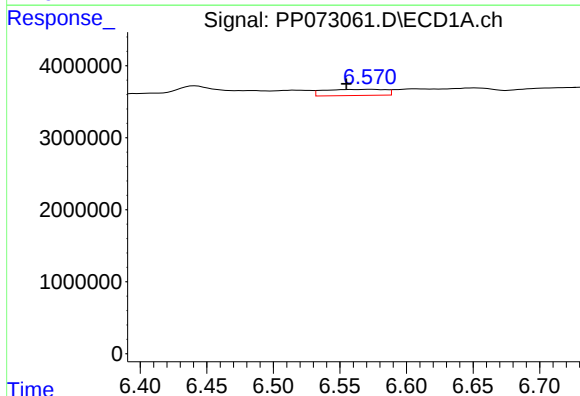


#20 AR-1242-5

R.T.: 6.574 min
Delta R.T.: 0.019 min
Response: 2758026
Conc: 55.65 ng/ml

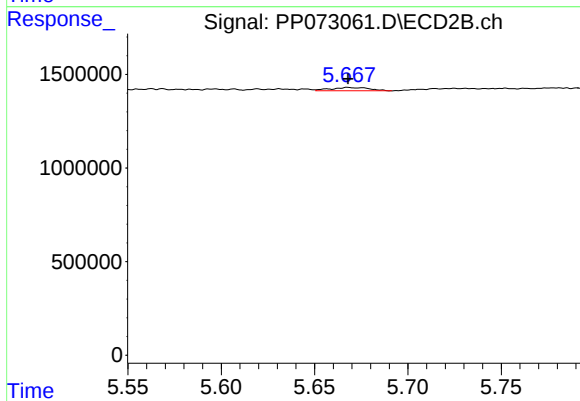

#20 AR-1242-5


R.T.: 5.668 min
Delta R.T.: 0.000 min
Response: 247285
Conc: 4.70 ng/ml

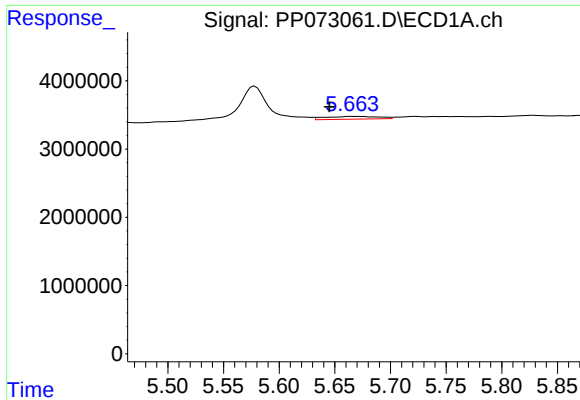

#21 AR-1248-1


R.T.: 5.665 min
Delta R.T.: 0.019 min
Response: 1390324
Conc: 29.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

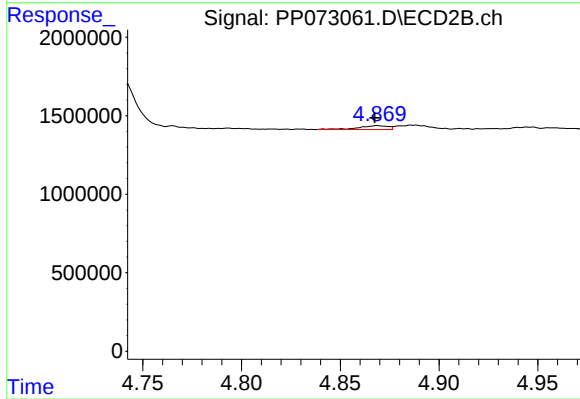


#21 AR-1248-1

R.T.: 4.869 min
Delta R.T.: 0.001 min
Response: 258662
Conc: 5.93 ng/ml

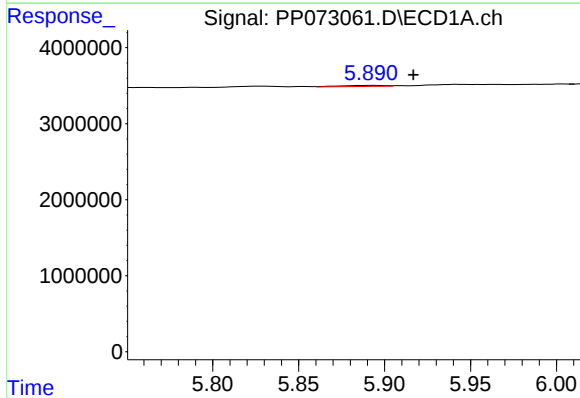


#22 AR-1248-2

R.T.: 5.892 min
Delta R.T.: -0.024 min
Response: 256731
Conc: 4.38 ng/ml

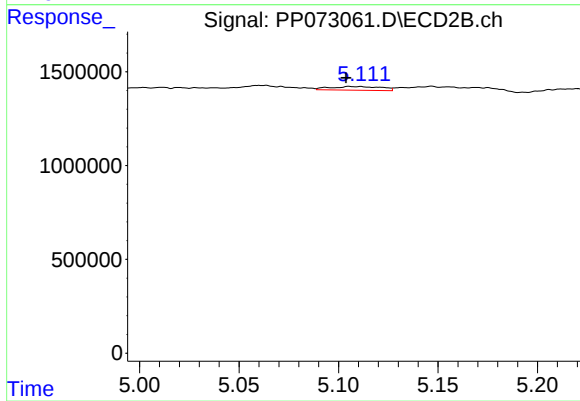

#22 AR-1248-2


R.T.: 5.106 min
Delta R.T.: 0.002 min
Response: 351336
Conc: 6.00 ng/ml

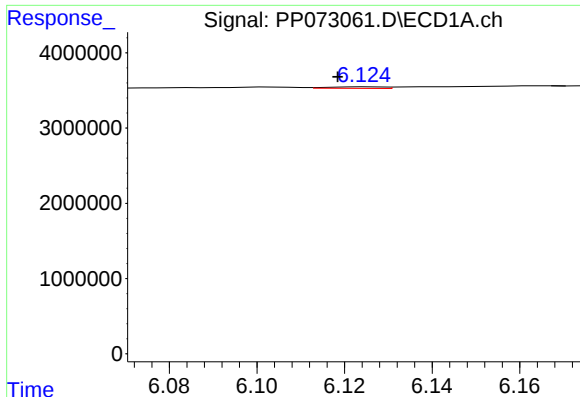

#23 AR-1248-3


R.T.: 6.125 min
Delta R.T.: 0.006 min
Response: 185582
Conc: 2.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

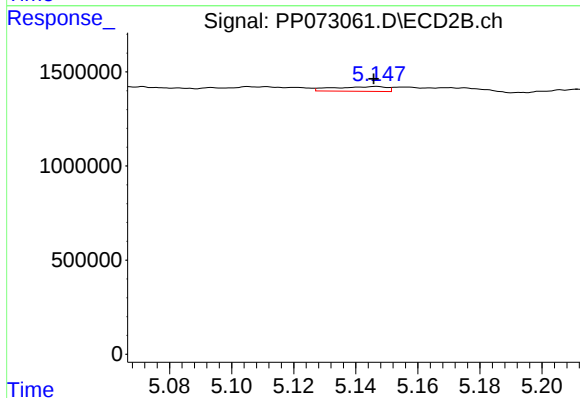


#23 AR-1248-3

R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 302054
Conc: 4.99 ng/ml

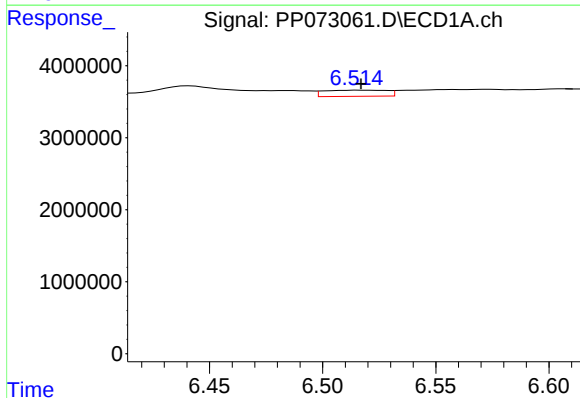


#24 AR-1248-4

R.T.: 6.516 min
Delta R.T.: -0.001 min
Response: 1638251
Conc: 19.26 ng/ml

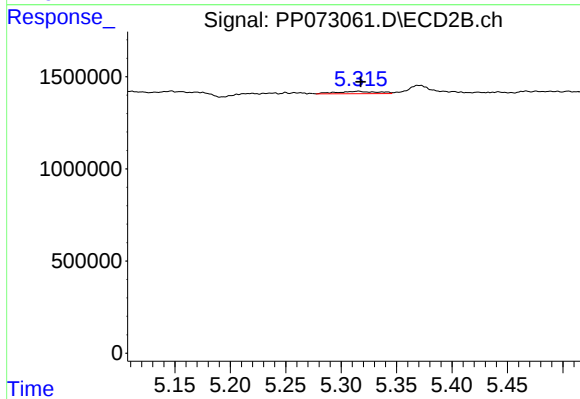

#24 AR-1248-4


R.T.: 5.316 min
Delta R.T.: -0.002 min
Response: 328547
Conc: 4.69 ng/ml

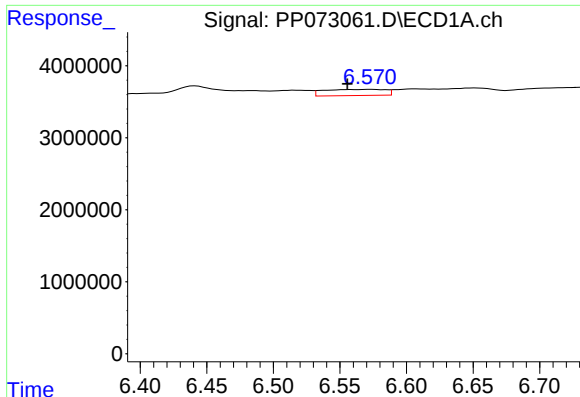

#25 AR-1248-5


R.T.: 6.574 min
Delta R.T.: 0.018 min
Response: 2758026
Conc: 32.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

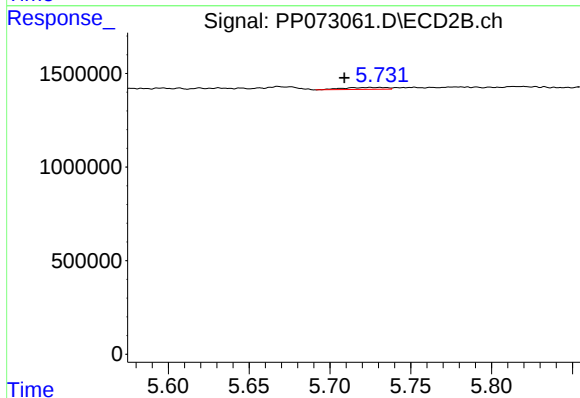


#25 AR-1248-5

R.T.: 5.731 min
Delta R.T.: 0.022 min
Response: 198249
Conc: 2.79 ng/ml

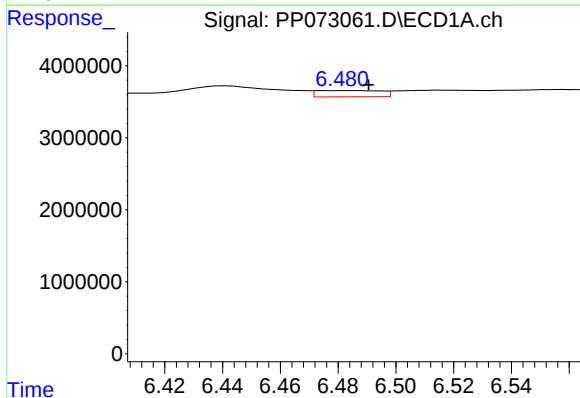


#26 AR-1254-1

R.T.: 6.482 min
Delta R.T.: -0.008 min
Response: 1341370
Conc: 15.94 ng/ml

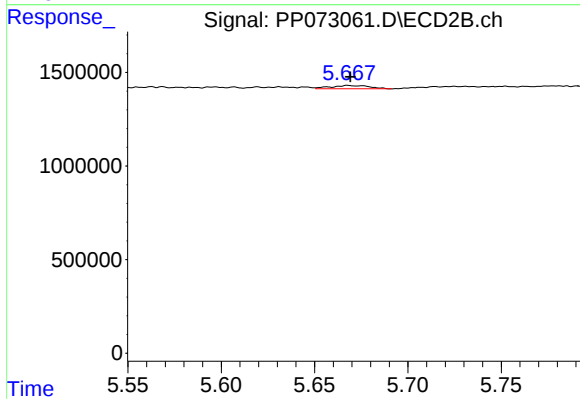

#26 AR-1254-1


R.T.: 5.668 min
Delta R.T.: -0.001 min
Response: 247285
Conc: 2.26 ng/ml

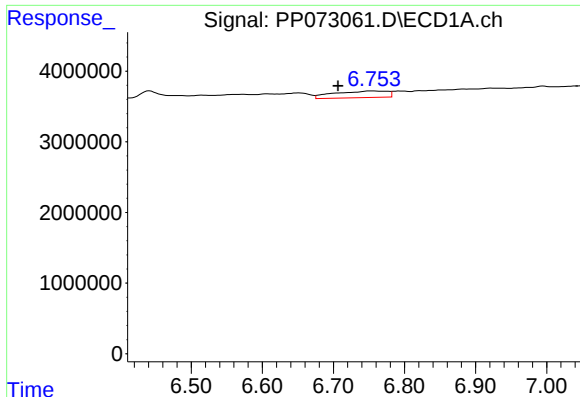

#27 AR-1254-2


R.T.: 6.754 min
Delta R.T.: 0.048 min
Response: 4851005
Conc: 38.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

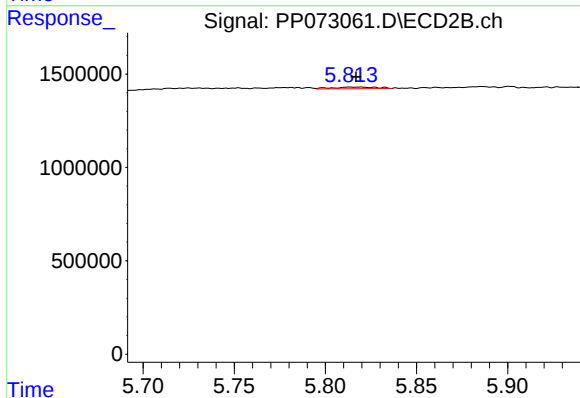


#27 AR-1254-2

R.T.: 5.814 min
Delta R.T.: -0.003 min
Response: 156327
Conc: 1.65 ng/ml

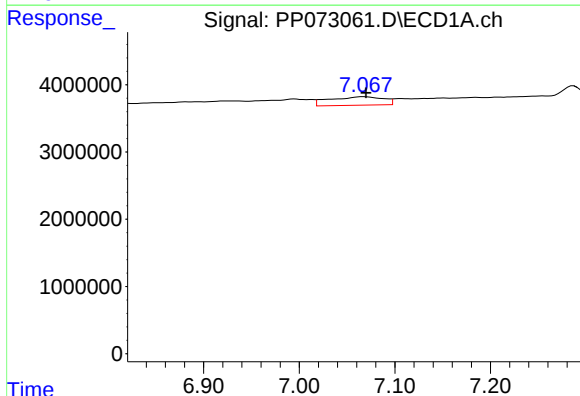


#28 AR-1254-3

R.T.: 7.068 min
Delta R.T.: -0.002 min
Response: 4930904
Conc: 37.58 ng/ml

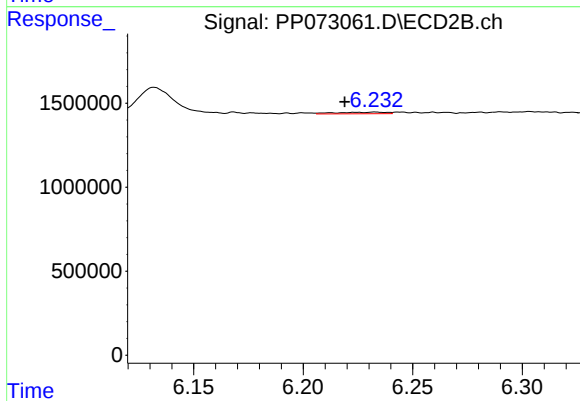

#28 AR-1254-3


R.T.: 6.233 min
Delta R.T.: 0.014 min
Response: 160666
Conc: 1.09 ng/ml

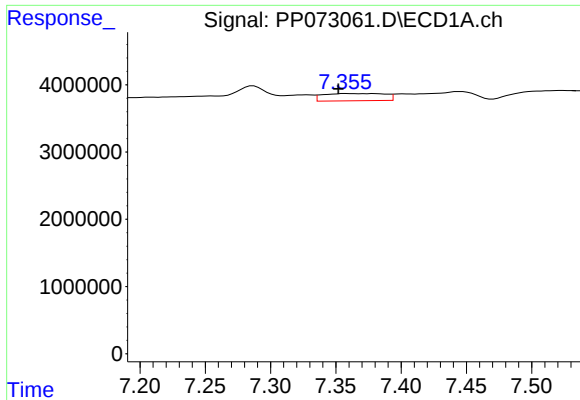

#29 AR-1254-4


R.T.: 7.357 min
Delta R.T.: 0.005 min
Response: 3537310
Conc: 29.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

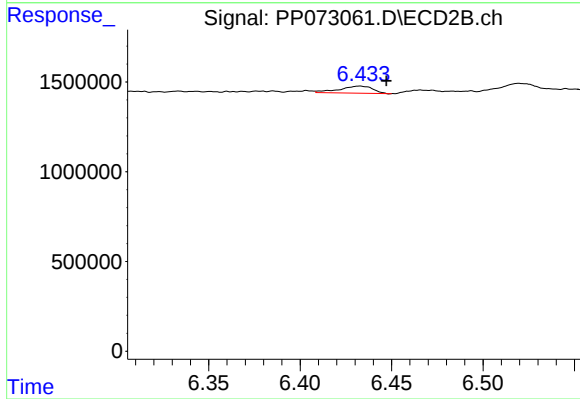


#29 AR-1254-4

R.T.: 6.433 min
Delta R.T.: -0.015 min
Response: 496289
Conc: 5.11 ng/ml

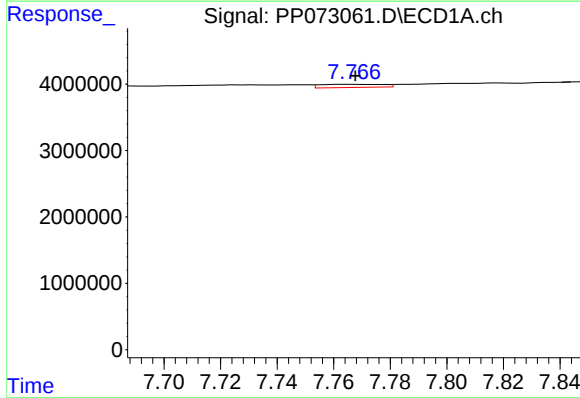


#30 AR-1254-5

R.T.: 7.767 min
Delta R.T.: 0.000 min
Response: 736437
Conc: 6.45 ng/ml

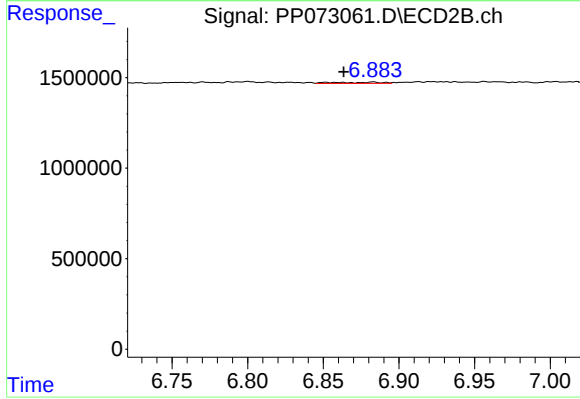

#30 AR-1254-5


R.T.: 6.883 min
Delta R.T.: 0.020 min
Response: 140128
Conc: 1.08 ng/ml

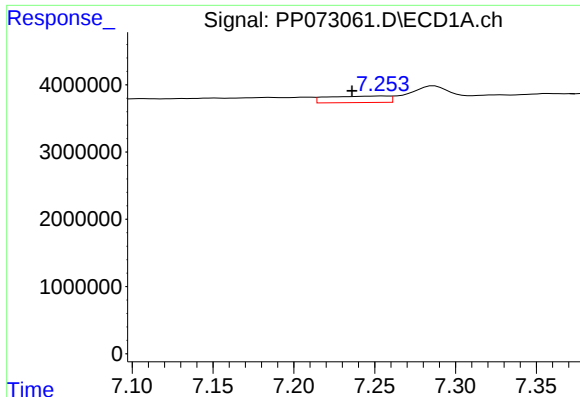

#31 AR-1260-1


R.T.: 7.255 min
Delta R.T.: 0.019 min
Response: 2555685
Conc: 28.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

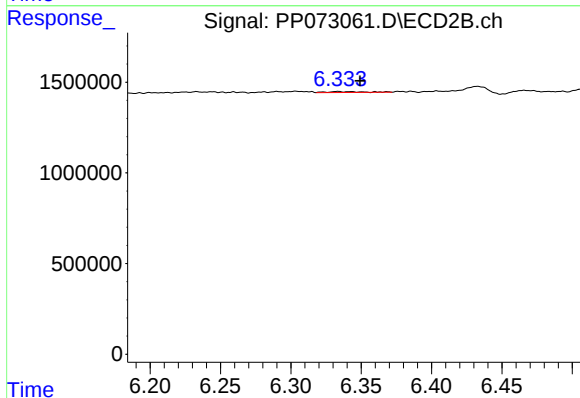


#31 AR-1260-1

R.T.: 6.333 min
Delta R.T.: -0.016 min
Response: 94803
Conc: 1.00 ng/ml

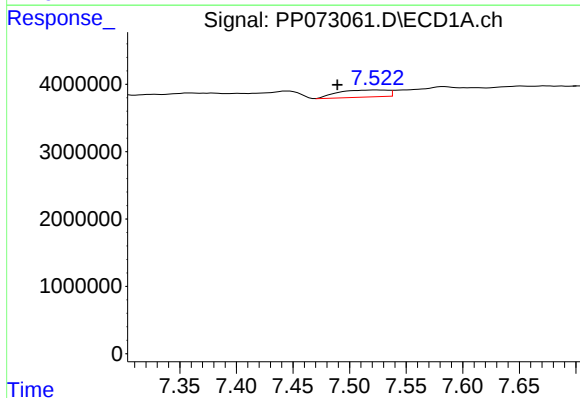


#32 AR-1260-2

R.T.: 7.523 min
Delta R.T.: 0.034 min
Response: 3191556
Conc: 23.49 ng/ml

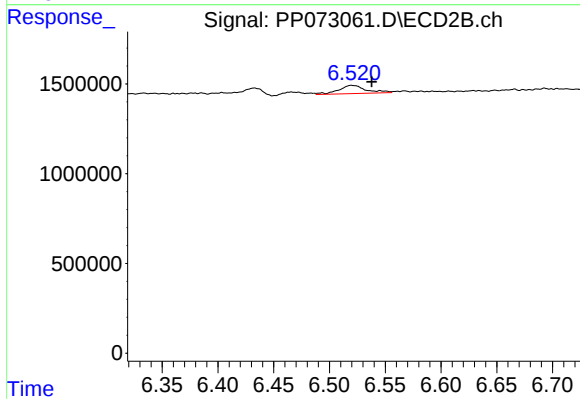

#32 AR-1260-2


R.T.: 6.520 min
Delta R.T.: -0.018 min
Response: 794371
Conc: 6.82 ng/ml

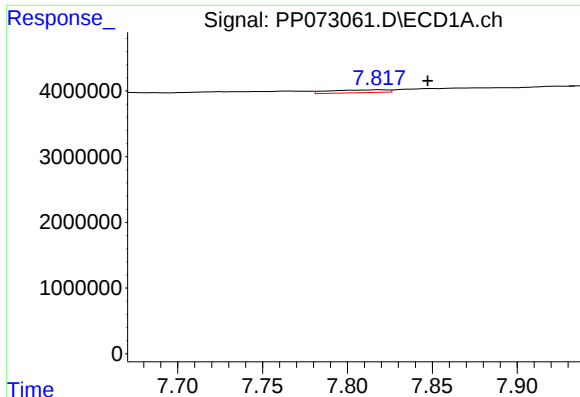

#33 AR-1260-3


R.T.: 7.819 min
Delta R.T.: -0.028 min
Response: 1025707
Conc: 8.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

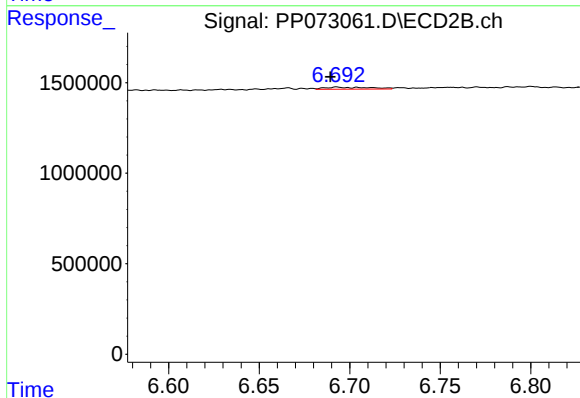


#33 AR-1260-3

R.T.: 6.693 min
Delta R.T.: 0.003 min
Response: 193707
Conc: 1.86 ng/ml

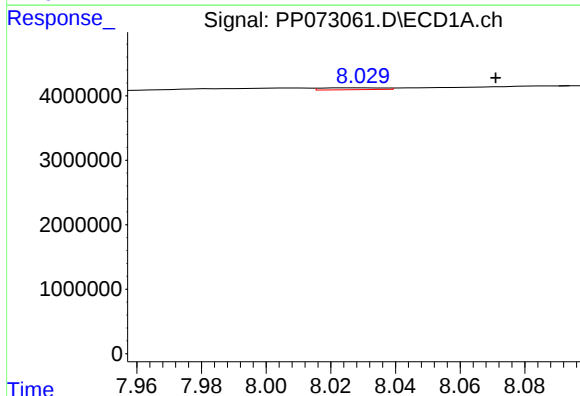


#34 AR-1260-4

R.T.: 8.027 min
Delta R.T.: -0.044 min
Response: 374011
Conc: 3.63 ng/ml

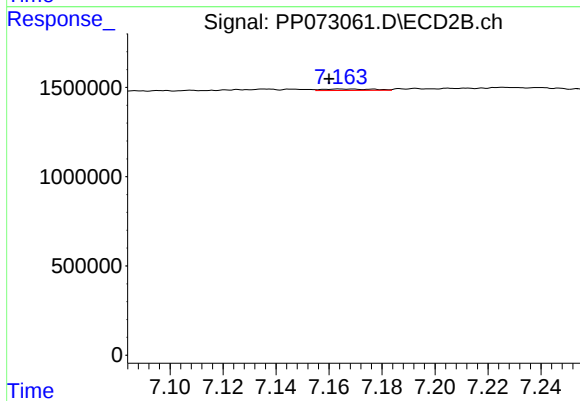

#34 AR-1260-4


R.T.: 7.164 min
Delta R.T.: 0.004 min
Response: 110849
Conc: 1.26 ng/ml

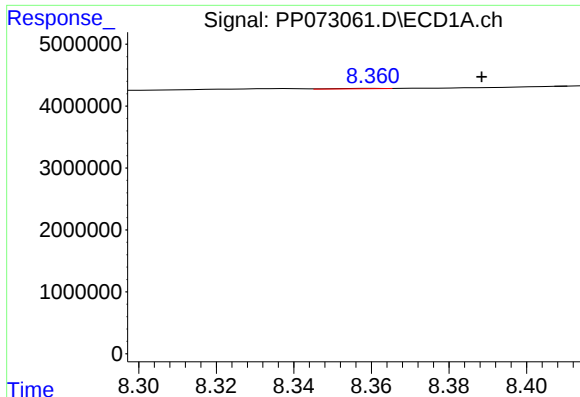

#35 AR-1260-5


R.T.: 8.360 min
Delta R.T.: -0.028 min
Response: 56990
Conc: 0.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

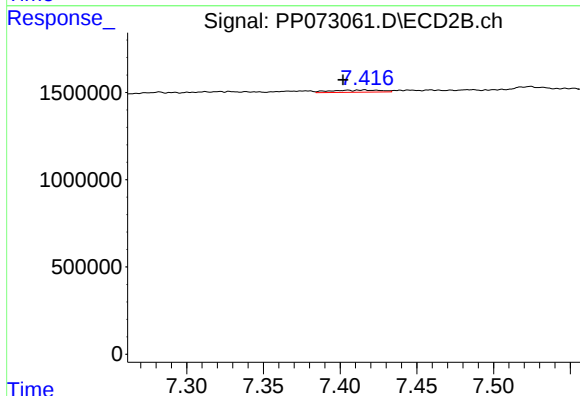


#35 AR-1260-5

R.T.: 7.416 min
Delta R.T.: 0.014 min
Response: 279667
Conc: 1.31 ng/ml

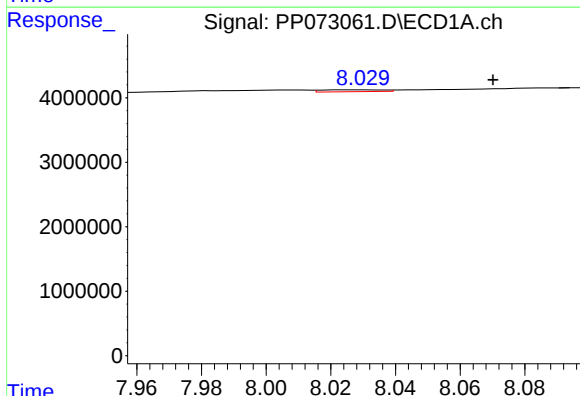


#36 AR-1262-1

R.T.: 8.027 min
Delta R.T.: -0.043 min
Response: 374011
Conc: 2.53 ng/ml

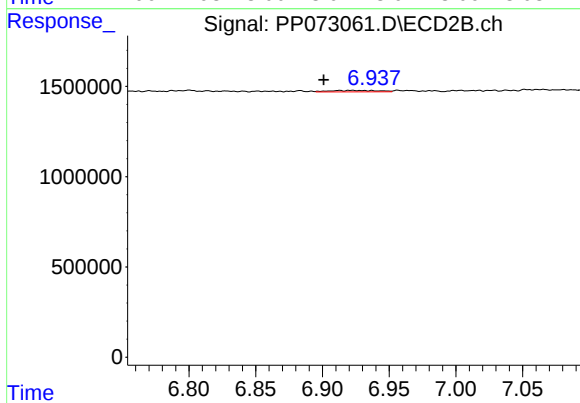

#36 AR-1262-1


R.T.: 6.913 min
Delta R.T.: 0.012 min
Response: 207327
Conc: 1.44 ng/ml

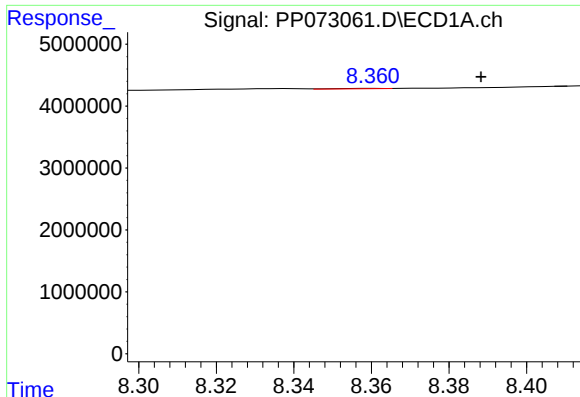

#37 AR-1262-2


R.T.: 8.360 min
Delta R.T.: -0.028 min
Response: 56990
Conc: 0.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

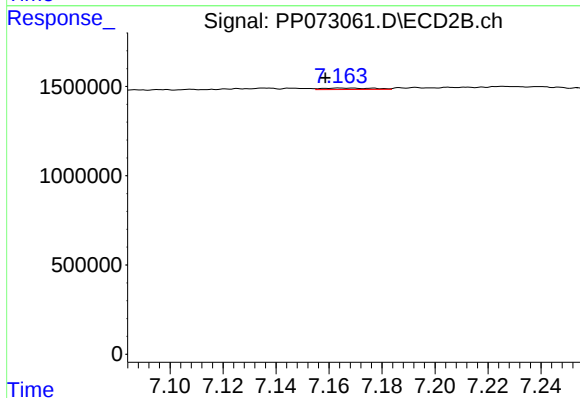


#37 AR-1262-2

R.T.: 7.164 min
Delta R.T.: 0.005 min
Response: 110849
Conc: 0.91 ng/ml

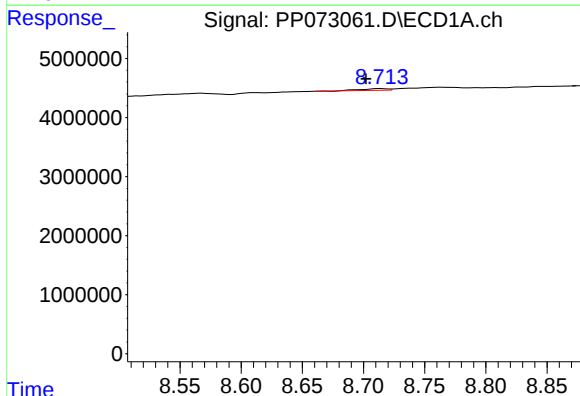


#38 AR-1262-3

R.T.: 8.714 min
Delta R.T.: 0.012 min
Response: 399885
Conc: 1.87 ng/ml

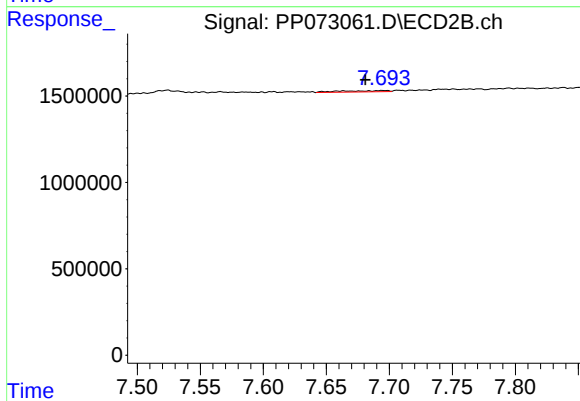

#38 AR-1262-3


R.T.: 7.695 min
Delta R.T.: 0.014 min
Response: 199984
Conc: 1.77 ng/ml

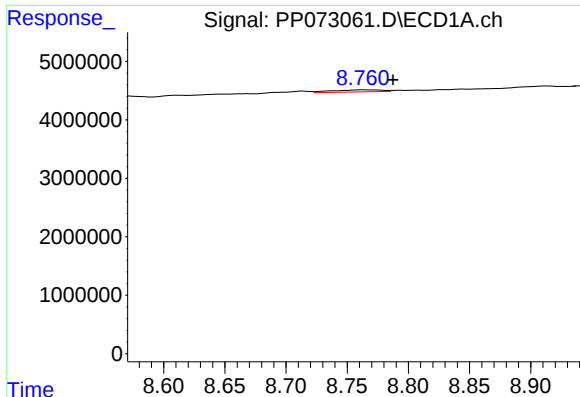

#39 AR-1262-4


R.T.: 8.762 min
Delta R.T.: -0.025 min
Response: 994791
Conc: 6.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

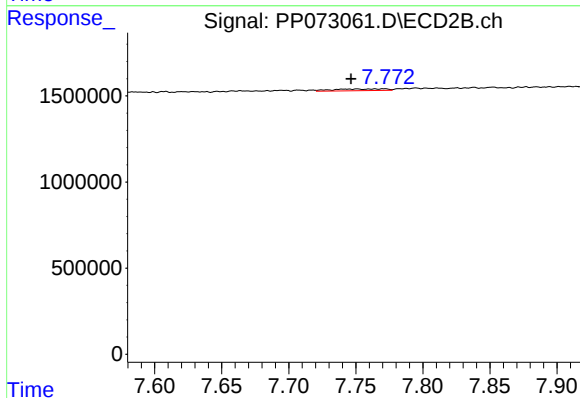


#39 AR-1262-4

R.T.: 7.771 min
Delta R.T.: 0.025 min
Response: 278749
Conc: 1.52 ng/ml

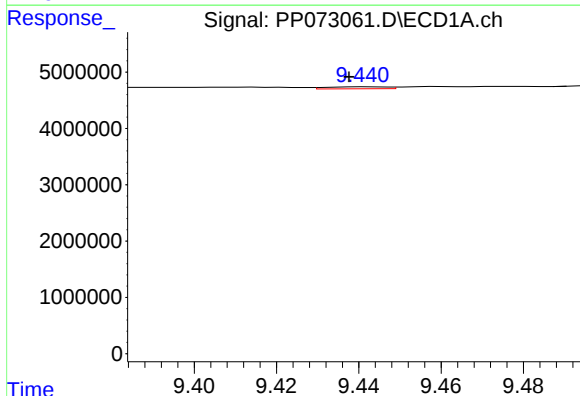


#40 AR-1262-5

R.T.: 9.441 min
Delta R.T.: 0.004 min
Response: 350036
Conc: 3.13 ng/ml

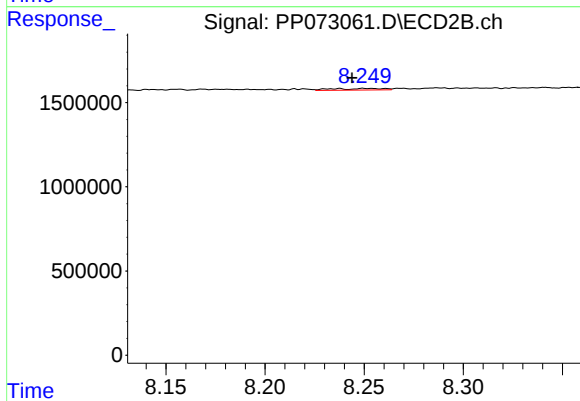

#40 AR-1262-5


R.T.: 8.238 min
Delta R.T.: -0.006 min
Response: 167985
Conc: 1.94 ng/ml

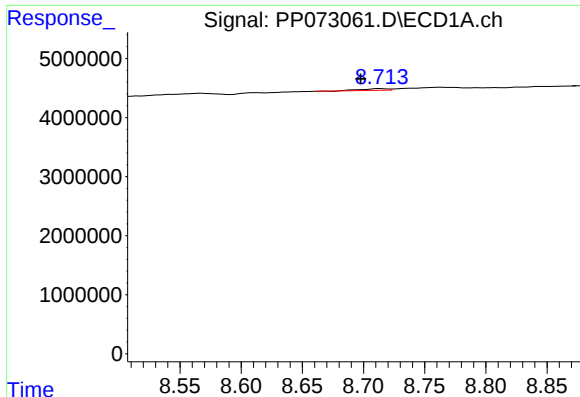

#41 AR-1268-1


R.T.: 8.714 min
Delta R.T.: 0.016 min
Response: 399885
Conc: 1.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

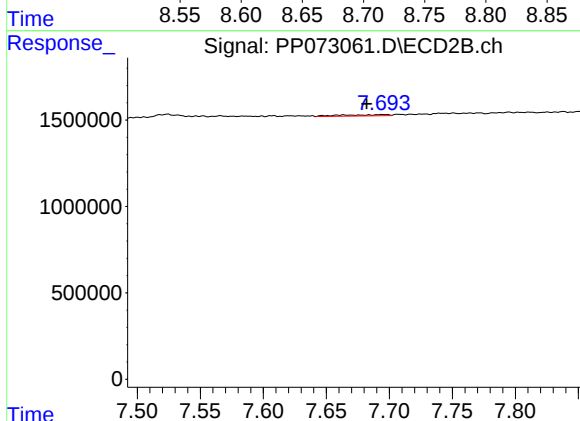


#41 AR-1268-1

R.T.: 7.695 min
Delta R.T.: 0.013 min
Response: 199984
Conc: 0.70 ng/ml

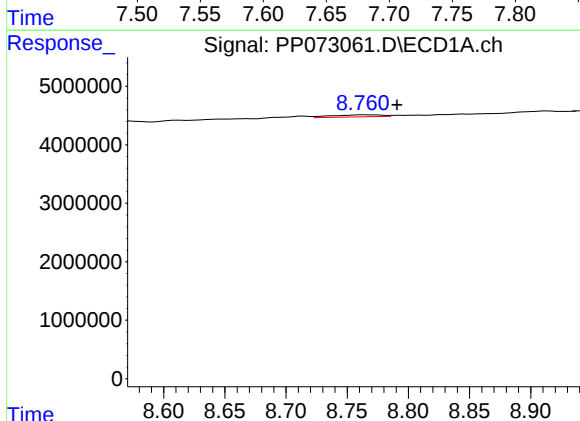


#42 AR-1268-2

R.T.: 8.762 min
Delta R.T.: -0.028 min
Response: 994791
Conc: 3.26 ng/ml

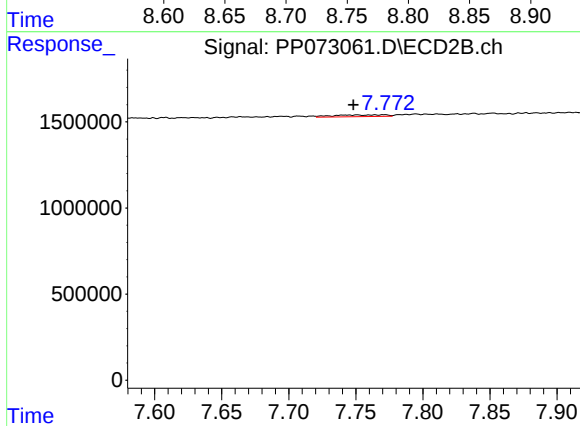

#42 AR-1268-2


R.T.: 7.771 min
Delta R.T.: 0.023 min
Response: 278749
Conc: 1.08 ng/ml

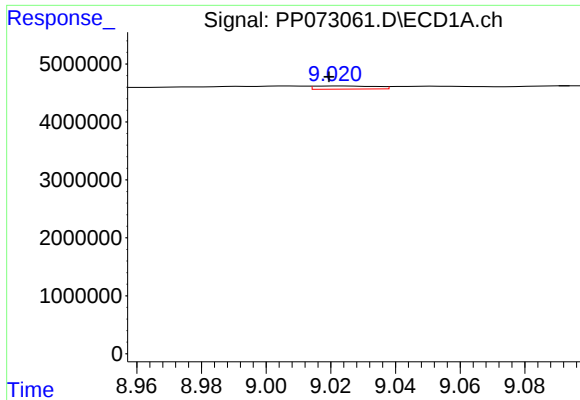

#43 AR-1268-3


R.T.: 9.022 min
Delta R.T.: 0.003 min
Response: 719300
Conc: 2.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

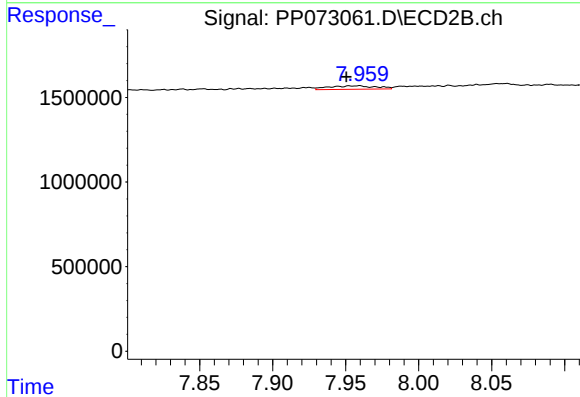


#43 AR-1268-3

R.T.: 7.959 min
Delta R.T.: 0.009 min
Response: 452521
Conc: 2.10 ng/ml

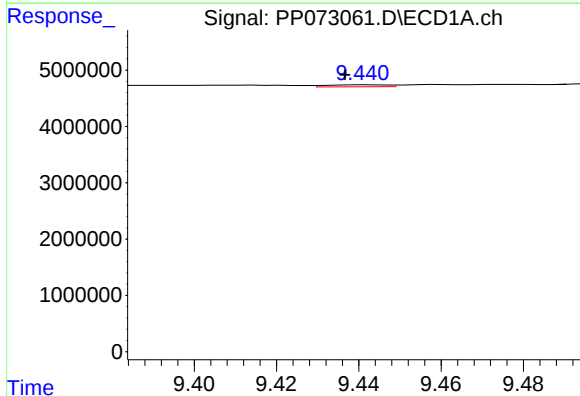


#44 AR-1268-4

R.T.: 9.441 min
Delta R.T.: 0.005 min
Response: 350036
Conc: 2.99 ng/ml

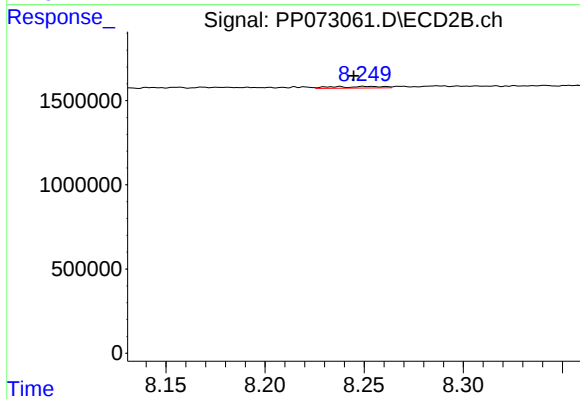

#44 AR-1268-4


R.T.: 8.238 min
Delta R.T.: -0.007 min
Response: 167985
Conc: 1.78 ng/ml

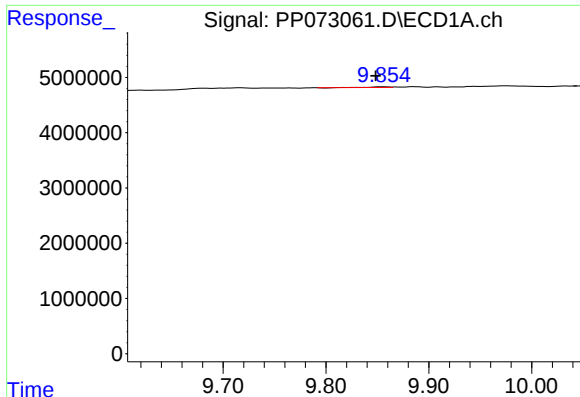

#45 AR-1268-5

R.T.: 9.856 min
Delta R.T.: 0.008 min
Response: 119726
Conc: 0.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

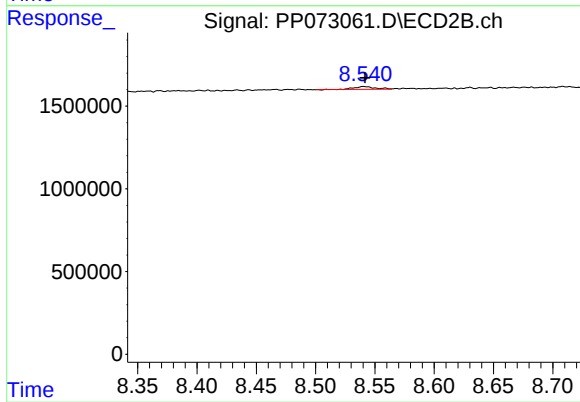

#45 AR-1268-5

R.T.: 8.541 min
Delta R.T.: -0.001 min
Response: 202392
Conc: 0.35 ng/ml