

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
 Data File : PP073065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 00:08
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:43:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.492	3.788	39384991	33711420	18.659	18.710
2)	SA Decachlor...	10.186	8.797	36964106	27418935	21.630	20.543
Target Compounds							
3)	L1 AR-1016-1	5.639	4.868	1238500	456523	17.042	6.643 #
4)	L1 AR-1016-2	5.669	4.888	293060	278801	2.817	2.770
5)	L1 AR-1016-3	5.702	5.063	679858	476054	10.404	8.700
6)	L1 AR-1016-4	5.825	5.103	440171	2203512	8.419	49.462 #
7)	L1 AR-1016-5	6.117	5.318	1031471	1189415	20.627	21.515
8)	L2 AR-1221-1	0.000	4.006	0	140578	N.D.	5.231 #
9)	L2 AR-1221-2	4.795	4.090	1059653	843200	52.512	41.773
10)	L2 AR-1221-3	4.854	4.165	223273	64127	3.627	1.092 #
11)	L3 AR-1232-1	4.854	4.154	223273	67257	4.755	1.476 #
12)	L3 AR-1232-2	5.364	4.888	245340	278801	10.967	6.027 #
13)	L3 AR-1232-3	5.669	5.063	293060	476054	5.680	19.385 #
14)	L3 AR-1232-4	5.825	5.144	440171	929796	17.054	42.996 #
15)	L3 AR-1232-5	5.915	5.318	1723225	1189415	48.310	52.033
16)	L4 AR-1242-1	5.639	4.868	1238500	456523	21.194	8.267 #
17)	L4 AR-1242-2	5.669	4.888	293060	278801	3.386	3.508
18)	L4 AR-1242-3	5.702	5.063	679858	476054	12.899	10.993
19)	L4 AR-1242-4	5.825	5.144	440171	929796	10.013	22.403 #
20)	L4 AR-1242-5	6.559	5.669	2729899	4157471	55.083	79.060 #
21)	L5 AR-1248-1	5.639	4.868	1238500	456523	26.036	10.473 #
22)	L5 AR-1248-2	5.915	5.103	1723225	2203512	29.431	37.605 #
23)	L5 AR-1248-3	6.117	5.144	1031471	929796	15.808	15.357
24)	L5 AR-1248-4	6.515	5.318	2125926	1189415	24.992	16.986 #
25)	L5 AR-1248-5	6.559	5.711	2729899	476549	32.618	6.709 #
26)	L6 AR-1254-1	6.492	5.669	3996739	4157471	47.482	37.916
27)	L6 AR-1254-2	6.707	5.816	5568712	3582429	44.407	37.891
28)	L6 AR-1254-3	7.071	6.219	6387930	5428100	48.684	36.789
29)	L6 AR-1254-4	7.354	6.447	6127718	3534580	51.156	36.401 #
30)	L6 AR-1254-5	7.769	6.863	3897993	4671148	34.116	35.942
31)	L7 AR-1260-1	7.235	6.349	3206877	2574267	36.354	27.175 #
32)	L7 AR-1260-2	7.489	6.537	2890104	2597800	21.269	22.311
33)	L7 AR-1260-3	7.845	6.688	839598	2240917	7.355	21.514 #
34)	L7 AR-1260-4	8.056	7.159	1356842	302245	13.167	3.445 #
35)	L7 AR-1260-5	8.386	7.400	690002	565968	2.868	2.652
36)	L8 AR-1262-1	8.056	6.933	1356842	416639	9.166	2.884 #
37)	L8 AR-1262-2	8.386	7.159	690002	302245	2.180	2.473
38)	L8 AR-1262-3	8.717	7.671	305915	106137	1.430	0.942 #
39)	L8 AR-1262-4	8.768	7.744	1114948	760157	7.075	4.146 #
40)	L8 AR-1262-5	9.437	8.250	339219	59166	3.032	0.683 #
41)	L9 AR-1268-1	8.717	7.693	305915	26017	0.855	0.091 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
 Data File : PP073065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 00:08
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:43:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.768	7.744	1114948	760157	3.655	2.956
43) L9	AR-1268-3	9.012	7.955	729589	457418	2.748	2.118
44) L9	AR-1268-4	9.437	8.250	339219	59166	2.899	0.628 #
45) L9	AR-1268-5	9.855	8.539	284693	161977	0.385	0.280 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
Data File : PP073065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 00:08
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:43:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

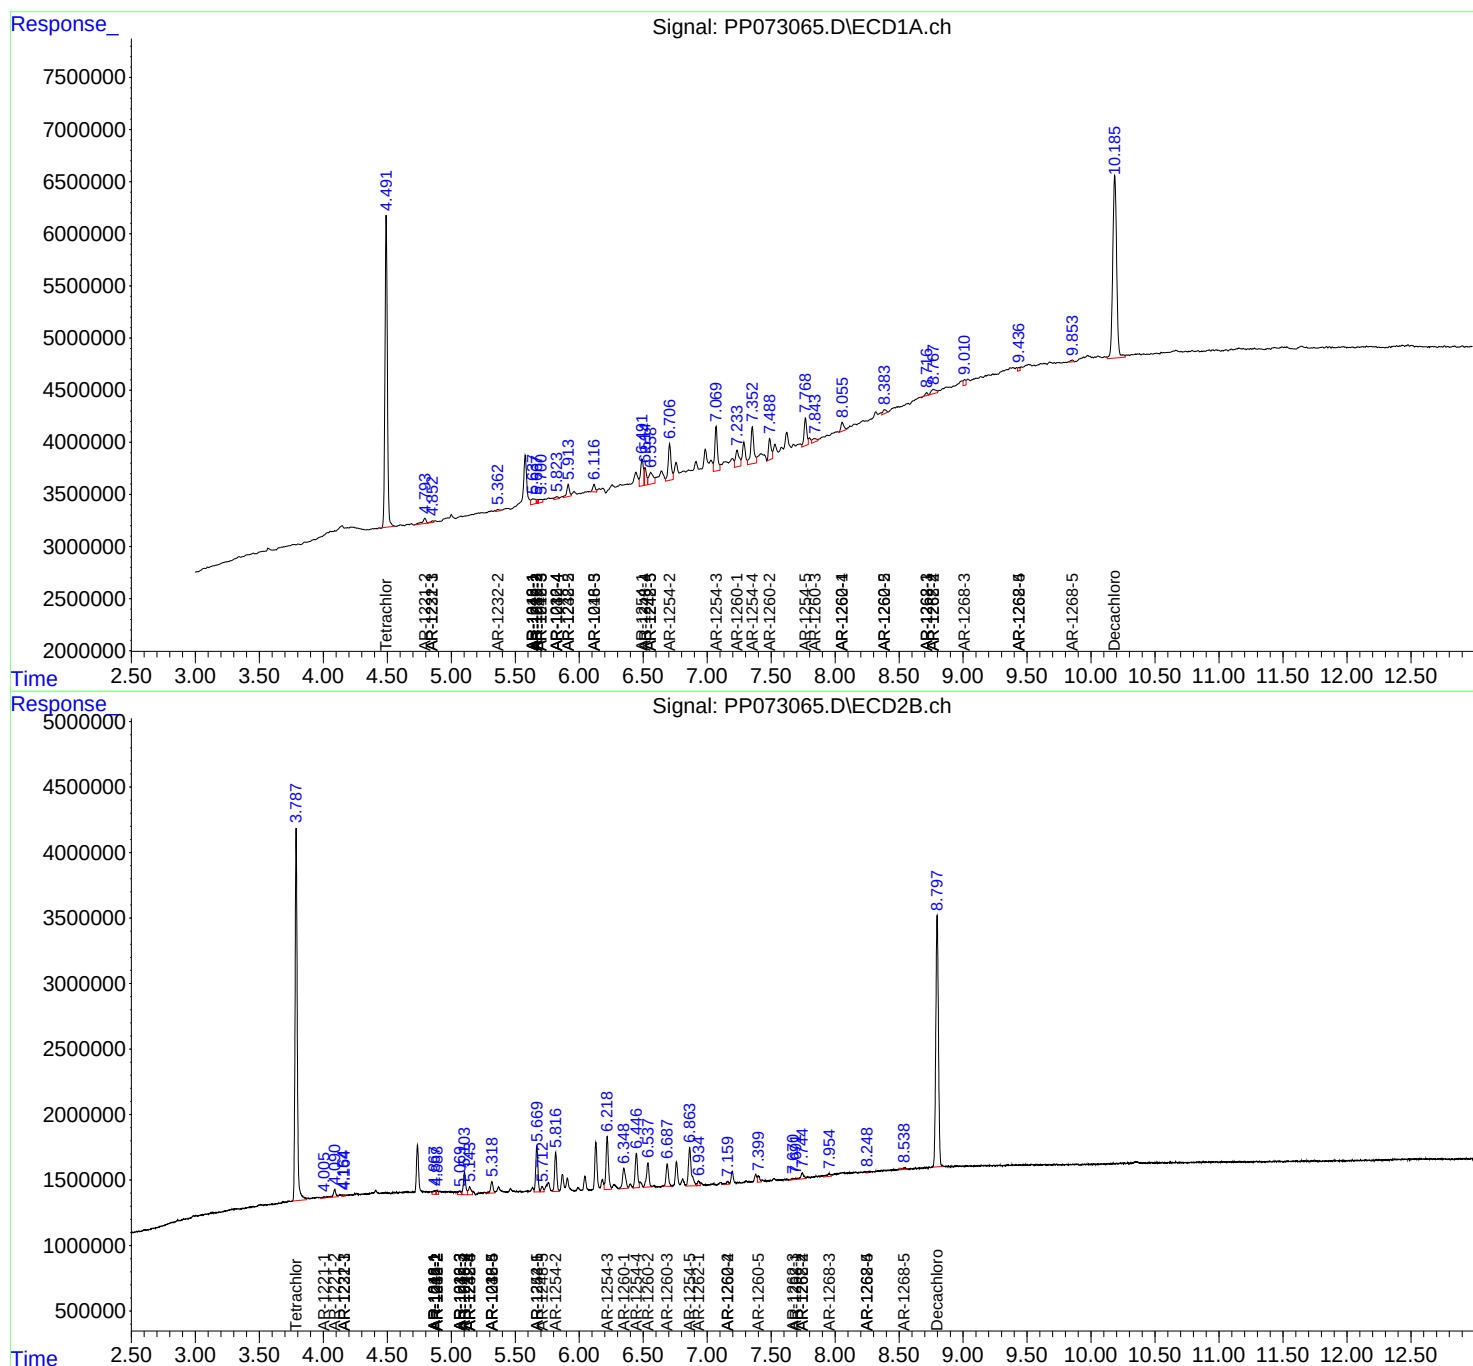


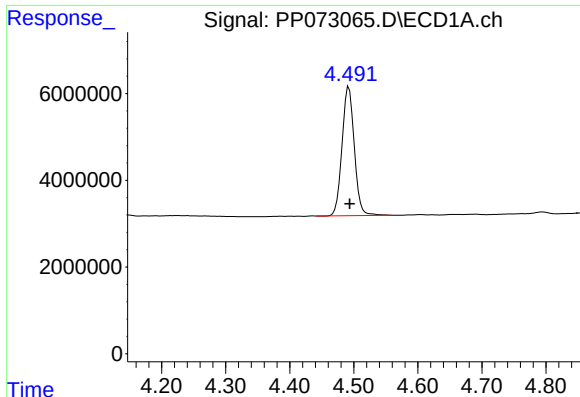

#1 Tetrachloro-m-xylene


R.T.: 4.492 min
Delta R.T.: -0.002 min
Response: 39384991
Conc: 18.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

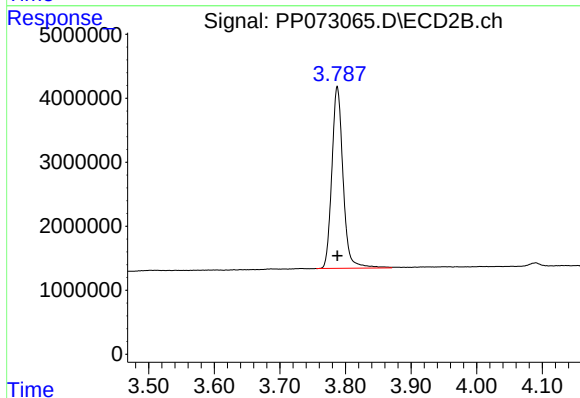


#1 Tetrachloro-m-xylene

R.T.: 3.788 min
Delta R.T.: 0.000 min
Response: 33711420
Conc: 18.71 ng/ml

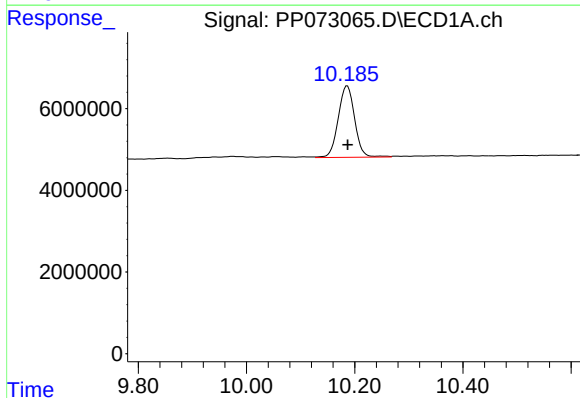


#2 Decachlorobiphenyl

R.T.: 10.186 min
Delta R.T.: 0.000 min
Response: 36964106
Conc: 21.63 ng/ml

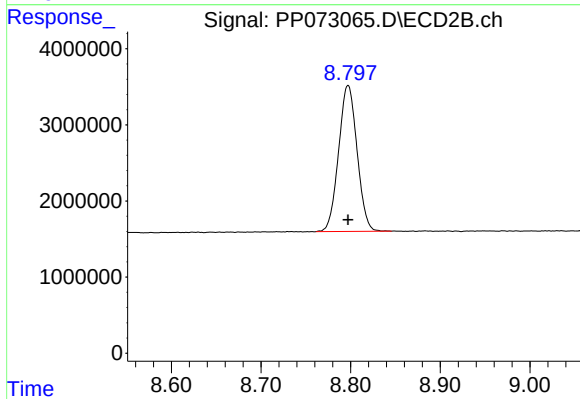

#2 Decachlorobiphenyl


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 27418935
Conc: 20.54 ng/ml

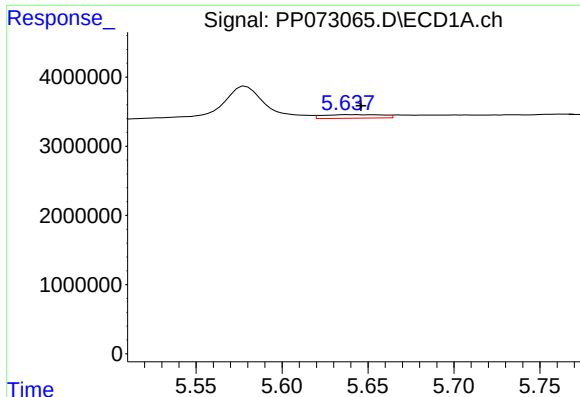

#3 AR-1016-1


R.T.: 5.639 min
Delta R.T.: -0.007 min
Response: 1238500
Conc: 17.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

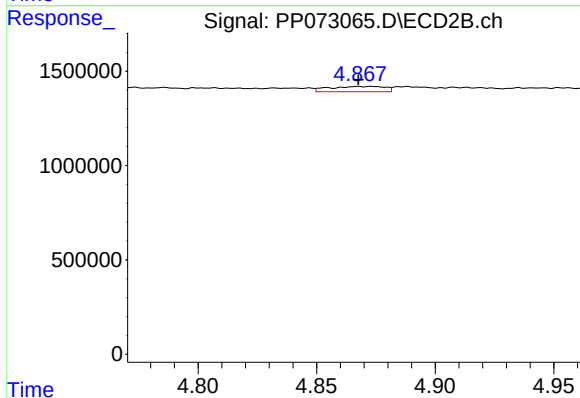


#3 AR-1016-1

R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 456523
Conc: 6.64 ng/ml

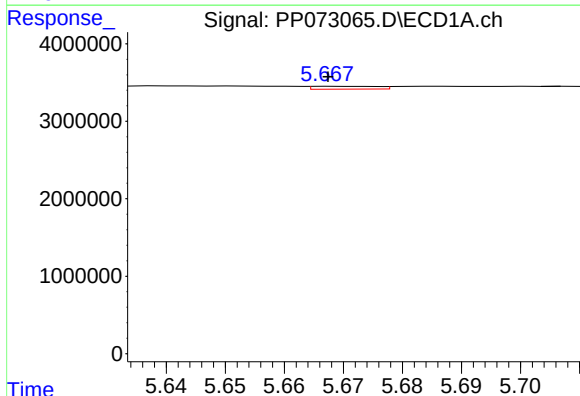


#4 AR-1016-2

R.T.: 5.669 min
Delta R.T.: 0.001 min
Response: 293060
Conc: 2.82 ng/ml

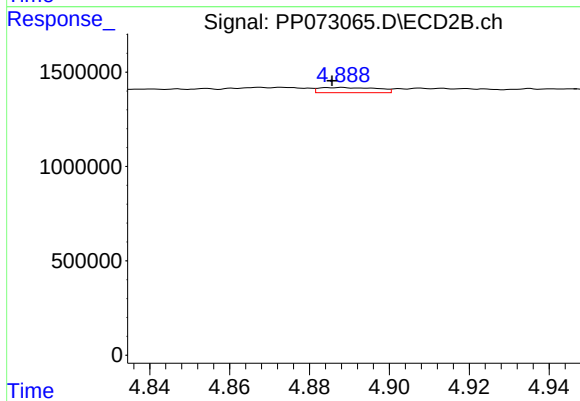

#4 AR-1016-2


R.T.: 4.888 min
Delta R.T.: 0.002 min
Response: 278801
Conc: 2.77 ng/ml

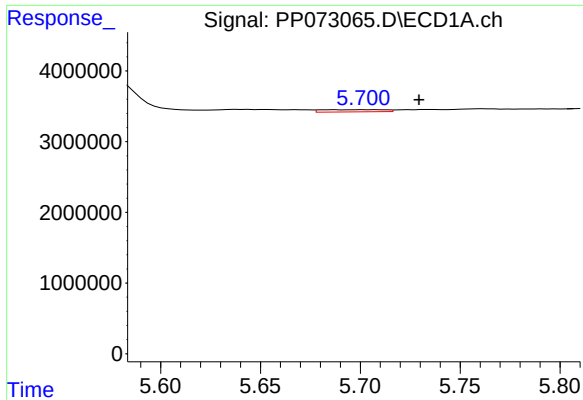

#5 AR-1016-3


R.T.: 5.702 min
Delta R.T.: -0.027 min
Response: 679858
Conc: 10.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

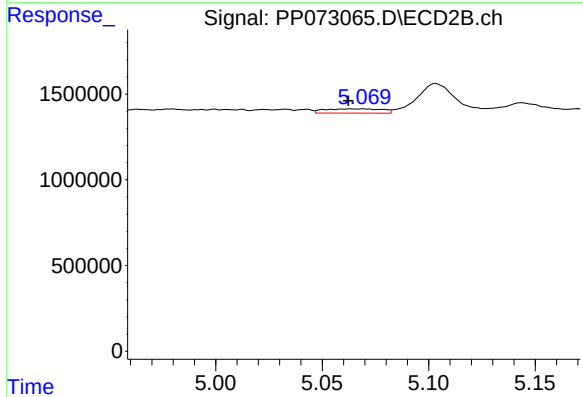


#5 AR-1016-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 476054
Conc: 8.70 ng/ml

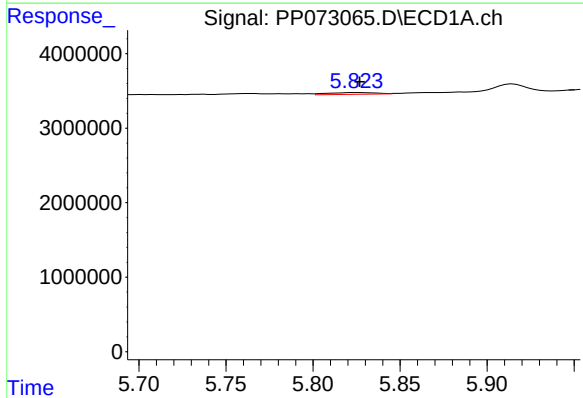


#6 AR-1016-4

R.T.: 5.825 min
Delta R.T.: -0.002 min
Response: 440171
Conc: 8.42 ng/ml

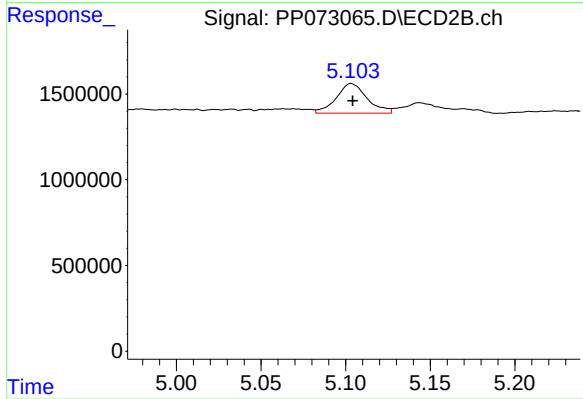

#6 AR-1016-4


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 2203512
Conc: 49.46 ng/ml

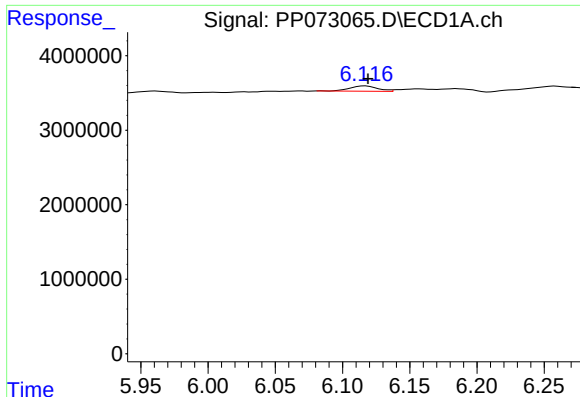

#7 AR-1016-5


R.T.: 6.117 min
Delta R.T.: -0.002 min
Response: 1031471
Conc: 20.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

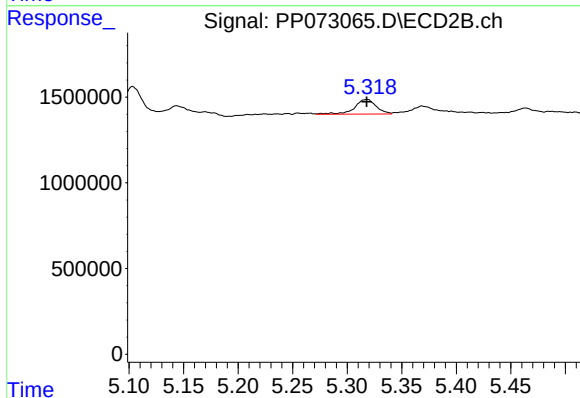


#7 AR-1016-5

R.T.: 5.318 min
Delta R.T.: 0.000 min
Response: 1189415
Conc: 21.52 ng/ml

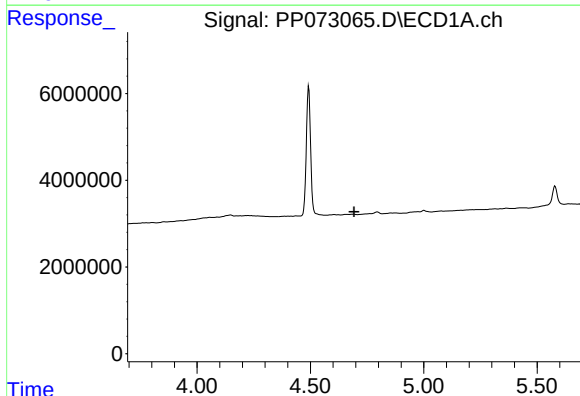


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.693 min
Response: 0
Conc: N.D.

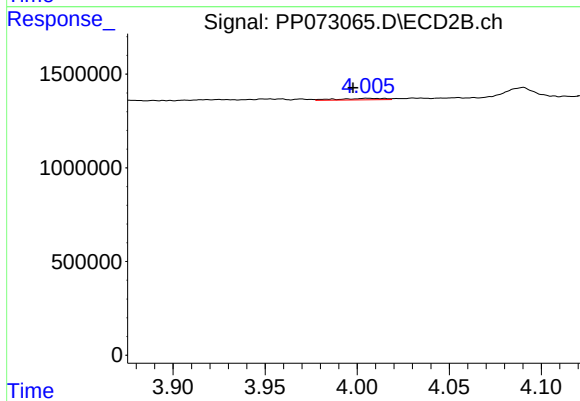

#8 AR-1221-1


R.T.: 4.006 min
Delta R.T.: 0.008 min
Response: 140578
Conc: 5.23 ng/ml

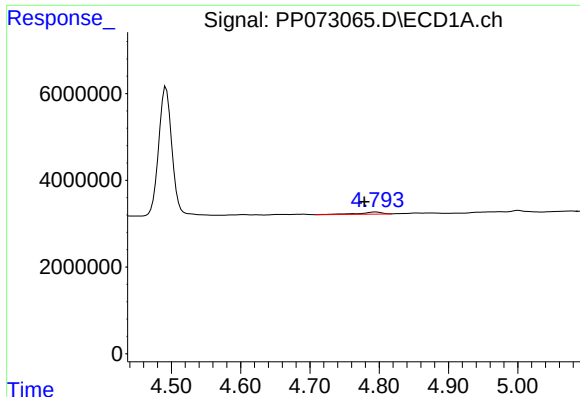

#9 AR-1221-2


R.T.: 4.795 min
Delta R.T.: 0.016 min
Response: 1059653
Conc: 52.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

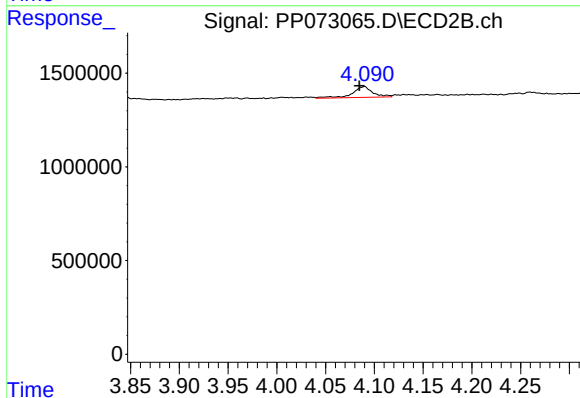


#9 AR-1221-2

R.T.: 4.090 min
Delta R.T.: 0.005 min
Response: 843200
Conc: 41.77 ng/ml

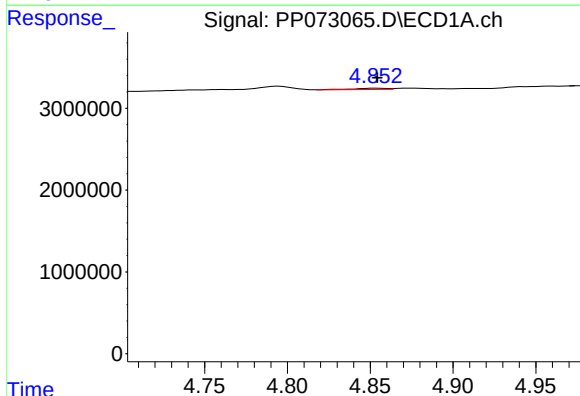


#10 AR-1221-3

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 223273
Conc: 3.63 ng/ml

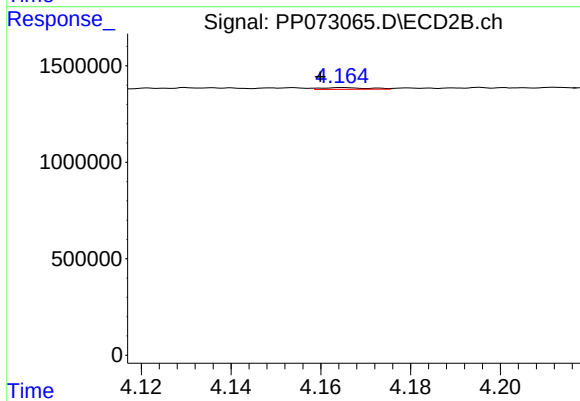

#10 AR-1221-3


R.T.: 4.165 min
Delta R.T.: 0.005 min
Response: 64127
Conc: 1.09 ng/ml

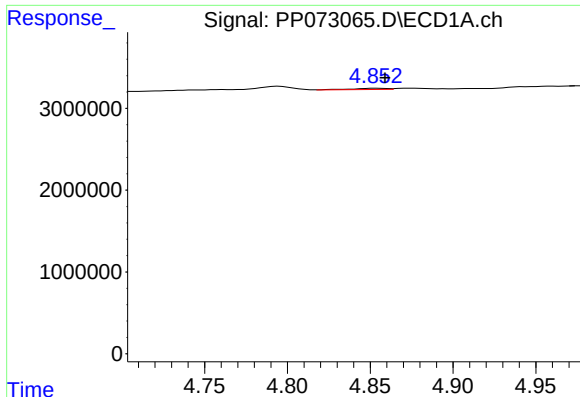

#11 AR-1232-1


R.T.: 4.854 min
Delta R.T.: -0.005 min
Response: 223273
Conc: 4.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

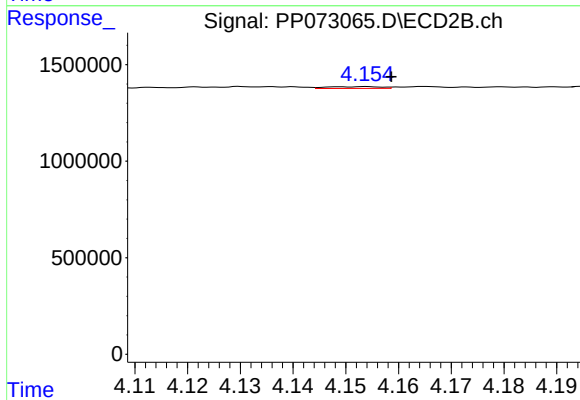


#11 AR-1232-1

R.T.: 4.154 min
Delta R.T.: -0.005 min
Response: 67257
Conc: 1.48 ng/ml

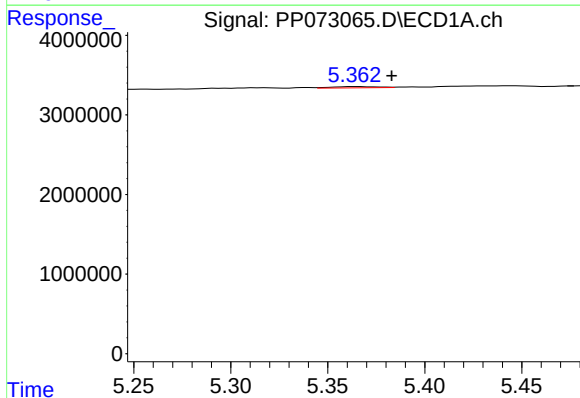


#12 AR-1232-2

R.T.: 5.364 min
Delta R.T.: -0.019 min
Response: 245340
Conc: 10.97 ng/ml

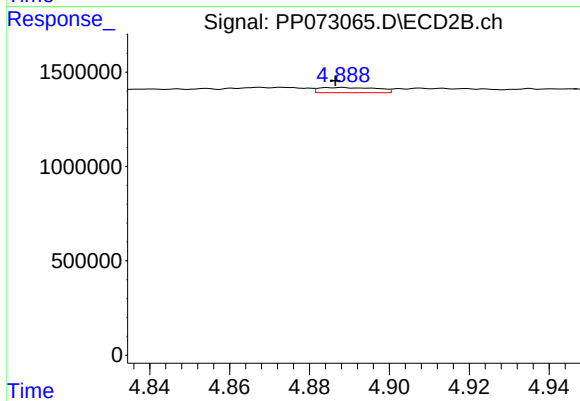

#12 AR-1232-2


R.T.: 4.888 min
Delta R.T.: 0.001 min
Response: 278801
Conc: 6.03 ng/ml

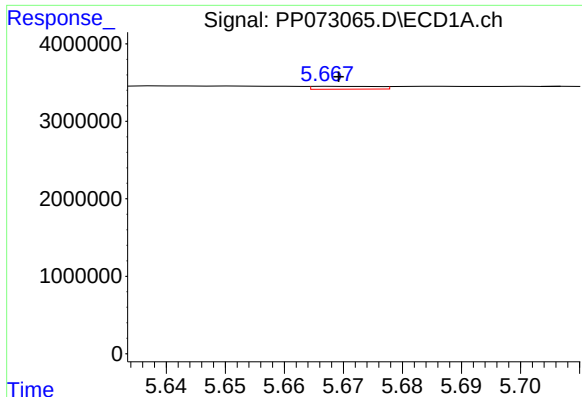

#13 AR-1232-3


R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 293060
Conc: 5.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

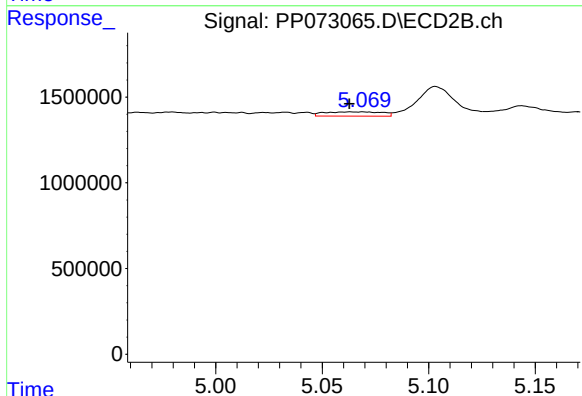


#13 AR-1232-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 476054
Conc: 19.38 ng/ml

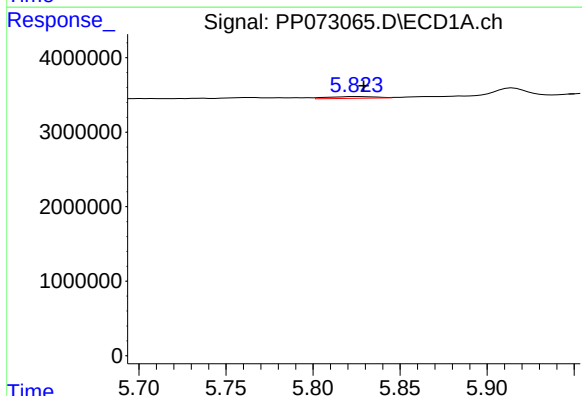


#14 AR-1232-4

R.T.: 5.825 min
Delta R.T.: -0.004 min
Response: 440171
Conc: 17.05 ng/ml

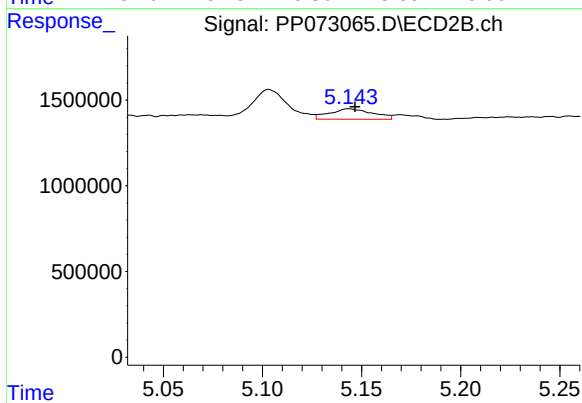

#14 AR-1232-4


R.T.: 5.144 min
Delta R.T.: -0.003 min
Response: 929796
Conc: 43.00 ng/ml

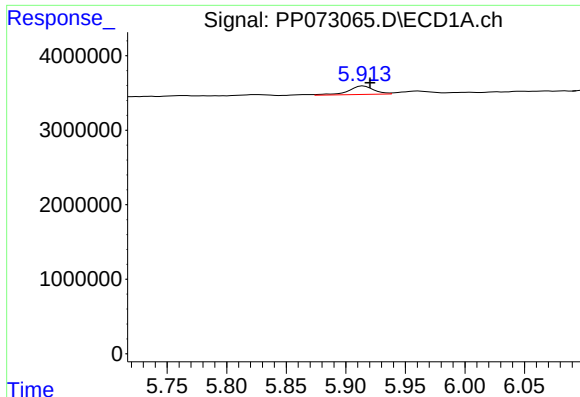

#15 AR-1232-5


R.T.: 5.915 min
Delta R.T.: -0.006 min
Response: 1723225
Conc: 48.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

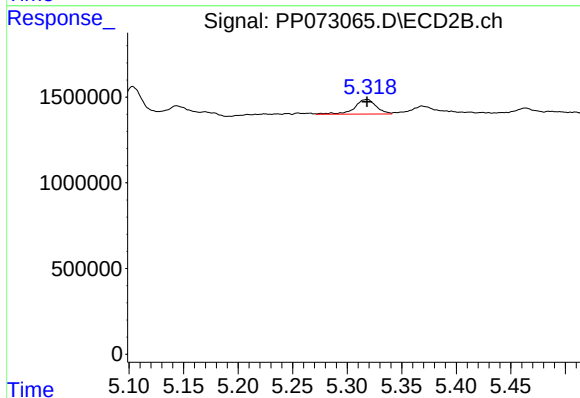


#15 AR-1232-5

R.T.: 5.318 min
Delta R.T.: 0.000 min
Response: 1189415
Conc: 52.03 ng/ml

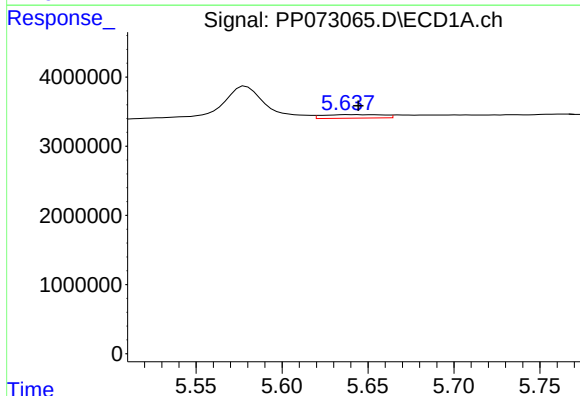


#16 AR-1242-1

R.T.: 5.639 min
Delta R.T.: -0.006 min
Response: 1238500
Conc: 21.19 ng/ml

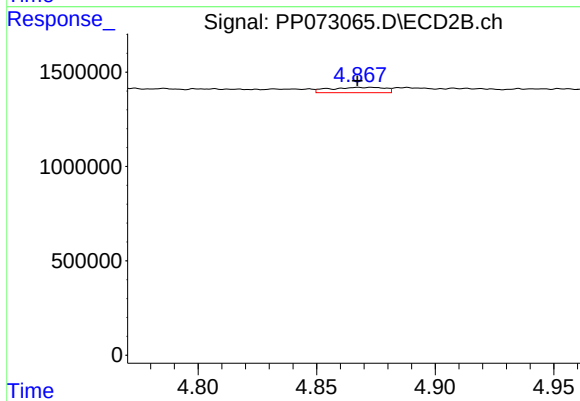

#16 AR-1242-1


R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 456523
Conc: 8.27 ng/ml

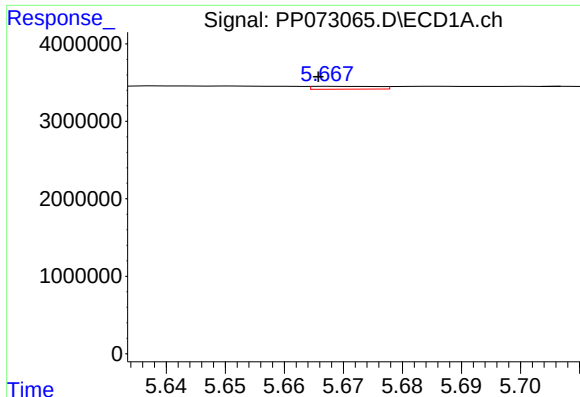

#17 AR-1242-2


R.T.: 5.669 min
Delta R.T.: 0.003 min
Response: 293060
Conc: 3.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

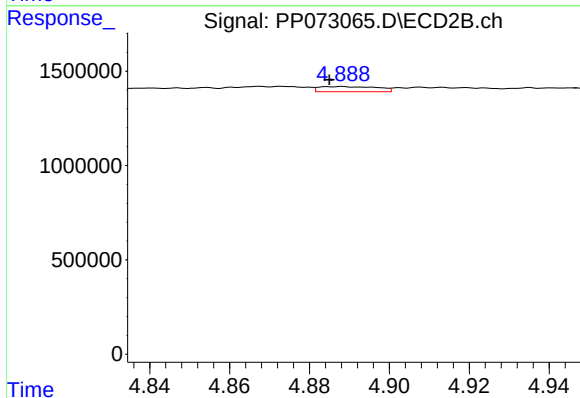


#17 AR-1242-2

R.T.: 4.888 min
Delta R.T.: 0.003 min
Response: 278801
Conc: 3.51 ng/ml

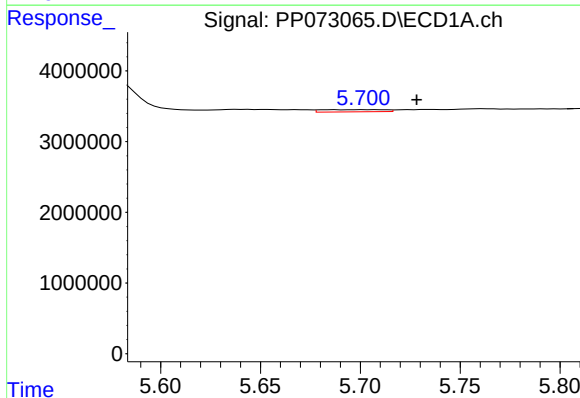


#18 AR-1242-3

R.T.: 5.702 min
Delta R.T.: -0.026 min
Response: 679858
Conc: 12.90 ng/ml

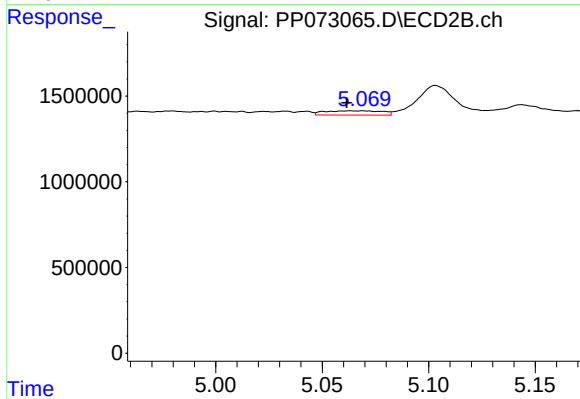

#18 AR-1242-3


R.T.: 5.063 min
Delta R.T.: 0.002 min
Response: 476054
Conc: 10.99 ng/ml

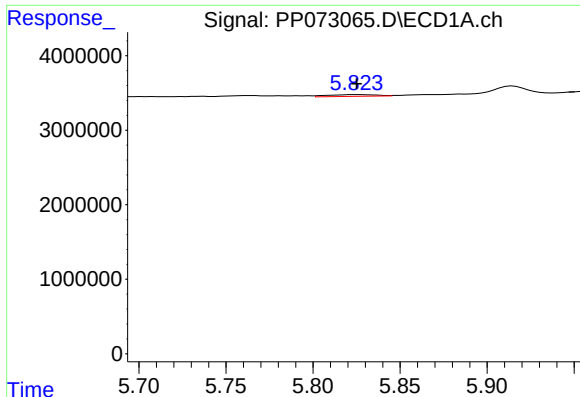

#19 AR-1242-4


R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 440171
Conc: 10.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

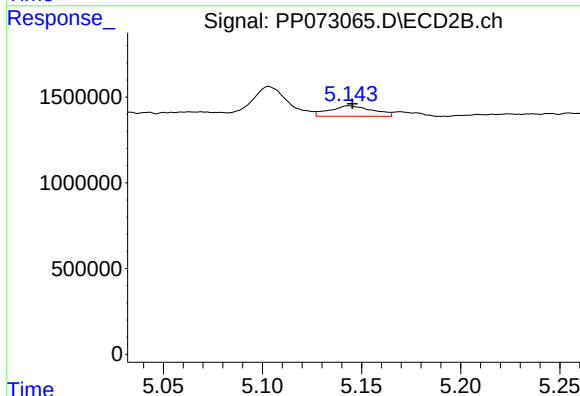


#19 AR-1242-4

R.T.: 5.144 min
Delta R.T.: -0.002 min
Response: 929796
Conc: 22.40 ng/ml

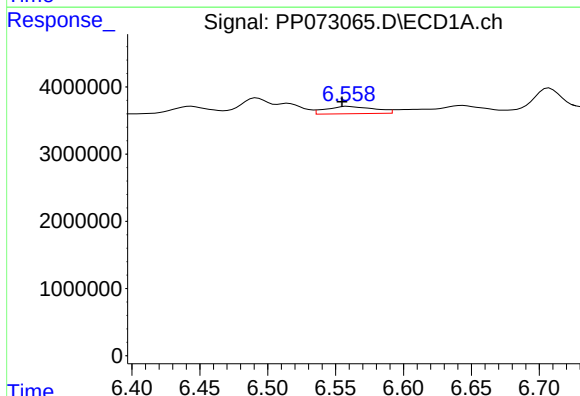


#20 AR-1242-5

R.T.: 6.559 min
Delta R.T.: 0.005 min
Response: 2729899
Conc: 55.08 ng/ml

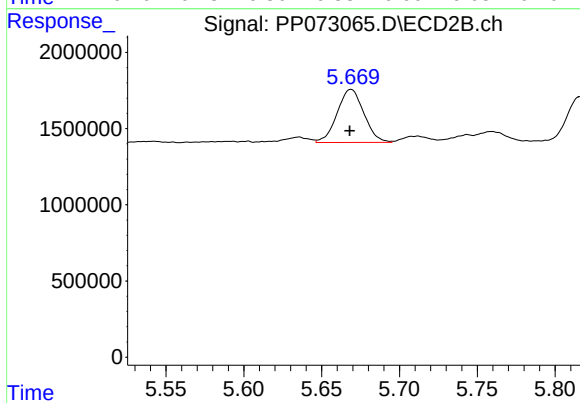

#20 AR-1242-5


R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 4157471
Conc: 79.06 ng/ml

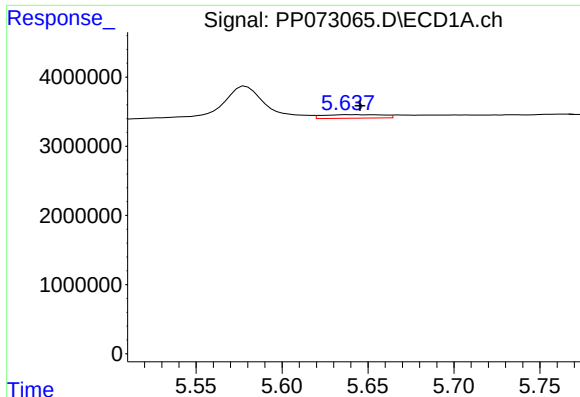

#21 AR-1248-1


R.T.: 5.639 min
Delta R.T.: -0.007 min
Response: 1238500
Conc: 26.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

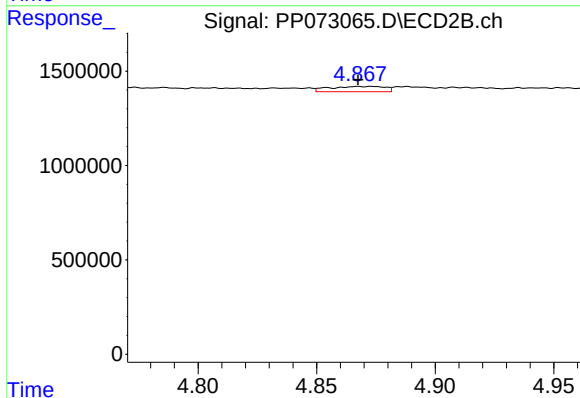


#21 AR-1248-1

R.T.: 4.868 min
Delta R.T.: 0.000 min
Response: 456523
Conc: 10.47 ng/ml

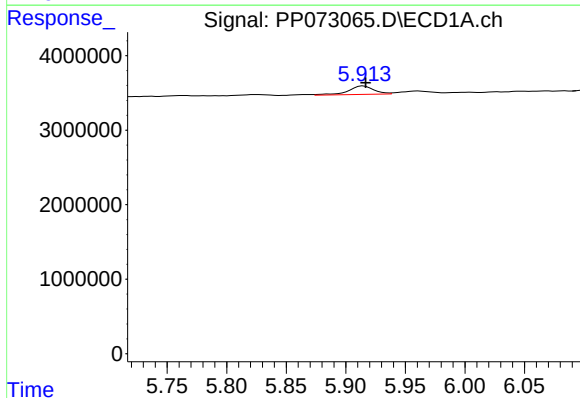


#22 AR-1248-2

R.T.: 5.915 min
Delta R.T.: -0.002 min
Response: 1723225
Conc: 29.43 ng/ml

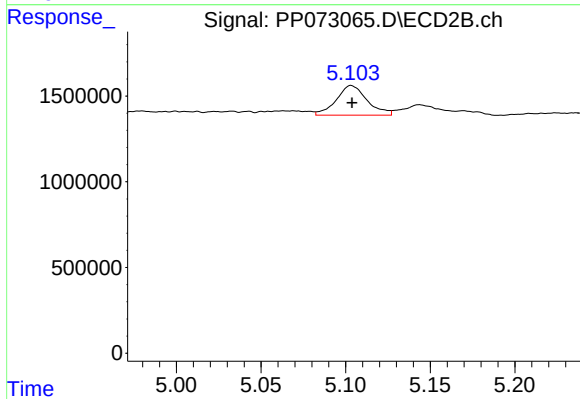

#22 AR-1248-2


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 2203512
Conc: 37.61 ng/ml

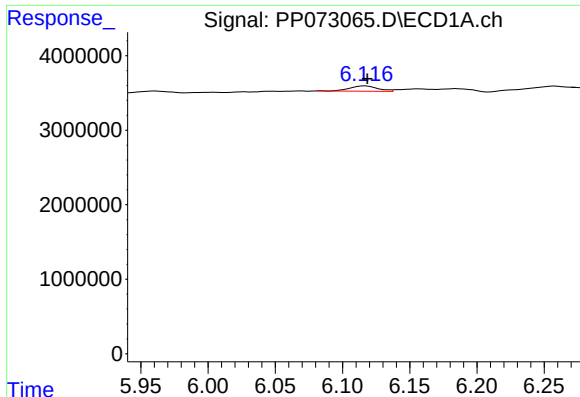

#23 AR-1248-3


R.T.: 6.117 min
Delta R.T.: -0.002 min
Response: 1031471
Conc: 15.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

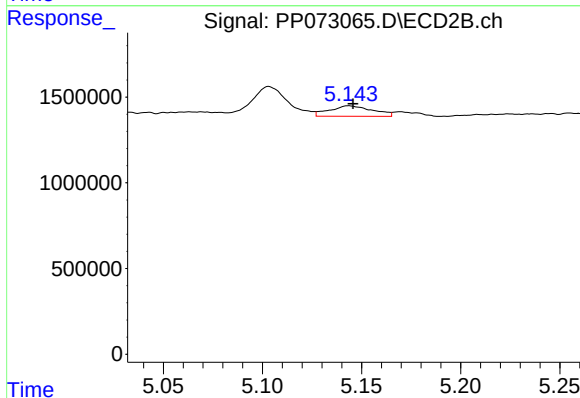


#23 AR-1248-3

R.T.: 5.144 min
Delta R.T.: -0.002 min
Response: 929796
Conc: 15.36 ng/ml

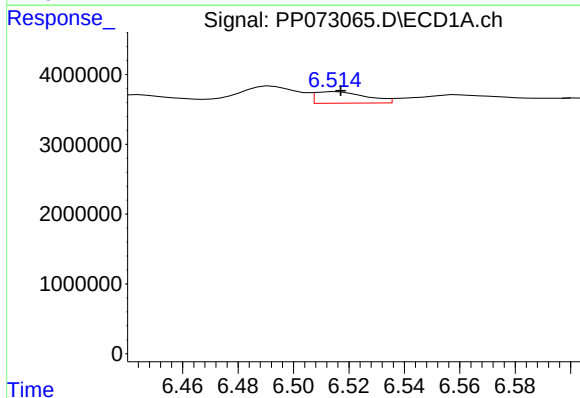


#24 AR-1248-4

R.T.: 6.515 min
Delta R.T.: -0.002 min
Response: 2125926
Conc: 24.99 ng/ml

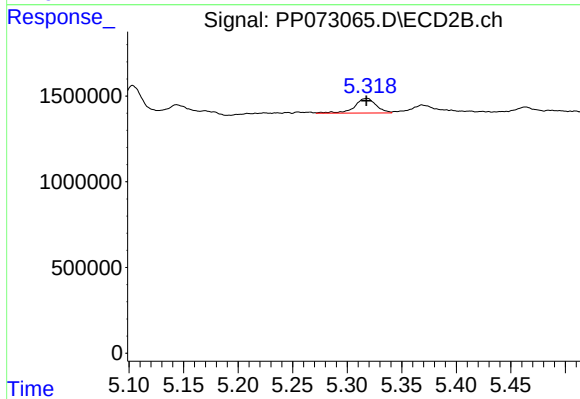

#24 AR-1248-4


R.T.: 5.318 min
Delta R.T.: 0.000 min
Response: 1189415
Conc: 16.99 ng/ml

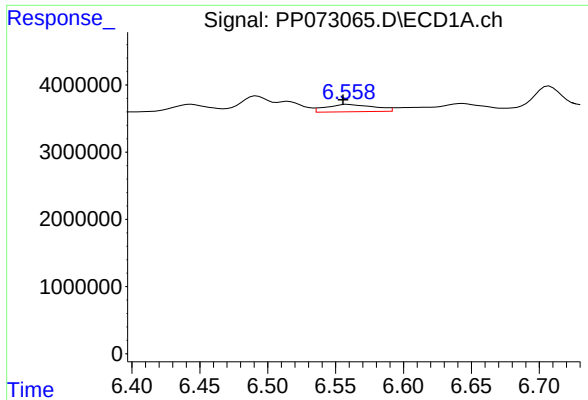

#25 AR-1248-5


R.T.: 6.559 min
Delta R.T.: 0.004 min
Response: 2729899
Conc: 32.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

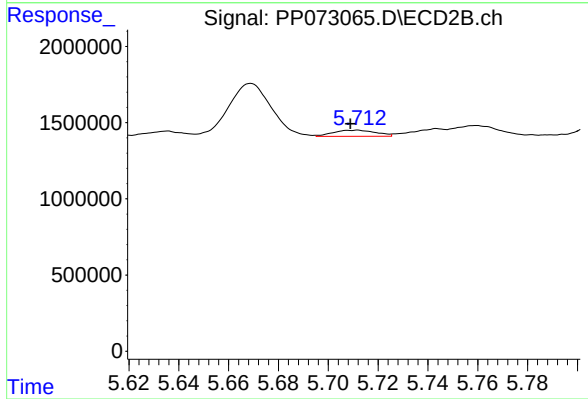


#25 AR-1248-5

R.T.: 5.711 min
Delta R.T.: 0.002 min
Response: 476549
Conc: 6.71 ng/ml

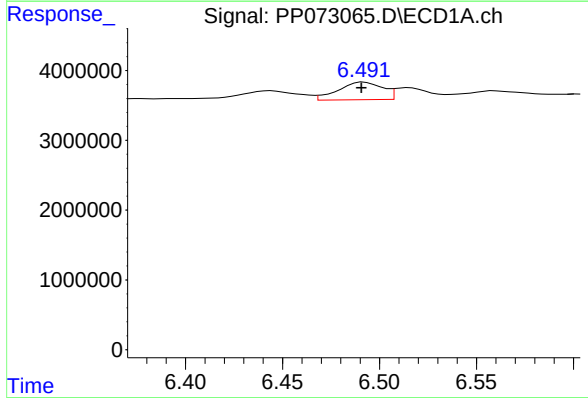


#26 AR-1254-1

R.T.: 6.492 min
Delta R.T.: 0.001 min
Response: 3996739
Conc: 47.48 ng/ml

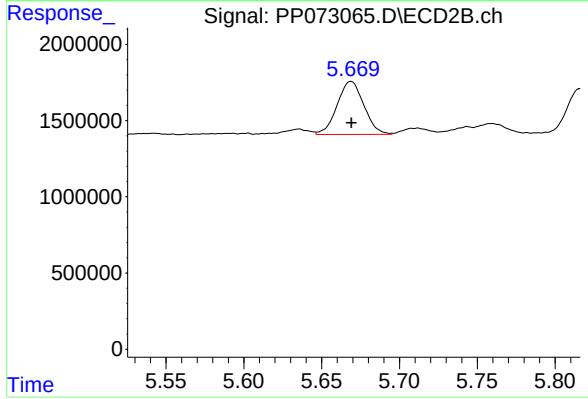

#26 AR-1254-1


R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 4157471
Conc: 37.92 ng/ml

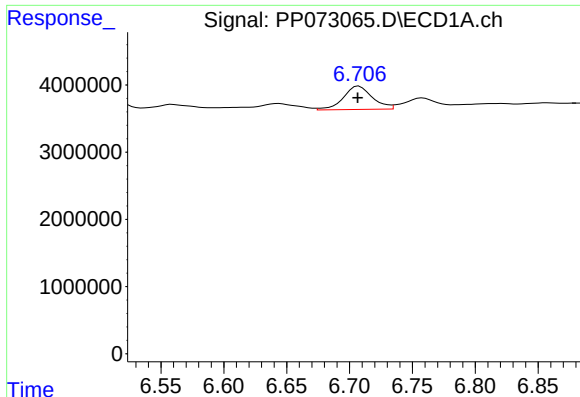

#27 AR-1254-2


R.T.: 6.707 min
Delta R.T.: 0.000 min
Response: 5568712
Conc: 44.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

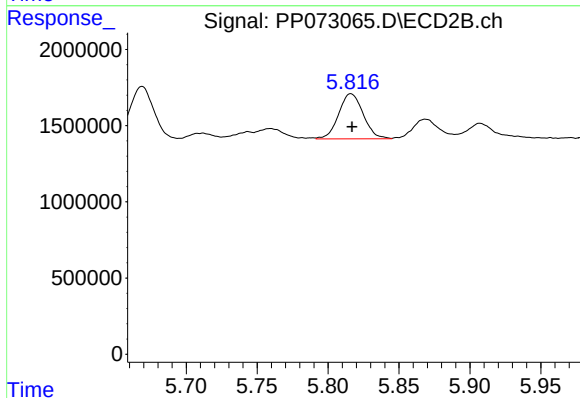


#27 AR-1254-2

R.T.: 5.816 min
Delta R.T.: 0.000 min
Response: 3582429
Conc: 37.89 ng/ml

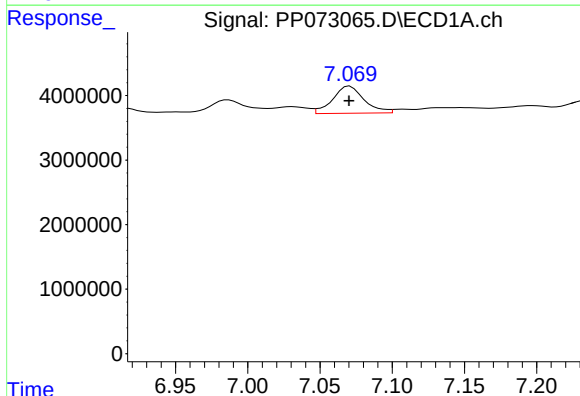


#28 AR-1254-3

R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 6387930
Conc: 48.68 ng/ml

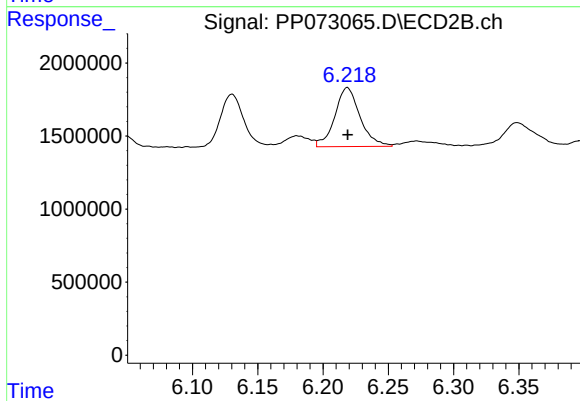

#28 AR-1254-3


R.T.: 6.219 min
Delta R.T.: 0.000 min
Response: 5428100
Conc: 36.79 ng/ml

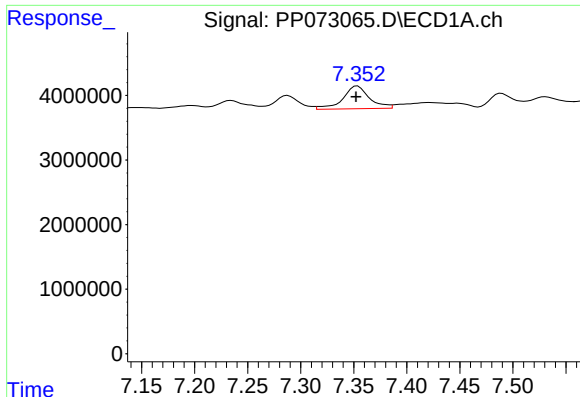

#29 AR-1254-4


R.T.: 7.354 min
Delta R.T.: 0.002 min
Response: 6127718
Conc: 51.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

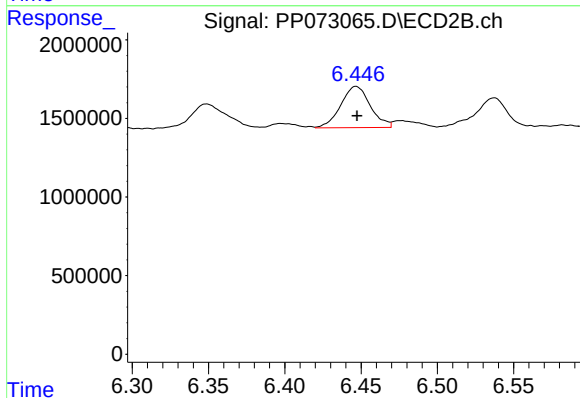


#29 AR-1254-4

R.T.: 6.447 min
Delta R.T.: 0.000 min
Response: 3534580
Conc: 36.40 ng/ml

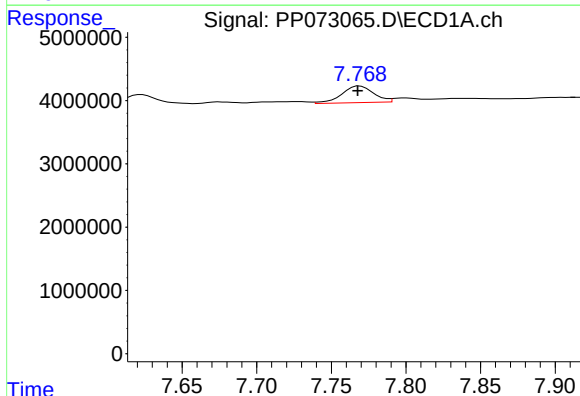


#30 AR-1254-5

R.T.: 7.769 min
Delta R.T.: 0.001 min
Response: 3897993
Conc: 34.12 ng/ml

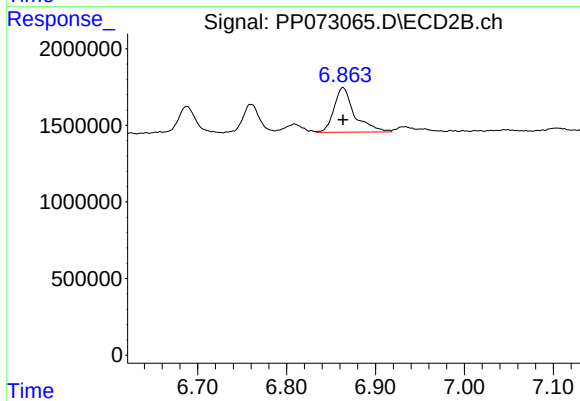

#30 AR-1254-5


R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 4671148
Conc: 35.94 ng/ml

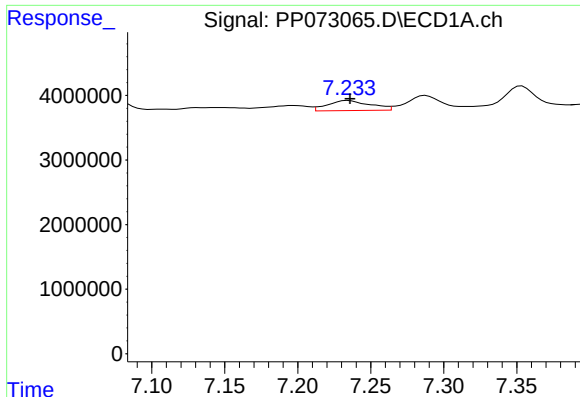

#31 AR-1260-1


R.T.: 7.235 min
Delta R.T.: -0.001 min
Response: 3206877
Conc: 36.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

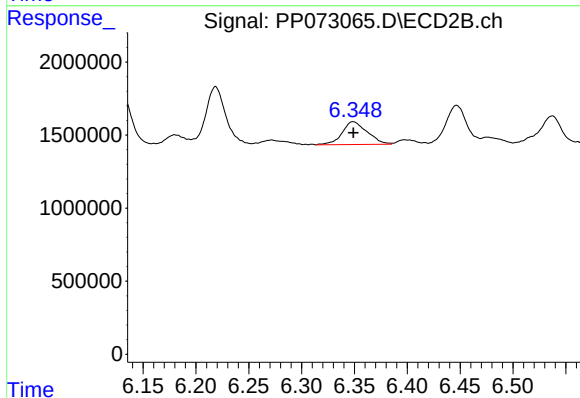


#31 AR-1260-1

R.T.: 6.349 min
Delta R.T.: 0.000 min
Response: 2574267
Conc: 27.17 ng/ml

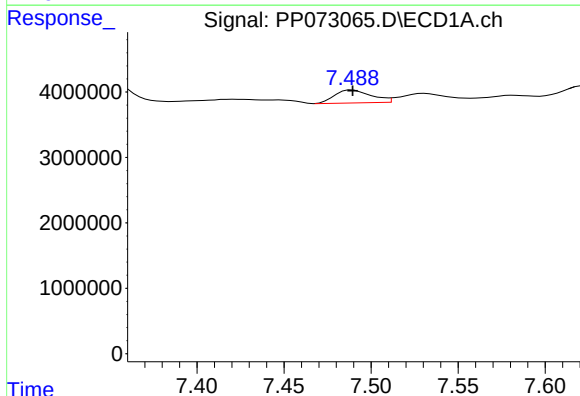


#32 AR-1260-2

R.T.: 7.489 min
Delta R.T.: 0.000 min
Response: 2890104
Conc: 21.27 ng/ml

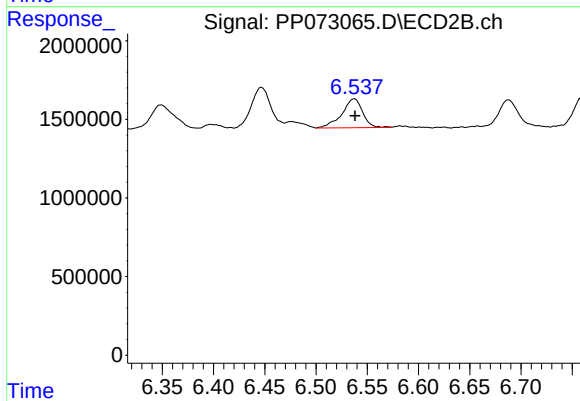

#32 AR-1260-2


R.T.: 6.537 min
Delta R.T.: 0.000 min
Response: 2597800
Conc: 22.31 ng/ml

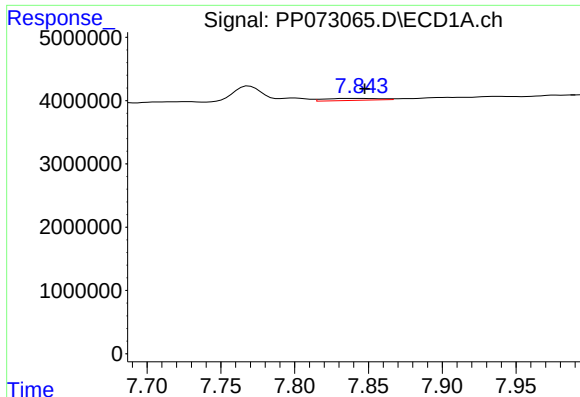

#33 AR-1260-3


R.T.: 7.845 min
Delta R.T.: -0.002 min
Response: 839598
Conc: 7.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

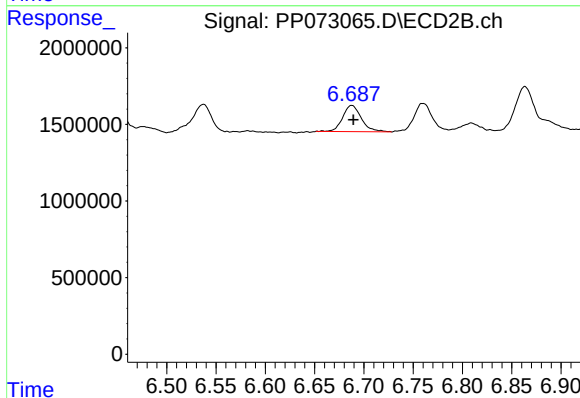


#33 AR-1260-3

R.T.: 6.688 min
Delta R.T.: -0.002 min
Response: 2240917
Conc: 21.51 ng/ml

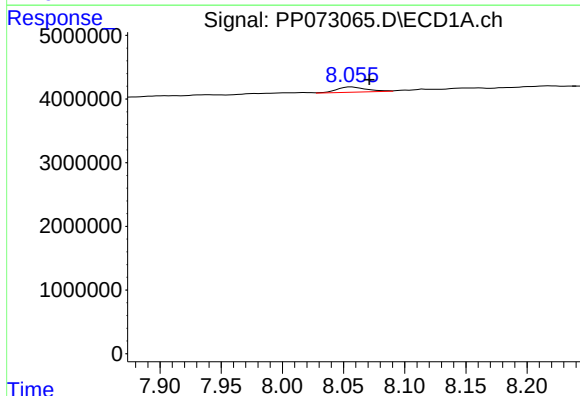


#34 AR-1260-4

R.T.: 8.056 min
Delta R.T.: -0.015 min
Response: 1356842
Conc: 13.17 ng/ml

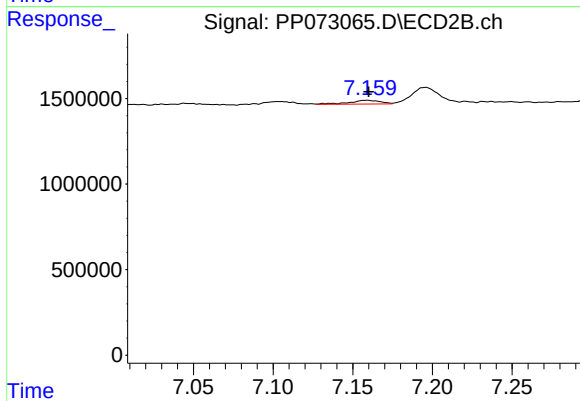

#34 AR-1260-4


R.T.: 7.159 min
Delta R.T.: -0.001 min
Response: 302245
Conc: 3.44 ng/ml

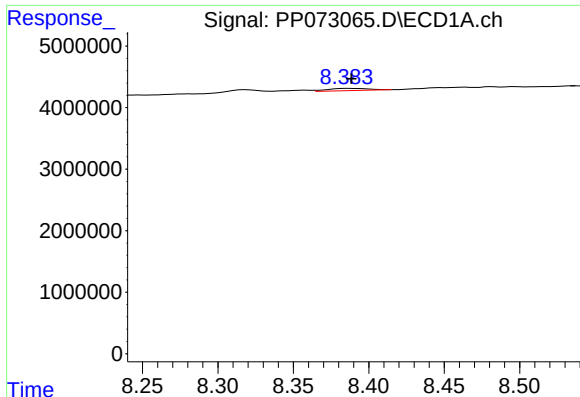

#35 AR-1260-5


R.T.: 8.386 min
Delta R.T.: -0.002 min
Response: 690002
Conc: 2.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

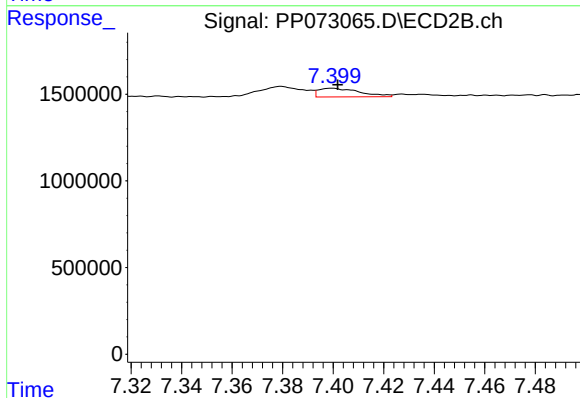


#35 AR-1260-5

R.T.: 7.400 min
Delta R.T.: -0.002 min
Response: 565968
Conc: 2.65 ng/ml

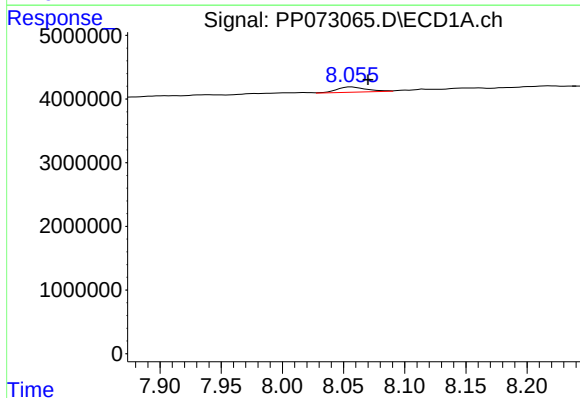


#36 AR-1262-1

R.T.: 8.056 min
Delta R.T.: -0.014 min
Response: 1356842
Conc: 9.17 ng/ml

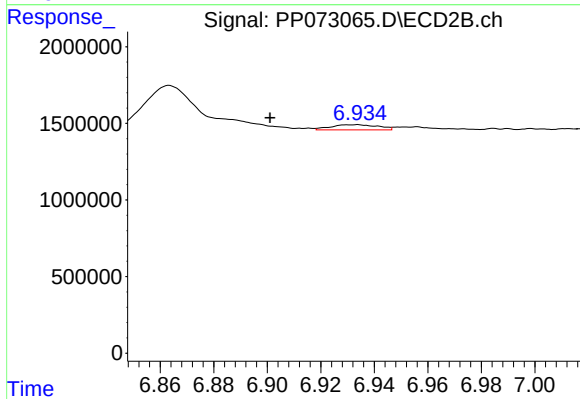

#36 AR-1262-1


R.T.: 6.933 min
Delta R.T.: 0.032 min
Response: 416639
Conc: 2.88 ng/ml

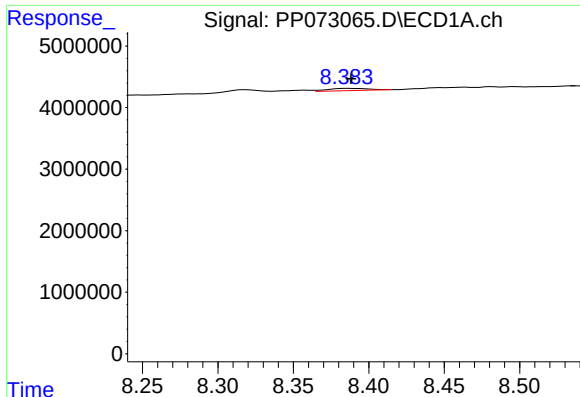

#37 AR-1262-2


R.T.: 8.386 min
Delta R.T.: -0.002 min
Response: 690002
Conc: 2.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

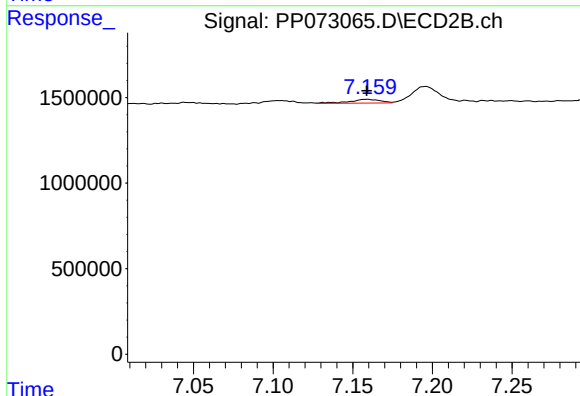


#37 AR-1262-2

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 302245
Conc: 2.47 ng/ml

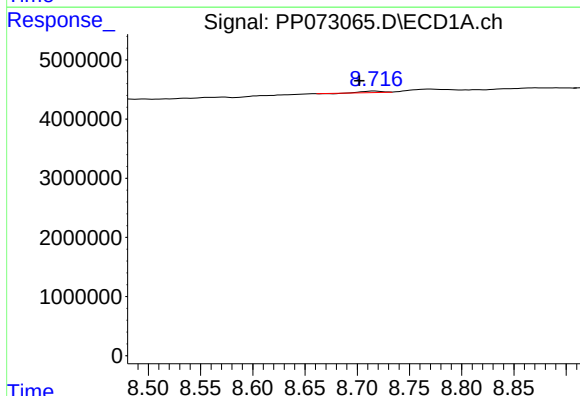


#38 AR-1262-3

R.T.: 8.717 min
Delta R.T.: 0.015 min
Response: 305915
Conc: 1.43 ng/ml

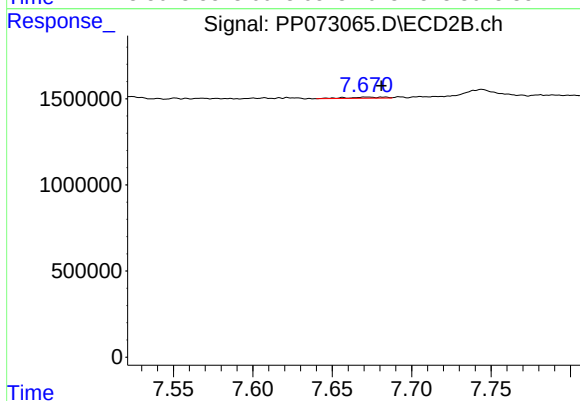

#38 AR-1262-3


R.T.: 7.671 min
Delta R.T.: -0.009 min
Response: 106137
Conc: 0.94 ng/ml

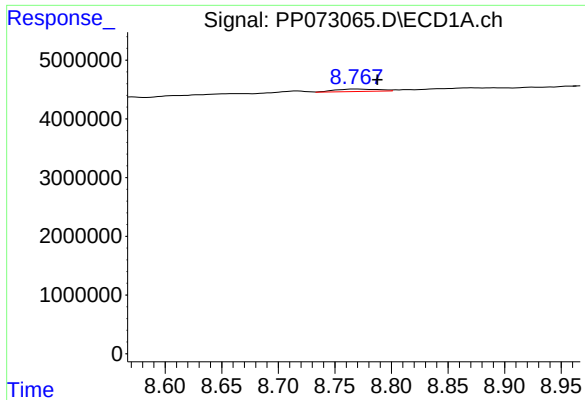

#39 AR-1262-4


R.T.: 8.768 min
Delta R.T.: -0.019 min
Response: 1114948
Conc: 7.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

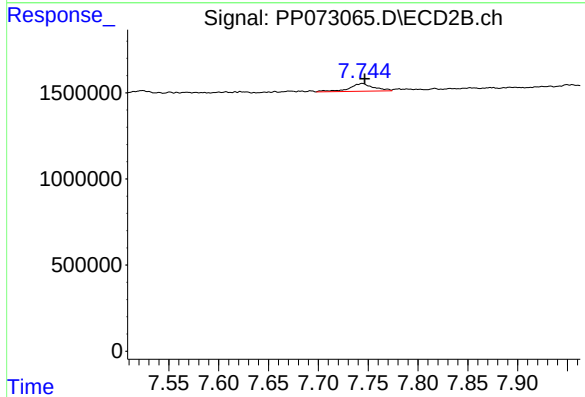


#39 AR-1262-4

R.T.: 7.744 min
Delta R.T.: -0.002 min
Response: 760157
Conc: 4.15 ng/ml

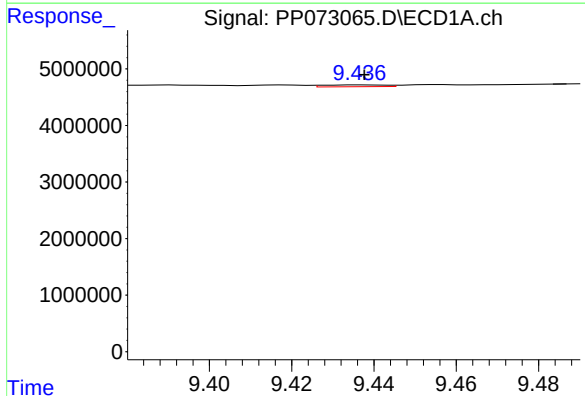


#40 AR-1262-5

R.T.: 9.437 min
Delta R.T.: 0.000 min
Response: 339219
Conc: 3.03 ng/ml

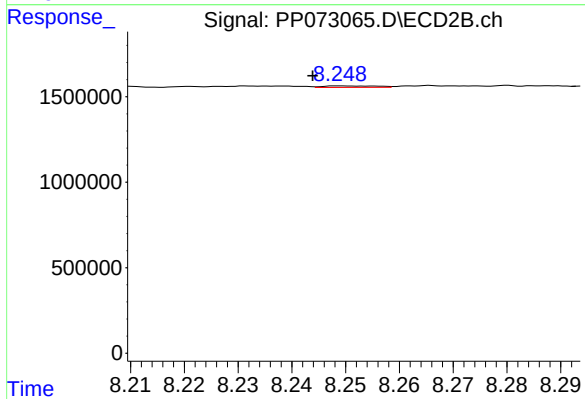

#40 AR-1262-5


R.T.: 8.250 min
Delta R.T.: 0.006 min
Response: 59166
Conc: 0.68 ng/ml

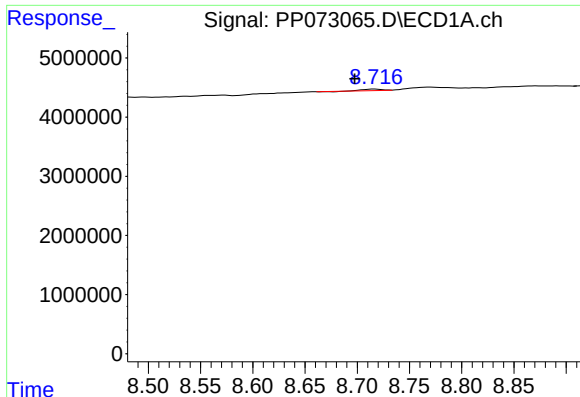

#41 AR-1268-1


R.T.: 8.717 min
Delta R.T.: 0.019 min
Response: 305915
Conc: 0.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

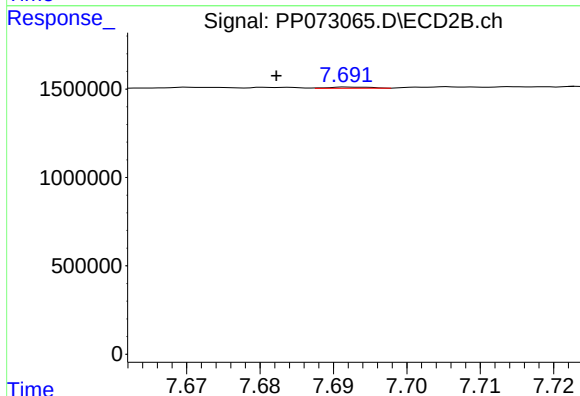


#41 AR-1268-1

R.T.: 7.693 min
Delta R.T.: 0.010 min
Response: 26017
Conc: 0.09 ng/ml

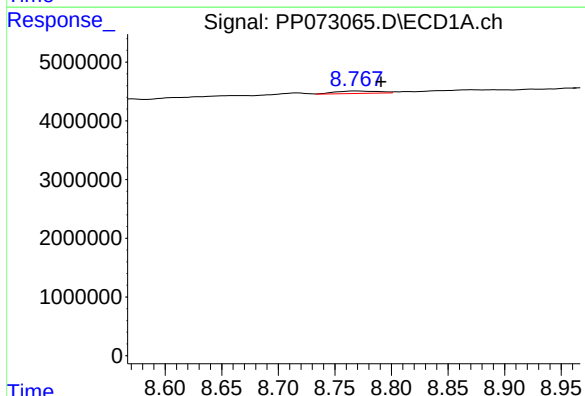


#42 AR-1268-2

R.T.: 8.768 min
Delta R.T.: -0.022 min
Response: 1114948
Conc: 3.65 ng/ml

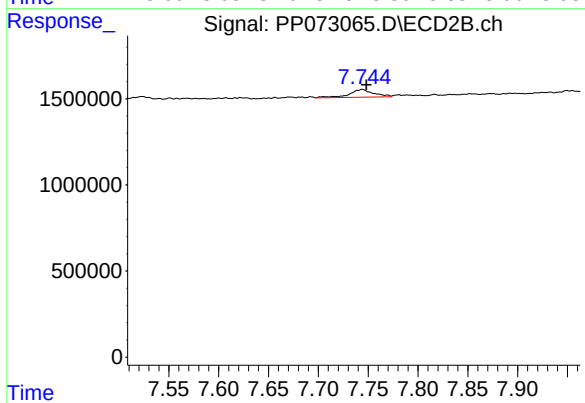

#42 AR-1268-2


R.T.: 7.744 min
Delta R.T.: -0.004 min
Response: 760157
Conc: 2.96 ng/ml

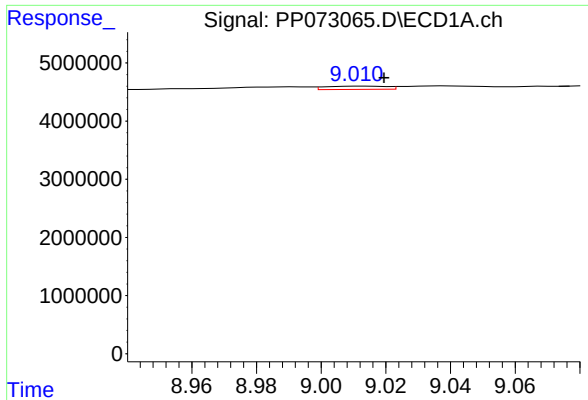

#43 AR-1268-3


R.T.: 9.012 min
Delta R.T.: -0.007 min
Response: 729589
Conc: 2.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

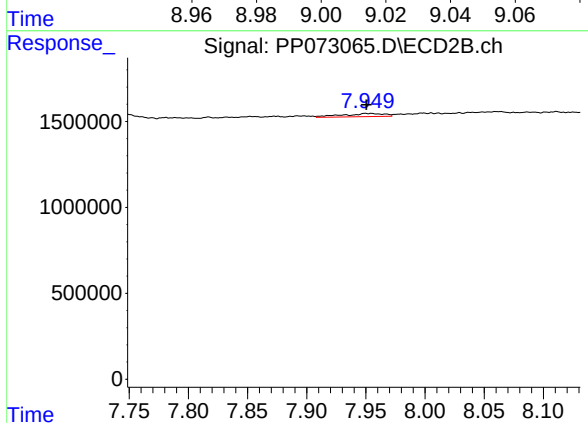


#43 AR-1268-3

R.T.: 7.955 min
Delta R.T.: 0.004 min
Response: 457418
Conc: 2.12 ng/ml

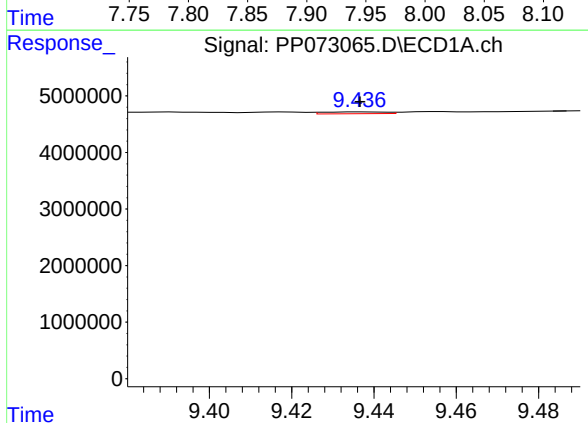


#44 AR-1268-4

R.T.: 9.437 min
Delta R.T.: 0.000 min
Response: 339219
Conc: 2.90 ng/ml

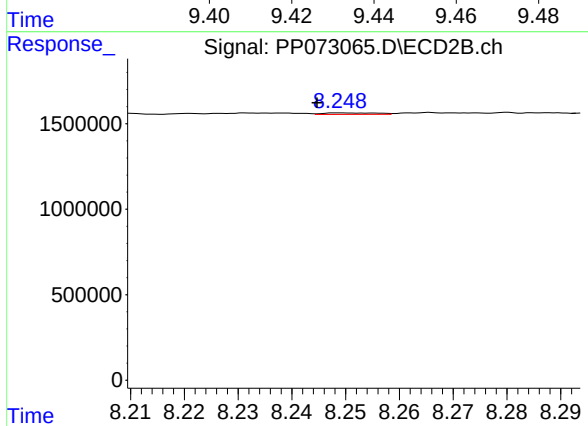

#44 AR-1268-4


R.T.: 8.250 min
Delta R.T.: 0.005 min
Response: 59166
Conc: 0.63 ng/ml

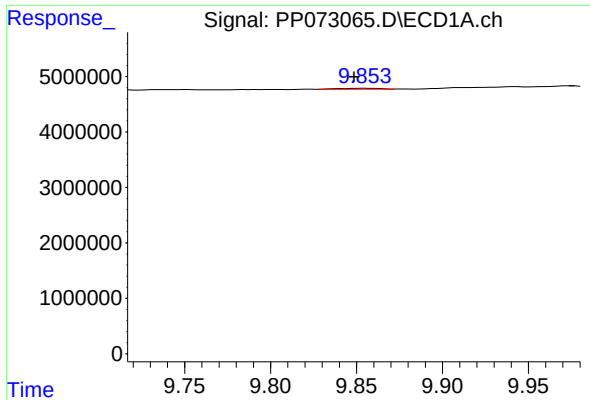

#45 AR-1268-5

R.T.: 9.855 min
Delta R.T.: 0.006 min
Response: 284693
Conc: 0.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

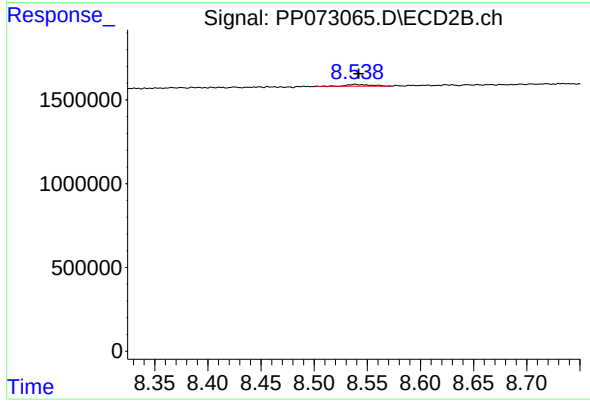

#45 AR-1268-5

R.T.: 8.539 min
Delta R.T.: -0.003 min
Response: 161977
Conc: 0.28 ng/ml