

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
 Data File : PP073066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 00:25
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:44:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.491	3.788	39751211	34007503	18.832	18.874
2)	SA Decachlor...	10.184	8.797	35598101	26569351	20.831	19.906
Target Compounds							
3)	L1 AR-1016-1	5.645	4.885	414001	413762	5.697	6.021
4)	L1 AR-1016-2	5.663	4.885	955814	413762	9.189	4.111 #
5)	L1 AR-1016-3	5.736	5.061	188329	185449	2.882	3.389
6)	L1 AR-1016-4	5.848	5.104	153518	156293	2.936	3.508
7)	L1 AR-1016-5	6.074f	5.317	177629	221886	3.552	4.014
8)	L2 AR-1221-1	4.753f	4.005	163156	87285	6.616	3.248 #
9)	L2 AR-1221-2	4.793	4.089	721697	743409	35.765	36.829
10)	L2 AR-1221-3	4.843	4.170	108497	241618	1.763	4.114 #
11)	L3 AR-1232-1	4.870	4.170	171758	241618	3.658	5.303 #
12)	L3 AR-1232-2	5.375	4.885	218143	413762	9.752	8.944
13)	L3 AR-1232-3	5.663	5.061	955814	185449	18.524	7.552 #
14)	L3 AR-1232-4	5.848	5.104f	153518	156293	5.948	7.227
15)	L3 AR-1232-5	5.914	5.317	281308	221886	7.886	9.707
16)	L4 AR-1242-1	5.645	4.885	414001	413762	7.085	7.493
17)	L4 AR-1242-2	5.663	4.885	955814	413762	11.043	5.205 #
18)	L4 AR-1242-3	5.736	5.061	188329	185449	3.573	4.282
19)	L4 AR-1242-4	5.848	5.104f	153518	156293	3.492	3.766
20)	L4 AR-1242-5	6.552	5.669	1086033	837375	21.914	15.924 #
21)	L5 AR-1248-1	5.645	4.885	414001	413762	8.703	9.492
22)	L5 AR-1248-2	5.914	5.104	281308	156293	4.804	2.667 #
23)	L5 AR-1248-3	6.074f	5.104f	177629	156293	2.722	2.581
24)	L5 AR-1248-4	6.526	5.317	766589	221886	9.012	3.169 #
25)	L5 AR-1248-5	6.552	5.669f	1086033	837375	12.976	11.789
26)	L6 AR-1254-1	6.490	5.669	2551592	837375	30.313	7.637 #
27)	L6 AR-1254-2	6.707	5.816	1773325	859719	14.141	9.093 #
28)	L6 AR-1254-3	7.069	6.234	2209790	2328305	16.842	15.780
29)	L6 AR-1254-4	7.356	6.433	1898529	406826	15.850	4.190 #
30)	L6 AR-1254-5	7.764	6.862	3509975	2455393	30.720	18.893 #
31)	L7 AR-1260-1	7.234	6.349	4124848	3162784	46.760	33.387 #
32)	L7 AR-1260-2	7.487	6.537	4601046	4020010	33.860	34.525
33)	L7 AR-1260-3	7.845	6.690	6166747	3579921	54.022	34.369 #
34)	L7 AR-1260-4	8.069	7.158	4359650	4442642	42.308	50.635
35)	L7 AR-1260-5	8.386	7.401	9955308	8529122	41.373	39.968
36)	L8 AR-1262-1	8.069	6.901	4359650	5334759	29.453	36.927 #
37)	L8 AR-1262-2	8.386	7.158	9955308	4442642	31.458	36.346
38)	L8 AR-1262-3	8.700	7.681	6387649	3950152	29.853	35.049
39)	L8 AR-1262-4	8.786	7.746	4678216	6516355	29.685	35.539
40)	L8 AR-1262-5	9.436	8.245	3458274	3341879	30.915	38.596
41)	L9 AR-1268-1	8.700	7.681	6387649	3950152	17.861	13.751

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061825\
Data File : PP073066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 00:25
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 39 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:44:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.786	7.746	4678216	6516355	15.335	25.344 #
43)	L9 AR-1268-3	9.018	7.951	1089963	1316757	4.105	6.098 #
44)	L9 AR-1268-4	9.436	8.245	3458274	3341879	29.552	35.482
45)	L9 AR-1268-5	9.848	8.540	1021346	1061976	1.381	1.835 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

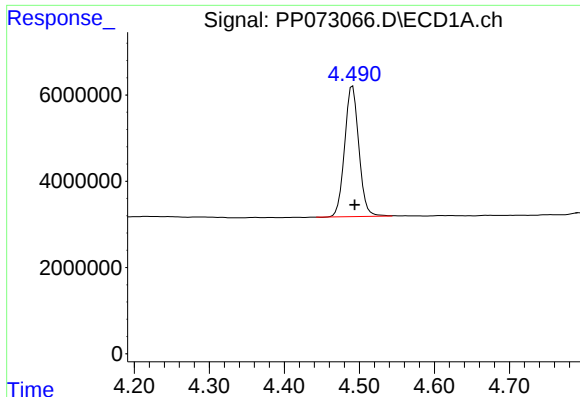

#1 Tetrachloro-m-xylene


R.T.: 4.491 min
Delta R.T.: -0.003 min
Response: 39751211
Conc: 18.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

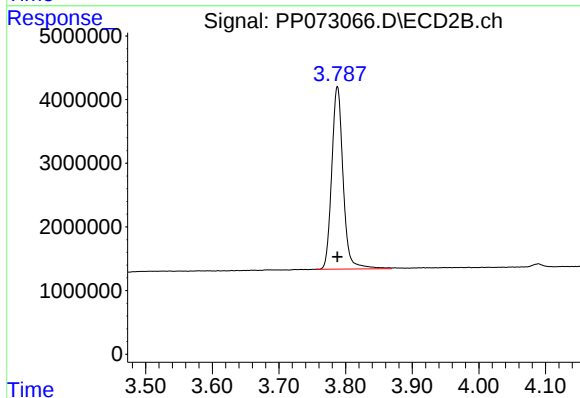


#1 Tetrachloro-m-xylene

R.T.: 3.788 min
Delta R.T.: 0.000 min
Response: 34007503
Conc: 18.87 ng/ml

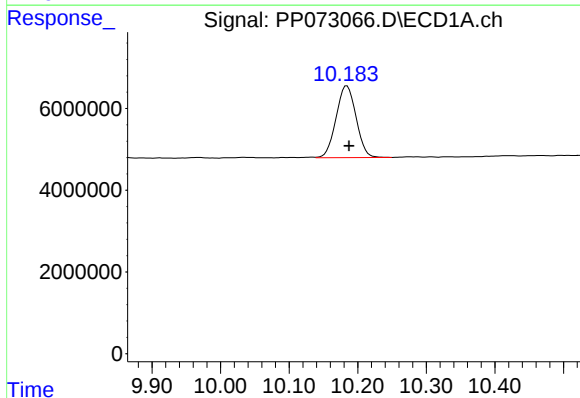


#2 Decachlorobiphenyl

R.T.: 10.184 min
Delta R.T.: -0.003 min
Response: 35598101
Conc: 20.83 ng/ml

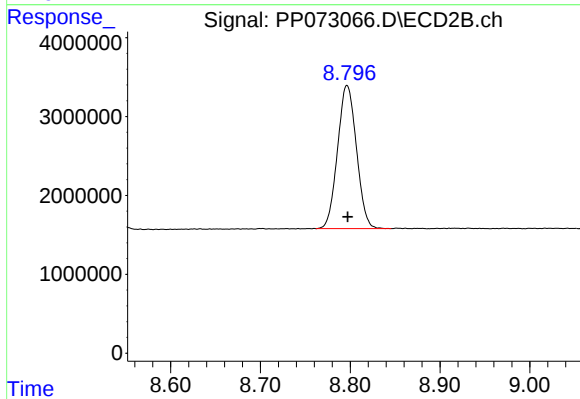

#2 Decachlorobiphenyl


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 26569351
Conc: 19.91 ng/ml

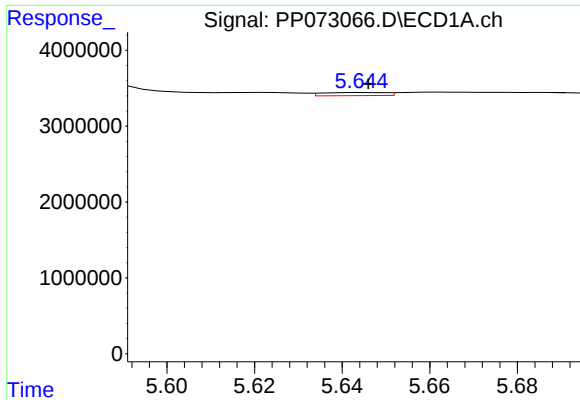

#3 AR-1016-1


R.T.: 5.645 min
Delta R.T.: 0.000 min
Response: 414001
Conc: 5.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

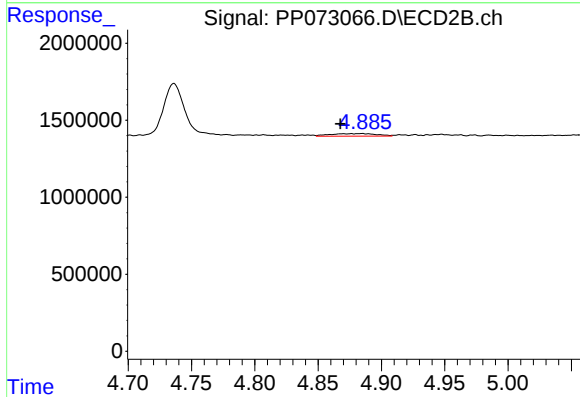


#3 AR-1016-1

R.T.: 4.885 min
Delta R.T.: 0.017 min
Response: 413762
Conc: 6.02 ng/ml

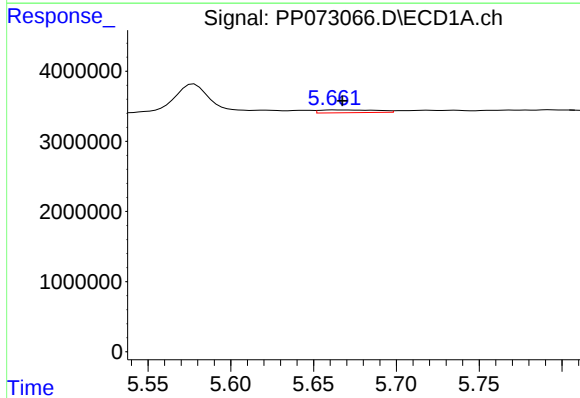


#4 AR-1016-2

R.T.: 5.663 min
Delta R.T.: -0.004 min
Response: 955814
Conc: 9.19 ng/ml

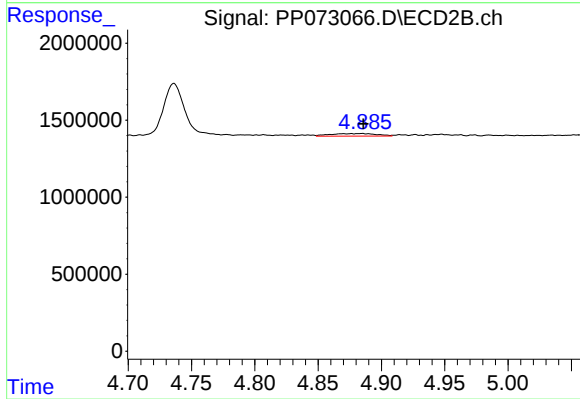

#4 AR-1016-2


R.T.: 4.885 min
Delta R.T.: -0.001 min
Response: 413762
Conc: 4.11 ng/ml

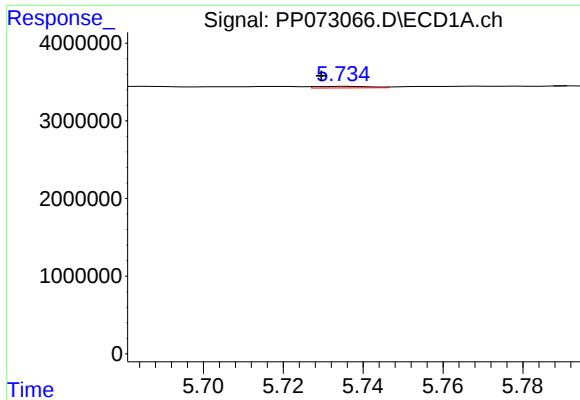

#5 AR-1016-3


R.T.: 5.736 min
Delta R.T.: 0.007 min
Response: 188329
Conc: 2.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

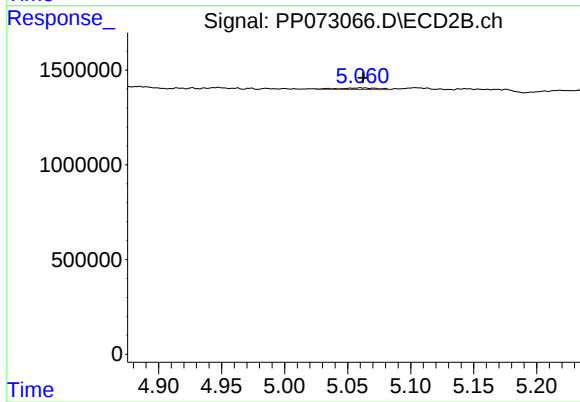


#5 AR-1016-3

R.T.: 5.061 min
Delta R.T.: -0.002 min
Response: 185449
Conc: 3.39 ng/ml

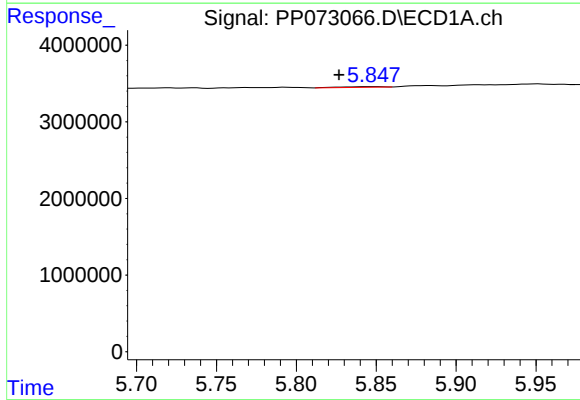


#6 AR-1016-4

R.T.: 5.848 min
Delta R.T.: 0.021 min
Response: 153518
Conc: 2.94 ng/ml

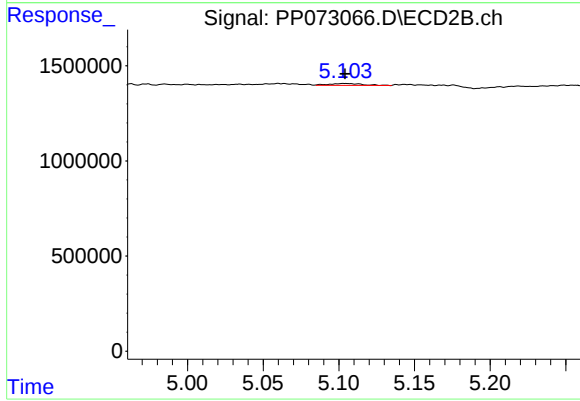

#6 AR-1016-4


R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 156293
Conc: 3.51 ng/ml

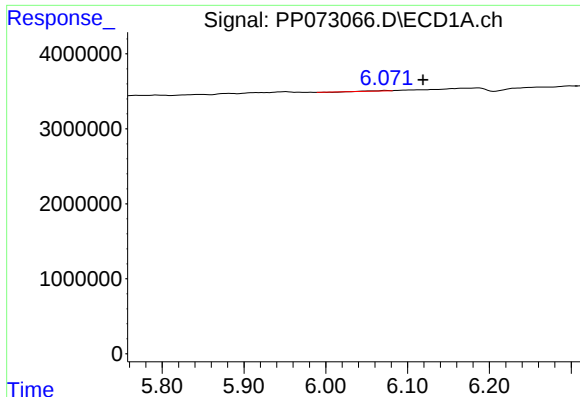

#7 AR-1016-5


R.T.: 6.074 min
Delta R.T.: -0.045 min
Response: 177629
Conc: 3.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

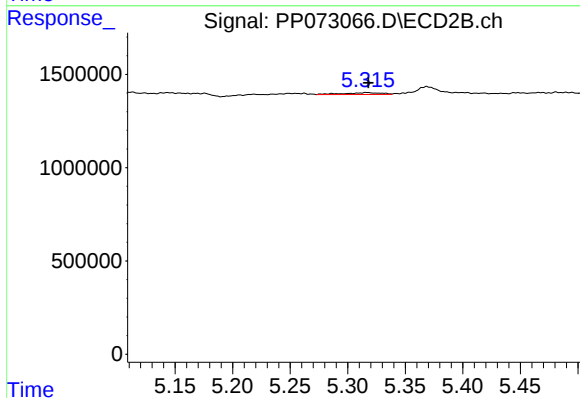


#7 AR-1016-5

R.T.: 5.317 min
Delta R.T.: -0.001 min
Response: 221886
Conc: 4.01 ng/ml

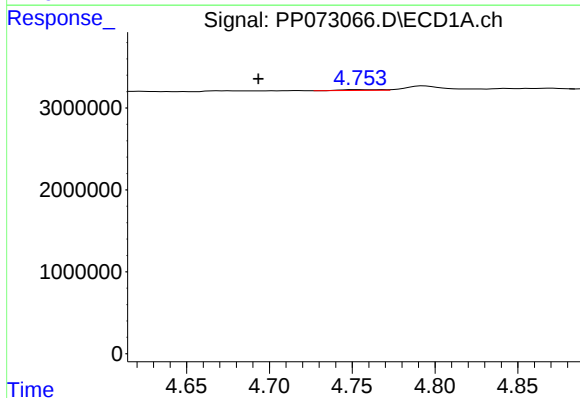


#8 AR-1221-1

R.T.: 4.753 min
Delta R.T.: 0.060 min
Response: 163156
Conc: 6.62 ng/ml

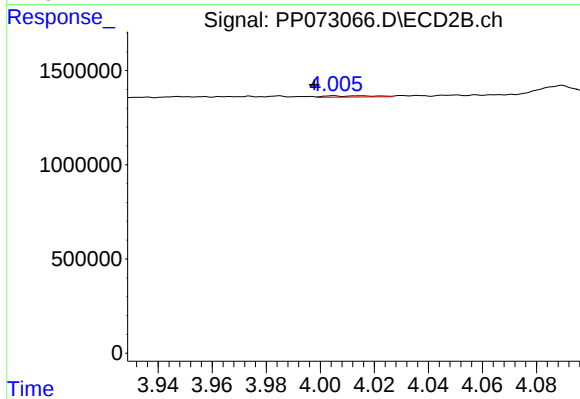

#8 AR-1221-1


R.T.: 4.005 min
Delta R.T.: 0.007 min
Response: 87285
Conc: 3.25 ng/ml

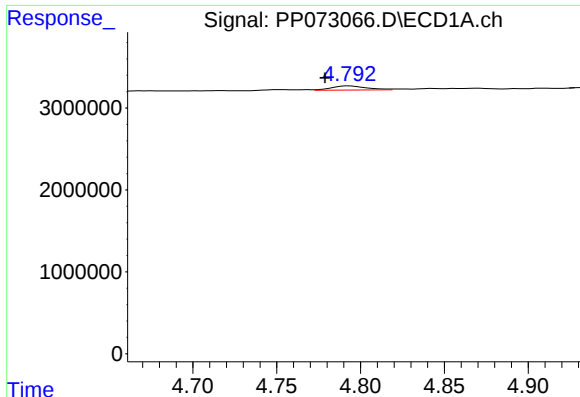

#9 AR-1221-2


R.T.: 4.793 min
Delta R.T.: 0.014 min
Response: 721697
Conc: 35.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

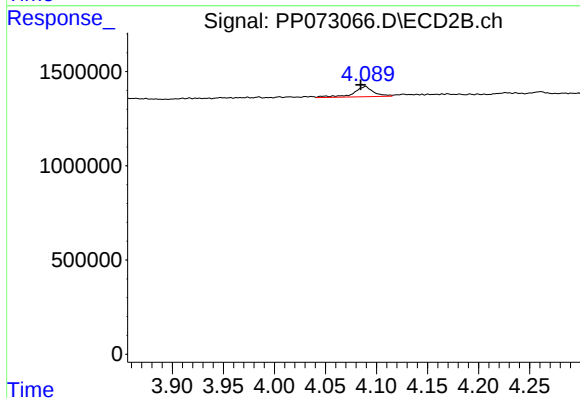


#9 AR-1221-2

R.T.: 4.089 min
Delta R.T.: 0.005 min
Response: 743409
Conc: 36.83 ng/ml

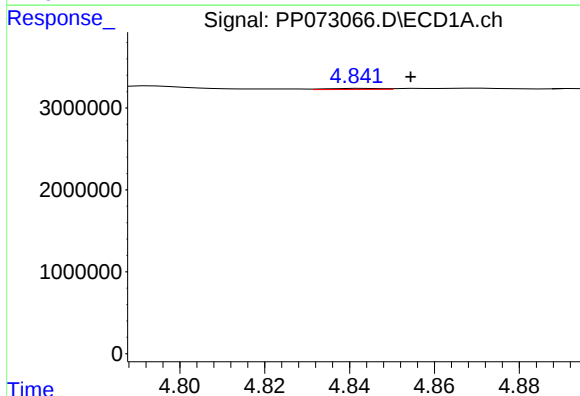


#10 AR-1221-3

R.T.: 4.843 min
Delta R.T.: -0.012 min
Response: 108497
Conc: 1.76 ng/ml

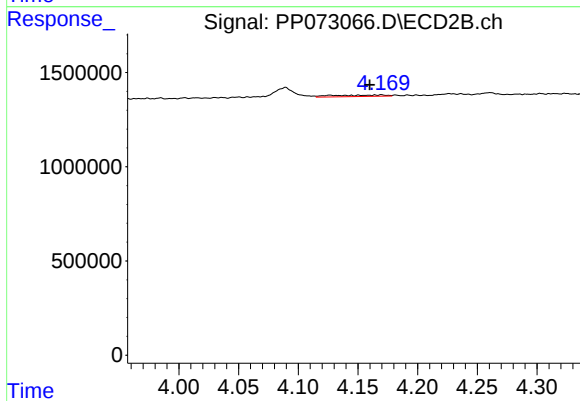

#10 AR-1221-3


R.T.: 4.170 min
Delta R.T.: 0.010 min
Response: 241618
Conc: 4.11 ng/ml

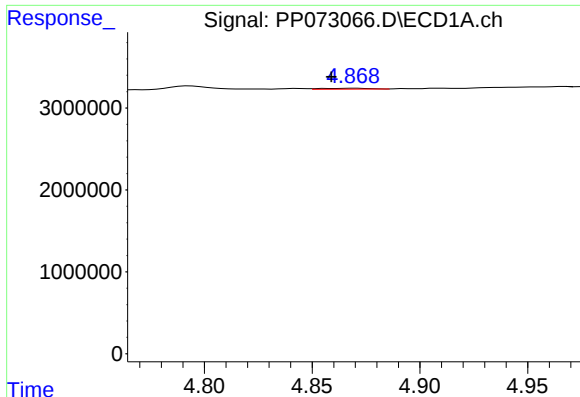

#11 AR-1232-1


R.T.: 4.870 min
Delta R.T.: 0.011 min
Response: 171758
Conc: 3.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

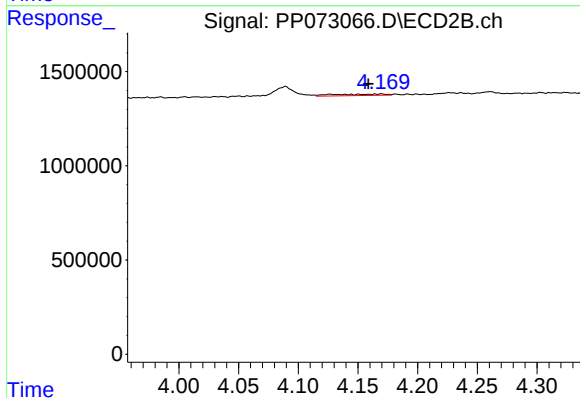


#11 AR-1232-1

R.T.: 4.170 min
Delta R.T.: 0.011 min
Response: 241618
Conc: 5.30 ng/ml

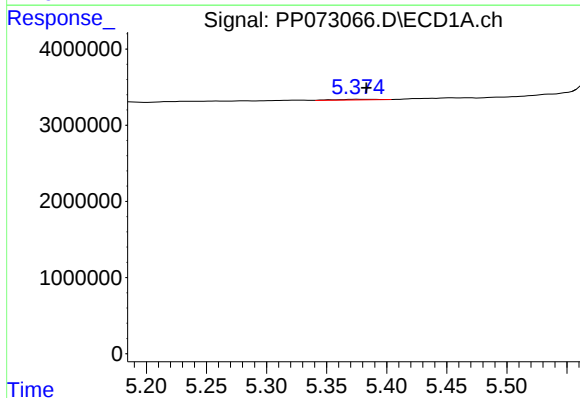


#12 AR-1232-2

R.T.: 5.375 min
Delta R.T.: -0.008 min
Response: 218143
Conc: 9.75 ng/ml

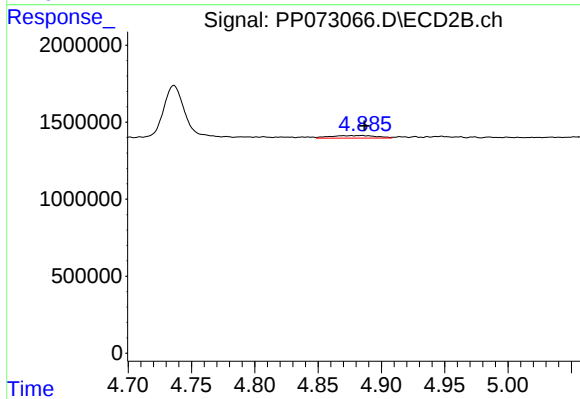

#12 AR-1232-2


R.T.: 4.885 min
Delta R.T.: -0.002 min
Response: 413762
Conc: 8.94 ng/ml

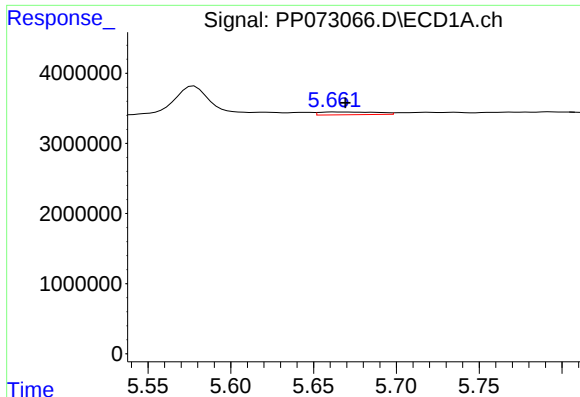

#13 AR-1232-3


R.T.: 5.663 min
Delta R.T.: -0.006 min
Response: 955814
Conc: 18.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

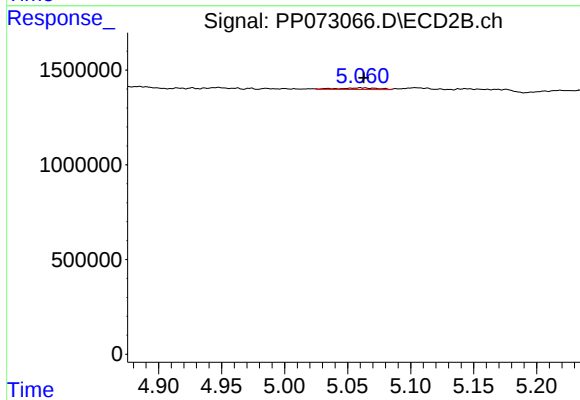


#13 AR-1232-3

R.T.: 5.061 min
Delta R.T.: -0.002 min
Response: 185449
Conc: 7.55 ng/ml

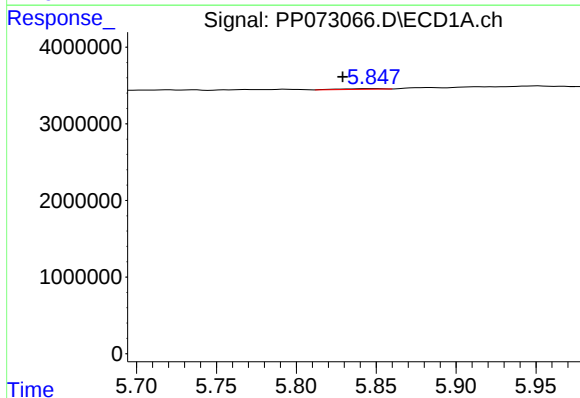


#14 AR-1232-4

R.T.: 5.848 min
Delta R.T.: 0.019 min
Response: 153518
Conc: 5.95 ng/ml

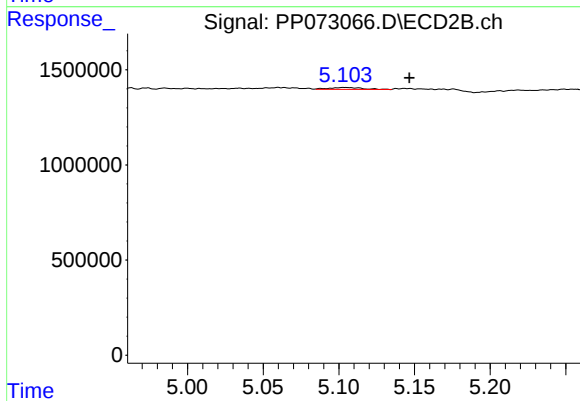

#14 AR-1232-4


R.T.: 5.104 min
Delta R.T.: -0.043 min
Response: 156293
Conc: 7.23 ng/ml

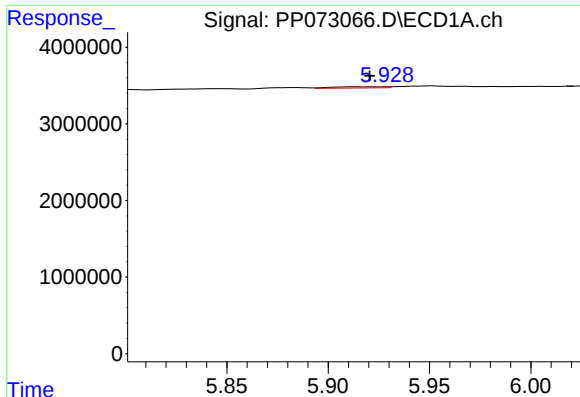

#15 AR-1232-5


R.T.: 5.914 min
Delta R.T.: -0.006 min
Response: 281308
Conc: 7.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

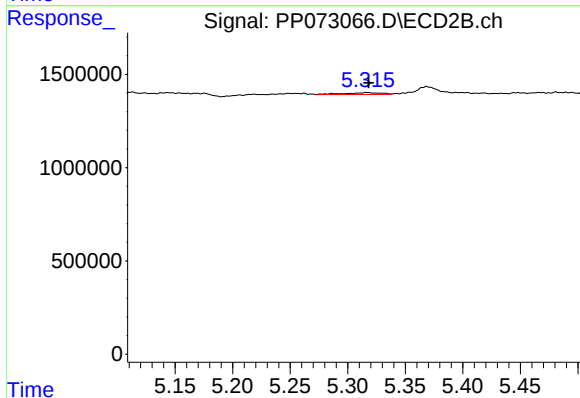


#15 AR-1232-5

R.T.: 5.317 min
Delta R.T.: -0.002 min
Response: 221886
Conc: 9.71 ng/ml

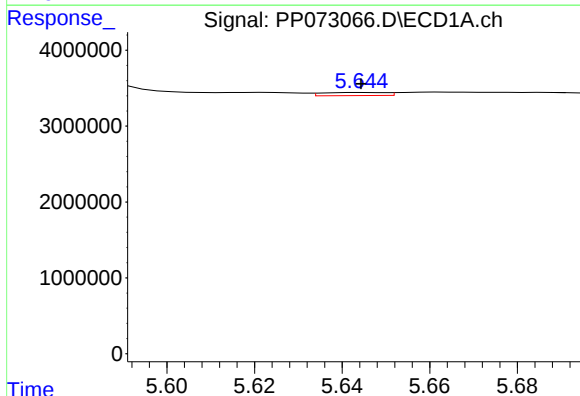


#16 AR-1242-1

R.T.: 5.645 min
Delta R.T.: 0.000 min
Response: 414001
Conc: 7.08 ng/ml

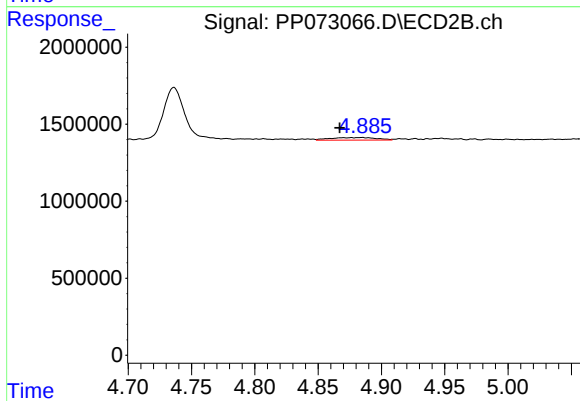

#16 AR-1242-1


R.T.: 4.885 min
Delta R.T.: 0.017 min
Response: 413762
Conc: 7.49 ng/ml

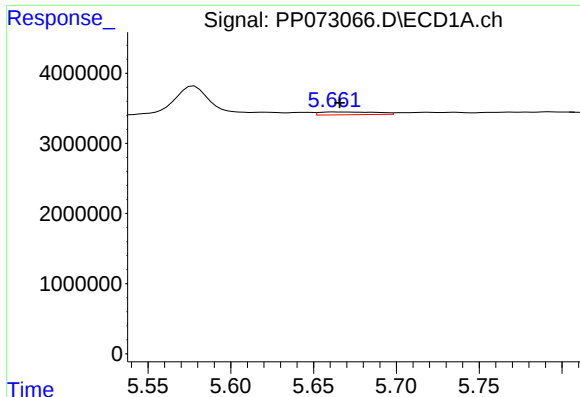

#17 AR-1242-2


R.T.: 5.663 min
Delta R.T.: -0.003 min
Response: 955814
Conc: 11.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

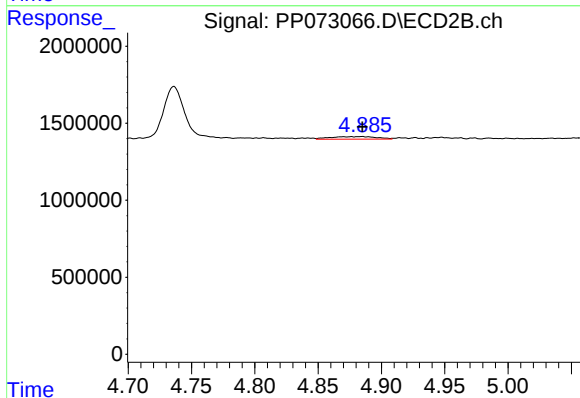


#17 AR-1242-2

R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 413762
Conc: 5.21 ng/ml

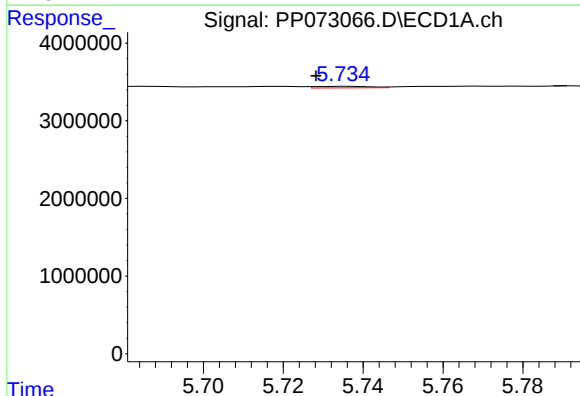


#18 AR-1242-3

R.T.: 5.736 min
Delta R.T.: 0.008 min
Response: 188329
Conc: 3.57 ng/ml

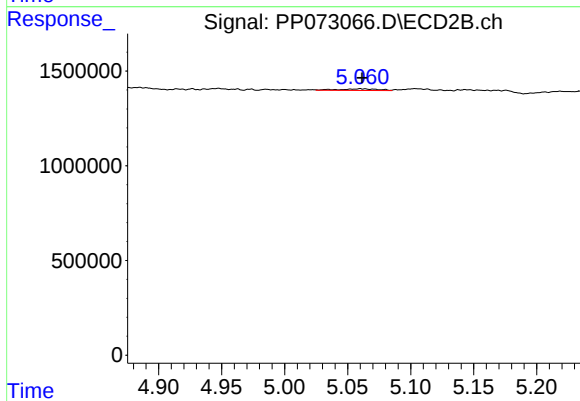

#18 AR-1242-3


R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 185449
Conc: 4.28 ng/ml

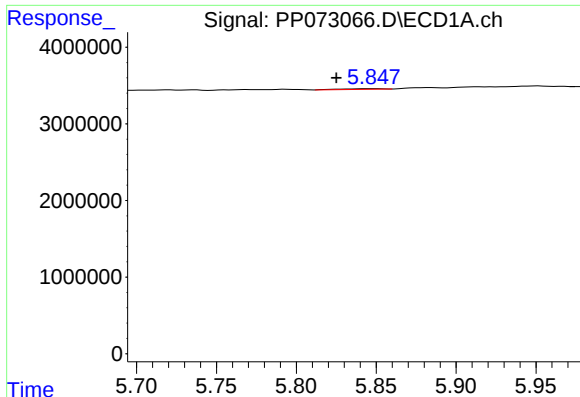

#19 AR-1242-4


R.T.: 5.848 min
Delta R.T.: 0.023 min
Response: 153518
Conc: 3.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

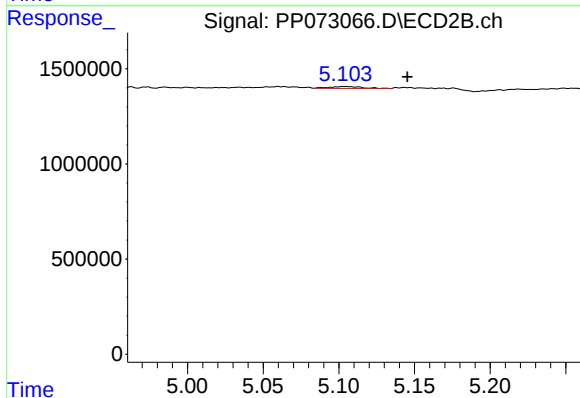


#19 AR-1242-4

R.T.: 5.104 min
Delta R.T.: -0.041 min
Response: 156293
Conc: 3.77 ng/ml

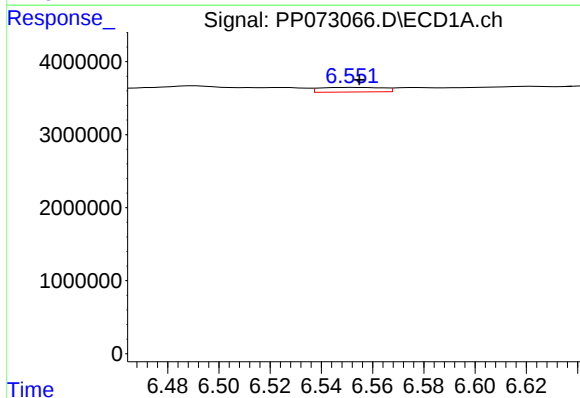


#20 AR-1242-5

R.T.: 6.552 min
Delta R.T.: -0.002 min
Response: 1086033
Conc: 21.91 ng/ml

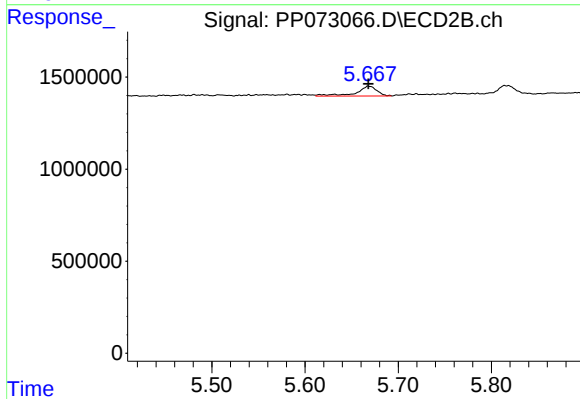

#20 AR-1242-5


R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 837375
Conc: 15.92 ng/ml

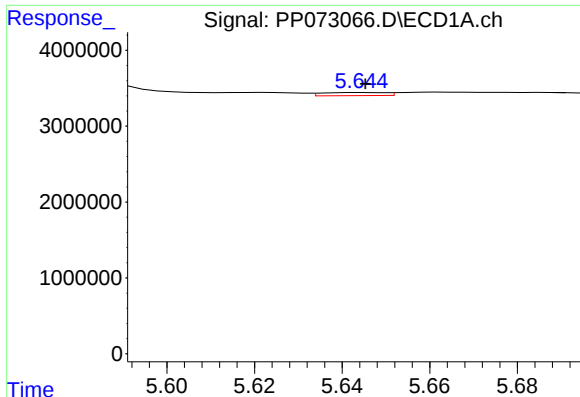

#21 AR-1248-1


R.T.: 5.645 min
Delta R.T.: 0.000 min
Response: 414001
Conc: 8.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

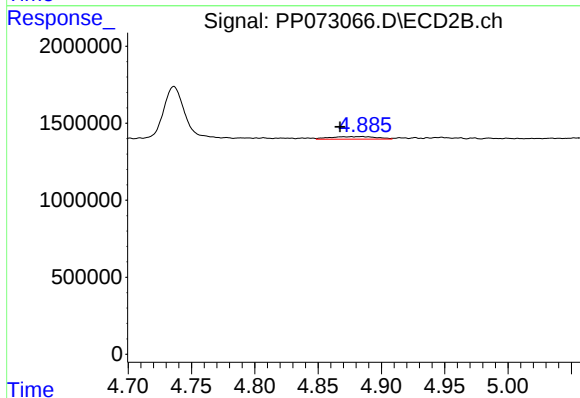


#21 AR-1248-1

R.T.: 4.885 min
Delta R.T.: 0.017 min
Response: 413762
Conc: 9.49 ng/ml

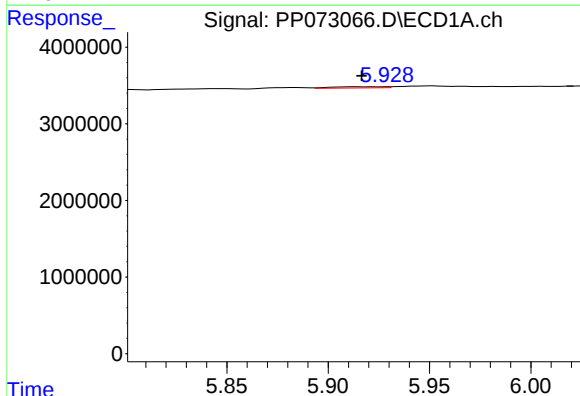


#22 AR-1248-2

R.T.: 5.914 min
Delta R.T.: -0.002 min
Response: 281308
Conc: 4.80 ng/ml

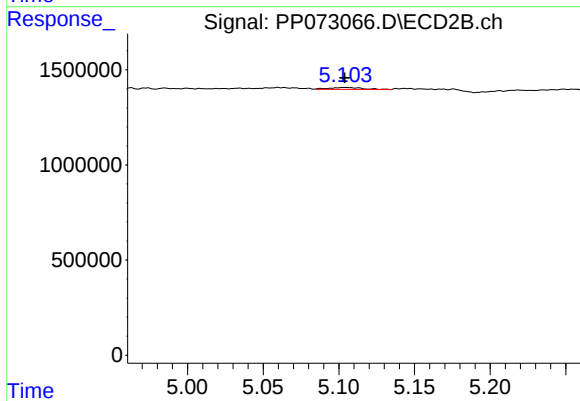

#22 AR-1248-2


R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 156293
Conc: 2.67 ng/ml

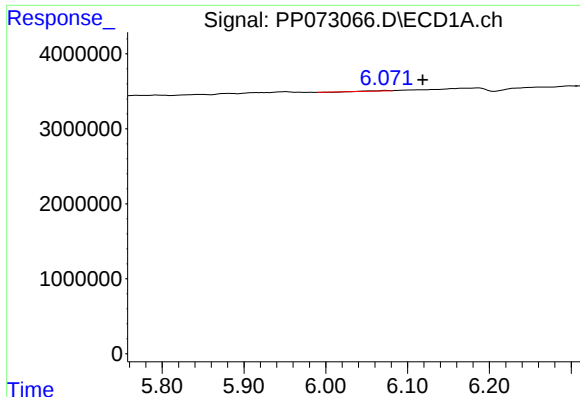

#23 AR-1248-3


R.T.: 6.074 min
Delta R.T.: -0.045 min
Response: 177629
Conc: 2.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

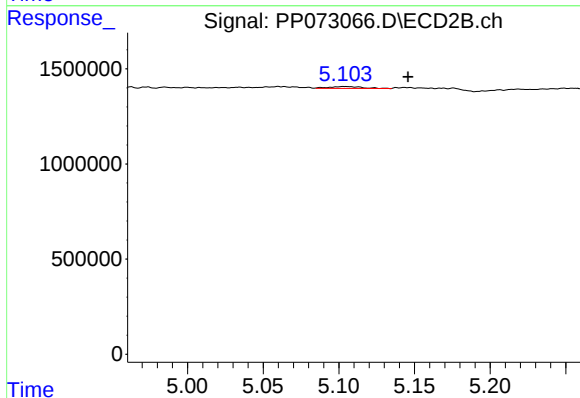


#23 AR-1248-3

R.T.: 5.104 min
Delta R.T.: -0.042 min
Response: 156293
Conc: 2.58 ng/ml

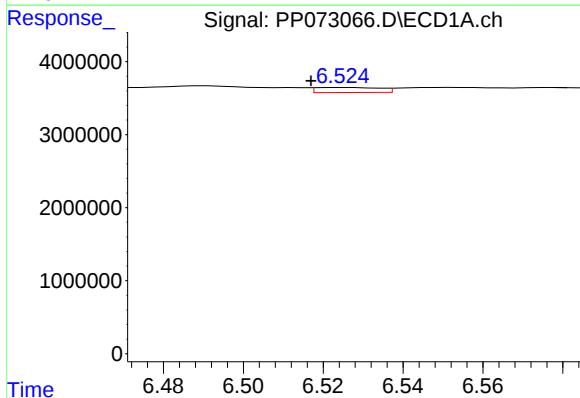


#24 AR-1248-4

R.T.: 6.526 min
Delta R.T.: 0.009 min
Response: 766589
Conc: 9.01 ng/ml

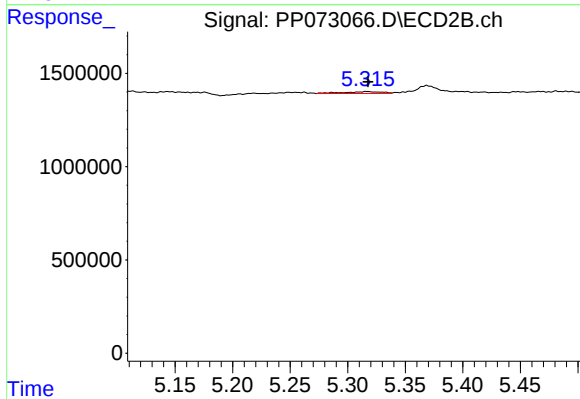

#24 AR-1248-4


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 221886
Conc: 3.17 ng/ml

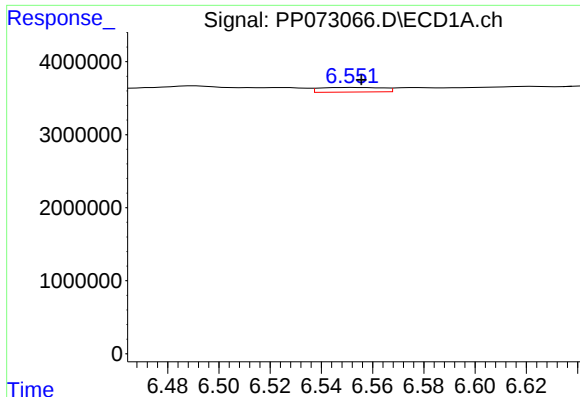

#25 AR-1248-5


R.T.: 6.552 min
Delta R.T.: -0.003 min
Response: 1086033
Conc: 12.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

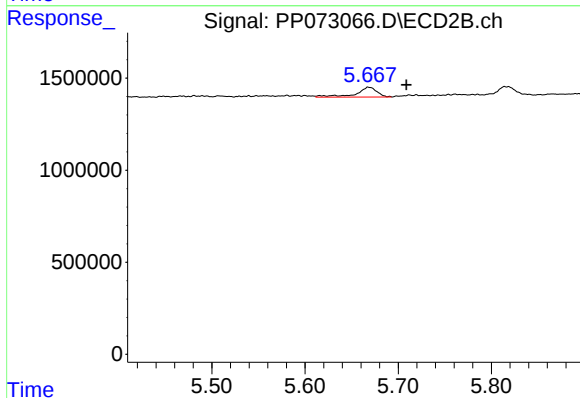


#25 AR-1248-5

R.T.: 5.669 min
Delta R.T.: -0.040 min
Response: 837375
Conc: 11.79 ng/ml

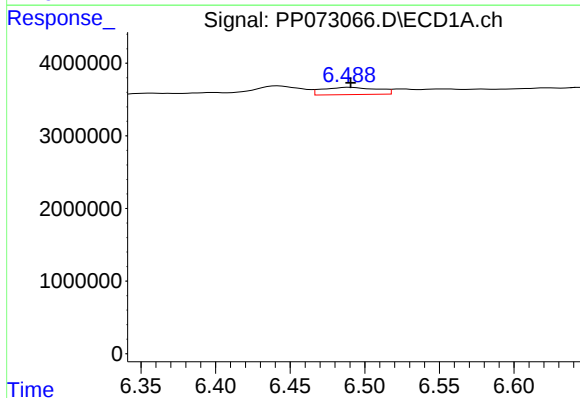


#26 AR-1254-1

R.T.: 6.490 min
Delta R.T.: 0.000 min
Response: 2551592
Conc: 30.31 ng/ml

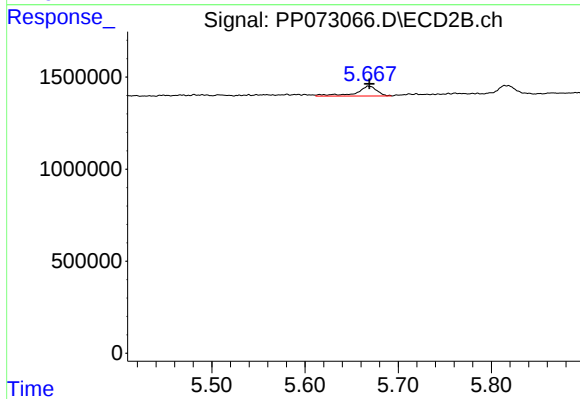

#26 AR-1254-1


R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 837375
Conc: 7.64 ng/ml

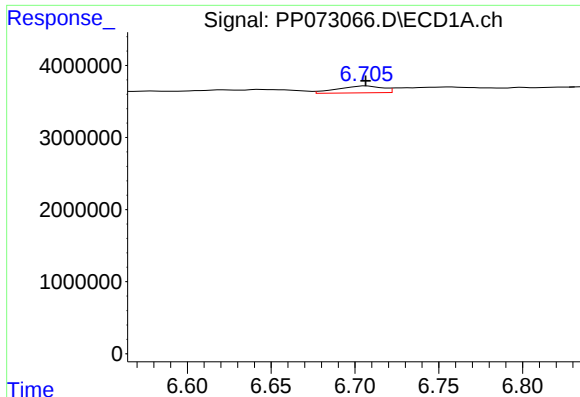

#27 AR-1254-2


R.T.: 6.707 min
Delta R.T.: 0.000 min
Response: 1773325
Conc: 14.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

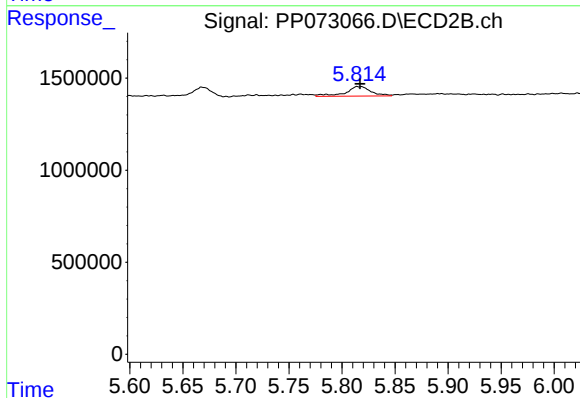


#27 AR-1254-2

R.T.: 5.816 min
Delta R.T.: 0.000 min
Response: 859719
Conc: 9.09 ng/ml

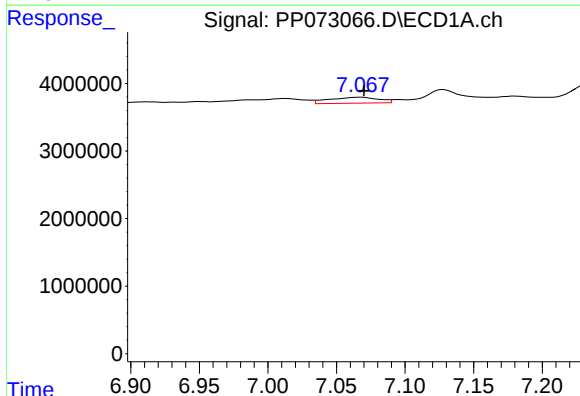


#28 AR-1254-3

R.T.: 7.069 min
Delta R.T.: -0.001 min
Response: 2209790
Conc: 16.84 ng/ml

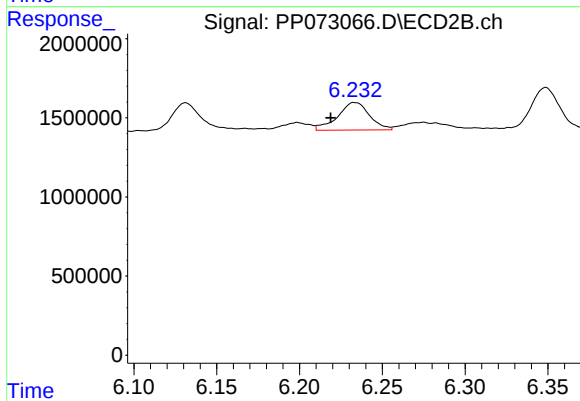

#28 AR-1254-3


R.T.: 6.234 min
Delta R.T.: 0.015 min
Response: 2328305
Conc: 15.78 ng/ml

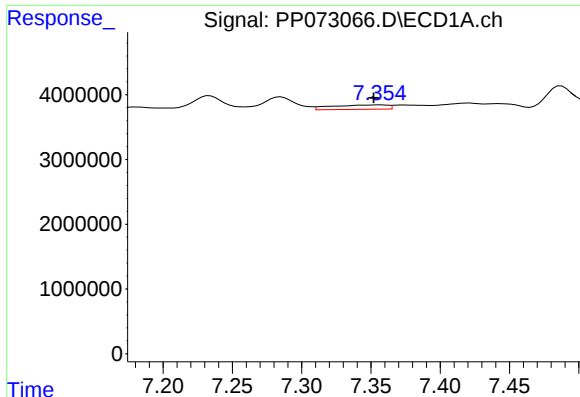

#29 AR-1254-4


R.T.: 7.356 min
Delta R.T.: 0.004 min
Response: 1898529
Conc: 15.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

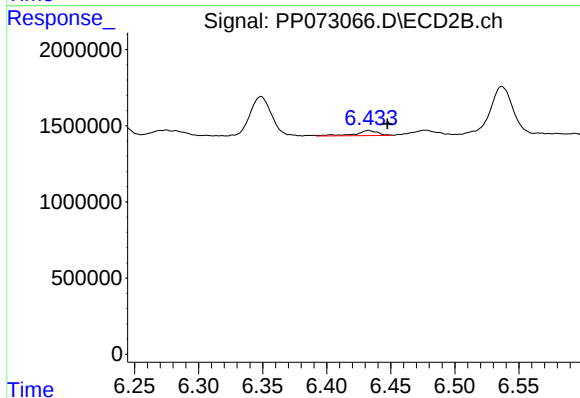


#29 AR-1254-4

R.T.: 6.433 min
Delta R.T.: -0.014 min
Response: 406826
Conc: 4.19 ng/ml

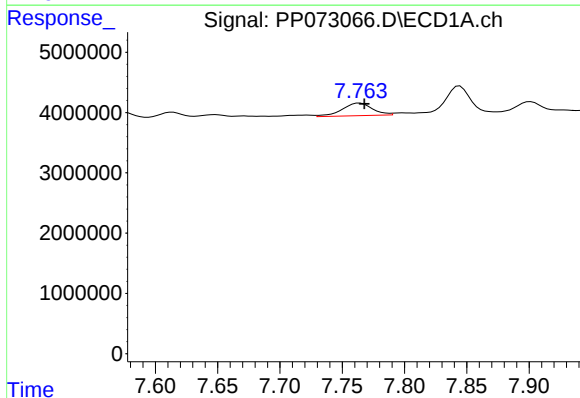


#30 AR-1254-5

R.T.: 7.764 min
Delta R.T.: -0.004 min
Response: 3509975
Conc: 30.72 ng/ml

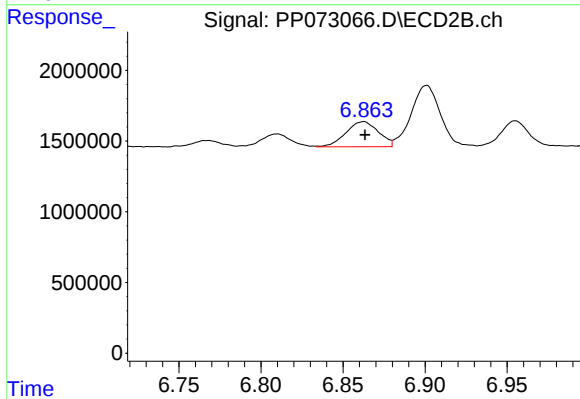

#30 AR-1254-5


R.T.: 6.862 min
Delta R.T.: -0.001 min
Response: 2455393
Conc: 18.89 ng/ml

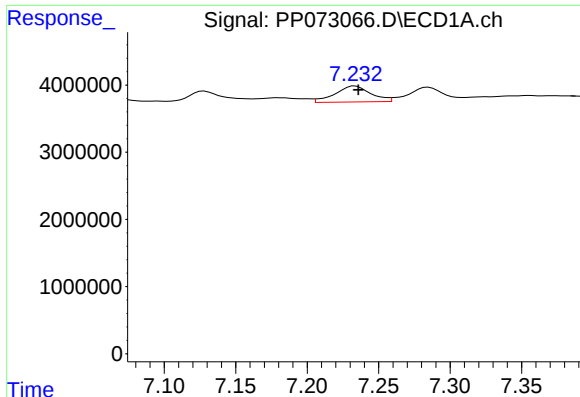

#31 AR-1260-1


R.T.: 7.234 min
Delta R.T.: -0.002 min
Response: 4124848
Conc: 46.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

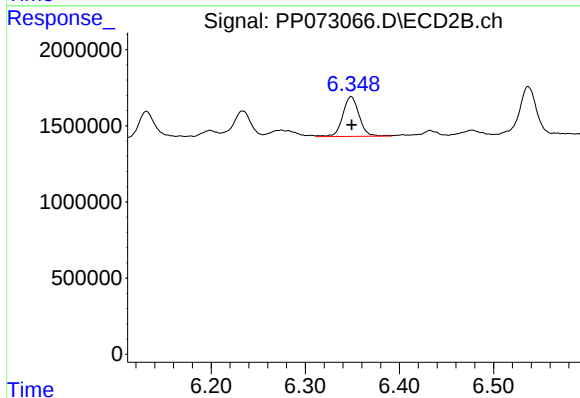


#31 AR-1260-1

R.T.: 6.349 min
Delta R.T.: 0.000 min
Response: 3162784
Conc: 33.39 ng/ml

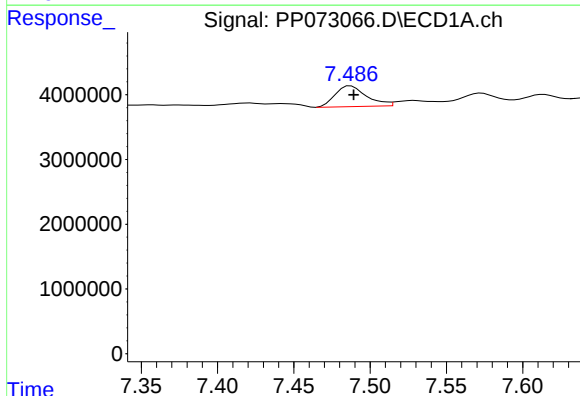


#32 AR-1260-2

R.T.: 7.487 min
Delta R.T.: -0.002 min
Response: 4601046
Conc: 33.86 ng/ml

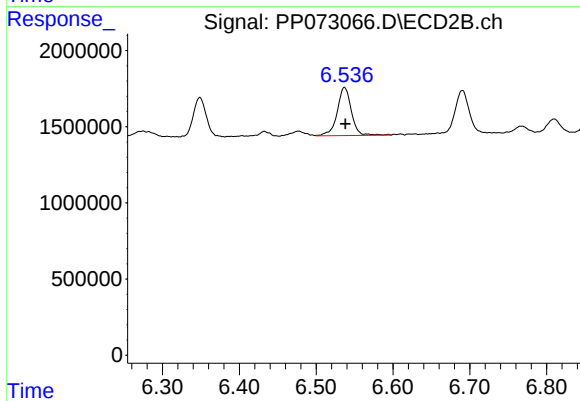

#32 AR-1260-2


R.T.: 6.537 min
Delta R.T.: -0.001 min
Response: 4020010
Conc: 34.53 ng/ml

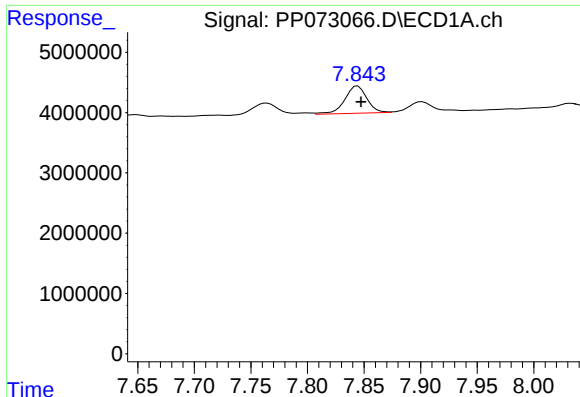

#33 AR-1260-3


R.T.: 7.845 min
Delta R.T.: -0.003 min
Response: 6166747
Conc: 54.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

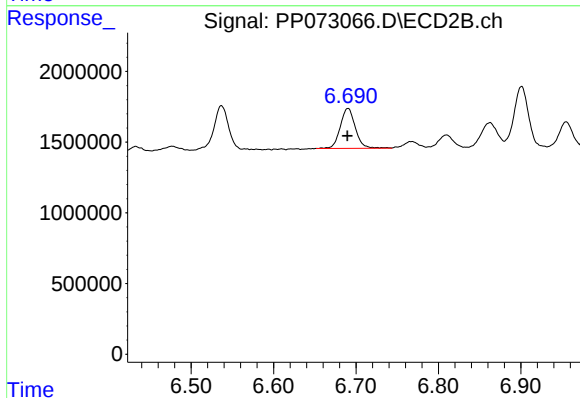


#33 AR-1260-3

R.T.: 6.690 min
Delta R.T.: 0.000 min
Response: 3579921
Conc: 34.37 ng/ml

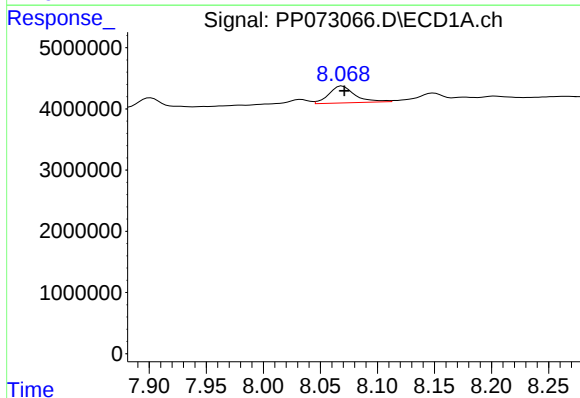


#34 AR-1260-4

R.T.: 8.069 min
Delta R.T.: -0.002 min
Response: 4359650
Conc: 42.31 ng/ml

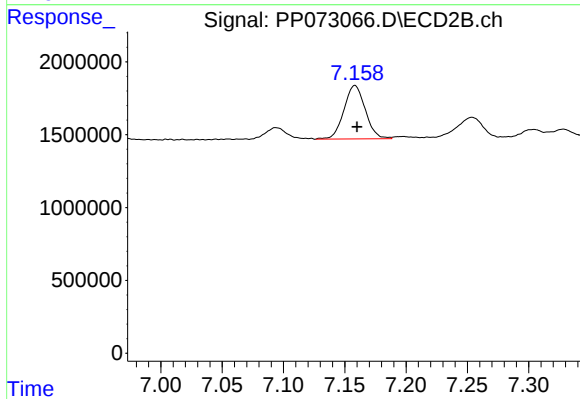

#34 AR-1260-4


R.T.: 7.158 min
Delta R.T.: -0.002 min
Response: 4442642
Conc: 50.64 ng/ml

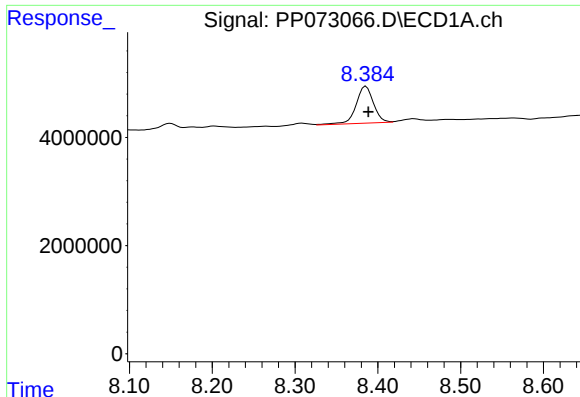

#35 AR-1260-5


R.T.: 8.386 min
Delta R.T.: -0.003 min
Response: 9955308
Conc: 41.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

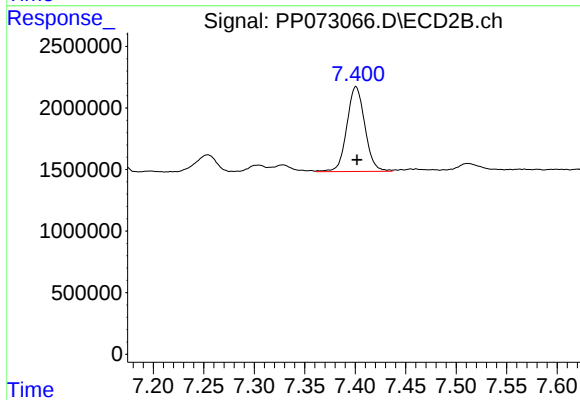


#35 AR-1260-5

R.T.: 7.401 min
Delta R.T.: -0.001 min
Response: 8529122
Conc: 39.97 ng/ml

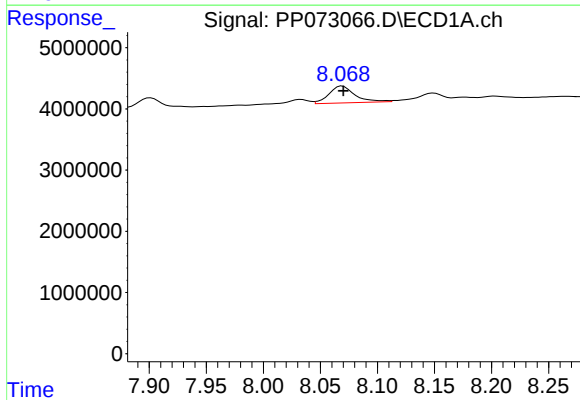


#36 AR-1262-1

R.T.: 8.069 min
Delta R.T.: 0.000 min
Response: 4359650
Conc: 29.45 ng/ml

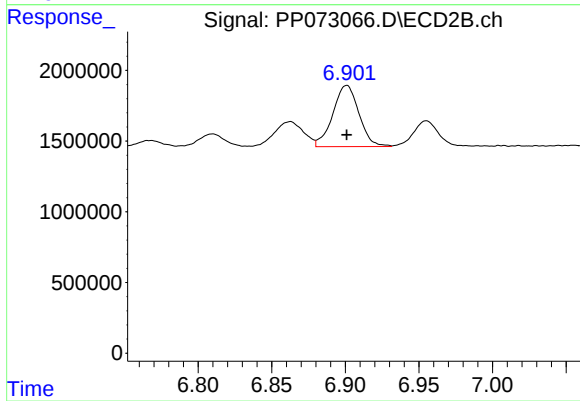

#36 AR-1262-1


R.T.: 6.901 min
Delta R.T.: 0.000 min
Response: 5334759
Conc: 36.93 ng/ml

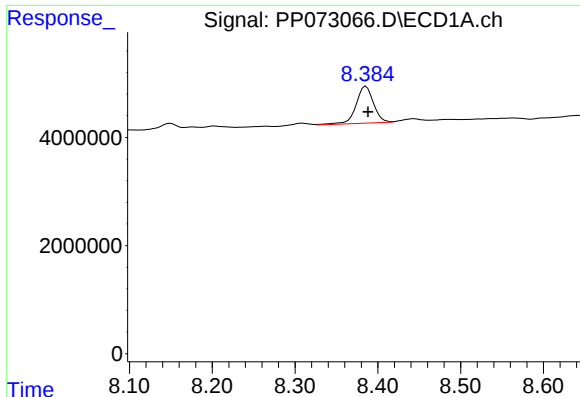

#37 AR-1262-2


R.T.: 8.386 min
Delta R.T.: -0.003 min
Response: 9955308
Conc: 31.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

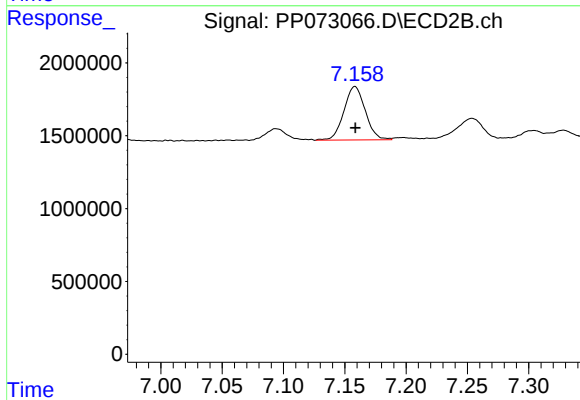


#37 AR-1262-2

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 4442642
Conc: 36.35 ng/ml

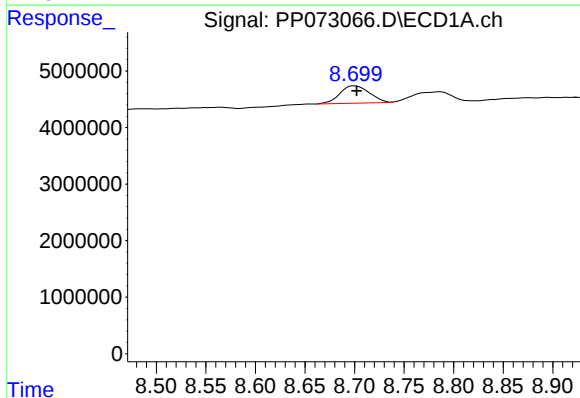


#38 AR-1262-3

R.T.: 8.700 min
Delta R.T.: -0.002 min
Response: 6387649
Conc: 29.85 ng/ml

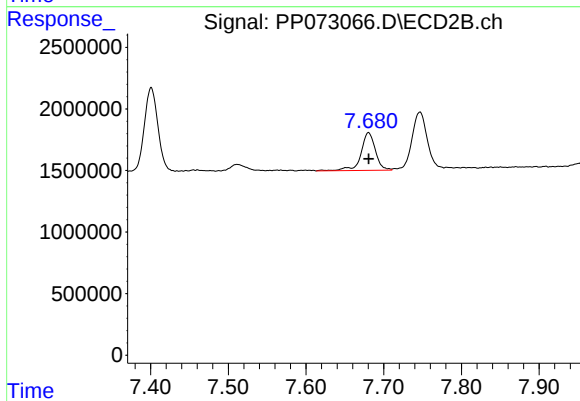

#38 AR-1262-3


R.T.: 7.681 min
Delta R.T.: 0.000 min
Response: 3950152
Conc: 35.05 ng/ml

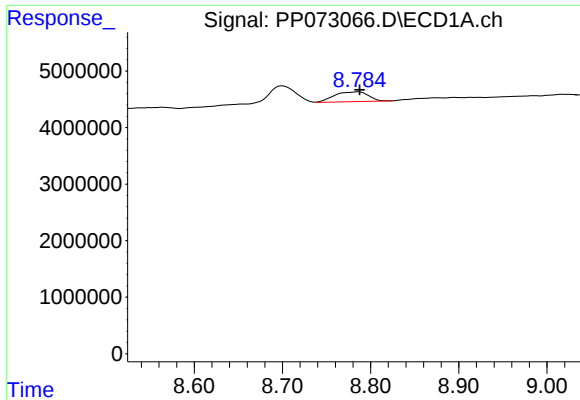

#39 AR-1262-4


R.T.: 8.786 min
Delta R.T.: -0.001 min
Response: 4678216
Conc: 29.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

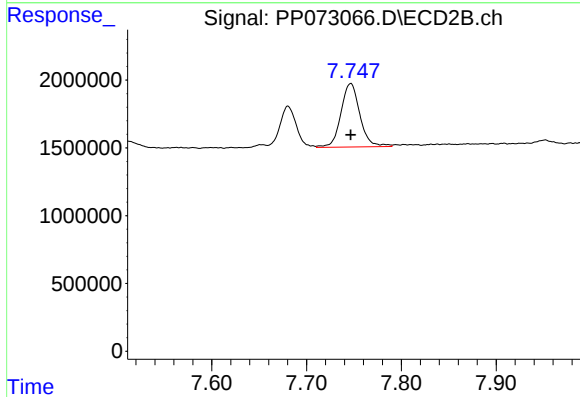


#39 AR-1262-4

R.T.: 7.746 min
Delta R.T.: 0.000 min
Response: 6516355
Conc: 35.54 ng/ml

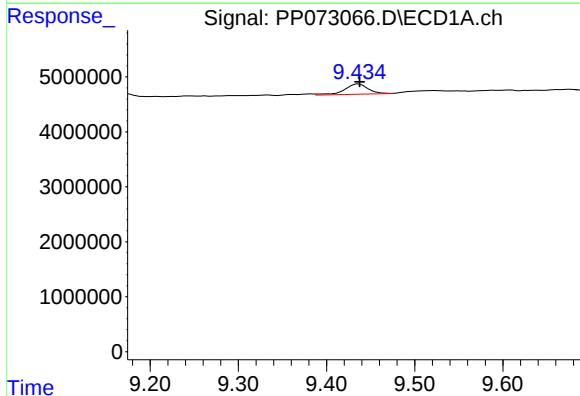


#40 AR-1262-5

R.T.: 9.436 min
Delta R.T.: -0.002 min
Response: 3458274
Conc: 30.92 ng/ml

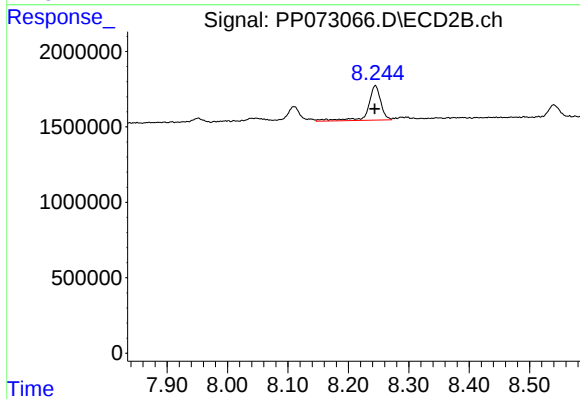

#40 AR-1262-5


R.T.: 8.245 min
Delta R.T.: 0.000 min
Response: 3341879
Conc: 38.60 ng/ml

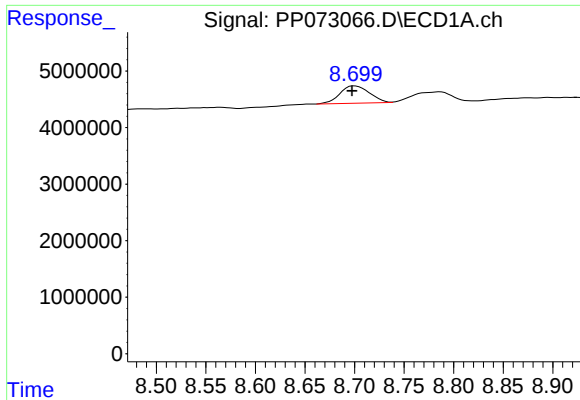

#41 AR-1268-1


R.T.: 8.700 min
Delta R.T.: 0.002 min
Response: 6387649
Conc: 17.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

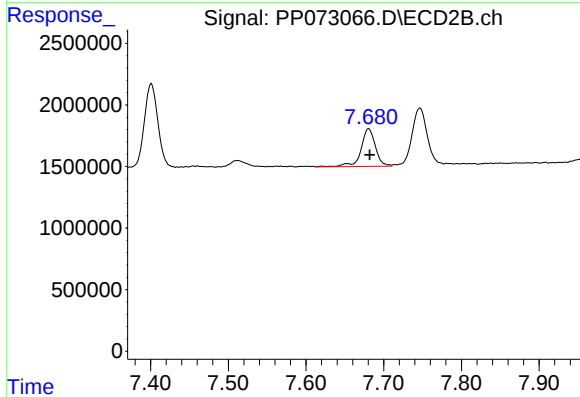


#41 AR-1268-1

R.T.: 7.681 min
Delta R.T.: -0.002 min
Response: 3950152
Conc: 13.75 ng/ml

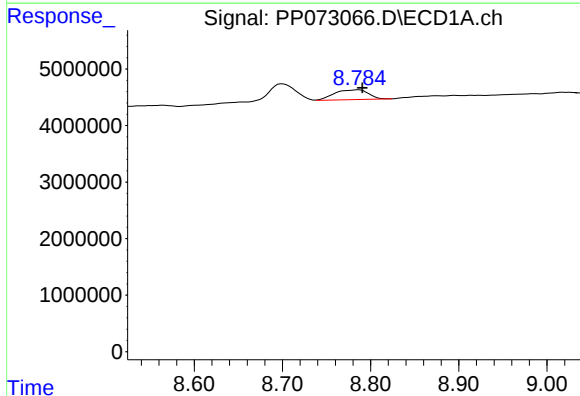


#42 AR-1268-2

R.T.: 8.786 min
Delta R.T.: -0.005 min
Response: 4678216
Conc: 15.34 ng/ml

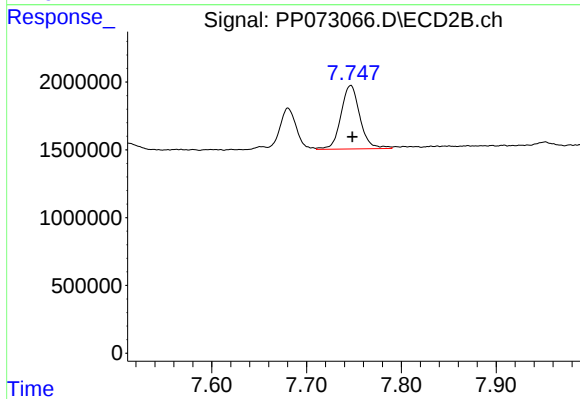

#42 AR-1268-2


R.T.: 7.746 min
Delta R.T.: -0.002 min
Response: 6516355
Conc: 25.34 ng/ml

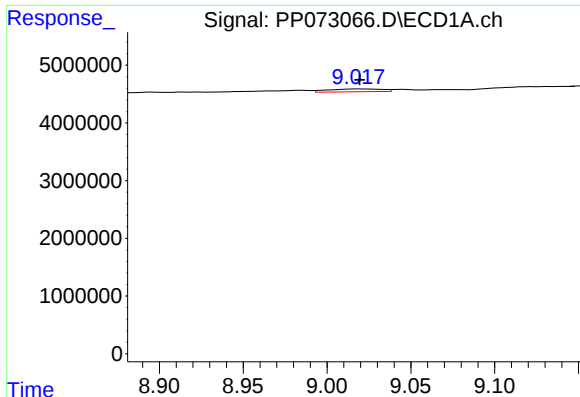

#43 AR-1268-3


R.T.: 9.018 min
Delta R.T.: -0.001 min
Response: 1089963
Conc: 4.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

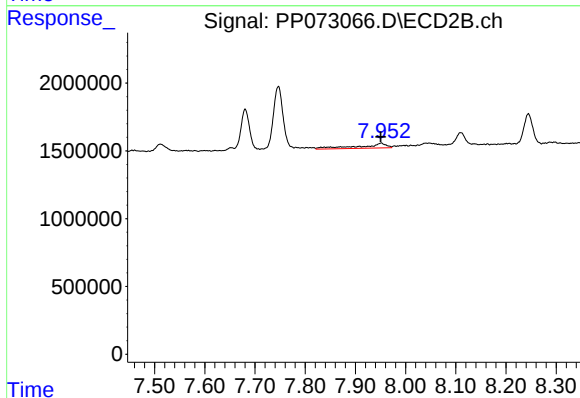


#43 AR-1268-3

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 1316757
Conc: 6.10 ng/ml

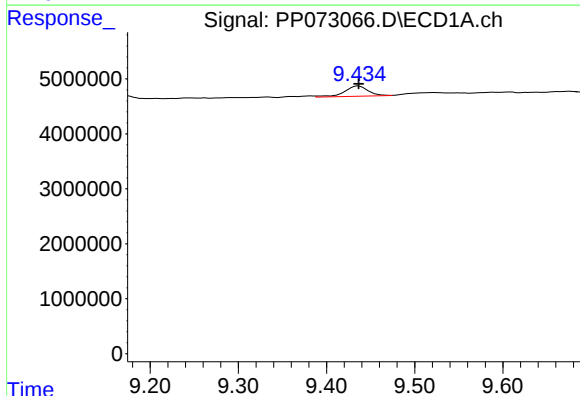


#44 AR-1268-4

R.T.: 9.436 min
Delta R.T.: 0.000 min
Response: 3458274
Conc: 29.55 ng/ml

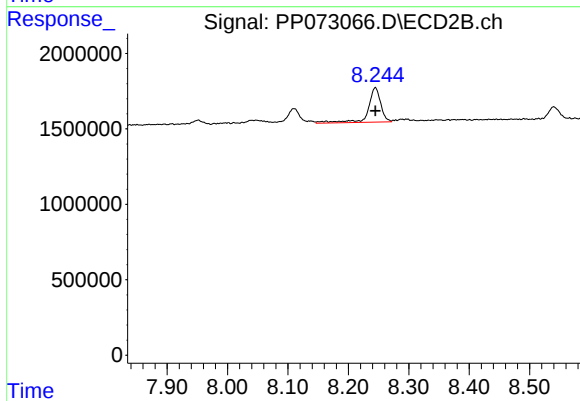

#44 AR-1268-4


R.T.: 8.245 min
Delta R.T.: 0.000 min
Response: 3341879
Conc: 35.48 ng/ml

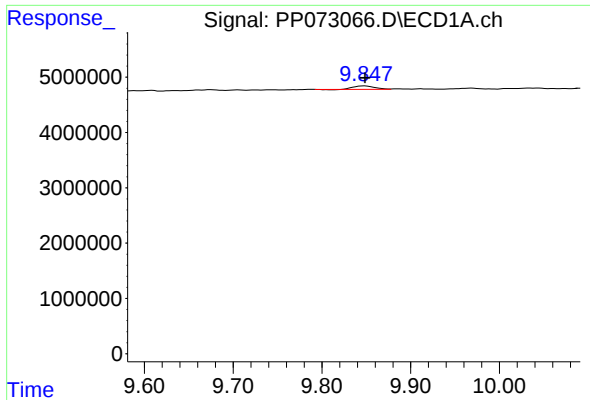

#45 AR-1268-5

R.T.: 9.848 min
Delta R.T.: 0.000 min
Response: 1021346
Conc: 1.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

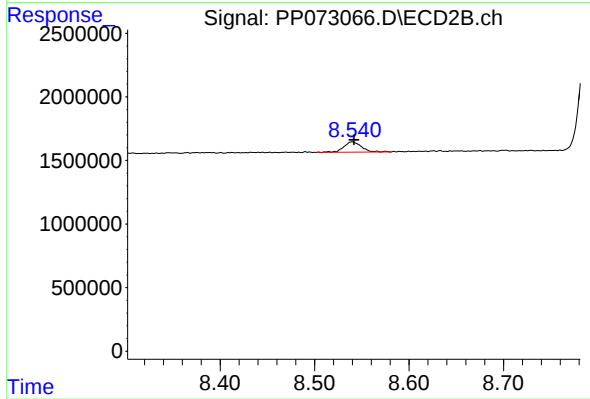

#45 AR-1268-5

R.T.: 8.540 min
Delta R.T.: -0.002 min
Response: 1061976
Conc: 1.83 ng/ml