

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061924\
Data File : PP065807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 11:08
Operator : YP\AJ
Sample : P2938-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
403

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 13:17:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.827	4.069	15530575	21402048	8.187m	7.665
2) SA Decachlor...	10.833	9.245	14006682	9610349	7.121	6.523m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061924\
Data File : PP065807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 11:08
Operator : YP\AJ
Sample : P2938-06
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
403


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 13:17:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

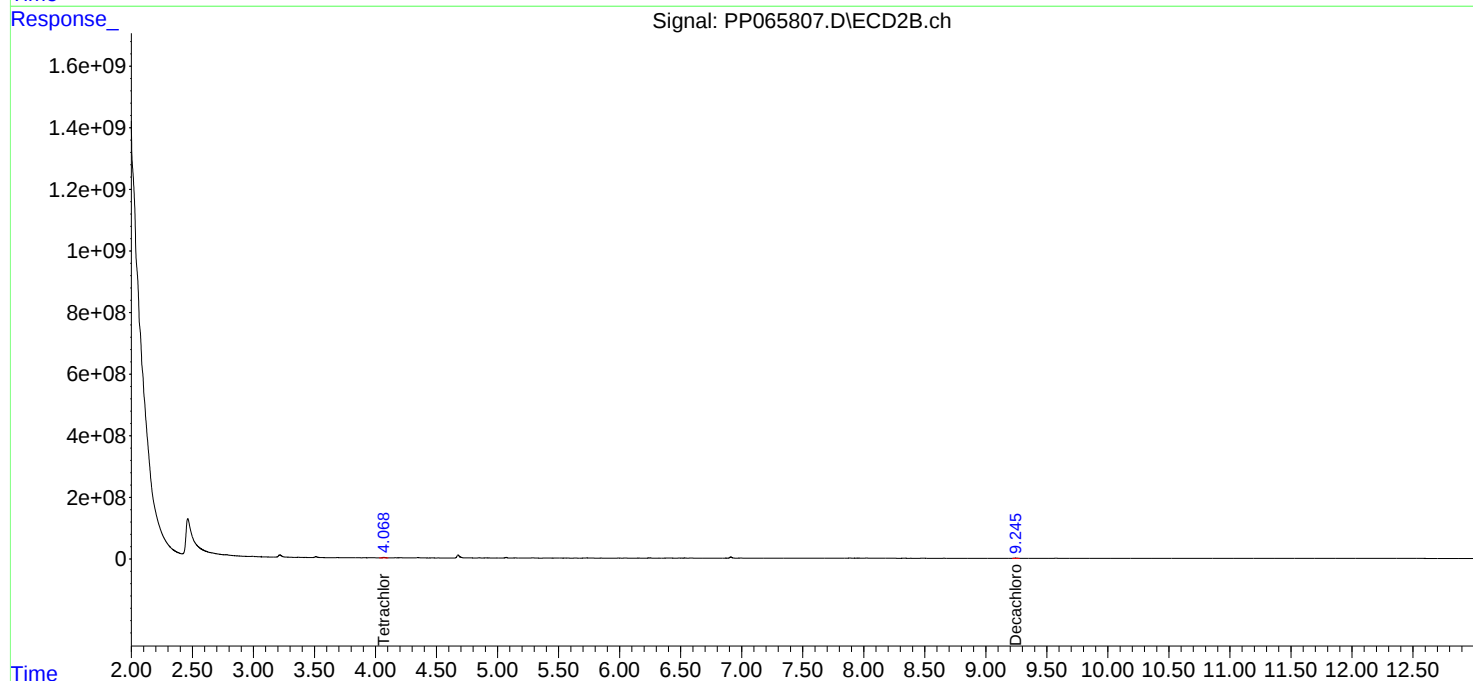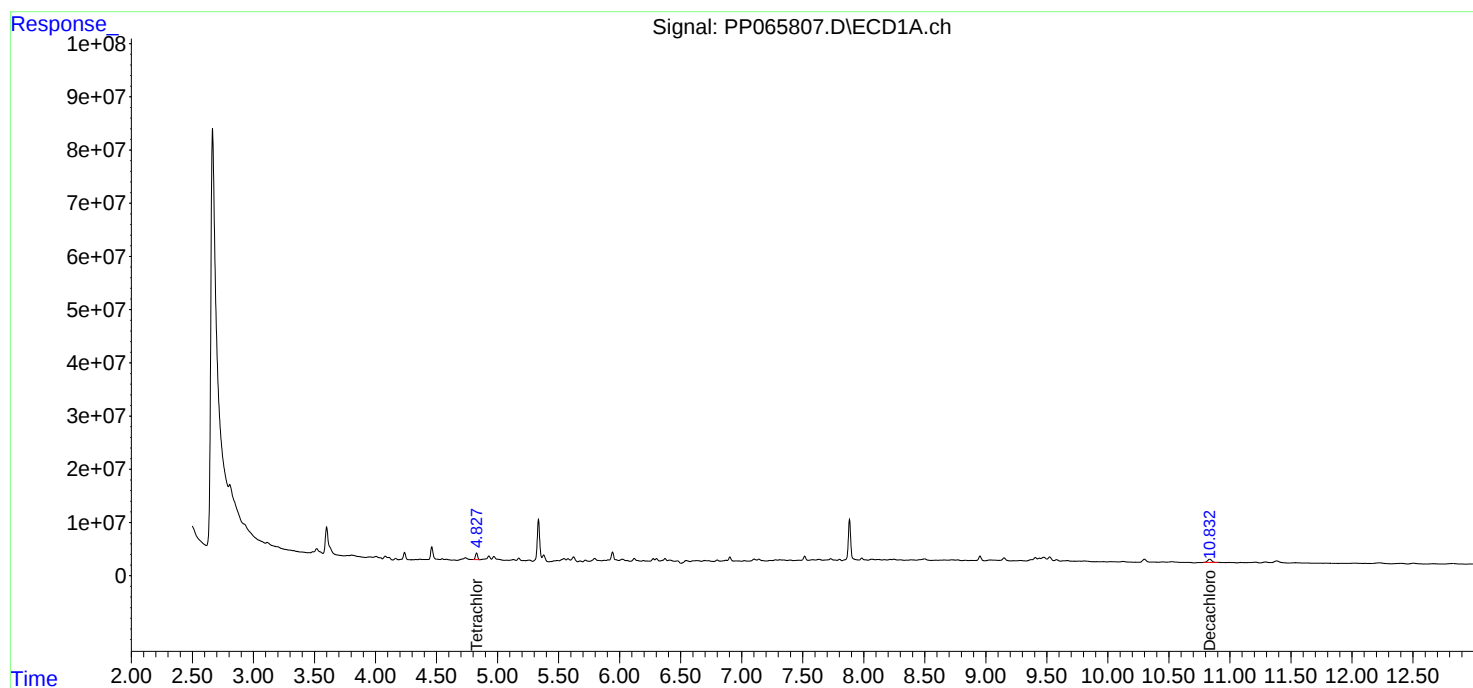

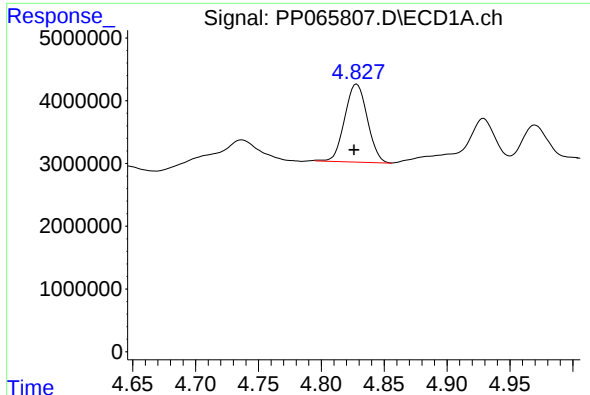


#1 Tetrachloro-m-xylene

R.T.: 4.827 min
Delta R.T.: 0.001 min
Response: 15530575
Conc: 8.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
403


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

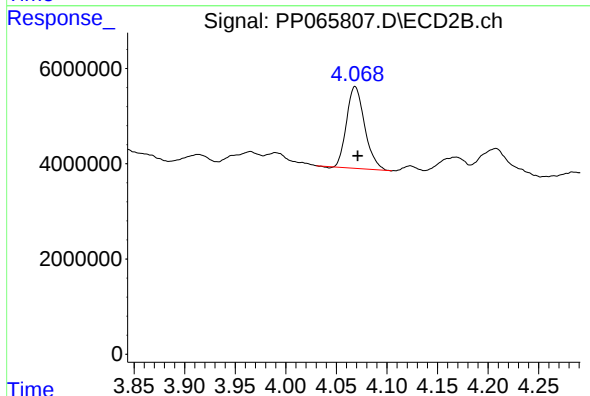


#1 Tetrachloro-m-xylene

R.T.: 4.069 min
Delta R.T.: -0.003 min
Response: 21402048
Conc: 7.66 ng/ml

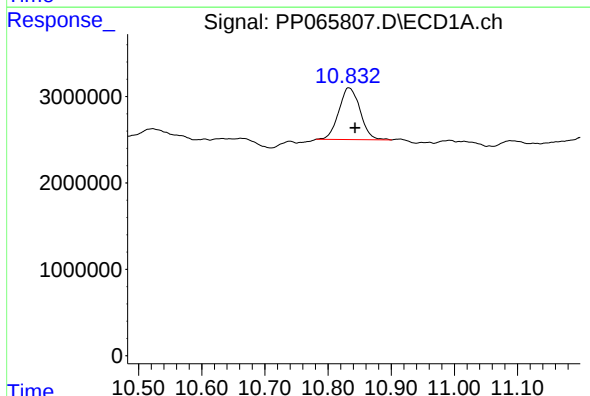

#2 Decachlorobiphenyl

R.T.: 10.833 min
Delta R.T.: -0.009 min
Response: 14006682
Conc: 7.12 ng/ml

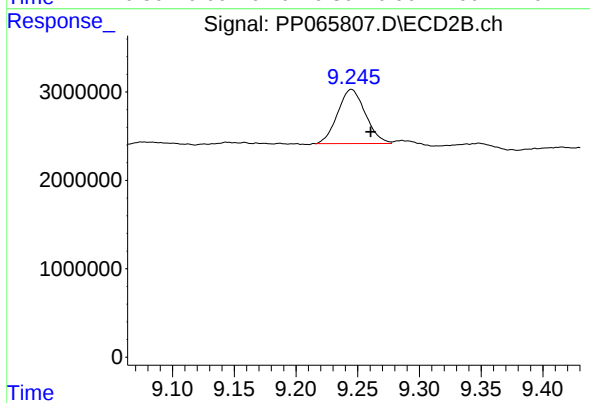

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.016 min
Response: 9610349
Conc: 6.52 ng/ml m