

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061924\
 Data File : PP065811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2024 12:13
 Operator : YP\AJ
 Sample : P2937-20 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC270896-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/20/2024
 Supervised By :Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 13:20:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 06 05:25:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.826	4.065	2698146	4020374	1.422	1.440
2) SA Decachlor...	10.839	9.249	3326845	2076856	1.691	1.410m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061924\
Data File : PP065811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 12:13
Operator : YP\AJ
Sample : P2937-20 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC270896-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 13:20:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP060524.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 06 05:25:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

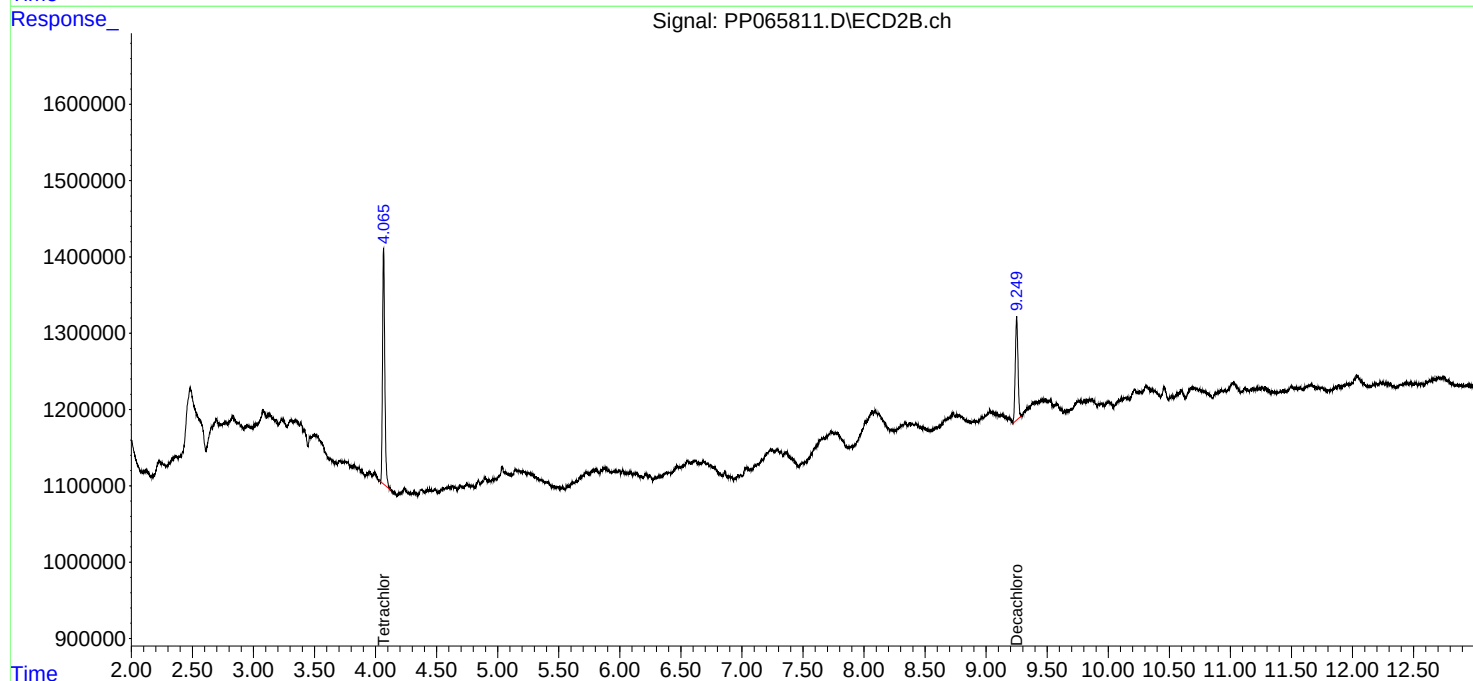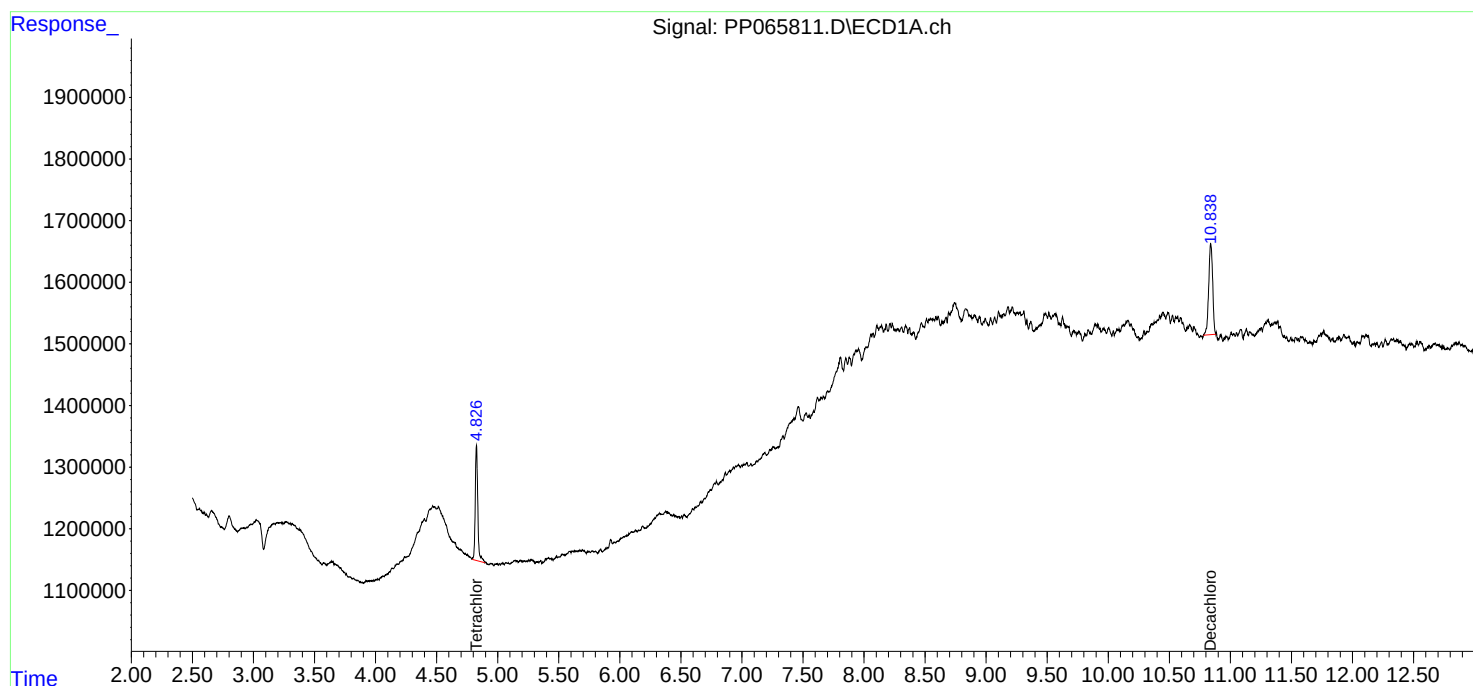

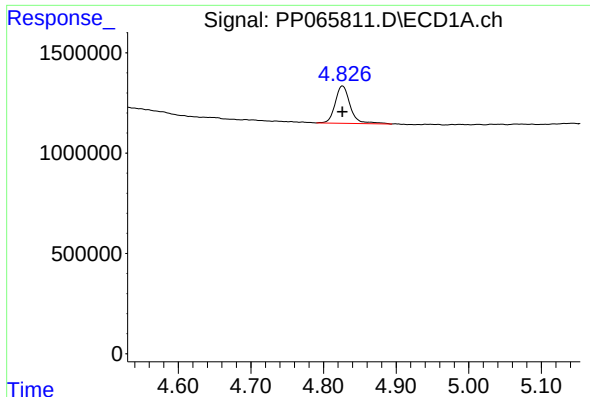


#1 Tetrachloro-m-xylene

R.T.: 4.826 min
Delta R.T.: 0.000 min
Response: 2698146
Conc: 1.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC270896-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

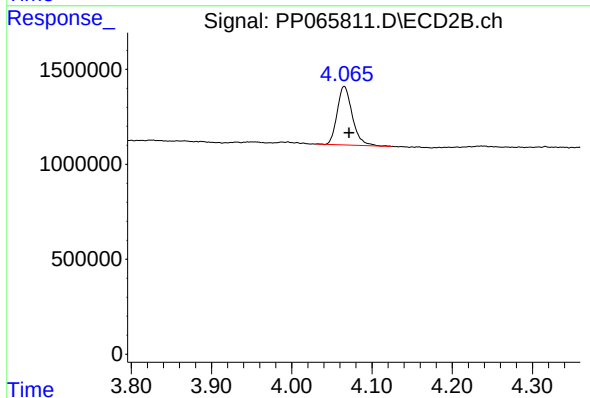


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: -0.006 min
Response: 4020374
Conc: 1.44 ng/ml

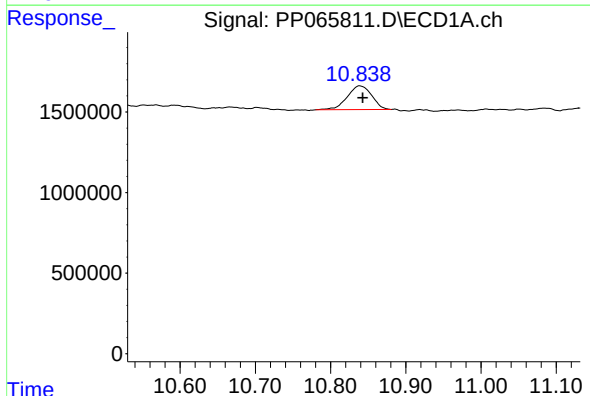

#2 Decachlorobiphenyl

R.T.: 10.839 min
Delta R.T.: -0.004 min
Response: 3326845
Conc: 1.69 ng/ml

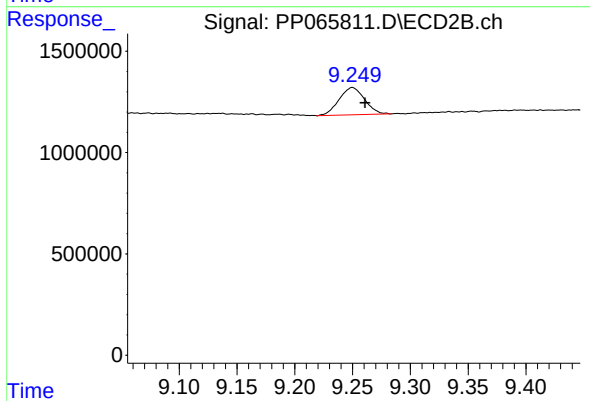

#2 Decachlorobiphenyl

R.T.: 9.249 min
Delta R.T.: -0.011 min
Response: 2076856
Conc: 1.41 ng/ml m