

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 17:05
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:27:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.495	3.789	43074357	37597423	20.407	20.867
2) SA Decachlor...	10.191	8.800	40859217	29524003	23.910	22.120
Target Compounds						
3) L1 AR-1016-1	5.647	4.871	627635	249499	8.637	3.631 #
4) L1 AR-1016-2	5.675	4.889	741424	278463	7.128	2.767 #
5) L1 AR-1016-3	5.734	5.063	128521	179214	1.967	3.275 #
6) L1 AR-1016-4	5.846	5.104	426050	105997	8.149	2.379 #
7) L1 AR-1016-5	6.116	5.323	77294	198743	1.546	3.595 #
8) L2 AR-1221-1	4.698	4.001	558426	801112	22.646	29.812 #
9) L2 AR-1221-2	4.794	4.088	1325906	1216059	65.707	60.244
10) L2 AR-1221-3	4.859	4.161	1526600	1635649	24.802	27.849
11) L3 AR-1232-1	4.859	4.161	1526600	1635649	32.511	35.897
12) L3 AR-1232-2	5.368	4.889	246080	278463	11.001	6.020 #
13) L3 AR-1232-3	5.675	5.063	741424	179214	14.369	7.298 #
14) L3 AR-1232-4	5.846	5.104f	426050	105997	16.507	4.902 #
15) L3 AR-1232-5	5.933	5.323	247987	198743	6.952	8.694 #
16) L4 AR-1242-1	5.647	4.871	627635	249499	10.740	4.518 #
17) L4 AR-1242-2	5.675	4.889	741424	278463	8.566	3.503 #
18) L4 AR-1242-3	5.734	5.063	128521	179214	2.438	4.138 #
19) L4 AR-1242-4	5.846	5.104f	426050	105997	9.692	2.554 #
20) L4 AR-1242-5	6.559	5.674	1153672	255479	23.278	4.858 #
21) L5 AR-1248-1	5.647	4.871	627635	249499	13.194	5.724 #
22) L5 AR-1248-2	5.933	5.104	247987	105997	4.235	1.809 #
23) L5 AR-1248-3	6.116	5.104f	77294	105997	1.185	1.751 #
24) L5 AR-1248-4	6.499	5.323	662274	198743	7.786	2.838 #
25) L5 AR-1248-5	6.559	5.674f	1153672	255479	13.785	3.597 #
26) L6 AR-1254-1	6.499	5.674	662274	255479	7.868	2.330 #
27) L6 AR-1254-2	6.714	5.827	410237	353649	3.271	3.740
28) L6 AR-1254-3	7.074	6.239	1177259	172001	8.972	1.166 #
29) L6 AR-1254-4	7.327	6.436	85663	426185	0.715	4.389 #
30) L6 AR-1254-5	7.755	6.837	100587	64952	0.880	0.500 #
31) L7 AR-1260-1	7.251	6.348	253992	32549	2.879	0.344 #
32) L7 AR-1260-2	7.506	6.523	543352	496621	3.999	4.265
33) L7 AR-1260-3	7.871	6.691	709335	152254	6.214	1.462 #
34) L7 AR-1260-4	8.089	7.162	388838	132377	3.773	1.509 #
35) L7 AR-1260-5	8.351f	7.387	115869	45482	0.482	0.213 #
36) L8 AR-1262-1	8.089	6.924	388838	126812	2.627	0.878 #
37) L8 AR-1262-2	8.351f	7.162	115869	132377	0.366	1.083 #
38) L8 AR-1262-3	8.701	7.680	128014	141556	0.598	1.256 #
39) L8 AR-1262-4	8.779	7.771	790301	306357	5.015	1.671 #
40) L8 AR-1262-5	9.421	8.249	882667	101585	7.891	1.173 #
41) L9 AR-1268-1	8.701	7.680	128014	141556	0.358	0.493 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 17:05
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:27:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.779	7.771	790301	306357	2.591	1.192 #
43) L9	AR-1268-3	8.987	7.958	243322	1199979	0.916	5.557 #
44) L9	AR-1268-4	9.421	8.249	882667	101585	7.543	1.079 #
45) L9	AR-1268-5	9.860	8.544	193867	301184	0.262	0.520 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
Data File : PP073087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 17:05
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1221 MDL 25 PPB
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:27:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

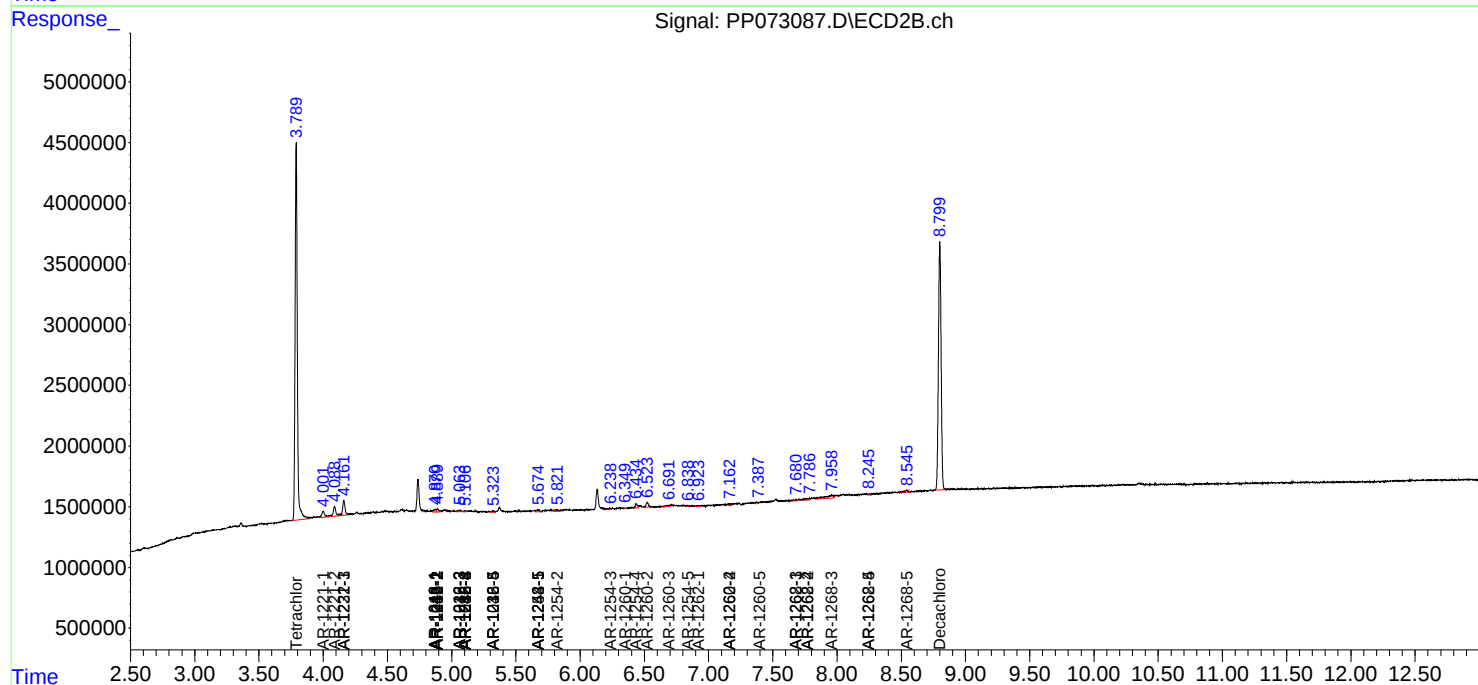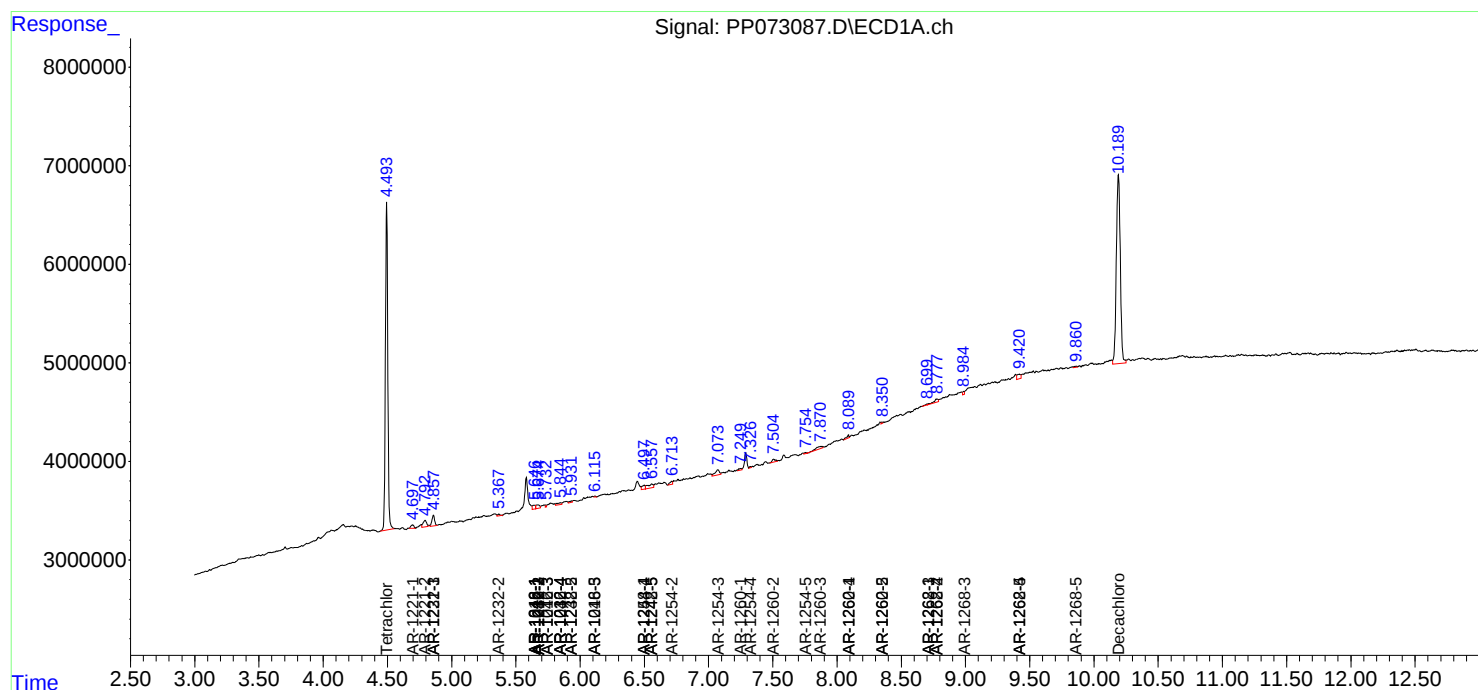


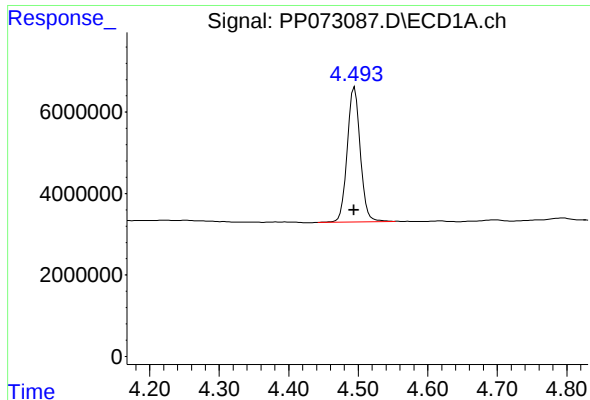

#1 Tetrachloro-m-xylene


R.T.: 4.495 min
Delta R.T.: 0.000 min
Response: 43074357
Conc: 20.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

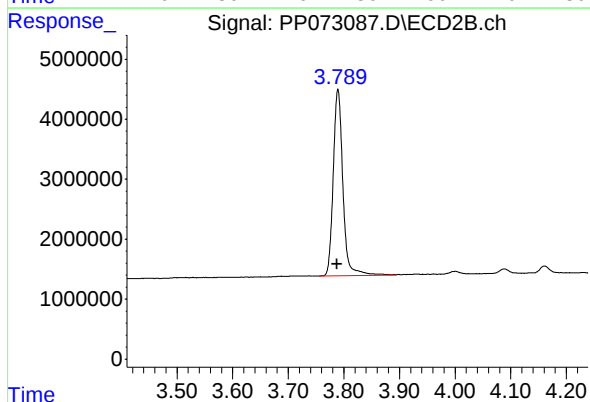


#1 Tetrachloro-m-xylene

R.T.: 3.789 min
Delta R.T.: 0.002 min
Response: 37597423
Conc: 20.87 ng/ml

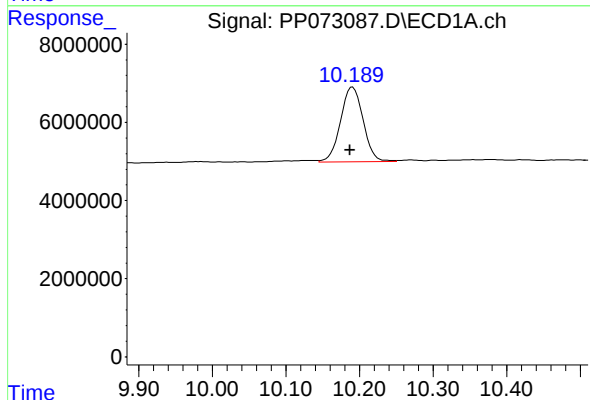


#2 Decachlorobiphenyl

R.T.: 10.191 min
Delta R.T.: 0.003 min
Response: 40859217
Conc: 23.91 ng/ml

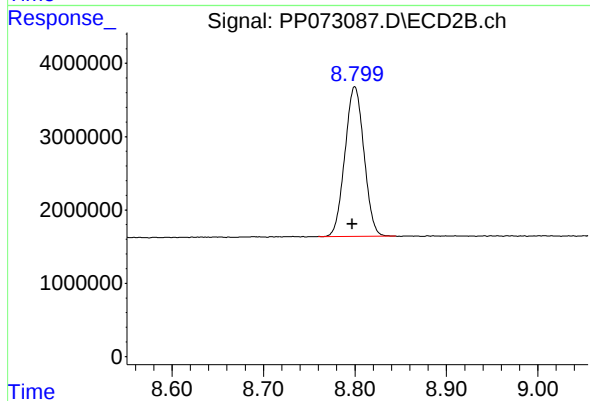

#2 Decachlorobiphenyl


R.T.: 8.800 min
Delta R.T.: 0.003 min
Response: 29524003
Conc: 22.12 ng/ml

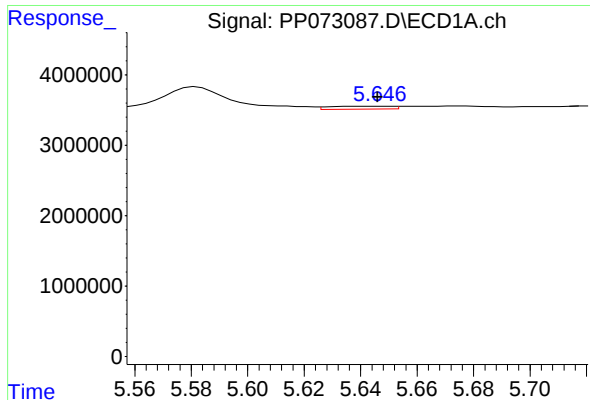

#3 AR-1016-1


R.T.: 5.647 min
Delta R.T.: 0.000 min
Response: 627635
Conc: 8.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

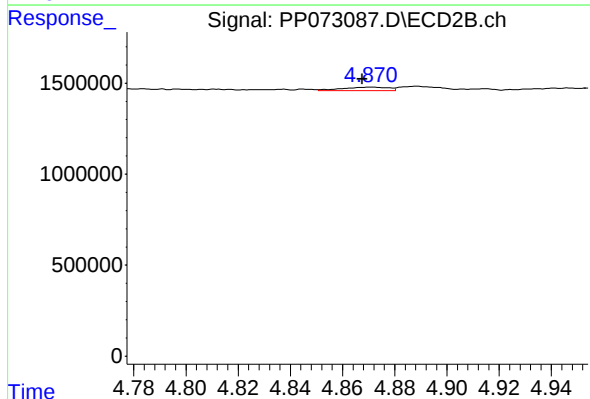


#3 AR-1016-1

R.T.: 4.871 min
Delta R.T.: 0.004 min
Response: 249499
Conc: 3.63 ng/ml

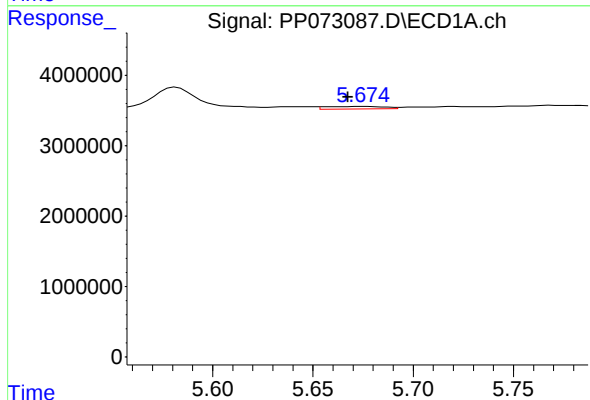


#4 AR-1016-2

R.T.: 5.675 min
Delta R.T.: 0.007 min
Response: 741424
Conc: 7.13 ng/ml

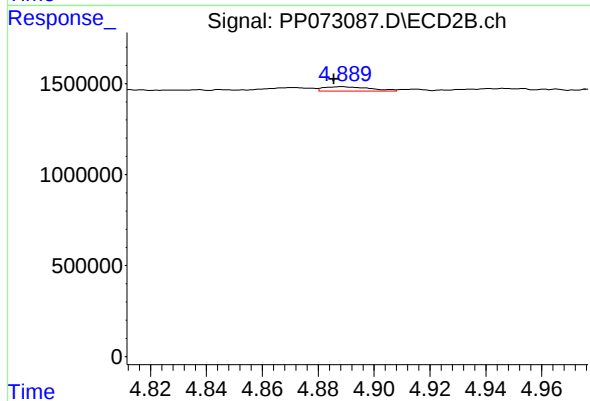

#4 AR-1016-2


R.T.: 4.889 min
Delta R.T.: 0.003 min
Response: 278463
Conc: 2.77 ng/ml

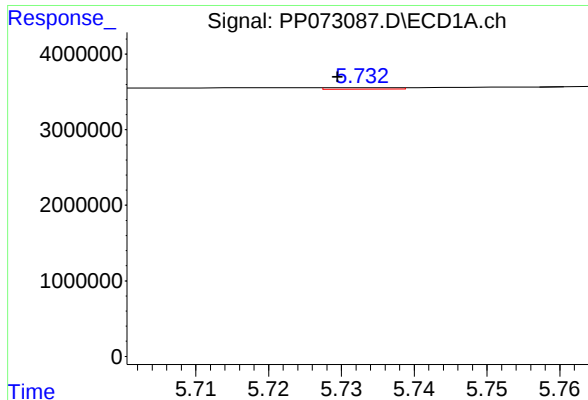

#5 AR-1016-3


R.T.: 5.734 min
Delta R.T.: 0.005 min
Response: 128521
Conc: 1.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

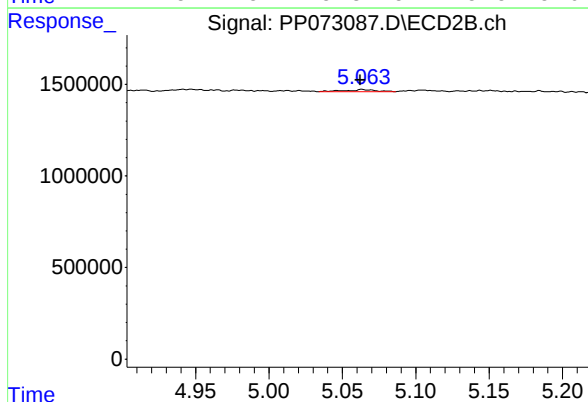


#5 AR-1016-3

R.T.: 5.063 min
Delta R.T.: 0.001 min
Response: 179214
Conc: 3.28 ng/ml

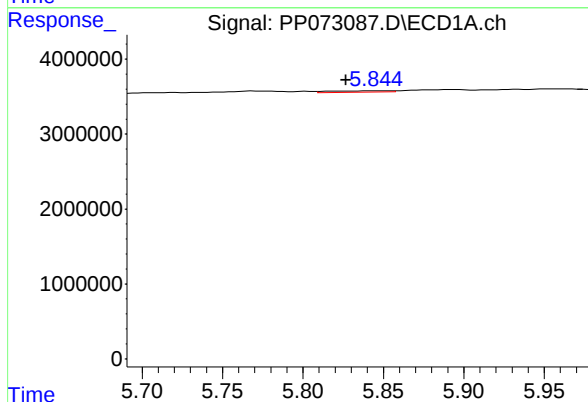


#6 AR-1016-4

R.T.: 5.846 min
Delta R.T.: 0.019 min
Response: 426050
Conc: 8.15 ng/ml

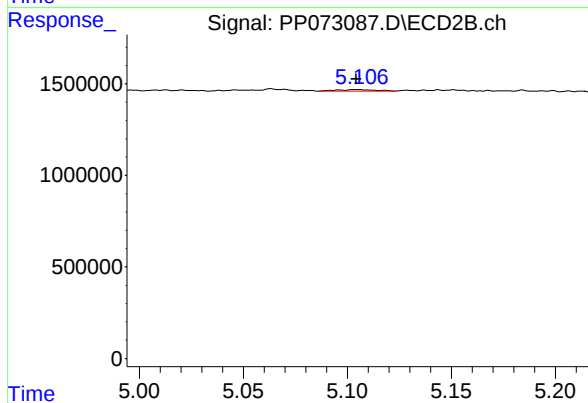

#6 AR-1016-4


R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 105997
Conc: 2.38 ng/ml

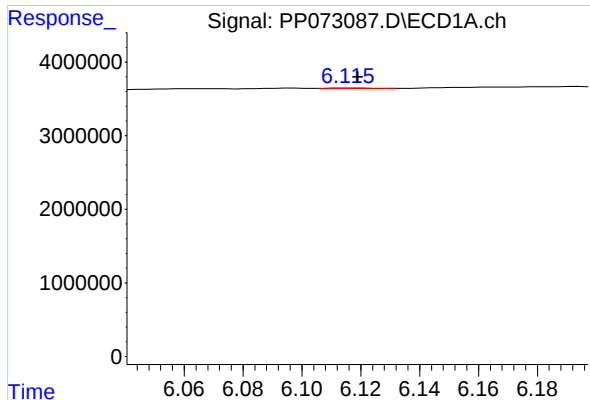

#7 AR-1016-5


R.T.: 6.116 min
Delta R.T.: -0.003 min
Response: 77294
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

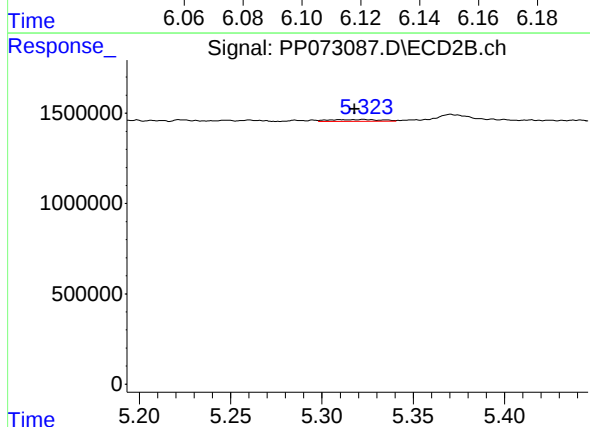


#7 AR-1016-5

R.T.: 5.323 min
Delta R.T.: 0.005 min
Response: 198743
Conc: 3.60 ng/ml

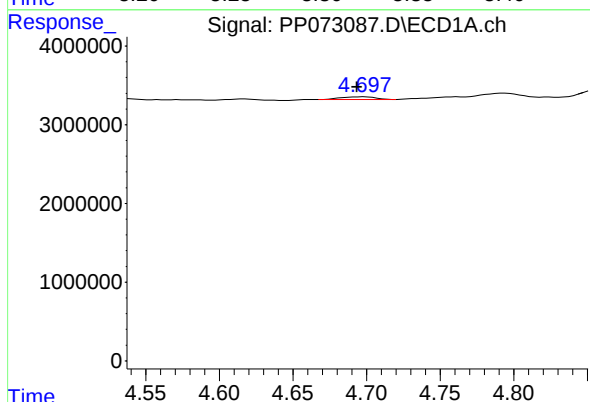


#8 AR-1221-1

R.T.: 4.698 min
Delta R.T.: 0.005 min
Response: 558426
Conc: 22.65 ng/ml

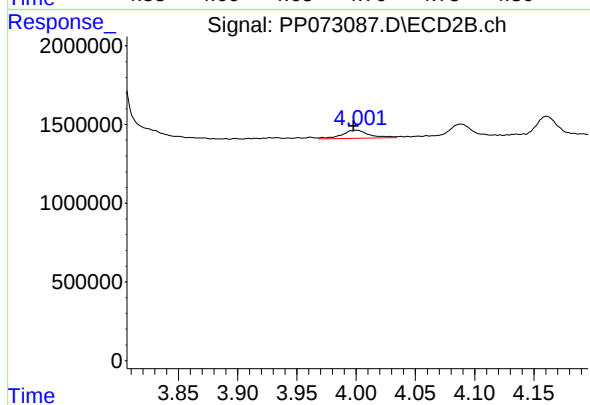

#8 AR-1221-1


R.T.: 4.001 min
Delta R.T.: 0.003 min
Response: 801112
Conc: 29.81 ng/ml

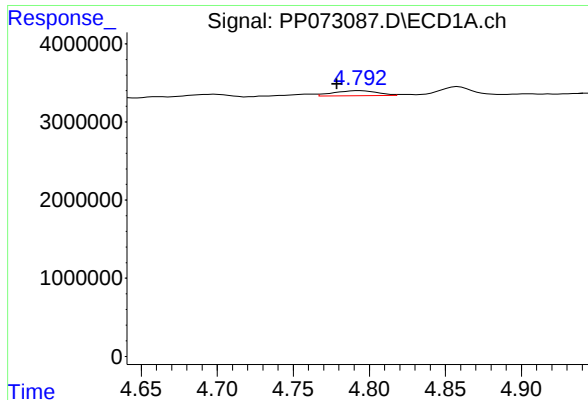

#9 AR-1221-2


R.T.: 4.794 min
Delta R.T.: 0.015 min
Response: 1325906
Conc: 65.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

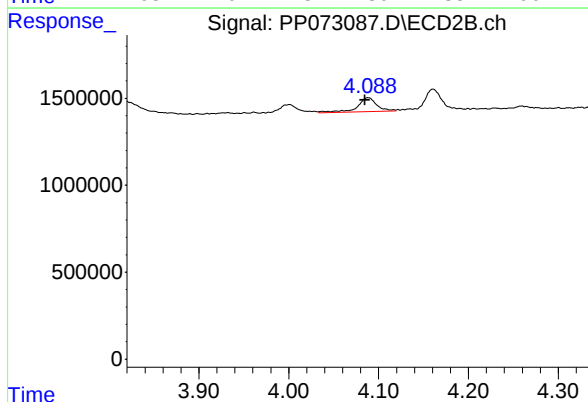


#9 AR-1221-2

R.T.: 4.088 min
Delta R.T.: 0.004 min
Response: 1216059
Conc: 60.24 ng/ml

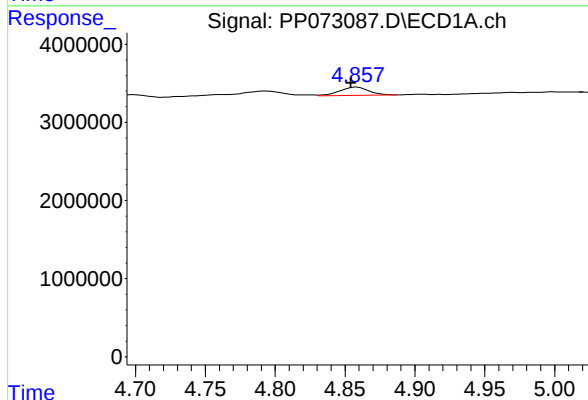


#10 AR-1221-3

R.T.: 4.859 min
Delta R.T.: 0.004 min
Response: 1526600
Conc: 24.80 ng/ml

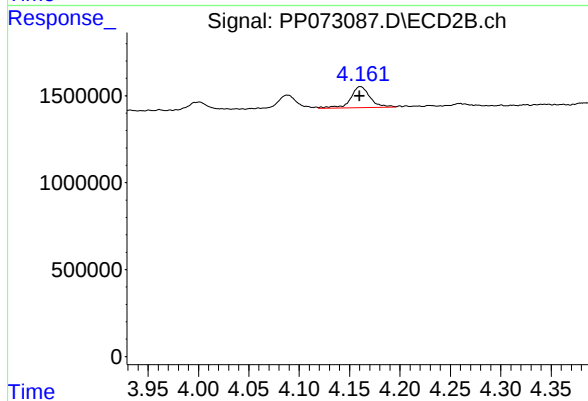

#10 AR-1221-3


R.T.: 4.161 min
Delta R.T.: 0.000 min
Response: 1635649
Conc: 27.85 ng/ml

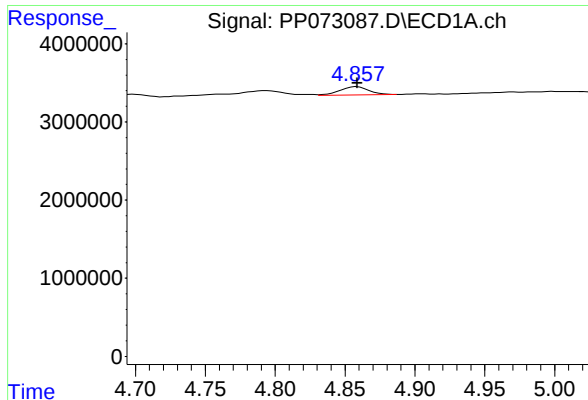

#11 AR-1232-1


R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 1526600
Conc: 32.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

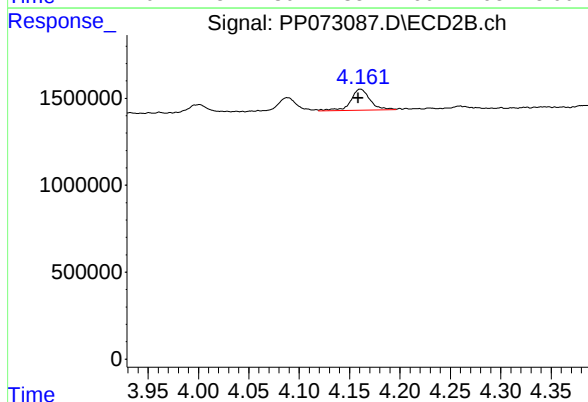


#11 AR-1232-1

R.T.: 4.161 min
Delta R.T.: 0.002 min
Response: 1635649
Conc: 35.90 ng/ml

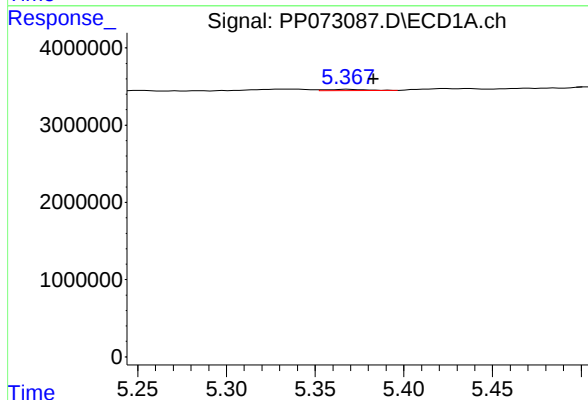


#12 AR-1232-2

R.T.: 5.368 min
Delta R.T.: -0.015 min
Response: 246080
Conc: 11.00 ng/ml

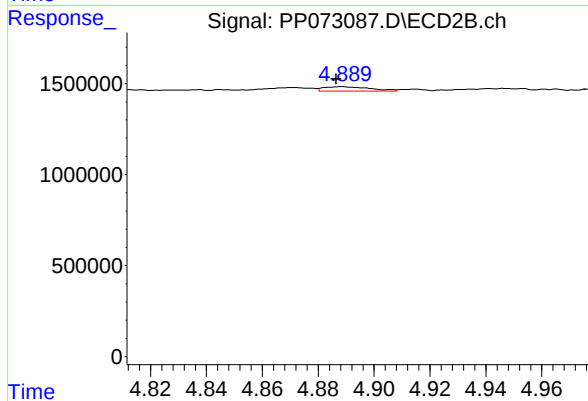

#12 AR-1232-2


R.T.: 4.889 min
Delta R.T.: 0.002 min
Response: 278463
Conc: 6.02 ng/ml

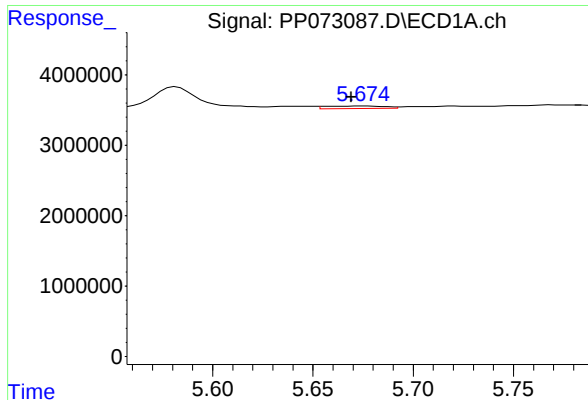

#13 AR-1232-3


R.T.: 5.675 min
Delta R.T.: 0.006 min
Response: 741424
Conc: 14.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

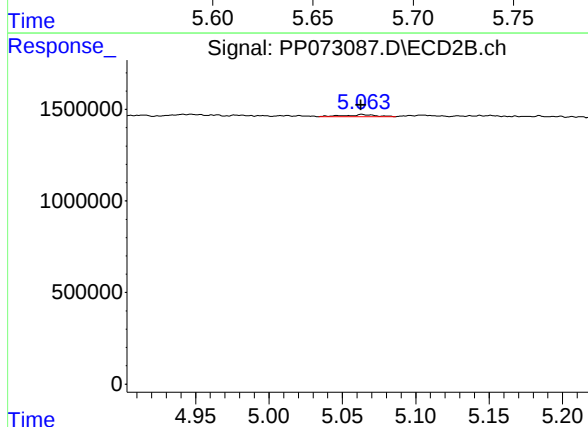


#13 AR-1232-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 179214
Conc: 7.30 ng/ml

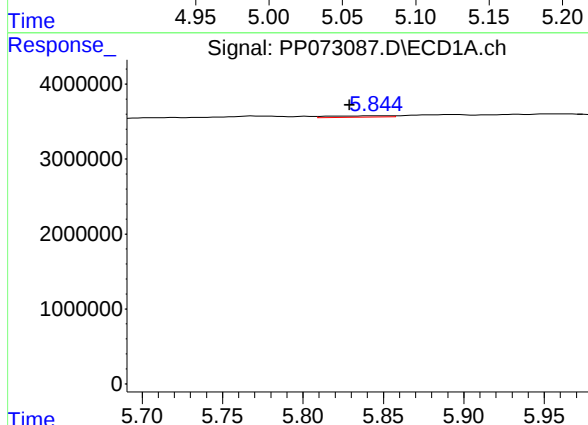


#14 AR-1232-4

R.T.: 5.846 min
Delta R.T.: 0.017 min
Response: 426050
Conc: 16.51 ng/ml

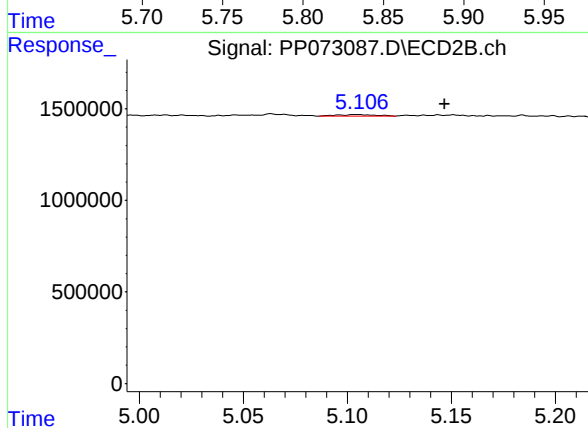

#14 AR-1232-4


R.T.: 5.104 min
Delta R.T.: -0.042 min
Response: 105997
Conc: 4.90 ng/ml

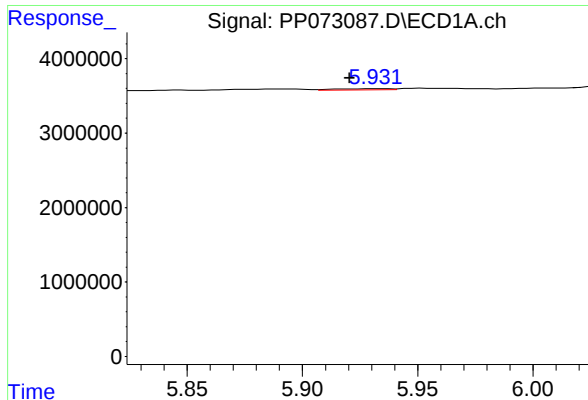

#15 AR-1232-5


R.T.: 5.933 min
Delta R.T.: 0.013 min
Response: 247987
Conc: 6.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

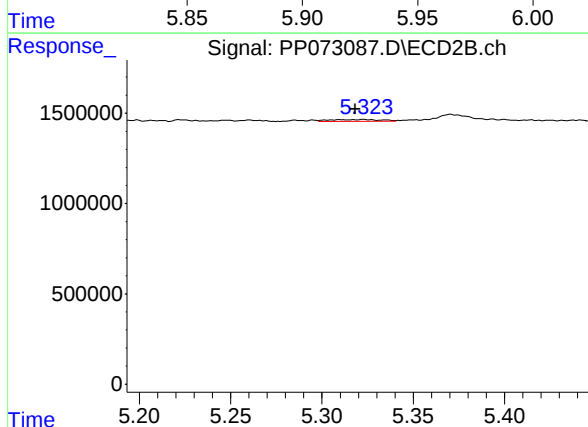


#15 AR-1232-5

R.T.: 5.323 min
Delta R.T.: 0.005 min
Response: 198743
Conc: 8.69 ng/ml

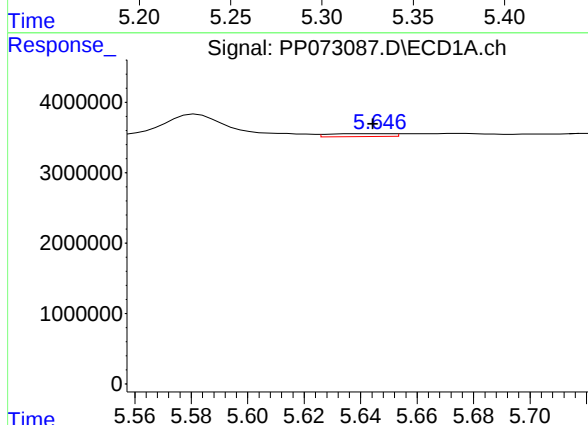


#16 AR-1242-1

R.T.: 5.647 min
Delta R.T.: 0.003 min
Response: 627635
Conc: 10.74 ng/ml

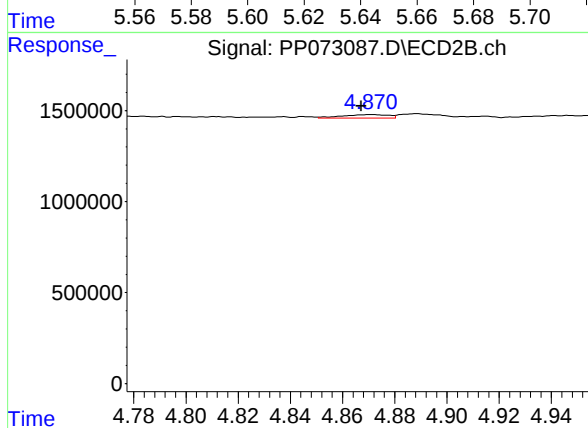

#16 AR-1242-1


R.T.: 4.871 min
Delta R.T.: 0.004 min
Response: 249499
Conc: 4.52 ng/ml

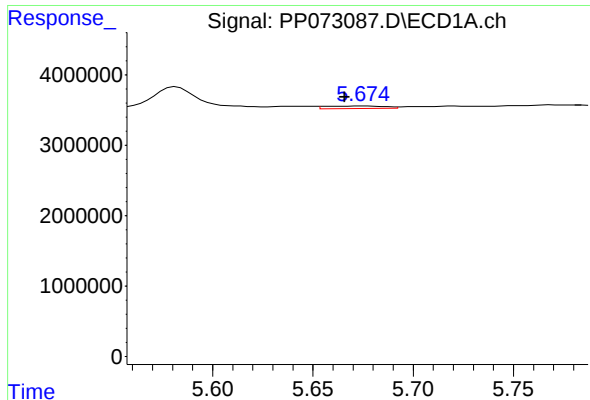

#17 AR-1242-2


R.T.: 5.675 min
Delta R.T.: 0.009 min
Response: 741424
Conc: 8.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

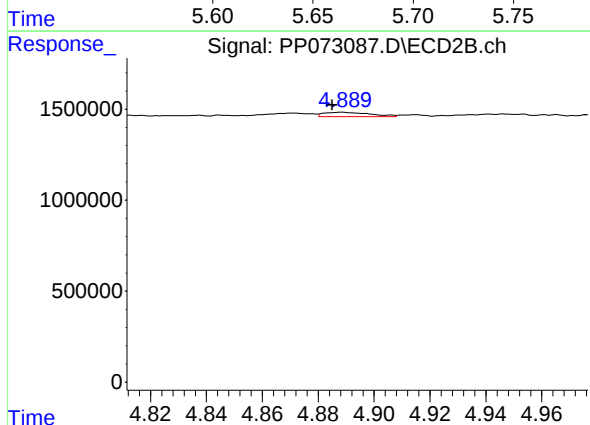


#17 AR-1242-2

R.T.: 4.889 min
Delta R.T.: 0.003 min
Response: 278463
Conc: 3.50 ng/ml

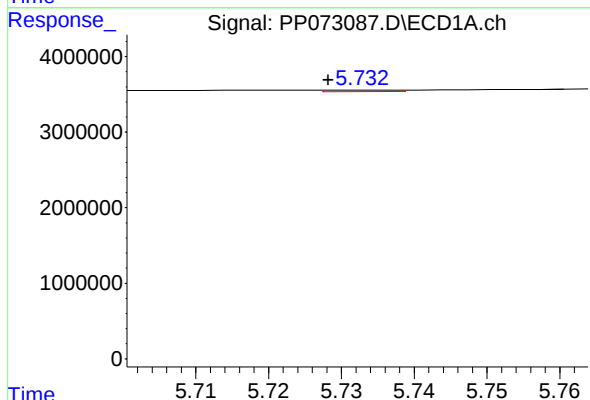


#18 AR-1242-3

R.T.: 5.734 min
Delta R.T.: 0.006 min
Response: 128521
Conc: 2.44 ng/ml

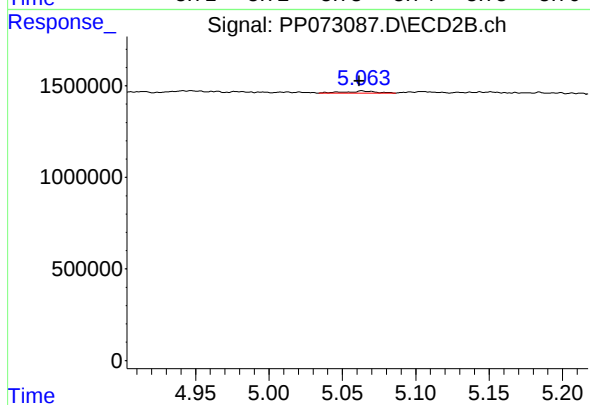

#18 AR-1242-3


R.T.: 5.063 min
Delta R.T.: 0.002 min
Response: 179214
Conc: 4.14 ng/ml

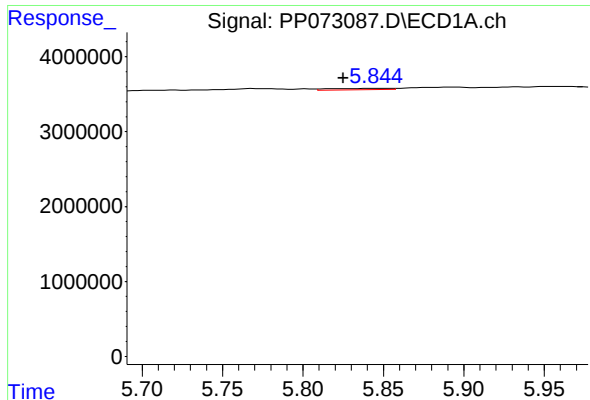

#19 AR-1242-4


R.T.: 5.846 min
Delta R.T.: 0.021 min
Response: 426050
Conc: 9.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

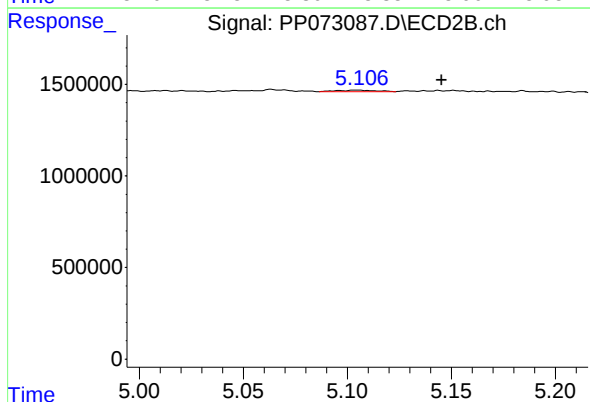


#19 AR-1242-4

R.T.: 5.104 min
Delta R.T.: -0.041 min
Response: 105997
Conc: 2.55 ng/ml

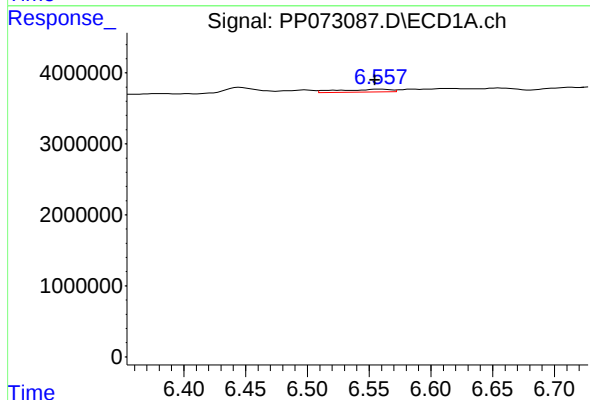


#20 AR-1242-5

R.T.: 6.559 min
Delta R.T.: 0.004 min
Response: 1153672
Conc: 23.28 ng/ml

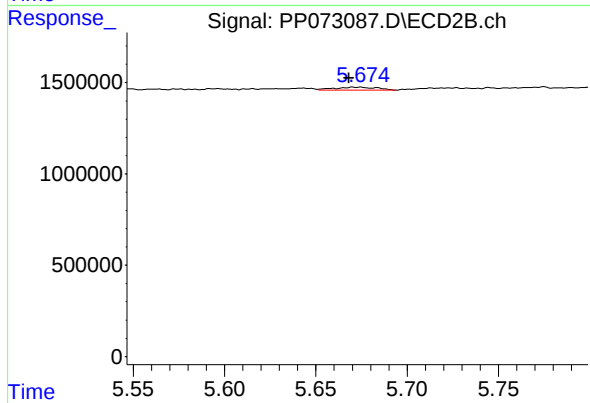

#20 AR-1242-5


R.T.: 5.674 min
Delta R.T.: 0.006 min
Response: 255479
Conc: 4.86 ng/ml

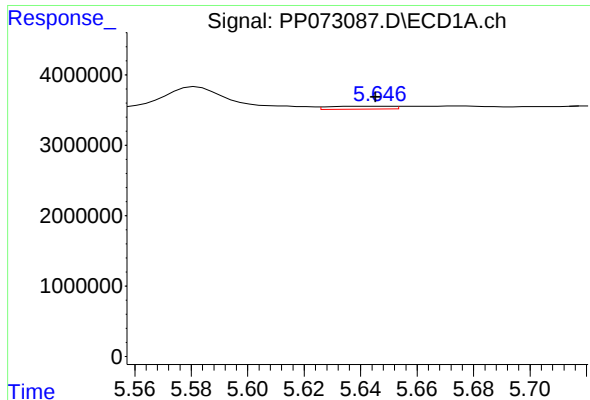

#21 AR-1248-1


R.T.: 5.647 min
Delta R.T.: 0.002 min
Response: 627635
Conc: 13.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

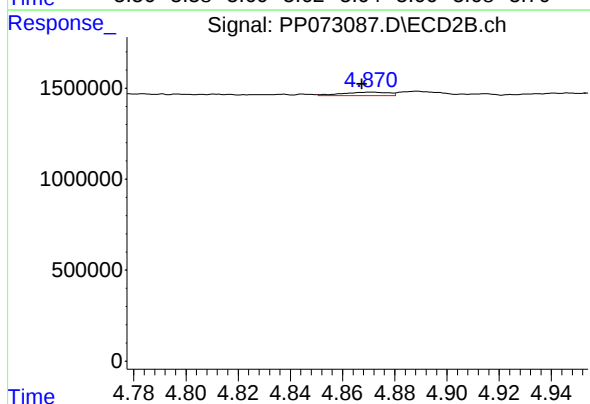


#21 AR-1248-1

R.T.: 4.871 min
Delta R.T.: 0.004 min
Response: 249499
Conc: 5.72 ng/ml

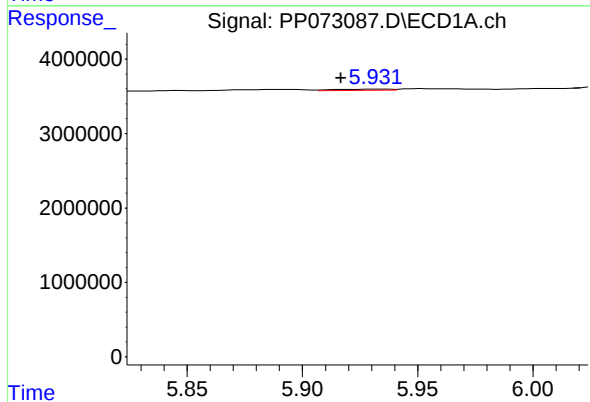


#22 AR-1248-2

R.T.: 5.933 min
Delta R.T.: 0.016 min
Response: 247987
Conc: 4.24 ng/ml

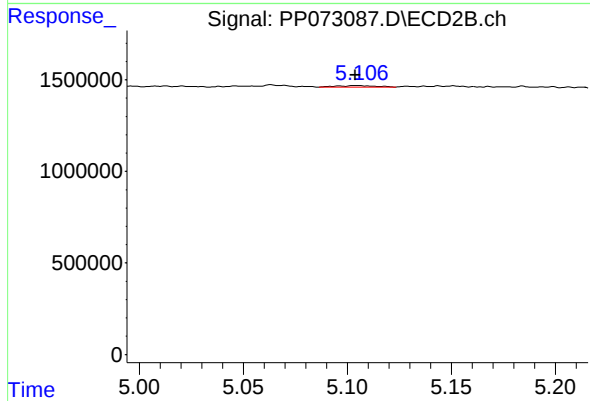

#22 AR-1248-2


R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 105997
Conc: 1.81 ng/ml

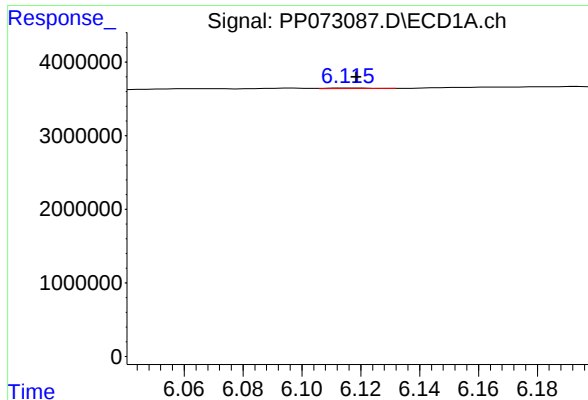

#23 AR-1248-3


R.T.: 6.116 min
Delta R.T.: -0.002 min
Response: 77294
Conc: 1.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

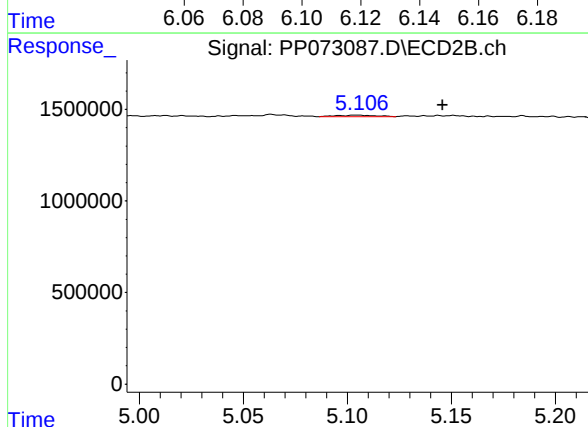


#23 AR-1248-3

R.T.: 5.104 min
Delta R.T.: -0.041 min
Response: 105997
Conc: 1.75 ng/ml

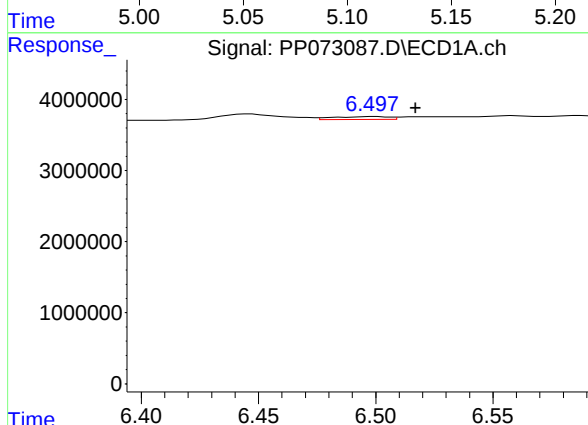


#24 AR-1248-4

R.T.: 6.499 min
Delta R.T.: -0.018 min
Response: 662274
Conc: 7.79 ng/ml

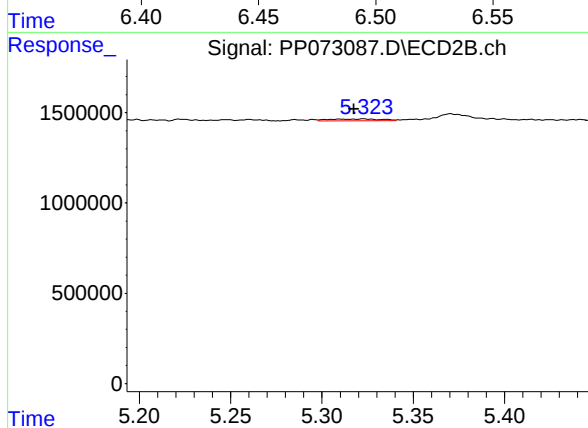

#24 AR-1248-4


R.T.: 5.323 min
Delta R.T.: 0.005 min
Response: 198743
Conc: 2.84 ng/ml

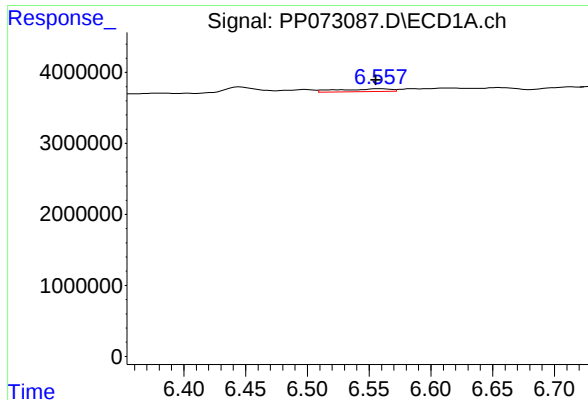

#25 AR-1248-5


R.T.: 6.559 min
Delta R.T.: 0.003 min
Response: 1153672
Conc: 13.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

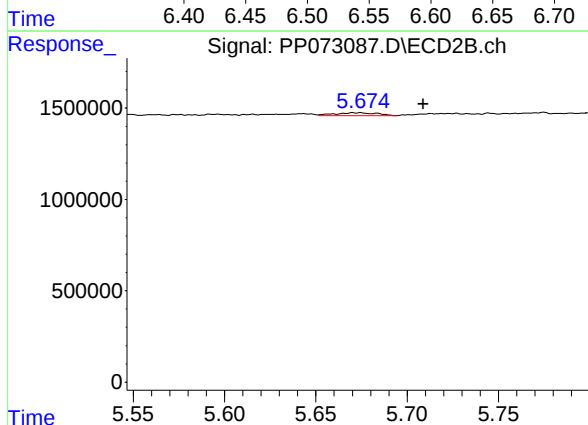


#25 AR-1248-5

R.T.: 5.674 min
Delta R.T.: -0.035 min
Response: 255479
Conc: 3.60 ng/ml

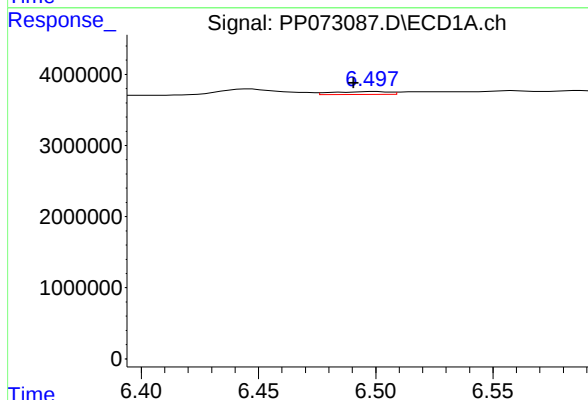


#26 AR-1254-1

R.T.: 6.499 min
Delta R.T.: 0.009 min
Response: 662274
Conc: 7.87 ng/ml

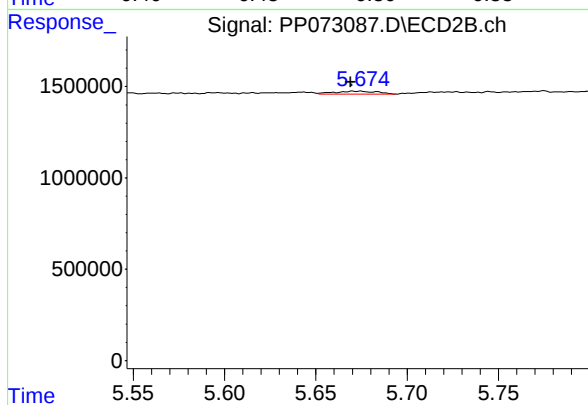

#26 AR-1254-1


R.T.: 5.674 min
Delta R.T.: 0.005 min
Response: 255479
Conc: 2.33 ng/ml

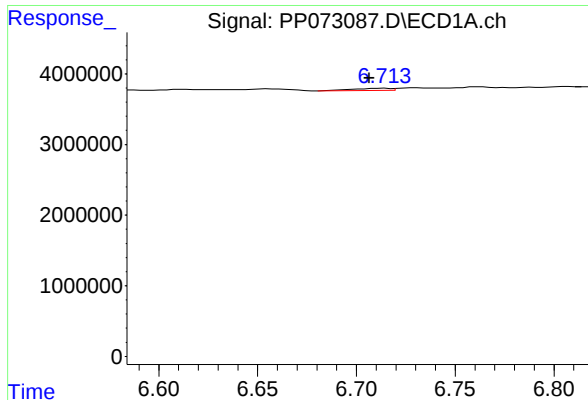

#27 AR-1254-2


R.T.: 6.714 min
Delta R.T.: 0.008 min
Response: 410237
Conc: 3.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

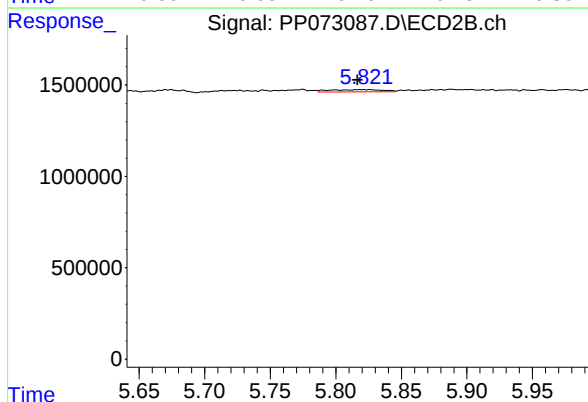


#27 AR-1254-2

R.T.: 5.827 min
Delta R.T.: 0.010 min
Response: 353649
Conc: 3.74 ng/ml

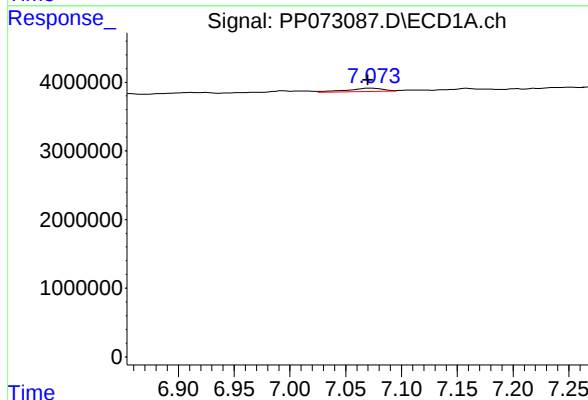


#28 AR-1254-3

R.T.: 7.074 min
Delta R.T.: 0.004 min
Response: 1177259
Conc: 8.97 ng/ml

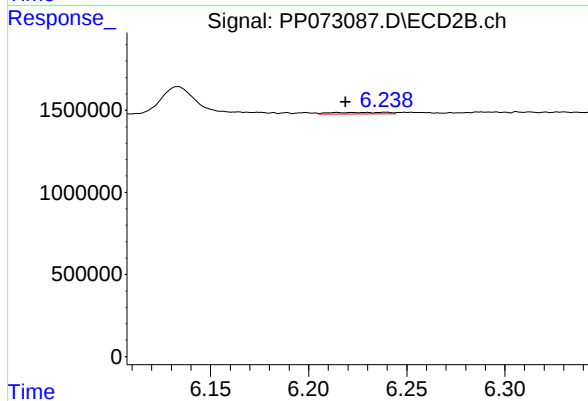

#28 AR-1254-3


R.T.: 6.239 min
Delta R.T.: 0.020 min
Response: 172001
Conc: 1.17 ng/ml

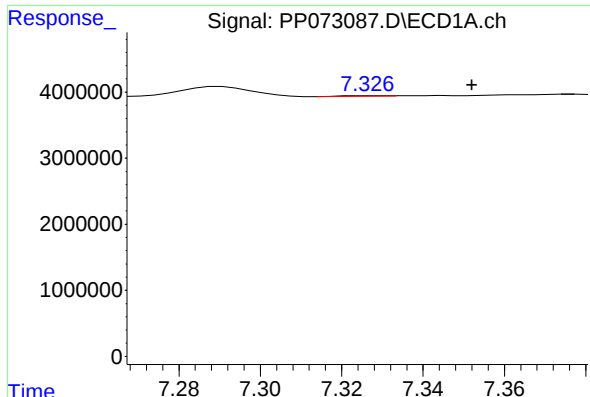

#29 AR-1254-4


R.T.: 7.327 min
Delta R.T.: -0.025 min
Response: 85663
Conc: 0.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

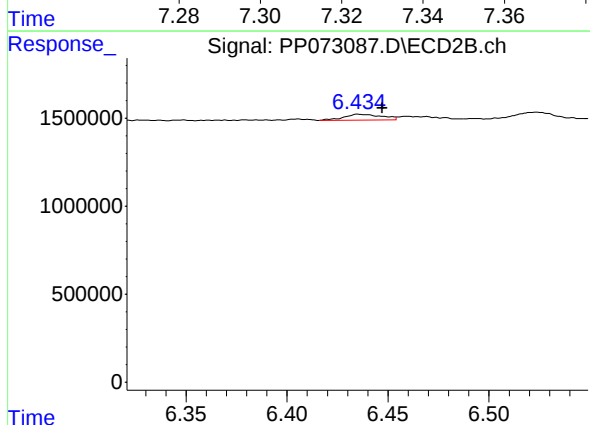


#29 AR-1254-4

R.T.: 6.436 min
Delta R.T.: -0.012 min
Response: 426185
Conc: 4.39 ng/ml

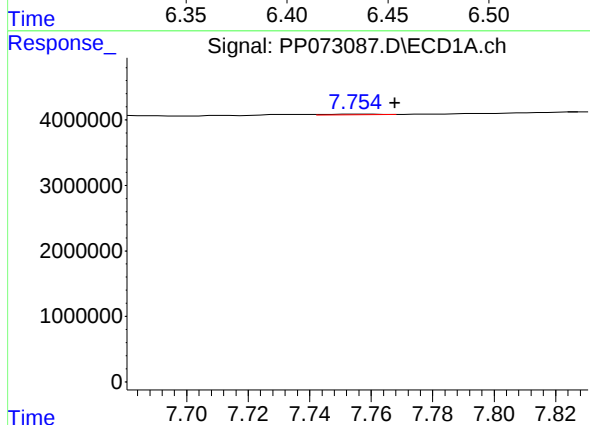


#30 AR-1254-5

R.T.: 7.755 min
Delta R.T.: -0.012 min
Response: 100587
Conc: 0.88 ng/ml

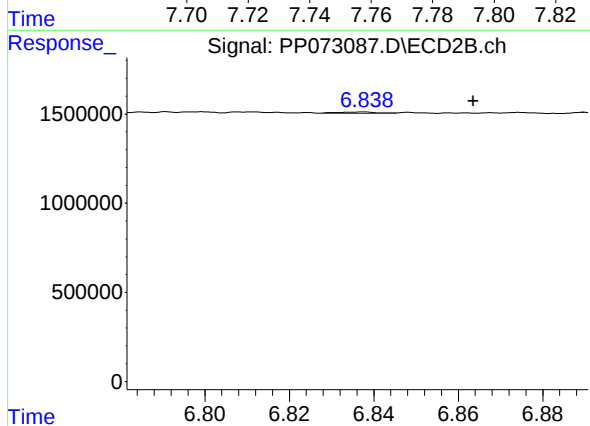

#30 AR-1254-5


R.T.: 6.837 min
Delta R.T.: -0.026 min
Response: 64952
Conc: 0.50 ng/ml

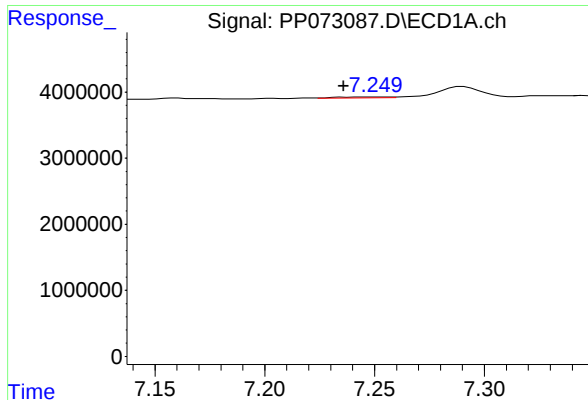

#31 AR-1260-1


R.T.: 7.251 min
Delta R.T.: 0.015 min
Response: 253992
Conc: 2.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

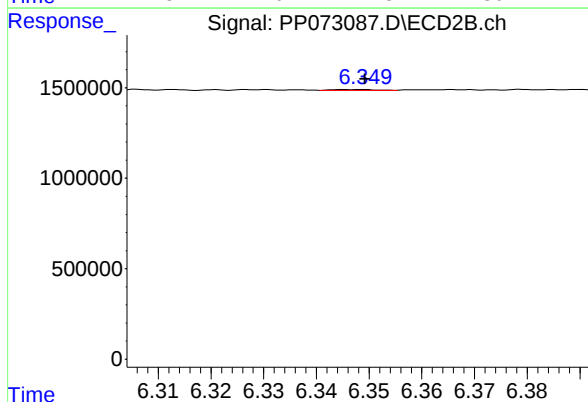


#31 AR-1260-1

R.T.: 6.348 min
Delta R.T.: -0.001 min
Response: 32549
Conc: 0.34 ng/ml

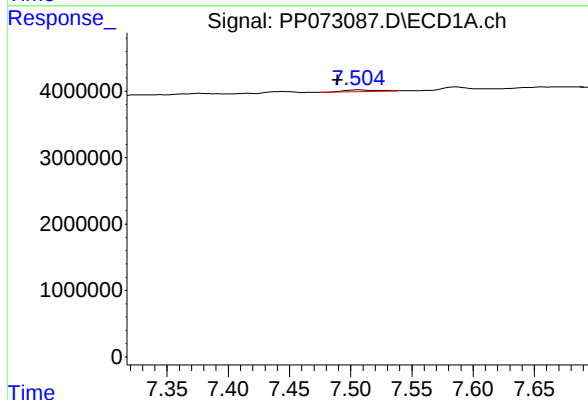


#32 AR-1260-2

R.T.: 7.506 min
Delta R.T.: 0.017 min
Response: 543352
Conc: 4.00 ng/ml

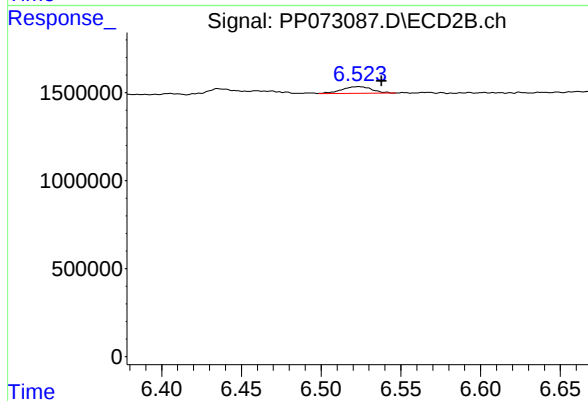

#32 AR-1260-2


R.T.: 6.523 min
Delta R.T.: -0.015 min
Response: 496621
Conc: 4.27 ng/ml

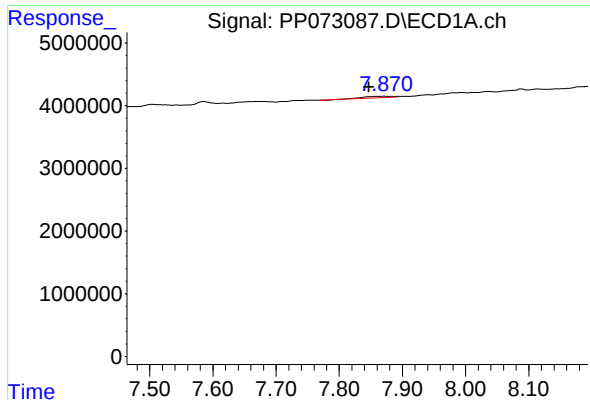

#33 AR-1260-3


R.T.: 7.871 min
Delta R.T.: 0.024 min
Response: 709335
Conc: 6.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

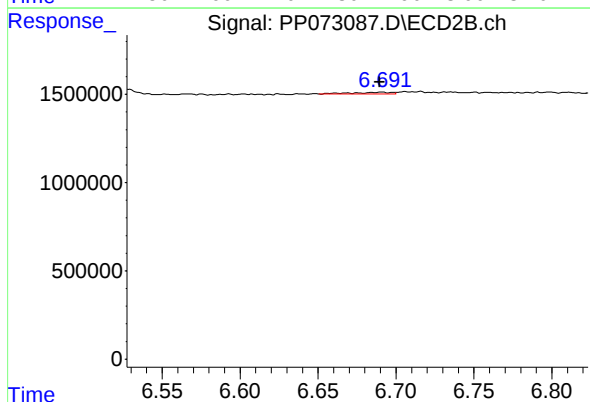


#33 AR-1260-3

R.T.: 6.691 min
Delta R.T.: 0.001 min
Response: 152254
Conc: 1.46 ng/ml

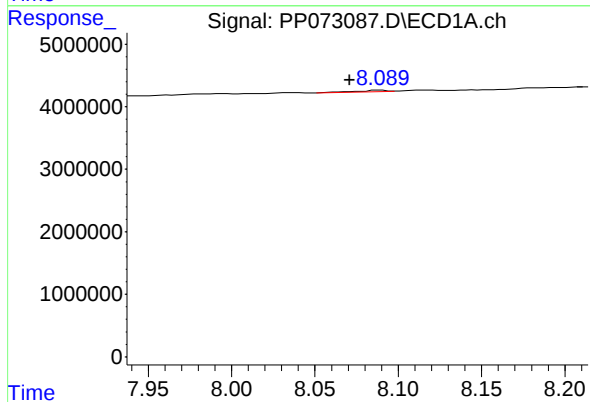


#34 AR-1260-4

R.T.: 8.089 min
Delta R.T.: 0.018 min
Response: 388838
Conc: 3.77 ng/ml

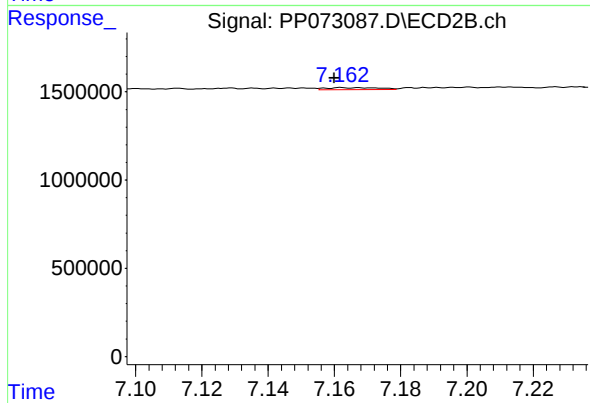

#34 AR-1260-4


R.T.: 7.162 min
Delta R.T.: 0.002 min
Response: 132377
Conc: 1.51 ng/ml

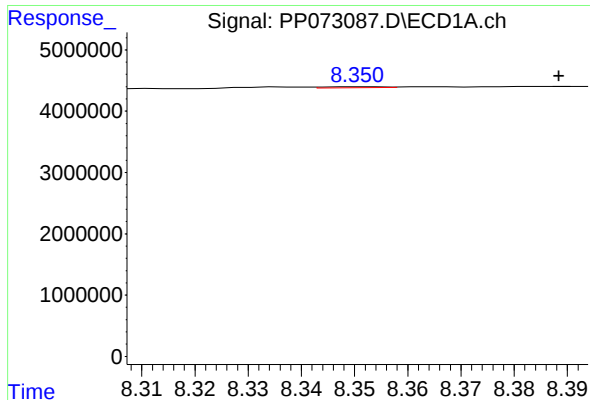

#35 AR-1260-5


R.T.: 8.351 min
Delta R.T.: -0.037 min
Response: 115869
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

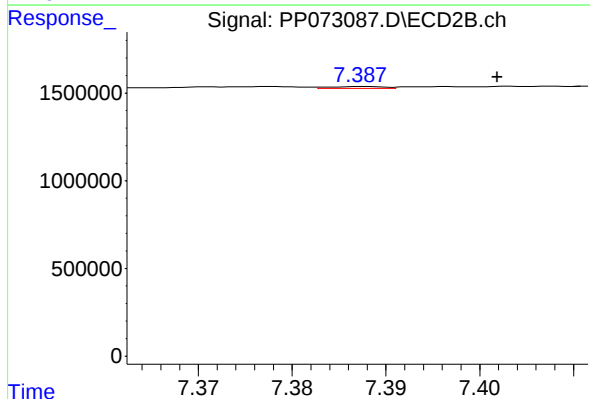


#35 AR-1260-5

R.T.: 7.387 min
Delta R.T.: -0.014 min
Response: 45482
Conc: 0.21 ng/ml

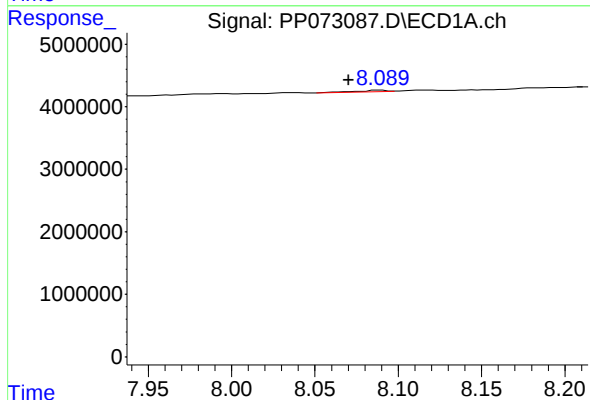


#36 AR-1262-1

R.T.: 8.089 min
Delta R.T.: 0.019 min
Response: 388838
Conc: 2.63 ng/ml

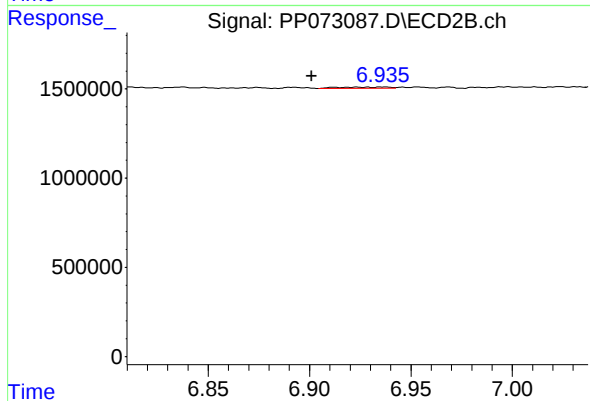

#36 AR-1262-1


R.T.: 6.924 min
Delta R.T.: 0.023 min
Response: 126812
Conc: 0.88 ng/ml

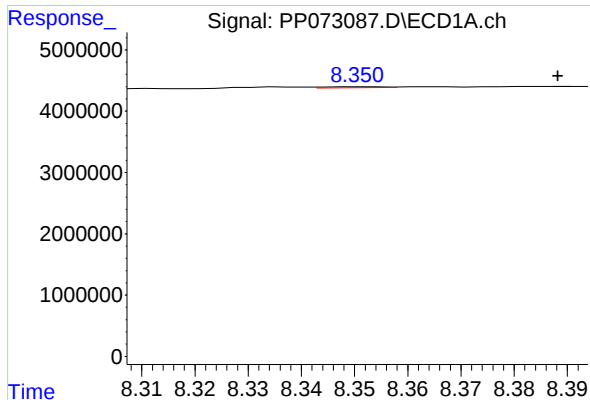

#37 AR-1262-2


R.T.: 8.351 min
Delta R.T.: -0.037 min
Response: 115869
Conc: 0.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

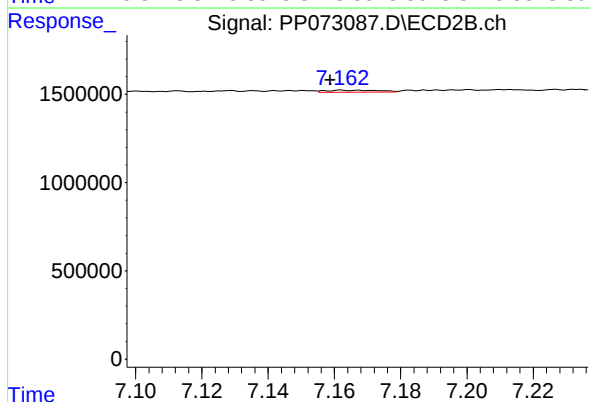


#37 AR-1262-2

R.T.: 7.162 min
Delta R.T.: 0.003 min
Response: 132377
Conc: 1.08 ng/ml

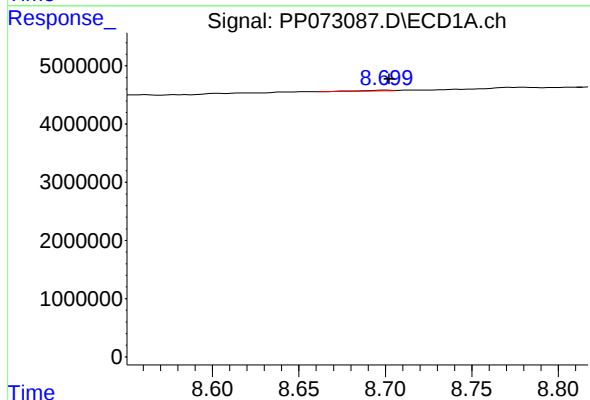


#38 AR-1262-3

R.T.: 8.701 min
Delta R.T.: -0.001 min
Response: 128014
Conc: 0.60 ng/ml

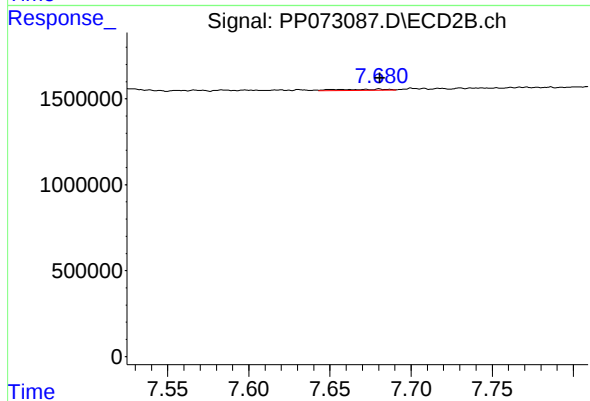

#38 AR-1262-3


R.T.: 7.680 min
Delta R.T.: 0.000 min
Response: 141556
Conc: 1.26 ng/ml

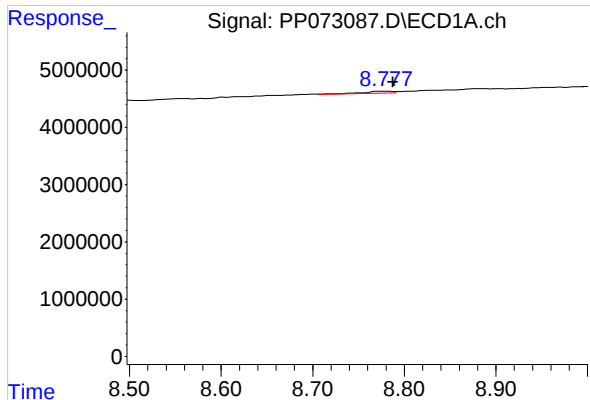

#39 AR-1262-4


R.T.: 8.779 min
Delta R.T.: -0.009 min
Response: 790301
Conc: 5.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

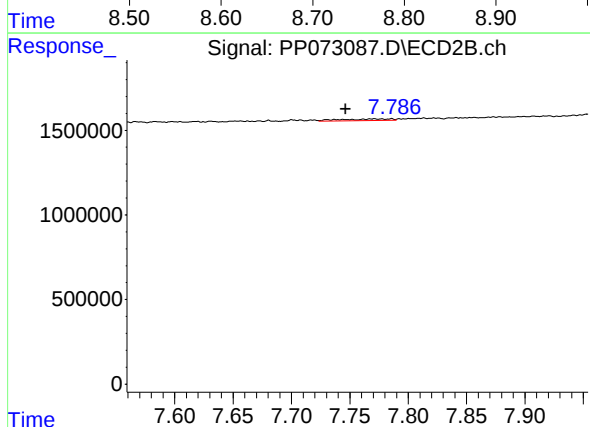


#39 AR-1262-4

R.T.: 7.771 min
Delta R.T.: 0.024 min
Response: 306357
Conc: 1.67 ng/ml

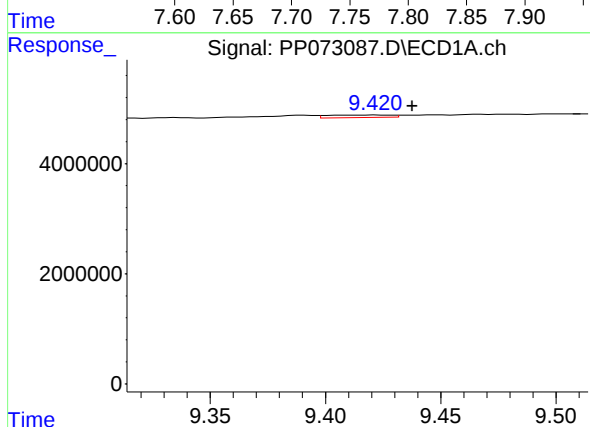


#40 AR-1262-5

R.T.: 9.421 min
Delta R.T.: -0.016 min
Response: 882667
Conc: 7.89 ng/ml

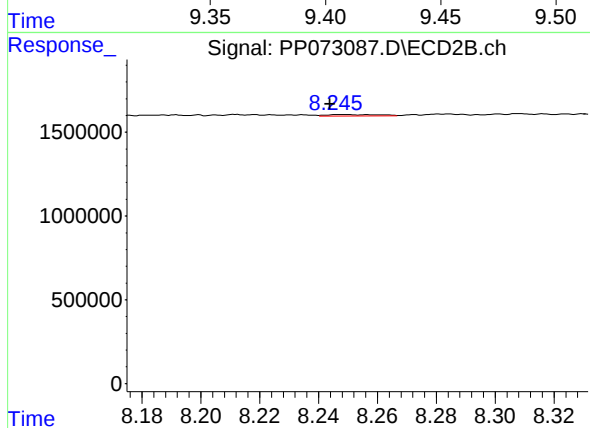

#40 AR-1262-5


R.T.: 8.249 min
Delta R.T.: 0.005 min
Response: 101585
Conc: 1.17 ng/ml

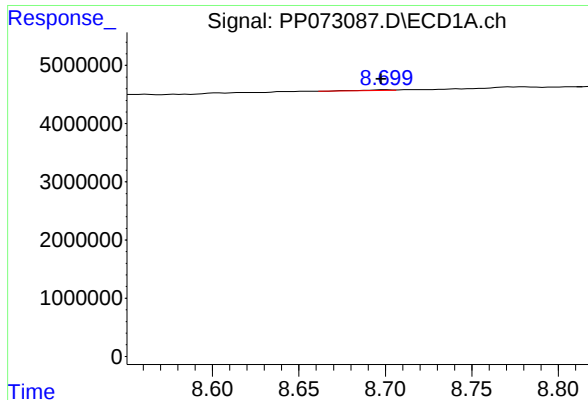

#41 AR-1268-1


R.T.: 8.701 min
Delta R.T.: 0.003 min
Response: 128014
Conc: 0.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

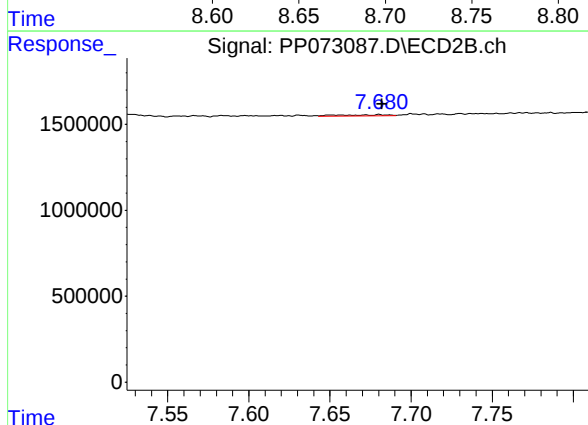


#41 AR-1268-1

R.T.: 7.680 min
Delta R.T.: -0.002 min
Response: 141556
Conc: 0.49 ng/ml

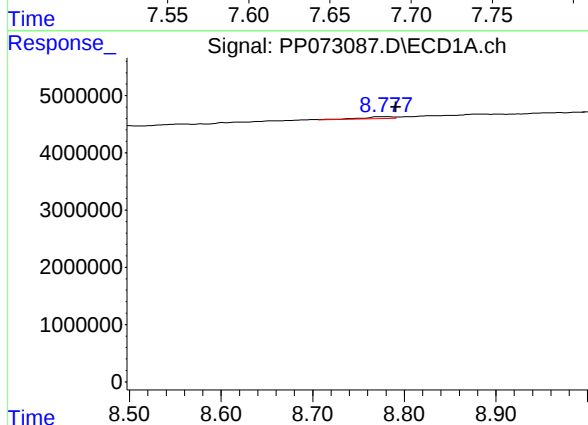


#42 AR-1268-2

R.T.: 8.779 min
Delta R.T.: -0.012 min
Response: 790301
Conc: 2.59 ng/ml

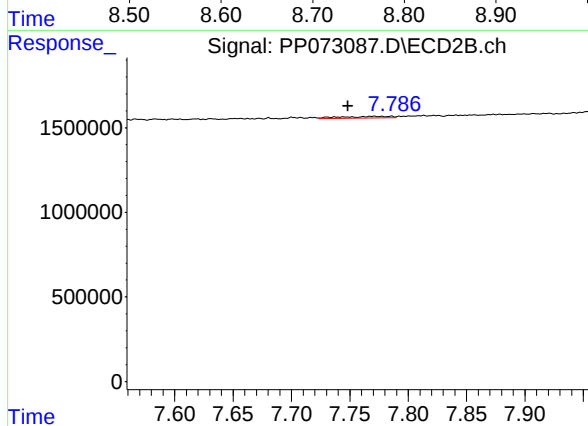

#42 AR-1268-2


R.T.: 7.771 min
Delta R.T.: 0.022 min
Response: 306357
Conc: 1.19 ng/ml

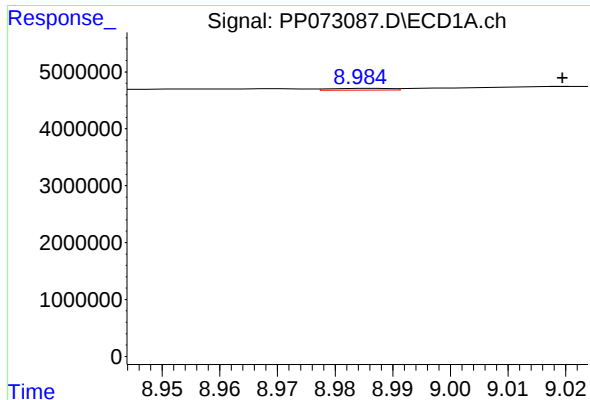

#43 AR-1268-3


R.T.: 8.987 min
Delta R.T.: -0.033 min
Response: 243322
Conc: 0.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

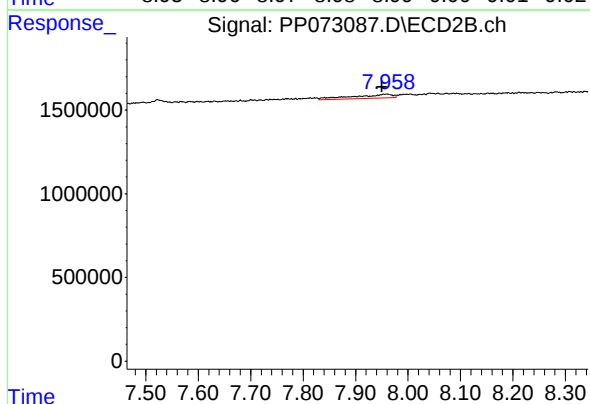


#43 AR-1268-3

R.T.: 7.958 min
Delta R.T.: 0.008 min
Response: 1199979
Conc: 5.56 ng/ml

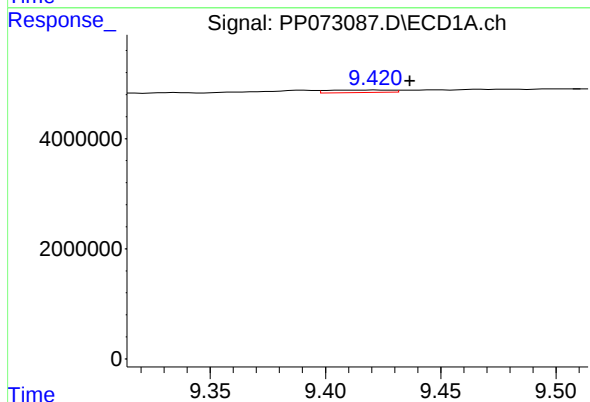


#44 AR-1268-4

R.T.: 9.421 min
Delta R.T.: -0.015 min
Response: 882667
Conc: 7.54 ng/ml

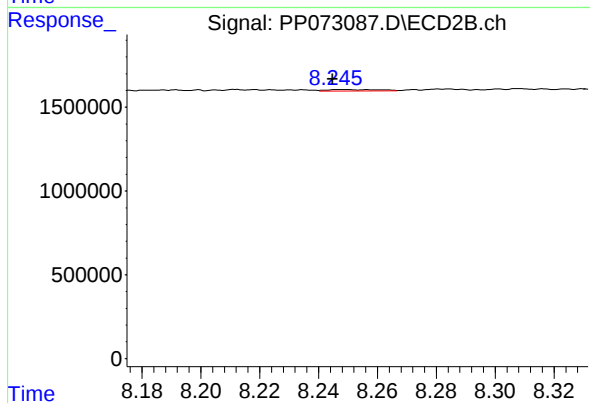

#44 AR-1268-4


R.T.: 8.249 min
Delta R.T.: 0.004 min
Response: 101585
Conc: 1.08 ng/ml

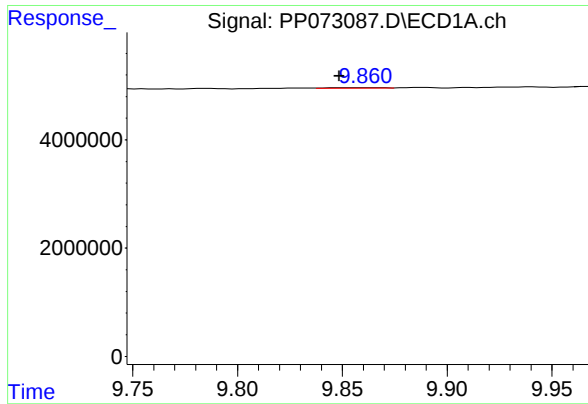

#45 AR-1268-5

R.T.: 9.860 min
Delta R.T.: 0.012 min
Response: 193867
Conc: 0.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

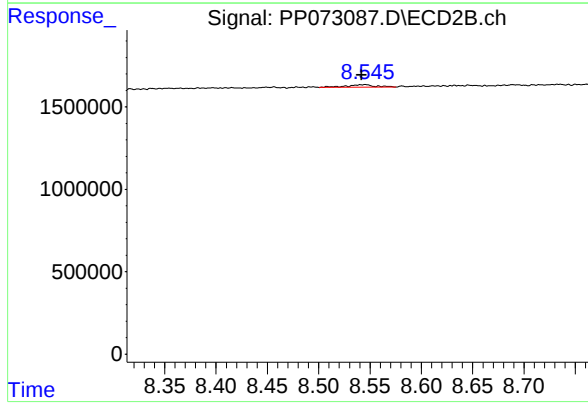

#45 AR-1268-5

R.T.: 8.544 min
Delta R.T.: 0.003 min
Response: 301184
Conc: 0.52 ng/ml