

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 17:21
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:27:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.789	43371716	36267481	20.547	20.129
2) SA Decachlor...	10.188	8.799	40707412	29954096	23.821	22.442
Target Compounds						
3) L1 AR-1016-1	5.644	4.869	1285923	776866	17.695	11.305 #
4) L1 AR-1016-2	5.665	4.887	2113265	1338273	20.316	13.298 #
5) L1 AR-1016-3	5.728	5.063	1104800	667040	16.906	12.191 #
6) L1 AR-1016-4	5.826	5.106	645129	510043	12.340	11.449
7) L1 AR-1016-5	6.117	5.319	420489	666528	8.409	12.057 #
8) L2 AR-1221-1	4.692	3.998	548747	605096	22.253	22.517
9) L2 AR-1221-2	4.794	4.088	1109774	1055376	54.996	52.284
10) L2 AR-1221-3	4.856	4.160	1232784	1324610	20.029	22.553
11) L3 AR-1232-1	4.856	4.160	1232784	1324610	26.254	29.071
12) L3 AR-1232-2	5.379	4.887	822830	1338273	36.783	28.929
13) L3 AR-1232-3	5.665	5.063	2113265	667040	40.957	27.162 #
14) L3 AR-1232-4	5.826	5.148	645129	580358	24.995	26.837
15) L3 AR-1232-5	5.916	5.319	478642	666528	13.419	29.158 #
16) L4 AR-1242-1	5.644	4.869	1285923	776866	22.005	14.069 #
17) L4 AR-1242-2	5.665	4.887	2113265	1338273	24.415	16.837 #
18) L4 AR-1242-3	5.728	5.063	1104800	667040	20.961	15.403 #
19) L4 AR-1242-4	5.826	5.148	645129	580358	14.676	13.983
20) L4 AR-1242-5	6.555	5.671	847395	668508	17.098	12.713 #
21) L5 AR-1248-1	5.644	4.869	1285923	776866	27.033	17.822 #
22) L5 AR-1248-2	5.916	5.106	478642	510043	8.175	8.704
23) L5 AR-1248-3	6.117	5.148	420489	580358	6.444	9.586 #
24) L5 AR-1248-4	6.515	5.319	840011	666528	9.875	9.519
25) L5 AR-1248-5	6.555	5.711	847395	492724	10.125	6.937 #
26) L6 AR-1254-1	6.490	5.671	800213	668508	9.507	6.097 #
27) L6 AR-1254-2	6.713	5.817	1216623	215745	9.702	2.282 #
28) L6 AR-1254-3	7.075	6.221	972945	235203	7.415	1.594 #
29) L6 AR-1254-4	7.352	6.457	290290	334040	2.423	3.440 #
30) L6 AR-1254-5	7.759	6.882	204740	26792	1.792	0.206 #
31) L7 AR-1260-1	7.194f	6.368	290821	193307	3.297	2.041 #
32) L7 AR-1260-2	7.501	6.521	615313	437219	4.528	3.755
33) L7 AR-1260-3	7.845	6.693	311322	209922	2.727	2.015 #
34) L7 AR-1260-4	8.024f	7.165	394932	51351	3.833	0.585 #
35) L7 AR-1260-5	8.386	7.416	132977	126609	0.553	0.593
36) L8 AR-1262-1	8.024f	6.896	394932	60051	2.668	0.416 #
37) L8 AR-1262-2	8.386	7.165	132977	51351	0.420	0.420
38) L8 AR-1262-3	8.769f	7.693	1272327	124222	5.946	1.102 #
39) L8 AR-1262-4	8.795	7.750	369898	30272	2.347	0.165 #
40) L8 AR-1262-5	9.419	8.252	498442	31936	4.456	0.369 #
41) L9 AR-1268-1	0.000	7.693	0	124222	N.D.	0.432 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
Data File : PP073088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 17:21
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1232 MDL 25 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:27:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.795	7.750	369898	30272	1.213	0.118 #
43) L9	AR-1268-3	9.026	7.952	1125409	258881	4.239	1.199 #
44) L9	AR-1268-4	9.419	8.252	498442	31936	4.259	0.339 #
45) L9	AR-1268-5	9.831	8.544	-113242	266172	N.D.	0.460 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

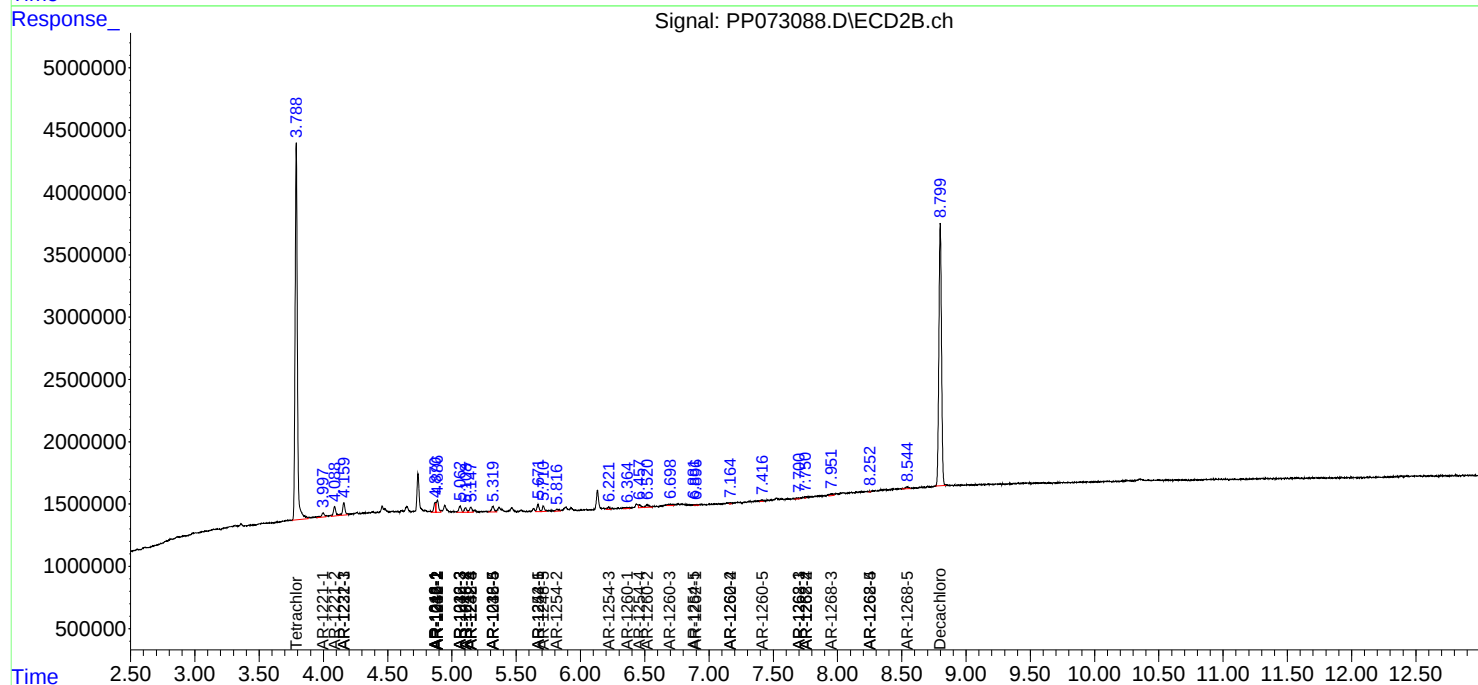


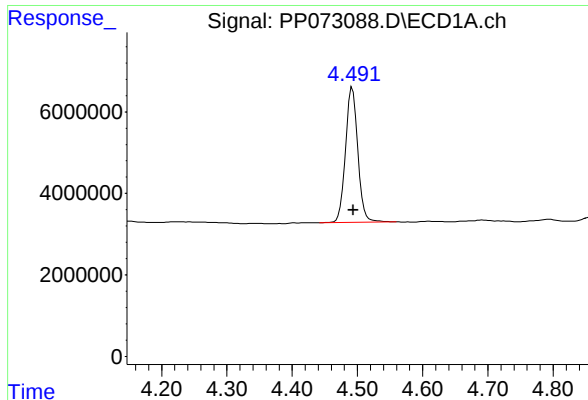

#1 Tetrachloro-m-xylene


R.T.: 4.492 min
Delta R.T.: -0.002 min
Response: 43371716
Conc: 20.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

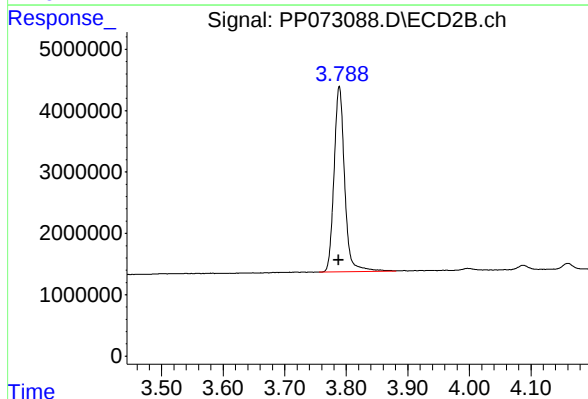


#1 Tetrachloro-m-xylene

R.T.: 3.789 min
Delta R.T.: 0.001 min
Response: 36267481
Conc: 20.13 ng/ml

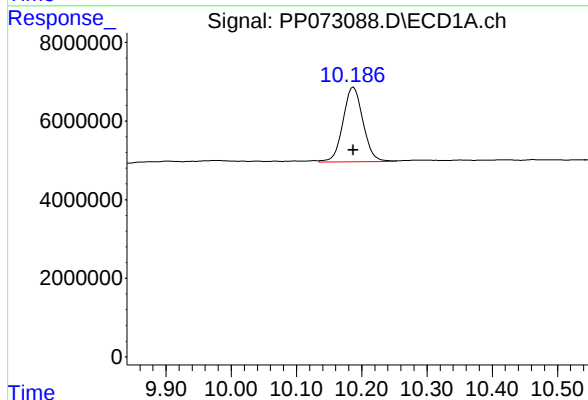


#2 Decachlorobiphenyl

R.T.: 10.188 min
Delta R.T.: 0.000 min
Response: 40707412
Conc: 23.82 ng/ml

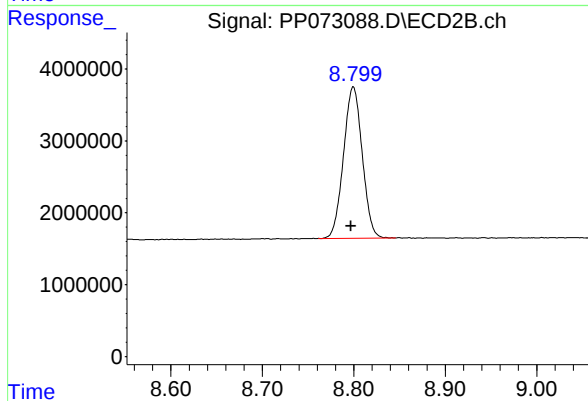

#2 Decachlorobiphenyl


R.T.: 8.799 min
Delta R.T.: 0.002 min
Response: 29954096
Conc: 22.44 ng/ml

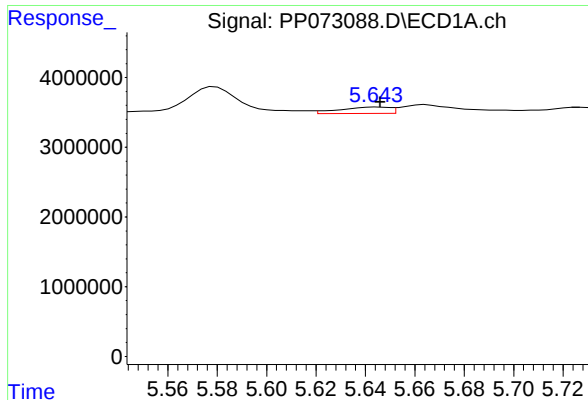

#3 AR-1016-1


R.T.: 5.644 min
Delta R.T.: -0.002 min
Response: 1285923
Conc: 17.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

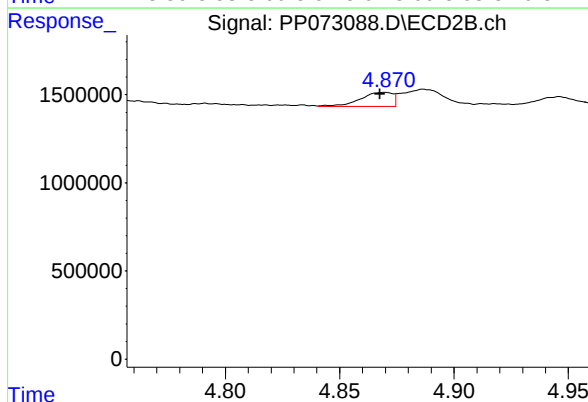


#3 AR-1016-1

R.T.: 4.869 min
Delta R.T.: 0.002 min
Response: 776866
Conc: 11.31 ng/ml

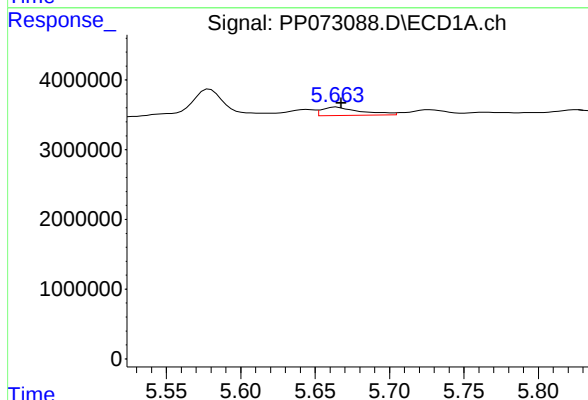


#4 AR-1016-2

R.T.: 5.665 min
Delta R.T.: -0.003 min
Response: 2113265
Conc: 20.32 ng/ml

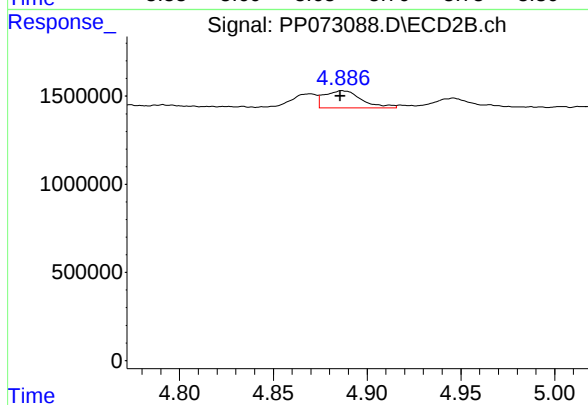

#4 AR-1016-2


R.T.: 4.887 min
Delta R.T.: 0.001 min
Response: 1338273
Conc: 13.30 ng/ml

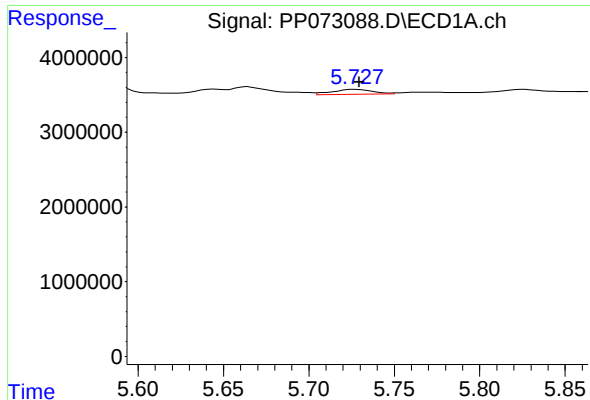

#5 AR-1016-3


R.T.: 5.728 min
Delta R.T.: -0.002 min
Response: 1104800
Conc: 16.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

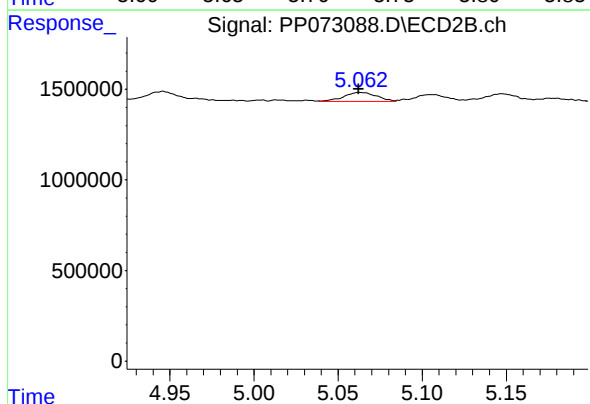


#5 AR-1016-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 667040
Conc: 12.19 ng/ml

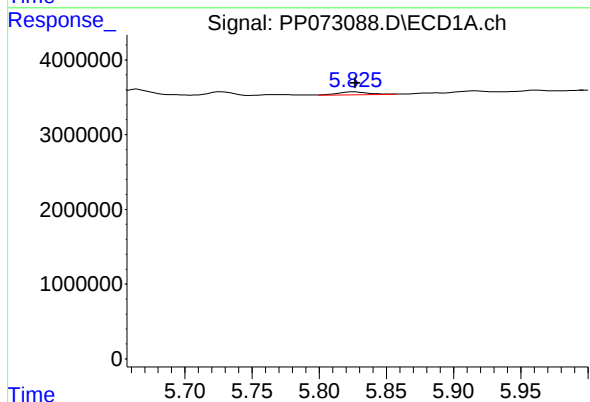


#6 AR-1016-4

R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 645129
Conc: 12.34 ng/ml

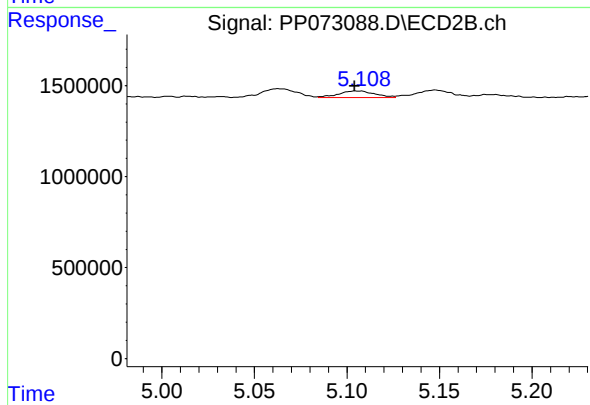

#6 AR-1016-4


R.T.: 5.106 min
Delta R.T.: 0.001 min
Response: 510043
Conc: 11.45 ng/ml

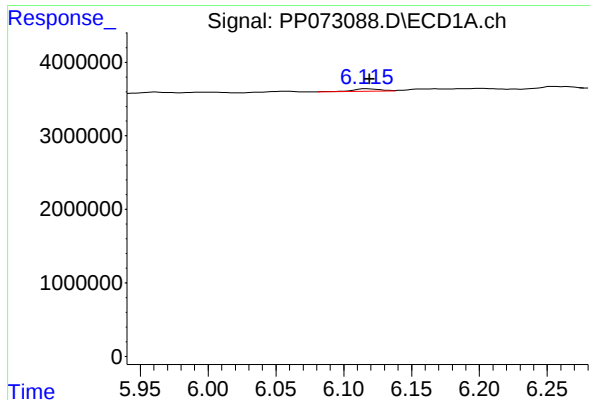

#7 AR-1016-5


R.T.: 6.117 min
Delta R.T.: -0.002 min
Response: 420489
Conc: 8.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

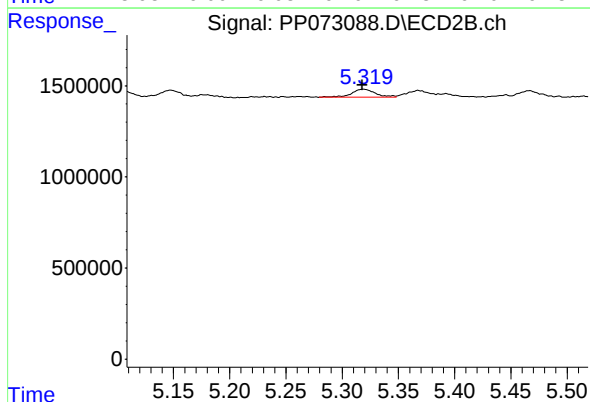


#7 AR-1016-5

R.T.: 5.319 min
Delta R.T.: 0.001 min
Response: 666528
Conc: 12.06 ng/ml

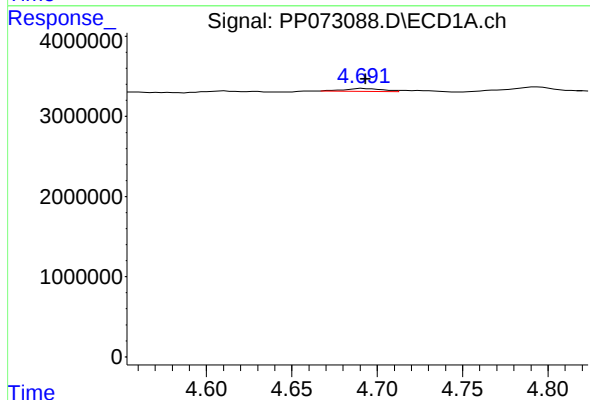


#8 AR-1221-1

R.T.: 4.692 min
Delta R.T.: -0.001 min
Response: 548747
Conc: 22.25 ng/ml

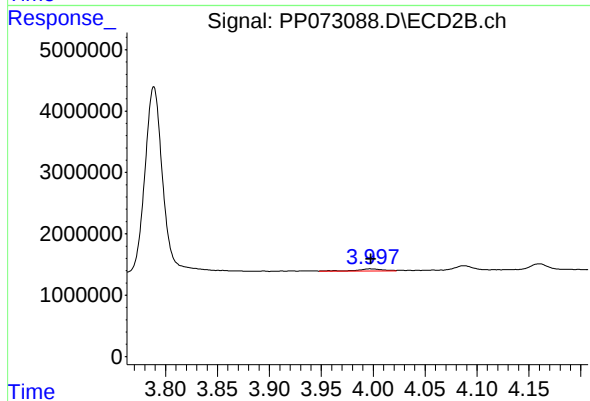

#8 AR-1221-1


R.T.: 3.998 min
Delta R.T.: 0.000 min
Response: 605096
Conc: 22.52 ng/ml

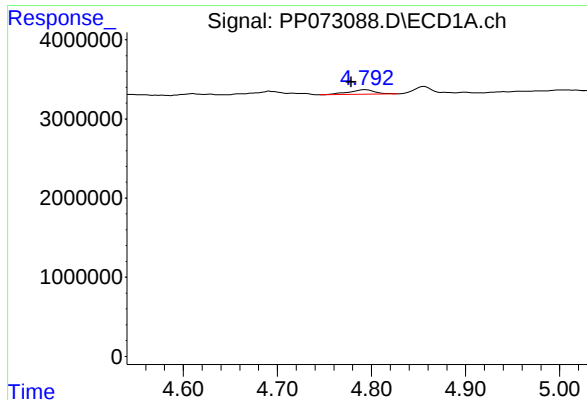

#9 AR-1221-2


R.T.: 4.794 min
Delta R.T.: 0.015 min
Response: 1109774
Conc: 55.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

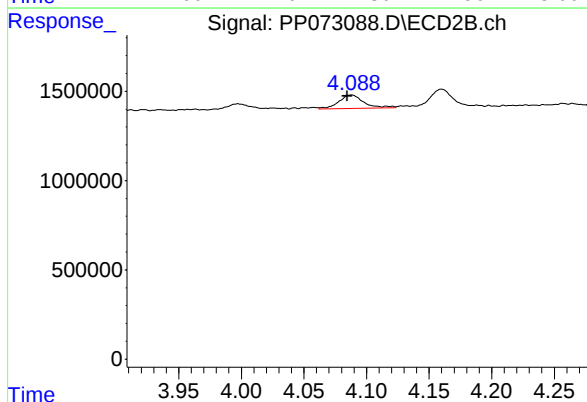


#9 AR-1221-2

R.T.: 4.088 min
Delta R.T.: 0.003 min
Response: 1055376
Conc: 52.28 ng/ml

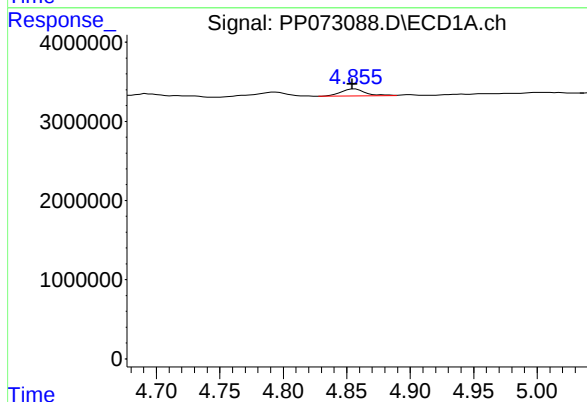


#10 AR-1221-3

R.T.: 4.856 min
Delta R.T.: 0.002 min
Response: 1232784
Conc: 20.03 ng/ml

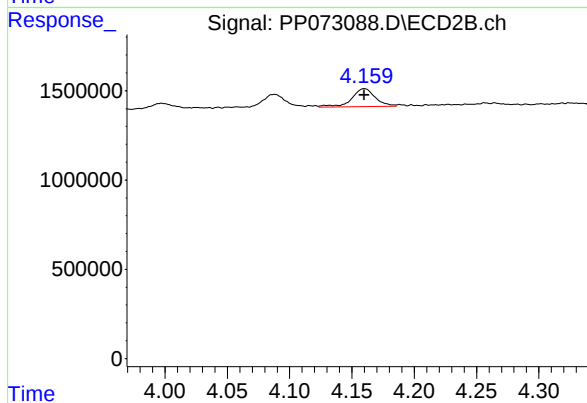

#10 AR-1221-3


R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 1324610
Conc: 22.55 ng/ml

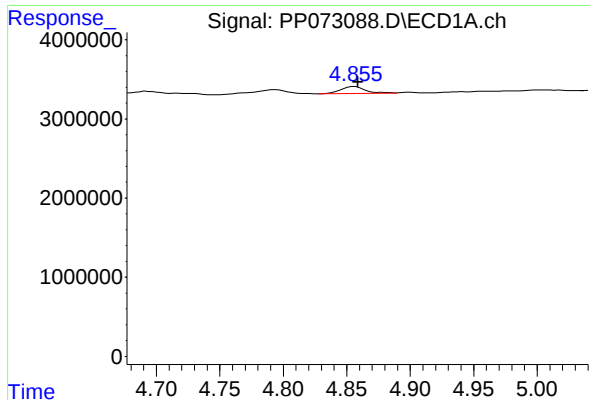

#11 AR-1232-1


R.T.: 4.856 min
Delta R.T.: -0.003 min
Response: 1232784
Conc: 26.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

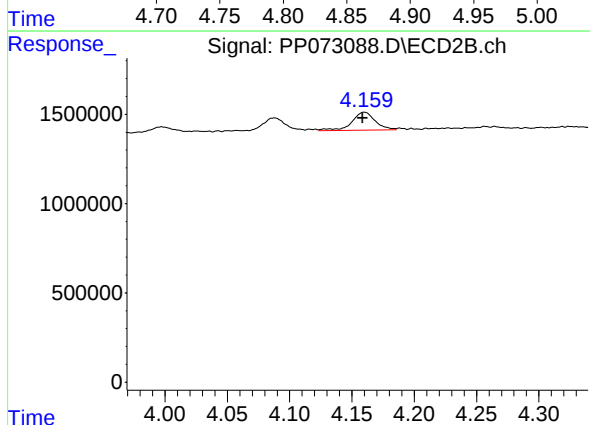


#11 AR-1232-1

R.T.: 4.160 min
Delta R.T.: 0.001 min
Response: 1324610
Conc: 29.07 ng/ml

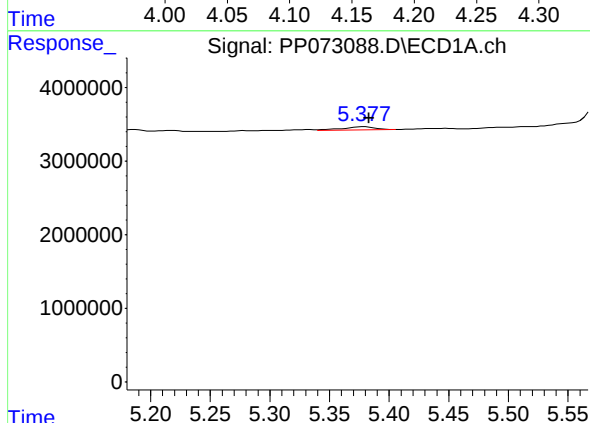


#12 AR-1232-2

R.T.: 5.379 min
Delta R.T.: -0.004 min
Response: 822830
Conc: 36.78 ng/ml

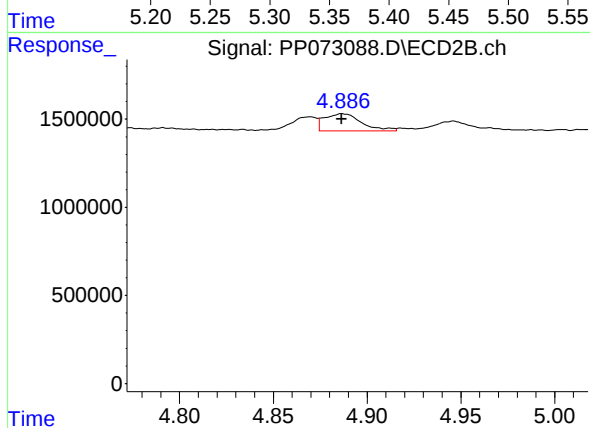

#12 AR-1232-2


R.T.: 4.887 min
Delta R.T.: 0.000 min
Response: 1338273
Conc: 28.93 ng/ml

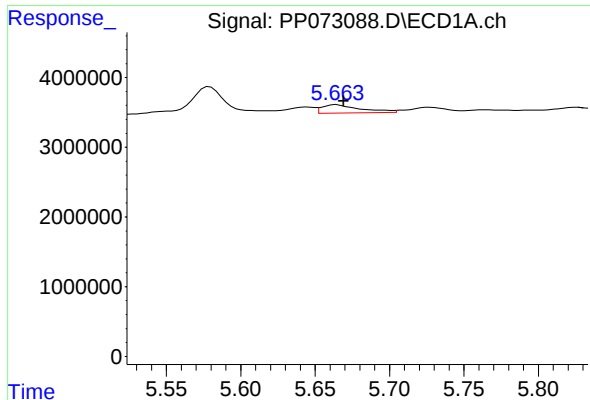

#13 AR-1232-3


R.T.: 5.665 min
Delta R.T.: -0.005 min
Response: 2113265
Conc: 40.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

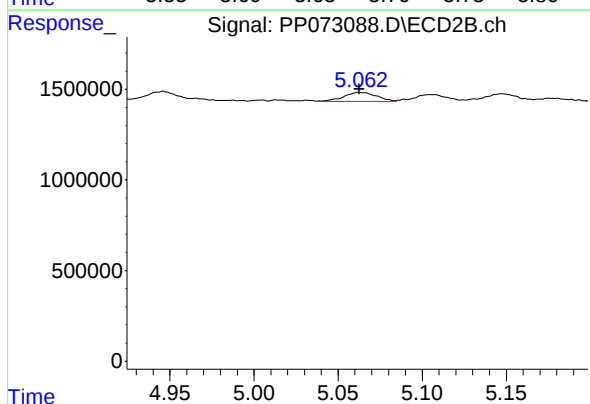


#13 AR-1232-3

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 667040
Conc: 27.16 ng/ml

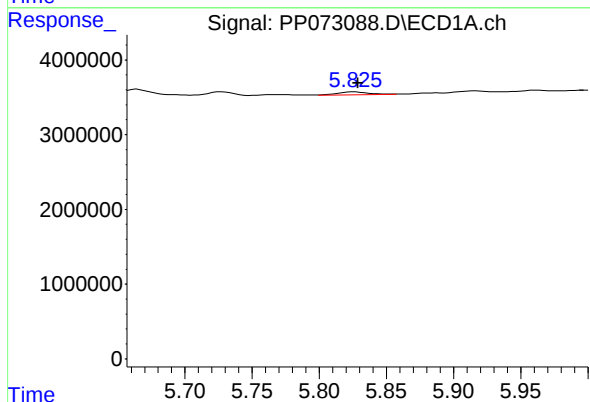


#14 AR-1232-4

R.T.: 5.826 min
Delta R.T.: -0.003 min
Response: 645129
Conc: 24.99 ng/ml

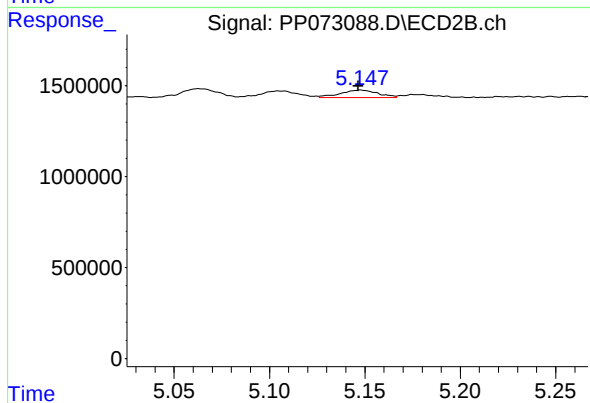

#14 AR-1232-4


R.T.: 5.148 min
Delta R.T.: 0.000 min
Response: 580358
Conc: 26.84 ng/ml

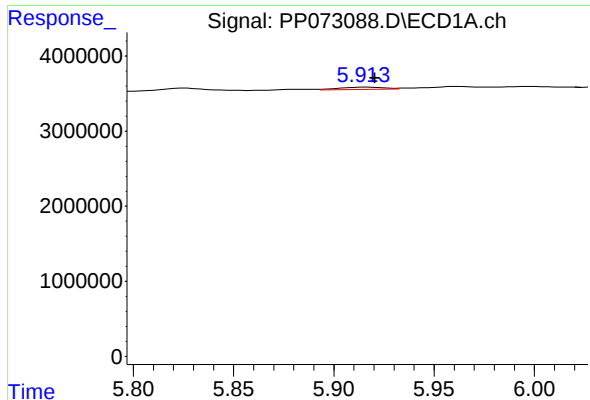

#15 AR-1232-5


R.T.: 5.916 min
Delta R.T.: -0.005 min
Response: 478642
Conc: 13.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

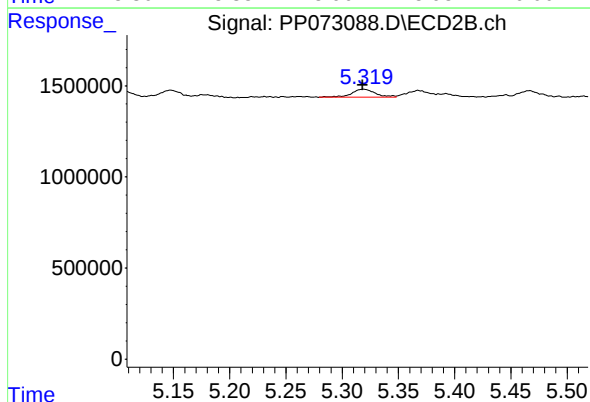


#15 AR-1232-5

R.T.: 5.319 min
Delta R.T.: 0.000 min
Response: 666528
Conc: 29.16 ng/ml

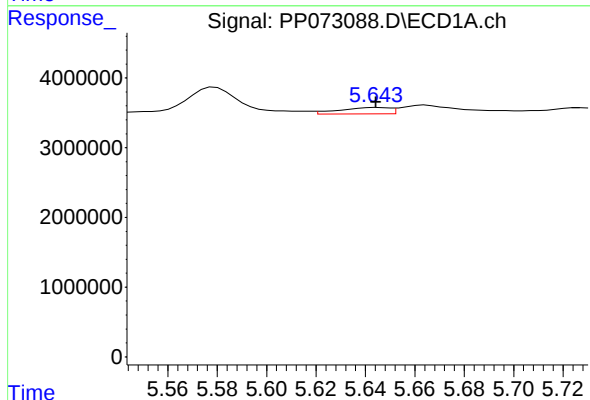


#16 AR-1242-1

R.T.: 5.644 min
Delta R.T.: 0.000 min
Response: 1285923
Conc: 22.01 ng/ml

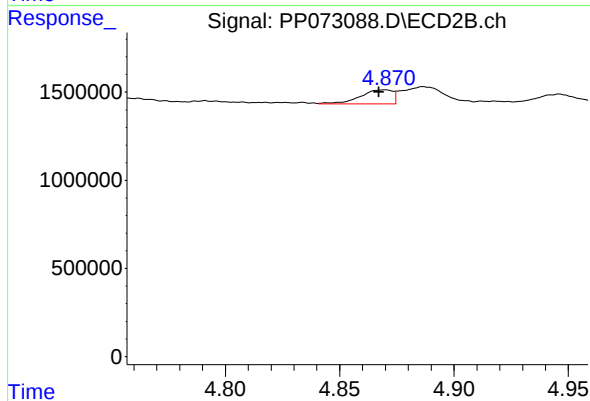

#16 AR-1242-1


R.T.: 4.869 min
Delta R.T.: 0.002 min
Response: 776866
Conc: 14.07 ng/ml

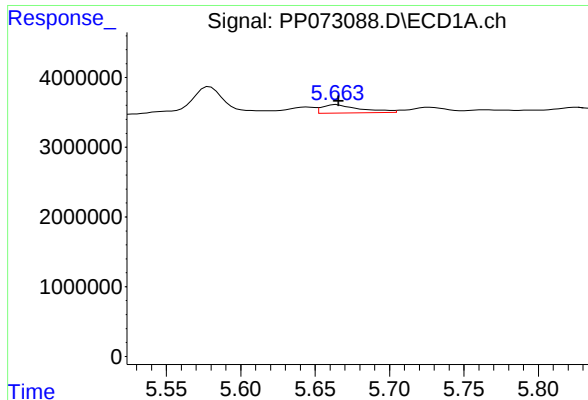

#17 AR-1242-2


R.T.: 5.665 min
Delta R.T.: -0.001 min
Response: 2113265
Conc: 24.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

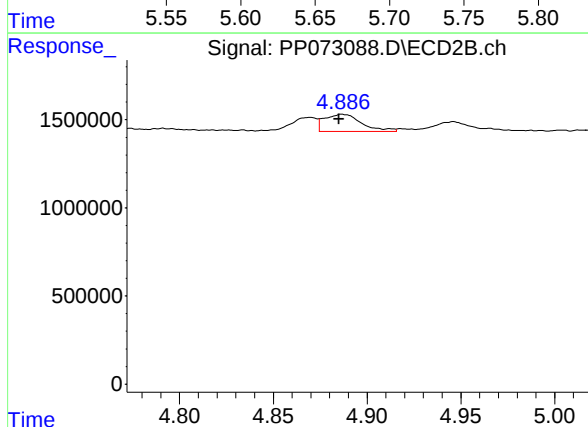


#17 AR-1242-2

R.T.: 4.887 min
Delta R.T.: 0.002 min
Response: 1338273
Conc: 16.84 ng/ml

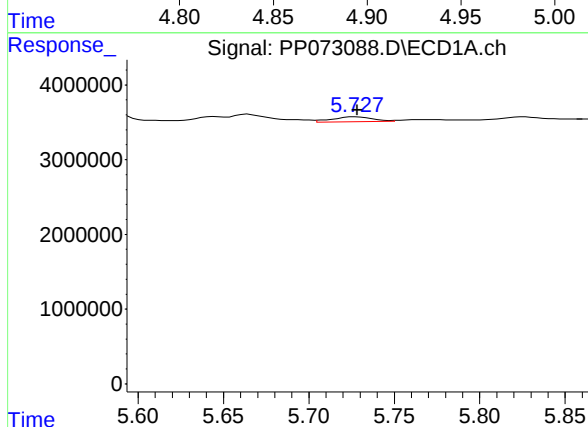


#18 AR-1242-3

R.T.: 5.728 min
Delta R.T.: 0.000 min
Response: 1104800
Conc: 20.96 ng/ml

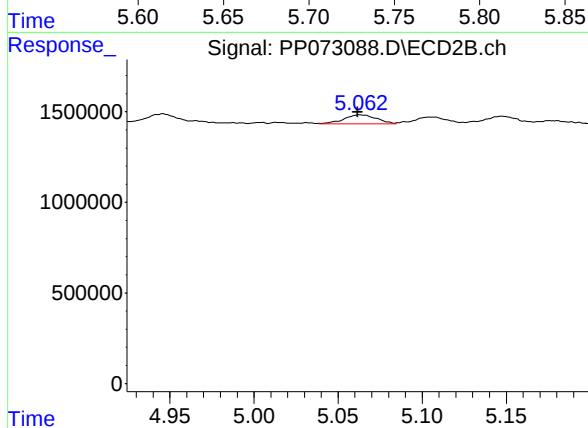

#18 AR-1242-3


R.T.: 5.063 min
Delta R.T.: 0.002 min
Response: 667040
Conc: 15.40 ng/ml

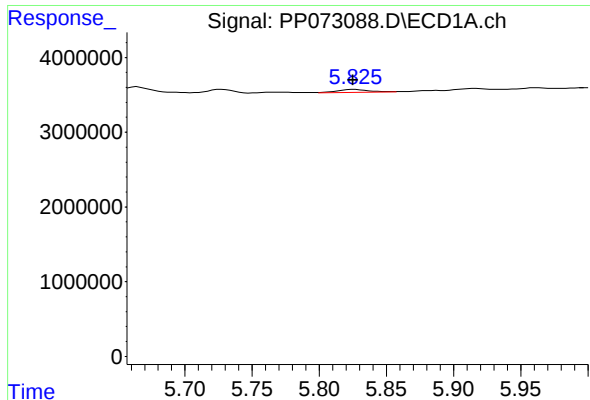

#19 AR-1242-4


R.T.: 5.826 min
Delta R.T.: 0.001 min
Response: 645129
Conc: 14.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

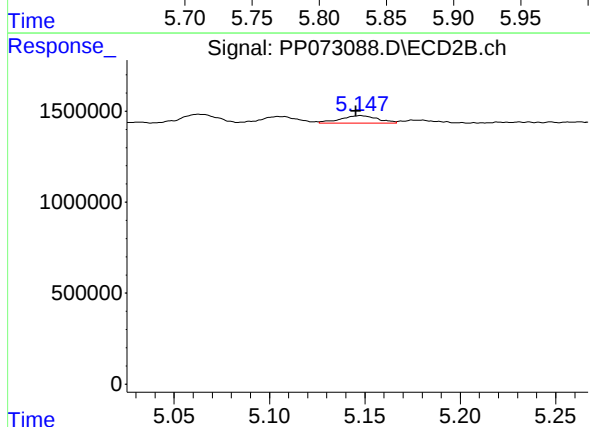


#19 AR-1242-4

R.T.: 5.148 min
Delta R.T.: 0.002 min
Response: 580358
Conc: 13.98 ng/ml

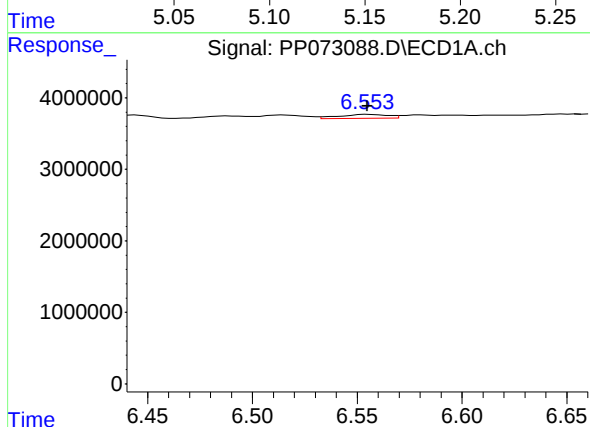


#20 AR-1242-5

R.T.: 6.555 min
Delta R.T.: 0.000 min
Response: 847395
Conc: 17.10 ng/ml

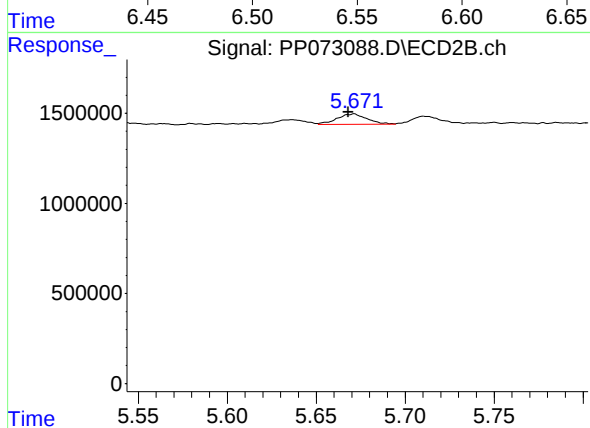

#20 AR-1242-5


R.T.: 5.671 min
Delta R.T.: 0.003 min
Response: 668508
Conc: 12.71 ng/ml

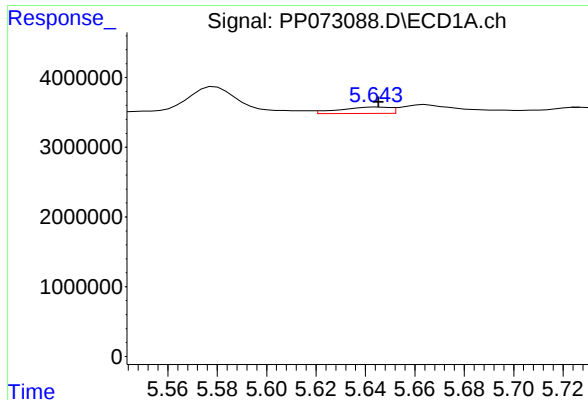

#21 AR-1248-1


R.T.: 5.644 min
Delta R.T.: 0.000 min
Response: 1285923
Conc: 27.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

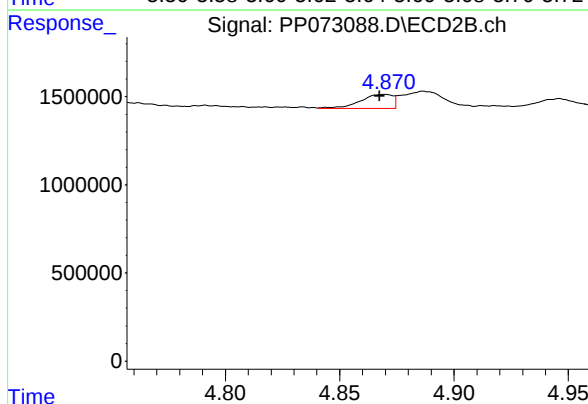


#21 AR-1248-1

R.T.: 4.869 min
Delta R.T.: 0.002 min
Response: 776866
Conc: 17.82 ng/ml

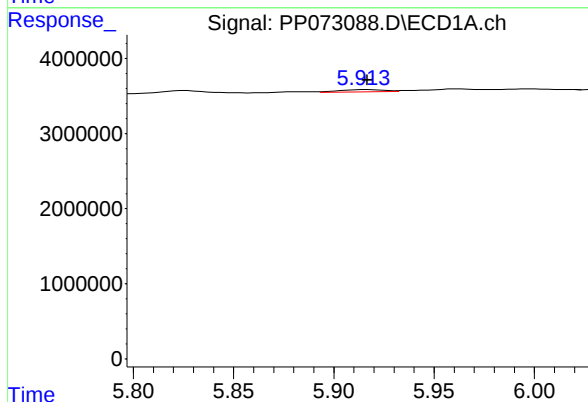


#22 AR-1248-2

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 478642
Conc: 8.17 ng/ml

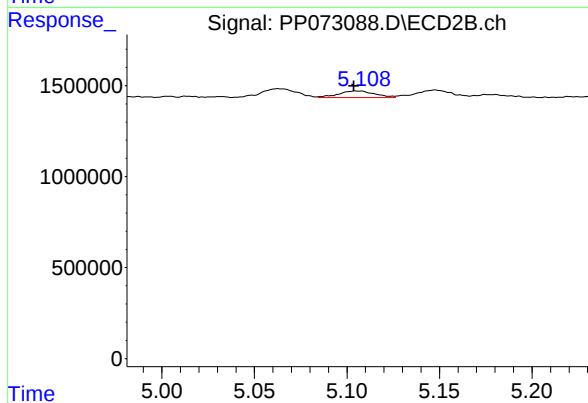

#22 AR-1248-2


R.T.: 5.106 min
Delta R.T.: 0.002 min
Response: 510043
Conc: 8.70 ng/ml

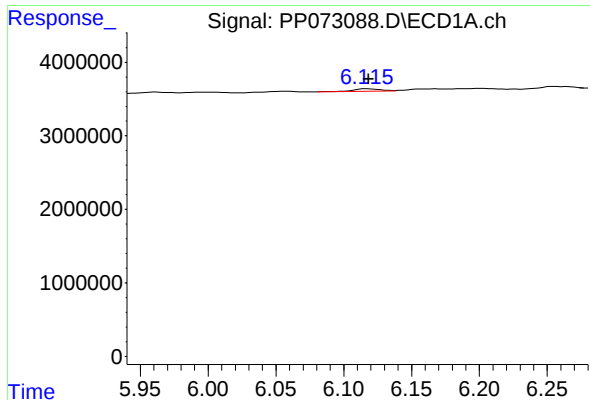

#23 AR-1248-3


R.T.: 6.117 min
Delta R.T.: -0.002 min
Response: 420489
Conc: 6.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

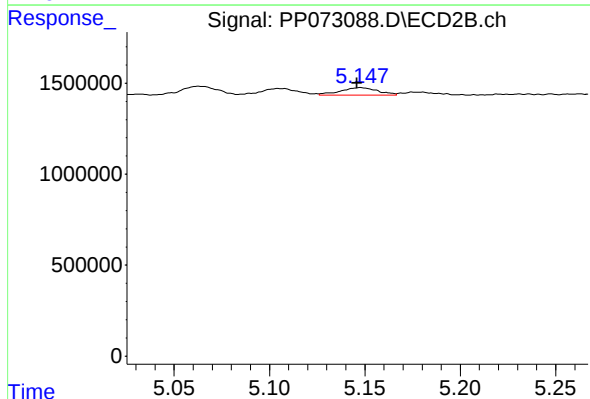


#23 AR-1248-3

R.T.: 5.148 min
Delta R.T.: 0.002 min
Response: 580358
Conc: 9.59 ng/ml

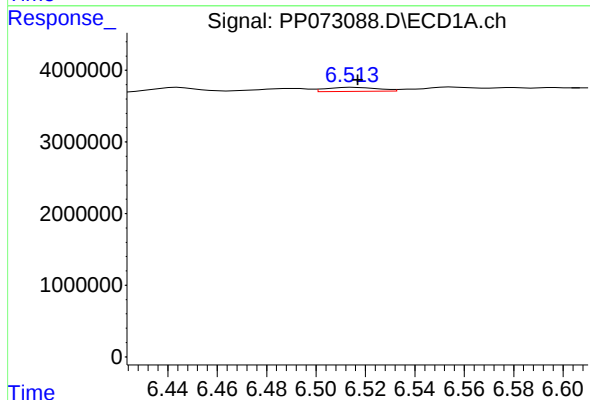


#24 AR-1248-4

R.T.: 6.515 min
Delta R.T.: -0.002 min
Response: 840011
Conc: 9.87 ng/ml

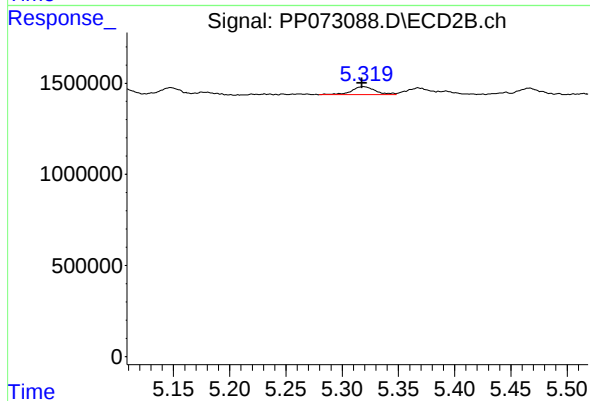

#24 AR-1248-4


R.T.: 5.319 min
Delta R.T.: 0.002 min
Response: 666528
Conc: 9.52 ng/ml

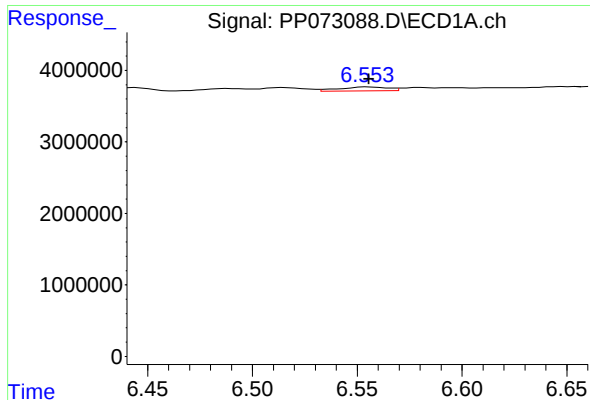

#25 AR-1248-5


R.T.: 6.555 min
Delta R.T.: 0.000 min
Response: 847395
Conc: 10.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

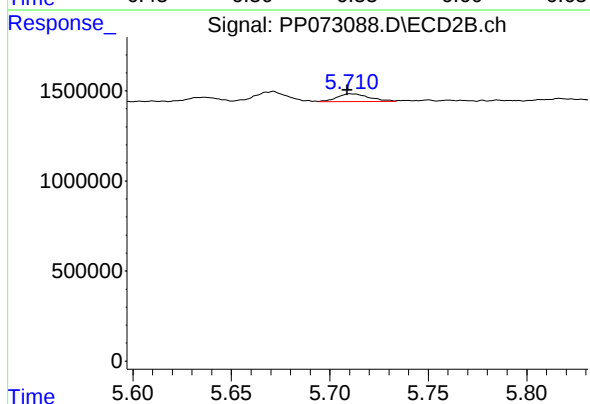


#25 AR-1248-5

R.T.: 5.711 min
Delta R.T.: 0.002 min
Response: 492724
Conc: 6.94 ng/ml

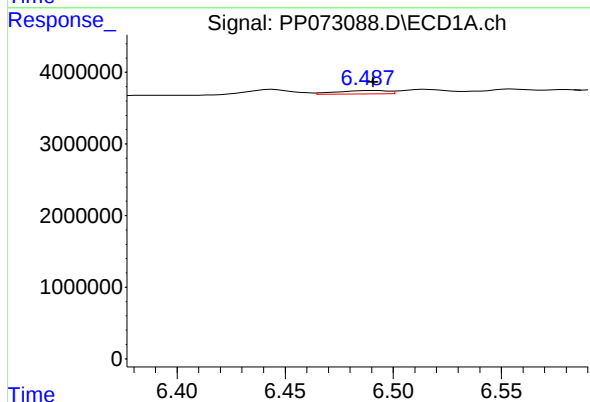


#26 AR-1254-1

R.T.: 6.490 min
Delta R.T.: 0.000 min
Response: 800213
Conc: 9.51 ng/ml

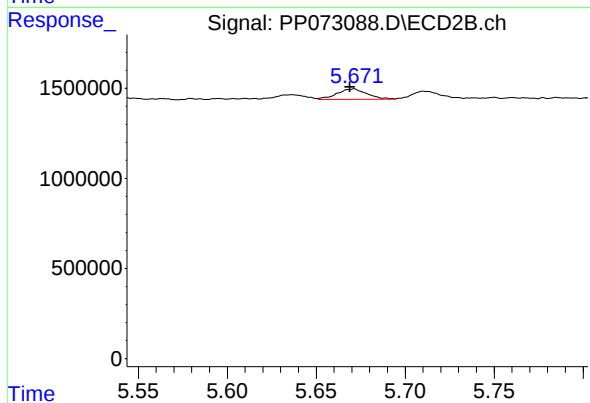

#26 AR-1254-1


R.T.: 5.671 min
Delta R.T.: 0.002 min
Response: 668508
Conc: 6.10 ng/ml

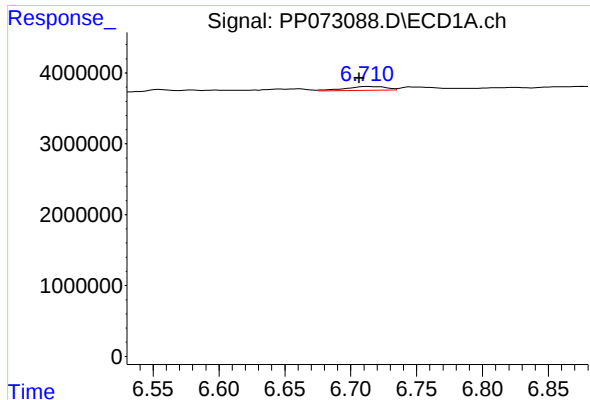

#27 AR-1254-2


R.T.: 6.713 min
Delta R.T.: 0.006 min
Response: 1216623
Conc: 9.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

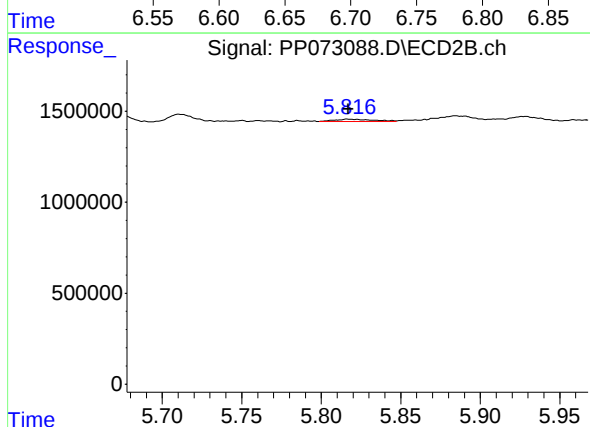


#27 AR-1254-2

R.T.: 5.817 min
Delta R.T.: 0.000 min
Response: 215745
Conc: 2.28 ng/ml

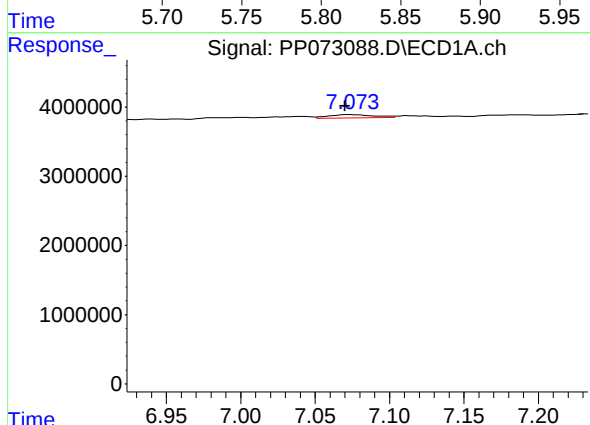


#28 AR-1254-3

R.T.: 7.075 min
Delta R.T.: 0.005 min
Response: 972945
Conc: 7.42 ng/ml

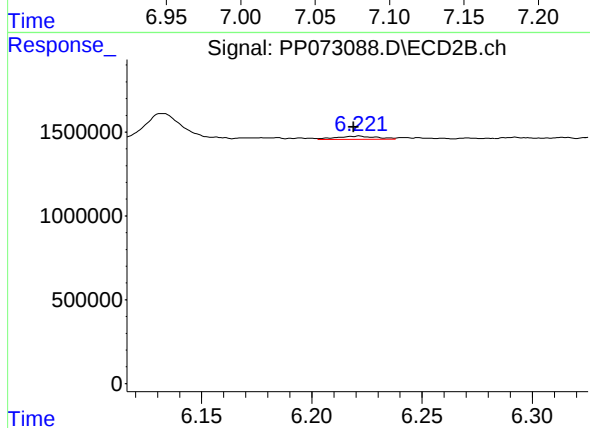

#28 AR-1254-3


R.T.: 6.221 min
Delta R.T.: 0.002 min
Response: 235203
Conc: 1.59 ng/ml

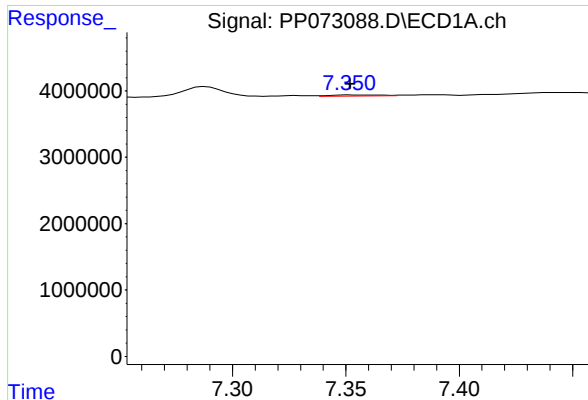

#29 AR-1254-4


R.T.: 7.352 min
Delta R.T.: 0.000 min
Response: 290290
Conc: 2.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

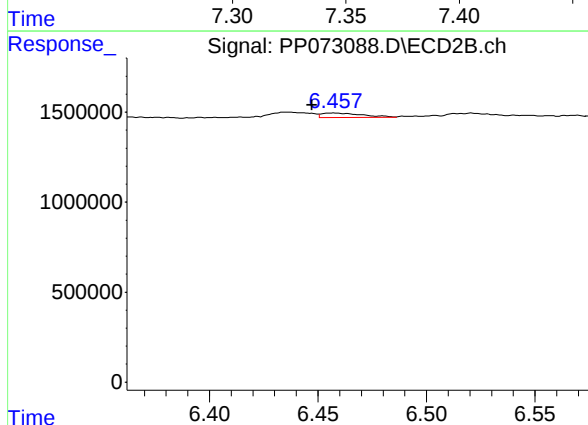


#29 AR-1254-4

R.T.: 6.457 min
Delta R.T.: 0.010 min
Response: 334040
Conc: 3.44 ng/ml

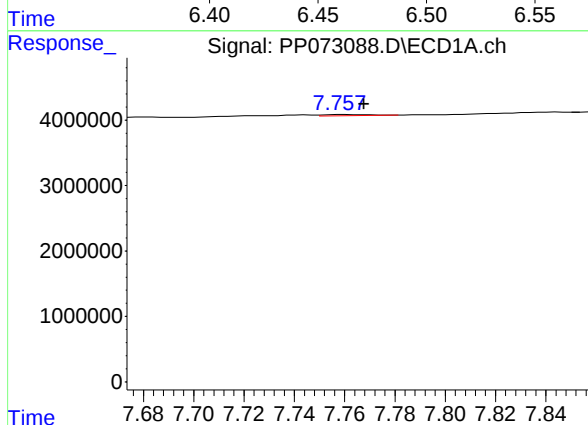


#30 AR-1254-5

R.T.: 7.759 min
Delta R.T.: -0.008 min
Response: 204740
Conc: 1.79 ng/ml

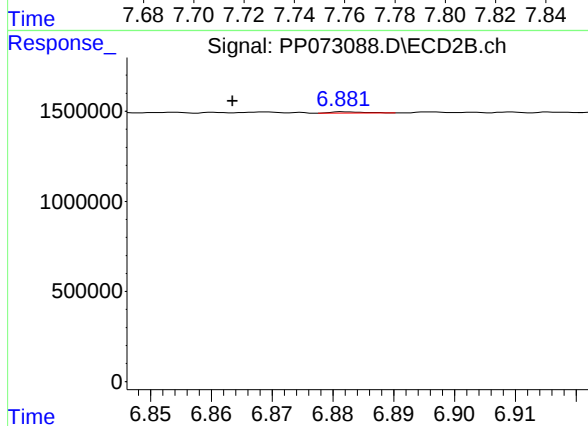

#30 AR-1254-5


R.T.: 6.882 min
Delta R.T.: 0.019 min
Response: 26792
Conc: 0.21 ng/ml

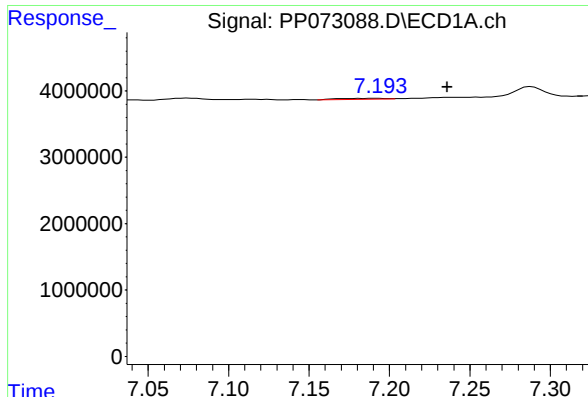

#31 AR-1260-1


R.T.: 7.194 min
Delta R.T.: -0.042 min
Response: 290821
Conc: 3.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

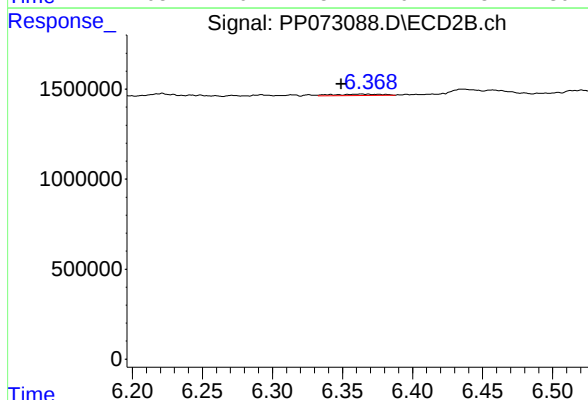


#31 AR-1260-1

R.T.: 6.368 min
Delta R.T.: 0.019 min
Response: 193307
Conc: 2.04 ng/ml

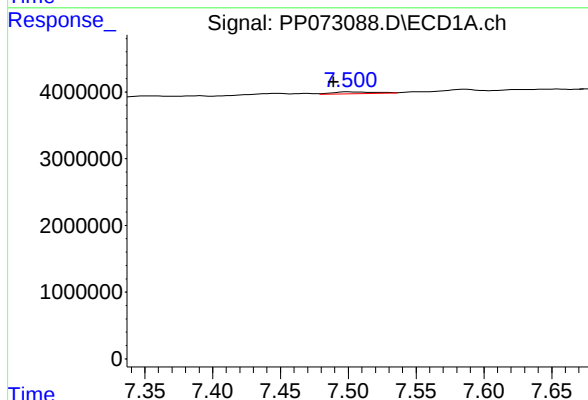


#32 AR-1260-2

R.T.: 7.501 min
Delta R.T.: 0.012 min
Response: 615313
Conc: 4.53 ng/ml

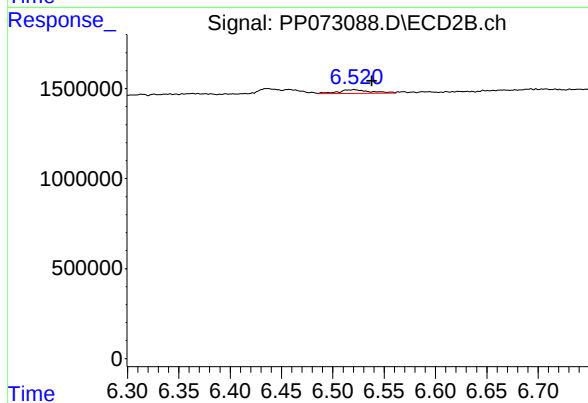

#32 AR-1260-2


R.T.: 6.521 min
Delta R.T.: -0.017 min
Response: 437219
Conc: 3.76 ng/ml

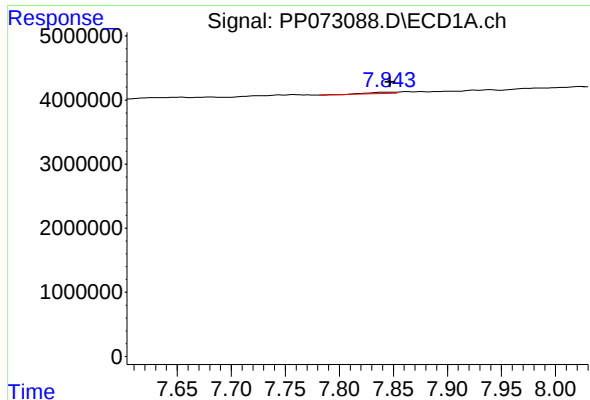

#33 AR-1260-3


R.T.: 7.845 min
Delta R.T.: -0.002 min
Response: 311322
Conc: 2.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

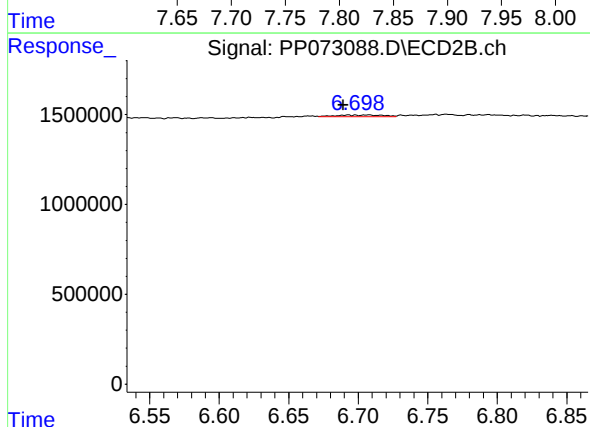


#33 AR-1260-3

R.T.: 6.693 min
Delta R.T.: 0.003 min
Response: 209922
Conc: 2.02 ng/ml

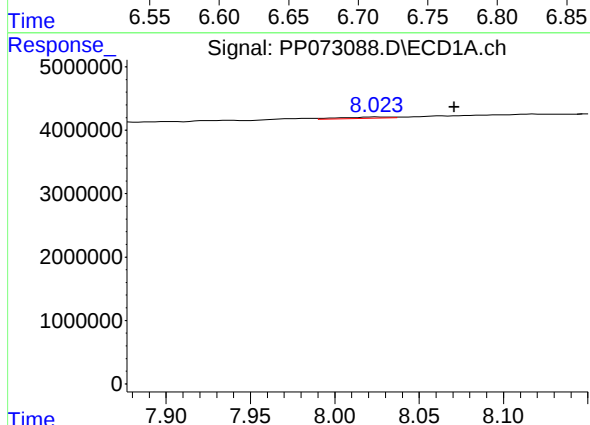


#34 AR-1260-4

R.T.: 8.024 min
Delta R.T.: -0.047 min
Response: 394932
Conc: 3.83 ng/ml

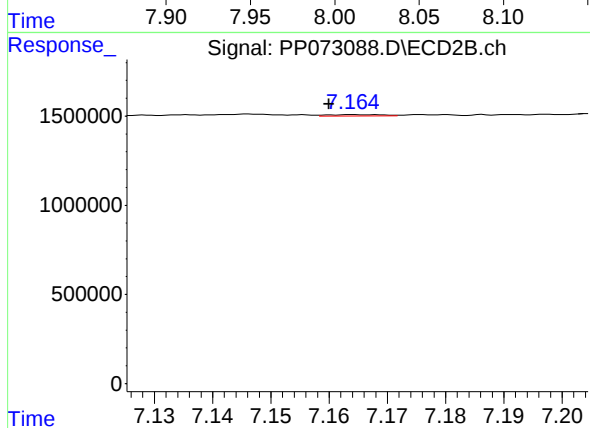

#34 AR-1260-4


R.T.: 7.165 min
Delta R.T.: 0.005 min
Response: 51351
Conc: 0.59 ng/ml

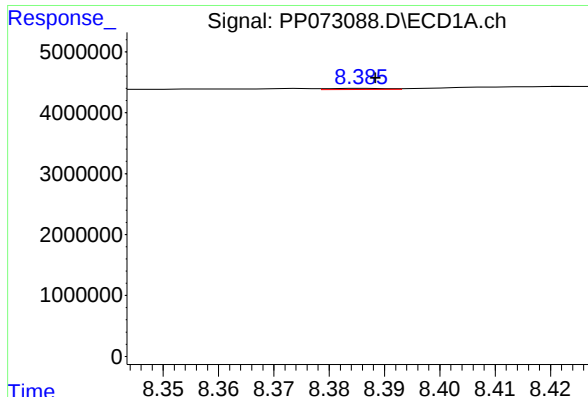

#35 AR-1260-5


R.T.: 8.386 min
Delta R.T.: -0.002 min
Response: 132977
Conc: 0.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

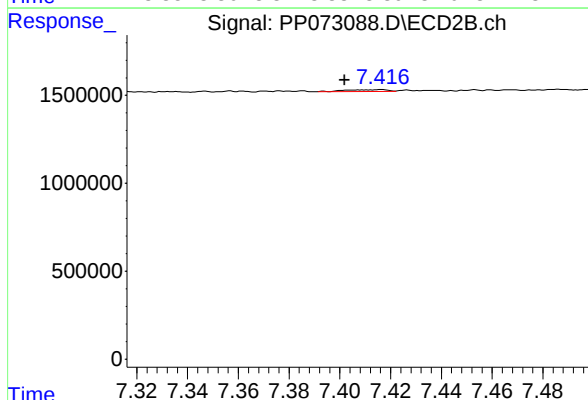


#35 AR-1260-5

R.T.: 7.416 min
Delta R.T.: 0.014 min
Response: 126609
Conc: 0.59 ng/ml

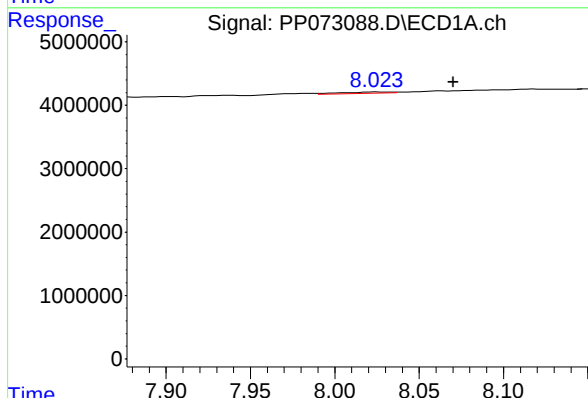


#36 AR-1262-1

R.T.: 8.024 min
Delta R.T.: -0.046 min
Response: 394932
Conc: 2.67 ng/ml

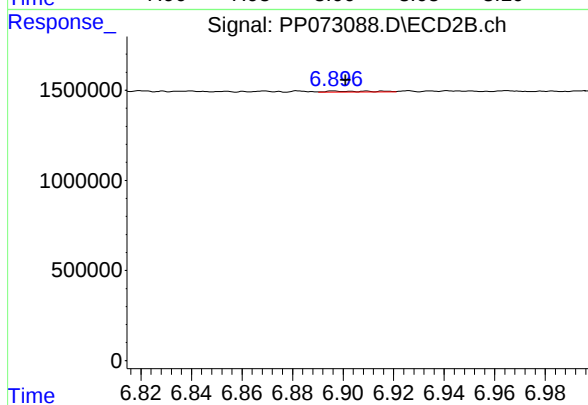

#36 AR-1262-1


R.T.: 6.896 min
Delta R.T.: -0.005 min
Response: 60051
Conc: 0.42 ng/ml

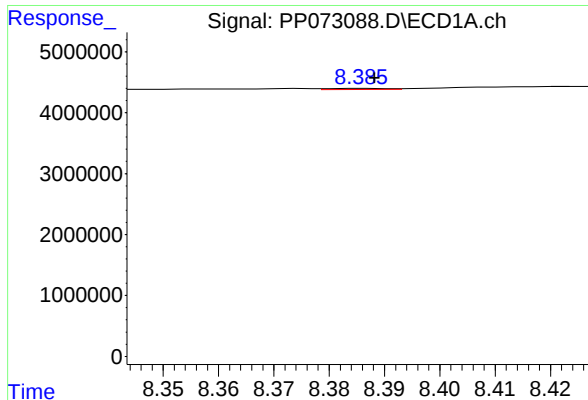

#37 AR-1262-2


R.T.: 8.386 min
Delta R.T.: -0.002 min
Response: 132977
Conc: 0.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

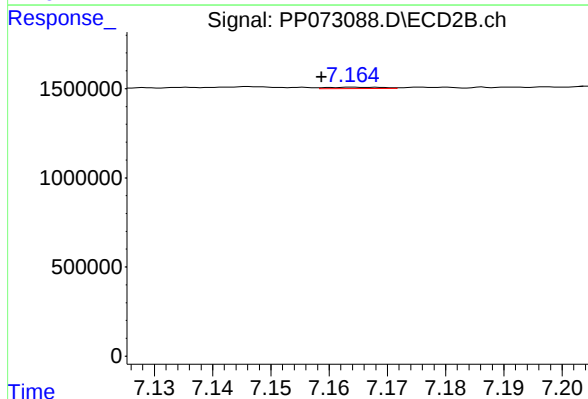


#37 AR-1262-2

R.T.: 7.165 min
Delta R.T.: 0.006 min
Response: 51351
Conc: 0.42 ng/ml

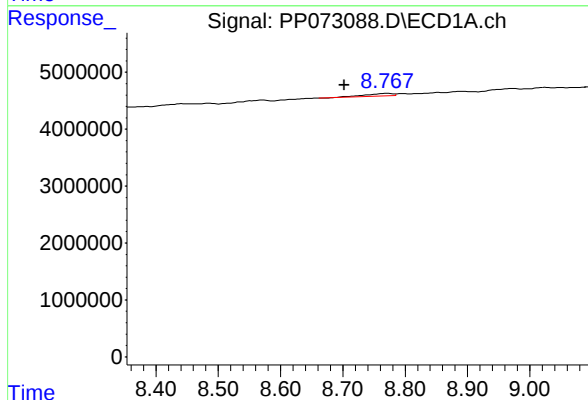


#38 AR-1262-3

R.T.: 8.769 min
Delta R.T.: 0.067 min
Response: 1272327
Conc: 5.95 ng/ml

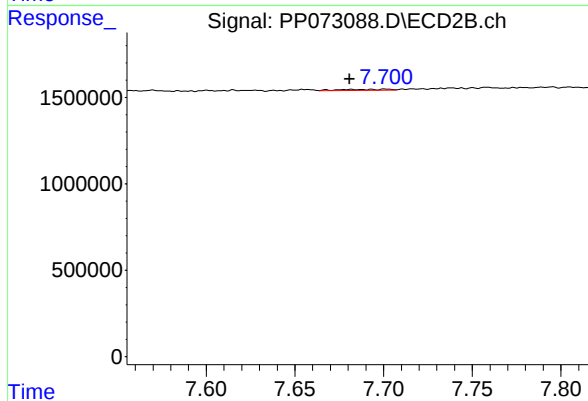

#38 AR-1262-3


R.T.: 7.693 min
Delta R.T.: 0.012 min
Response: 124222
Conc: 1.10 ng/ml

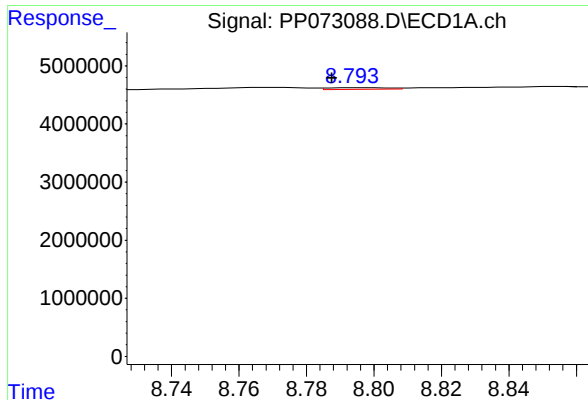

#39 AR-1262-4


R.T.: 8.795 min
Delta R.T.: 0.007 min
Response: 369898
Conc: 2.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

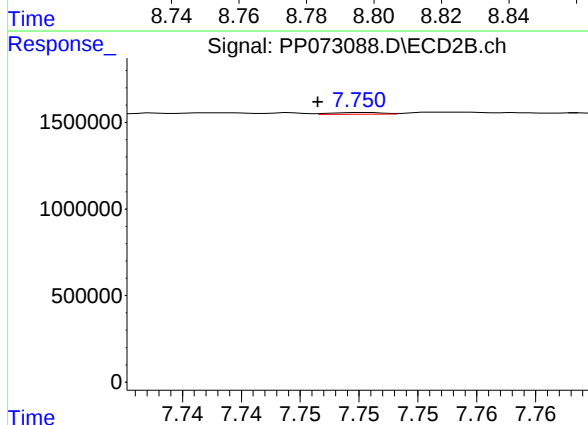


#39 AR-1262-4

R.T.: 7.750 min
Delta R.T.: 0.004 min
Response: 30272
Conc: 0.17 ng/ml

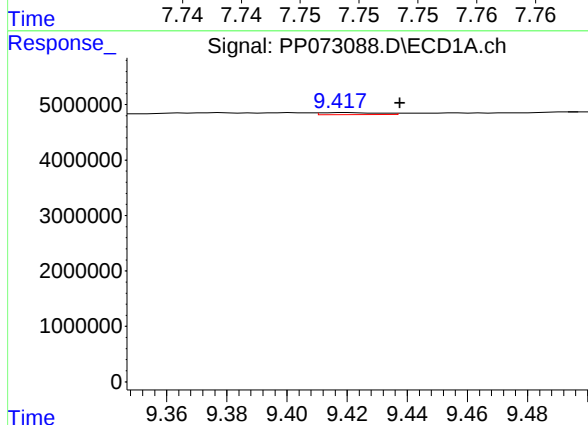


#40 AR-1262-5

R.T.: 9.419 min
Delta R.T.: -0.018 min
Response: 498442
Conc: 4.46 ng/ml

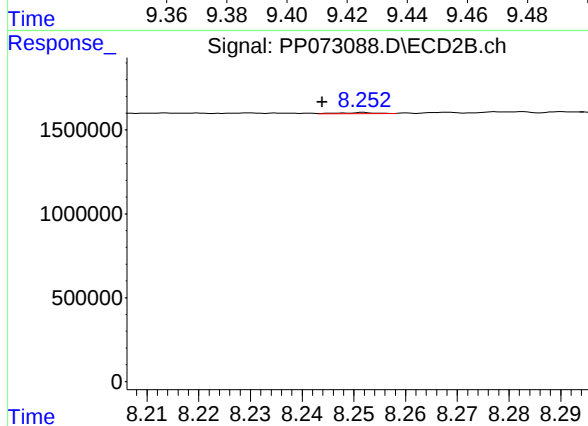

#40 AR-1262-5


R.T.: 8.252 min
Delta R.T.: 0.008 min
Response: 31936
Conc: 0.37 ng/ml

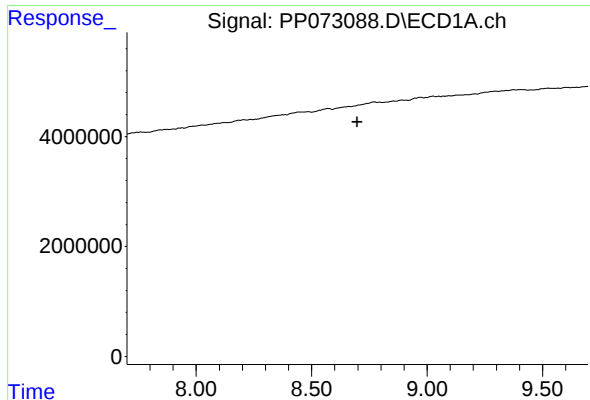

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.698 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

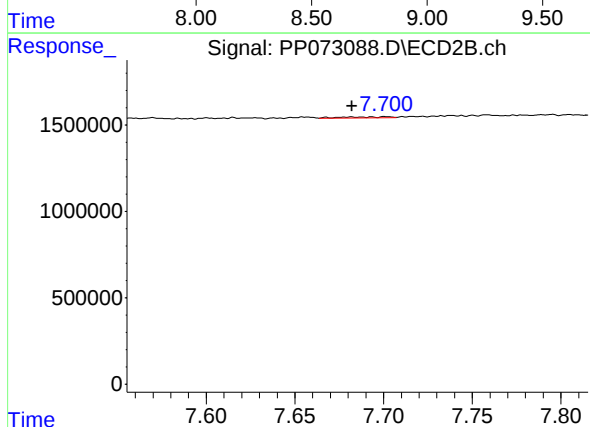


#41 AR-1268-1

R.T.: 7.693 min
Delta R.T.: 0.011 min
Response: 124222
Conc: 0.43 ng/ml

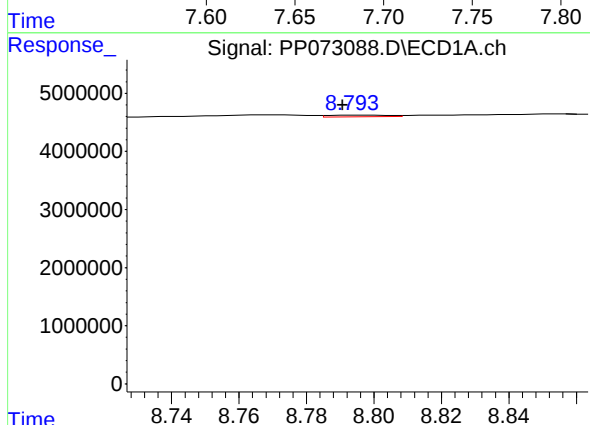


#42 AR-1268-2

R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 369898
Conc: 1.21 ng/ml

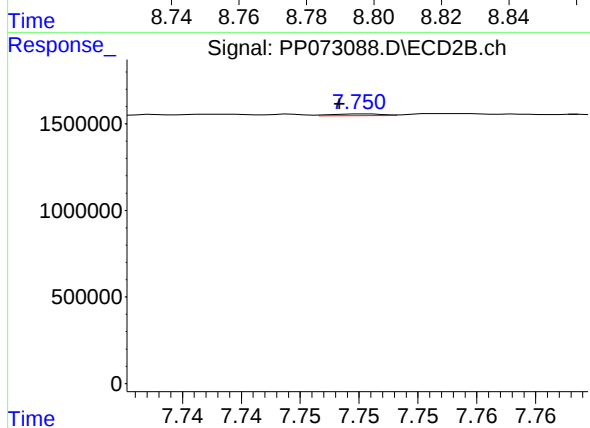

#42 AR-1268-2


R.T.: 7.750 min
Delta R.T.: 0.002 min
Response: 30272
Conc: 0.12 ng/ml

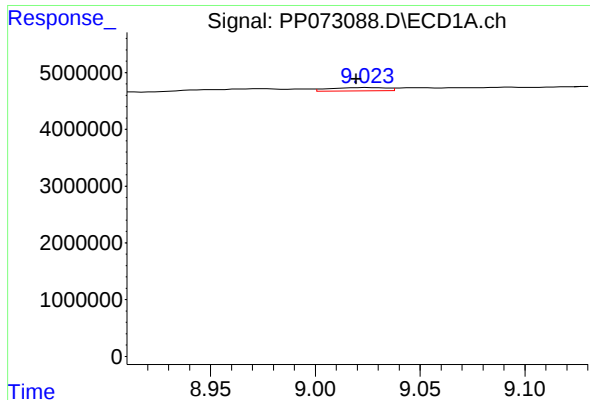

#43 AR-1268-3


R.T.: 9.026 min
Delta R.T.: 0.007 min
Response: 1125409
Conc: 4.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

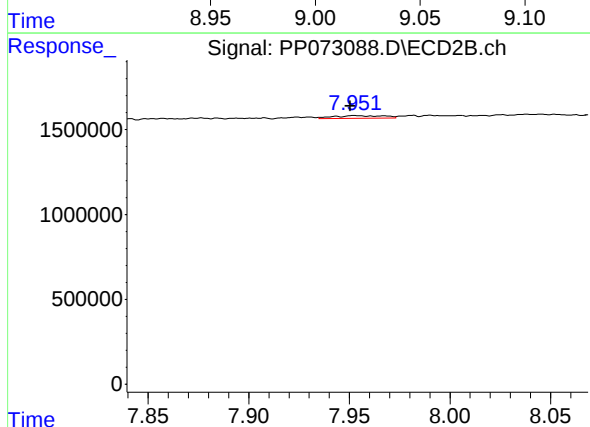


#43 AR-1268-3

R.T.: 7.952 min
Delta R.T.: 0.002 min
Response: 258881
Conc: 1.20 ng/ml

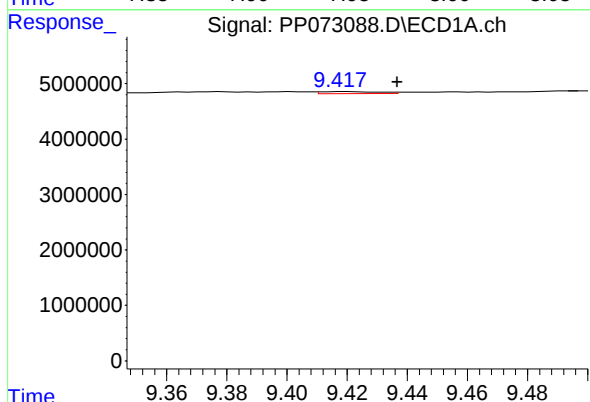


#44 AR-1268-4

R.T.: 9.419 min
Delta R.T.: -0.017 min
Response: 498442
Conc: 4.26 ng/ml

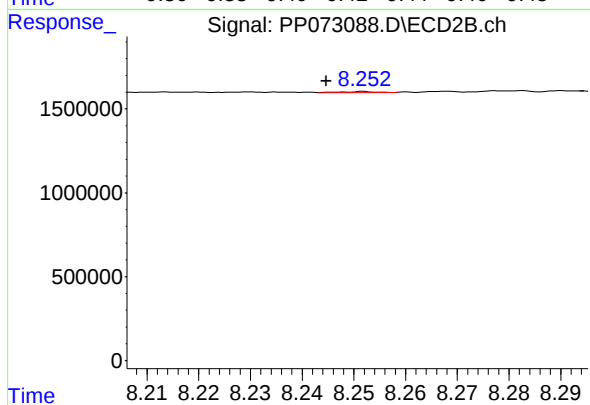

#44 AR-1268-4


R.T.: 8.252 min
Delta R.T.: 0.007 min
Response: 31936
Conc: 0.34 ng/ml

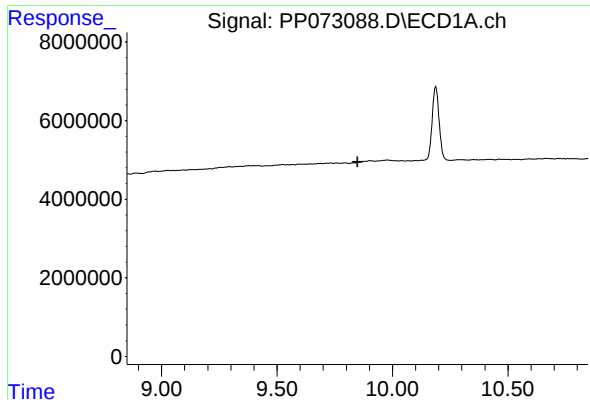

#45 AR-1268-5

R.T.: 9.831 min
Delta R.T.: -0.018 min
Response: -113242
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

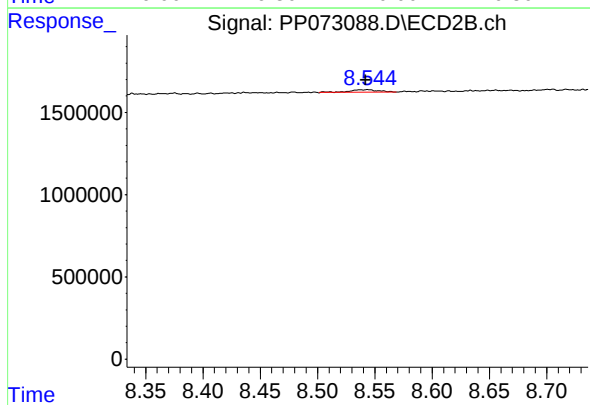

#45 AR-1268-5

R.T.: 8.544 min
Delta R.T.: 0.002 min
Response: 266172
Conc: 0.46 ng/ml