

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 17:38
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:27:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.496	3.790	42620379	36708796	20.192	20.373
2) SA Decachlor...	10.193	8.801	40060520	29875205	23.442	22.383
Target Compounds						
3) L1 AR-1016-1	5.649	4.871	1992138	1665218	27.413	24.233
4) L1 AR-1016-2	5.670	4.889	2728778	2391225	26.233	23.761
5) L1 AR-1016-3	5.732	5.066	1918045	1149437	29.351	21.007 #
6) L1 AR-1016-4	5.830	5.107	1061104	942028	20.296	21.146
7) L1 AR-1016-5	6.122	5.321	1455657	1138406	29.110	20.593 #
8) L2 AR-1221-1	4.698	3.998	603928	286529	24.491	10.663 #
9) L2 AR-1221-2	4.799	4.092	1016996	1244925	50.399	61.674
10) L2 AR-1221-3	4.859	4.161	1024386	1026734	16.643	17.482
11) L3 AR-1232-1	4.859	4.161	1024386	1026734	21.816	22.534
12) L3 AR-1232-2	5.383	4.889	934300	2391225	41.766	51.691
13) L3 AR-1232-3	5.670	5.066	2728778	1149437	52.886	46.805
14) L3 AR-1232-4	5.830	5.148	1061104	1122188	41.111	51.893 #
15) L3 AR-1232-5	5.919	5.321	866179	1138406	24.283	49.801 #
16) L4 AR-1242-1	5.649	4.871	1992138	1665218	34.090	30.157
17) L4 AR-1242-2	5.670	4.889	2728778	2391225	31.527	30.083
18) L4 AR-1242-3	5.732	5.066	1918045	1149437	36.390	26.543 #
19) L4 AR-1242-4	5.830	5.148	1061104	1122188	24.139	27.038
20) L4 AR-1242-5	6.560	5.672	1965817	1325613	39.666	25.208 #
21) L5 AR-1248-1	5.649	4.871	1992138	1665218	41.879	38.201
22) L5 AR-1248-2	5.919	5.107	866179	942028	14.794	16.077
23) L5 AR-1248-3	6.122	5.148	1455657	1122188	22.309	18.535
24) L5 AR-1248-4	6.521	5.321	1869249	1138406	21.974	16.258 #
25) L5 AR-1248-5	6.560	5.714	1965817	1106513	23.488	15.578 #
26) L6 AR-1254-1	6.493	5.672	1706325	1325613	20.271	12.089 #
27) L6 AR-1254-2	6.716	5.821	1588678	577020	12.669	6.103 #
28) L6 AR-1254-3	7.074	6.222	1455814	563438	11.095	3.819 #
29) L6 AR-1254-4	7.357	6.450	714428	542480	5.964	5.587
30) L6 AR-1254-5	7.762	6.867	700314	156018	6.129	1.200 #
31) L7 AR-1260-1	7.245	6.341	405677	177461	4.599	1.873 #
32) L7 AR-1260-2	7.508	6.549	730597	47638	5.377	0.409 #
33) L7 AR-1260-3	7.847	6.701	968091	392857	8.481	3.772 #
34) L7 AR-1260-4	8.082	7.157	193588	211544	1.879	2.411 #
35) L7 AR-1260-5	8.392	7.410	318885	341462	1.325	1.600
36) L8 AR-1262-1	8.082	6.913	193588	77453	1.308	0.536 #
37) L8 AR-1262-2	8.392	7.157	318885	211544	1.008	1.731 #
38) L8 AR-1262-3	8.717	7.667	73148	61448	0.342	0.545 #
39) L8 AR-1262-4	8.772	7.753	1052907	219214	6.681	1.196 #
40) L8 AR-1262-5	9.434	8.217	189075	378790	1.690	4.375 #
41) L9 AR-1268-1	8.717	7.667	73148	61448	0.205	0.214

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 17:38
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:27:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.808	7.753	218504	219214	0.716	0.853
43) L9	AR-1268-3	9.027	7.956	1203998	526940	4.535	2.440 #
44) L9	AR-1268-4	9.434	8.217	189075	378790	1.616	4.022 #
45) L9	AR-1268-5	9.856	8.547	611122	205762	0.826	0.355 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
Data File : PP073089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 17:38
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1242 MDL 25 PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:27:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

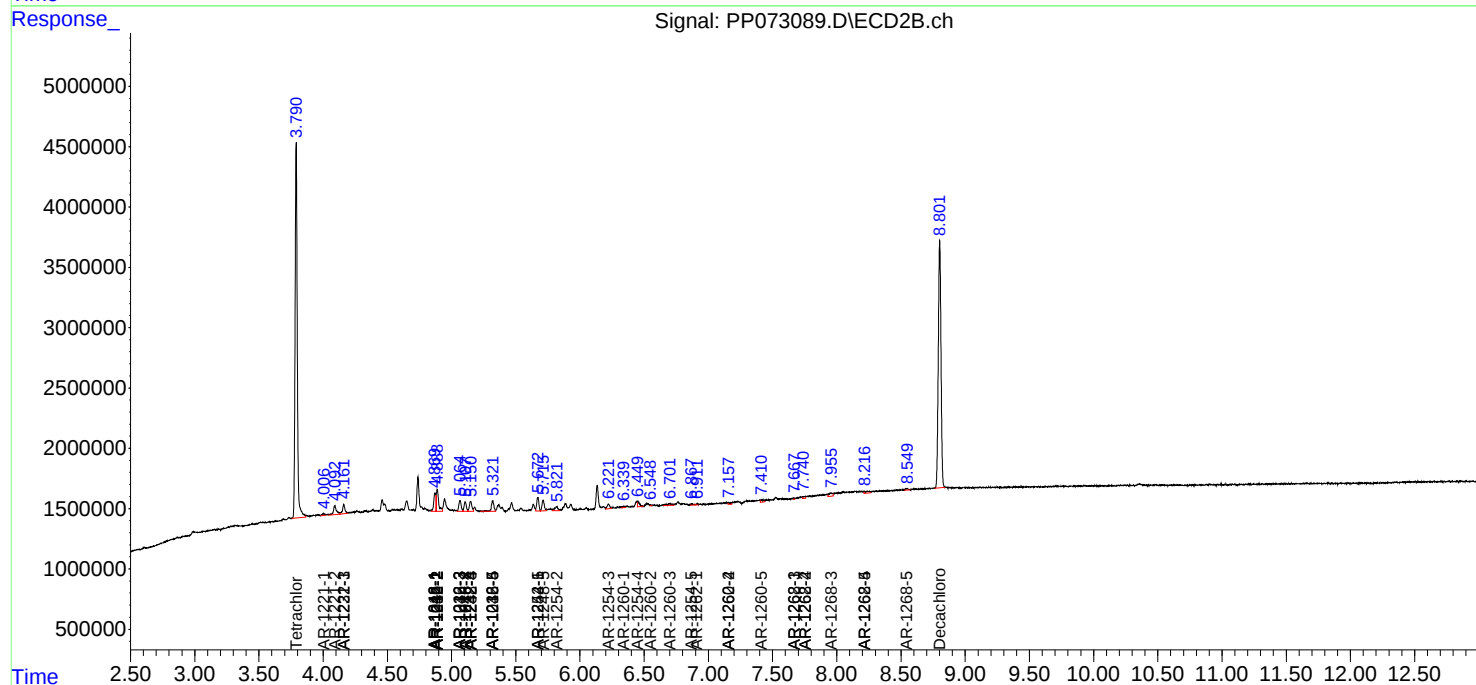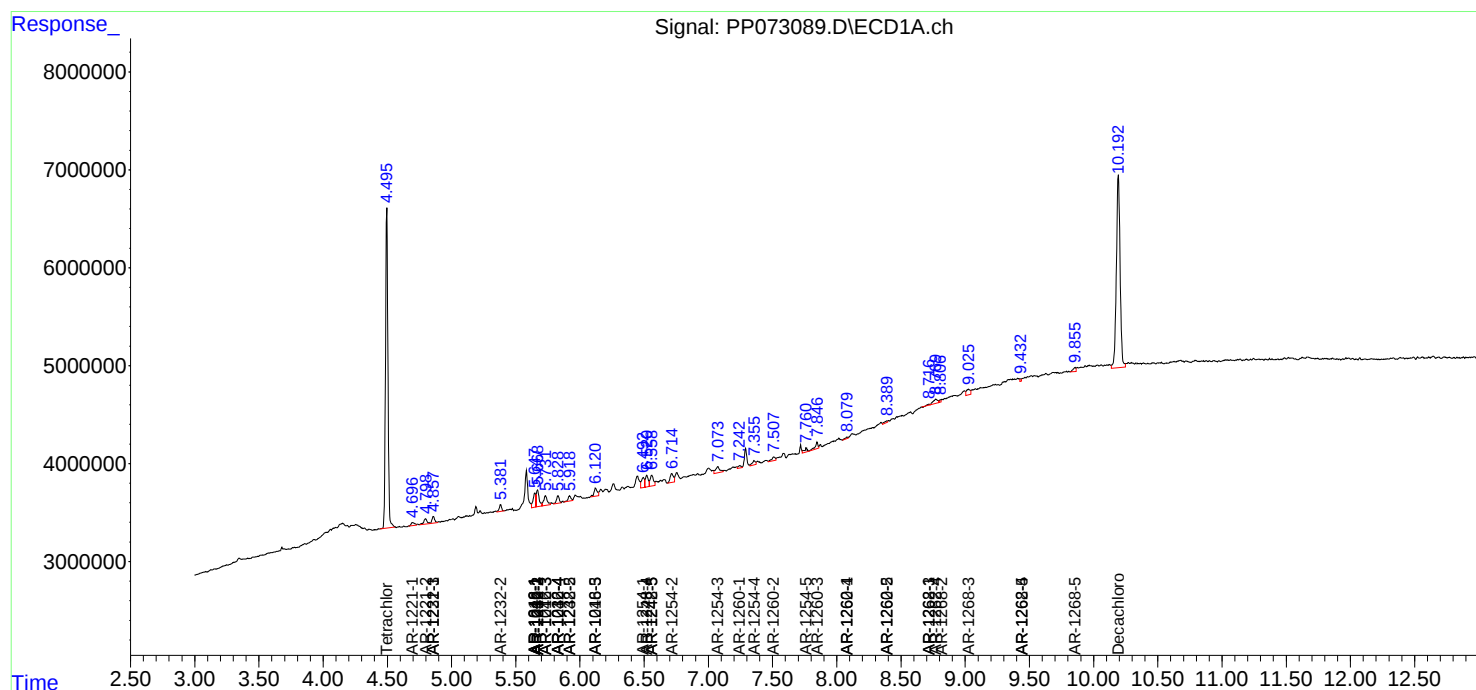


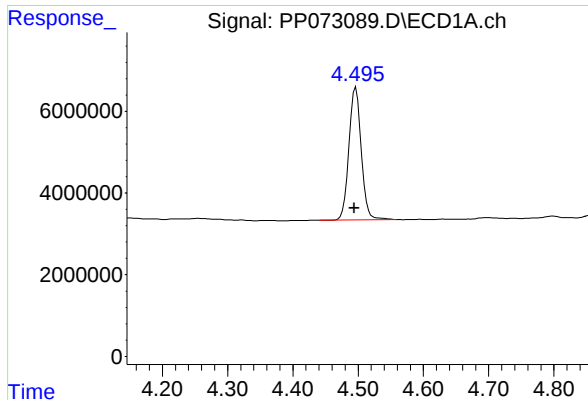

#1 Tetrachloro-m-xylene


R.T.: 4.496 min
Delta R.T.: 0.002 min
Response: 42620379
Conc: 20.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

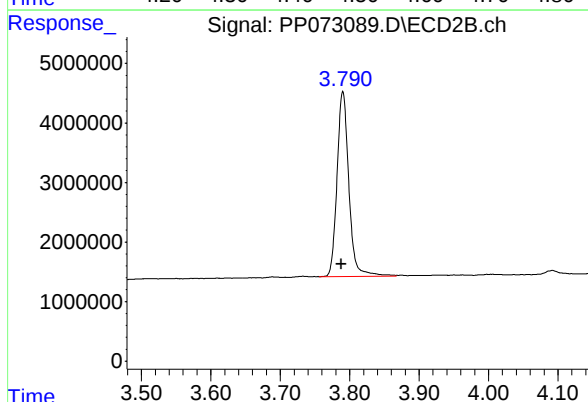


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.003 min
Response: 36708796
Conc: 20.37 ng/ml

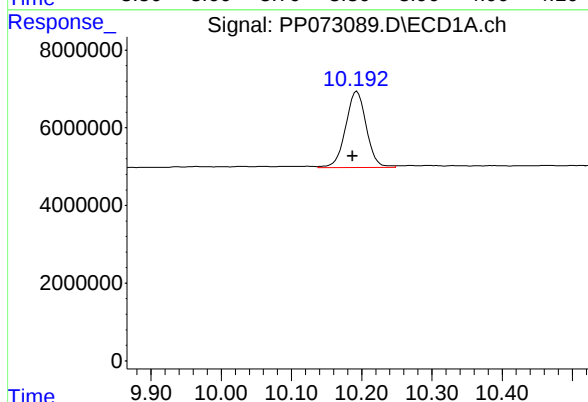


#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: 0.006 min
Response: 40060520
Conc: 23.44 ng/ml

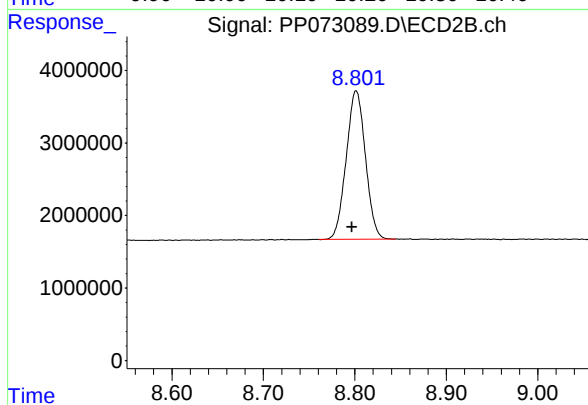

#2 Decachlorobiphenyl


R.T.: 8.801 min
Delta R.T.: 0.004 min
Response: 29875205
Conc: 22.38 ng/ml

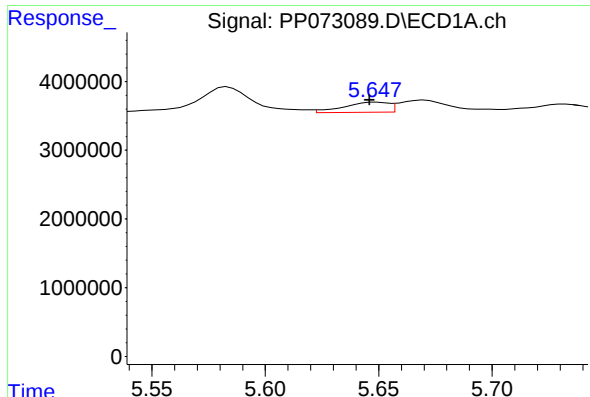

#3 AR-1016-1


R.T.: 5.649 min
Delta R.T.: 0.003 min
Response: 1992138
Conc: 27.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

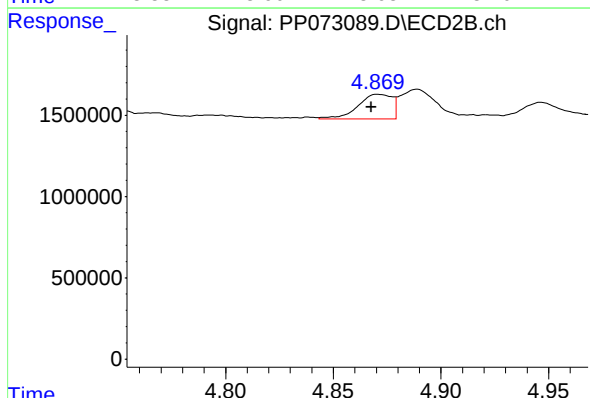


#3 AR-1016-1

R.T.: 4.871 min
Delta R.T.: 0.003 min
Response: 1665218
Conc: 24.23 ng/ml

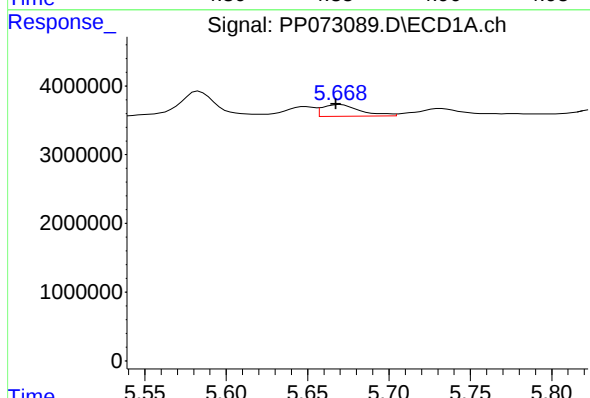


#4 AR-1016-2

R.T.: 5.670 min
Delta R.T.: 0.003 min
Response: 2728778
Conc: 26.23 ng/ml

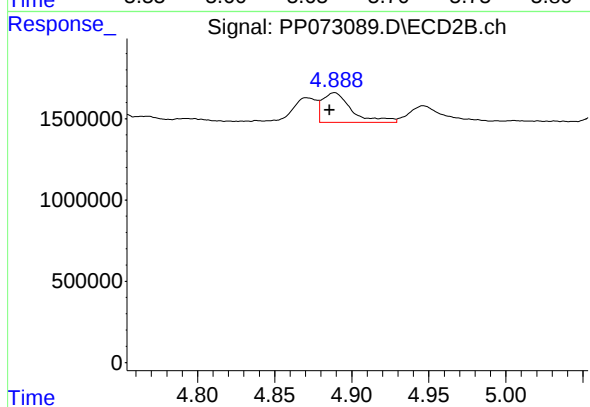

#4 AR-1016-2


R.T.: 4.889 min
Delta R.T.: 0.003 min
Response: 2391225
Conc: 23.76 ng/ml

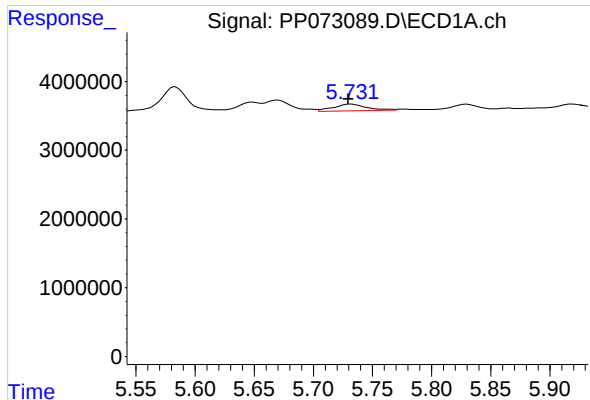

#5 AR-1016-3


R.T.: 5.732 min
Delta R.T.: 0.002 min
Response: 1918045
Conc: 29.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

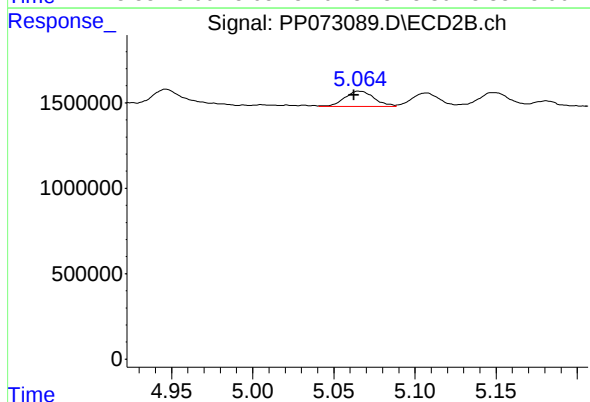


#5 AR-1016-3

R.T.: 5.066 min
Delta R.T.: 0.003 min
Response: 1149437
Conc: 21.01 ng/ml

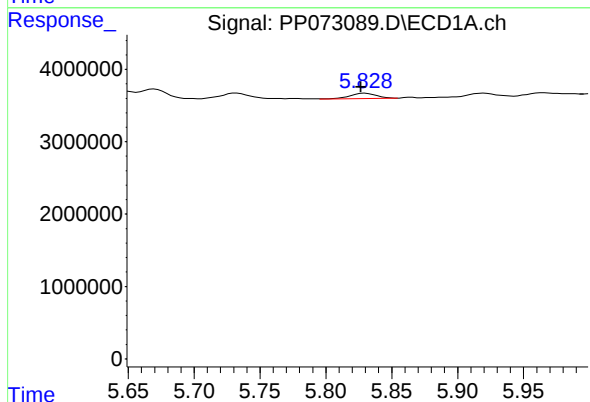


#6 AR-1016-4

R.T.: 5.830 min
Delta R.T.: 0.003 min
Response: 1061104
Conc: 20.30 ng/ml

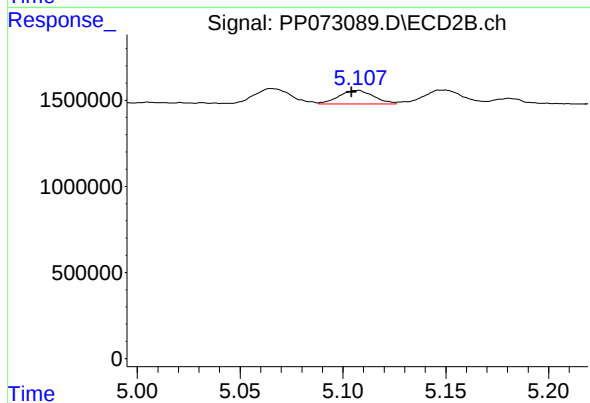

#6 AR-1016-4


R.T.: 5.107 min
Delta R.T.: 0.003 min
Response: 942028
Conc: 21.15 ng/ml

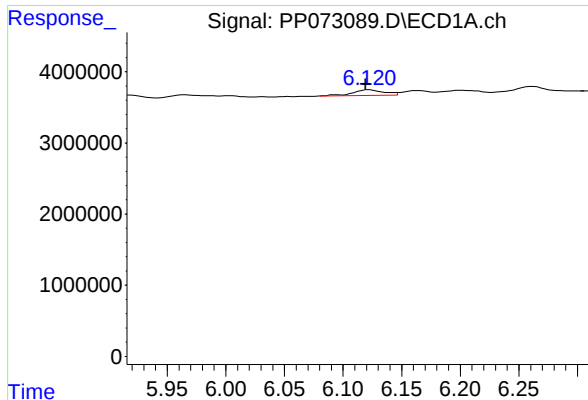

#7 AR-1016-5


R.T.: 6.122 min
Delta R.T.: 0.003 min
Response: 1455657
Conc: 29.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

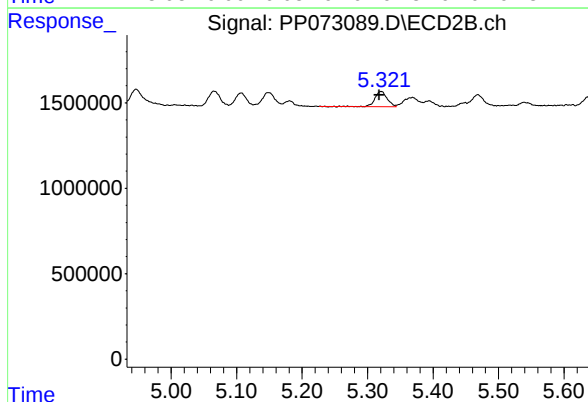


#7 AR-1016-5

R.T.: 5.321 min
Delta R.T.: 0.003 min
Response: 1138406
Conc: 20.59 ng/ml

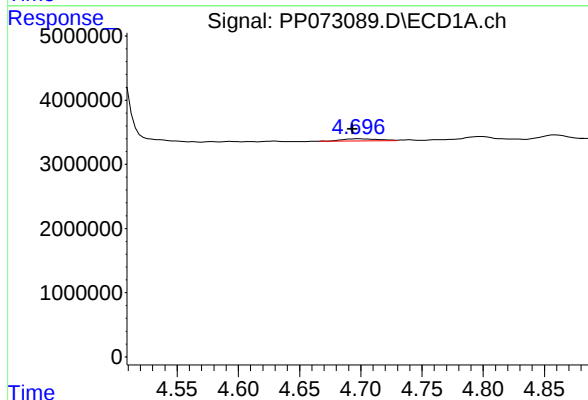


#8 AR-1221-1

R.T.: 4.698 min
Delta R.T.: 0.004 min
Response: 603928
Conc: 24.49 ng/ml

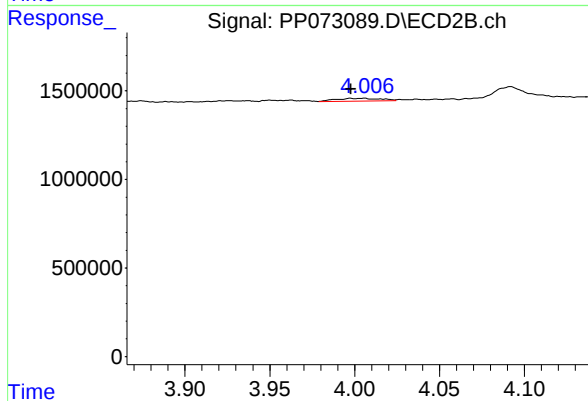

#8 AR-1221-1


R.T.: 3.998 min
Delta R.T.: 0.000 min
Response: 286529
Conc: 10.66 ng/ml

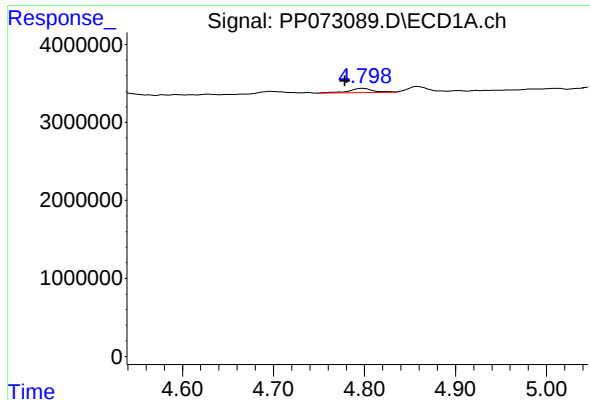

#9 AR-1221-2


R.T.: 4.799 min
Delta R.T.: 0.020 min
Response: 1016996
Conc: 50.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

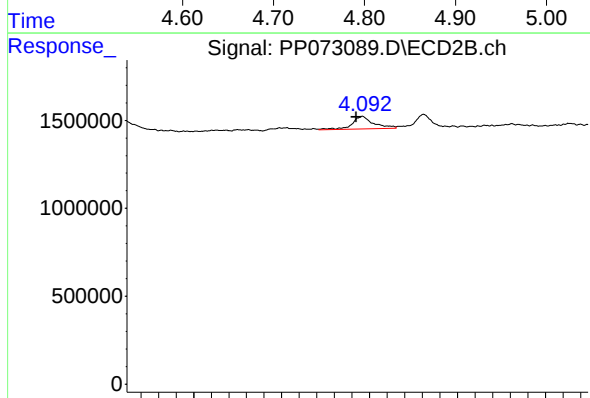


#9 AR-1221-2

R.T.: 4.092 min
Delta R.T.: 0.007 min
Response: 1244925
Conc: 61.67 ng/ml

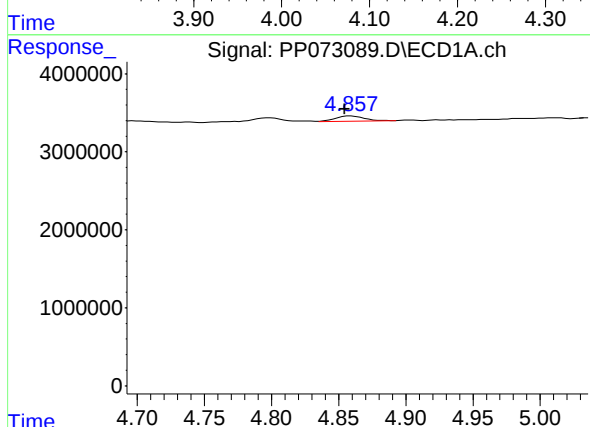


#10 AR-1221-3

R.T.: 4.859 min
Delta R.T.: 0.004 min
Response: 1024386
Conc: 16.64 ng/ml

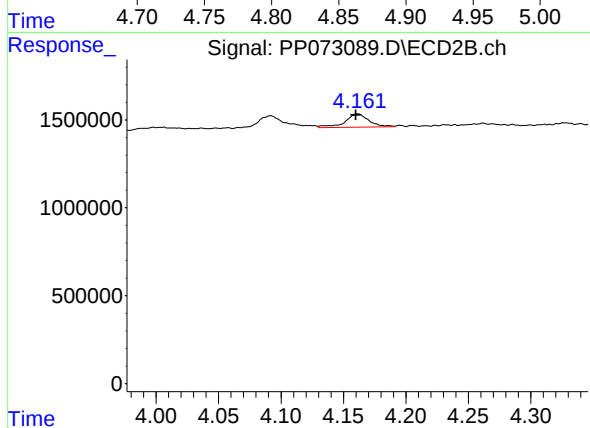

#10 AR-1221-3


R.T.: 4.161 min
Delta R.T.: 0.002 min
Response: 1026734
Conc: 17.48 ng/ml

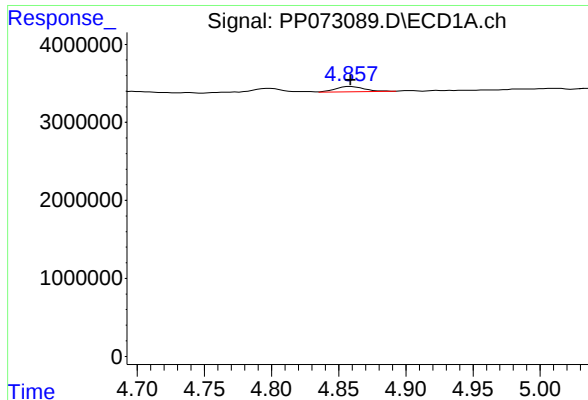

#11 AR-1232-1


R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 1024386
Conc: 21.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

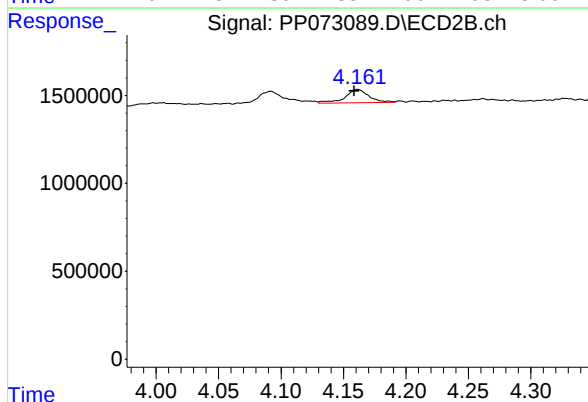


#11 AR-1232-1

R.T.: 4.161 min
Delta R.T.: 0.003 min
Response: 1026734
Conc: 22.53 ng/ml

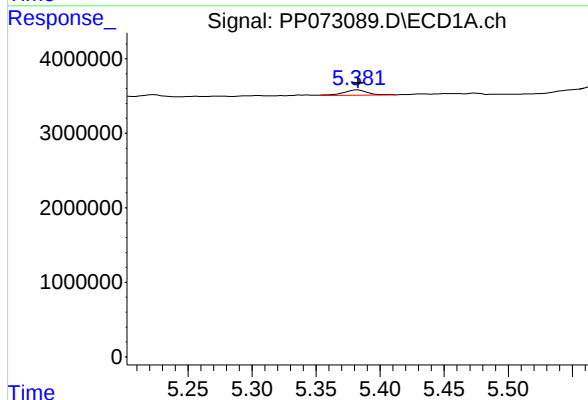


#12 AR-1232-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 934300
Conc: 41.77 ng/ml

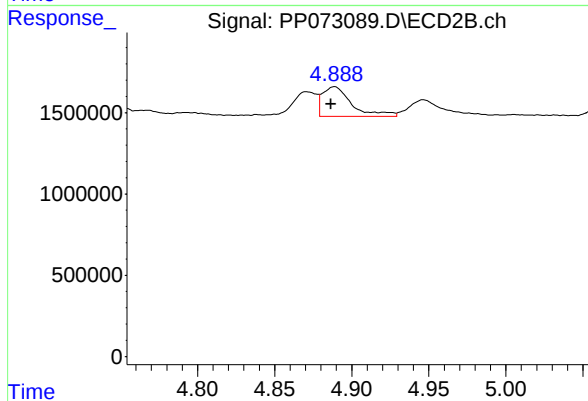

#12 AR-1232-2


R.T.: 4.889 min
Delta R.T.: 0.002 min
Response: 2391225
Conc: 51.69 ng/ml

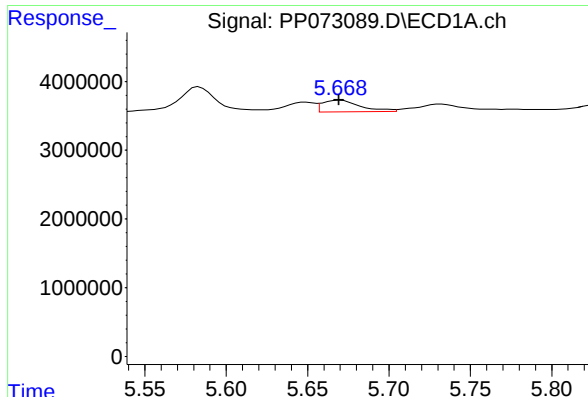

#13 AR-1232-3


R.T.: 5.670 min
Delta R.T.: 0.000 min
Response: 2728778
Conc: 52.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

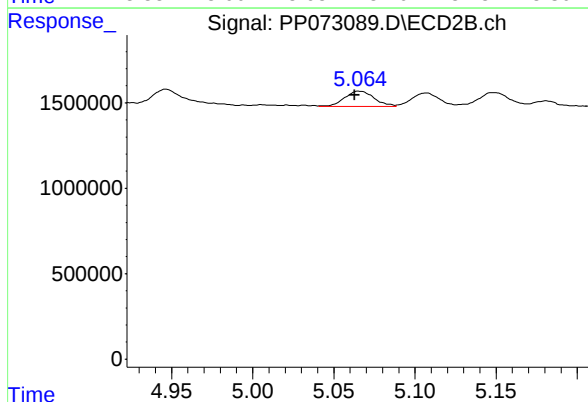


#13 AR-1232-3

R.T.: 5.066 min
Delta R.T.: 0.003 min
Response: 1149437
Conc: 46.81 ng/ml

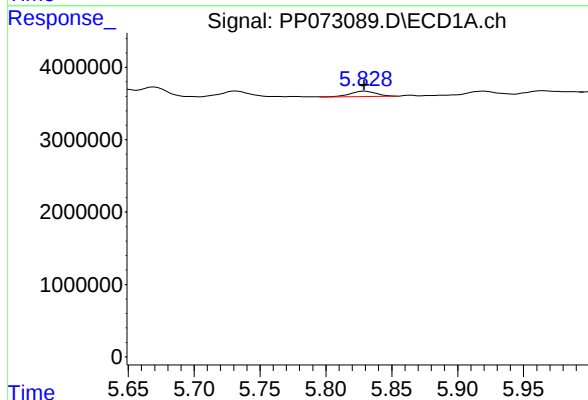


#14 AR-1232-4

R.T.: 5.830 min
Delta R.T.: 0.000 min
Response: 1061104
Conc: 41.11 ng/ml

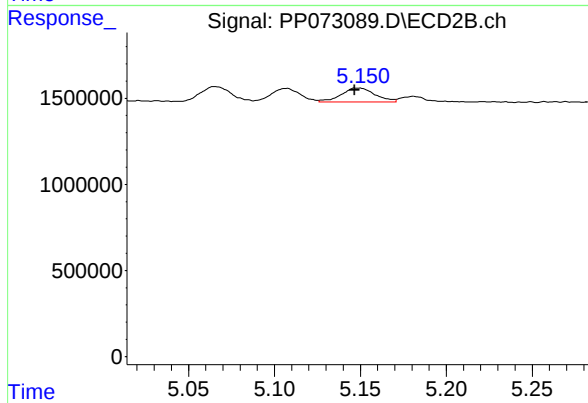

#14 AR-1232-4


R.T.: 5.148 min
Delta R.T.: 0.002 min
Response: 1122188
Conc: 51.89 ng/ml

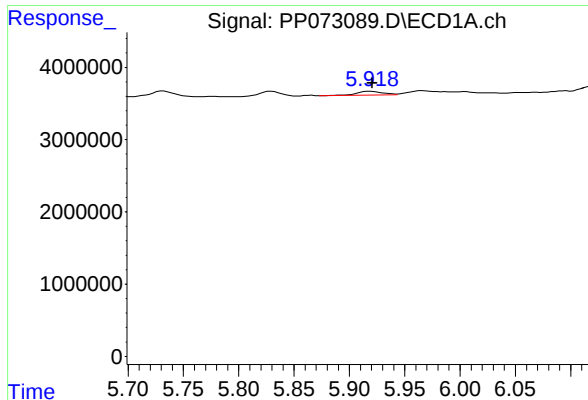

#15 AR-1232-5


R.T.: 5.919 min
Delta R.T.: -0.001 min
Response: 866179
Conc: 24.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

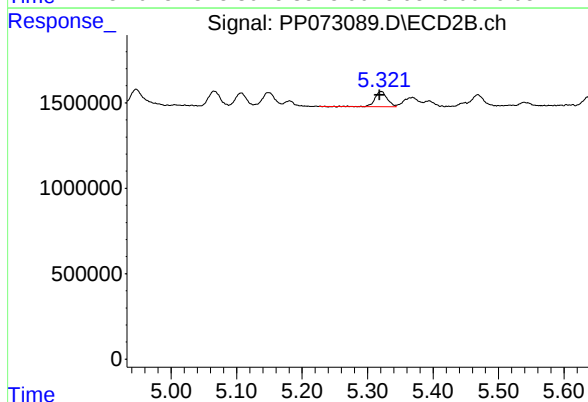


#15 AR-1232-5

R.T.: 5.321 min
Delta R.T.: 0.002 min
Response: 1138406
Conc: 49.80 ng/ml

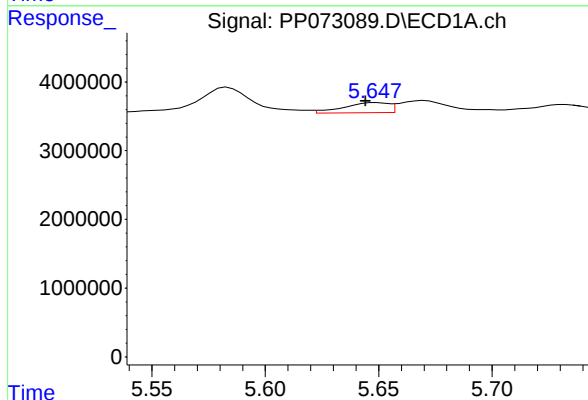


#16 AR-1242-1

R.T.: 5.649 min
Delta R.T.: 0.005 min
Response: 1992138
Conc: 34.09 ng/ml

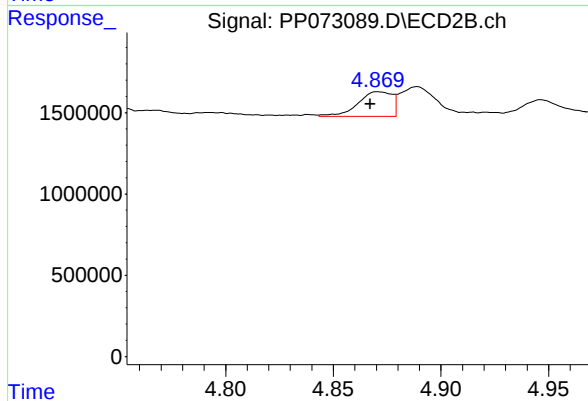

#16 AR-1242-1


R.T.: 4.871 min
Delta R.T.: 0.004 min
Response: 1665218
Conc: 30.16 ng/ml

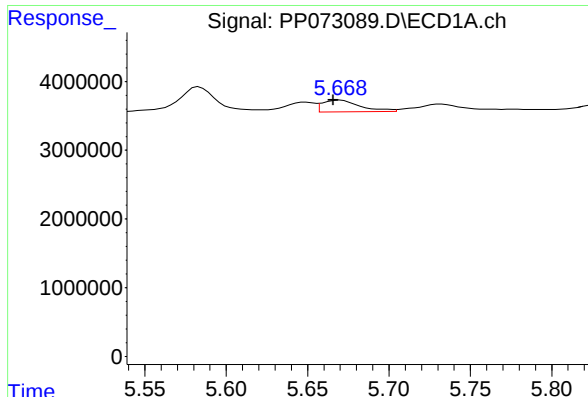

#17 AR-1242-2


R.T.: 5.670 min
Delta R.T.: 0.004 min
Response: 2728778
Conc: 31.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

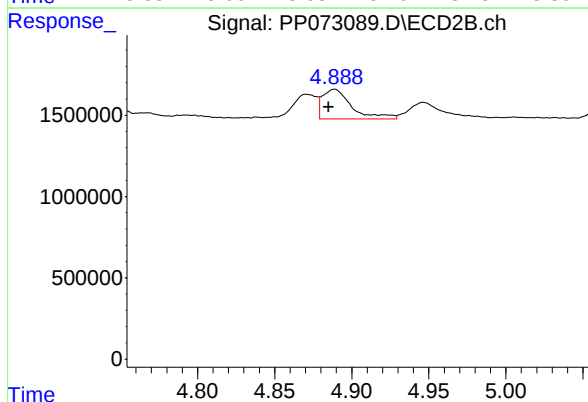


#17 AR-1242-2

R.T.: 4.889 min
Delta R.T.: 0.004 min
Response: 2391225
Conc: 30.08 ng/ml

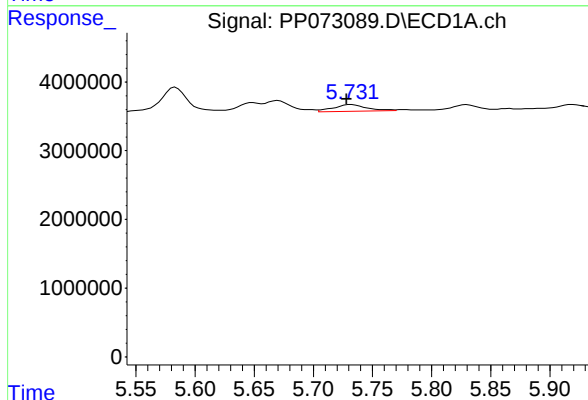


#18 AR-1242-3

R.T.: 5.732 min
Delta R.T.: 0.004 min
Response: 1918045
Conc: 36.39 ng/ml

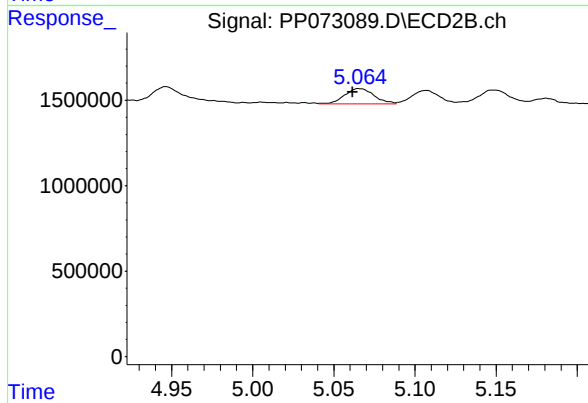

#18 AR-1242-3


R.T.: 5.066 min
Delta R.T.: 0.004 min
Response: 1149437
Conc: 26.54 ng/ml

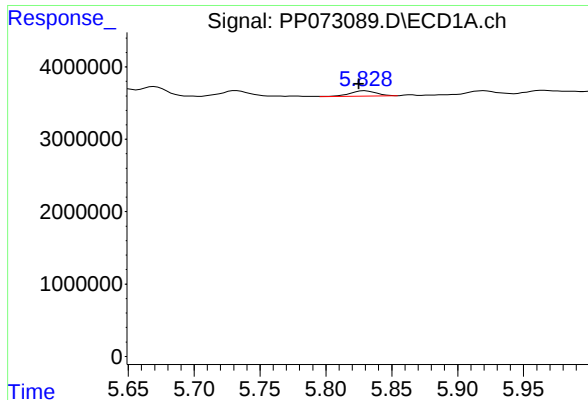

#19 AR-1242-4


R.T.: 5.830 min
Delta R.T.: 0.004 min
Response: 1061104
Conc: 24.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

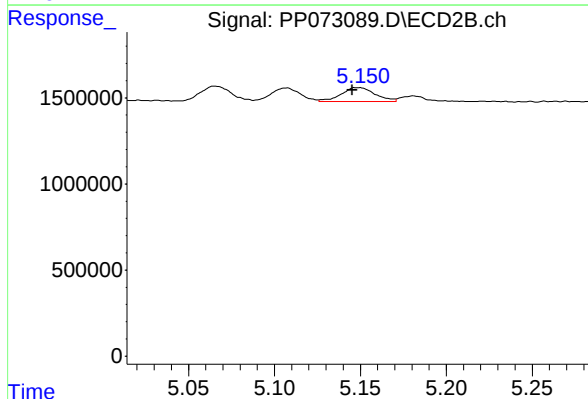


#19 AR-1242-4

R.T.: 5.148 min
Delta R.T.: 0.003 min
Response: 1122188
Conc: 27.04 ng/ml

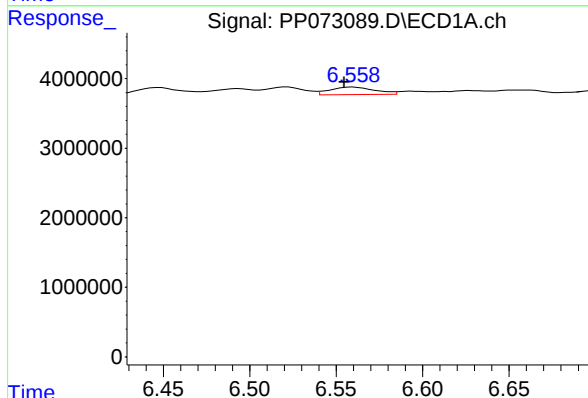


#20 AR-1242-5

R.T.: 6.560 min
Delta R.T.: 0.005 min
Response: 1965817
Conc: 39.67 ng/ml

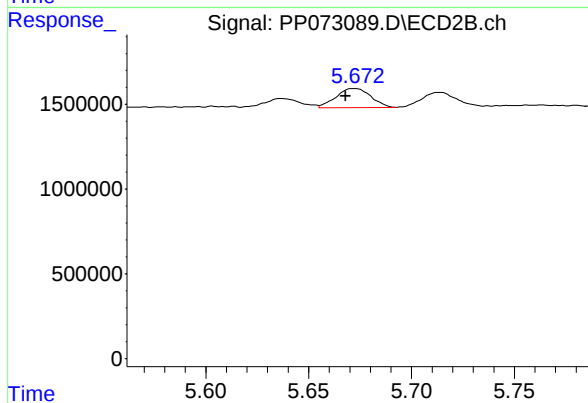

#20 AR-1242-5


R.T.: 5.672 min
Delta R.T.: 0.004 min
Response: 1325613
Conc: 25.21 ng/ml

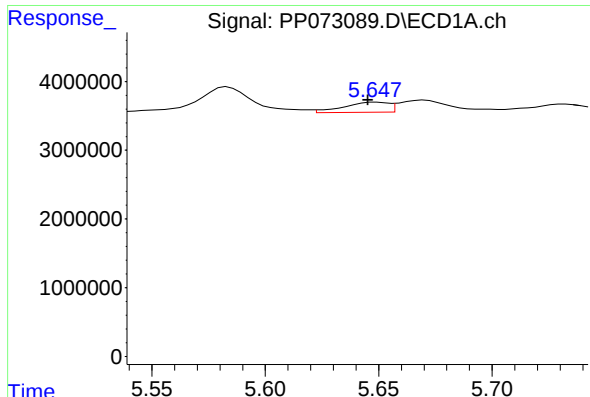

#21 AR-1248-1


R.T.: 5.649 min
Delta R.T.: 0.004 min
Response: 1992138
Conc: 41.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

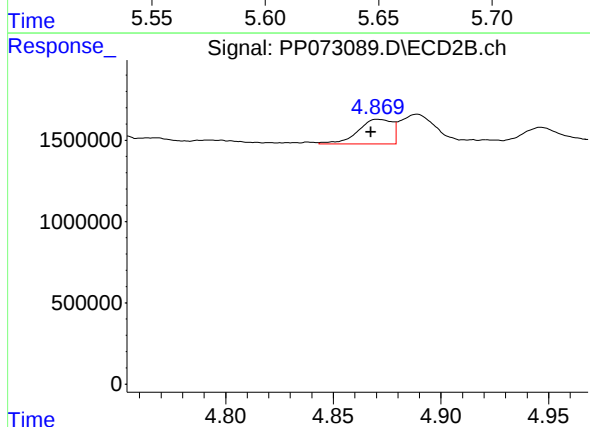


#21 AR-1248-1

R.T.: 4.871 min
Delta R.T.: 0.003 min
Response: 1665218
Conc: 38.20 ng/ml

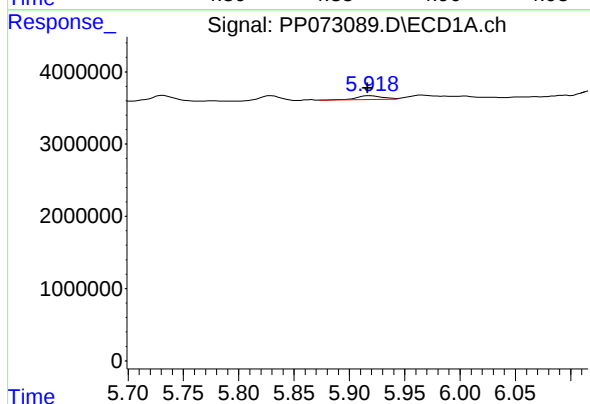


#22 AR-1248-2

R.T.: 5.919 min
Delta R.T.: 0.003 min
Response: 866179
Conc: 14.79 ng/ml

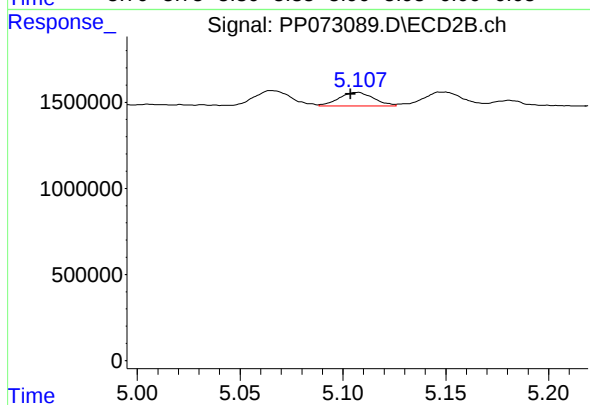

#22 AR-1248-2


R.T.: 5.107 min
Delta R.T.: 0.003 min
Response: 942028
Conc: 16.08 ng/ml

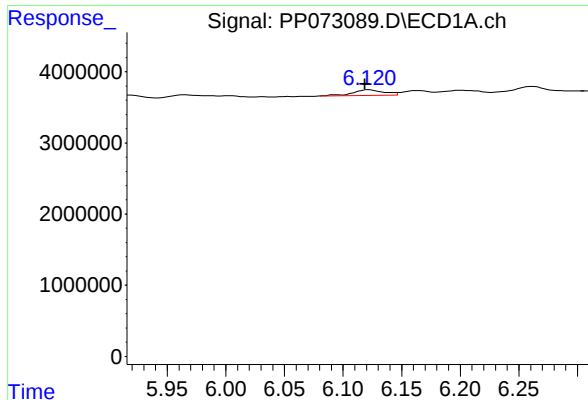

#23 AR-1248-3


R.T.: 6.122 min
Delta R.T.: 0.004 min
Response: 1455657
Conc: 22.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

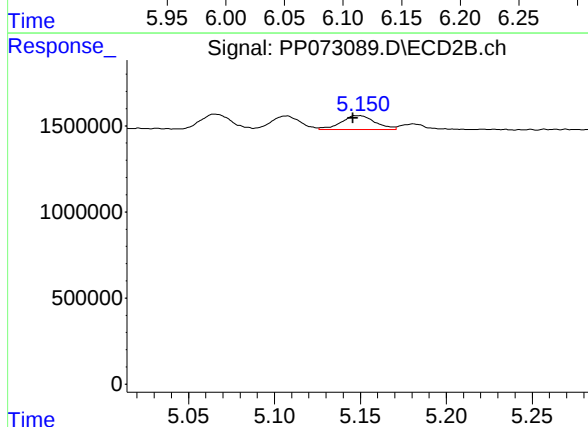


#23 AR-1248-3

R.T.: 5.148 min
Delta R.T.: 0.003 min
Response: 1122188
Conc: 18.54 ng/ml

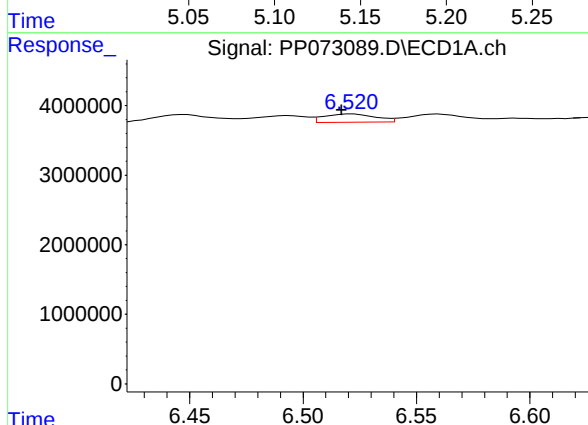


#24 AR-1248-4

R.T.: 6.521 min
Delta R.T.: 0.004 min
Response: 1869249
Conc: 21.97 ng/ml

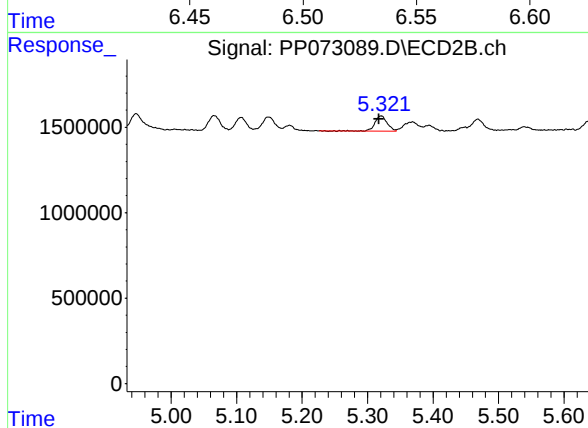

#24 AR-1248-4


R.T.: 5.321 min
Delta R.T.: 0.003 min
Response: 1138406
Conc: 16.26 ng/ml

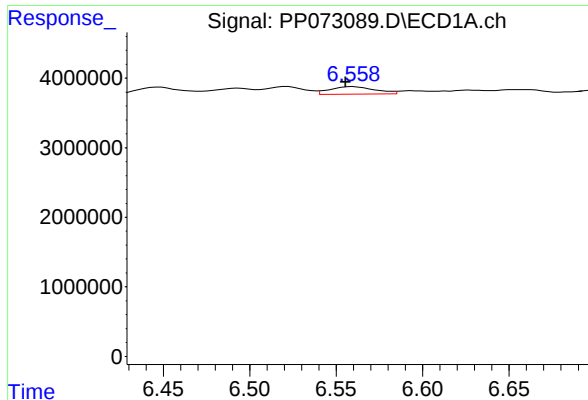

#25 AR-1248-5


R.T.: 6.560 min
Delta R.T.: 0.004 min
Response: 1965817
Conc: 23.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

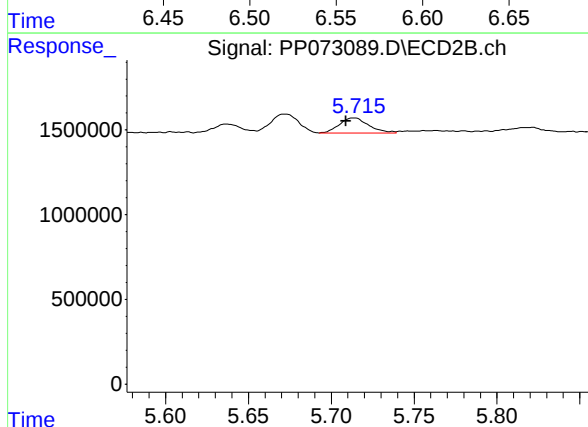


#25 AR-1248-5

R.T.: 5.714 min
Delta R.T.: 0.005 min
Response: 1106513
Conc: 15.58 ng/ml

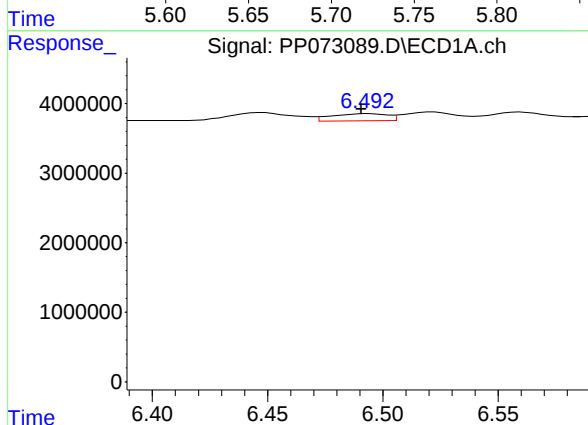


#26 AR-1254-1

R.T.: 6.493 min
Delta R.T.: 0.003 min
Response: 1706325
Conc: 20.27 ng/ml

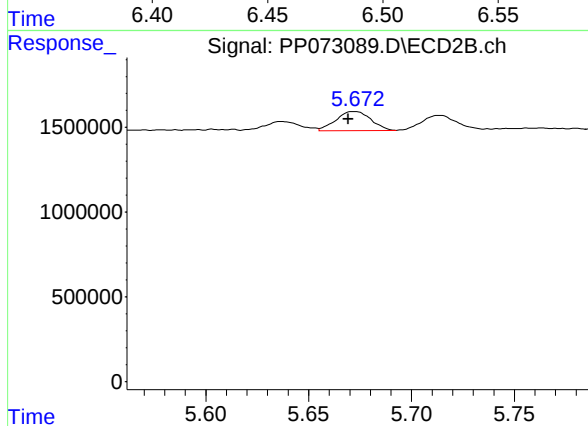

#26 AR-1254-1


R.T.: 5.672 min
Delta R.T.: 0.003 min
Response: 1325613
Conc: 12.09 ng/ml

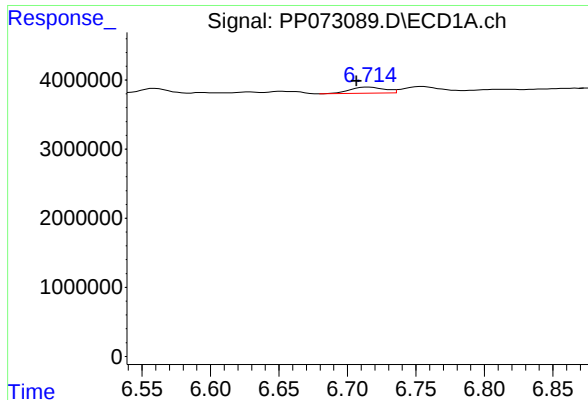

#27 AR-1254-2


R.T.: 6.716 min
Delta R.T.: 0.009 min
Response: 1588678
Conc: 12.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

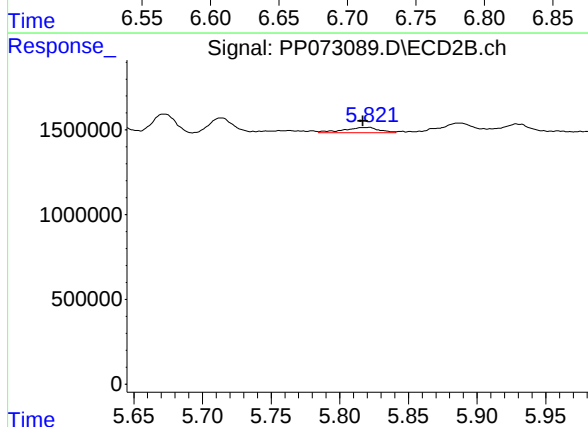


#27 AR-1254-2

R.T.: 5.821 min
Delta R.T.: 0.004 min
Response: 577020
Conc: 6.10 ng/ml

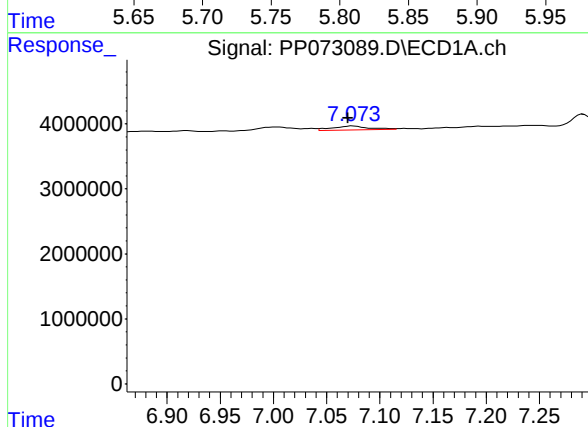


#28 AR-1254-3

R.T.: 7.074 min
Delta R.T.: 0.004 min
Response: 1455814
Conc: 11.10 ng/ml

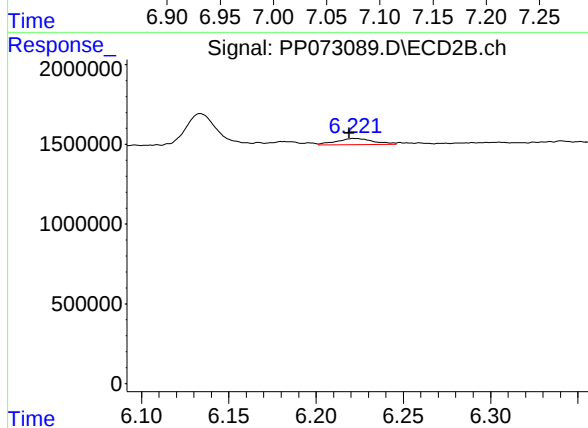

#28 AR-1254-3


R.T.: 6.222 min
Delta R.T.: 0.003 min
Response: 563438
Conc: 3.82 ng/ml

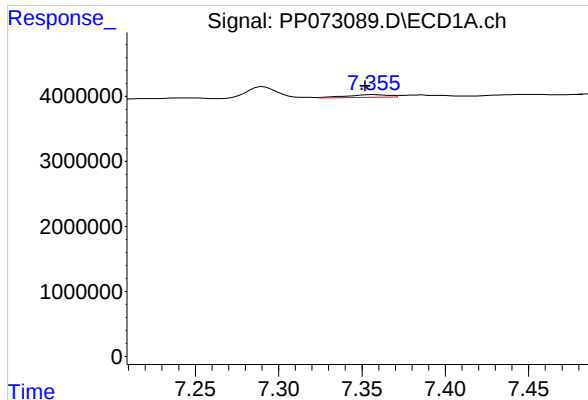

#29 AR-1254-4


R.T.: 7.357 min
Delta R.T.: 0.005 min
Response: 714428
Conc: 5.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

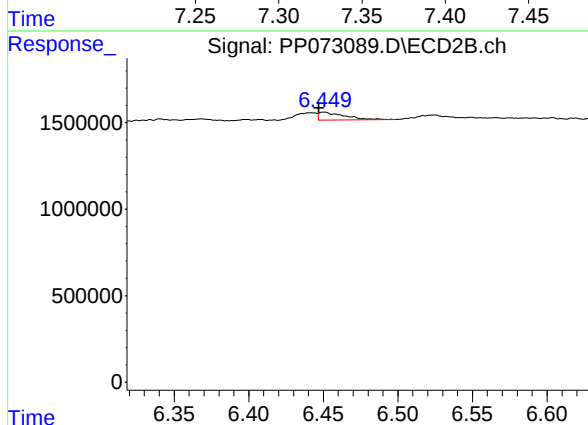


#29 AR-1254-4

R.T.: 6.450 min
Delta R.T.: 0.003 min
Response: 542480
Conc: 5.59 ng/ml

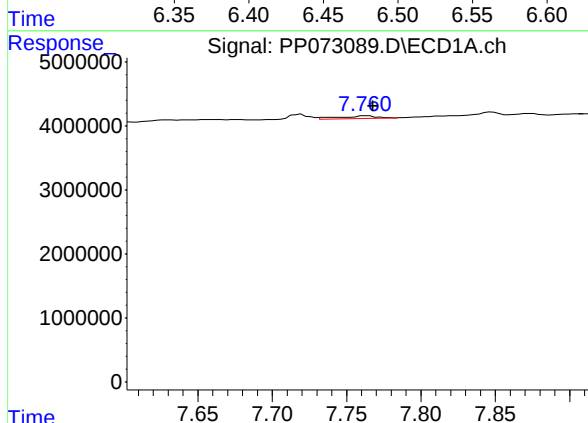


#30 AR-1254-5

R.T.: 7.762 min
Delta R.T.: -0.005 min
Response: 700314
Conc: 6.13 ng/ml

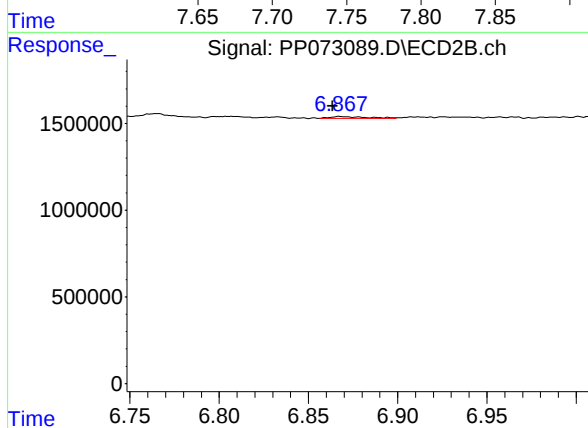

#30 AR-1254-5


R.T.: 6.867 min
Delta R.T.: 0.004 min
Response: 156018
Conc: 1.20 ng/ml

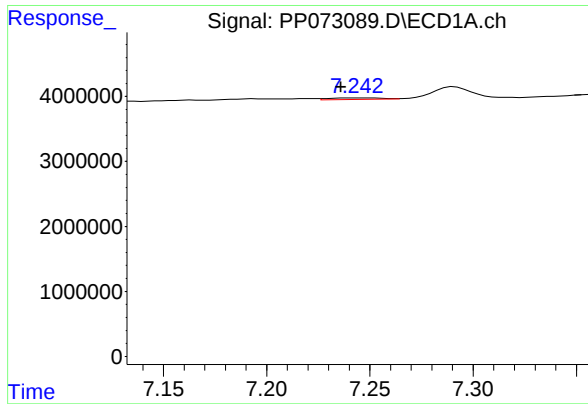

#31 AR-1260-1


R.T.: 7.245 min
Delta R.T.: 0.009 min
Response: 405677
Conc: 4.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

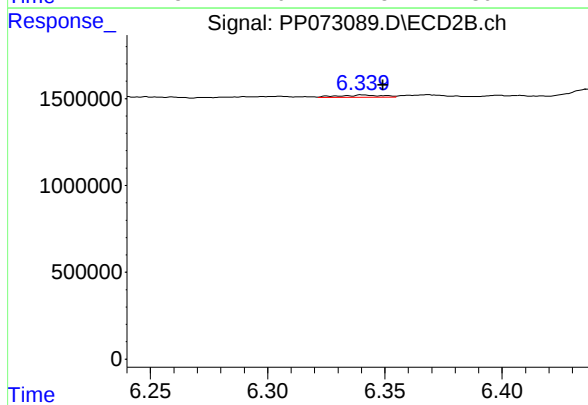


#31 AR-1260-1

R.T.: 6.341 min
Delta R.T.: -0.008 min
Response: 177461
Conc: 1.87 ng/ml

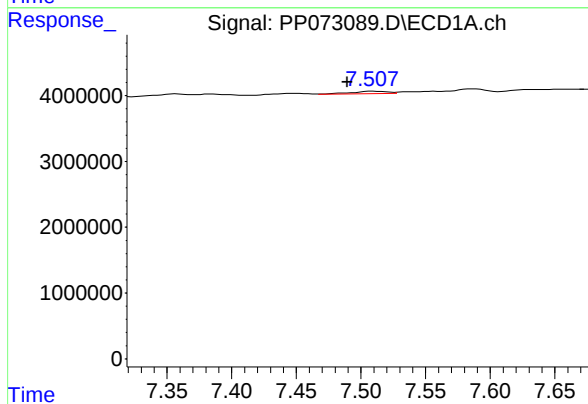


#32 AR-1260-2

R.T.: 7.508 min
Delta R.T.: 0.019 min
Response: 730597
Conc: 5.38 ng/ml

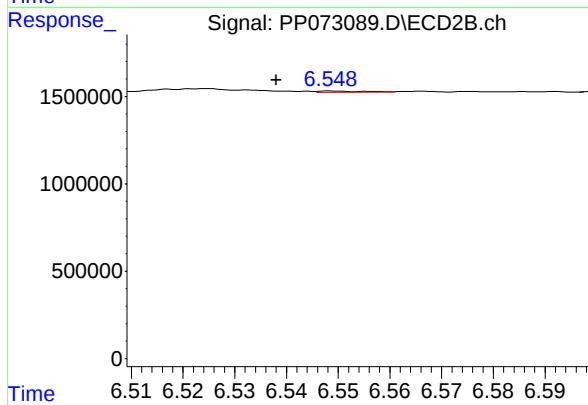

#32 AR-1260-2


R.T.: 6.549 min
Delta R.T.: 0.011 min
Response: 47638
Conc: 0.41 ng/ml

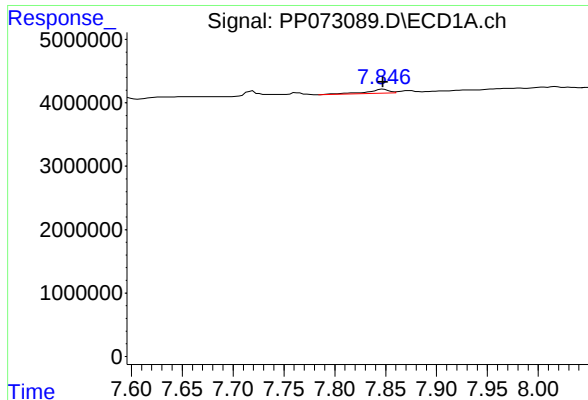

#33 AR-1260-3


R.T.: 7.847 min
Delta R.T.: 0.000 min
Response: 968091
Conc: 8.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

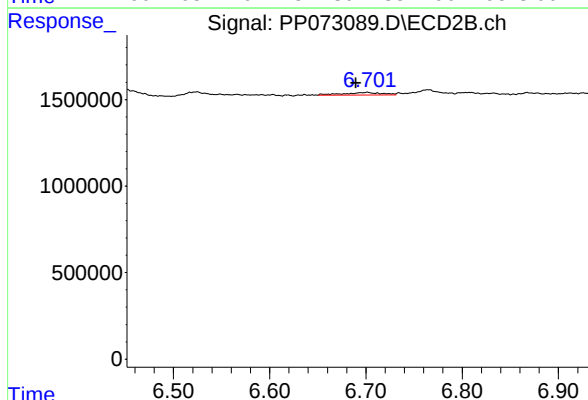


#33 AR-1260-3

R.T.: 6.701 min
Delta R.T.: 0.012 min
Response: 392857
Conc: 3.77 ng/ml

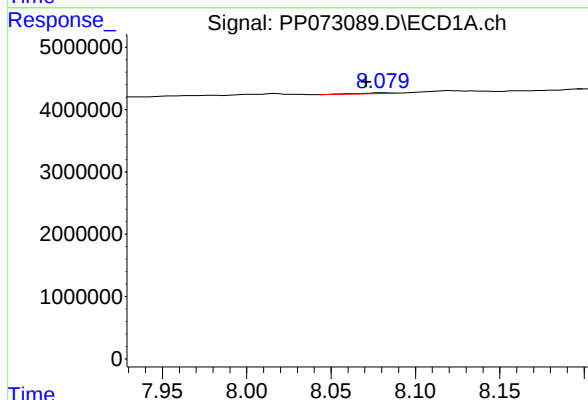


#34 AR-1260-4

R.T.: 8.082 min
Delta R.T.: 0.011 min
Response: 193588
Conc: 1.88 ng/ml

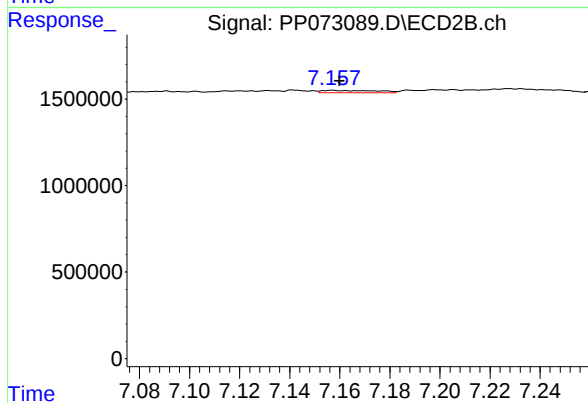

#34 AR-1260-4


R.T.: 7.157 min
Delta R.T.: -0.003 min
Response: 211544
Conc: 2.41 ng/ml

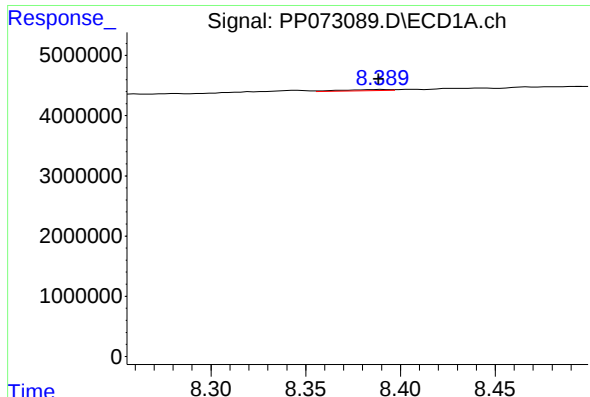

#35 AR-1260-5


R.T.: 8.392 min
Delta R.T.: 0.003 min
Response: 318885
Conc: 1.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

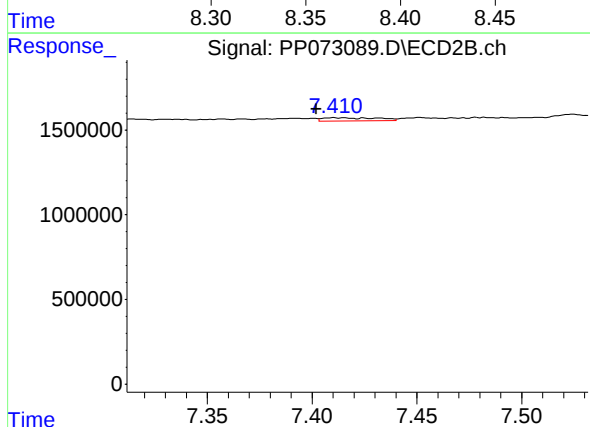


#35 AR-1260-5

R.T.: 7.410 min
Delta R.T.: 0.008 min
Response: 341462
Conc: 1.60 ng/ml

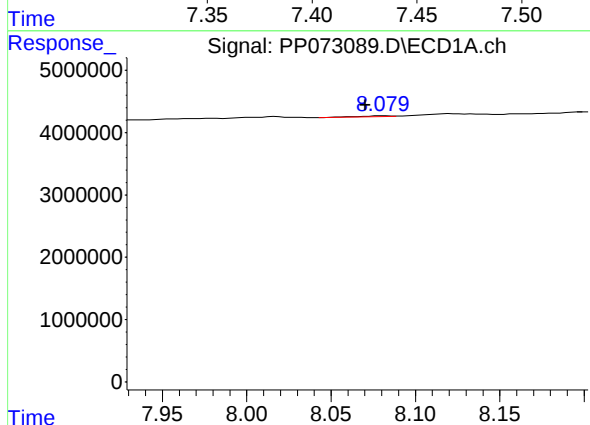


#36 AR-1262-1

R.T.: 8.082 min
Delta R.T.: 0.011 min
Response: 193588
Conc: 1.31 ng/ml

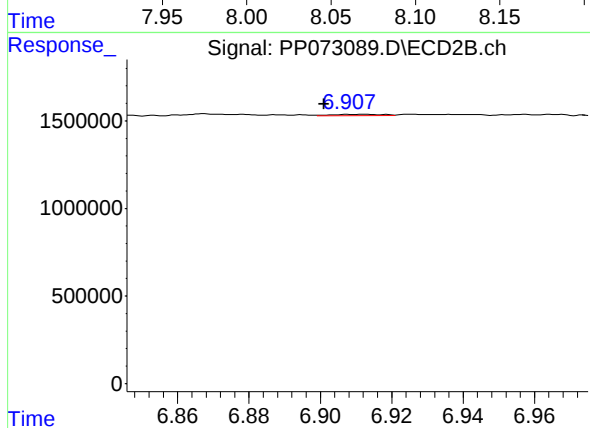

#36 AR-1262-1


R.T.: 6.913 min
Delta R.T.: 0.012 min
Response: 77453
Conc: 0.54 ng/ml

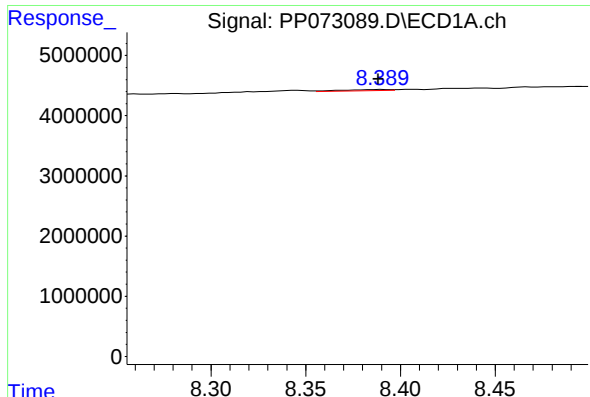

#37 AR-1262-2


R.T.: 8.392 min
Delta R.T.: 0.003 min
Response: 318885
Conc: 1.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

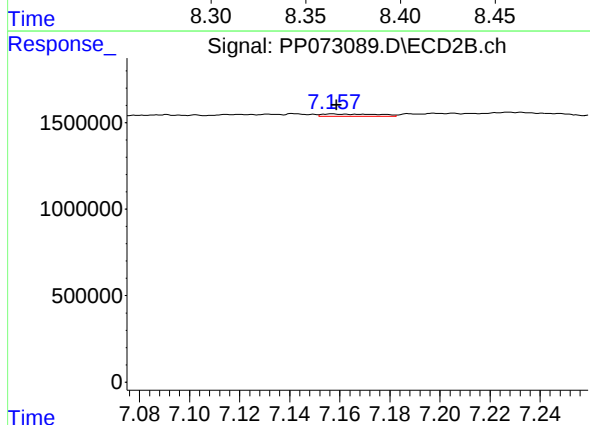


#37 AR-1262-2

R.T.: 7.157 min
Delta R.T.: -0.002 min
Response: 211544
Conc: 1.73 ng/ml

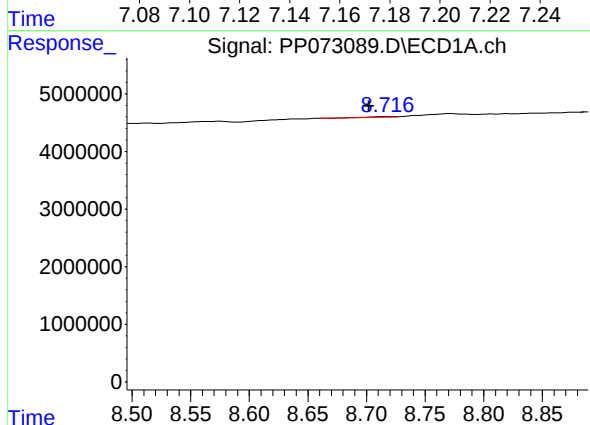


#38 AR-1262-3

R.T.: 8.717 min
Delta R.T.: 0.015 min
Response: 73148
Conc: 0.34 ng/ml

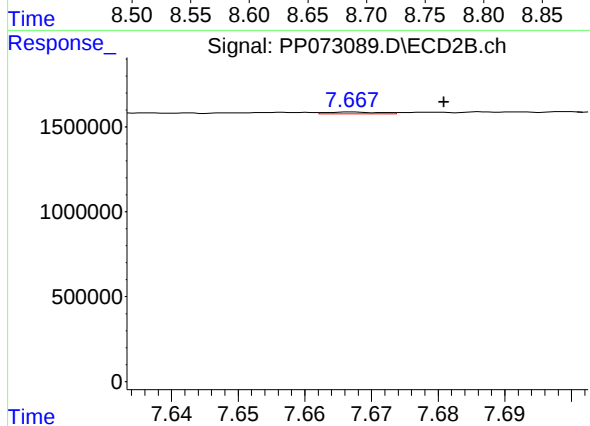

#38 AR-1262-3


R.T.: 7.667 min
Delta R.T.: -0.014 min
Response: 61448
Conc: 0.55 ng/ml

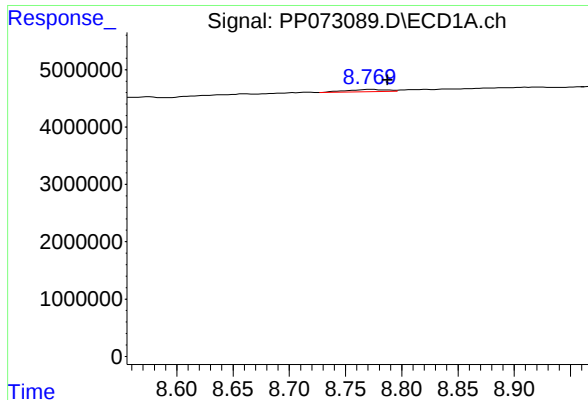

#39 AR-1262-4


R.T.: 8.772 min
Delta R.T.: -0.016 min
Response: 1052907
Conc: 6.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

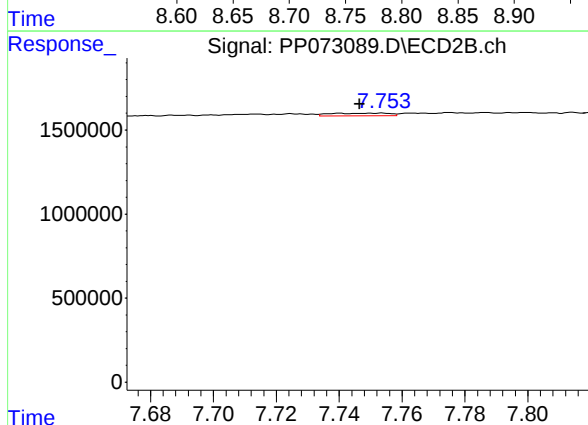


#39 AR-1262-4

R.T.: 7.753 min
Delta R.T.: 0.007 min
Response: 219214
Conc: 1.20 ng/ml

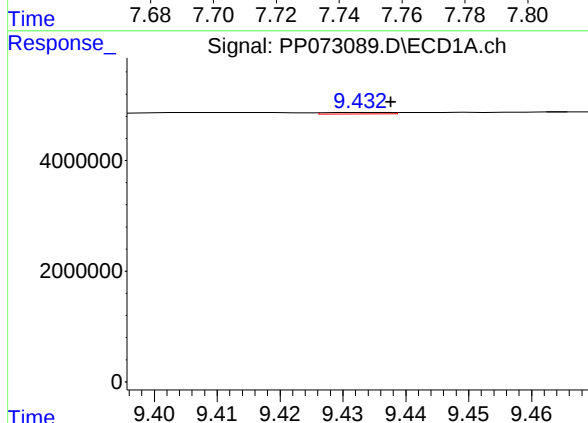


#40 AR-1262-5

R.T.: 9.434 min
Delta R.T.: -0.004 min
Response: 189075
Conc: 1.69 ng/ml

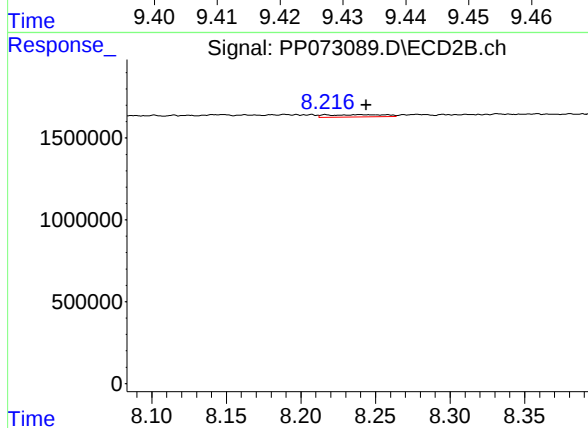

#40 AR-1262-5


R.T.: 8.217 min
Delta R.T.: -0.027 min
Response: 378790
Conc: 4.37 ng/ml

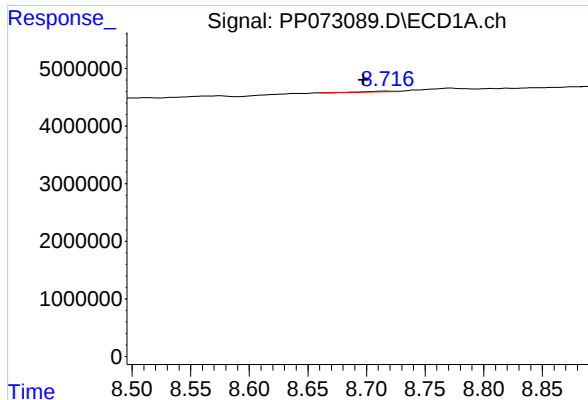

#41 AR-1268-1


R.T.: 8.717 min
Delta R.T.: 0.020 min
Response: 73148
Conc: 0.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

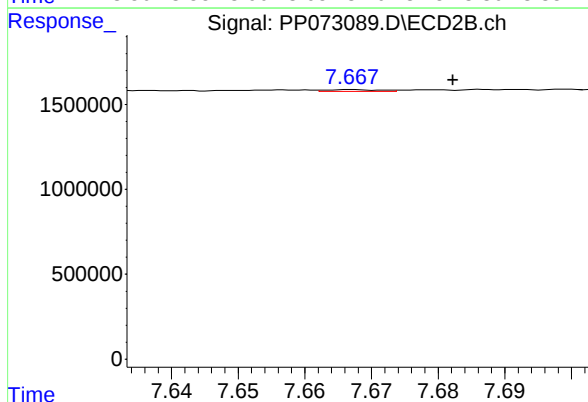


#41 AR-1268-1

R.T.: 7.667 min
Delta R.T.: -0.015 min
Response: 61448
Conc: 0.21 ng/ml

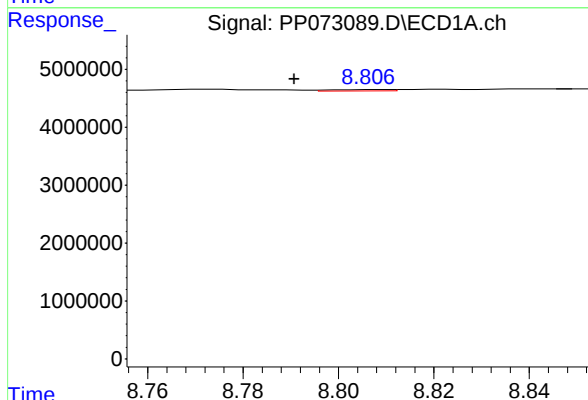


#42 AR-1268-2

R.T.: 8.808 min
Delta R.T.: 0.017 min
Response: 218504
Conc: 0.72 ng/ml

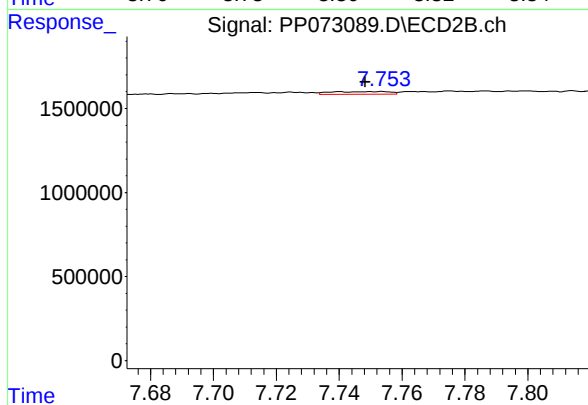

#42 AR-1268-2


R.T.: 7.753 min
Delta R.T.: 0.005 min
Response: 219214
Conc: 0.85 ng/ml

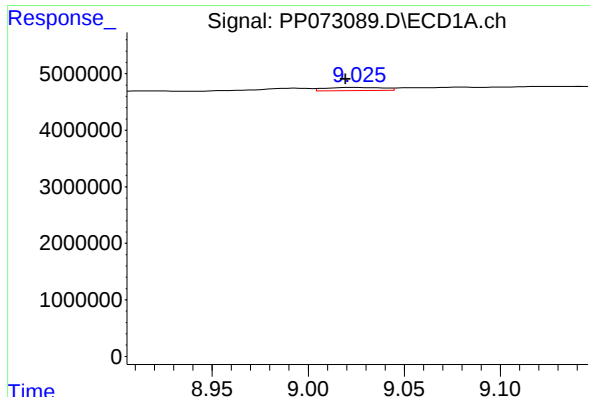

#43 AR-1268-3


R.T.: 9.027 min
Delta R.T.: 0.007 min
Response: 1203998
Conc: 4.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

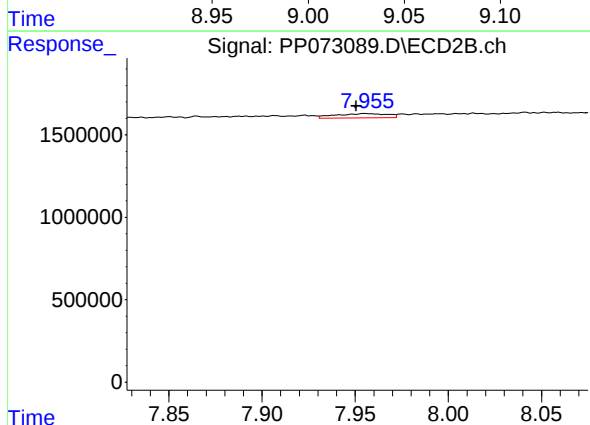


#43 AR-1268-3

R.T.: 7.956 min
Delta R.T.: 0.005 min
Response: 526940
Conc: 2.44 ng/ml

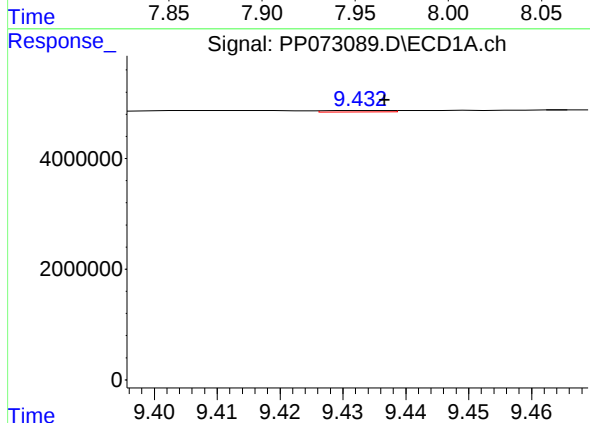


#44 AR-1268-4

R.T.: 9.434 min
Delta R.T.: -0.003 min
Response: 189075
Conc: 1.62 ng/ml

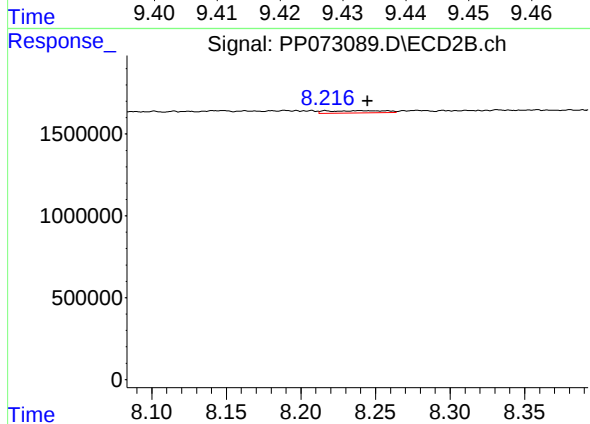

#44 AR-1268-4


R.T.: 8.217 min
Delta R.T.: -0.028 min
Response: 378790
Conc: 4.02 ng/ml

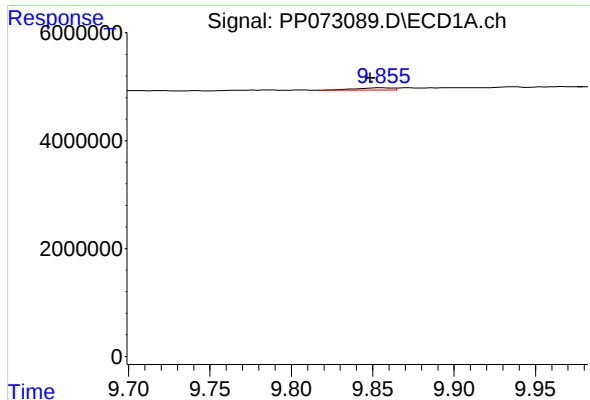

#45 AR-1268-5

R.T.: 9.856 min
Delta R.T.: 0.008 min
Response: 611122
Conc: 0.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

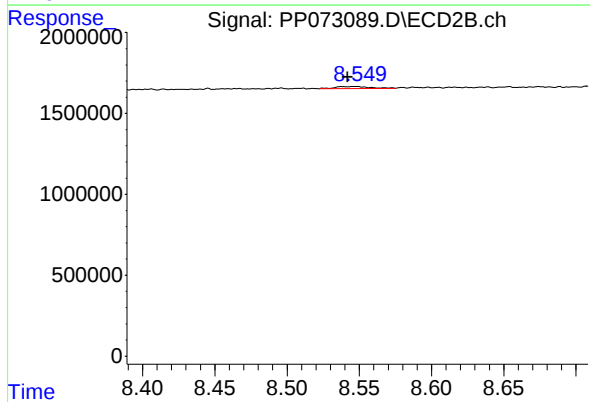

#45 AR-1268-5

R.T.: 8.547 min
Delta R.T.: 0.005 min
Response: 205762
Conc: 0.36 ng/ml