

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 17:54
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:28:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.495	3.789	41639116	35589857	19.727	19.752
2) SA Decachlor...	10.190	8.800	37614633	28112503	22.011	21.063
Target Compounds						
3) L1 AR-1016-1	5.646	4.870	1691696	1418193	23.279	20.638
4) L1 AR-1016-2	5.669	4.887	1342616	1284072	12.907	12.759
5) L1 AR-1016-3	5.728	5.065	852004	1058478	13.038	19.345 #
6) L1 AR-1016-4	5.826	5.105	688031	1816748	13.160	40.780 #
7) L1 AR-1016-5	6.120	5.319	1566712	1935987	31.331	35.020
8) L2 AR-1221-1	4.698	4.014	121626	131909	4.932	4.909
9) L2 AR-1221-2	4.763	4.090	158331	799627	7.846	39.614 #
10) L2 AR-1221-3	4.855	4.160	392349	320901	6.374	5.464
11) L3 AR-1232-1	4.855	4.160	392349	320901	8.356	7.043
12) L3 AR-1232-2	5.378	4.887	560252	1284072	25.045	27.758
13) L3 AR-1232-3	5.669	5.065	1342616	1058478	26.021	43.101 #
14) L3 AR-1232-4	5.826	5.149	688031	1839471	26.657	85.062 #
15) L3 AR-1232-5	5.916	5.319	1851749	1935987	51.913	84.693 #
16) L4 AR-1242-1	5.646	4.870	1691696	1418193	28.949	25.683
17) L4 AR-1242-2	5.669	4.887	1342616	1284072	15.512	16.155
18) L4 AR-1242-3	5.728	5.065	852004	1058478	16.165	24.442 #
19) L4 AR-1242-4	5.826	5.149	688031	1839471	15.652	44.320 #
20) L4 AR-1242-5	6.558	5.671	2836461	2696502	57.233	51.277
21) L5 AR-1248-1	5.646	4.870	1691696	1418193	35.563	32.535
22) L5 AR-1248-2	5.916	5.105	1851749	1816748	31.626	31.005
23) L5 AR-1248-3	6.120	5.149	1566712	1839471	24.011	30.382 #
24) L5 AR-1248-4	6.519	5.319	2652361	1935987	31.181	27.648
25) L5 AR-1248-5	6.558	5.711	2836461	1769685	33.891	24.914 #
26) L6 AR-1254-1	6.493	5.671	2375343	2696502	28.219	24.592
27) L6 AR-1254-2	6.713	5.819	2447947	874929	19.521	9.254 #
28) L6 AR-1254-3	7.073	6.221	2002388	1259233	15.261	8.534 #
29) L6 AR-1254-4	7.357	6.448	2338051	1230375	19.519	12.671 #
30) L6 AR-1254-5	7.766	6.867	540872	143911	4.734	1.107 #
31) L7 AR-1260-1	7.260	6.363	1393818	598692	15.801	6.320 #
32) L7 AR-1260-2	7.452f	6.537	731588	125989	5.384	1.082 #
33) L7 AR-1260-3	7.867	6.687	1205536	75252	10.561	0.722 #
34) L7 AR-1260-4	8.079	7.161	663107	86708	6.435	0.988 #
35) L7 AR-1260-5	8.448f	7.416	740558	321672	3.078	1.507 #
36) L8 AR-1262-1	8.079	6.932	663107	83476	4.480	0.578 #
37) L8 AR-1262-2	8.329f	7.161	299146	86708	0.945	0.709
38) L8 AR-1262-3	8.719	7.677	320464	58284	1.498	0.517 #
39) L8 AR-1262-4	8.776	7.748	739791	235168	4.694	1.283 #
40) L8 AR-1262-5	9.418	8.240	306036	168891	2.736	1.951 #
41) L9 AR-1268-1	8.719	7.677	320464	58284	0.896	0.203 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 17:54
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:28:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.776	7.748	739791	235168	2.425	0.915 #
43) L9	AR-1268-3	9.024	7.953	938913	551104	3.536	2.552 #
44) L9	AR-1268-4	9.418	8.240	306036	168891	2.615	1.793 #
45) L9	AR-1268-5	9.854	8.543	209178	157294	0.283	0.272



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
Data File : PP073090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 17:54
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1248 MDL 25 PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:28:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

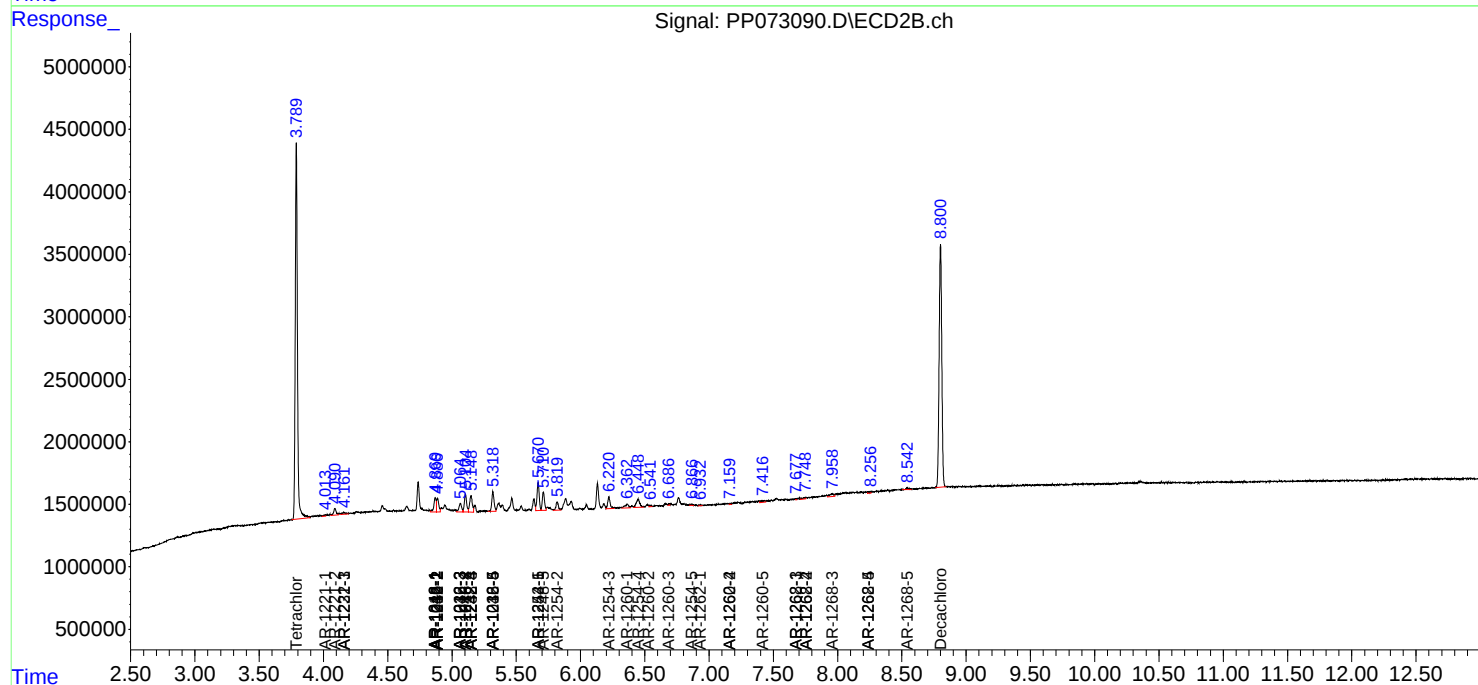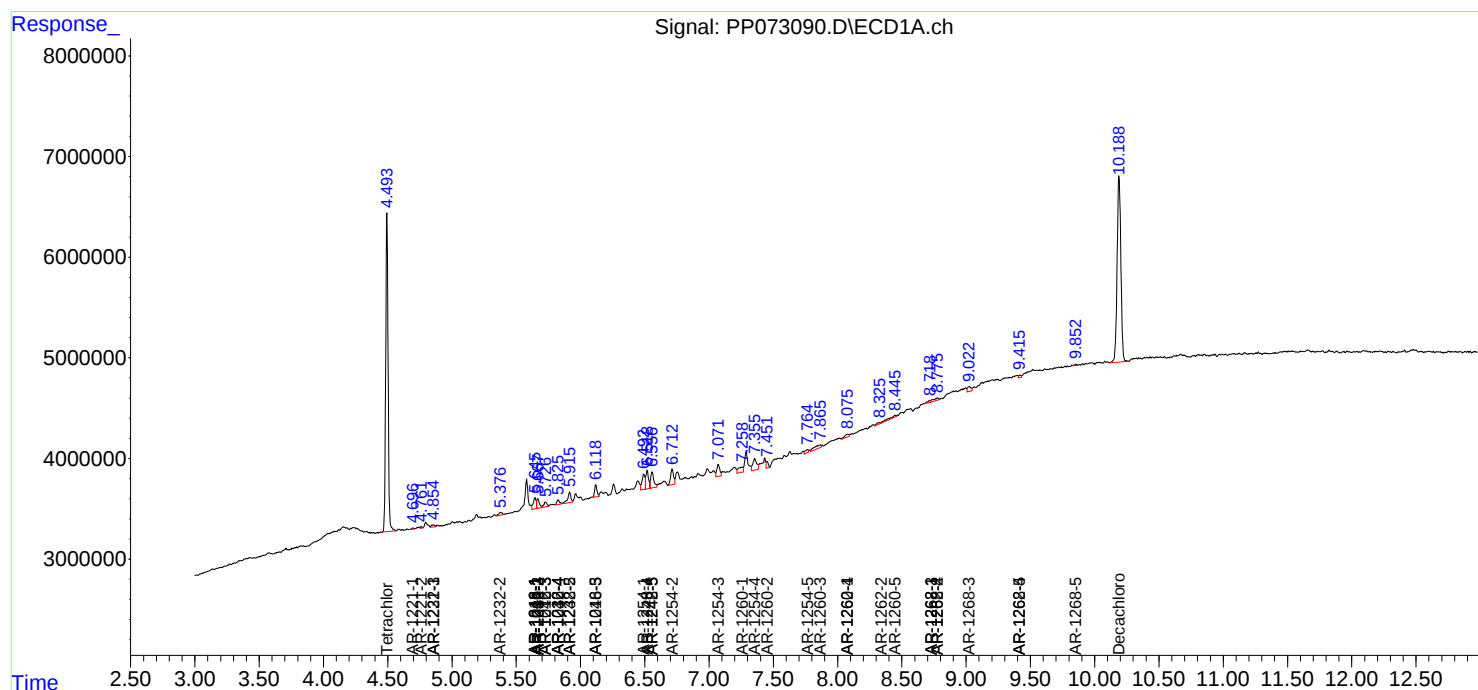


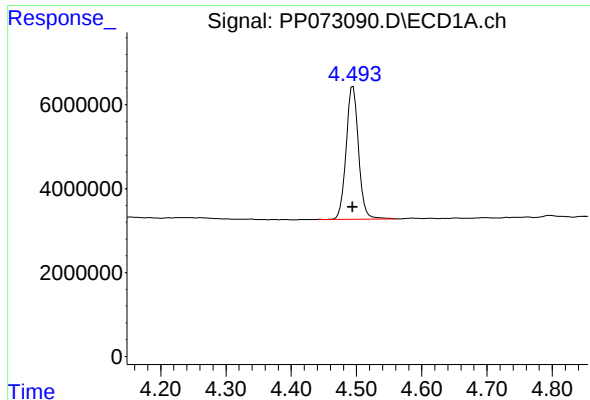

#1 Tetrachloro-m-xylene


R.T.: 4.495 min
Delta R.T.: 0.000 min
Response: 41639116
Conc: 19.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

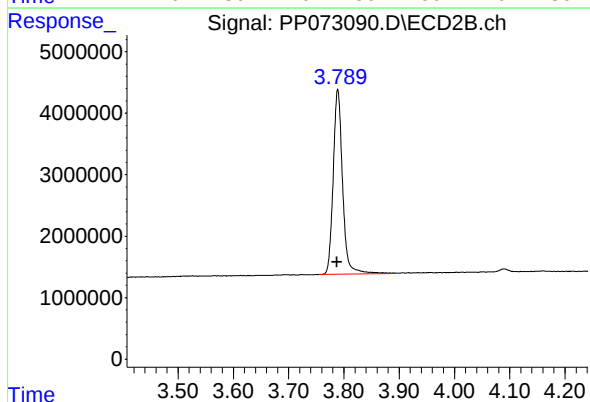


#1 Tetrachloro-m-xylene

R.T.: 3.789 min
Delta R.T.: 0.001 min
Response: 35589857
Conc: 19.75 ng/ml

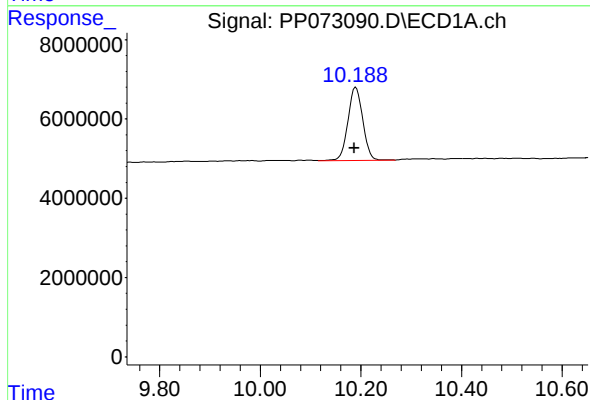


#2 Decachlorobiphenyl

R.T.: 10.190 min
Delta R.T.: 0.003 min
Response: 37614633
Conc: 22.01 ng/ml

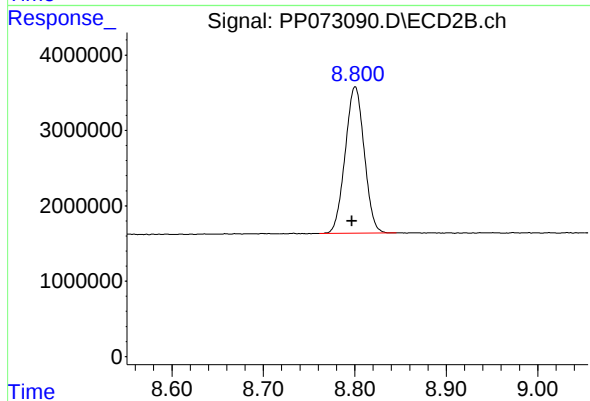

#2 Decachlorobiphenyl


R.T.: 8.800 min
Delta R.T.: 0.003 min
Response: 28112503
Conc: 21.06 ng/ml

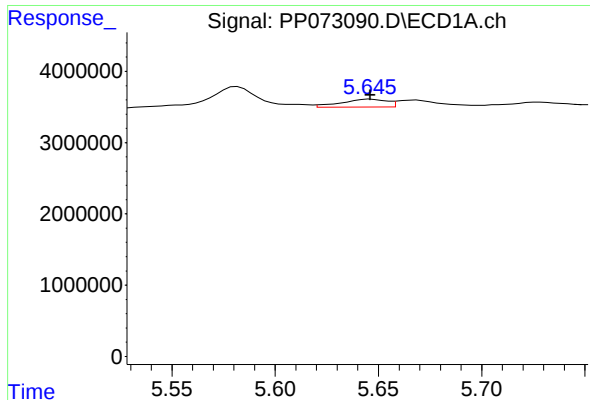

#3 AR-1016-1


R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 1691696
Conc: 23.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

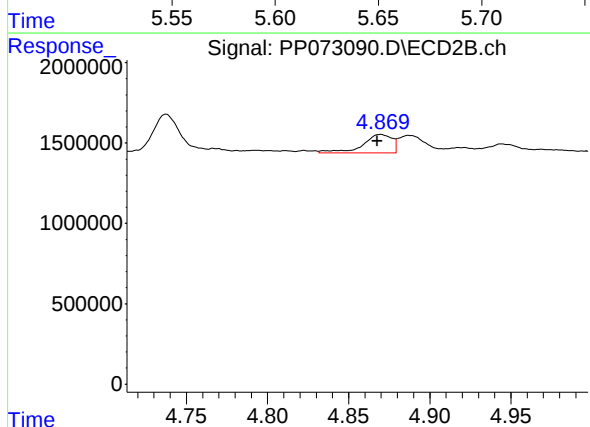


#3 AR-1016-1

R.T.: 4.870 min
Delta R.T.: 0.002 min
Response: 1418193
Conc: 20.64 ng/ml

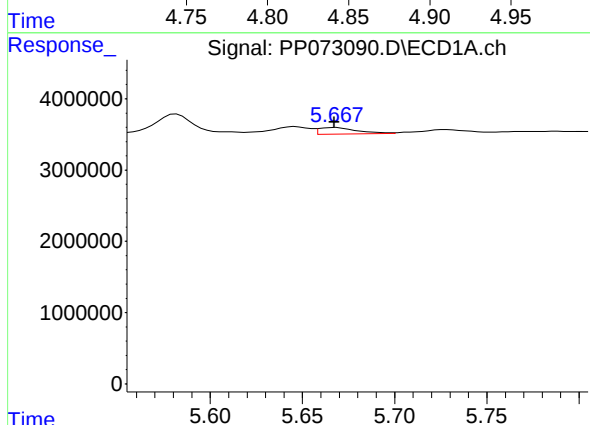


#4 AR-1016-2

R.T.: 5.669 min
Delta R.T.: 0.001 min
Response: 1342616
Conc: 12.91 ng/ml

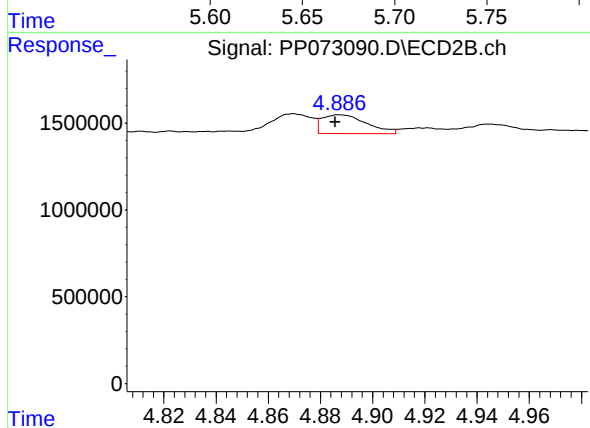

#4 AR-1016-2


R.T.: 4.887 min
Delta R.T.: 0.002 min
Response: 1284072
Conc: 12.76 ng/ml

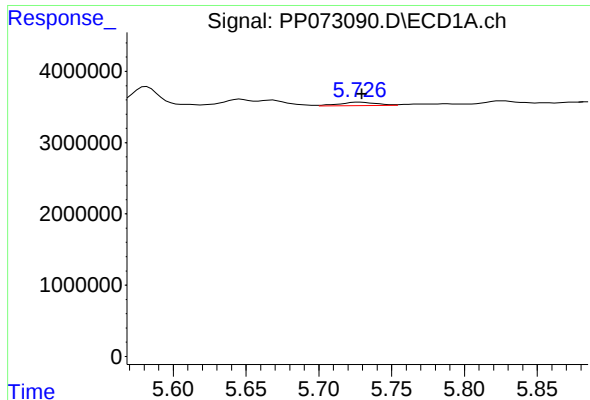

#5 AR-1016-3


R.T.: 5.728 min
Delta R.T.: -0.002 min
Response: 852004
Conc: 13.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

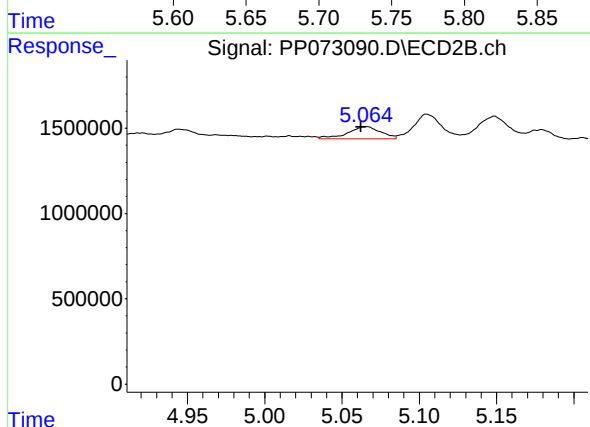


#5 AR-1016-3

R.T.: 5.065 min
Delta R.T.: 0.003 min
Response: 1058478
Conc: 19.34 ng/ml

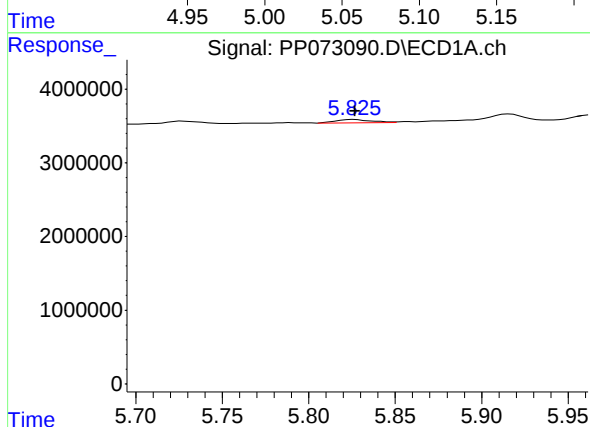


#6 AR-1016-4

R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 688031
Conc: 13.16 ng/ml

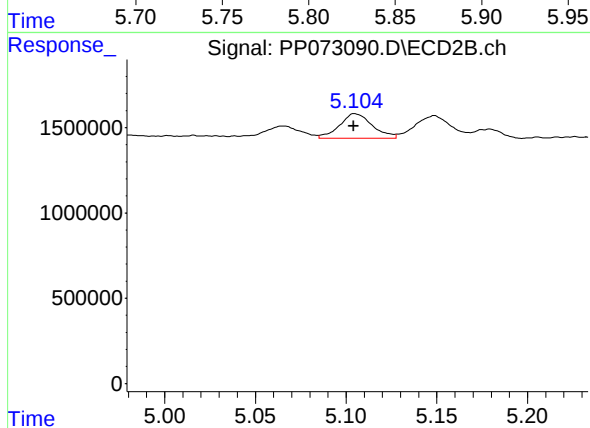

#6 AR-1016-4


R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 1816748
Conc: 40.78 ng/ml

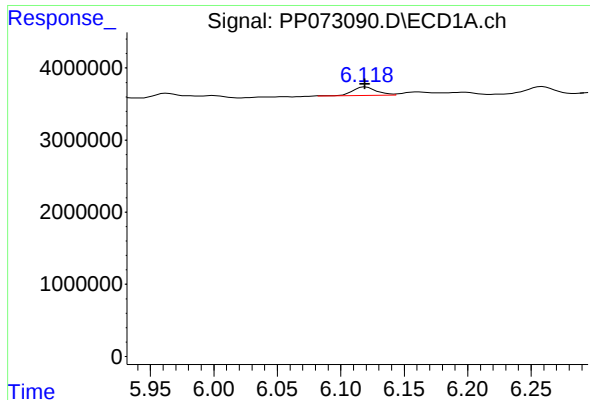

#7 AR-1016-5


R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 1566712
Conc: 31.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

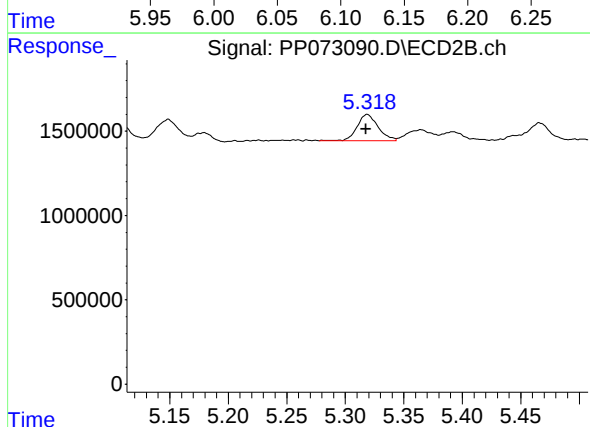


#7 AR-1016-5

R.T.: 5.319 min
Delta R.T.: 0.000 min
Response: 1935987
Conc: 35.02 ng/ml

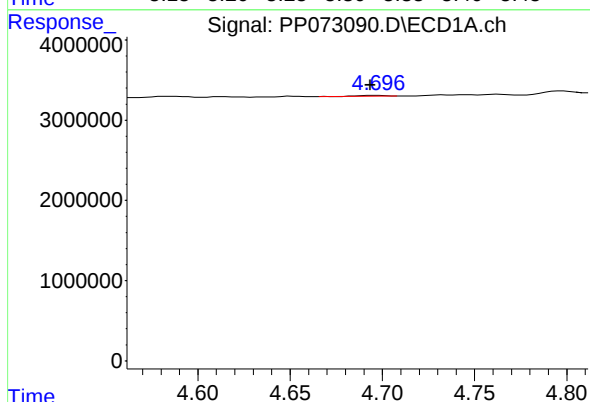


#8 AR-1221-1

R.T.: 4.698 min
Delta R.T.: 0.004 min
Response: 121626
Conc: 4.93 ng/ml

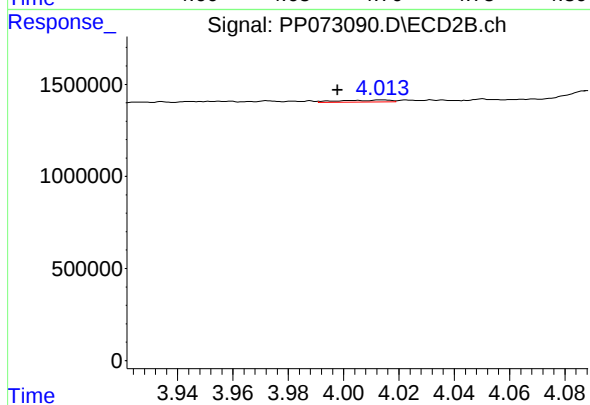

#8 AR-1221-1


R.T.: 4.014 min
Delta R.T.: 0.016 min
Response: 131909
Conc: 4.91 ng/ml

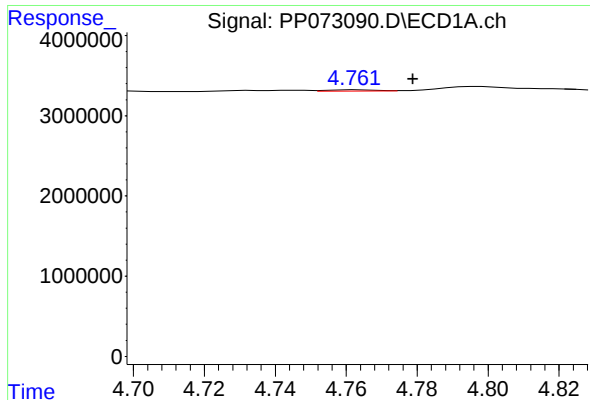

#9 AR-1221-2


R.T.: 4.763 min
Delta R.T.: -0.016 min
Response: 158331
Conc: 7.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

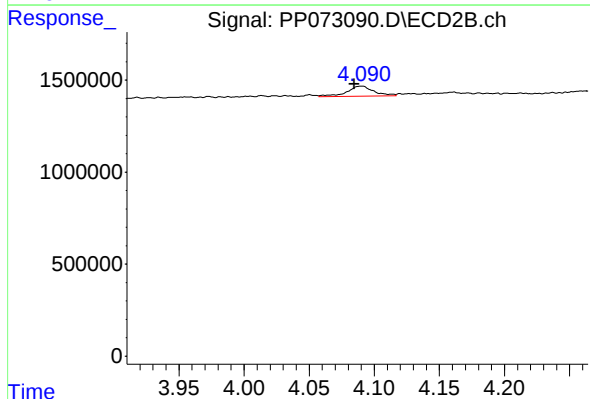


#9 AR-1221-2

R.T.: 4.090 min
Delta R.T.: 0.006 min
Response: 799627
Conc: 39.61 ng/ml

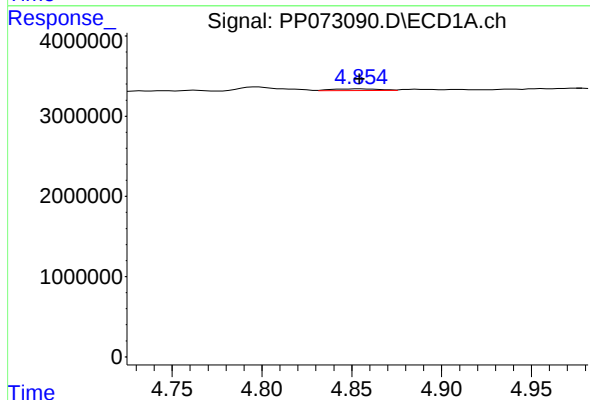


#10 AR-1221-3

R.T.: 4.855 min
Delta R.T.: 0.000 min
Response: 392349
Conc: 6.37 ng/ml

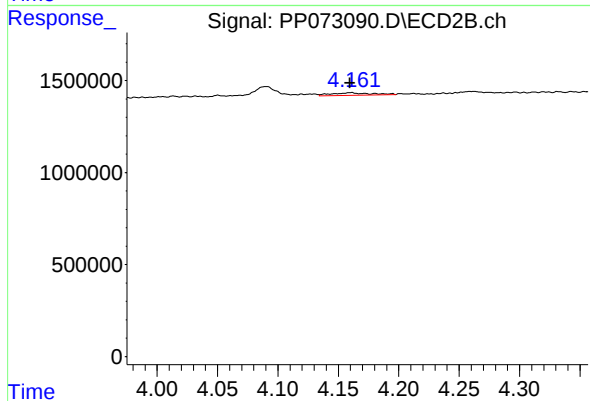

#10 AR-1221-3


R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 320901
Conc: 5.46 ng/ml

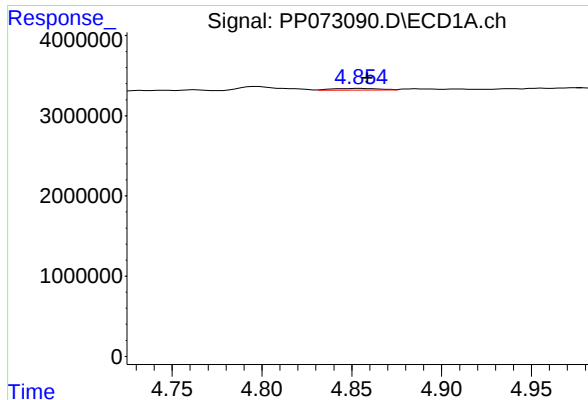

#11 AR-1232-1


R.T.: 4.855 min
Delta R.T.: -0.004 min
Response: 392349
Conc: 8.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

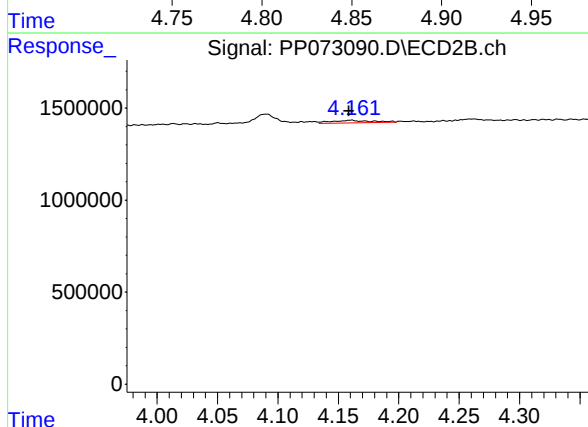


#11 AR-1232-1

R.T.: 4.160 min
Delta R.T.: 0.002 min
Response: 320901
Conc: 7.04 ng/ml

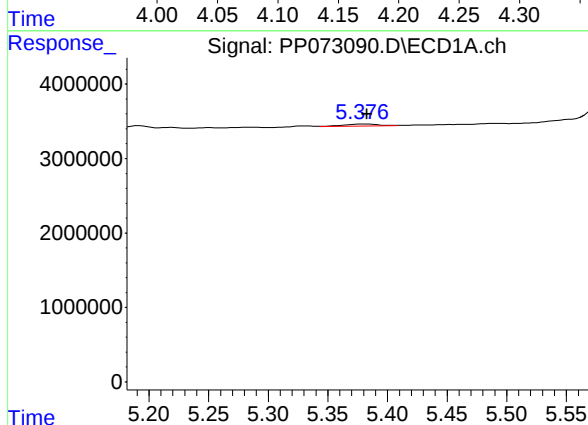


#12 AR-1232-2

R.T.: 5.378 min
Delta R.T.: -0.005 min
Response: 560252
Conc: 25.04 ng/ml

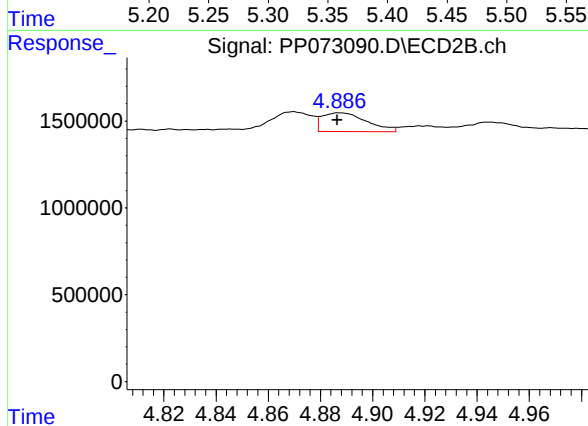

#12 AR-1232-2


R.T.: 4.887 min
Delta R.T.: 0.000 min
Response: 1284072
Conc: 27.76 ng/ml

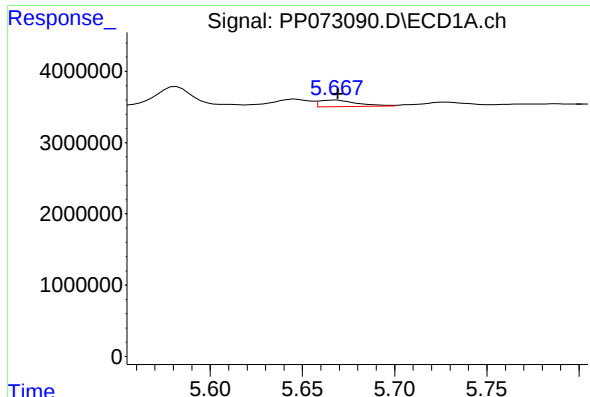

#13 AR-1232-3


R.T.: 5.669 min
Delta R.T.: 0.000 min
Response: 1342616
Conc: 26.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

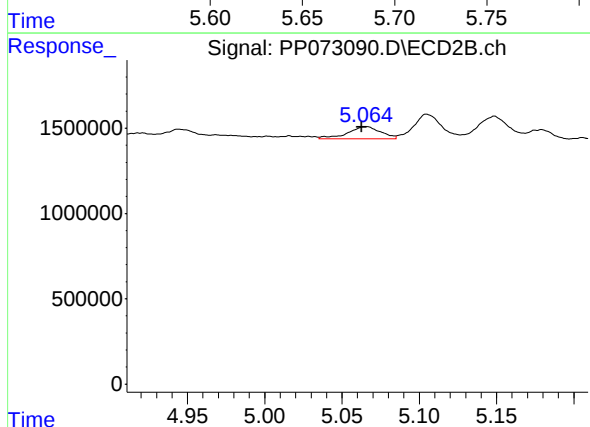


#13 AR-1232-3

R.T.: 5.065 min
Delta R.T.: 0.003 min
Response: 1058478
Conc: 43.10 ng/ml

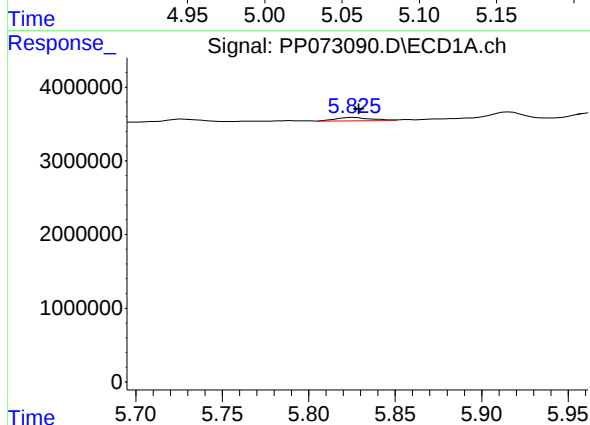


#14 AR-1232-4

R.T.: 5.826 min
Delta R.T.: -0.003 min
Response: 688031
Conc: 26.66 ng/ml

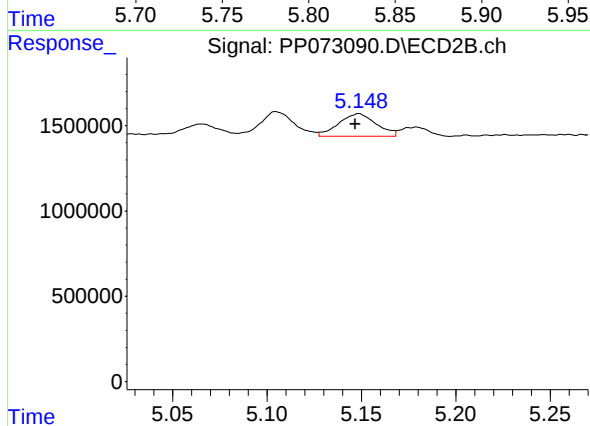

#14 AR-1232-4


R.T.: 5.149 min
Delta R.T.: 0.002 min
Response: 1839471
Conc: 85.06 ng/ml

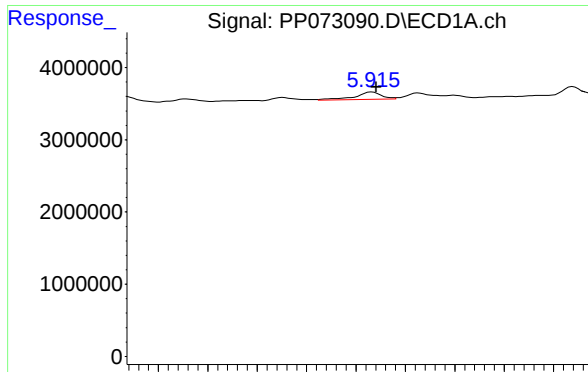

#15 AR-1232-5


R.T.: 5.916 min
Delta R.T.: -0.004 min
Response: 1851749
Conc: 51.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

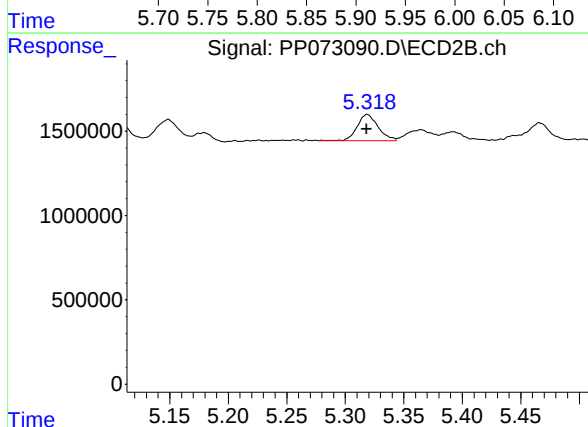


#15 AR-1232-5

R.T.: 5.319 min
Delta R.T.: 0.000 min
Response: 1935987
Conc: 84.69 ng/ml

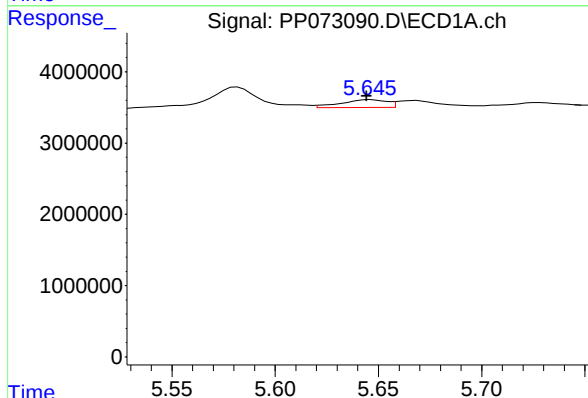


#16 AR-1242-1

R.T.: 5.646 min
Delta R.T.: 0.001 min
Response: 1691696
Conc: 28.95 ng/ml

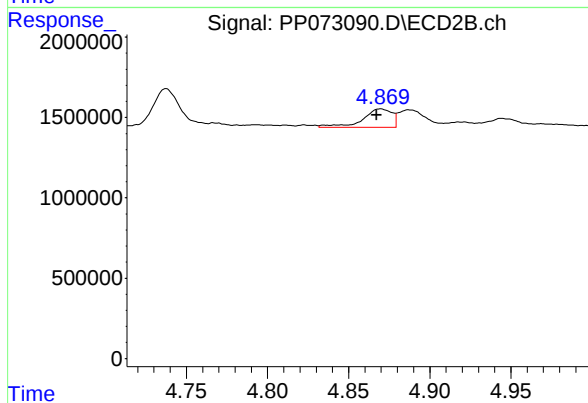

#16 AR-1242-1


R.T.: 4.870 min
Delta R.T.: 0.002 min
Response: 1418193
Conc: 25.68 ng/ml

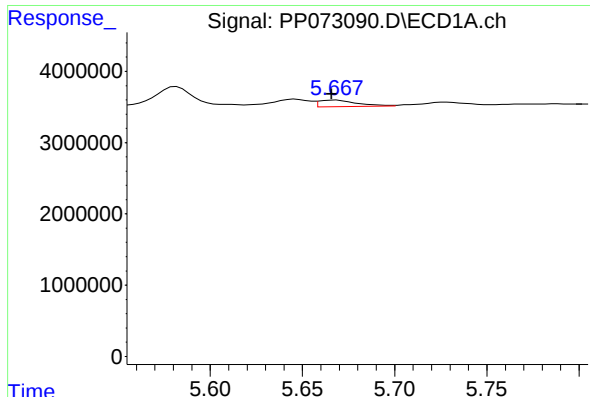

#17 AR-1242-2


R.T.: 5.669 min
Delta R.T.: 0.003 min
Response: 1342616
Conc: 15.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

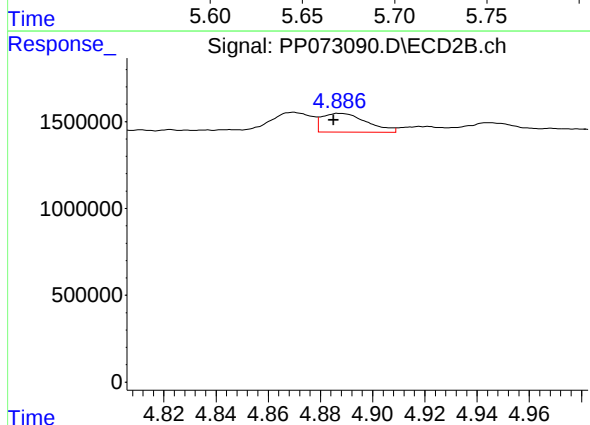


#17 AR-1242-2

R.T.: 4.887 min
Delta R.T.: 0.002 min
Response: 1284072
Conc: 16.15 ng/ml

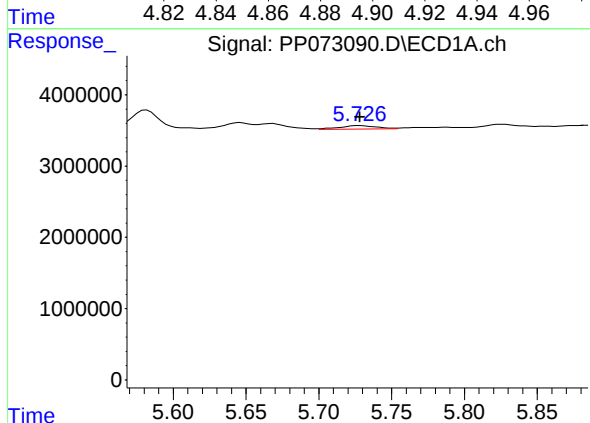


#18 AR-1242-3

R.T.: 5.728 min
Delta R.T.: 0.000 min
Response: 852004
Conc: 16.16 ng/ml

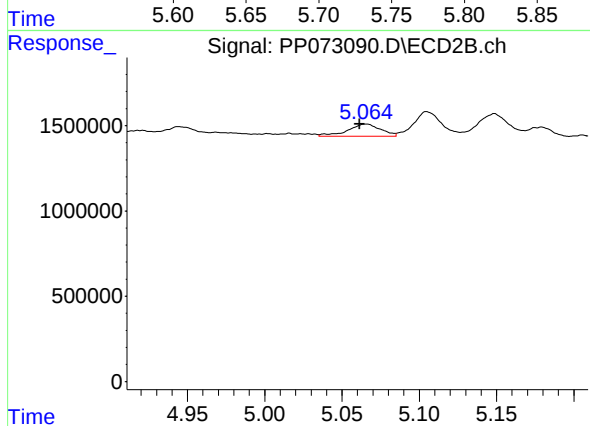

#18 AR-1242-3


R.T.: 5.065 min
Delta R.T.: 0.004 min
Response: 1058478
Conc: 24.44 ng/ml

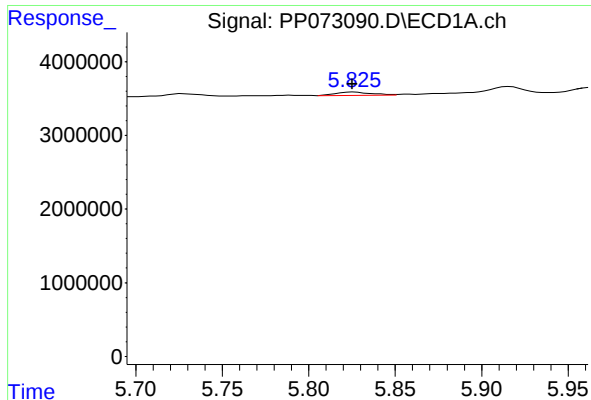

#19 AR-1242-4


R.T.: 5.826 min
Delta R.T.: 0.001 min
Response: 688031
Conc: 15.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

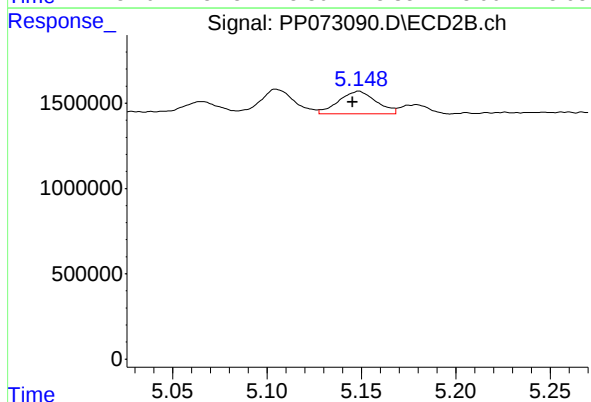


#19 AR-1242-4

R.T.: 5.149 min
Delta R.T.: 0.003 min
Response: 1839471
Conc: 44.32 ng/ml

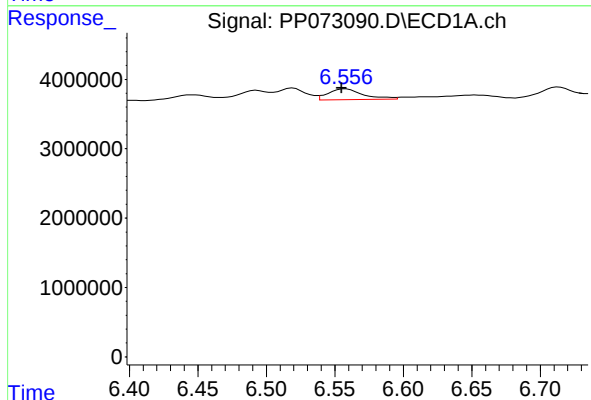


#20 AR-1242-5

R.T.: 6.558 min
Delta R.T.: 0.003 min
Response: 2836461
Conc: 57.23 ng/ml

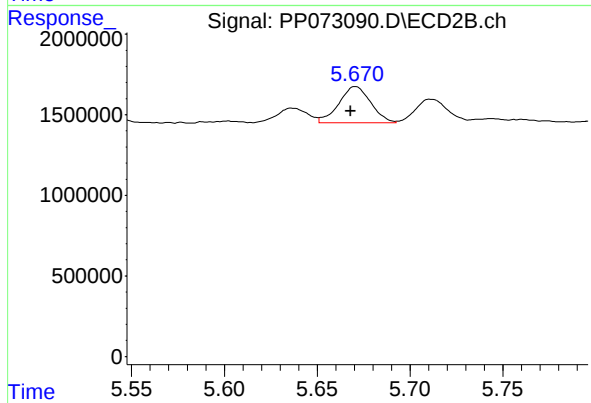

#20 AR-1242-5


R.T.: 5.671 min
Delta R.T.: 0.003 min
Response: 2696502
Conc: 51.28 ng/ml

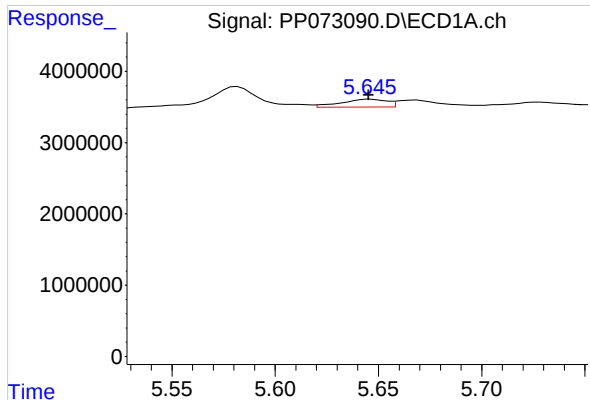

#21 AR-1248-1


R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 1691696
Conc: 35.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

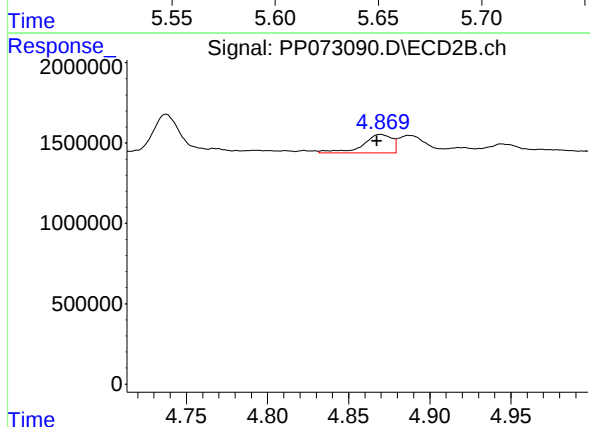


#21 AR-1248-1

R.T.: 4.870 min
Delta R.T.: 0.002 min
Response: 1418193
Conc: 32.53 ng/ml

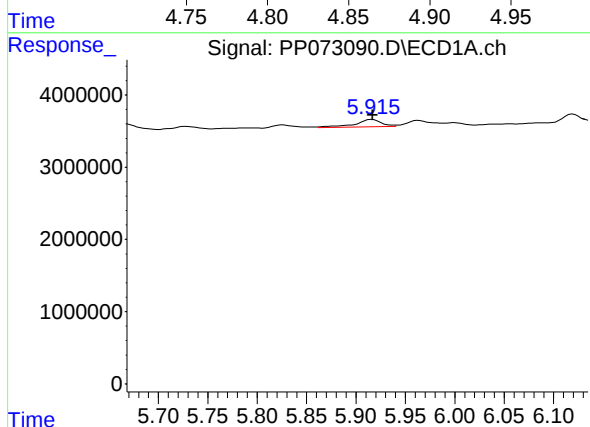


#22 AR-1248-2

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 1851749
Conc: 31.63 ng/ml

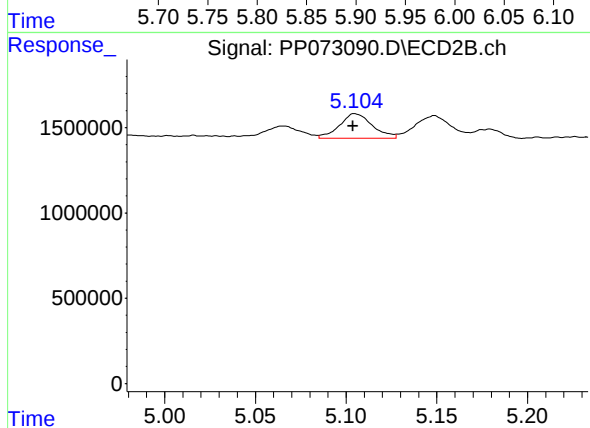

#22 AR-1248-2


R.T.: 5.105 min
Delta R.T.: 0.001 min
Response: 1816748
Conc: 31.00 ng/ml

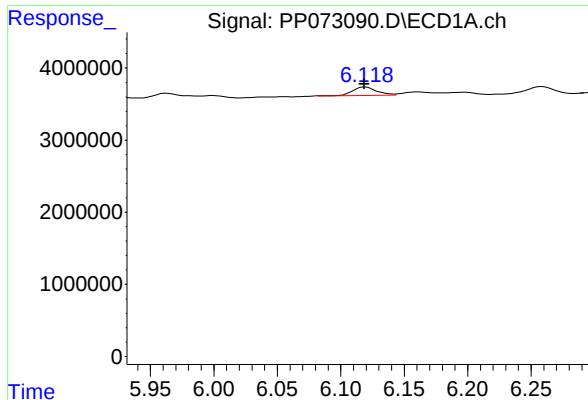

#23 AR-1248-3


R.T.: 6.120 min
Delta R.T.: 0.001 min
Response: 1566712
Conc: 24.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

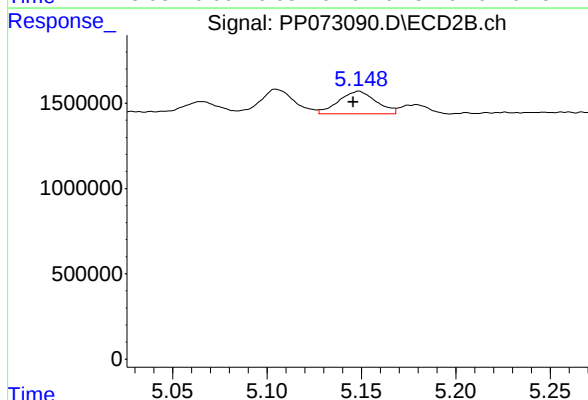


#23 AR-1248-3

R.T.: 5.149 min
Delta R.T.: 0.003 min
Response: 1839471
Conc: 30.38 ng/ml

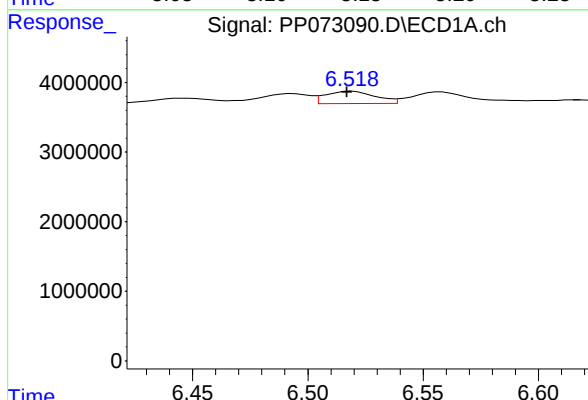


#24 AR-1248-4

R.T.: 6.519 min
Delta R.T.: 0.002 min
Response: 2652361
Conc: 31.18 ng/ml

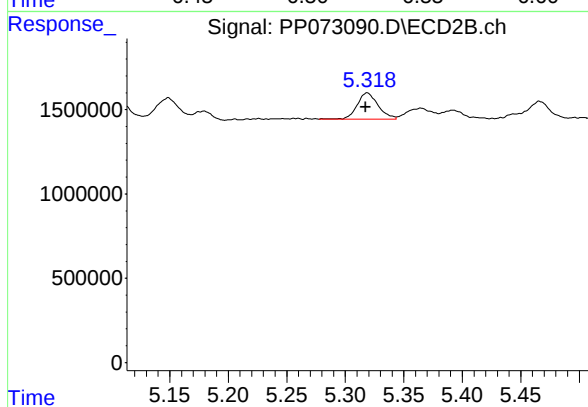

#24 AR-1248-4


R.T.: 5.319 min
Delta R.T.: 0.001 min
Response: 1935987
Conc: 27.65 ng/ml

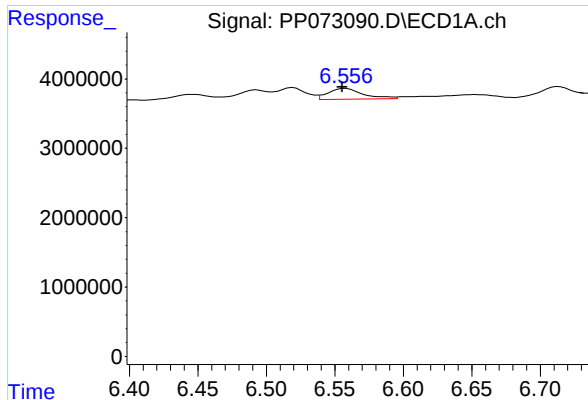

#25 AR-1248-5


R.T.: 6.558 min
Delta R.T.: 0.002 min
Response: 2836461
Conc: 33.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

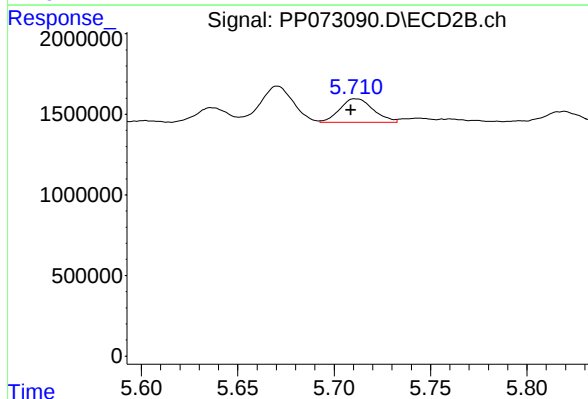


#25 AR-1248-5

R.T.: 5.711 min
Delta R.T.: 0.002 min
Response: 1769685
Conc: 24.91 ng/ml

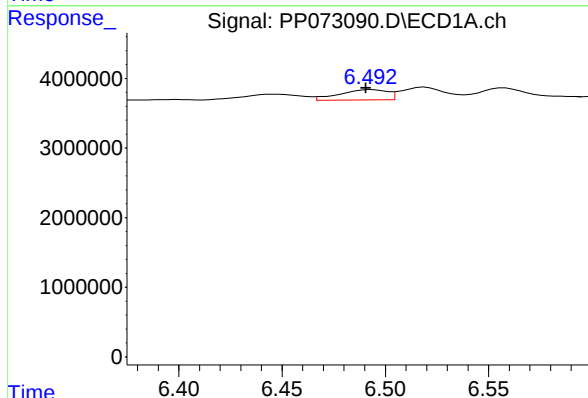


#26 AR-1254-1

R.T.: 6.493 min
Delta R.T.: 0.003 min
Response: 2375343
Conc: 28.22 ng/ml

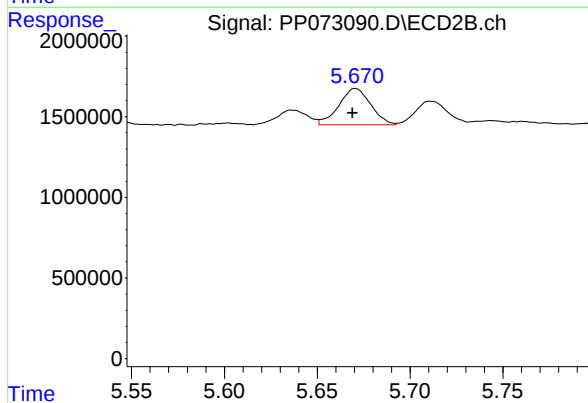

#26 AR-1254-1


R.T.: 5.671 min
Delta R.T.: 0.001 min
Response: 2696502
Conc: 24.59 ng/ml

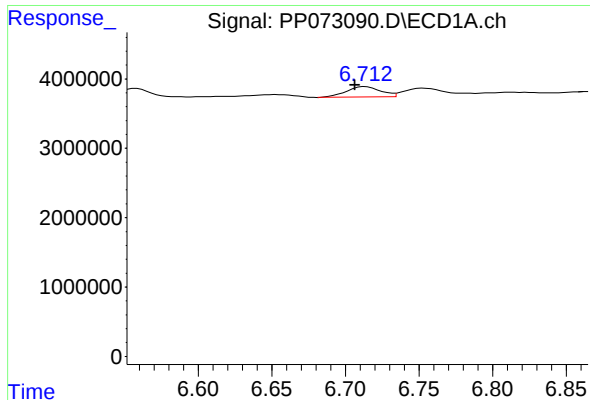

#27 AR-1254-2


R.T.: 6.713 min
Delta R.T.: 0.007 min
Response: 2447947
Conc: 19.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

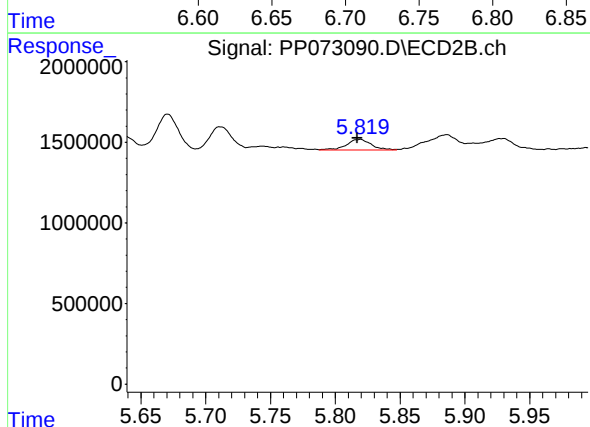


#27 AR-1254-2

R.T.: 5.819 min
Delta R.T.: 0.002 min
Response: 874929
Conc: 9.25 ng/ml

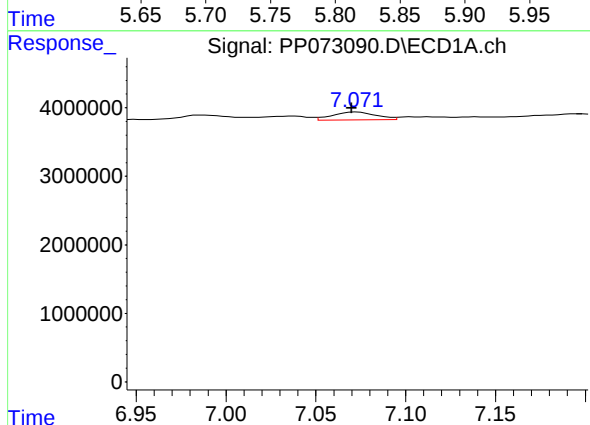


#28 AR-1254-3

R.T.: 7.073 min
Delta R.T.: 0.003 min
Response: 2002388
Conc: 15.26 ng/ml

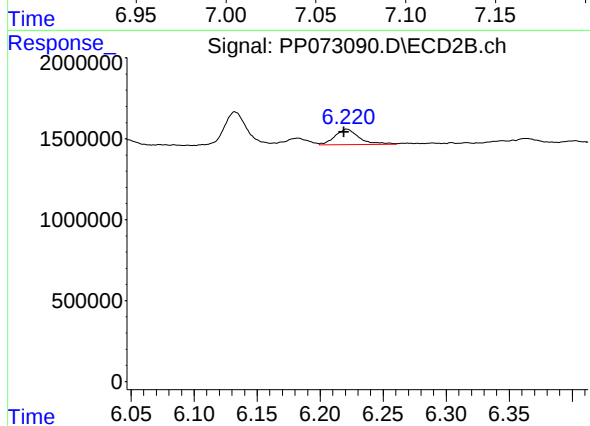

#28 AR-1254-3


R.T.: 6.221 min
Delta R.T.: 0.002 min
Response: 1259233
Conc: 8.53 ng/ml

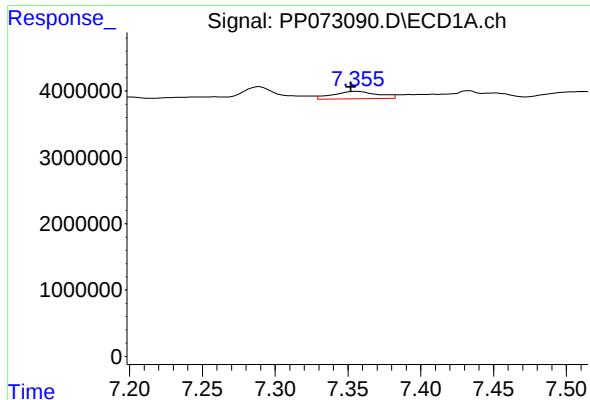

#29 AR-1254-4


R.T.: 7.357 min
Delta R.T.: 0.005 min
Response: 2338051
Conc: 19.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

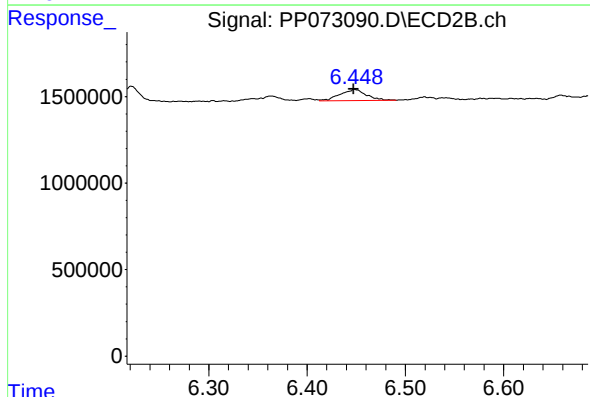


#29 AR-1254-4

R.T.: 6.448 min
Delta R.T.: 0.001 min
Response: 1230375
Conc: 12.67 ng/ml

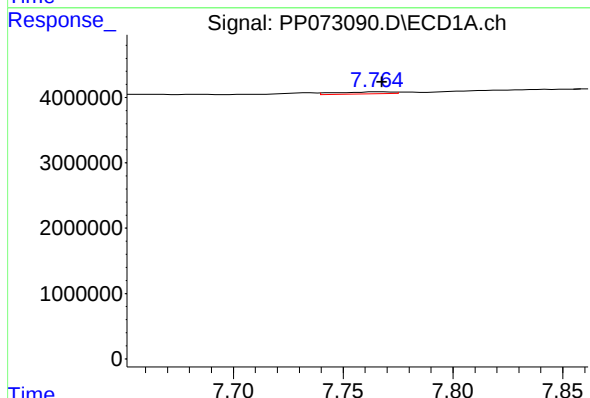


#30 AR-1254-5

R.T.: 7.766 min
Delta R.T.: -0.002 min
Response: 540872
Conc: 4.73 ng/ml

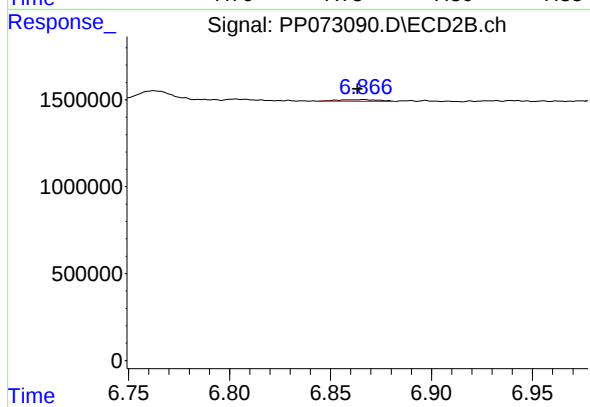

#30 AR-1254-5


R.T.: 6.867 min
Delta R.T.: 0.003 min
Response: 143911
Conc: 1.11 ng/ml

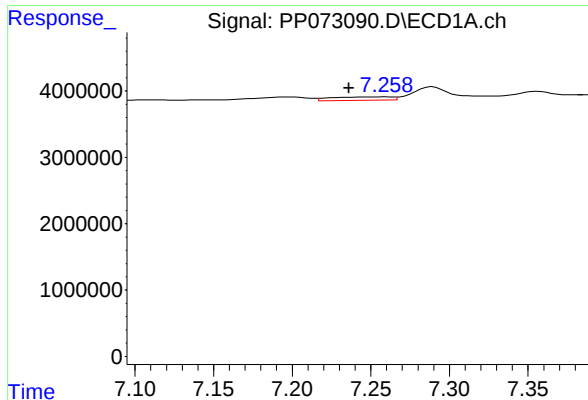

#31 AR-1260-1


R.T.: 7.260 min
Delta R.T.: 0.024 min
Response: 1393818
Conc: 15.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

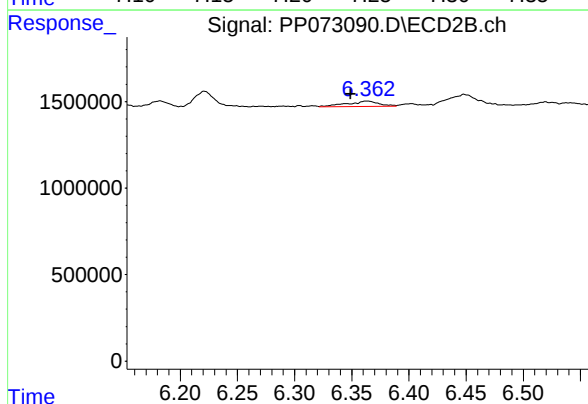


#31 AR-1260-1

R.T.: 6.363 min
Delta R.T.: 0.014 min
Response: 598692
Conc: 6.32 ng/ml

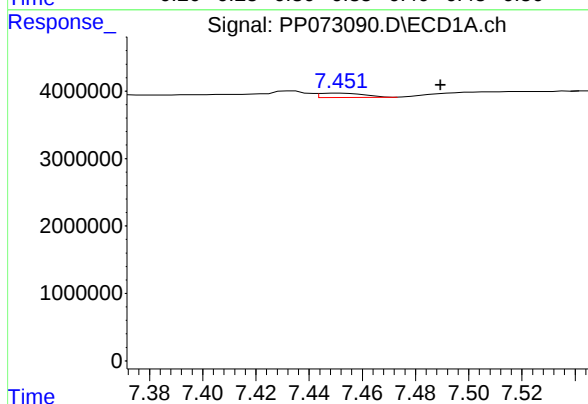


#32 AR-1260-2

R.T.: 7.452 min
Delta R.T.: -0.038 min
Response: 731588
Conc: 5.38 ng/ml

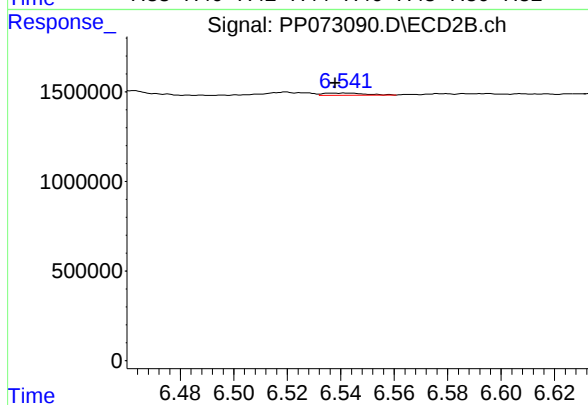

#32 AR-1260-2


R.T.: 6.537 min
Delta R.T.: 0.000 min
Response: 125989
Conc: 1.08 ng/ml

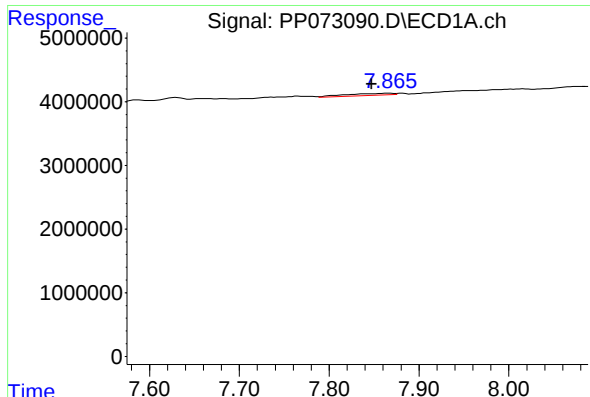

#33 AR-1260-3


R.T.: 7.867 min
Delta R.T.: 0.019 min
Response: 1205536
Conc: 10.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

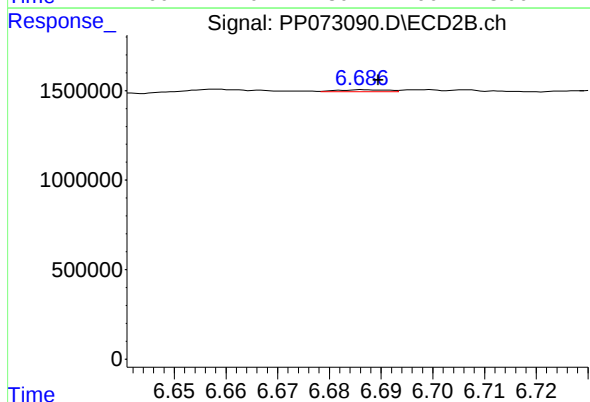


#33 AR-1260-3

R.T.: 6.687 min
Delta R.T.: -0.003 min
Response: 75252
Conc: 0.72 ng/ml

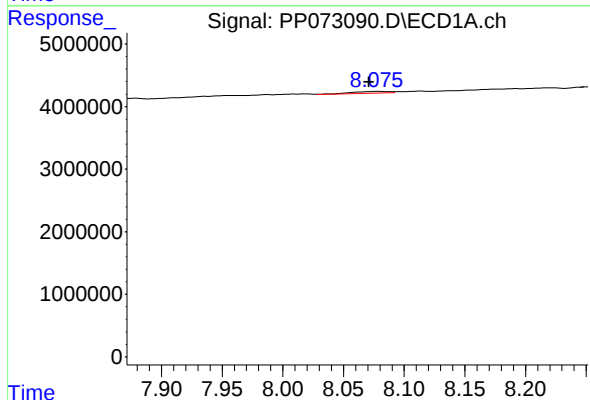


#34 AR-1260-4

R.T.: 8.079 min
Delta R.T.: 0.007 min
Response: 663107
Conc: 6.44 ng/ml

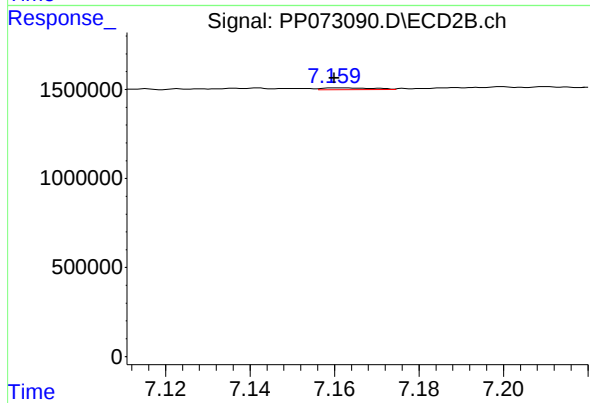

#34 AR-1260-4


R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 86708
Conc: 0.99 ng/ml

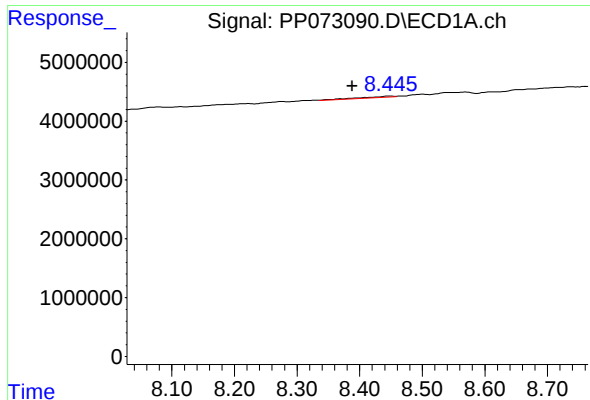

#35 AR-1260-5


R.T.: 8.448 min
Delta R.T.: 0.060 min
Response: 740558
Conc: 3.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

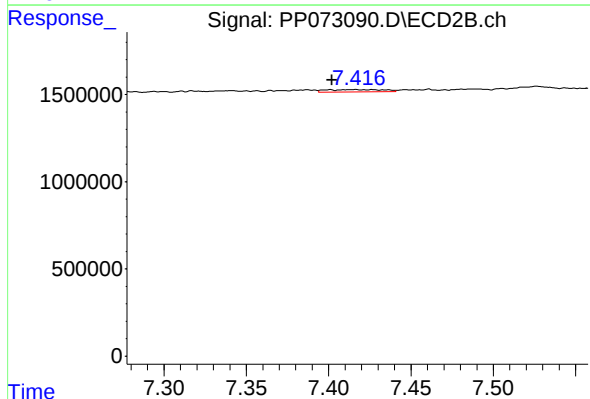


#35 AR-1260-5

R.T.: 7.416 min
Delta R.T.: 0.014 min
Response: 321672
Conc: 1.51 ng/ml

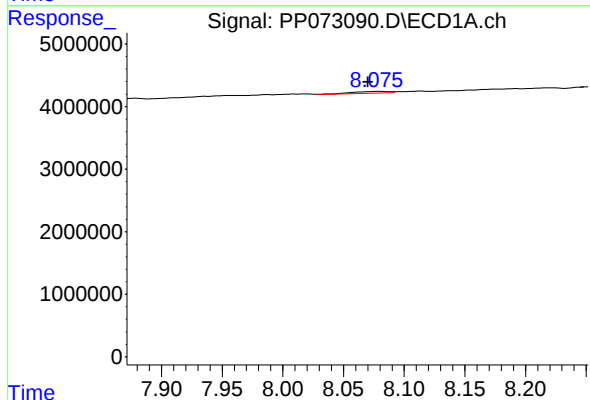


#36 AR-1262-1

R.T.: 8.079 min
Delta R.T.: 0.008 min
Response: 663107
Conc: 4.48 ng/ml

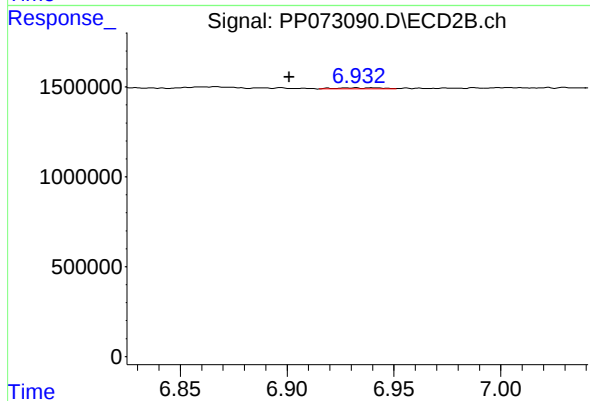

#36 AR-1262-1


R.T.: 6.932 min
Delta R.T.: 0.031 min
Response: 83476
Conc: 0.58 ng/ml

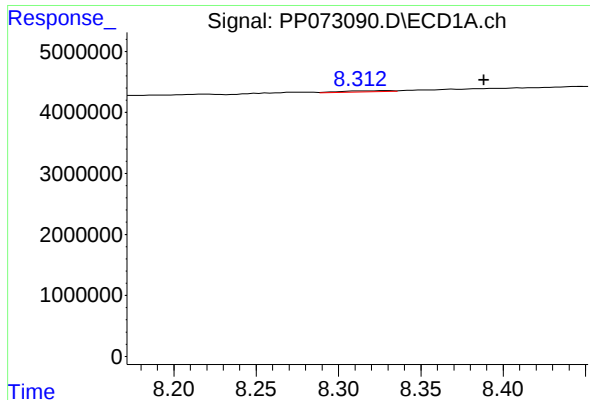

#37 AR-1262-2


R.T.: 8.329 min
Delta R.T.: -0.059 min
Response: 299146
Conc: 0.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

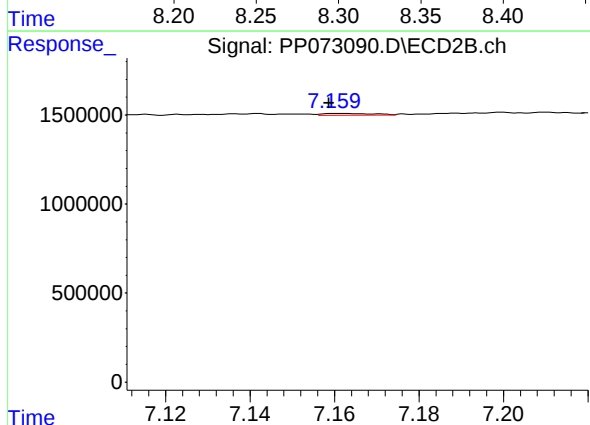


#37 AR-1262-2

R.T.: 7.161 min
Delta R.T.: 0.002 min
Response: 86708
Conc: 0.71 ng/ml

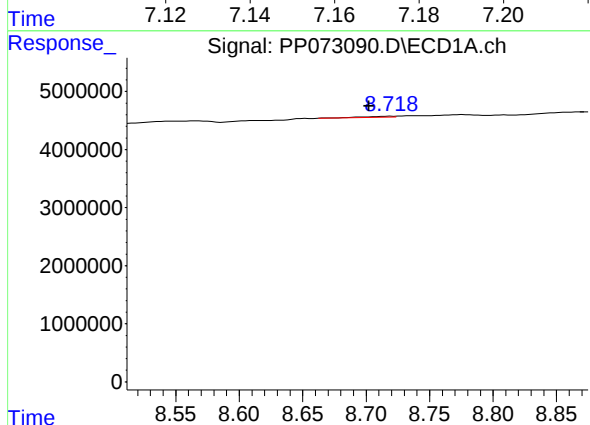


#38 AR-1262-3

R.T.: 8.719 min
Delta R.T.: 0.017 min
Response: 320464
Conc: 1.50 ng/ml

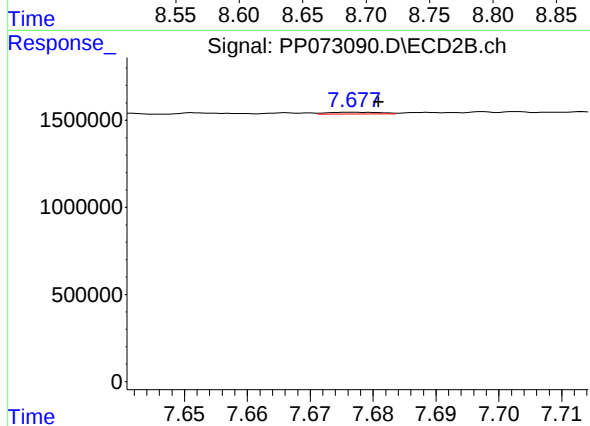

#38 AR-1262-3


R.T.: 7.677 min
Delta R.T.: -0.004 min
Response: 58284
Conc: 0.52 ng/ml

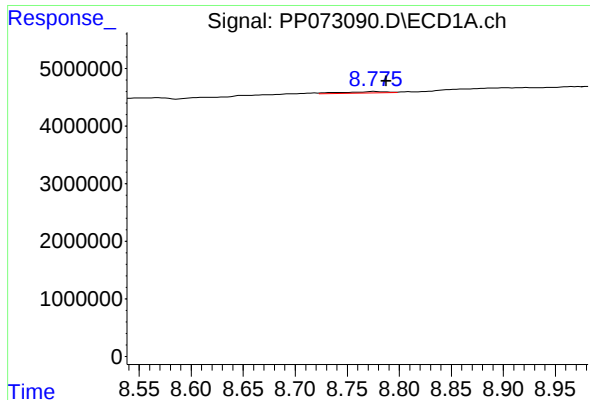

#39 AR-1262-4


R.T.: 8.776 min
Delta R.T.: -0.012 min
Response: 739791
Conc: 4.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

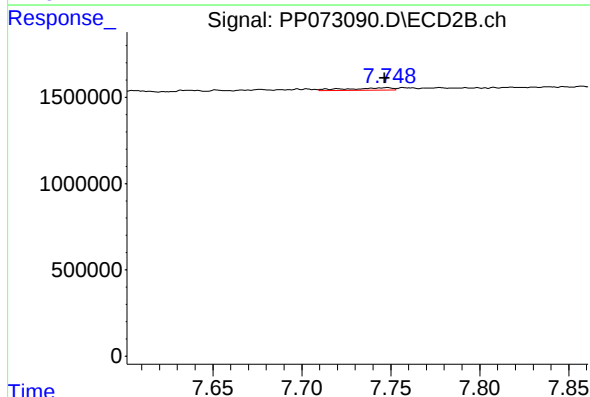


#39 AR-1262-4

R.T.: 7.748 min
Delta R.T.: 0.001 min
Response: 235168
Conc: 1.28 ng/ml

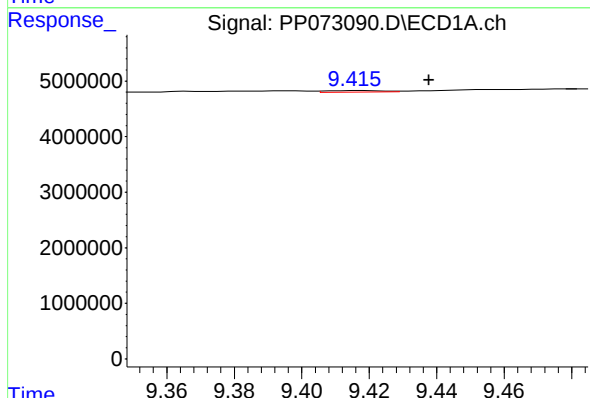


#40 AR-1262-5

R.T.: 9.418 min
Delta R.T.: -0.020 min
Response: 306036
Conc: 2.74 ng/ml

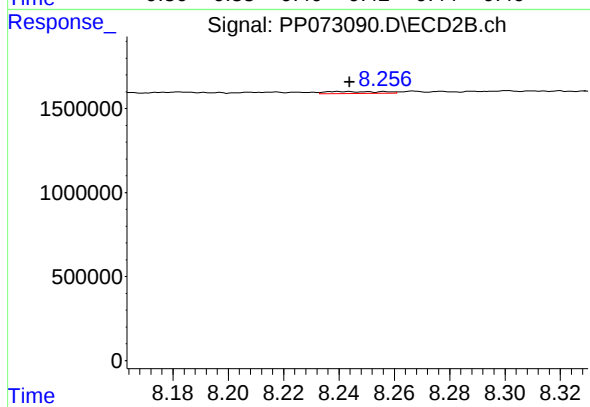

#40 AR-1262-5


R.T.: 8.240 min
Delta R.T.: -0.004 min
Response: 168891
Conc: 1.95 ng/ml

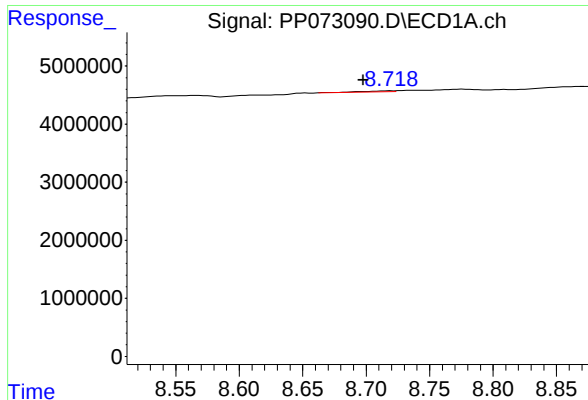

#41 AR-1268-1


R.T.: 8.719 min
Delta R.T.: 0.021 min
Response: 320464
Conc: 0.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

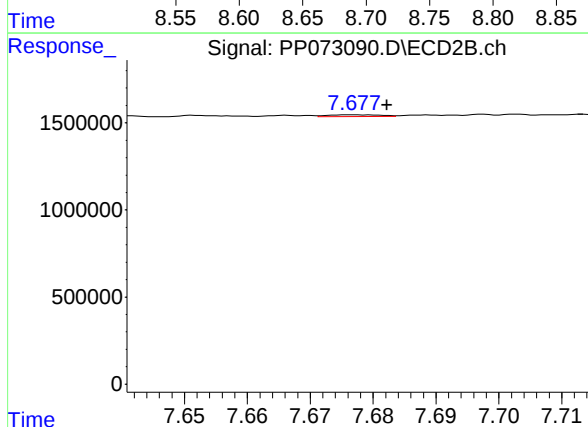


#41 AR-1268-1

R.T.: 7.677 min
Delta R.T.: -0.005 min
Response: 58284
Conc: 0.20 ng/ml

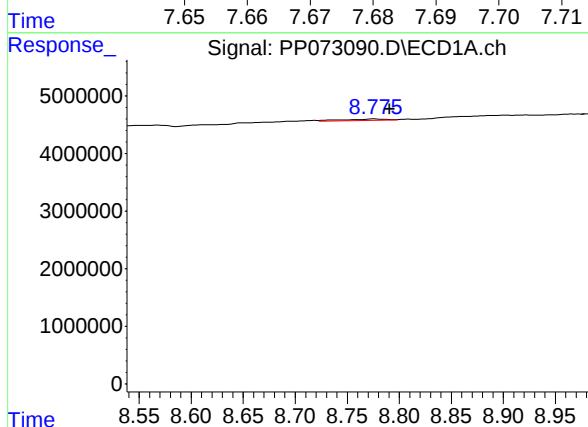


#42 AR-1268-2

R.T.: 8.776 min
Delta R.T.: -0.015 min
Response: 739791
Conc: 2.43 ng/ml

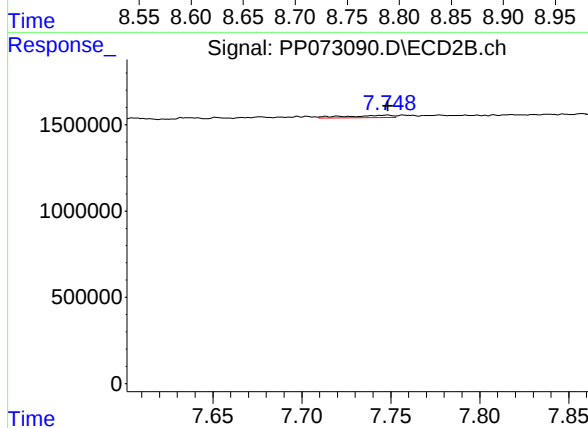

#42 AR-1268-2


R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 235168
Conc: 0.91 ng/ml

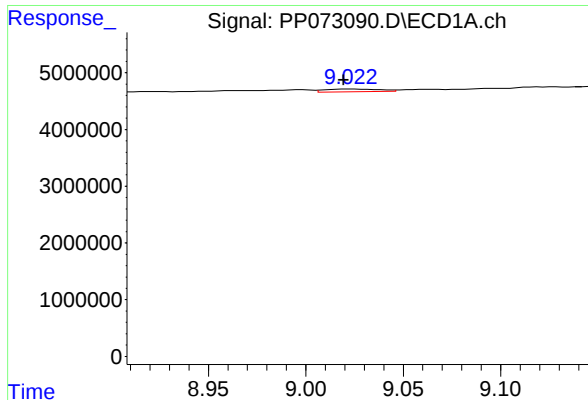

#43 AR-1268-3


R.T.: 9.024 min
Delta R.T.: 0.005 min
Response: 938913
Conc: 3.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

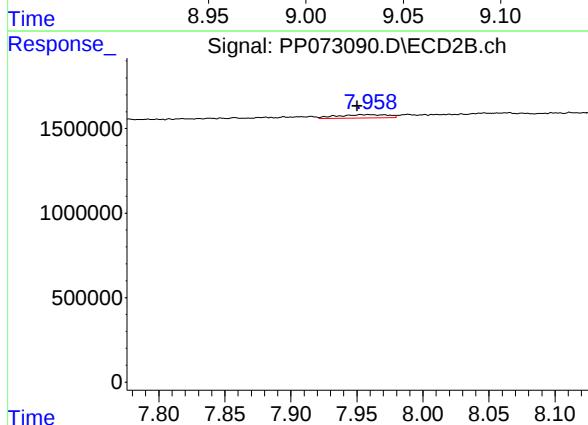


#43 AR-1268-3

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 551104
Conc: 2.55 ng/ml

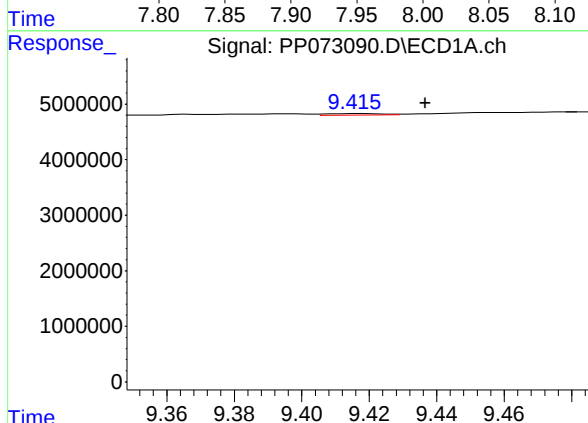


#44 AR-1268-4

R.T.: 9.418 min
Delta R.T.: -0.019 min
Response: 306036
Conc: 2.62 ng/ml

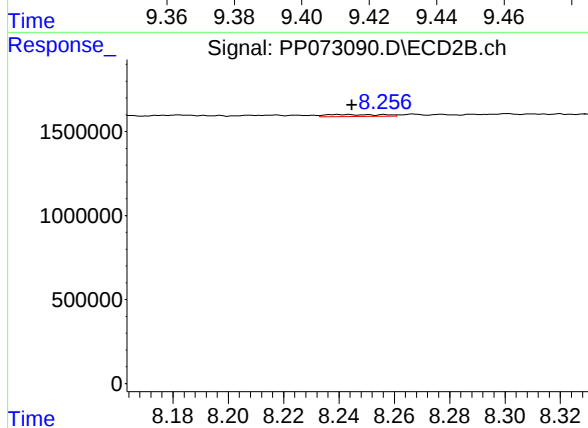

#44 AR-1268-4


R.T.: 8.240 min
Delta R.T.: -0.005 min
Response: 168891
Conc: 1.79 ng/ml

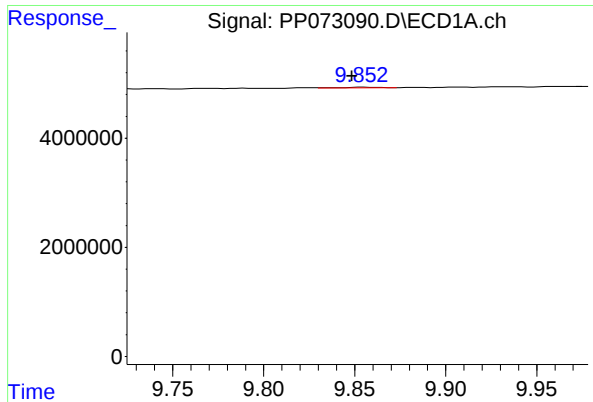

#45 AR-1268-5

R.T.: 9.854 min
Delta R.T.: 0.005 min
Response: 209178
Conc: 0.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

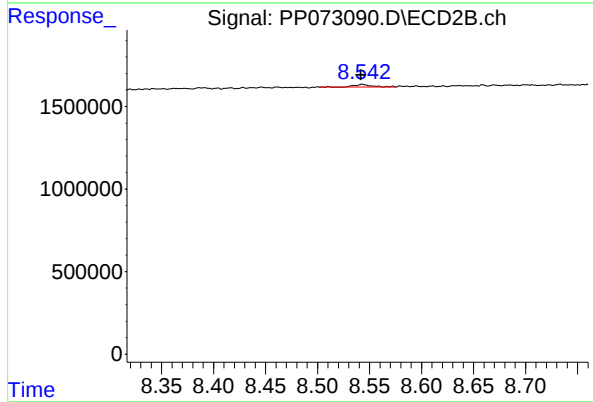

#45 AR-1268-5

R.T.: 8.543 min
Delta R.T.: 0.001 min
Response: 157294
Conc: 0.27 ng/ml