

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 18:27
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:28:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.495	3.790	40951604	34791832	19.401	19.310
2) SA Decachlor...	10.191	8.800	38039159	28394580	22.260	21.274
Target Compounds						
3) L1 AR-1016-1	5.647	4.872	243980	159486	3.357	2.321 #
4) L1 AR-1016-2	5.681	4.886	553327	220387	5.319	2.190 #
5) L1 AR-1016-3	5.739	5.064	309939	113274	4.743	2.070 #
6) L1 AR-1016-4	5.836	5.112	155384	141861	2.972	3.184
7) L1 AR-1016-5	6.127	5.309	255924	81961	5.118	1.483 #
8) L2 AR-1221-1	4.685	3.975	50967	203966	2.067	7.590 #
9) L2 AR-1221-2	4.770	4.091	30862	760498	1.529	37.676 #
10) L2 AR-1221-3	4.851	4.162	305878	60122	4.969	1.024 #
11) L3 AR-1232-1	4.851	4.162	305878	60122	6.514	1.319 #
12) L3 AR-1232-2	5.381	4.886	106600	220387	4.765	4.764
13) L3 AR-1232-3	5.681	5.064	553327	113274	10.724	4.613 #
14) L3 AR-1232-4	5.836	5.156	155384	106860	6.020	4.941
15) L3 AR-1232-5	5.916	5.309	307020	81961	8.607	3.586 #
16) L4 AR-1242-1	5.647	4.872	243980	159486	4.175	2.888 #
17) L4 AR-1242-2	5.681	4.886	553327	220387	6.393	2.773 #
18) L4 AR-1242-3	5.739	5.064	309939	113274	5.880	2.616 #
19) L4 AR-1242-4	5.836	5.156	155384	106860	3.535	2.575 #
20) L4 AR-1242-5	6.565	5.672	371037	504446	7.487	9.593 #
21) L5 AR-1248-1	5.647	4.872	243980	159486	5.129	3.659 #
22) L5 AR-1248-2	5.916	5.112	307020	141861	5.244	2.421 #
23) L5 AR-1248-3	6.127	5.156	255924	106860	3.922	1.765 #
24) L5 AR-1248-4	6.530	5.309	231379	81961	2.720	1.171 #
25) L5 AR-1248-5	6.565	5.724	371037	168269	4.433	2.369 #
26) L6 AR-1254-1	6.497	5.672	965870	504446	11.475	4.601 #
27) L6 AR-1254-2	6.710	5.820	790446	630654	6.303	6.670
28) L6 AR-1254-3	7.072	6.203	639717	373606	4.875	2.532 #
29) L6 AR-1254-4	7.363	6.478	287765	955989	2.402	9.845 #
30) L6 AR-1254-5	7.768	6.865	2099402	1690783	18.374	13.010 #
31) L7 AR-1260-1	7.238	6.351	1694610	1996354	19.210	21.074
32) L7 AR-1260-2	7.491	6.540	2964006	2525199	21.813	21.687
33) L7 AR-1260-3	7.849	6.694	4197931	2509204	36.775	24.090 #
34) L7 AR-1260-4	8.073	7.161	2966917	2871292	28.792	32.726
35) L7 AR-1260-5	8.390	7.404	6265402	5641387	26.038	26.436
36) L8 AR-1262-1	8.073	6.903	2966917	3419463	20.044	23.670
37) L8 AR-1262-2	8.390	7.161	6265402	2871292	19.798	23.491
38) L8 AR-1262-3	8.706	7.684	4694814	2452693	21.941	21.762
39) L8 AR-1262-4	8.786	7.749	3997119	4166415	25.364	22.723
40) L8 AR-1262-5	9.444	8.247	3428467	2063226	30.649	23.829
41) L9 AR-1268-1	8.706	7.684	4694814	2452693	13.128	8.538 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 18:27
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:28:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.786	7.749	3997119	4166415	13.103	16.204
43) L9	AR-1268-3	9.024	7.953	2225720	413629	8.383	1.915 #
44) L9	AR-1268-4	9.444	8.247	3428467	2063226	29.297	21.906 #
45) L9	AR-1268-5	9.856	8.544	883760	744504	1.195	1.286



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
Data File : PP073092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 18:27
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1262 MDL 25 PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:28:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

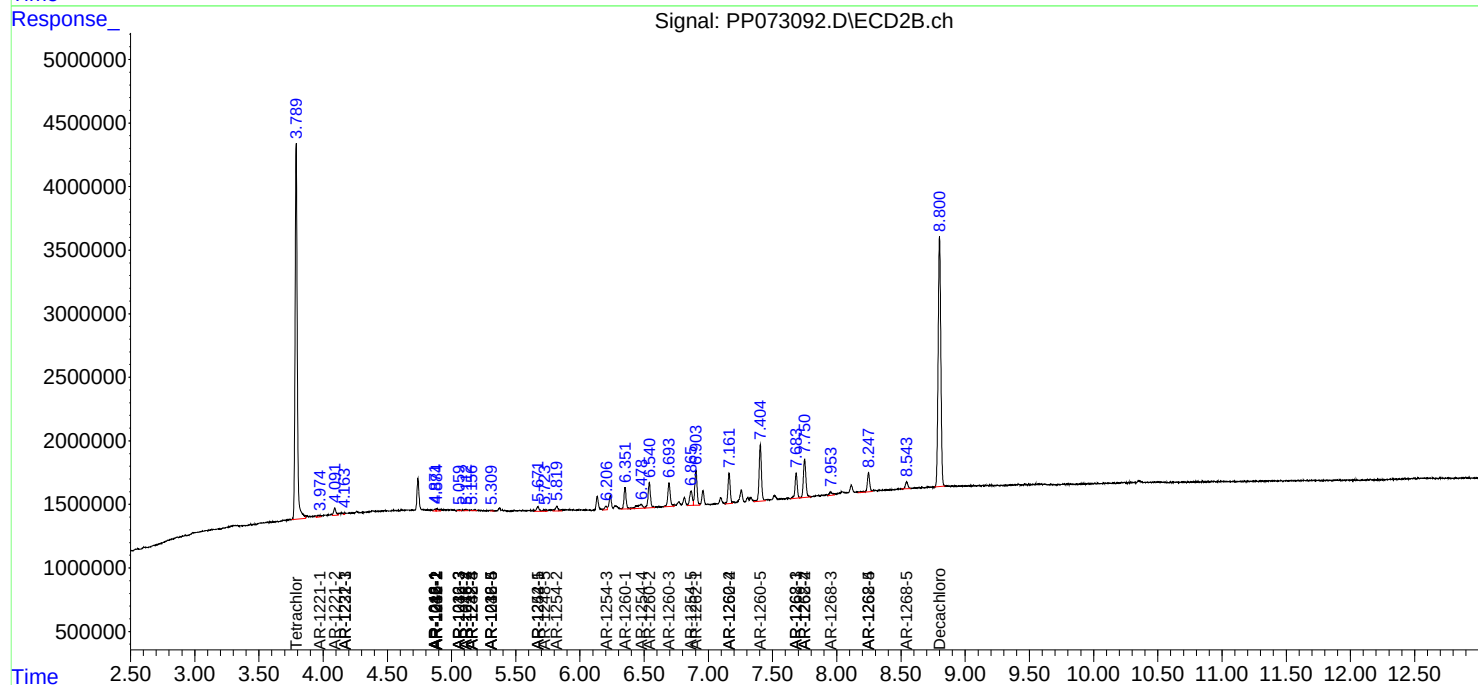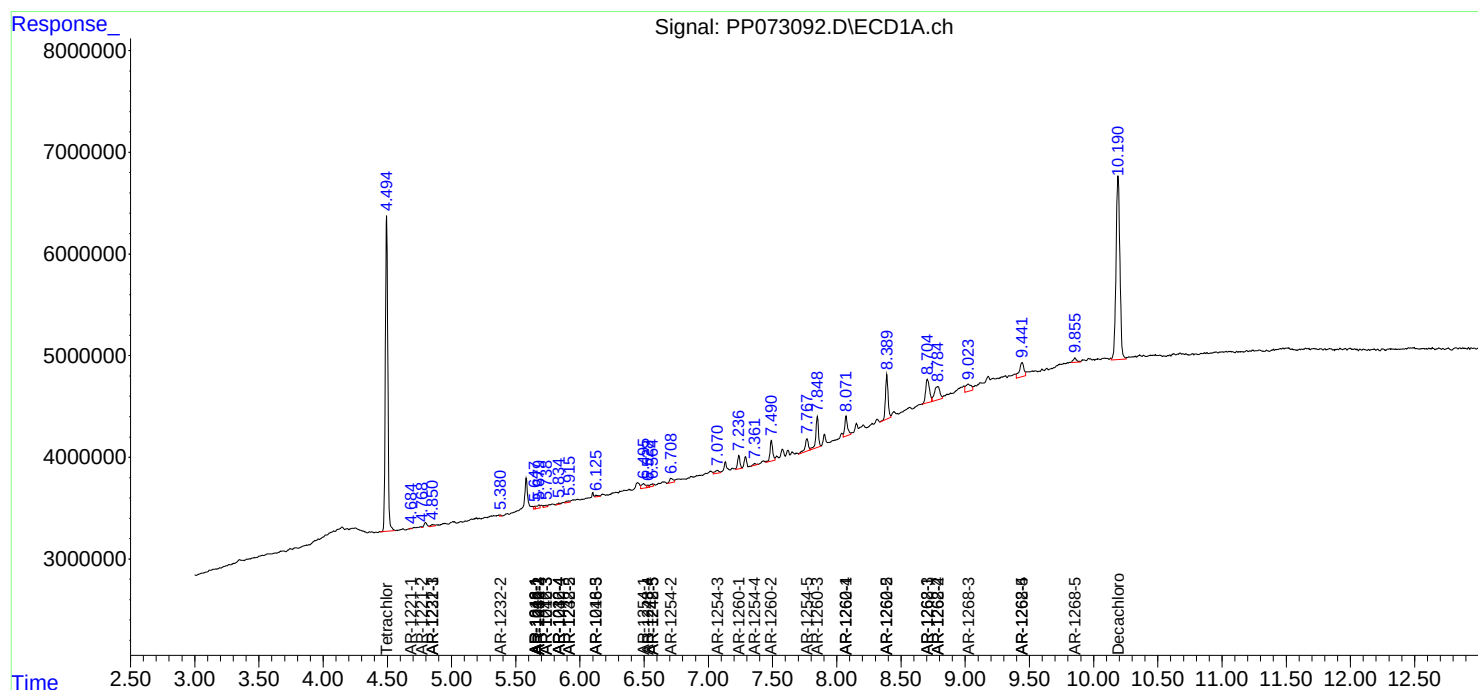


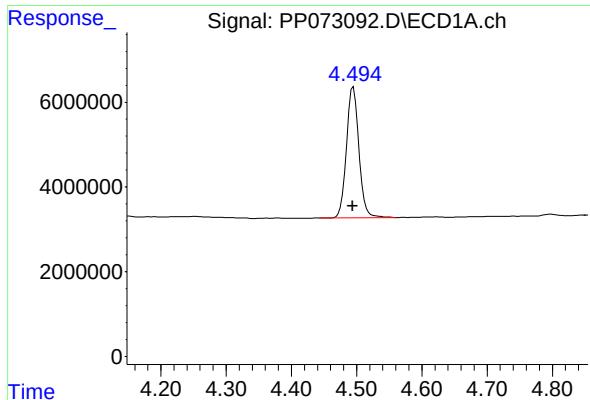

#1 Tetrachloro-m-xylene


R.T.: 4.495 min
Delta R.T.: 0.000 min
Response: 40951604
Conc: 19.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

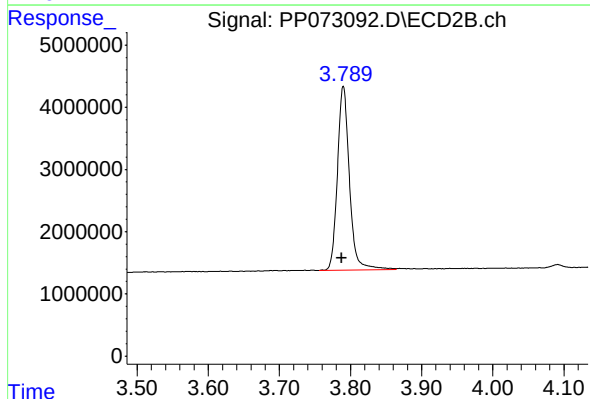


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.002 min
Response: 34791832
Conc: 19.31 ng/ml

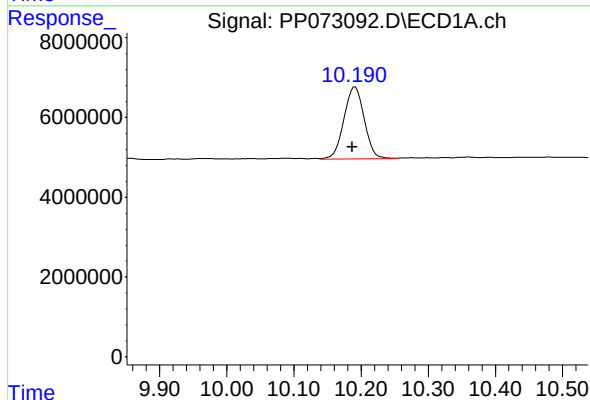


#2 Decachlorobiphenyl

R.T.: 10.191 min
Delta R.T.: 0.004 min
Response: 38039159
Conc: 22.26 ng/ml

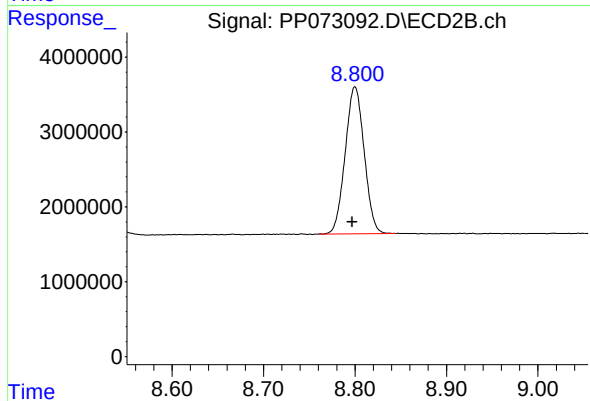

#2 Decachlorobiphenyl


R.T.: 8.800 min
Delta R.T.: 0.003 min
Response: 28394580
Conc: 21.27 ng/ml

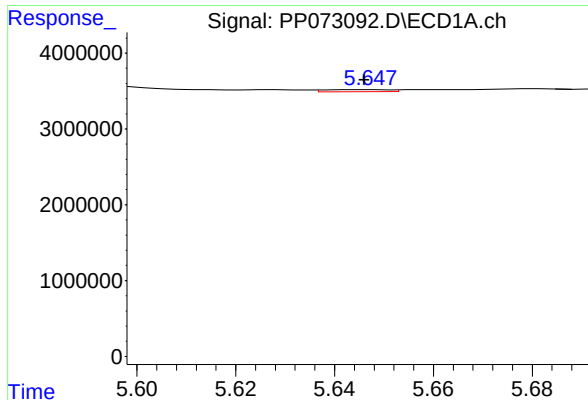

#3 AR-1016-1


R.T.: 5.647 min
Delta R.T.: 0.001 min
Response: 243980
Conc: 3.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

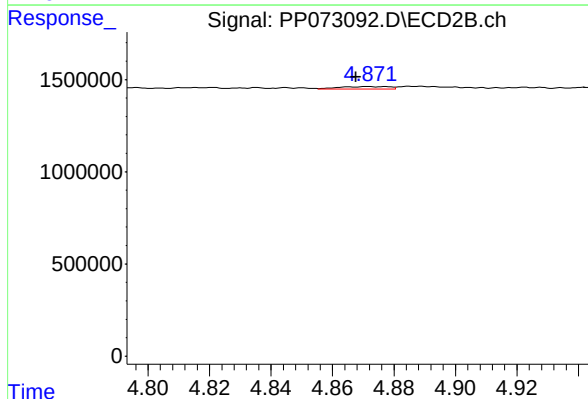


#3 AR-1016-1

R.T.: 4.872 min
Delta R.T.: 0.004 min
Response: 159486
Conc: 2.32 ng/ml

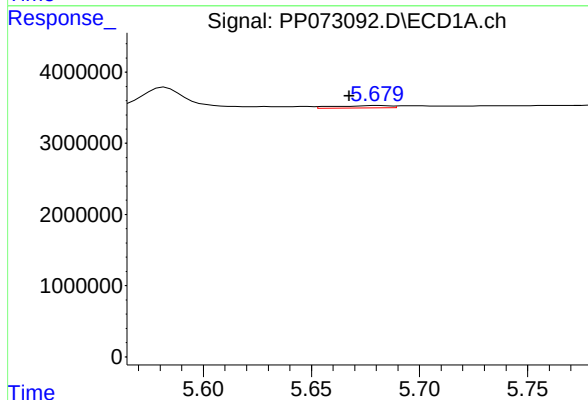


#4 AR-1016-2

R.T.: 5.681 min
Delta R.T.: 0.013 min
Response: 553327
Conc: 5.32 ng/ml

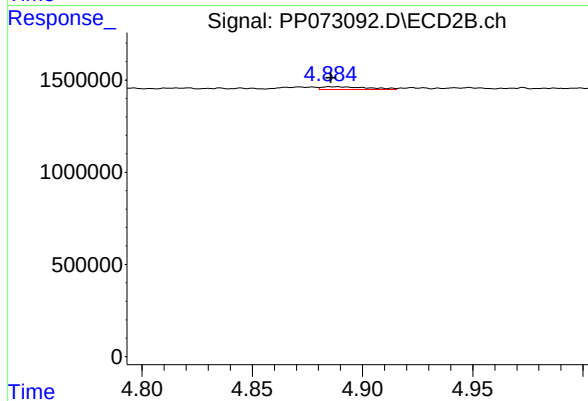

#4 AR-1016-2


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 220387
Conc: 2.19 ng/ml

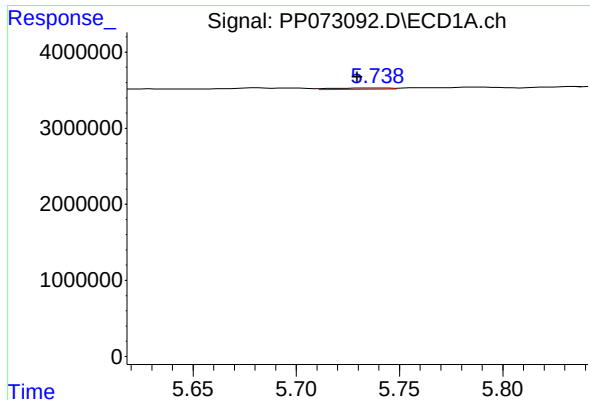

#5 AR-1016-3


R.T.: 5.739 min
Delta R.T.: 0.010 min
Response: 309939
Conc: 4.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

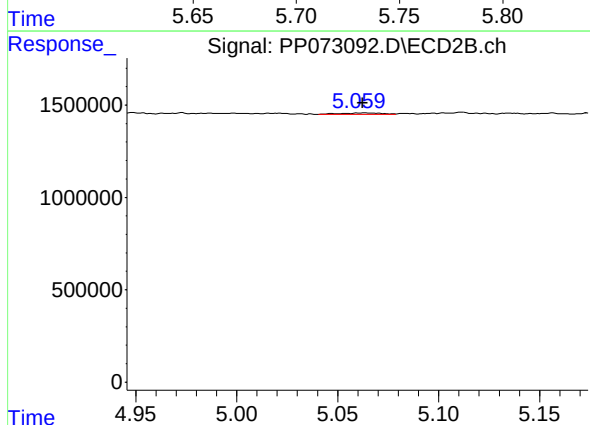


#5 AR-1016-3

R.T.: 5.064 min
Delta R.T.: 0.001 min
Response: 113274
Conc: 2.07 ng/ml

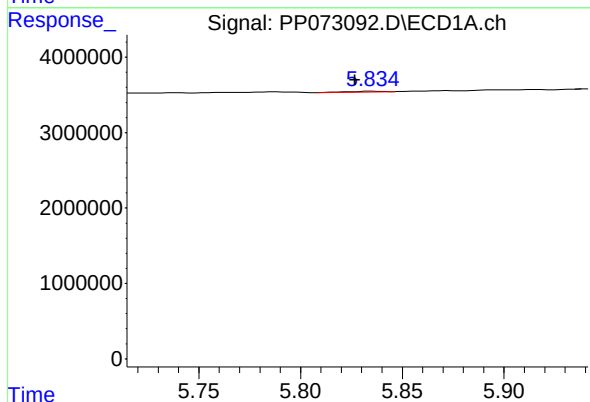


#6 AR-1016-4

R.T.: 5.836 min
Delta R.T.: 0.009 min
Response: 155384
Conc: 2.97 ng/ml

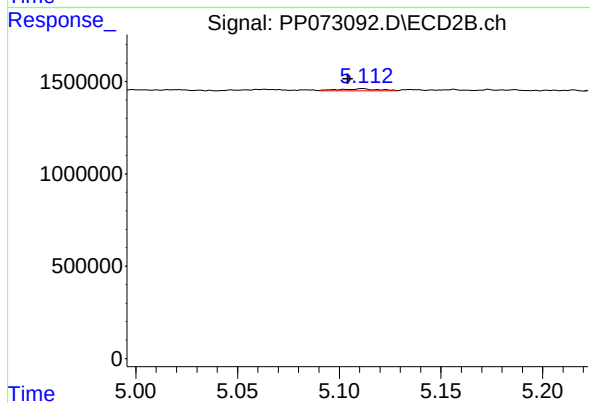

#6 AR-1016-4


R.T.: 5.112 min
Delta R.T.: 0.007 min
Response: 141861
Conc: 3.18 ng/ml

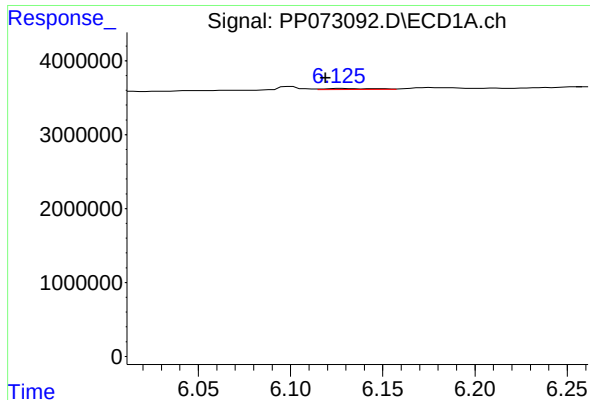

#7 AR-1016-5


R.T.: 6.127 min
Delta R.T.: 0.008 min
Response: 255924
Conc: 5.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

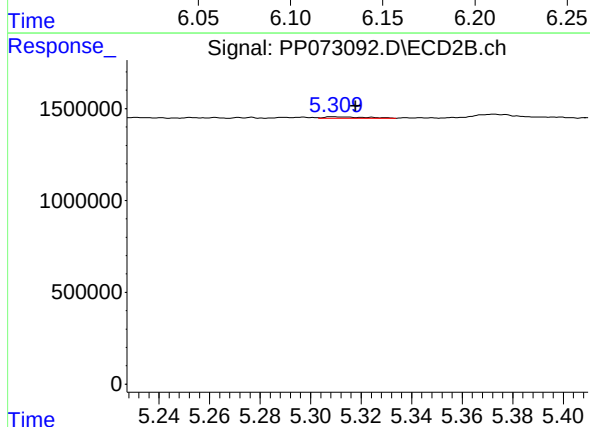


#7 AR-1016-5

R.T.: 5.309 min
Delta R.T.: -0.009 min
Response: 81961
Conc: 1.48 ng/ml

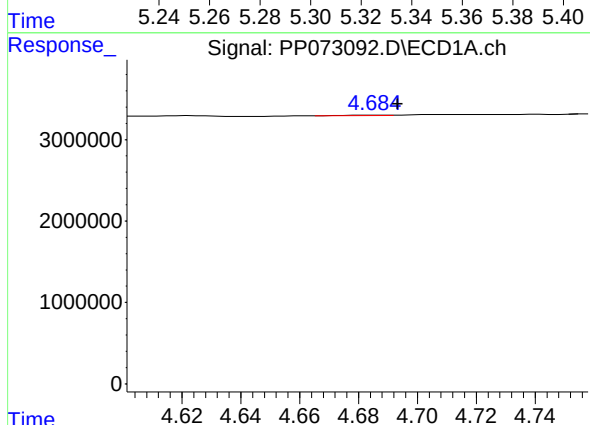


#8 AR-1221-1

R.T.: 4.685 min
Delta R.T.: -0.008 min
Response: 50967
Conc: 2.07 ng/ml

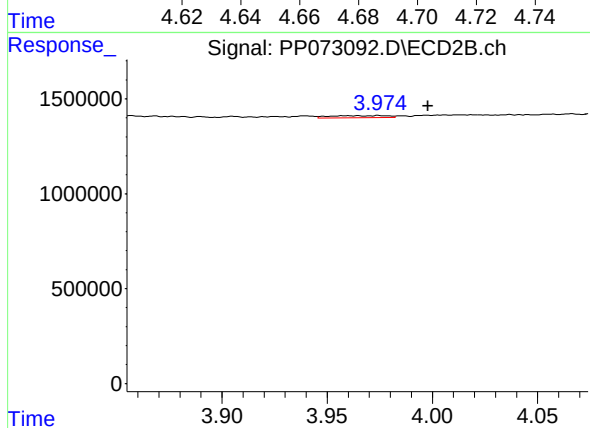

#8 AR-1221-1


R.T.: 3.975 min
Delta R.T.: -0.023 min
Response: 203966
Conc: 7.59 ng/ml

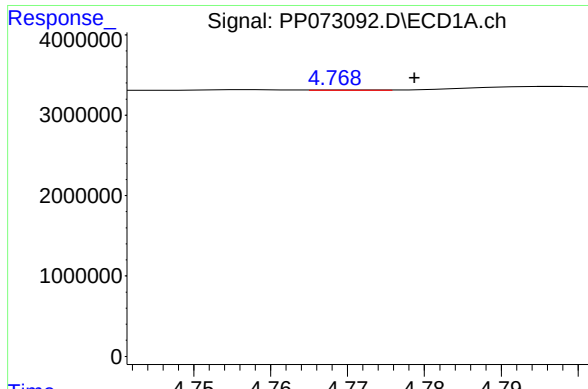

#9 AR-1221-2


R.T.: 4.770 min
Delta R.T.: -0.009 min
Response: 30862
Conc: 1.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

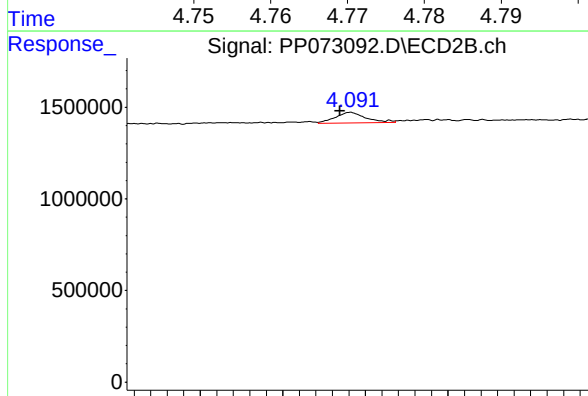


#9 AR-1221-2

R.T.: 4.091 min
Delta R.T.: 0.006 min
Response: 760498
Conc: 37.68 ng/ml

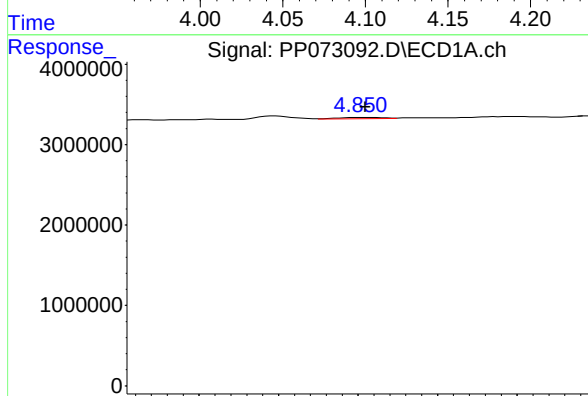


#10 AR-1221-3

R.T.: 4.851 min
Delta R.T.: -0.004 min
Response: 305878
Conc: 4.97 ng/ml

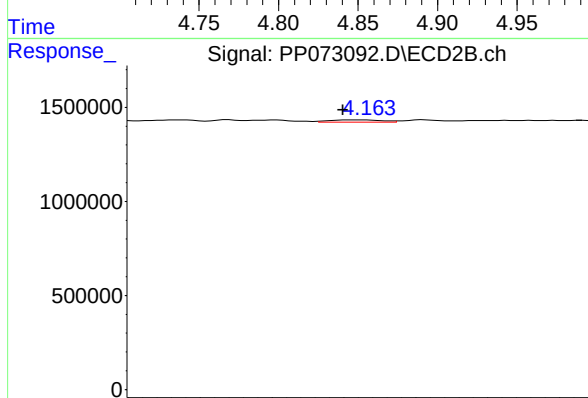

#10 AR-1221-3


R.T.: 4.162 min
Delta R.T.: 0.002 min
Response: 60122
Conc: 1.02 ng/ml

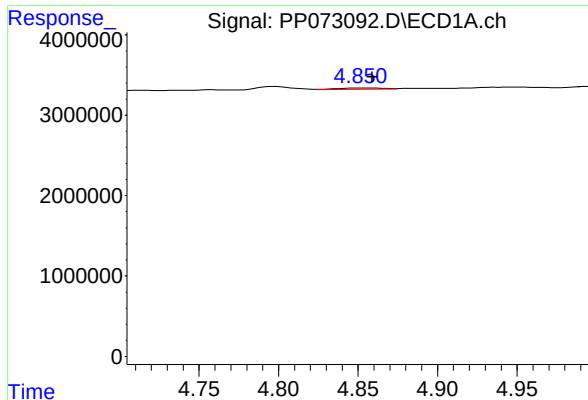

#11 AR-1232-1


R.T.: 4.851 min
Delta R.T.: -0.008 min
Response: 305878
Conc: 6.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

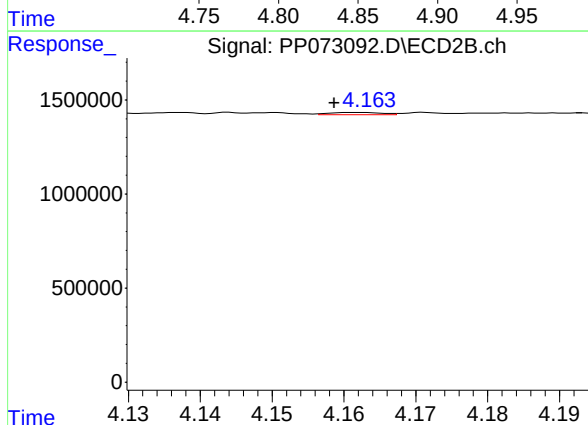


#11 AR-1232-1

R.T.: 4.162 min
Delta R.T.: 0.003 min
Response: 60122
Conc: 1.32 ng/ml

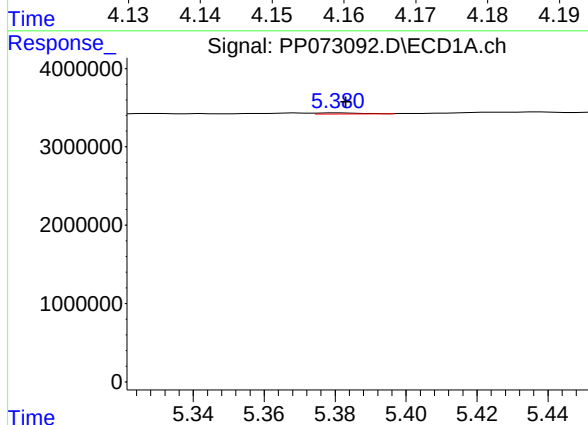


#12 AR-1232-2

R.T.: 5.381 min
Delta R.T.: -0.002 min
Response: 106600
Conc: 4.77 ng/ml

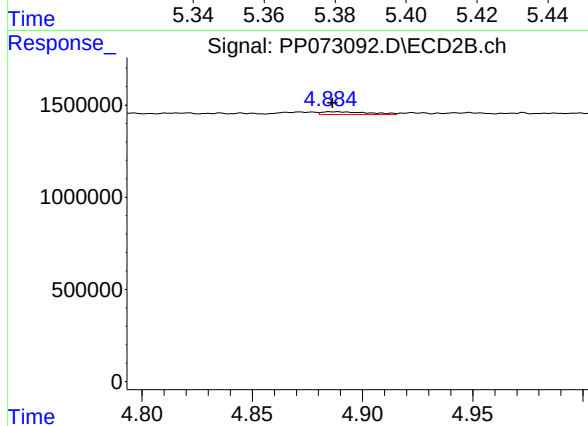

#12 AR-1232-2


R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 220387
Conc: 4.76 ng/ml

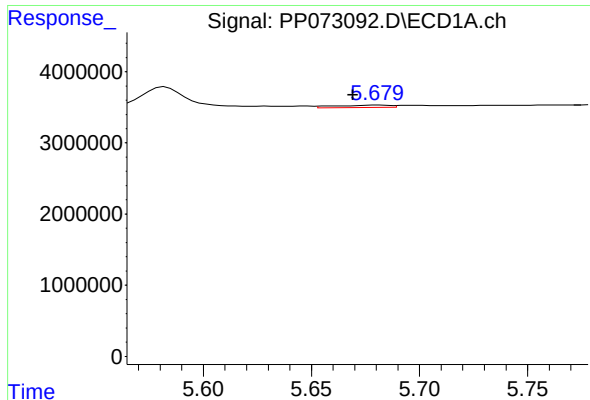

#13 AR-1232-3


R.T.: 5.681 min
Delta R.T.: 0.011 min
Response: 553327
Conc: 10.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

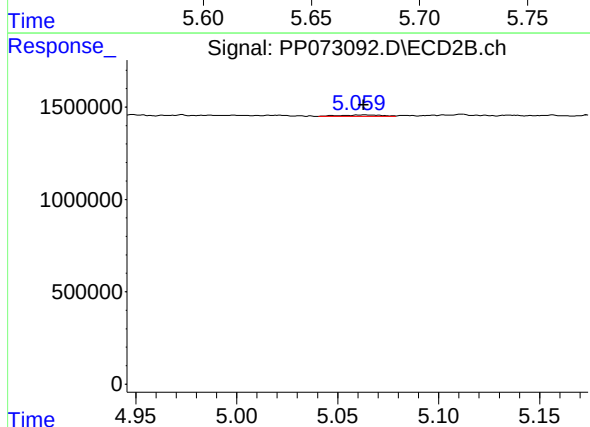


#13 AR-1232-3

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 113274
Conc: 4.61 ng/ml

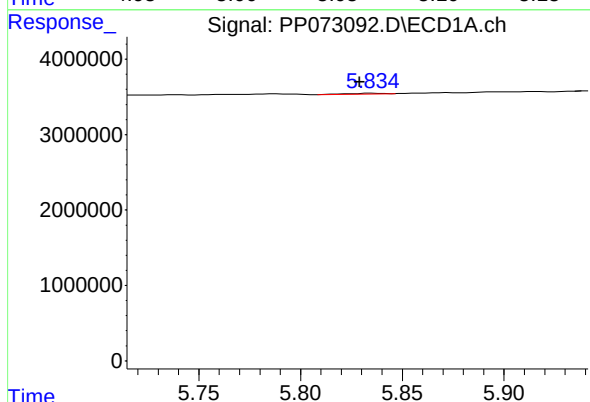


#14 AR-1232-4

R.T.: 5.836 min
Delta R.T.: 0.007 min
Response: 155384
Conc: 6.02 ng/ml

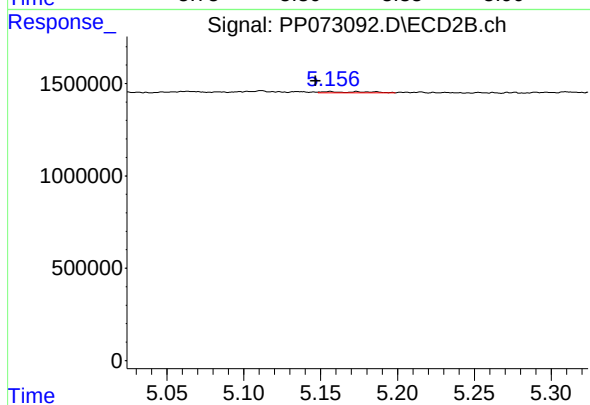

#14 AR-1232-4


R.T.: 5.156 min
Delta R.T.: 0.010 min
Response: 106860
Conc: 4.94 ng/ml

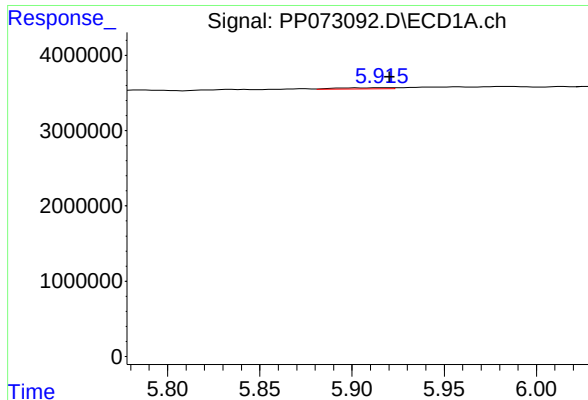

#15 AR-1232-5


R.T.: 5.916 min
Delta R.T.: -0.005 min
Response: 307020
Conc: 8.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

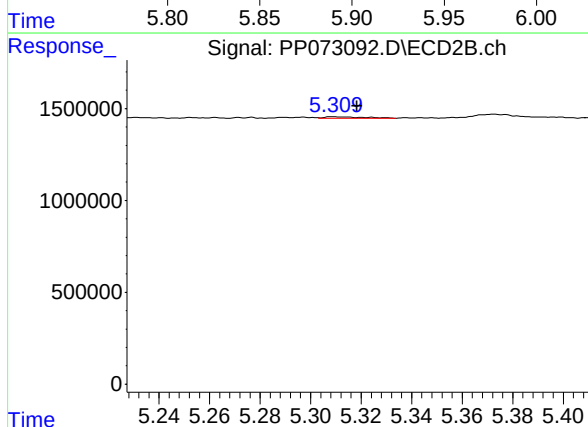


#15 AR-1232-5

R.T.: 5.309 min
Delta R.T.: -0.009 min
Response: 81961
Conc: 3.59 ng/ml

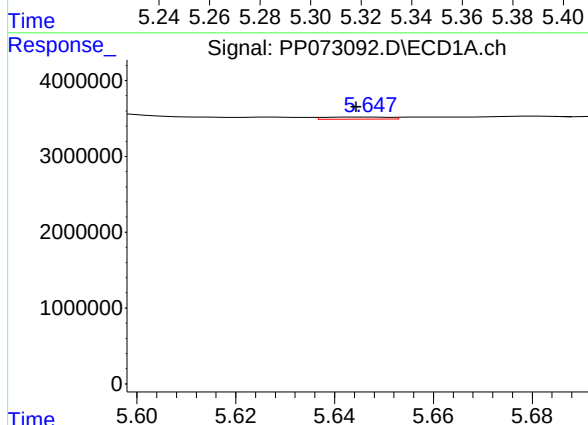


#16 AR-1242-1

R.T.: 5.647 min
Delta R.T.: 0.003 min
Response: 243980
Conc: 4.18 ng/ml

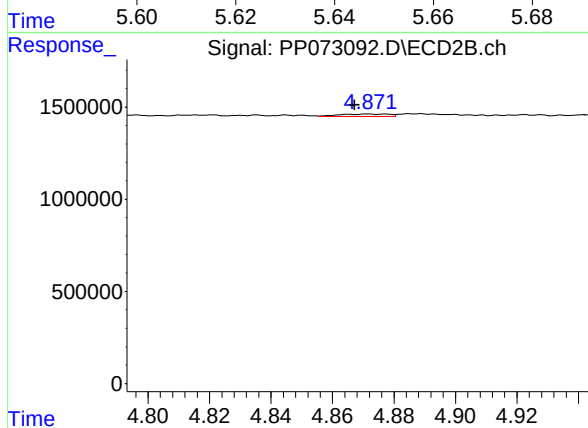

#16 AR-1242-1


R.T.: 4.872 min
Delta R.T.: 0.005 min
Response: 159486
Conc: 2.89 ng/ml

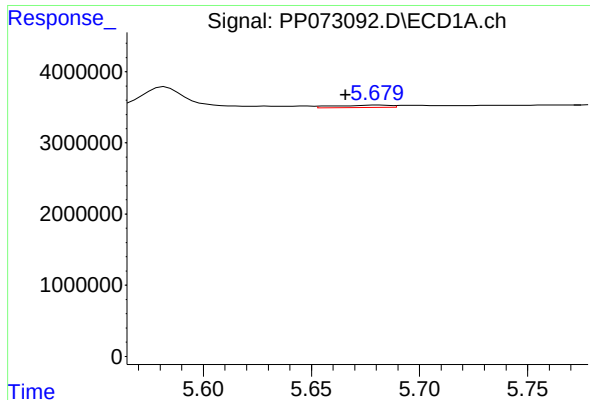

#17 AR-1242-2


R.T.: 5.681 min
Delta R.T.: 0.015 min
Response: 553327
Conc: 6.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

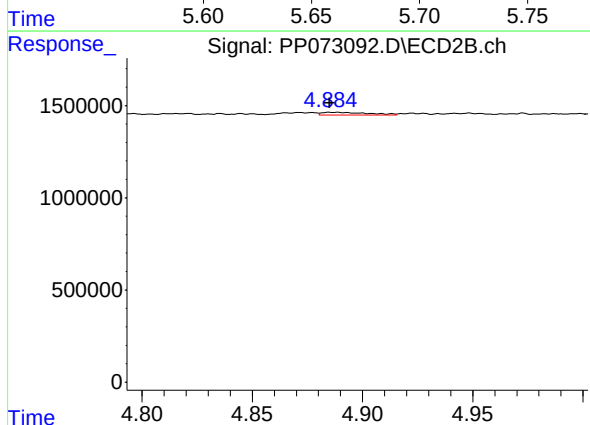


#17 AR-1242-2

R.T.: 4.886 min
Delta R.T.: 0.000 min
Response: 220387
Conc: 2.77 ng/ml

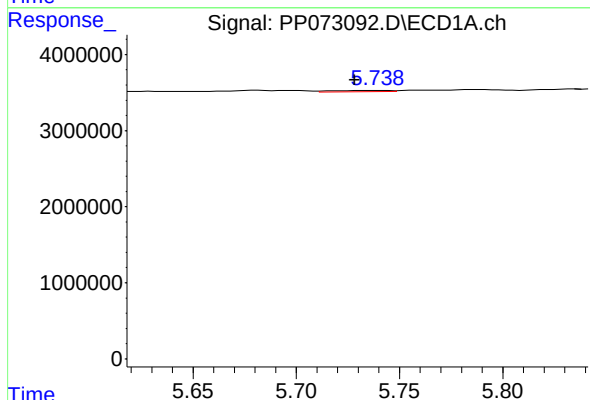


#18 AR-1242-3

R.T.: 5.739 min
Delta R.T.: 0.011 min
Response: 309939
Conc: 5.88 ng/ml

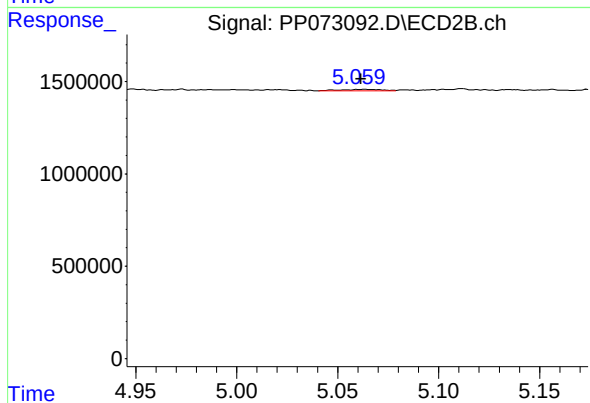

#18 AR-1242-3


R.T.: 5.064 min
Delta R.T.: 0.002 min
Response: 113274
Conc: 2.62 ng/ml

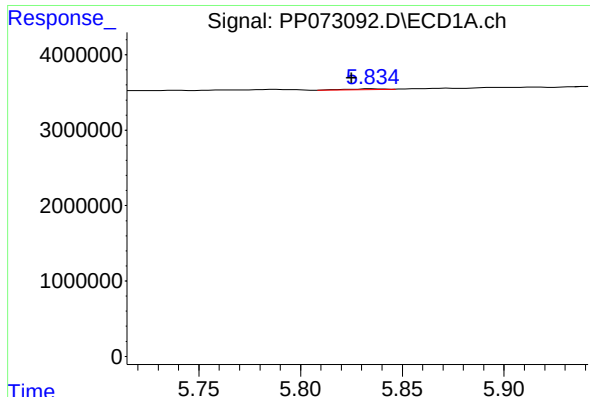

#19 AR-1242-4


R.T.: 5.836 min
Delta R.T.: 0.010 min
Response: 155384
Conc: 3.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

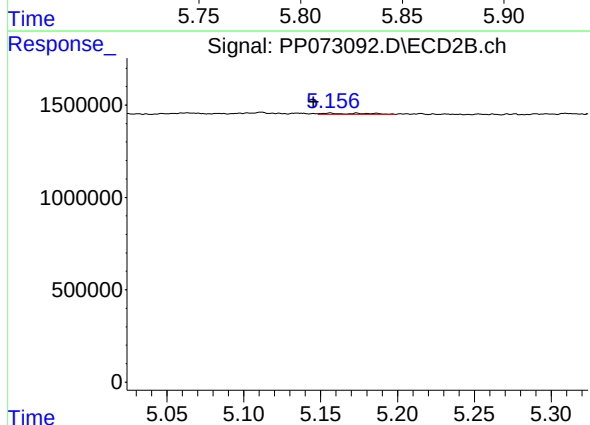


#19 AR-1242-4

R.T.: 5.156 min
Delta R.T.: 0.011 min
Response: 106860
Conc: 2.57 ng/ml

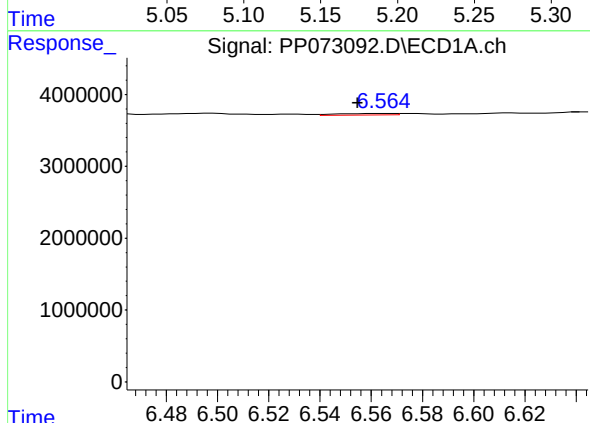


#20 AR-1242-5

R.T.: 6.565 min
Delta R.T.: 0.010 min
Response: 371037
Conc: 7.49 ng/ml

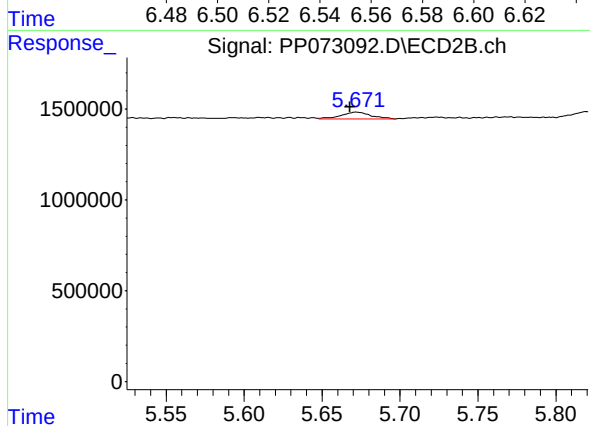

#20 AR-1242-5


R.T.: 5.672 min
Delta R.T.: 0.004 min
Response: 504446
Conc: 9.59 ng/ml

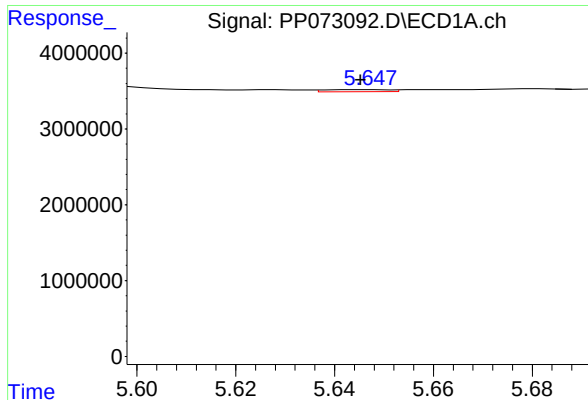

#21 AR-1248-1


R.T.: 5.647 min
Delta R.T.: 0.002 min
Response: 243980
Conc: 5.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

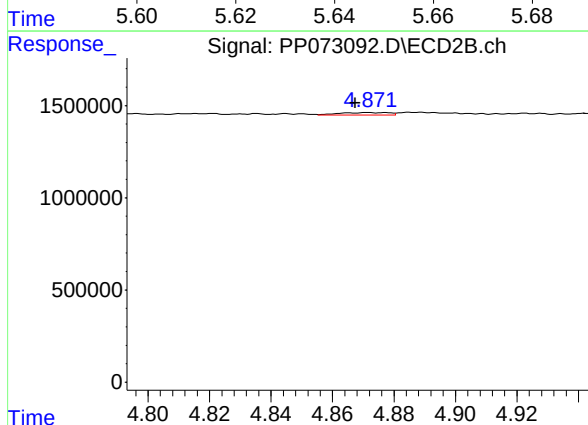


#21 AR-1248-1

R.T.: 4.872 min
Delta R.T.: 0.004 min
Response: 159486
Conc: 3.66 ng/ml

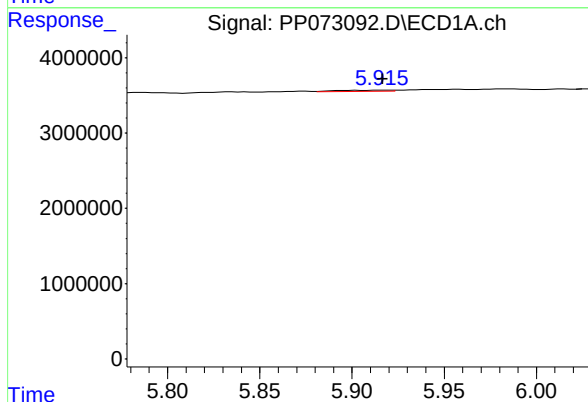


#22 AR-1248-2

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 307020
Conc: 5.24 ng/ml

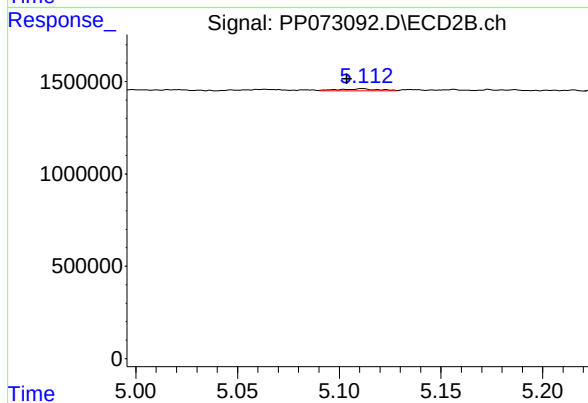

#22 AR-1248-2


R.T.: 5.112 min
Delta R.T.: 0.008 min
Response: 141861
Conc: 2.42 ng/ml

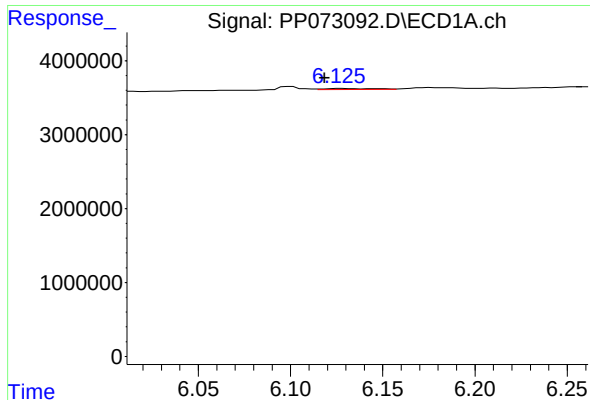

#23 AR-1248-3


R.T.: 6.127 min
Delta R.T.: 0.008 min
Response: 255924
Conc: 3.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

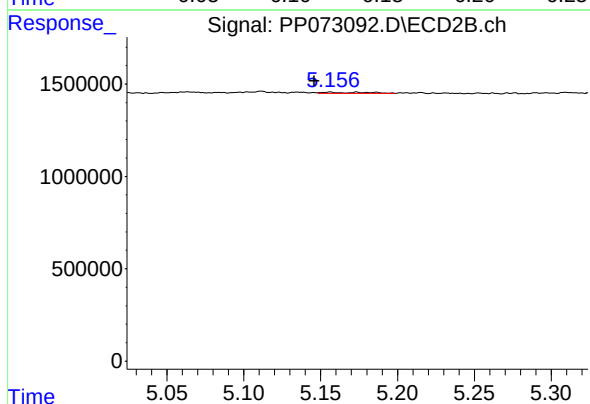


#23 AR-1248-3

R.T.: 5.156 min
Delta R.T.: 0.010 min
Response: 106860
Conc: 1.76 ng/ml

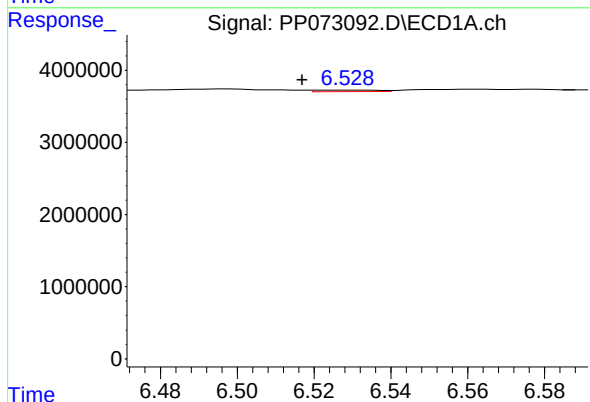


#24 AR-1248-4

R.T.: 6.530 min
Delta R.T.: 0.013 min
Response: 231379
Conc: 2.72 ng/ml

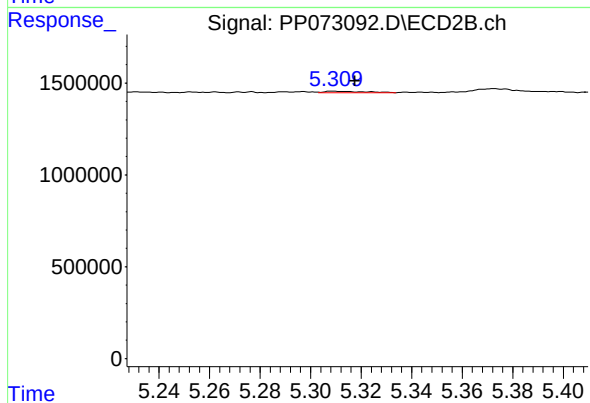

#24 AR-1248-4


R.T.: 5.309 min
Delta R.T.: -0.008 min
Response: 81961
Conc: 1.17 ng/ml

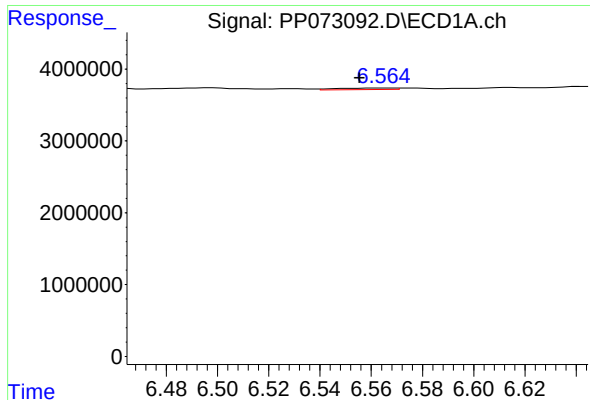

#25 AR-1248-5


R.T.: 6.565 min
Delta R.T.: 0.010 min
Response: 371037
Conc: 4.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

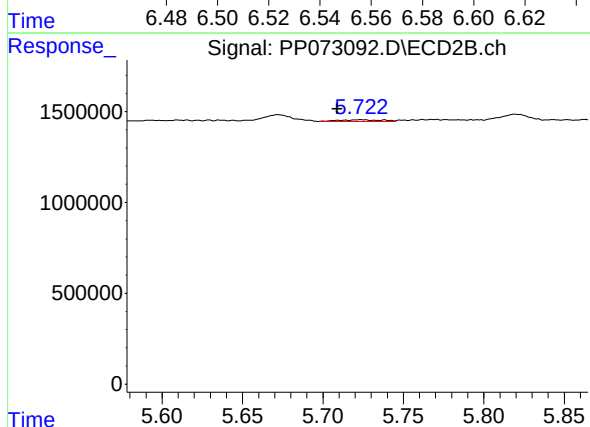


#25 AR-1248-5

R.T.: 5.724 min
Delta R.T.: 0.015 min
Response: 168269
Conc: 2.37 ng/ml

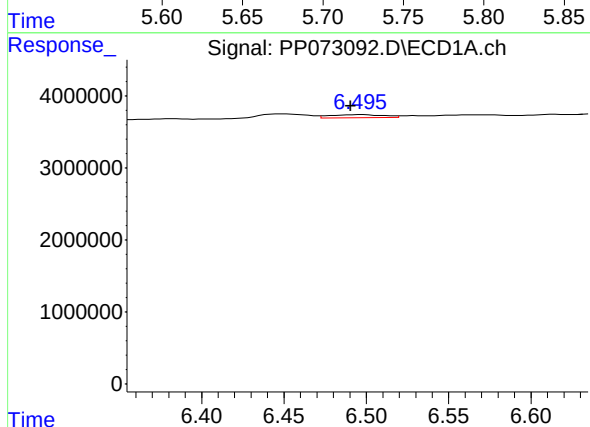


#26 AR-1254-1

R.T.: 6.497 min
Delta R.T.: 0.006 min
Response: 965870
Conc: 11.47 ng/ml

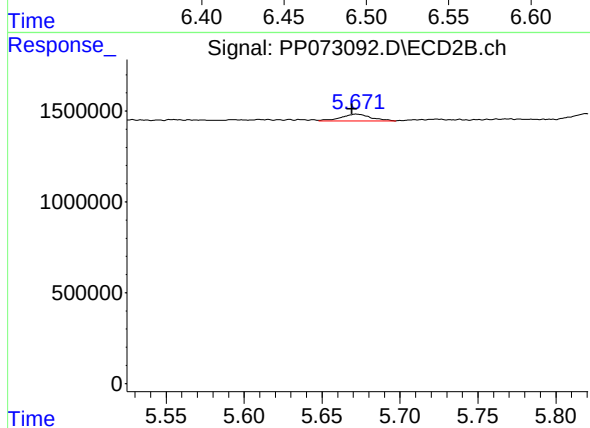

#26 AR-1254-1


R.T.: 5.672 min
Delta R.T.: 0.003 min
Response: 504446
Conc: 4.60 ng/ml

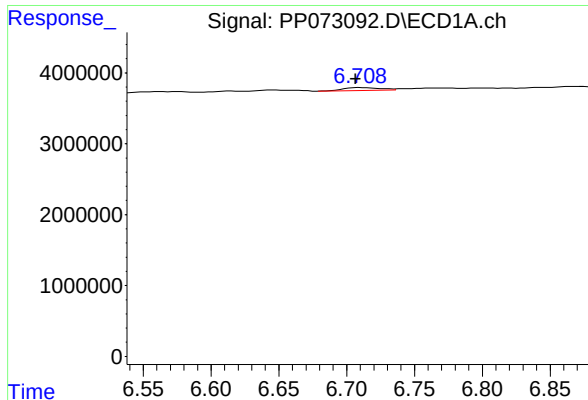

#27 AR-1254-2


R.T.: 6.710 min
Delta R.T.: 0.003 min
Response: 790446
Conc: 6.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

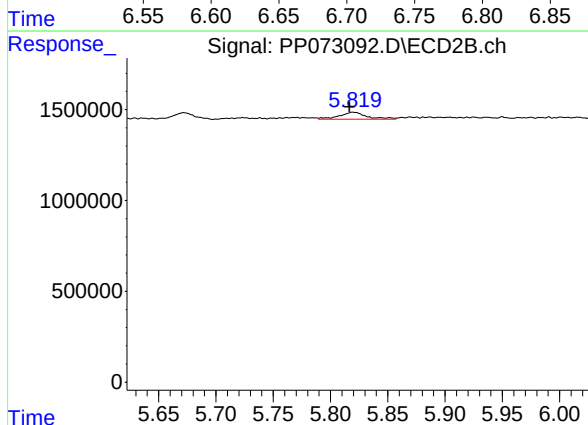


#27 AR-1254-2

R.T.: 5.820 min
Delta R.T.: 0.003 min
Response: 630654
Conc: 6.67 ng/ml

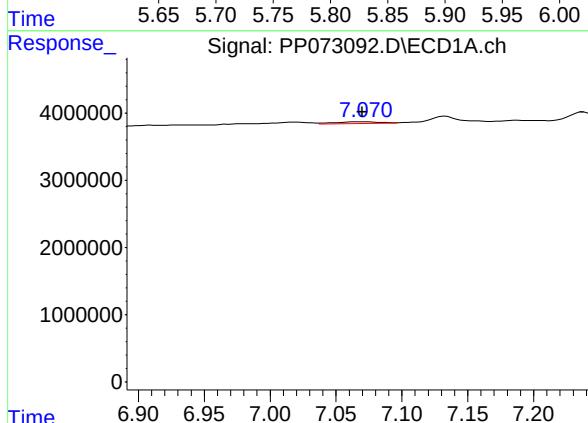


#28 AR-1254-3

R.T.: 7.072 min
Delta R.T.: 0.002 min
Response: 639717
Conc: 4.88 ng/ml

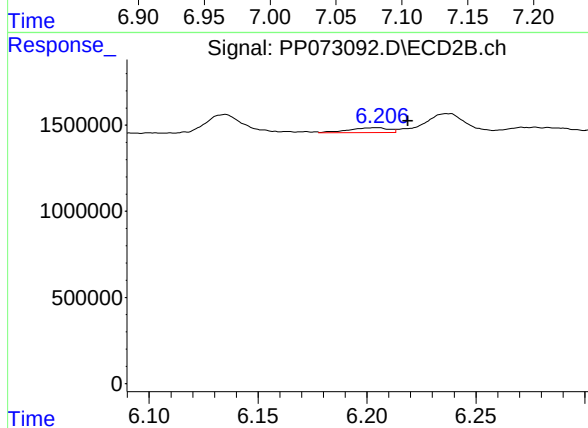

#28 AR-1254-3


R.T.: 6.203 min
Delta R.T.: -0.016 min
Response: 373606
Conc: 2.53 ng/ml

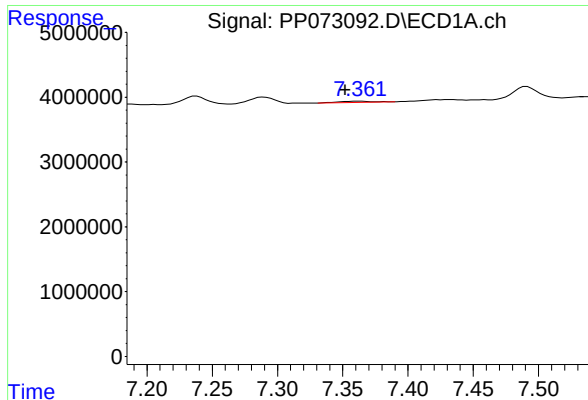

#29 AR-1254-4


R.T.: 7.363 min
Delta R.T.: 0.011 min
Response: 287765
Conc: 2.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

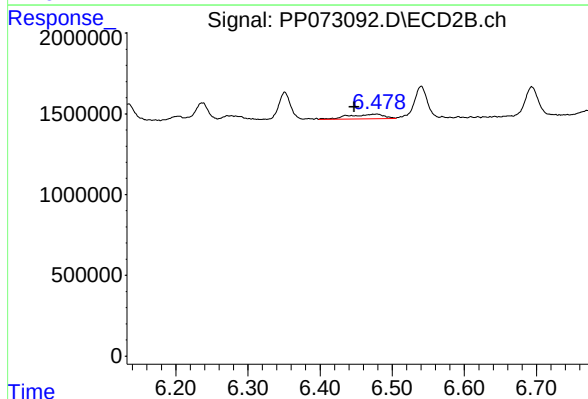


#29 AR-1254-4

R.T.: 6.478 min
Delta R.T.: 0.031 min
Response: 955989
Conc: 9.85 ng/ml

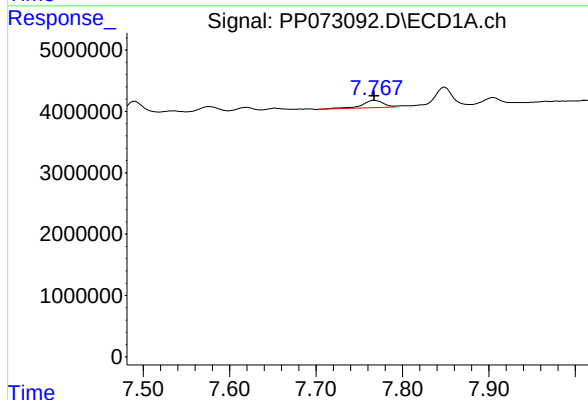


#30 AR-1254-5

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 2099402
Conc: 18.37 ng/ml

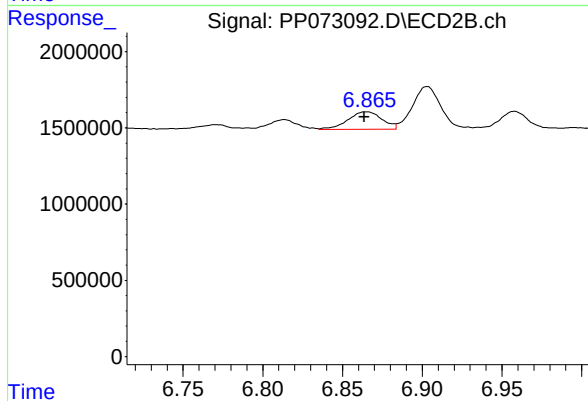

#30 AR-1254-5


R.T.: 6.865 min
Delta R.T.: 0.001 min
Response: 1690783
Conc: 13.01 ng/ml

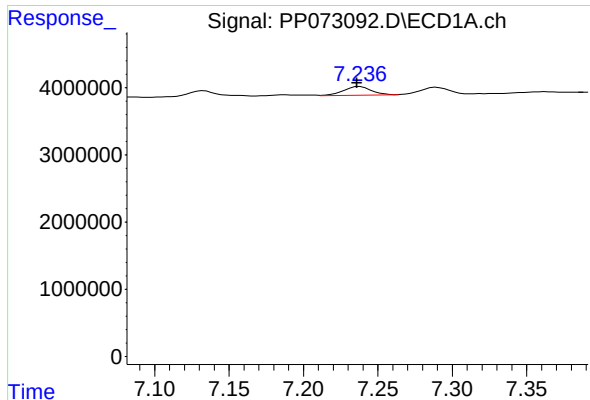

#31 AR-1260-1


R.T.: 7.238 min
Delta R.T.: 0.002 min
Response: 1694610
Conc: 19.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

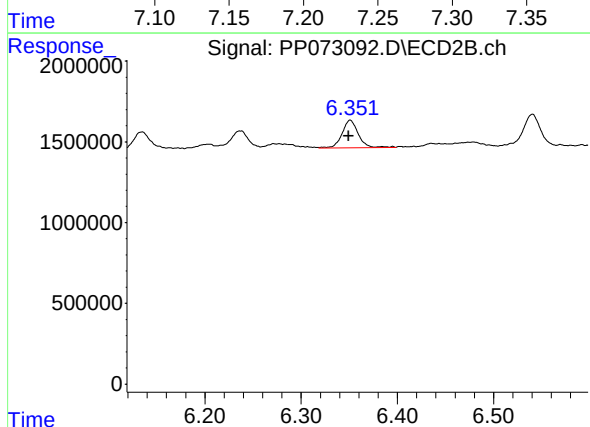


#31 AR-1260-1

R.T.: 6.351 min
Delta R.T.: 0.002 min
Response: 1996354
Conc: 21.07 ng/ml

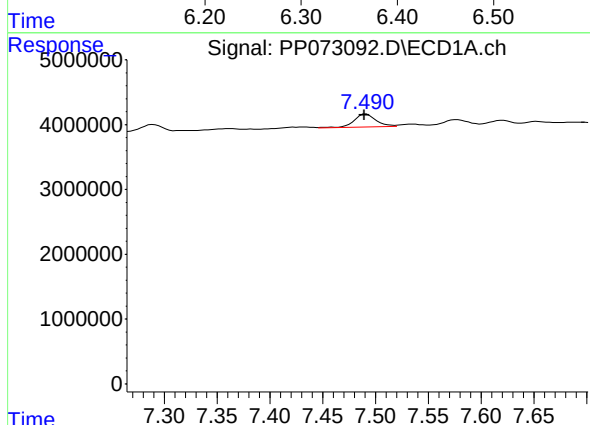


#32 AR-1260-2

R.T.: 7.491 min
Delta R.T.: 0.002 min
Response: 2964006
Conc: 21.81 ng/ml

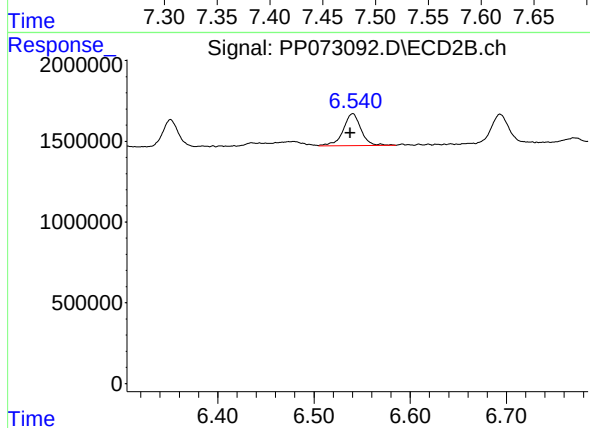

#32 AR-1260-2


R.T.: 6.540 min
Delta R.T.: 0.002 min
Response: 2525199
Conc: 21.69 ng/ml

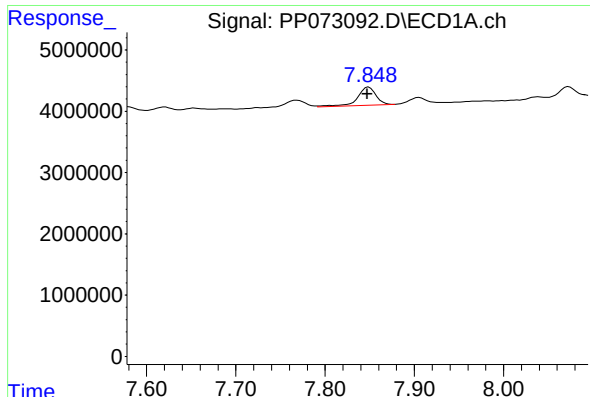

#33 AR-1260-3


R.T.: 7.849 min
Delta R.T.: 0.002 min
Response: 4197931
Conc: 36.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

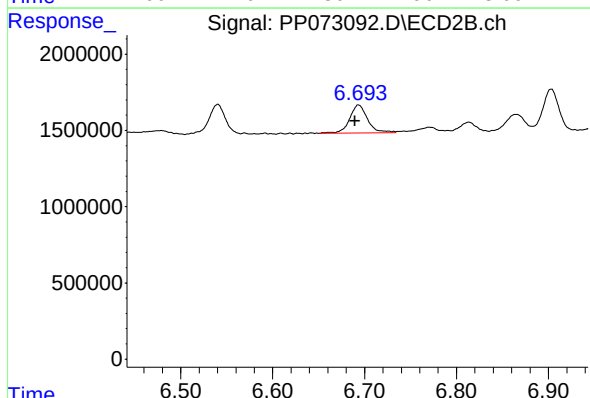


#33 AR-1260-3

R.T.: 6.694 min
Delta R.T.: 0.004 min
Response: 2509204
Conc: 24.09 ng/ml

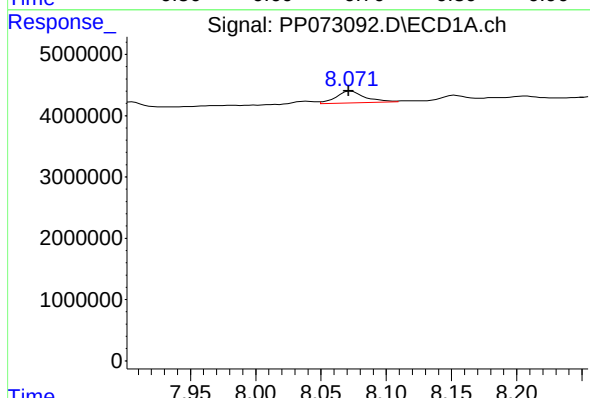


#34 AR-1260-4

R.T.: 8.073 min
Delta R.T.: 0.002 min
Response: 2966917
Conc: 28.79 ng/ml

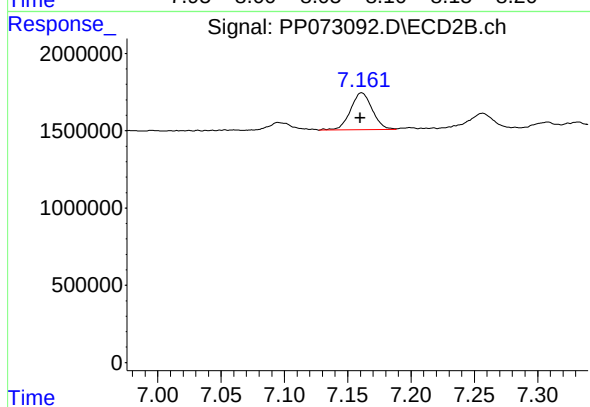

#34 AR-1260-4


R.T.: 7.161 min
Delta R.T.: 0.001 min
Response: 2871292
Conc: 32.73 ng/ml

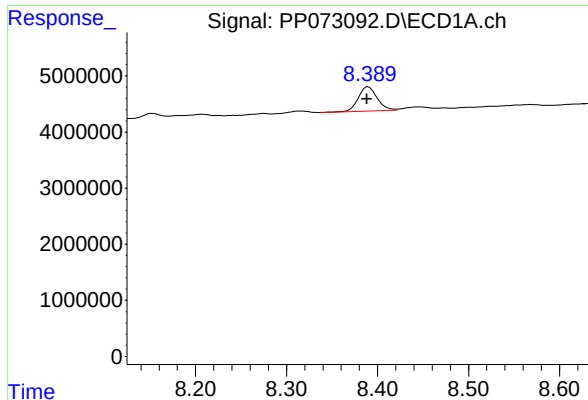

#35 AR-1260-5


R.T.: 8.390 min
Delta R.T.: 0.002 min
Response: 6265402
Conc: 26.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

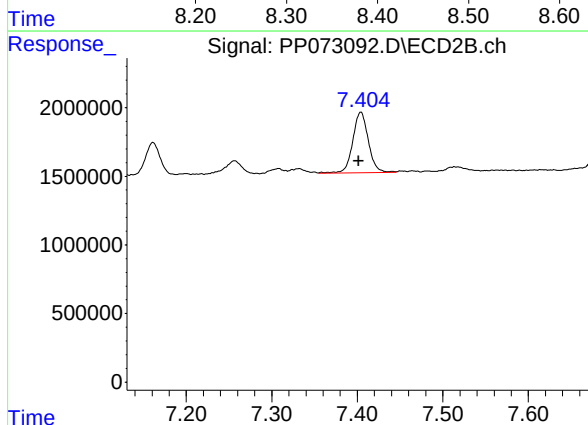


#35 AR-1260-5

R.T.: 7.404 min
Delta R.T.: 0.002 min
Response: 5641387
Conc: 26.44 ng/ml

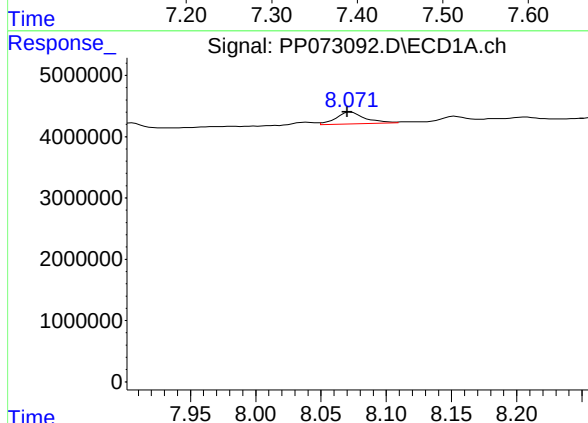


#36 AR-1262-1

R.T.: 8.073 min
Delta R.T.: 0.003 min
Response: 2966917
Conc: 20.04 ng/ml

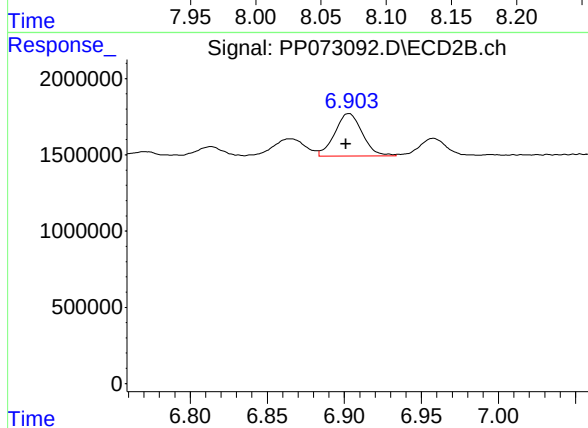

#36 AR-1262-1


R.T.: 6.903 min
Delta R.T.: 0.002 min
Response: 3419463
Conc: 23.67 ng/ml

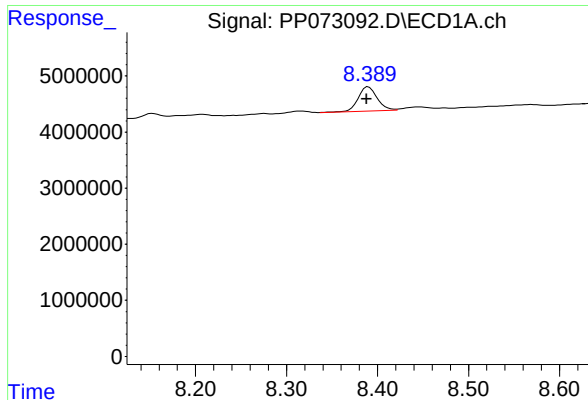

#37 AR-1262-2


R.T.: 8.390 min
Delta R.T.: 0.002 min
Response: 6265402
Conc: 19.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

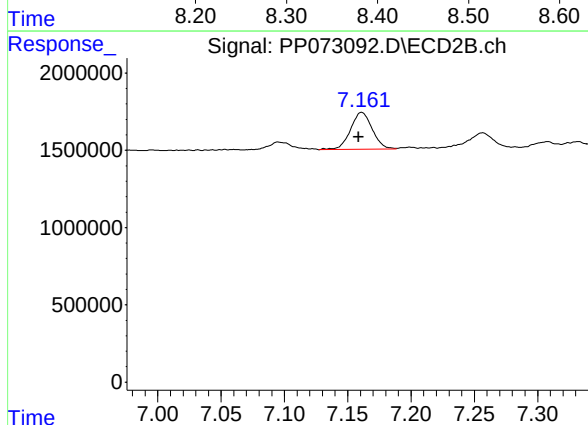


#37 AR-1262-2

R.T.: 7.161 min
Delta R.T.: 0.002 min
Response: 2871292
Conc: 23.49 ng/ml

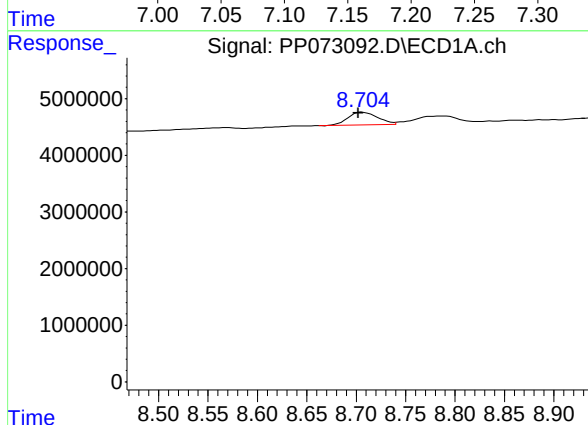


#38 AR-1262-3

R.T.: 8.706 min
Delta R.T.: 0.003 min
Response: 4694814
Conc: 21.94 ng/ml

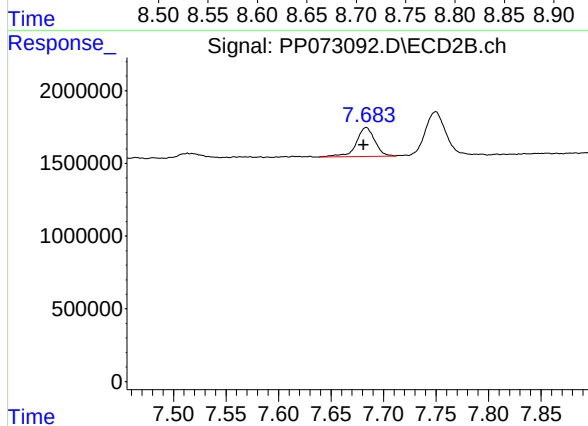

#38 AR-1262-3


R.T.: 7.684 min
Delta R.T.: 0.003 min
Response: 2452693
Conc: 21.76 ng/ml

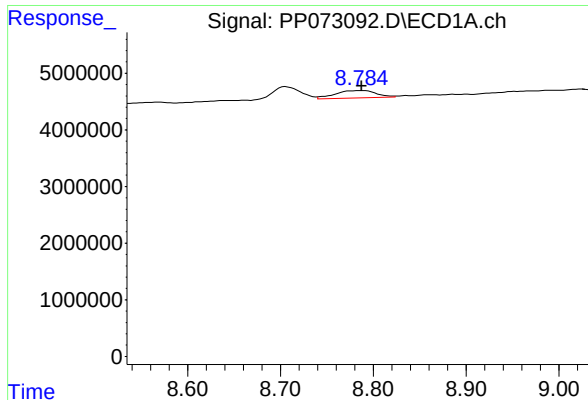

#39 AR-1262-4


R.T.: 8.786 min
Delta R.T.: -0.002 min
Response: 3997119
Conc: 25.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

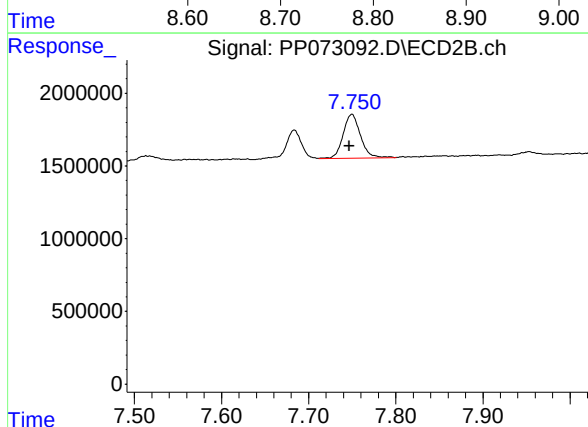


#39 AR-1262-4

R.T.: 7.749 min
Delta R.T.: 0.003 min
Response: 4166415
Conc: 22.72 ng/ml

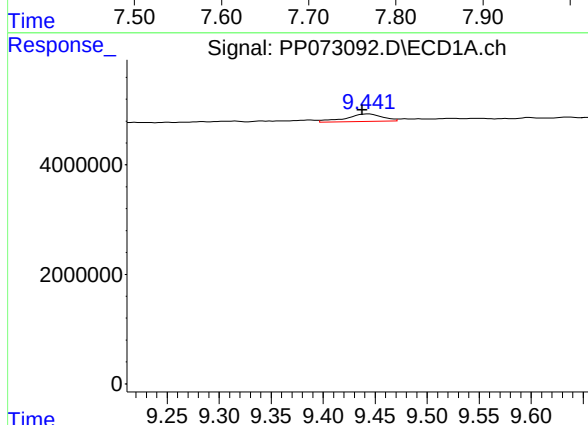


#40 AR-1262-5

R.T.: 9.444 min
Delta R.T.: 0.006 min
Response: 3428467
Conc: 30.65 ng/ml

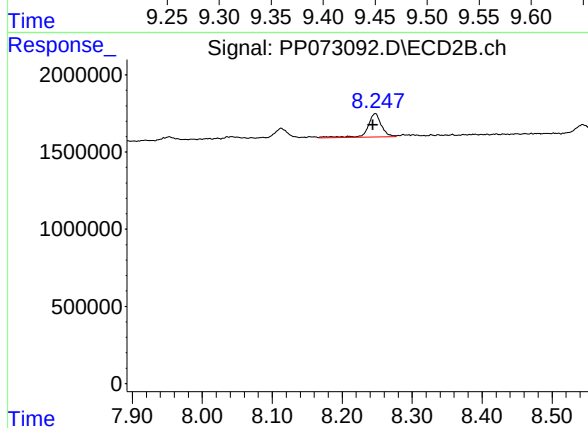

#40 AR-1262-5


R.T.: 8.247 min
Delta R.T.: 0.003 min
Response: 2063226
Conc: 23.83 ng/ml

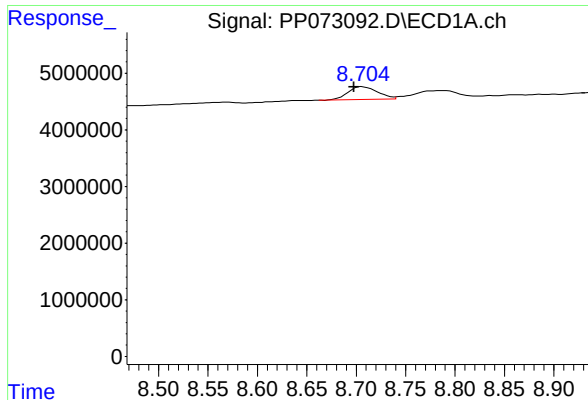

#41 AR-1268-1


R.T.: 8.706 min
Delta R.T.: 0.008 min
Response: 4694814
Conc: 13.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

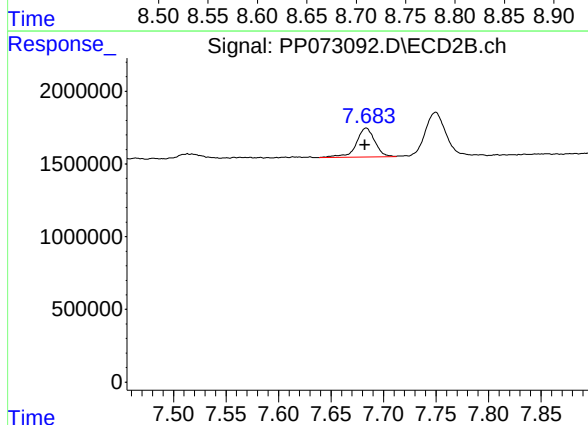


#41 AR-1268-1

R.T.: 7.684 min
Delta R.T.: 0.001 min
Response: 2452693
Conc: 8.54 ng/ml

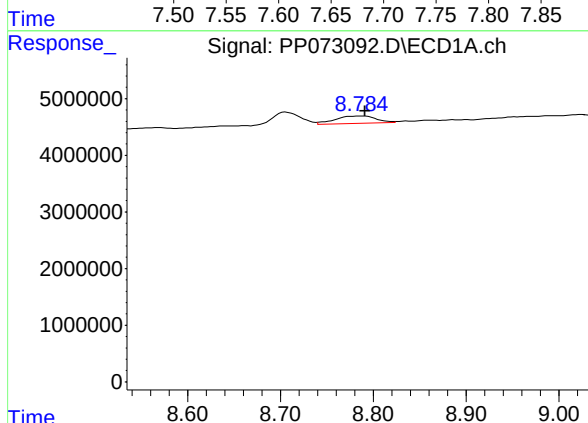


#42 AR-1268-2

R.T.: 8.786 min
Delta R.T.: -0.005 min
Response: 3997119
Conc: 13.10 ng/ml

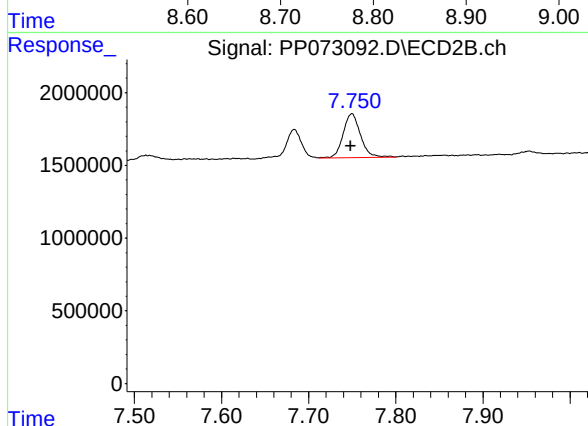

#42 AR-1268-2


R.T.: 7.749 min
Delta R.T.: 0.001 min
Response: 4166415
Conc: 16.20 ng/ml

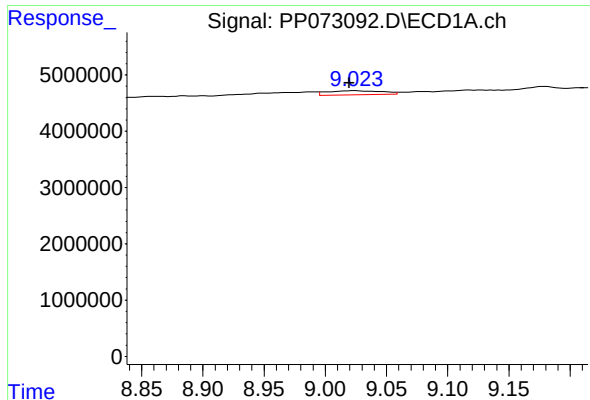

#43 AR-1268-3


R.T.: 9.024 min
Delta R.T.: 0.005 min
Response: 2225720
Conc: 8.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

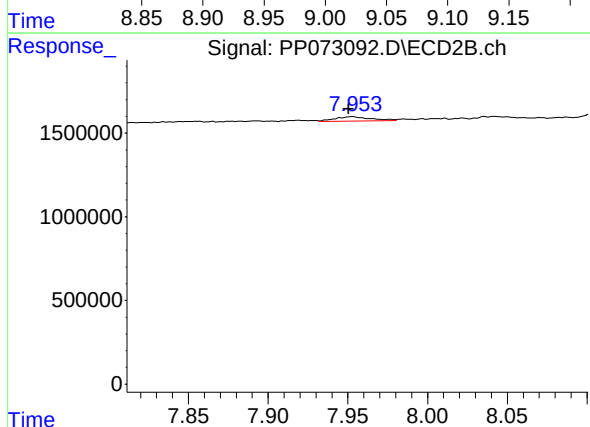


#43 AR-1268-3

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 413629
Conc: 1.92 ng/ml

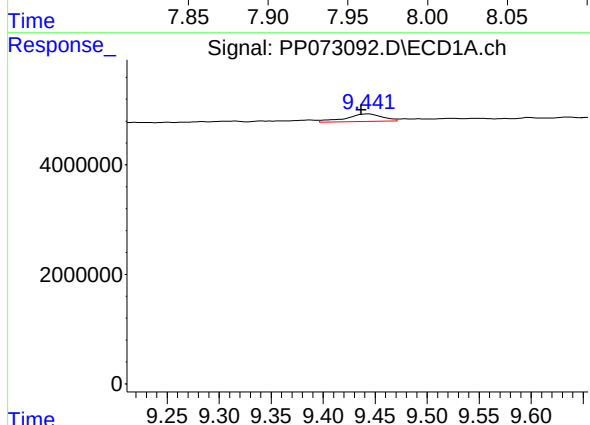


#44 AR-1268-4

R.T.: 9.444 min
Delta R.T.: 0.007 min
Response: 3428467
Conc: 29.30 ng/ml

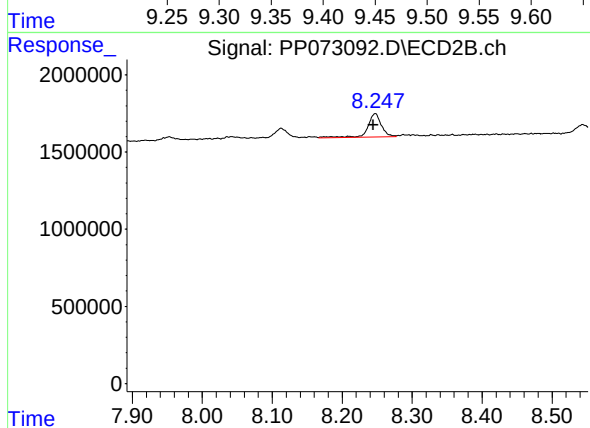

#44 AR-1268-4


R.T.: 8.247 min
Delta R.T.: 0.002 min
Response: 2063226
Conc: 21.91 ng/ml

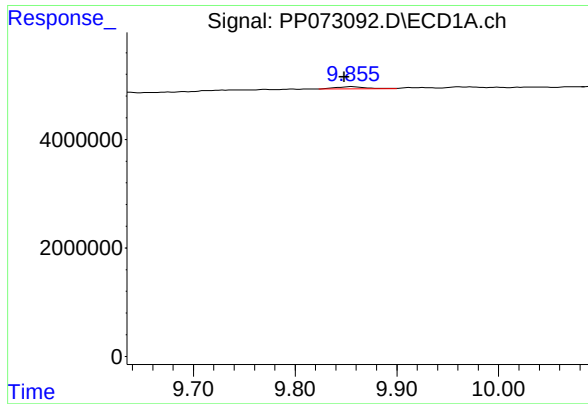

#45 AR-1268-5

R.T.: 9.856 min
Delta R.T.: 0.007 min
Response: 883760
Conc: 1.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

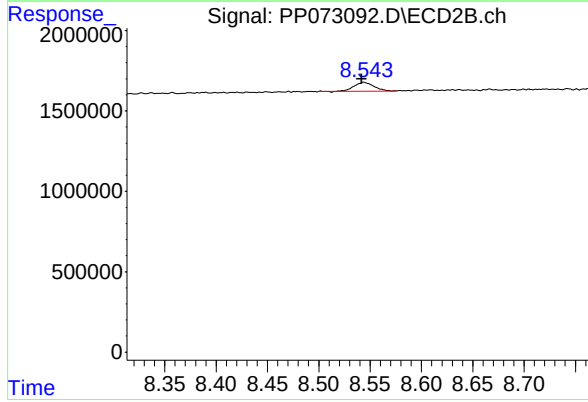

#45 AR-1268-5

R.T.: 8.544 min
Delta R.T.: 0.002 min
Response: 744504
Conc: 1.29 ng/ml