

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 18:44
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:29:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.497	3.790	42155629	36645091	19.971	20.338
2) SA Decachlor...	10.194	8.801	42240803	31277957	24.718	23.434
Target Compounds						
3) L1 AR-1016-1	5.655	4.882	358290	57877	4.930	0.842 #
4) L1 AR-1016-2	5.673	4.882	410983	57877	3.951	0.575 #
5) L1 AR-1016-3	5.734	0.000	132437	0	2.027	N.D. #
6) L1 AR-1016-4	5.803	0.000	352102	0	6.735	N.D. #
7) L1 AR-1016-5	6.137	5.313	357215	73643	7.144	1.332 #
8) L2 AR-1221-1	4.713	4.013	169572	376315	6.877	14.004 #
9) L2 AR-1221-2	4.770	4.091	107797	976877	5.342	48.395 #
10) L2 AR-1221-3	4.854	4.141	131540	92975	2.137	1.583 #
11) L3 AR-1232-1	4.854	4.141	131540	92975	2.801	2.041 #
12) L3 AR-1232-2	5.383	4.882	91050	57877	4.070	1.251 #
13) L3 AR-1232-3	5.673	0.000	410983	0	7.965	N.D. #
14) L3 AR-1232-4	5.803	0.000	352102	0	13.642	N.D. #
15) L3 AR-1232-5	5.924	5.313	161486	73643	4.527	3.222 #
16) L4 AR-1242-1	5.655	4.882	358290	57877	6.131	1.048 #
17) L4 AR-1242-2	5.673	4.882	410983	57877	4.748	0.728 #
18) L4 AR-1242-3	5.734	0.000	132437	0	2.513	N.D. #
19) L4 AR-1242-4	5.803	0.000	352102	0	8.010	N.D. #
20) L4 AR-1242-5	6.571	5.676	1624248	289757	32.774	5.510 #
21) L5 AR-1248-1	5.655	4.882	358290	57877	7.532	1.328 #
22) L5 AR-1248-2	5.924	0.000	161486	0	2.758	N.D. #
23) L5 AR-1248-3	6.137	0.000	357215	0	5.475	N.D. #
24) L5 AR-1248-4	6.515	5.313	1324548	73643	15.571	1.052 #
25) L5 AR-1248-5	6.571	5.720	1624248	186577	19.407	2.627 #
26) L6 AR-1254-1	6.492	5.676	832421	289757	9.889	2.643 #
27) L6 AR-1254-2	6.731	5.814	1436139	188852	11.452	1.997 #
28) L6 AR-1254-3	7.077	6.238	1821266	249818	13.880	1.693 #
29) L6 AR-1254-4	7.378	6.436	3315364	512255	27.678	5.275 #
30) L6 AR-1254-5	7.768	6.867	221704	55450	1.940	0.427 #
31) L7 AR-1260-1	7.253	6.359	1488460	15263	16.873	0.161 #
32) L7 AR-1260-2	7.509	6.524	1246309	396348	9.172	3.404 #
33) L7 AR-1260-3	7.850	6.697	2659641	314875	23.299	3.023 #
34) L7 AR-1260-4	8.048	7.158	100325	1799176	0.974	20.506 #
35) L7 AR-1260-5	8.395	7.404	871846	883427	3.623	4.140
36) L8 AR-1262-1	8.048	6.904	100325	1212987	0.678	8.396 #
37) L8 AR-1262-2	8.395	7.158	871846	1799176	2.755	14.720 #
38) L8 AR-1262-3	8.704	7.684	6851498	5844436	32.020	51.857 #
39) L8 AR-1262-4	8.797	7.751	6966108	5100747	44.203	27.819 #
40) L8 AR-1262-5	9.443	8.248	3268108	1788105	29.215	20.651 #
41) L9 AR-1268-1	8.704	7.684	6851498	5844436	19.158	20.345

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 18:44
 Operator : YP\AJ
 Sample : Q2126-07
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:29:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.797	7.751	6966108	5100747	22.835	19.838
43) L9	AR-1268-3	9.025	7.952	7928360	4694824	29.860	21.741 #
44) L9	AR-1268-4	9.443	8.248	3268108	1788105	27.927	18.985 #
45) L9	AR-1268-5	9.857	8.544	14807140	11979579	20.019	20.697



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
Data File : PP073093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 18:44
Operator : YP\AJ
Sample : Q2126-07
Misc : AR1268 MDL 25 PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:29:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

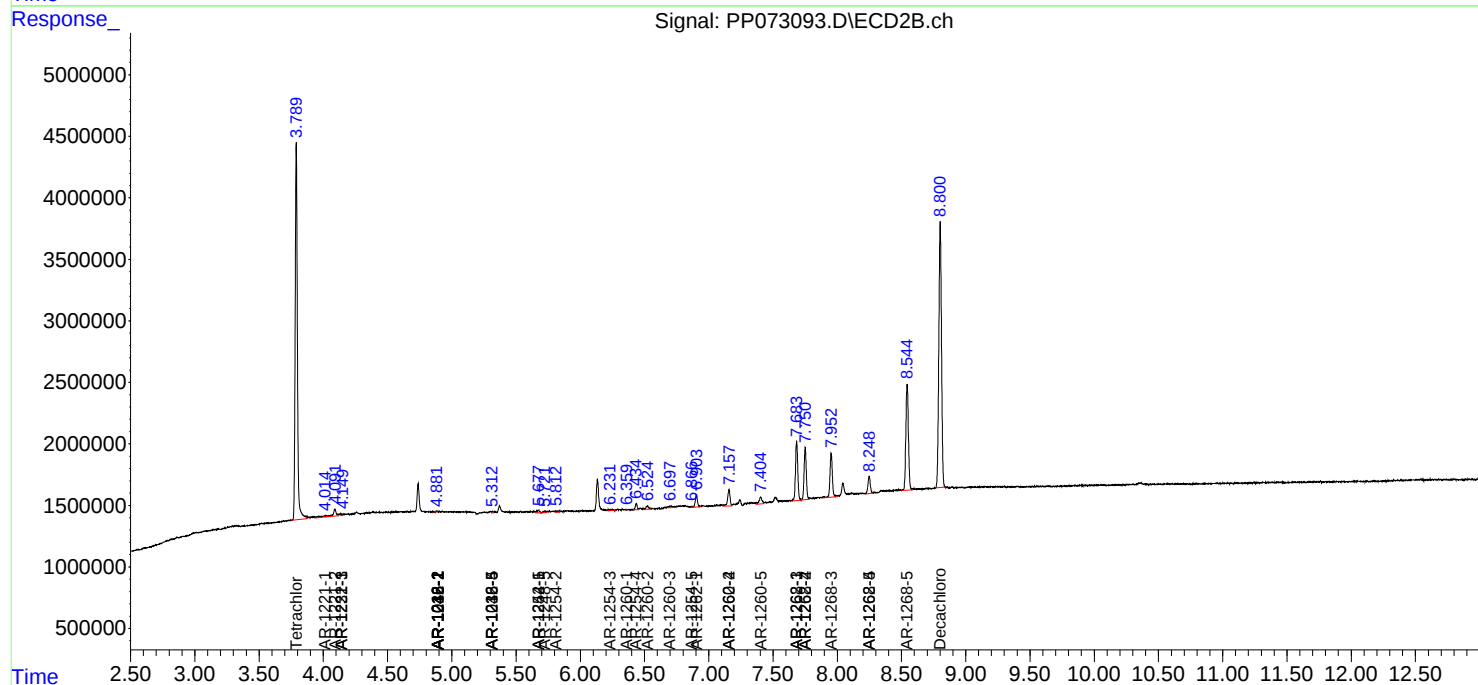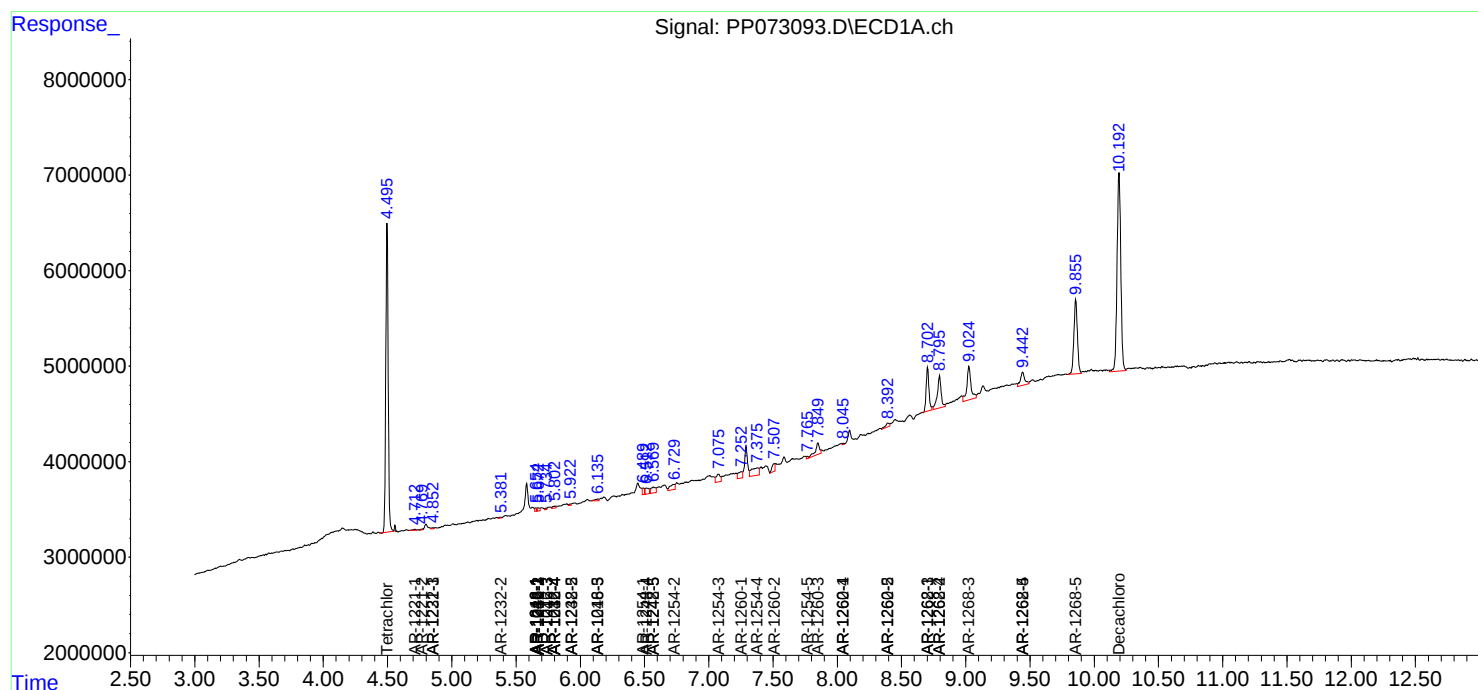


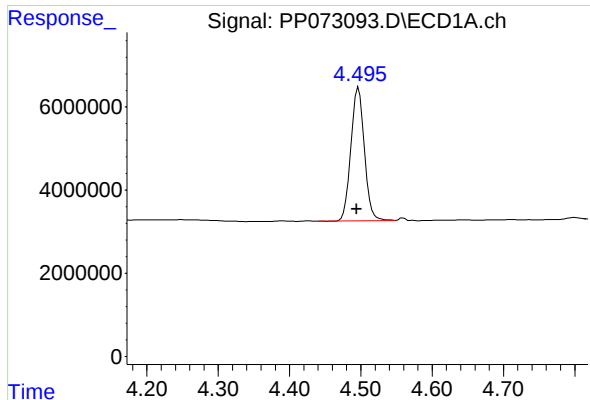

#1 Tetrachloro-m-xylene


R.T.: 4.497 min
Delta R.T.: 0.003 min
Response: 42155629
Conc: 19.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

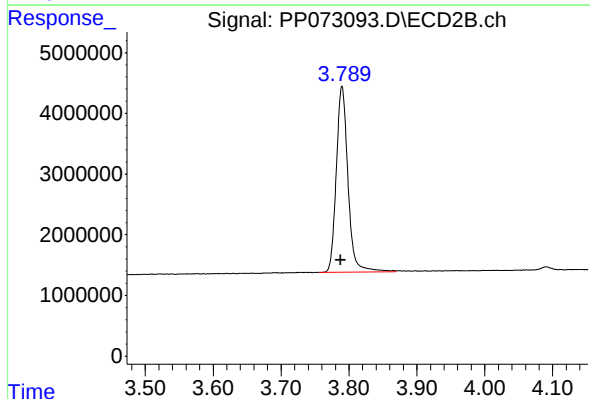


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.002 min
Response: 36645091
Conc: 20.34 ng/ml

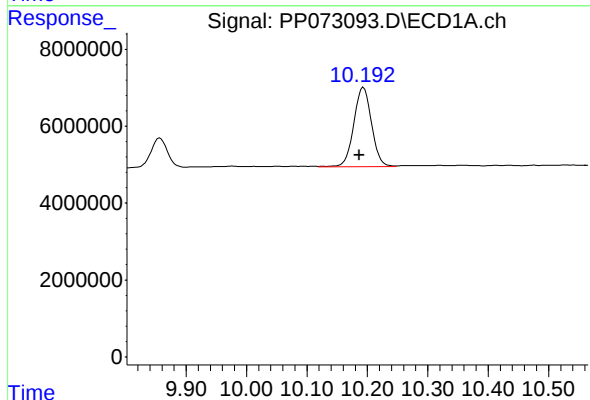


#2 Decachlorobiphenyl

R.T.: 10.194 min
Delta R.T.: 0.006 min
Response: 42240803
Conc: 24.72 ng/ml

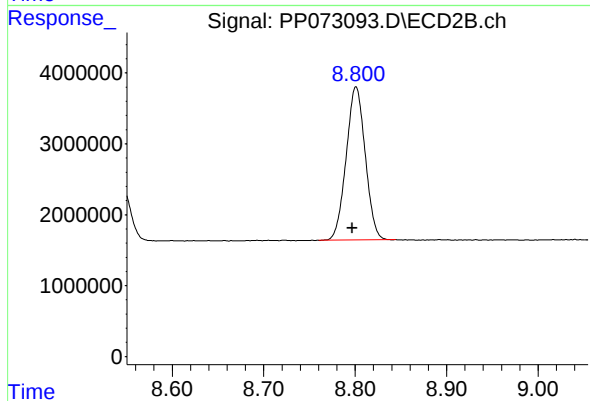

#2 Decachlorobiphenyl


R.T.: 8.801 min
Delta R.T.: 0.004 min
Response: 31277957
Conc: 23.43 ng/ml

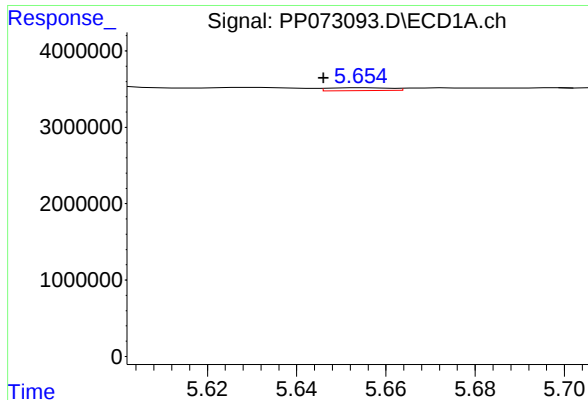

#3 AR-1016-1


R.T.: 5.655 min
Delta R.T.: 0.009 min
Response: 358290
Conc: 4.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

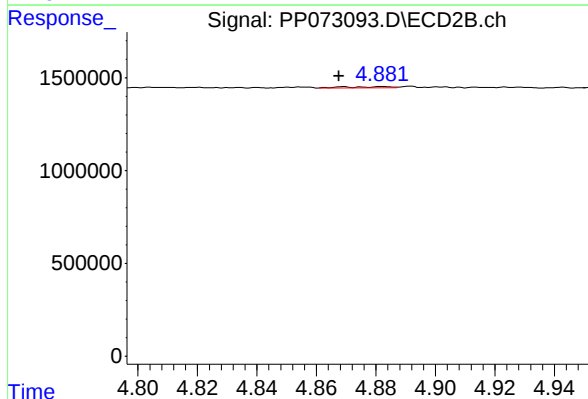


#3 AR-1016-1

R.T.: 4.882 min
Delta R.T.: 0.015 min
Response: 57877
Conc: 0.84 ng/ml

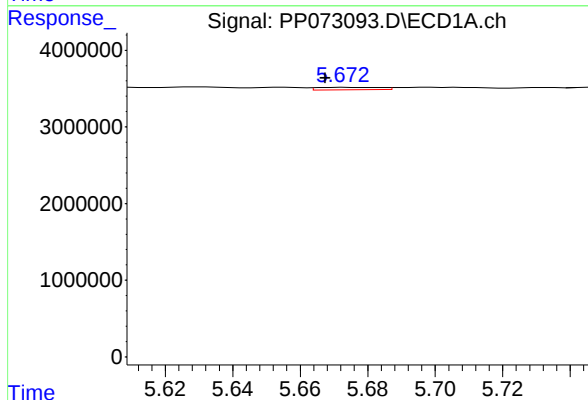


#4 AR-1016-2

R.T.: 5.673 min
Delta R.T.: 0.006 min
Response: 410983
Conc: 3.95 ng/ml

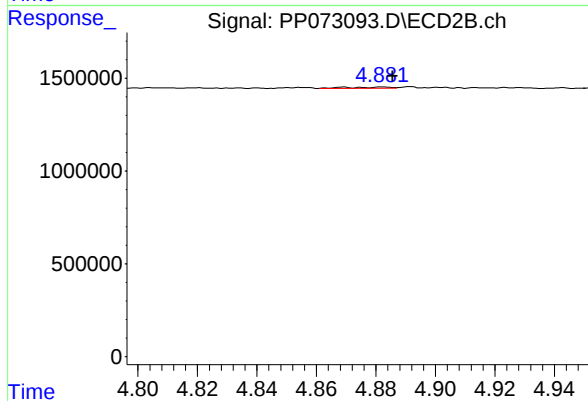

#4 AR-1016-2


R.T.: 4.882 min
Delta R.T.: -0.004 min
Response: 57877
Conc: 0.58 ng/ml

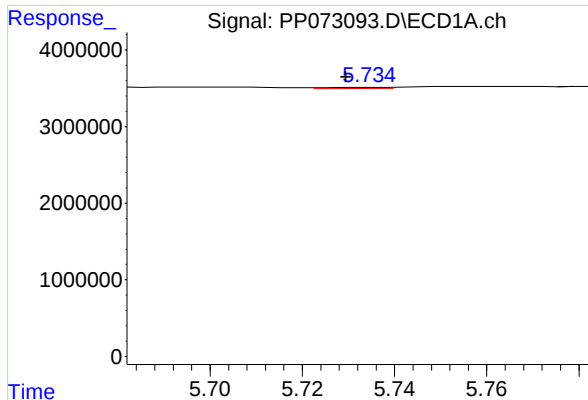

#5 AR-1016-3


R.T.: 5.734 min
Delta R.T.: 0.005 min
Response: 132437
Conc: 2.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

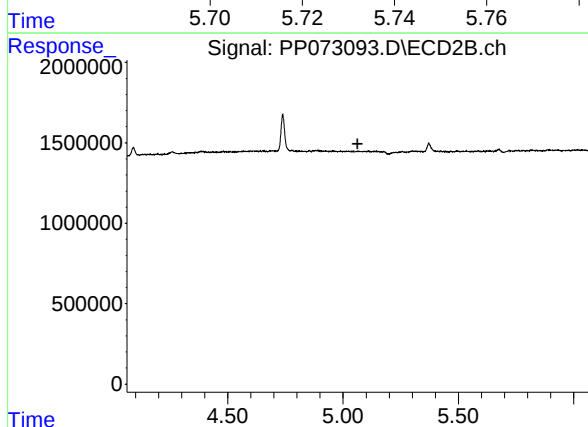


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.062 min
Response: 0
Conc: N.D.

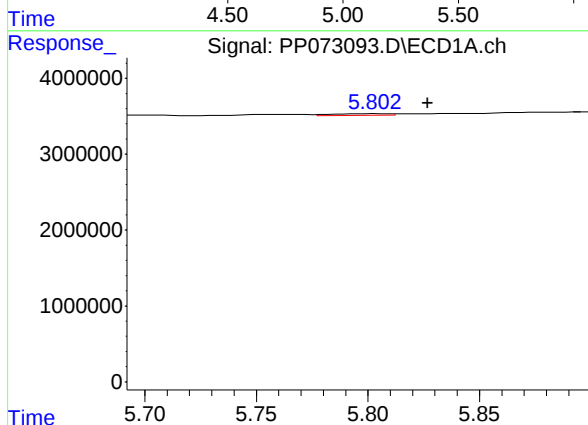


#6 AR-1016-4

R.T.: 5.803 min
Delta R.T.: -0.023 min
Response: 352102
Conc: 6.73 ng/ml

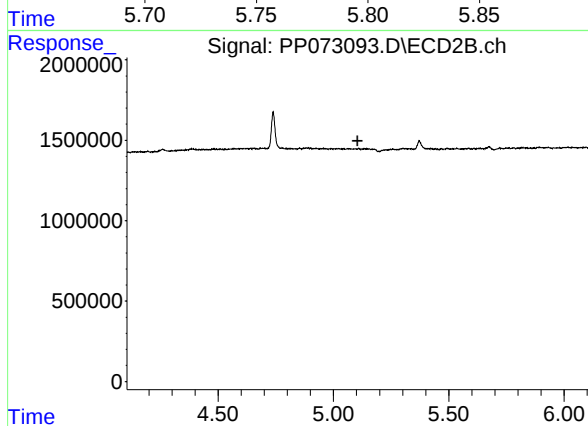

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 5.104 min
Response: 0
Conc: N.D.

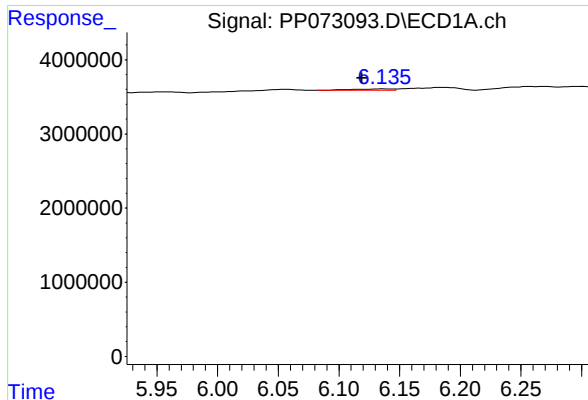

#7 AR-1016-5


R.T.: 6.137 min
Delta R.T.: 0.018 min
Response: 357215
Conc: 7.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

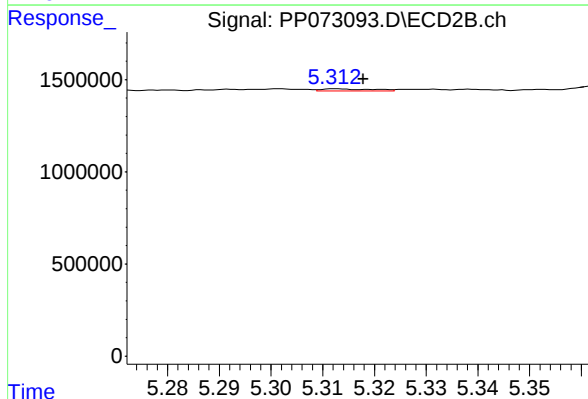


#7 AR-1016-5

R.T.: 5.313 min
Delta R.T.: -0.005 min
Response: 73643
Conc: 1.33 ng/ml

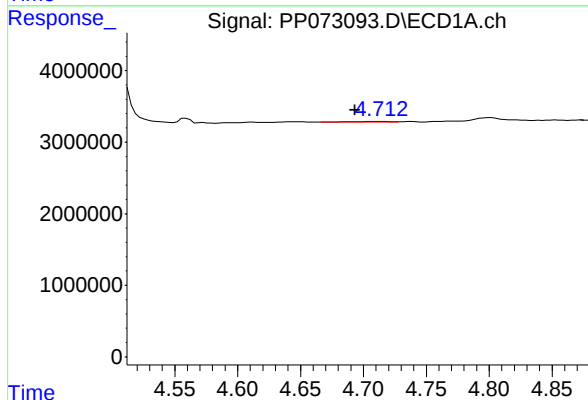


#8 AR-1221-1

R.T.: 4.713 min
Delta R.T.: 0.020 min
Response: 169572
Conc: 6.88 ng/ml

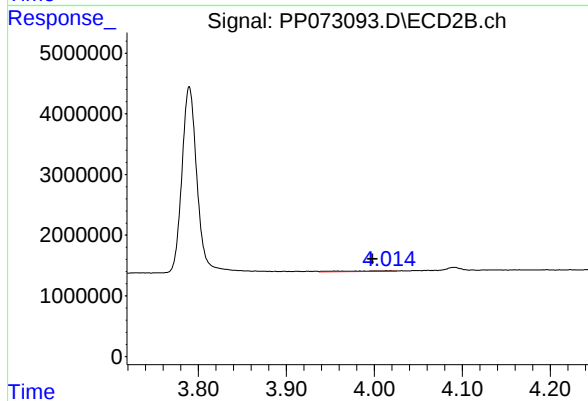

#8 AR-1221-1


R.T.: 4.013 min
Delta R.T.: 0.016 min
Response: 376315
Conc: 14.00 ng/ml

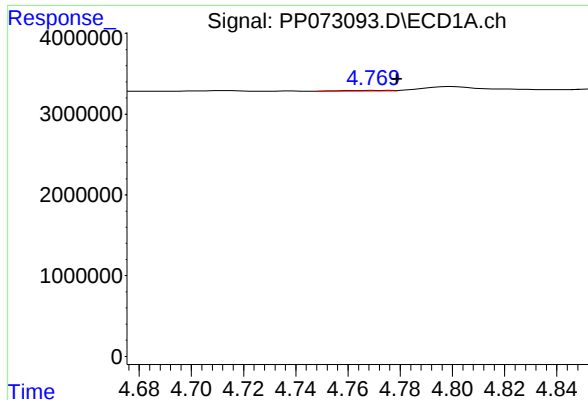

#9 AR-1221-2


R.T.: 4.770 min
Delta R.T.: -0.009 min
Response: 107797
Conc: 5.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

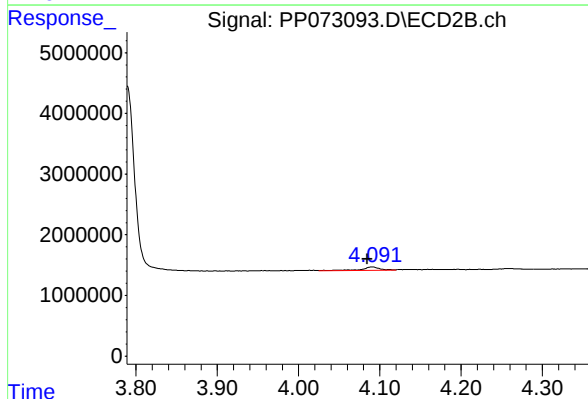


#9 AR-1221-2

R.T.: 4.091 min
Delta R.T.: 0.006 min
Response: 976877
Conc: 48.40 ng/ml

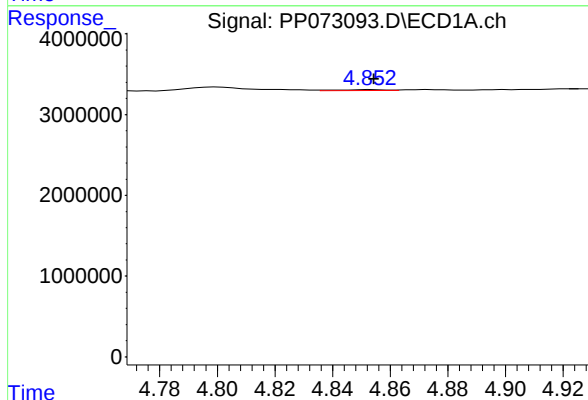


#10 AR-1221-3

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 131540
Conc: 2.14 ng/ml

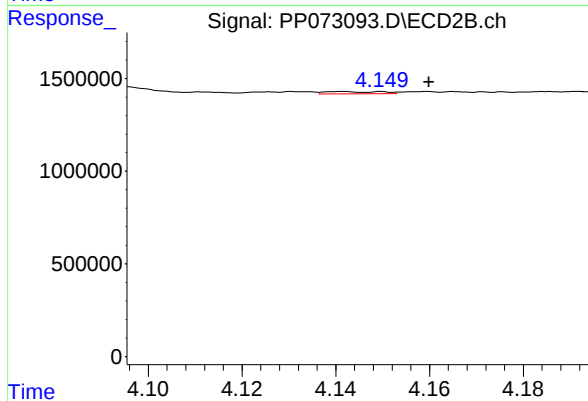

#10 AR-1221-3


R.T.: 4.141 min
Delta R.T.: -0.019 min
Response: 92975
Conc: 1.58 ng/ml

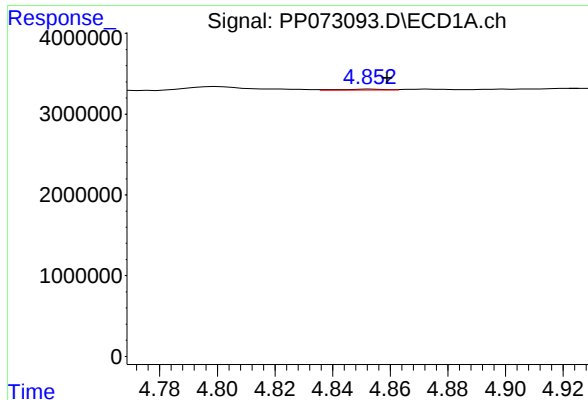

#11 AR-1232-1


R.T.: 4.854 min
Delta R.T.: -0.005 min
Response: 131540
Conc: 2.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

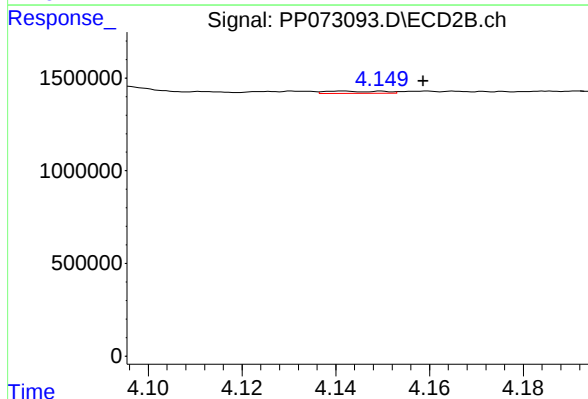


#11 AR-1232-1

R.T.: 4.141 min
Delta R.T.: -0.018 min
Response: 92975
Conc: 2.04 ng/ml

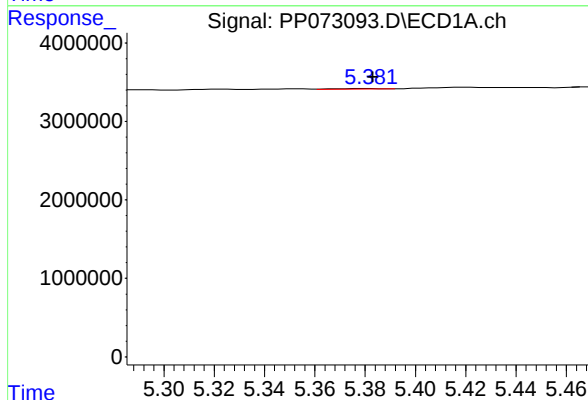


#12 AR-1232-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 91050
Conc: 4.07 ng/ml

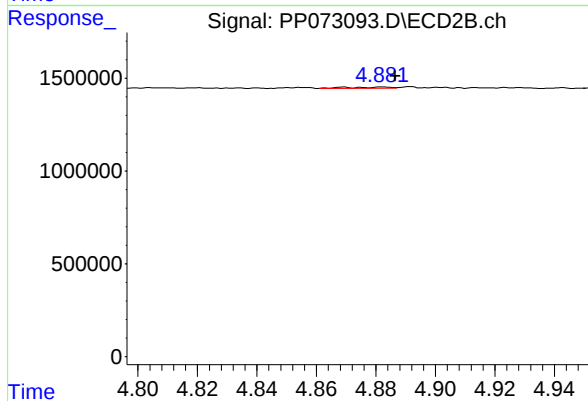

#12 AR-1232-2


R.T.: 4.882 min
Delta R.T.: -0.004 min
Response: 57877
Conc: 1.25 ng/ml

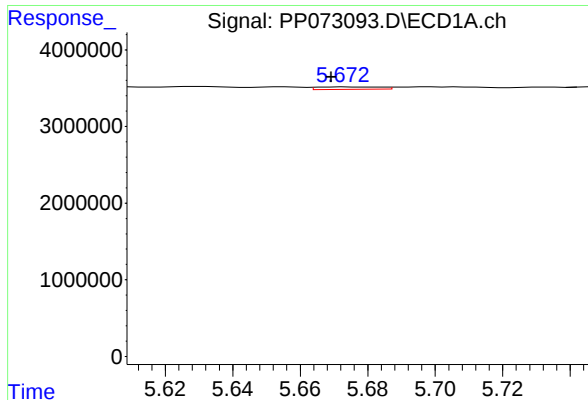

#13 AR-1232-3


R.T.: 5.673 min
Delta R.T.: 0.004 min
Response: 410983
Conc: 7.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

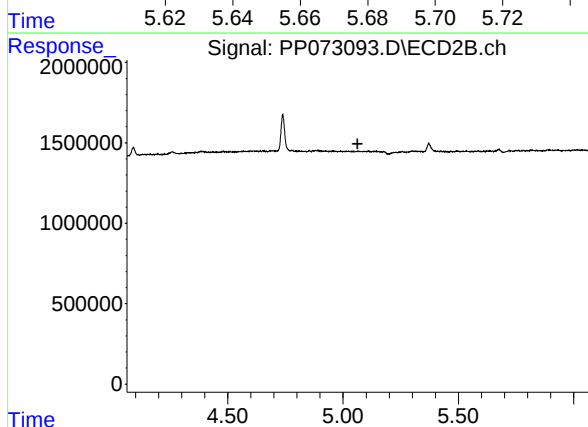


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 5.063 min
Response: 0
Conc: N.D.

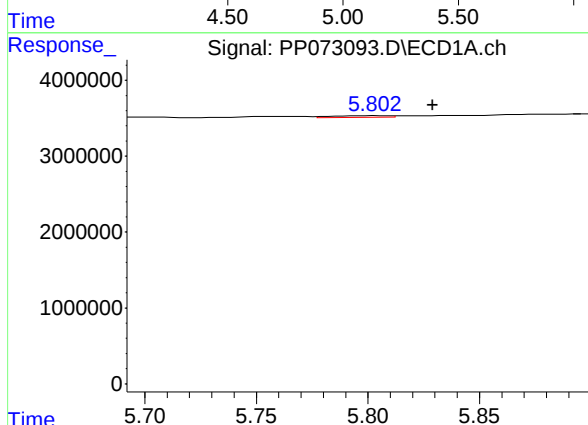


#14 AR-1232-4

R.T.: 5.803 min
Delta R.T.: -0.026 min
Response: 352102
Conc: 13.64 ng/ml

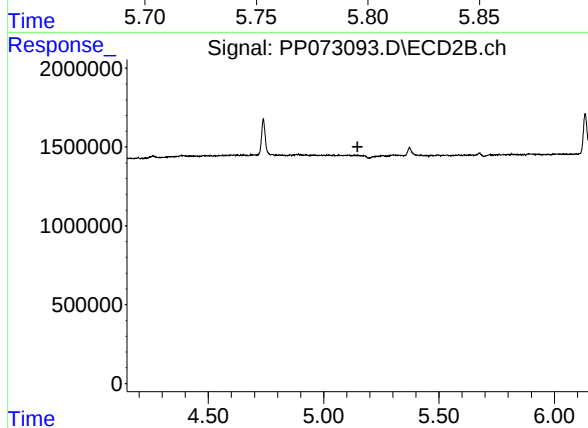

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.147 min
Response: 0
Conc: N.D.

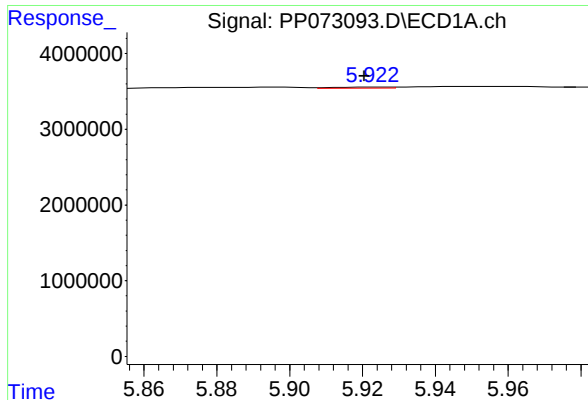

#15 AR-1232-5


R.T.: 5.924 min
Delta R.T.: 0.004 min
Response: 161486
Conc: 4.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

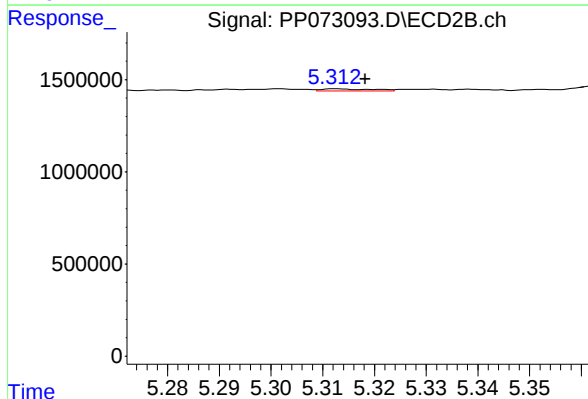


#15 AR-1232-5

R.T.: 5.313 min
Delta R.T.: -0.005 min
Response: 73643
Conc: 3.22 ng/ml

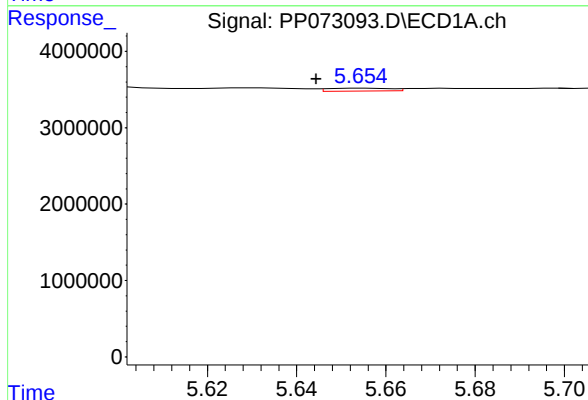


#16 AR-1242-1

R.T.: 5.655 min
Delta R.T.: 0.011 min
Response: 358290
Conc: 6.13 ng/ml

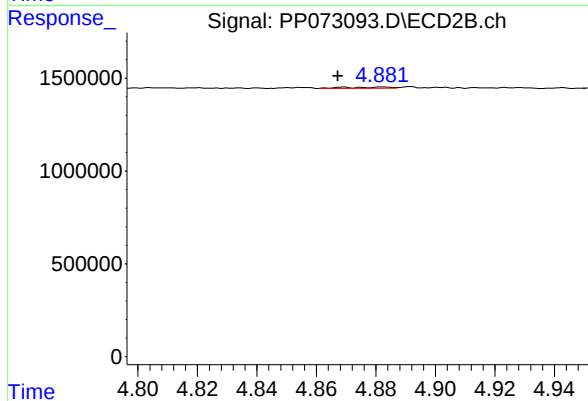

#16 AR-1242-1


R.T.: 4.882 min
Delta R.T.: 0.015 min
Response: 57877
Conc: 1.05 ng/ml

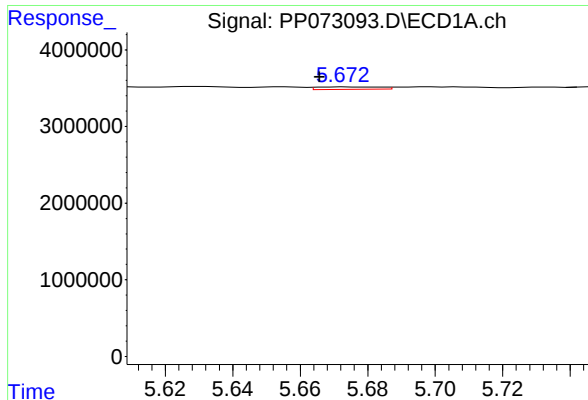

#17 AR-1242-2


R.T.: 5.673 min
Delta R.T.: 0.007 min
Response: 410983
Conc: 4.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

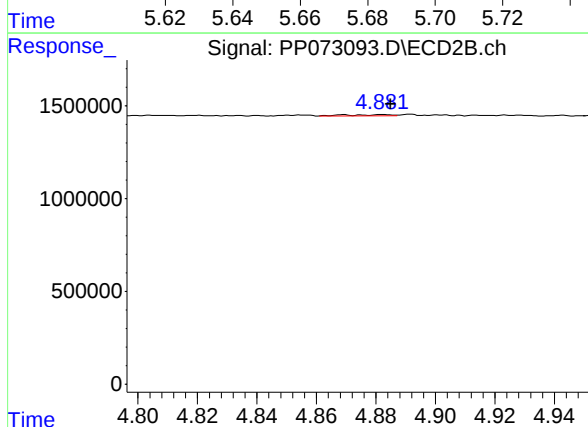


#17 AR-1242-2

R.T.: 4.882 min
Delta R.T.: -0.003 min
Response: 57877
Conc: 0.73 ng/ml

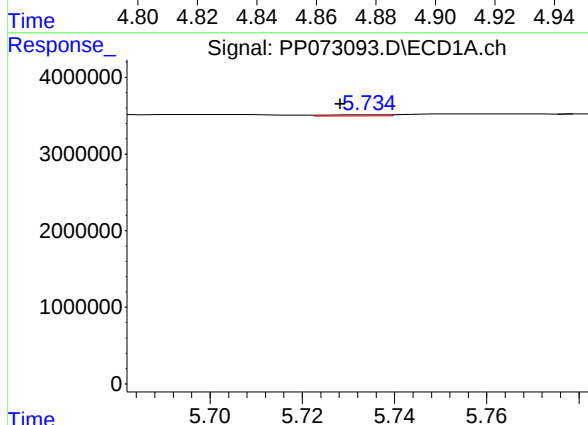


#18 AR-1242-3

R.T.: 5.734 min
Delta R.T.: 0.006 min
Response: 132437
Conc: 2.51 ng/ml

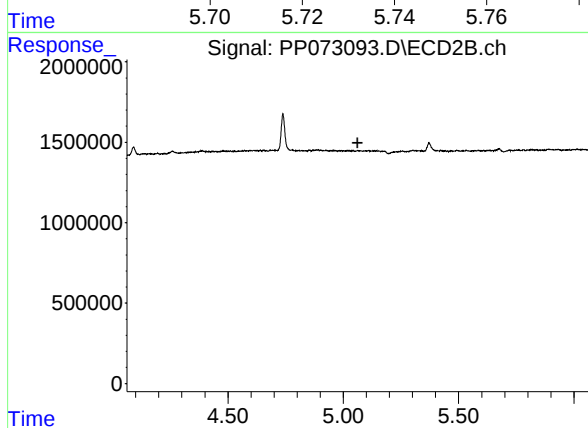

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 5.062 min
Response: 0
Conc: N.D.

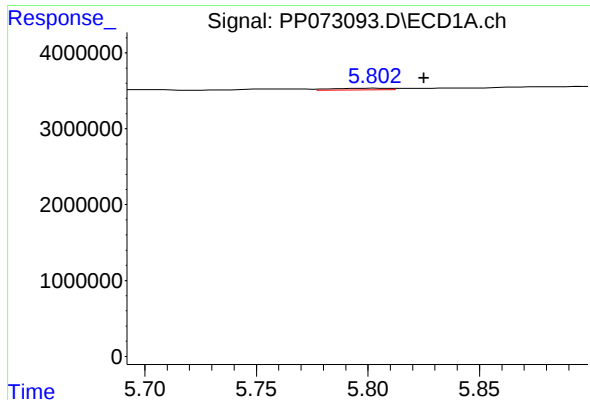

#19 AR-1242-4


R.T.: 5.803 min
Delta R.T.: -0.022 min
Response: 352102
Conc: 8.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

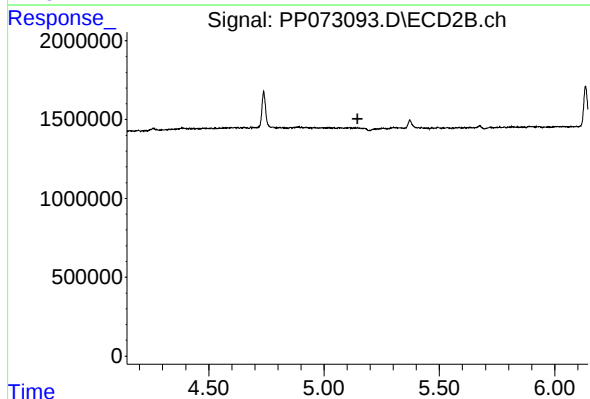


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.145 min
Response: 0
Conc: N.D.

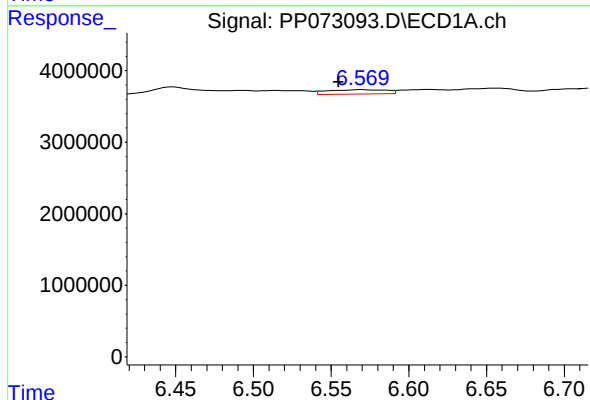


#20 AR-1242-5

R.T.: 6.571 min
Delta R.T.: 0.016 min
Response: 1624248
Conc: 32.77 ng/ml

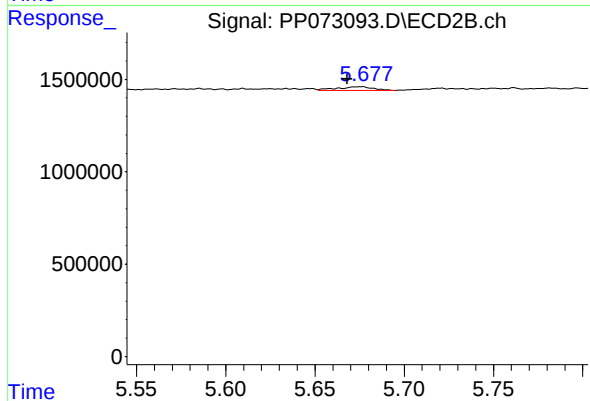

#20 AR-1242-5


R.T.: 5.676 min
Delta R.T.: 0.008 min
Response: 289757
Conc: 5.51 ng/ml

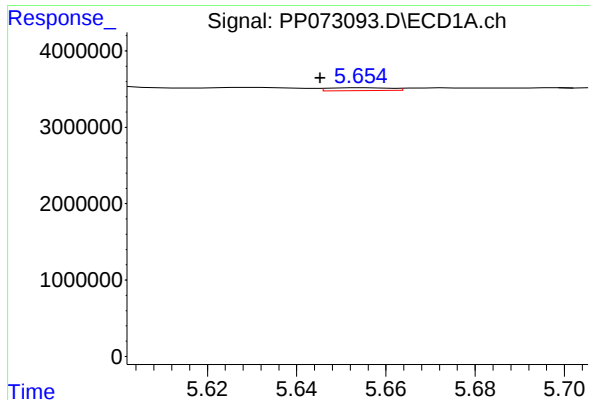

#21 AR-1248-1


R.T.: 5.655 min
Delta R.T.: 0.010 min
Response: 358290
Conc: 7.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

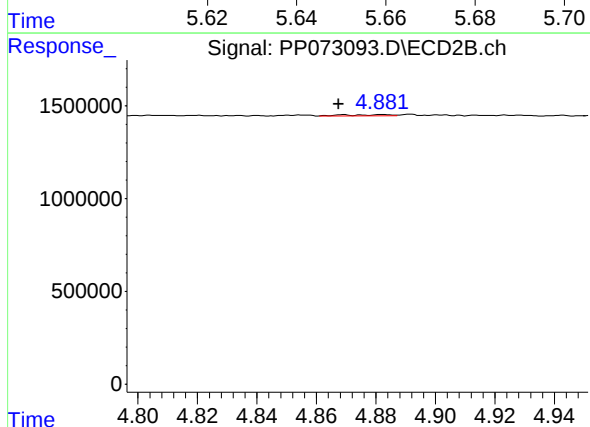


#21 AR-1248-1

R.T.: 4.882 min
Delta R.T.: 0.015 min
Response: 57877
Conc: 1.33 ng/ml

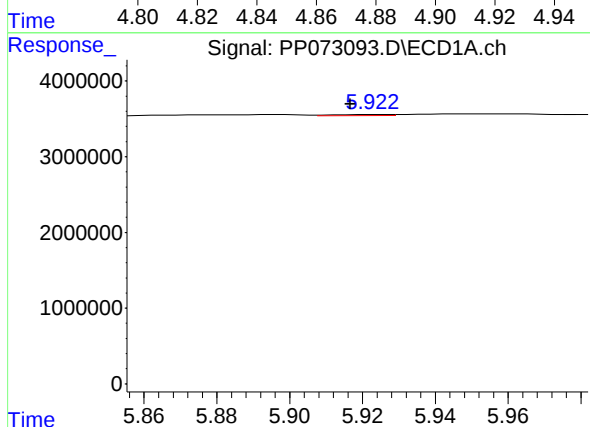


#22 AR-1248-2

R.T.: 5.924 min
Delta R.T.: 0.007 min
Response: 161486
Conc: 2.76 ng/ml

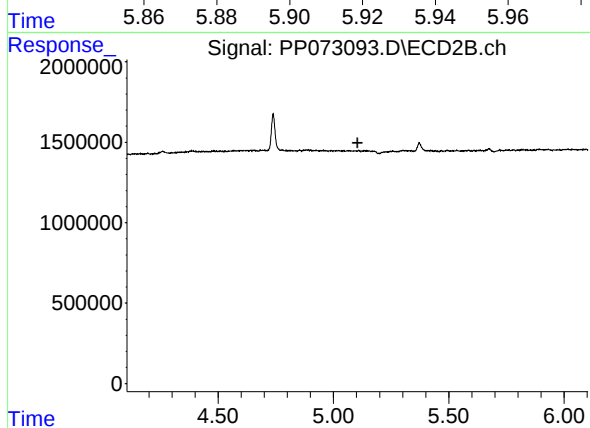

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.104 min
Response: 0
Conc: N.D.

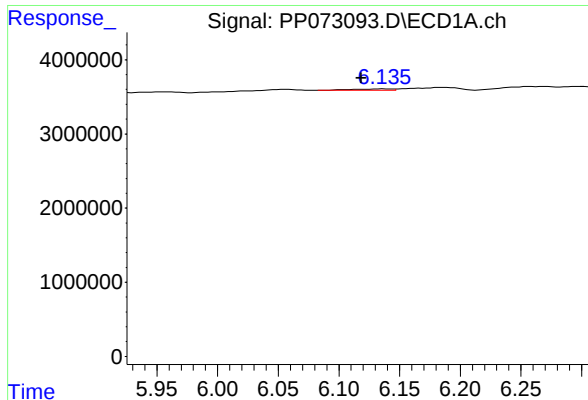

#23 AR-1248-3


R.T.: 6.137 min
Delta R.T.: 0.018 min
Response: 357215
Conc: 5.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

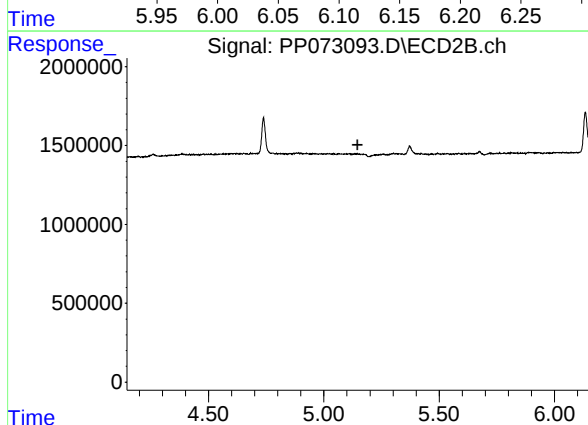


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 5.146 min
Response: 0
Conc: N.D.

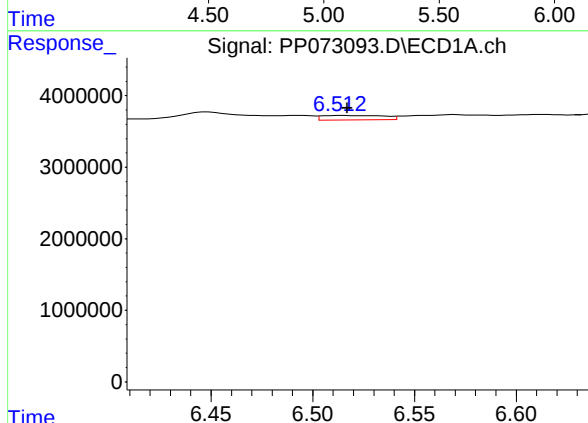


#24 AR-1248-4

R.T.: 6.515 min
Delta R.T.: -0.002 min
Response: 1324548
Conc: 15.57 ng/ml

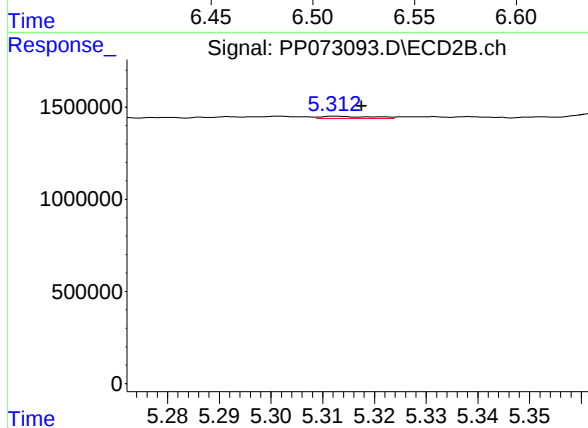

#24 AR-1248-4


R.T.: 5.313 min
Delta R.T.: -0.005 min
Response: 73643
Conc: 1.05 ng/ml

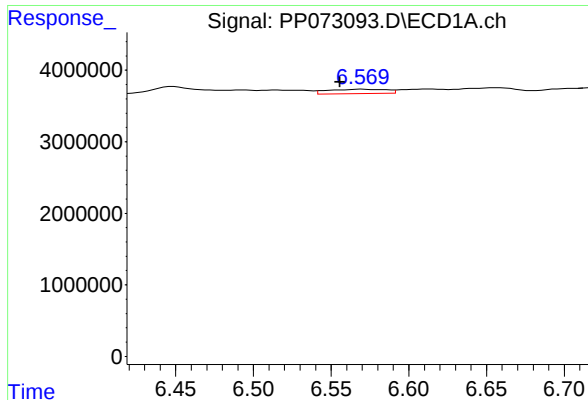

#25 AR-1248-5


R.T.: 6.571 min
Delta R.T.: 0.015 min
Response: 1624248
Conc: 19.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

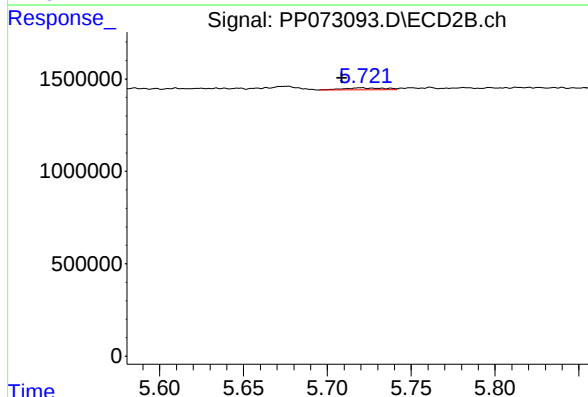


#25 AR-1248-5

R.T.: 5.720 min
Delta R.T.: 0.011 min
Response: 186577
Conc: 2.63 ng/ml

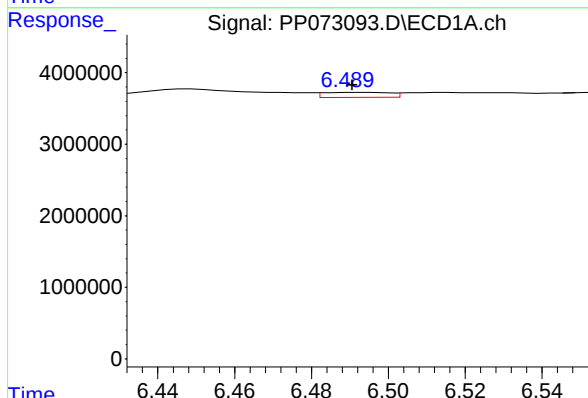


#26 AR-1254-1

R.T.: 6.492 min
Delta R.T.: 0.001 min
Response: 832421
Conc: 9.89 ng/ml

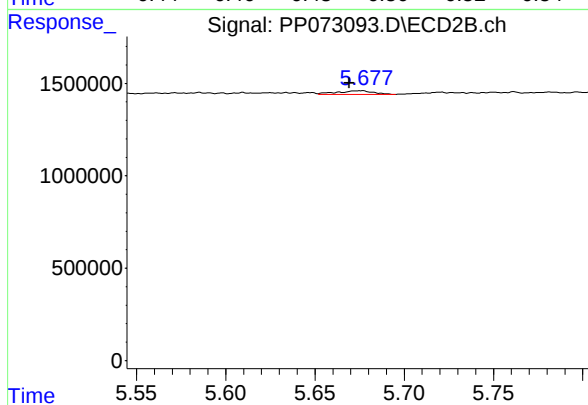

#26 AR-1254-1


R.T.: 5.676 min
Delta R.T.: 0.007 min
Response: 289757
Conc: 2.64 ng/ml

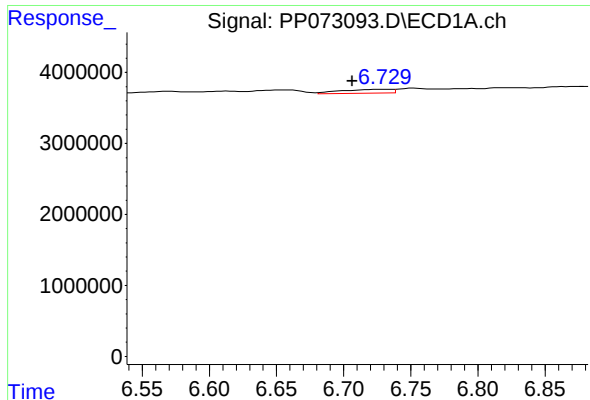

#27 AR-1254-2


R.T.: 6.731 min
Delta R.T.: 0.024 min
Response: 1436139
Conc: 11.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

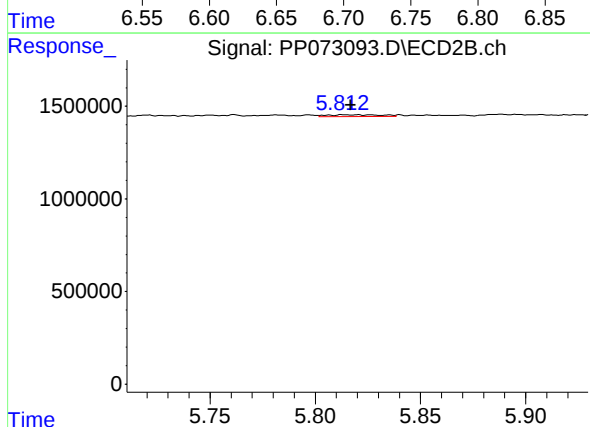


#27 AR-1254-2

R.T.: 5.814 min
Delta R.T.: -0.003 min
Response: 188852
Conc: 2.00 ng/ml

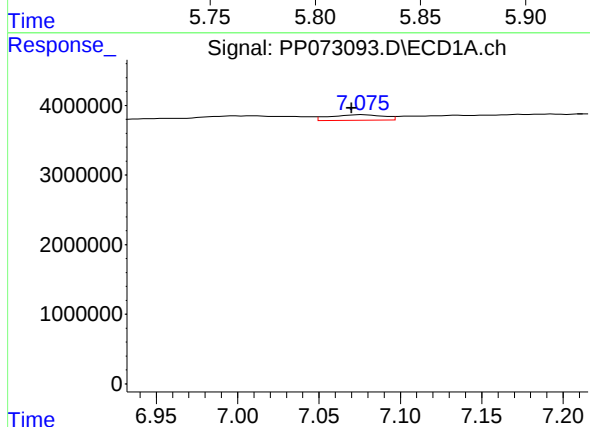


#28 AR-1254-3

R.T.: 7.077 min
Delta R.T.: 0.007 min
Response: 1821266
Conc: 13.88 ng/ml

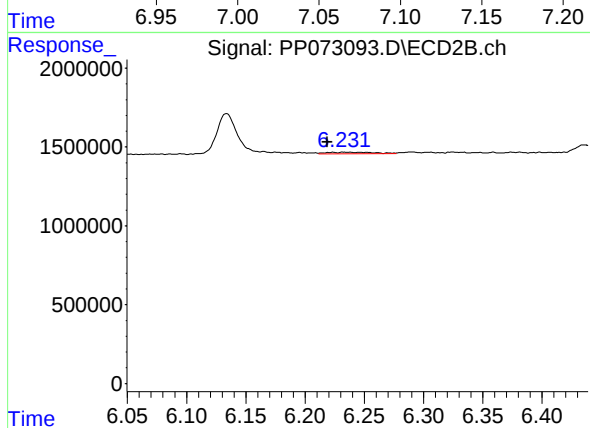

#28 AR-1254-3


R.T.: 6.238 min
Delta R.T.: 0.019 min
Response: 249818
Conc: 1.69 ng/ml

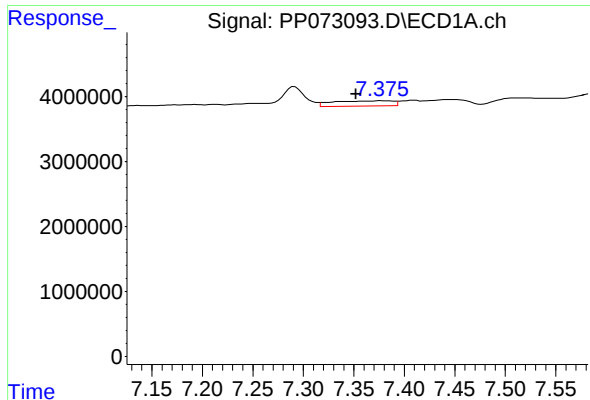

#29 AR-1254-4


R.T.: 7.378 min
Delta R.T.: 0.026 min
Response: 3315364
Conc: 27.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

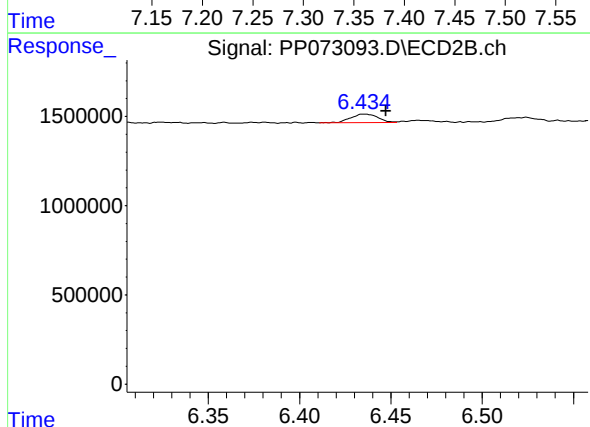


#29 AR-1254-4

R.T.: 6.436 min
Delta R.T.: -0.012 min
Response: 512255
Conc: 5.28 ng/ml

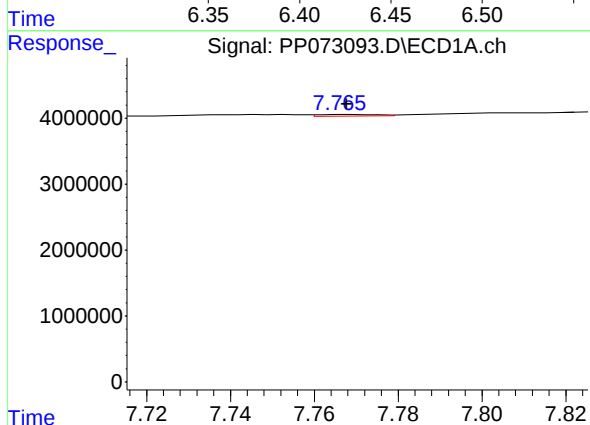


#30 AR-1254-5

R.T.: 7.768 min
Delta R.T.: 0.000 min
Response: 221704
Conc: 1.94 ng/ml

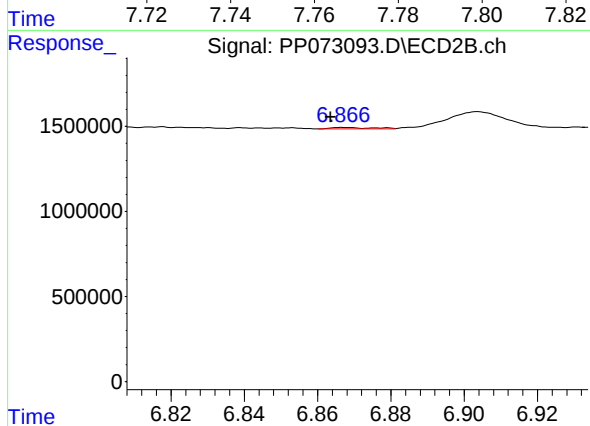

#30 AR-1254-5


R.T.: 6.867 min
Delta R.T.: 0.004 min
Response: 55450
Conc: 0.43 ng/ml

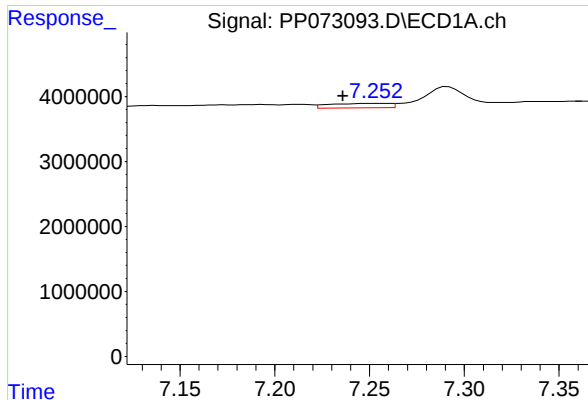

#31 AR-1260-1


R.T.: 7.253 min
Delta R.T.: 0.017 min
Response: 1488460
Conc: 16.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

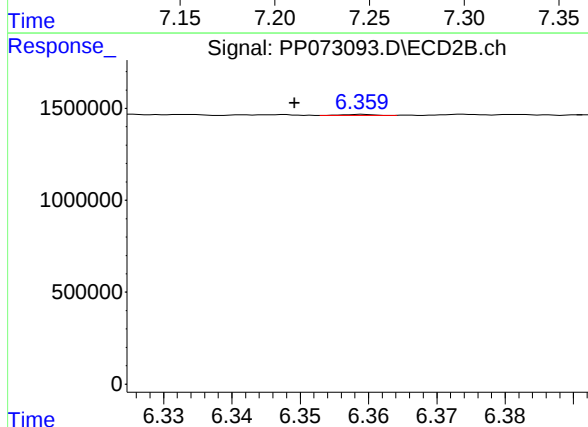


#31 AR-1260-1

R.T.: 6.359 min
Delta R.T.: 0.010 min
Response: 15263
Conc: 0.16 ng/ml

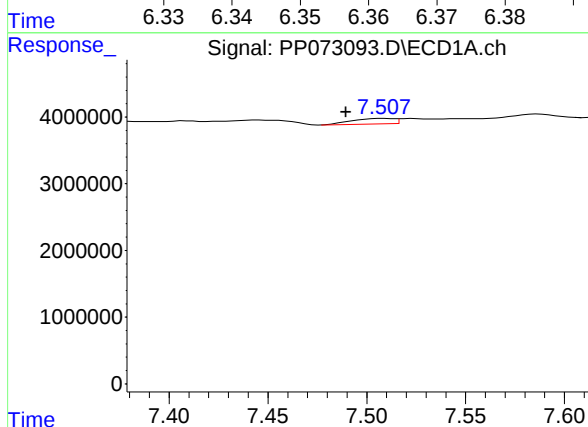


#32 AR-1260-2

R.T.: 7.509 min
Delta R.T.: 0.019 min
Response: 1246309
Conc: 9.17 ng/ml

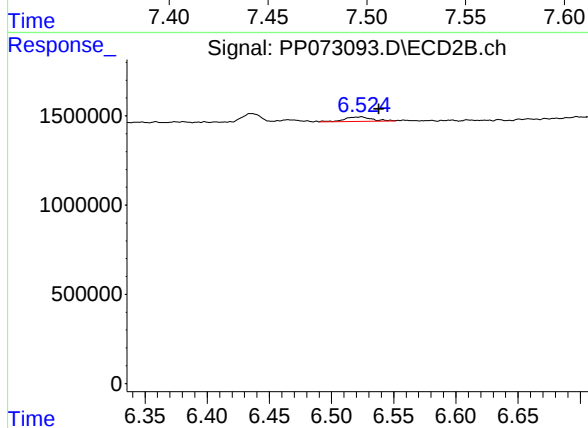

#32 AR-1260-2


R.T.: 6.524 min
Delta R.T.: -0.014 min
Response: 396348
Conc: 3.40 ng/ml

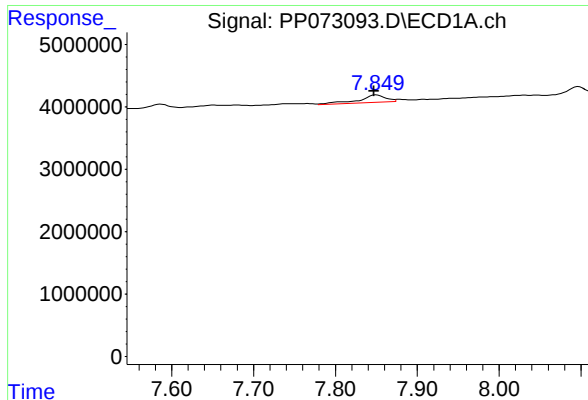

#33 AR-1260-3


R.T.: 7.850 min
Delta R.T.: 0.003 min
Response: 2659641
Conc: 23.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

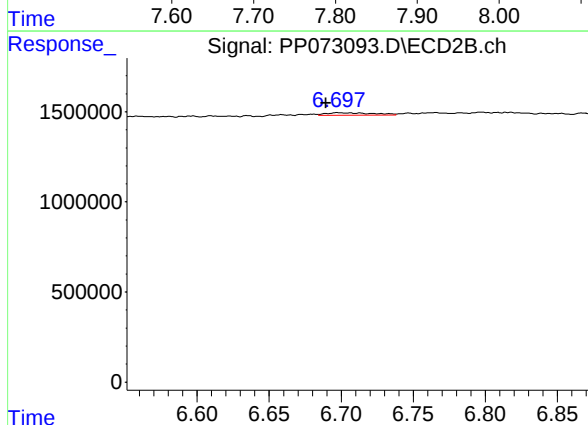


#33 AR-1260-3

R.T.: 6.697 min
Delta R.T.: 0.008 min
Response: 314875
Conc: 3.02 ng/ml

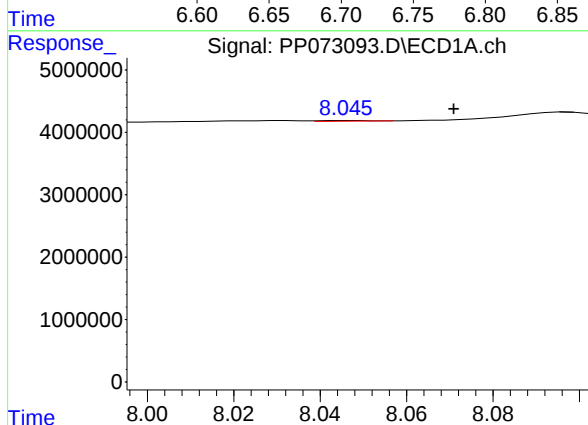


#34 AR-1260-4

R.T.: 8.048 min
Delta R.T.: -0.023 min
Response: 100325
Conc: 0.97 ng/ml

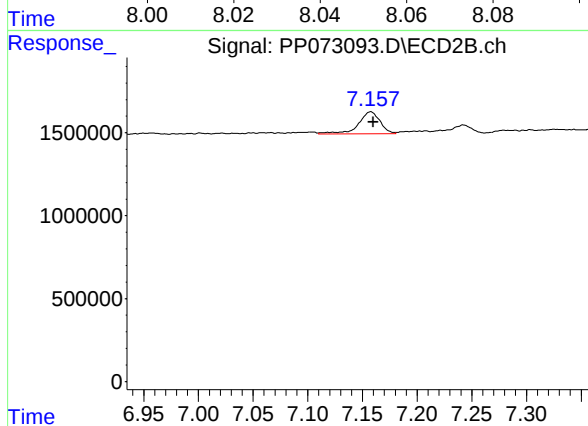

#34 AR-1260-4


R.T.: 7.158 min
Delta R.T.: -0.002 min
Response: 1799176
Conc: 20.51 ng/ml

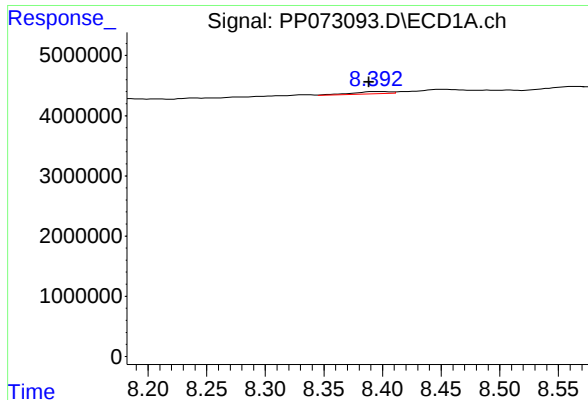

#35 AR-1260-5


R.T.: 8.395 min
Delta R.T.: 0.006 min
Response: 871846
Conc: 3.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

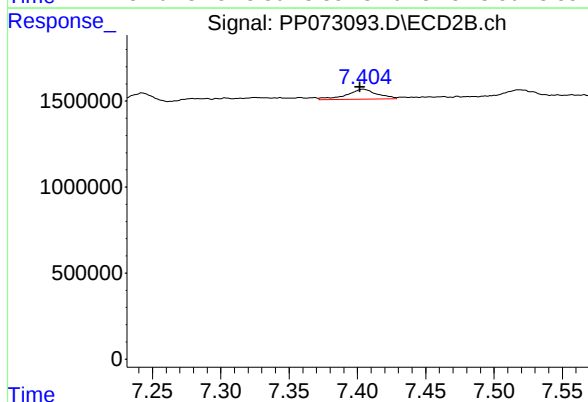


#35 AR-1260-5

R.T.: 7.404 min
Delta R.T.: 0.002 min
Response: 883427
Conc: 4.14 ng/ml

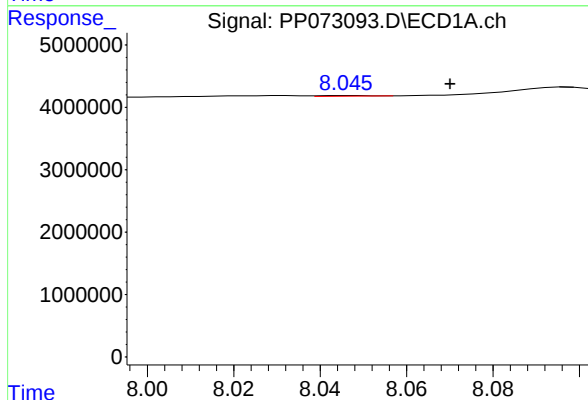


#36 AR-1262-1

R.T.: 8.048 min
Delta R.T.: -0.022 min
Response: 100325
Conc: 0.68 ng/ml

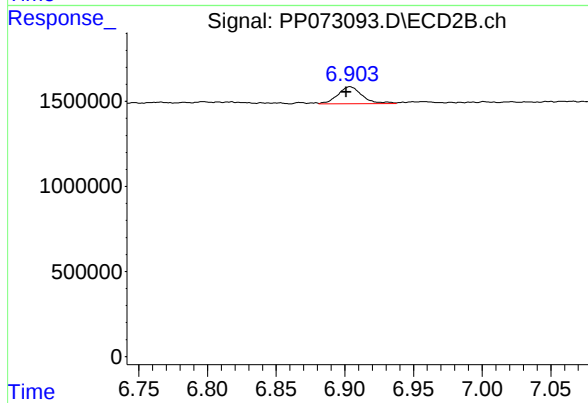

#36 AR-1262-1


R.T.: 6.904 min
Delta R.T.: 0.003 min
Response: 1212987
Conc: 8.40 ng/ml

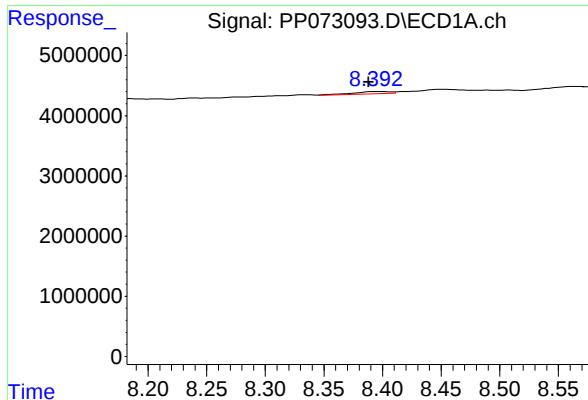

#37 AR-1262-2


R.T.: 8.395 min
Delta R.T.: 0.007 min
Response: 871846
Conc: 2.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

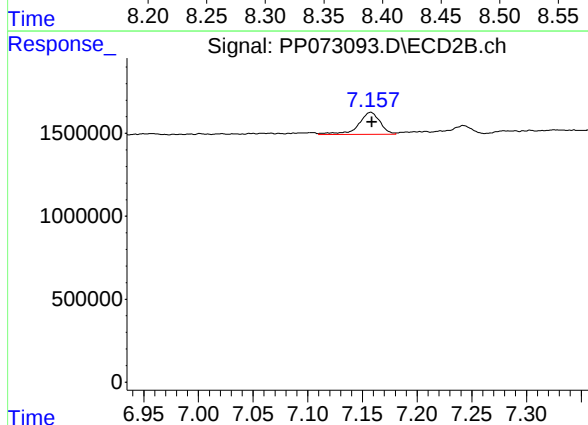


#37 AR-1262-2

R.T.: 7.158 min
Delta R.T.: -0.001 min
Response: 1799176
Conc: 14.72 ng/ml

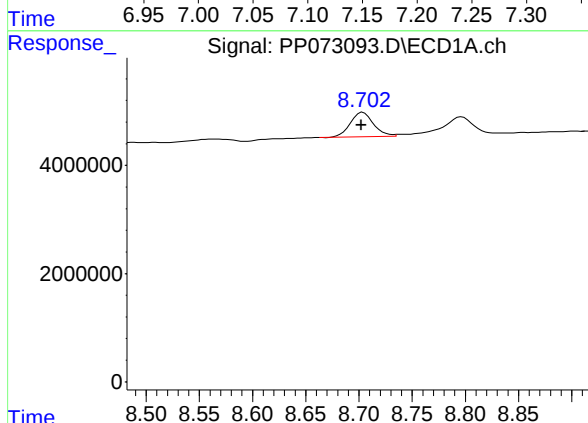


#38 AR-1262-3

R.T.: 8.704 min
Delta R.T.: 0.002 min
Response: 6851498
Conc: 32.02 ng/ml

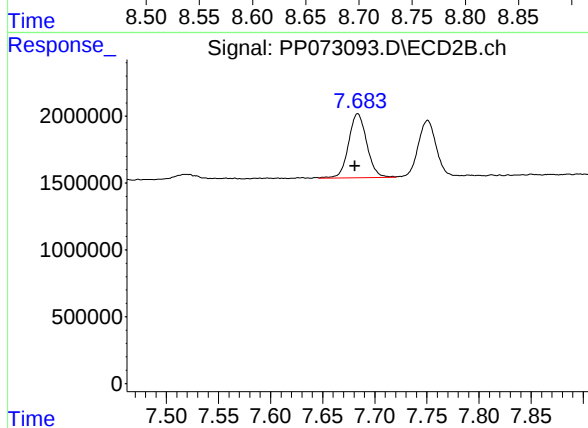

#38 AR-1262-3


R.T.: 7.684 min
Delta R.T.: 0.003 min
Response: 5844436
Conc: 51.86 ng/ml

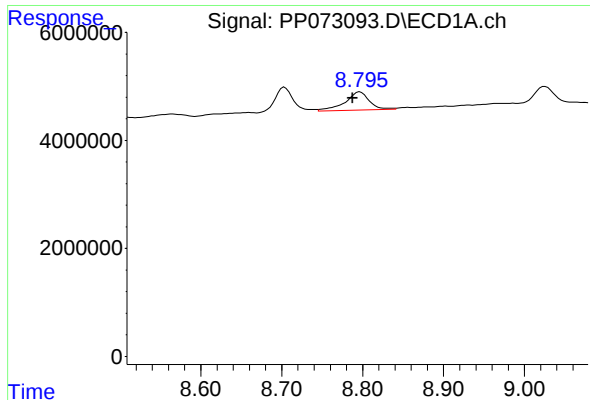

#39 AR-1262-4


R.T.: 8.797 min
Delta R.T.: 0.009 min
Response: 6966108
Conc: 44.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

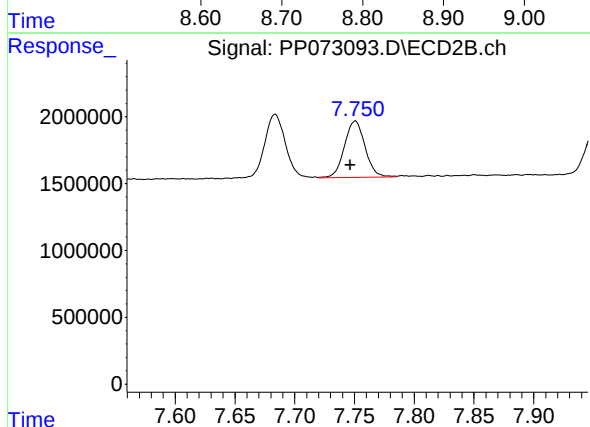


#39 AR-1262-4

R.T.: 7.751 min
Delta R.T.: 0.004 min
Response: 5100747
Conc: 27.82 ng/ml

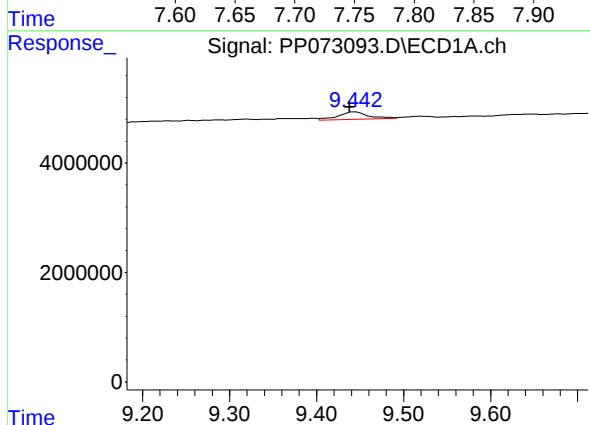


#40 AR-1262-5

R.T.: 9.443 min
Delta R.T.: 0.006 min
Response: 3268108
Conc: 29.22 ng/ml

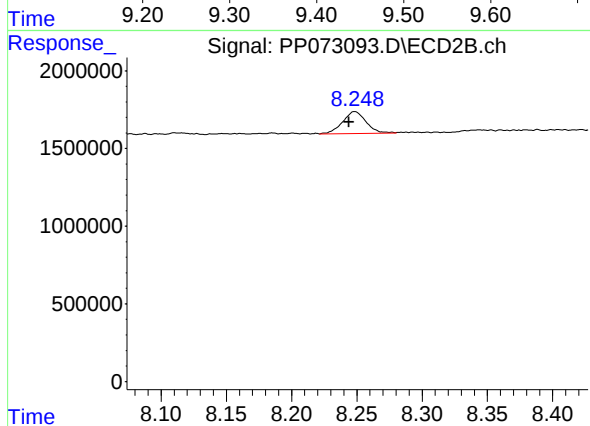

#40 AR-1262-5


R.T.: 8.248 min
Delta R.T.: 0.005 min
Response: 1788105
Conc: 20.65 ng/ml

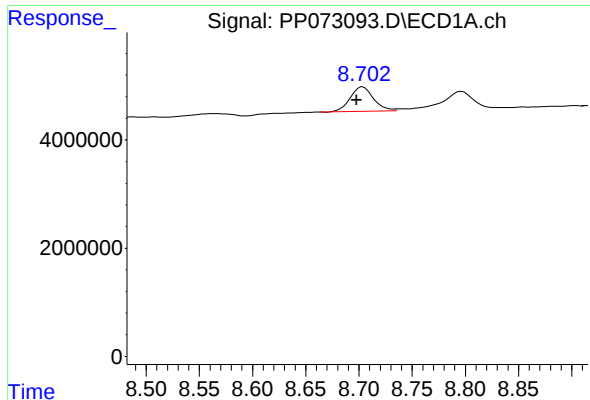

#41 AR-1268-1


R.T.: 8.704 min
Delta R.T.: 0.006 min
Response: 6851498
Conc: 19.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

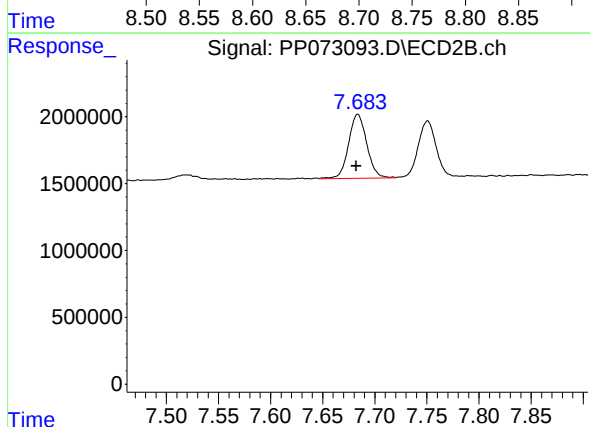


#41 AR-1268-1

R.T.: 7.684 min
Delta R.T.: 0.001 min
Response: 5844436
Conc: 20.35 ng/ml

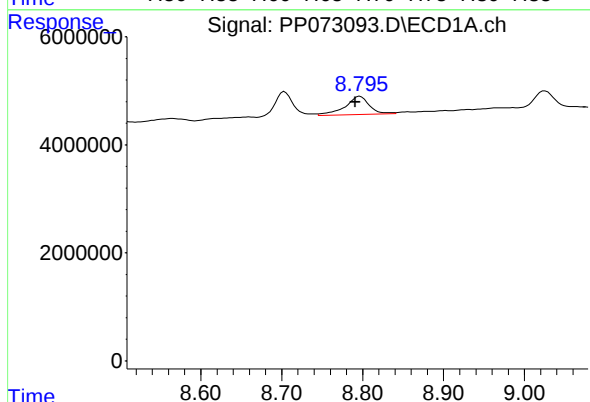


#42 AR-1268-2

R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 6966108
Conc: 22.84 ng/ml

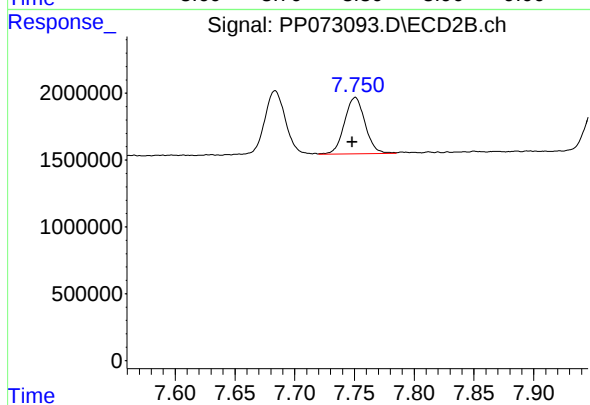

#42 AR-1268-2


R.T.: 7.751 min
Delta R.T.: 0.002 min
Response: 5100747
Conc: 19.84 ng/ml

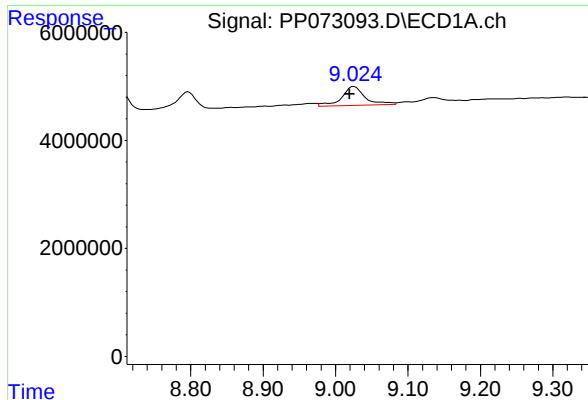

#43 AR-1268-3


R.T.: 9.025 min
Delta R.T.: 0.006 min
Response: 7928360
Conc: 29.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

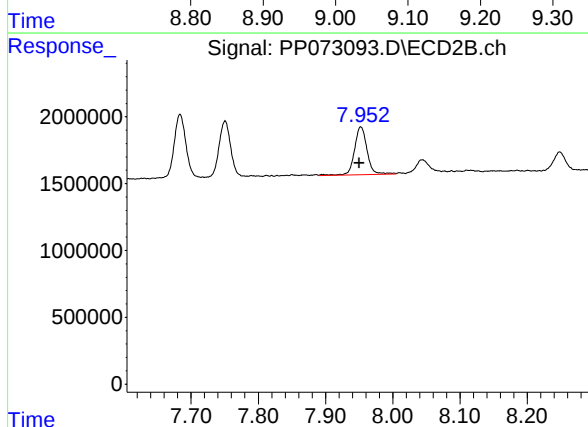


#43 AR-1268-3

R.T.: 7.952 min
Delta R.T.: 0.002 min
Response: 4694824
Conc: 21.74 ng/ml

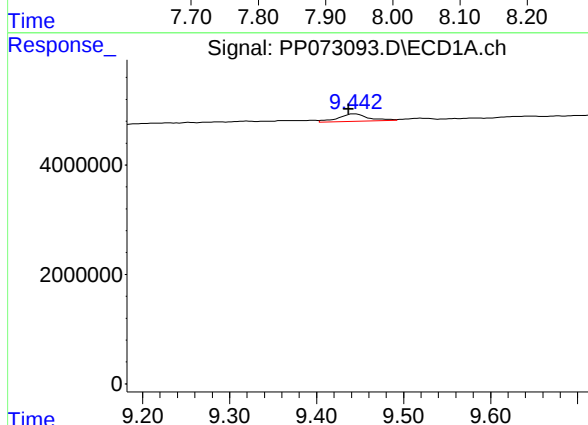


#44 AR-1268-4

R.T.: 9.443 min
Delta R.T.: 0.007 min
Response: 3268108
Conc: 27.93 ng/ml

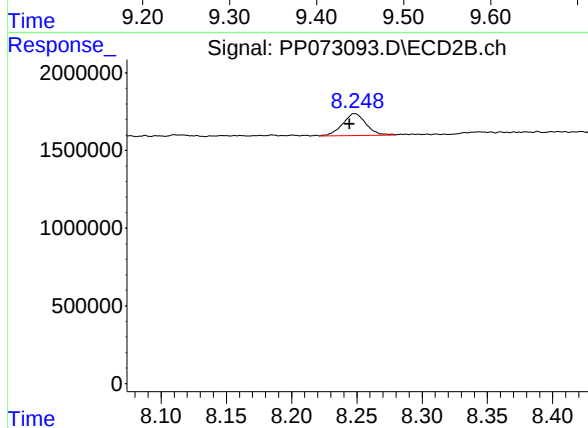

#44 AR-1268-4


R.T.: 8.248 min
Delta R.T.: 0.004 min
Response: 1788105
Conc: 18.98 ng/ml

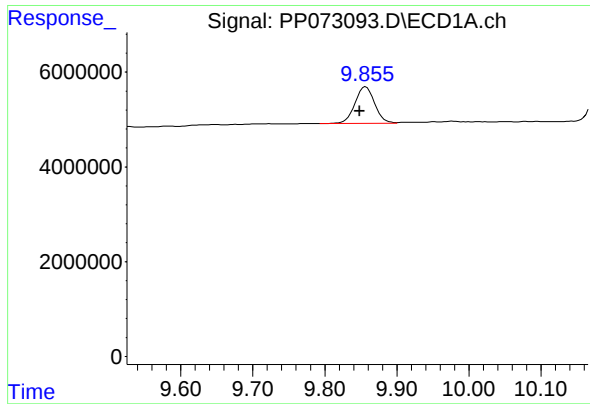

#45 AR-1268-5

R.T.: 9.857 min
Delta R.T.: 0.008 min
Response: 14807140
Conc: 20.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

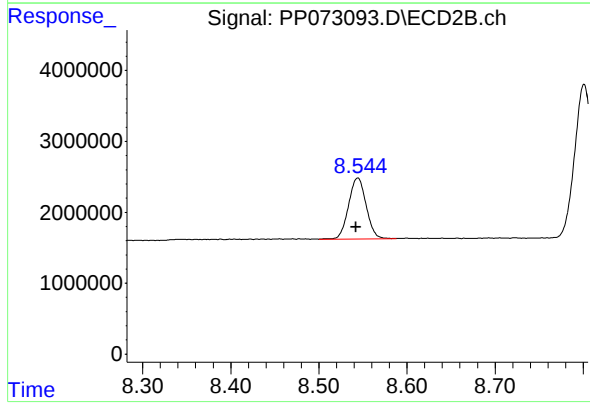

#45 AR-1268-5

R.T.: 8.544 min
Delta R.T.: 0.002 min
Response: 11979579
Conc: 20.70 ng/ml