

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
 Data File : PP073087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 17:05
 Operator : YP\AJ
 Sample : Q2126-09
 Misc : (Sig #1); AR1221 MDL 25 PPB (Sig #2)
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 23:27:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 18 08:17:15 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.495	3.789	43074357	37597423	20.407	20.867
2)	SA Decachlor...	10.191	8.800	40859217	29524003	23.910	22.120
Target Compounds							
8)	L2 AR-1221-1	4.698	4.001	558426	801112	22.646	29.812 #
9)	L2 AR-1221-2	4.792	4.087	768071	730626	38.063m	36.196m
10)	L2 AR-1221-3	4.859	4.161	1526600	1635649	24.802	27.849



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP061925\
Data File : PP073087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 17:05
Operator : YP\AJ
Sample : Q2126-09
Misc : (Sig #1); AR1221 MDL 25 PPB (Sig #2)
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 23:27:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP061725.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 18 08:17:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

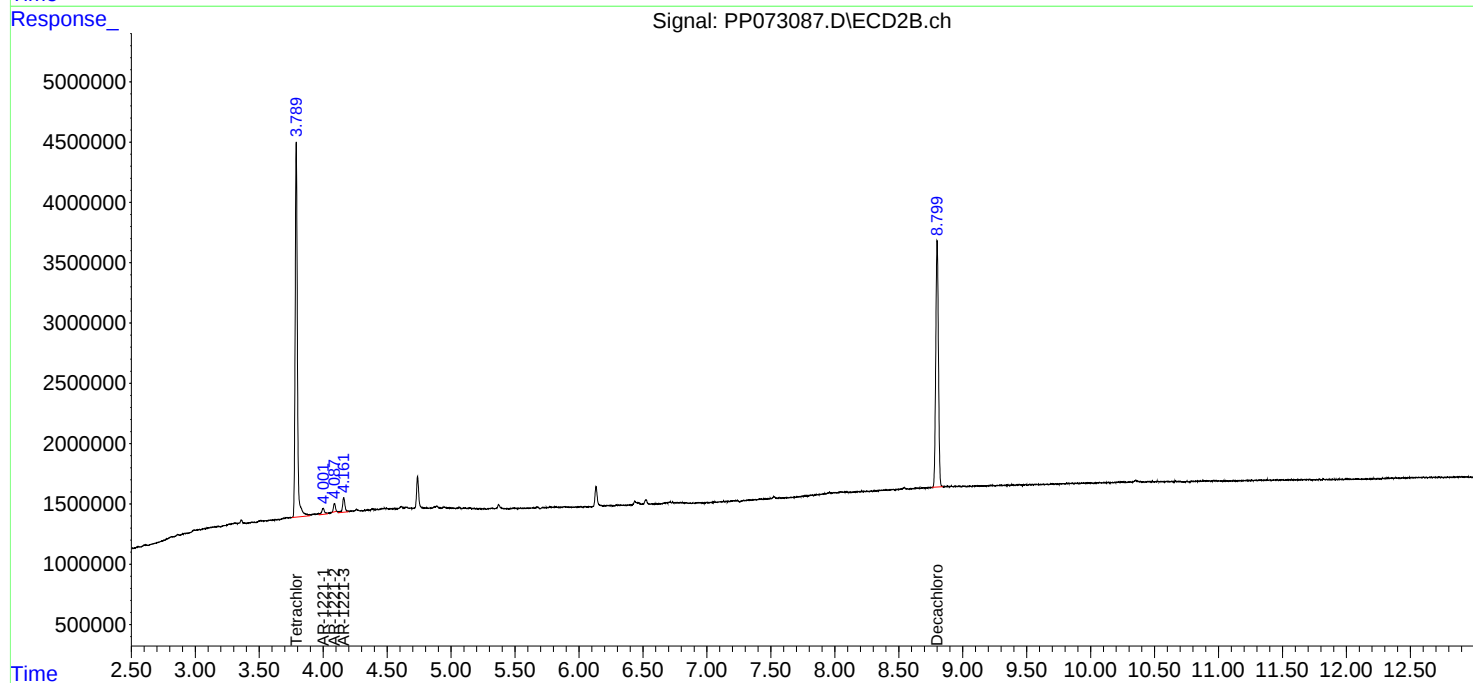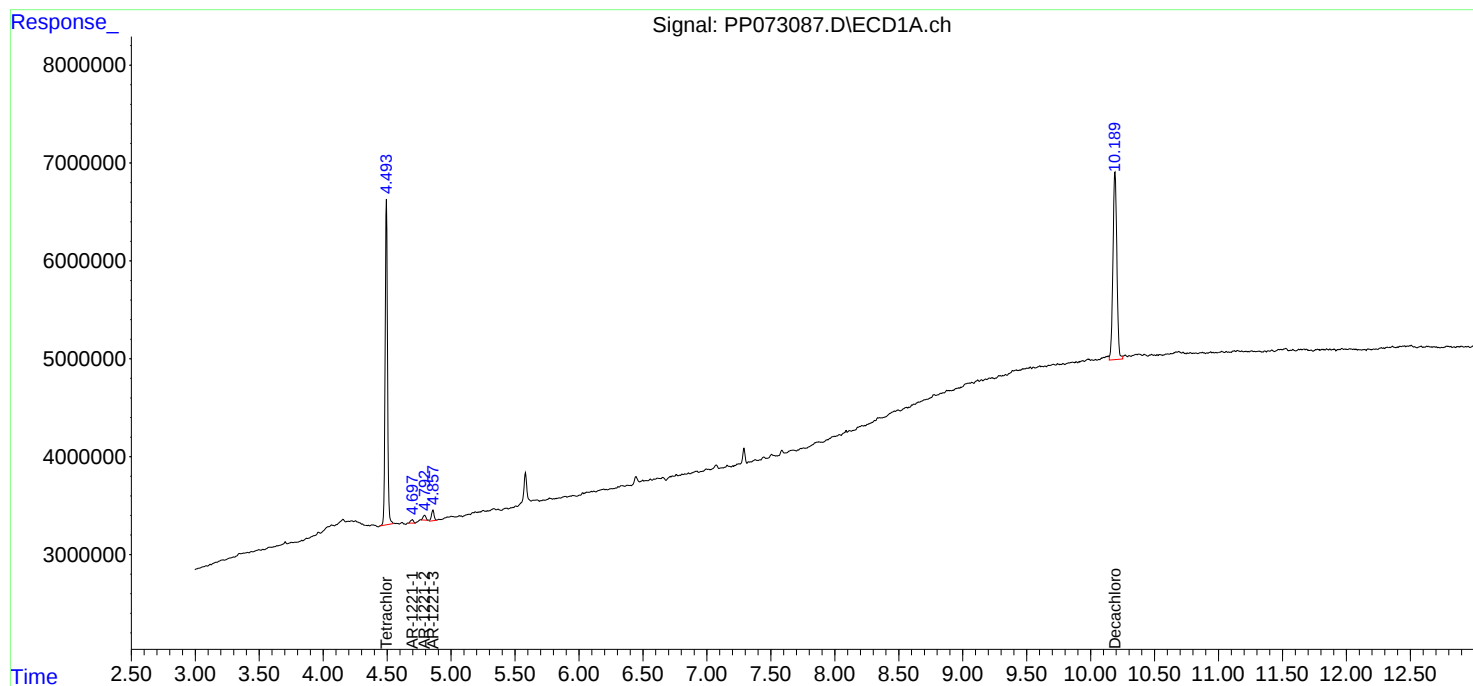


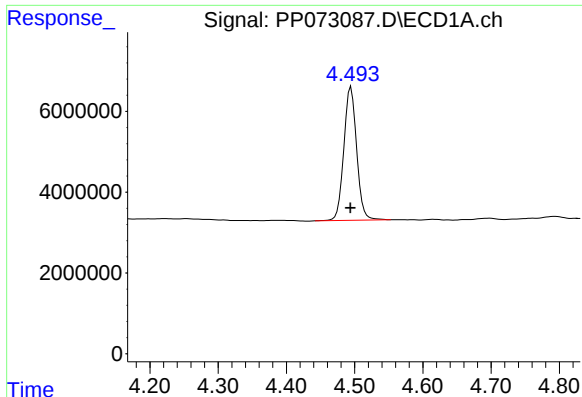

#1 Tetrachloro-m-xylene


R.T.: 4.495 min
Delta R.T.: 0.000 min
Response: 43074357
Conc: 20.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

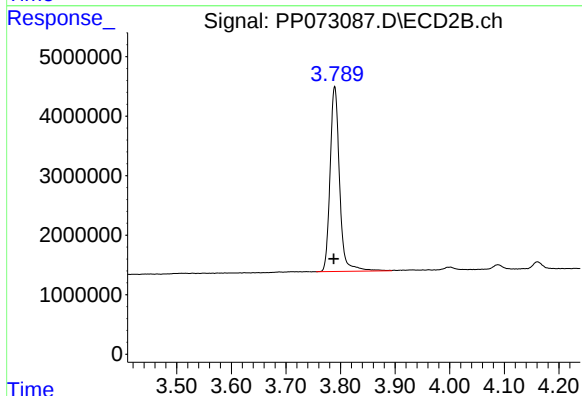


#1 Tetrachloro-m-xylene

R.T.: 3.789 min
Delta R.T.: 0.002 min
Response: 37597423
Conc: 20.87 ng/ml

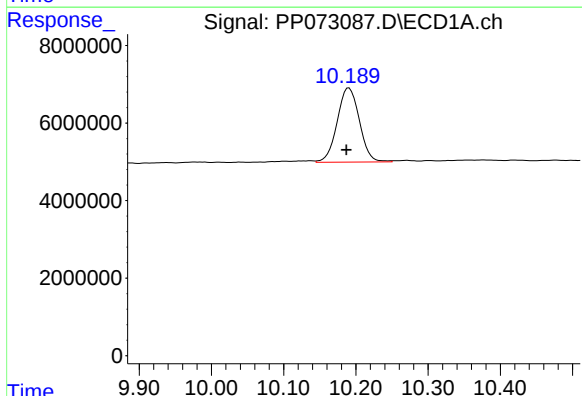


#2 Decachlorobiphenyl

R.T.: 10.191 min
Delta R.T.: 0.003 min
Response: 40859217
Conc: 23.91 ng/ml

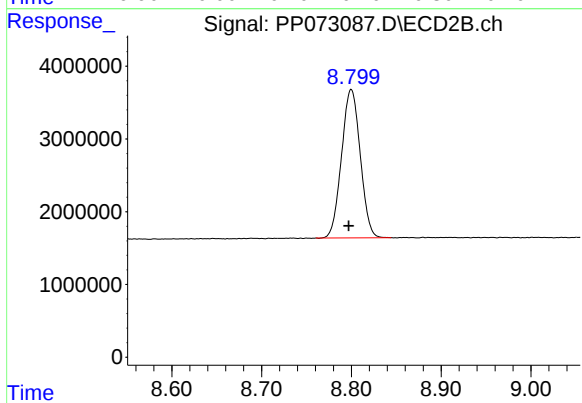

#2 Decachlorobiphenyl


R.T.: 8.800 min
Delta R.T.: 0.003 min
Response: 29524003
Conc: 22.12 ng/ml

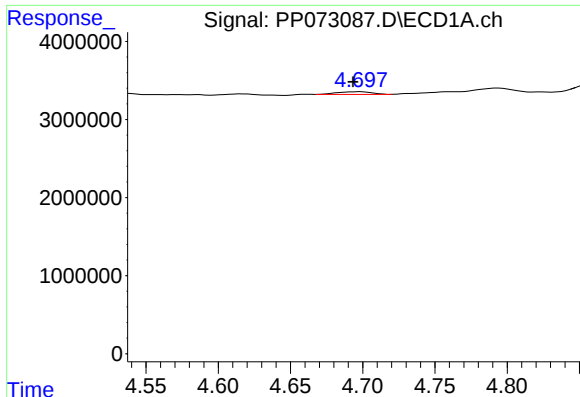

#8 AR-1221-1


R.T.: 4.698 min
Delta R.T.: 0.005 min
Response: 558426
Conc: 22.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

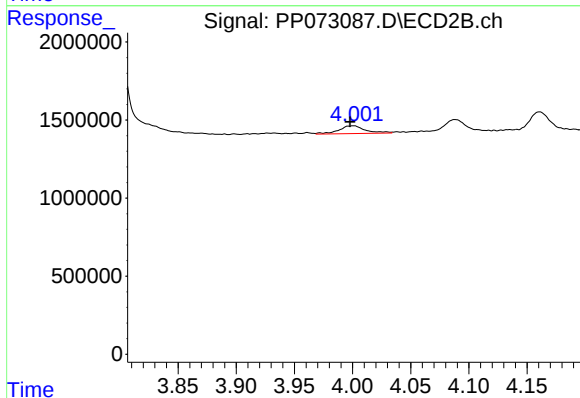


#8 AR-1221-1

R.T.: 4.001 min
Delta R.T.: 0.003 min
Response: 801112
Conc: 29.81 ng/ml

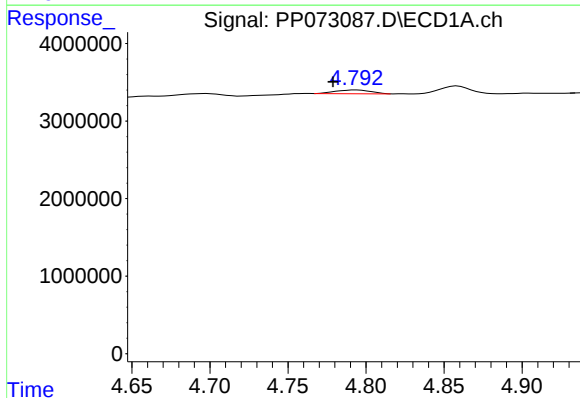


#9 AR-1221-2

R.T.: 4.792 min
Delta R.T.: 0.013 min
Response: 768071
Conc: 38.06 ng/ml m

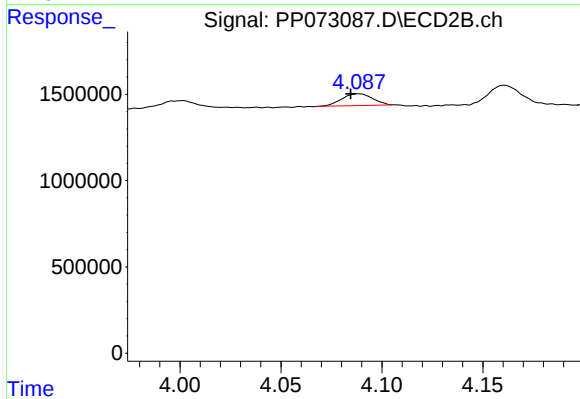

#9 AR-1221-2


R.T.: 4.087 min
Delta R.T.: 0.003 min
Response: 730626
Conc: 36.20 ng/ml m

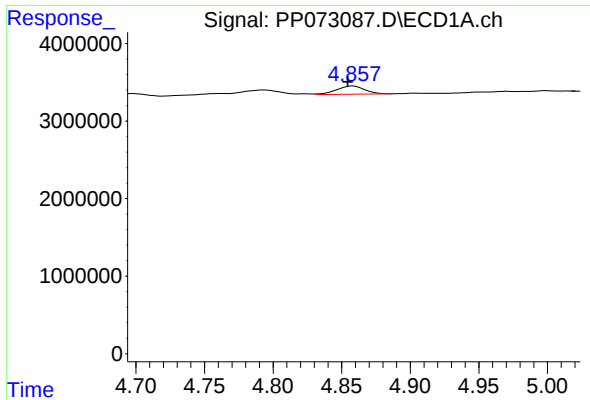

#10 AR-1221-3

R.T.: 4.859 min
Delta R.T.: 0.004 min
Response: 1526600
Conc: 24.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2025

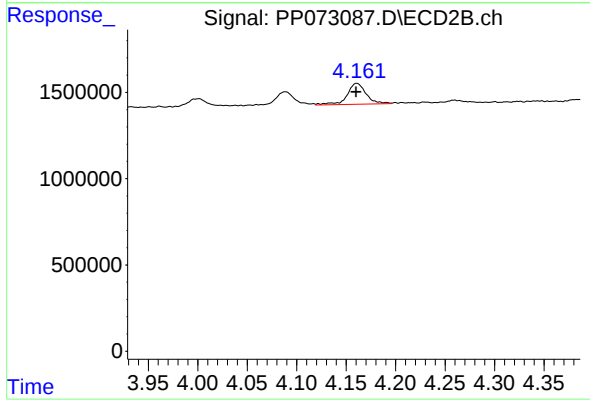

#10 AR-1221-3

R.T.: 4.161 min
Delta R.T.: 0.000 min
Response: 1635649
Conc: 27.85 ng/ml