

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP062018.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 18:51
 Operator : UA/AJ
 Sample : PB110343BSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB110343BSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 05:23:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 05:10:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.063	4.151	1466618	3598785	16.036	15.699
2) SA Decachlor...	8.334	8.979	2909710	2650099	19.266	16.507
Target Compounds						
3) L1 Aroclor-1...	4.569	4.506	180703	208398	78.983	53.319 #
4) L1 Aroclor-1...	4.996	4.977	117779	207574	44.462	71.600 #
5) L1 Aroclor-1...	4.996	5.298	117779	175093	64.870	29.828 #
6) L1 Aroclor-1...	5.289	5.354	183986	151293	150.244	39.819 #
7) L1 Aroclor-1...	0.000	5.599	0	105109	N.D.	26.287 #
8) L2 Aroclor-1...	0.000	4.426	0	98899	N.D.	137.745 #
9) L2 Aroclor-1...	4.347	4.426	3428490	98899	3691.683	313.018 #
10) L2 Aroclor-1...	4.347	4.476	3428490	148181	983.349	183.238 #
11) L3 Aroclor-1...	4.569	4.948	180703	182198	73.570	86.572
12) L3 Aroclor-1...	4.996	5.219	117779	266843	42.856	49.705
13) L3 Aroclor-1...	4.996	5.219	117779	266843	61.051	1158.536 #
14) L3 Aroclor-1...	5.289	5.563	183986	184785	143.031	47.336 #
15) L3 Aroclor-1...	0.000	5.879	0	144172	N.D.	96.199 #
16) L4 Aroclor-1...	4.569	4.793	180703	440241	73.570	62.618
17) L4 Aroclor-1...	4.901	5.119	283683	752198	47.391	53.606
18) L4 Aroclor-1...	4.996	5.219	117779	266843	42.856	1158.536 #
19) L4 Aroclor-1...	5.289	5.563	183986	184785	75.861	47.336 #
20) L4 Aroclor-1...	0.000	5.657	0	227942	N.D.	59.240 #
21) L5 Aroclor-1...	5.289	5.563	183986	184785	75.861	47.336 #
22) L5 Aroclor-1...	5.289	5.657	183986	227942	143.031	59.240 #
23) L5 Aroclor-1...	0.000	5.879	0	144172	N.D.	96.199 #
24) L5 Aroclor-1...	0.000	5.879	0	144172	N.D.	96.199 #
25) L5 Aroclor-1...	0.000	6.010	0	136143	N.D.	394.857 #
26) L6 Aroclor-1...	0.000	5.879	0	144172	N.D.	96.199 #
27) L6 Aroclor-1...	0.000	6.010	0	136143	N.D.	53.429 #
28) L6 Aroclor-1...	6.087	6.373	171045	87463	212.474	38.542 #
29) L6 Aroclor-1...	0.000	6.683	0	461349	N.D.	56.348 #
30) L6 Aroclor-1...	6.644	6.986	718409	712296	79.043	62.411
31) L7 Aroclor-1...	6.194	6.532	231235	416282	63.070	52.070
32) L7 Aroclor-1...	6.644	6.683	718409	461349	76.417	51.022 #
33) L7 Aroclor-1...	6.715	7.099	325311	151736	48.287	23.742 #
34) L7 Aroclor-1...	6.915	7.367	299601	242827	56.348	32.775 #
35) L7 Aroclor-1...	7.161	7.497	794469	703457	41.682	43.740
36) L8 Aroclor-1...	6.194	6.683	231235	461349	65.668	56.348
37) L8 Aroclor-1...	6.404	6.823	406693	233673	50.281	38.636
38) L8 Aroclor-1...	6.715	7.053	325311	391743	50.562	1817.817 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP026548.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 18:51
 Operator : UA/AJ
 Sample : PB110343BSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB110343BSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 05:23:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 05:10:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39)	L8 Aroclor-1...	6.915	7.306	299601	435326	56.382	66.221
40)	L8 Aroclor-1...	7.161	7.466	794469	153528	41.248	677.523 #
41)	L9 Aroclor-1...	7.397	7.819	914190	859805	72.999	3641.122 #
42)	L9 Aroclor-1...	7.462	7.819	303066	859805	60.414	75.415
44)	L9 Aroclor-1...	7.905	8.316	190090	301135	36.903	62.730 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 18:51
Operator : UA/AJ
Sample : PB110343BSD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 05:23:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 21 05:10:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

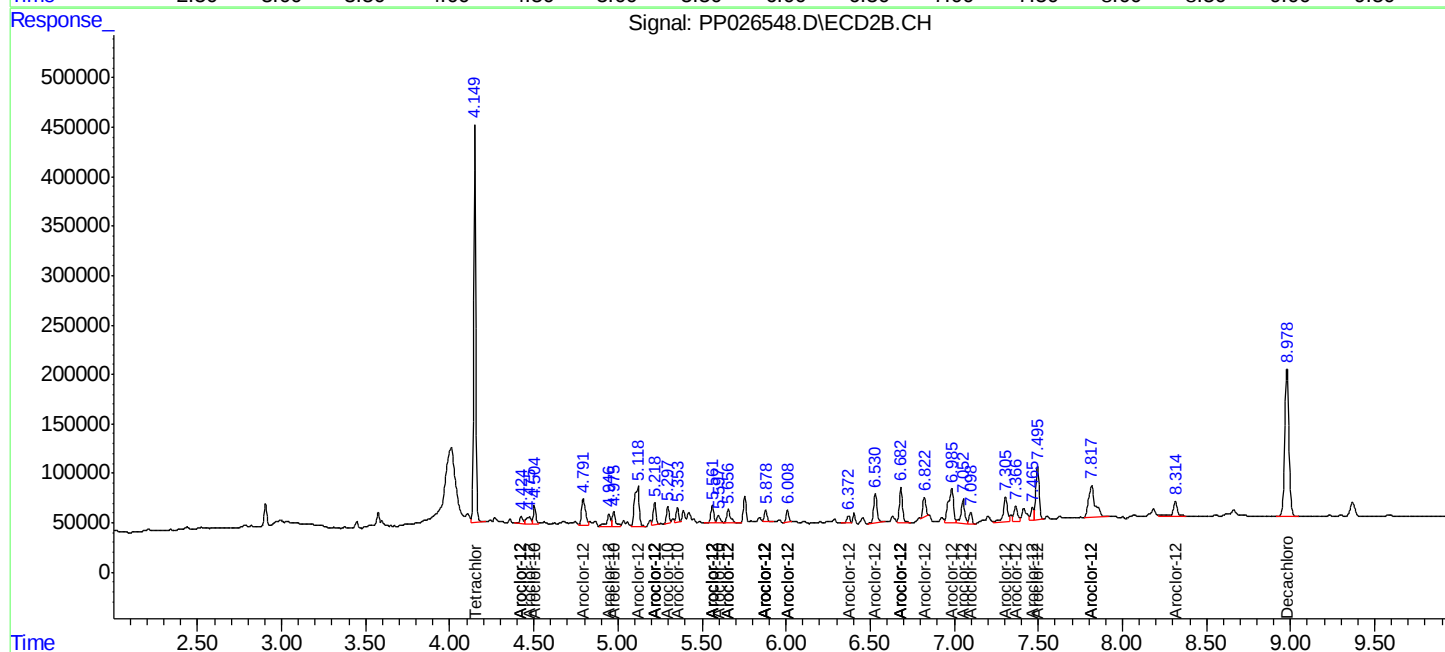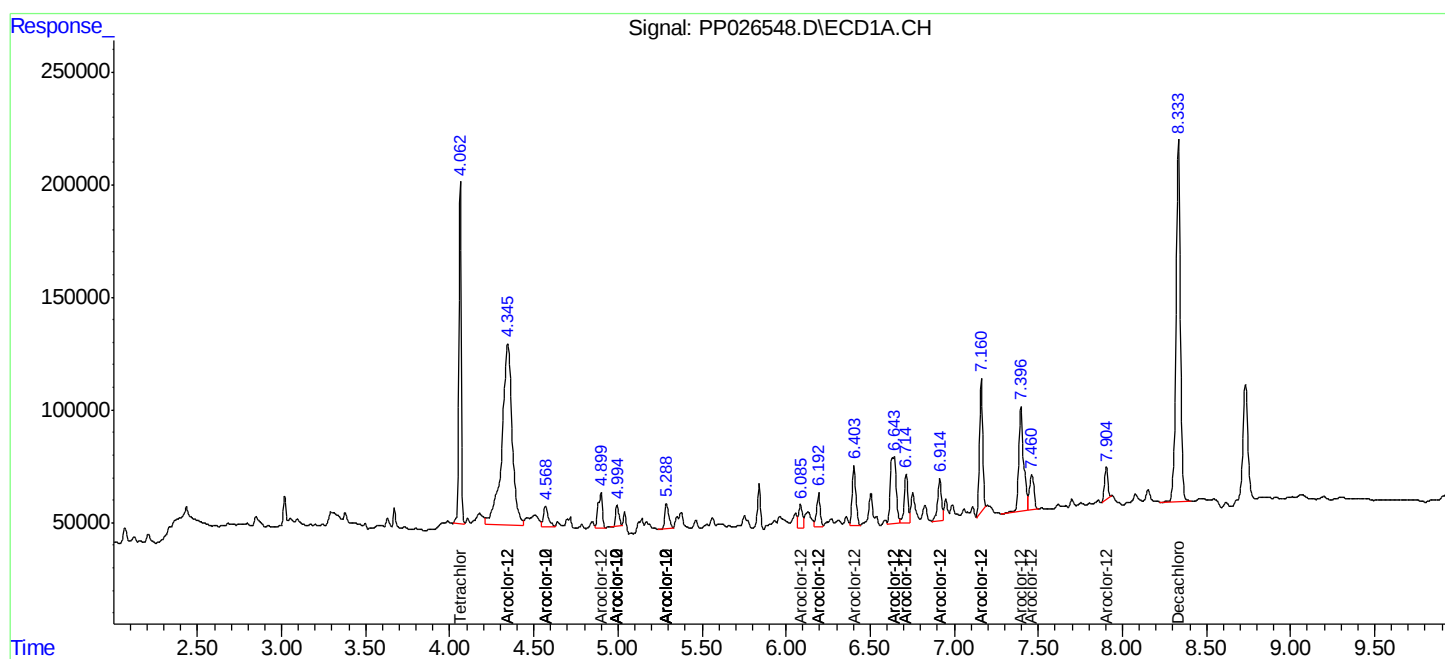


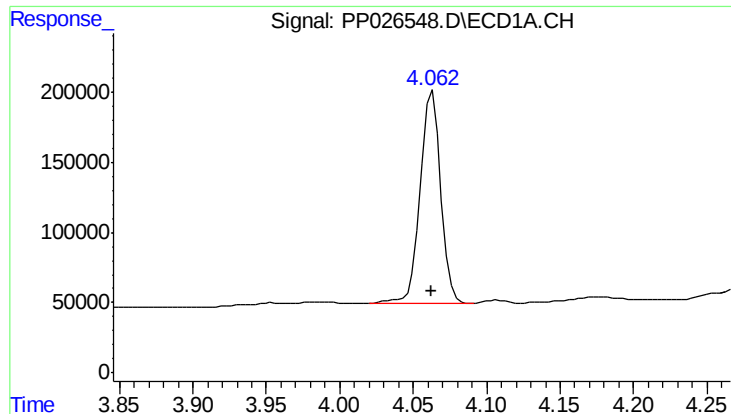

#1 Tetrachloro-m-xylene


R.T.: 4.063 min
Delta R.T.: 0.000 min
Response: 1466618
Conc: 16.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

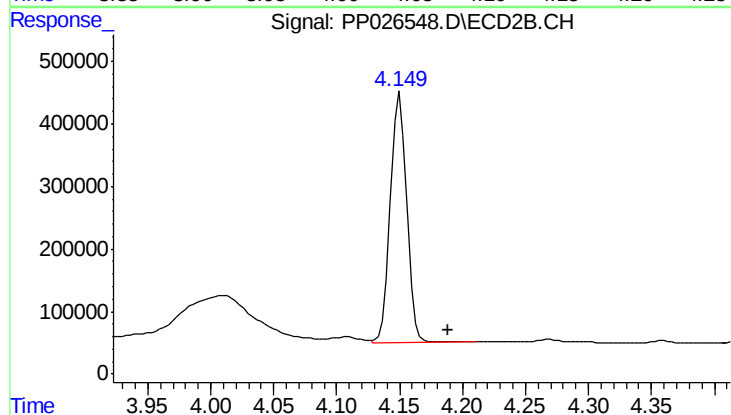


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.038 min
Response: 3598785
Conc: 15.70 ng/ml

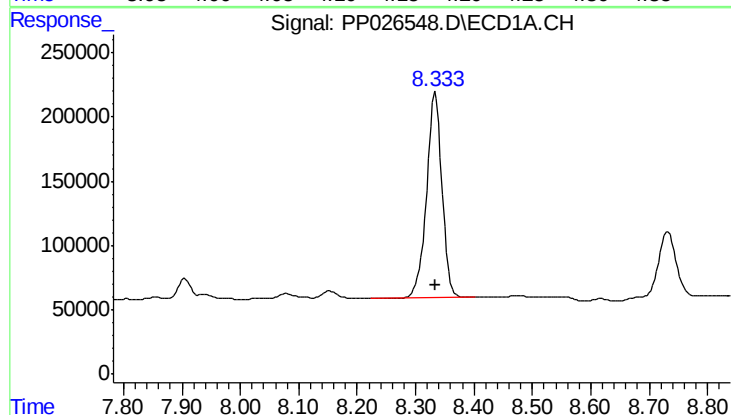


#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: 0.000 min
Response: 2909710
Conc: 19.27 ng/ml

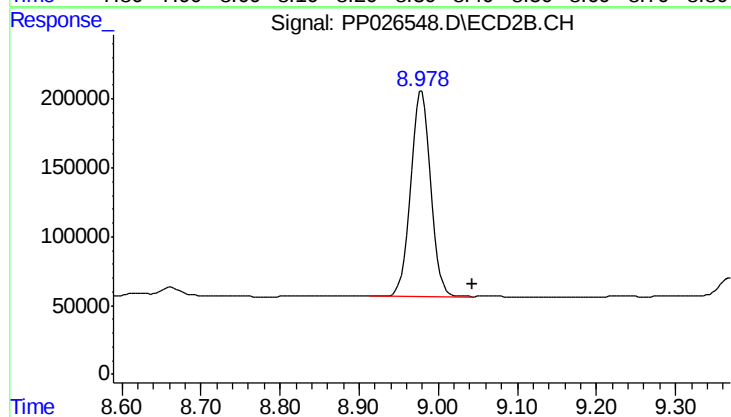

#2 Decachlorobiphenyl


R.T.: 8.979 min
Delta R.T.: -0.064 min
Response: 2650099
Conc: 16.51 ng/ml

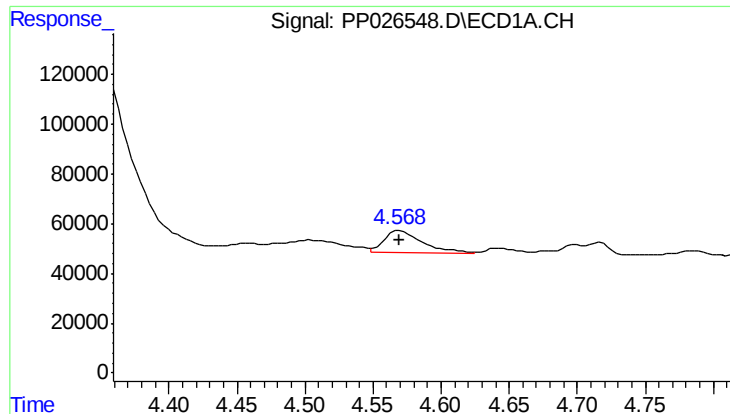

#3 Aroclor-1016-1


R.T.: 4.569 min
Delta R.T.: 0.000 min
Response: 180703
Conc: 78.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

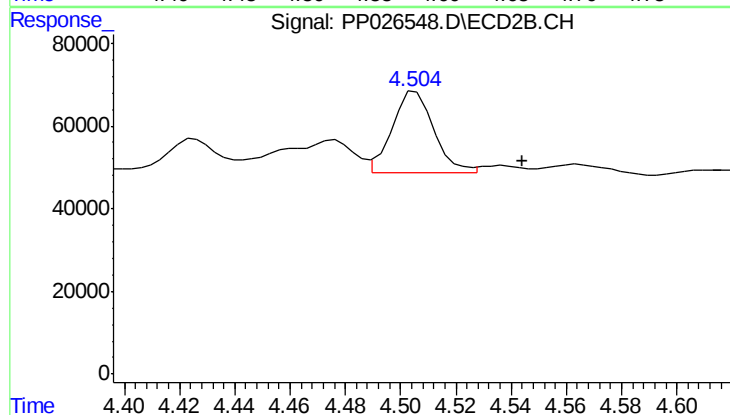


#3 Aroclor-1016-1

R.T.: 4.506 min
Delta R.T.: -0.038 min
Response: 208398
Conc: 53.32 ng/ml

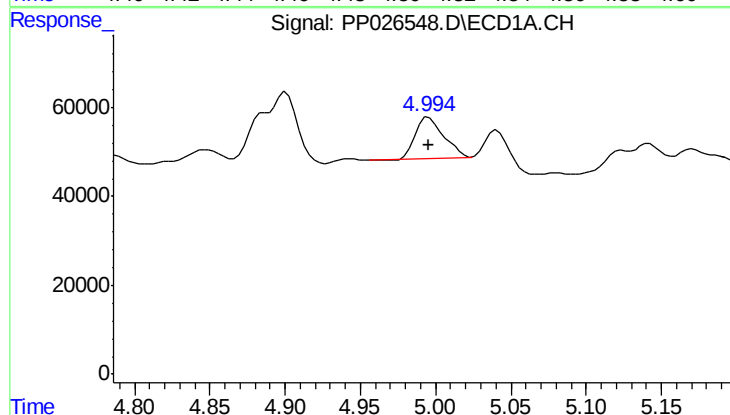


#4 Aroclor-1016-2

R.T.: 4.996 min
Delta R.T.: 0.000 min
Response: 117779
Conc: 44.46 ng/ml

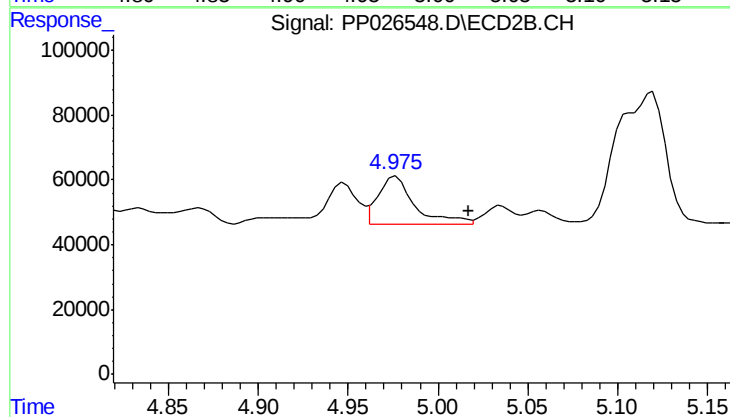

#4 Aroclor-1016-2


R.T.: 4.977 min
Delta R.T.: -0.040 min
Response: 207574
Conc: 71.60 ng/ml

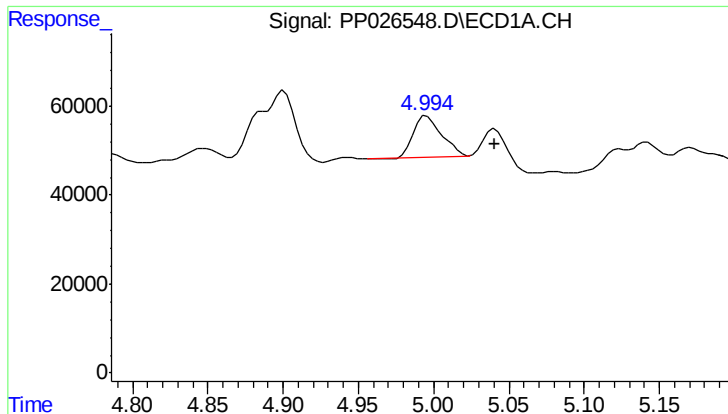

#5 Aroclor-1016-3


R.T.: 4.996 min
Delta R.T.: -0.045 min
Response: 117779
Conc: 64.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

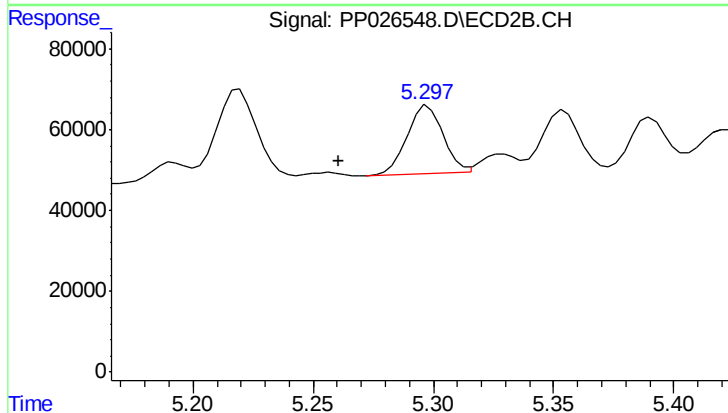


#5 Aroclor-1016-3

R.T.: 5.298 min
Delta R.T.: 0.037 min
Response: 175093
Conc: 29.83 ng/ml

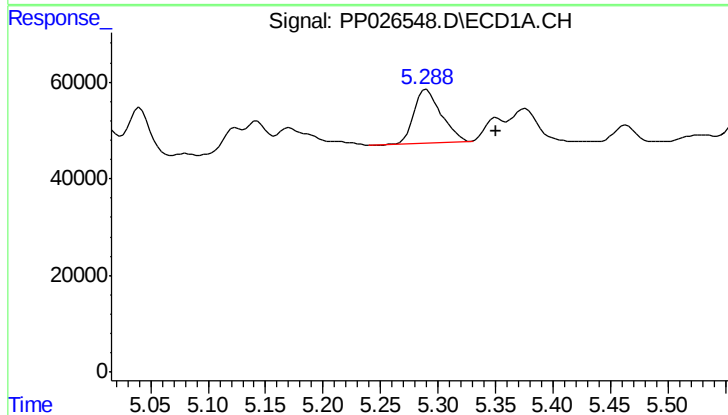


#6 Aroclor-1016-4

R.T.: 5.289 min
Delta R.T.: -0.061 min
Response: 183986
Conc: 150.24 ng/ml

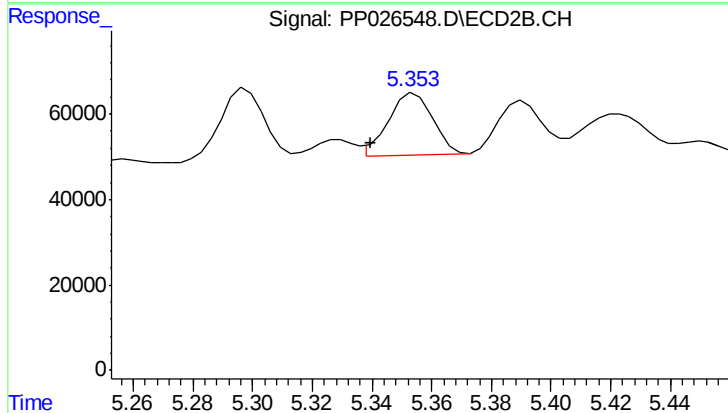

#6 Aroclor-1016-4


R.T.: 5.354 min
Delta R.T.: 0.015 min
Response: 151293
Conc: 39.82 ng/ml

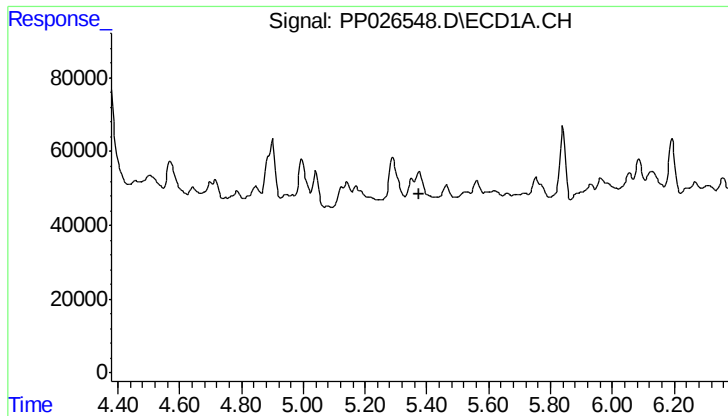

#7 Aroclor-1016-5


R.T.: 0.000 min
Exp R.T.: 5.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

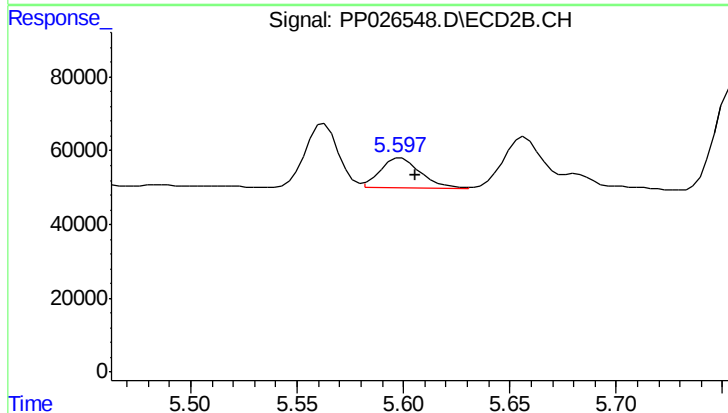


#7 Aroclor-1016-5

R.T.: 5.599 min
Delta R.T.: -0.007 min
Response: 105109
Conc: 26.29 ng/ml

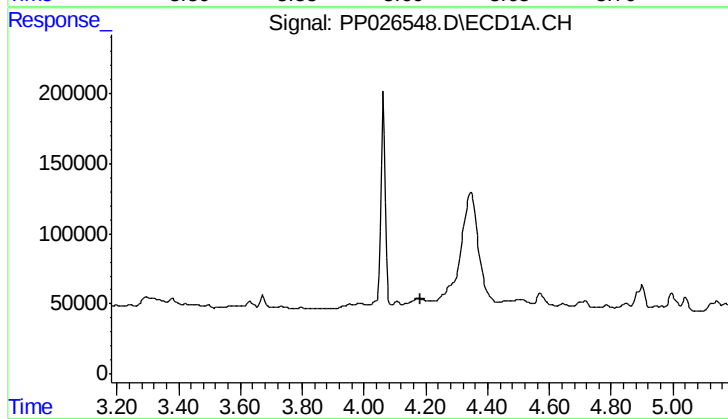


#8 Aroclor-1221-1

R.T.: 0.000 min
Exp R.T.: 4.182 min
Response: 0
Conc: N.D.

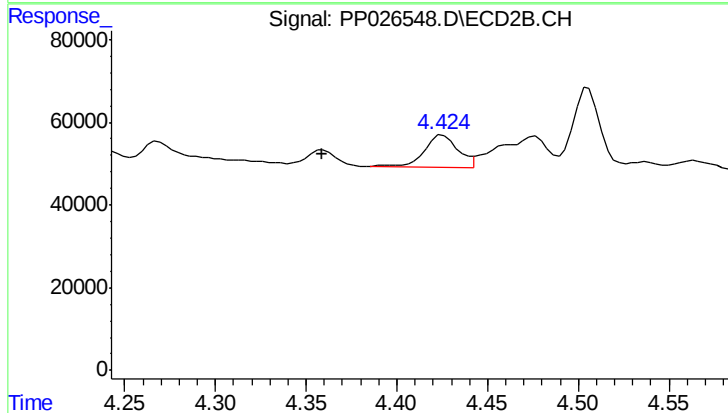

#8 Aroclor-1221-1


R.T.: 4.426 min
Delta R.T.: 0.067 min
Response: 98899
Conc: 137.74 ng/ml

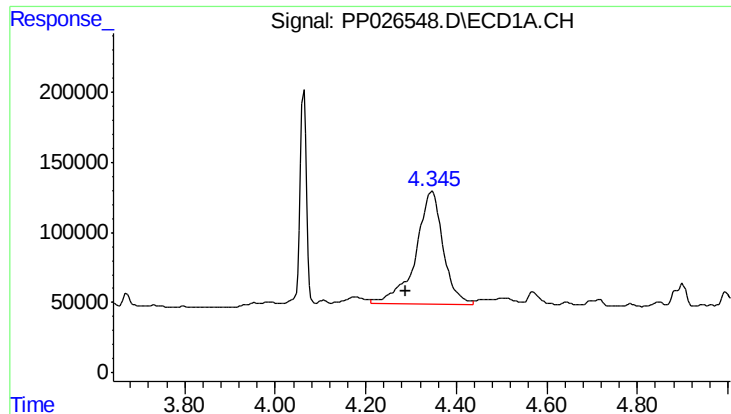

#9 Aroclor-1221-2


R.T.: 4.347 min
Delta R.T.: 0.057 min
Response: 3428490
Conc: 3691.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

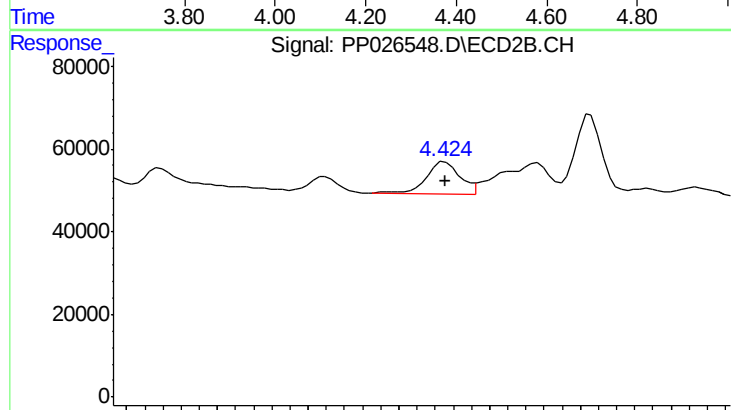


#9 Aroclor-1221-2

R.T.: 4.426 min
Delta R.T.: 0.000 min
Response: 98899
Conc: 313.02 ng/ml

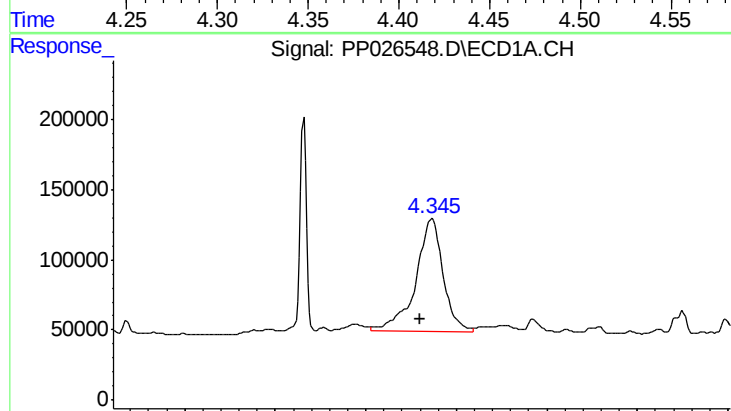


#10 Aroclor-1221-3

R.T.: 4.347 min
Delta R.T.: 0.027 min
Response: 3428490
Conc: 983.35 ng/ml

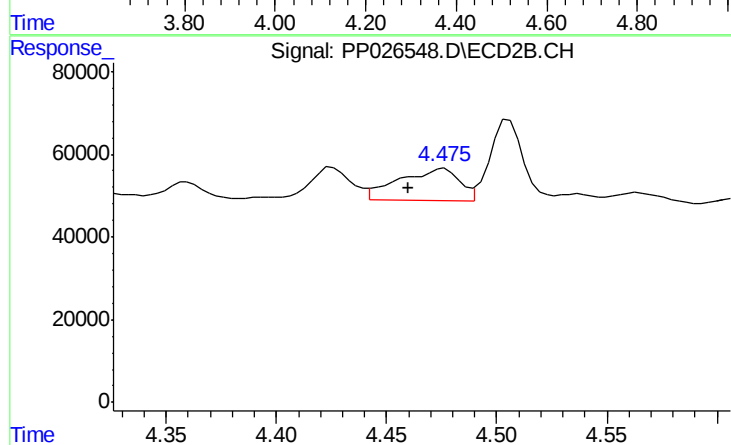

#10 Aroclor-1221-3


R.T.: 4.476 min
Delta R.T.: 0.016 min
Response: 148181
Conc: 183.24 ng/ml

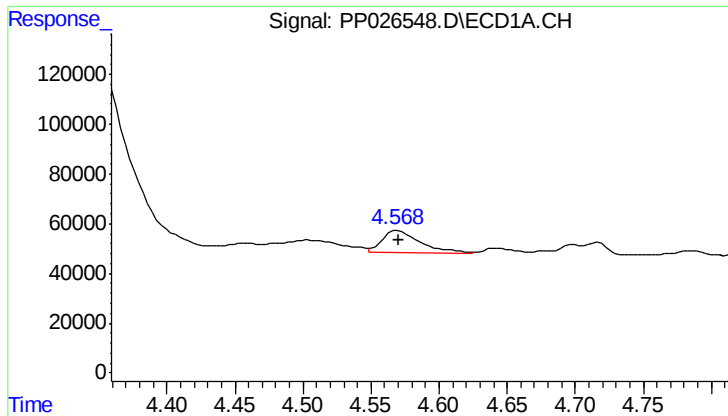

#11 Aroclor-1232-1


R.T.: 4.569 min
Delta R.T.: -0.001 min
Response: 180703
Conc: 73.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

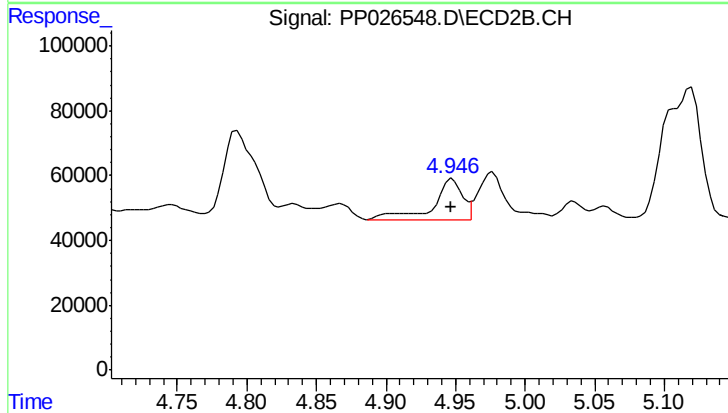


#11 Aroclor-1232-1

R.T.: 4.948 min
Delta R.T.: 0.001 min
Response: 182198
Conc: 86.57 ng/ml

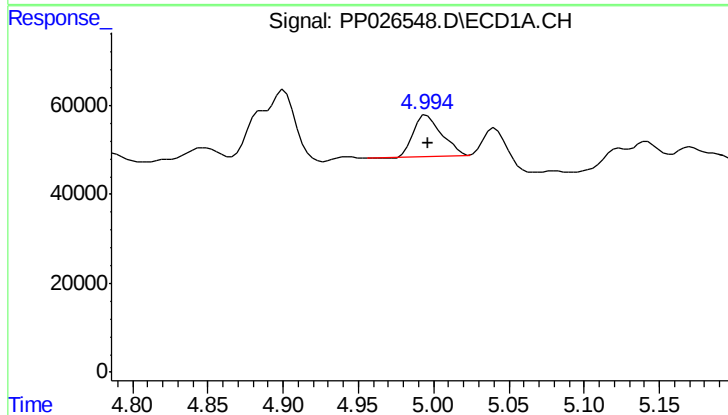


#12 Aroclor-1232-2

R.T.: 4.996 min
Delta R.T.: 0.000 min
Response: 117779
Conc: 42.86 ng/ml

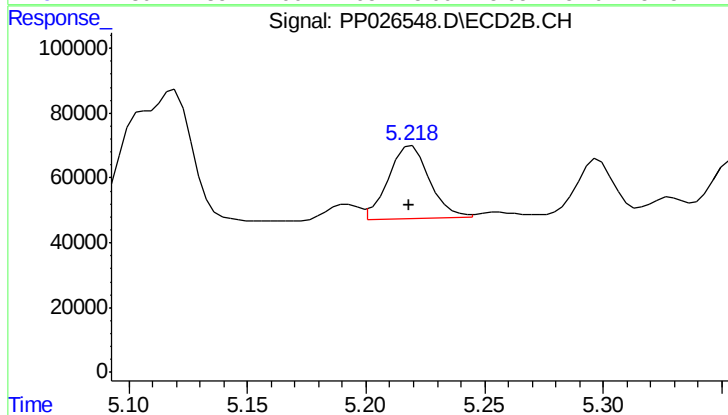

#12 Aroclor-1232-2


R.T.: 5.219 min
Delta R.T.: 0.001 min
Response: 266843
Conc: 49.71 ng/ml

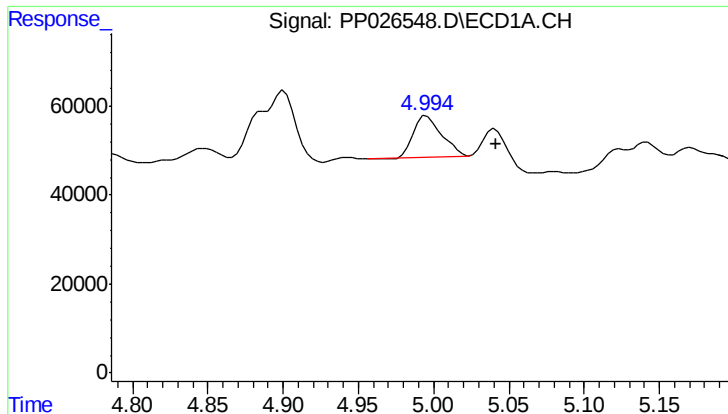

#13 Aroclor-1232-3


R.T.: 4.996 min
Delta R.T.: -0.046 min
Response: 117779
Conc: 61.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

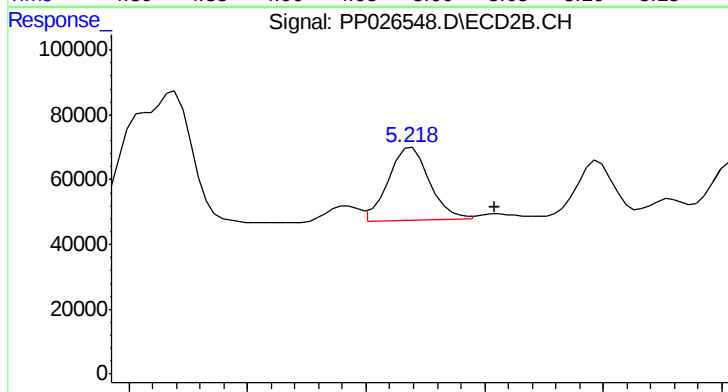


#13 Aroclor-1232-3

R.T.: 5.219 min
Delta R.T.: -0.035 min
Response: 266843
Conc: 1158.54 ng/ml

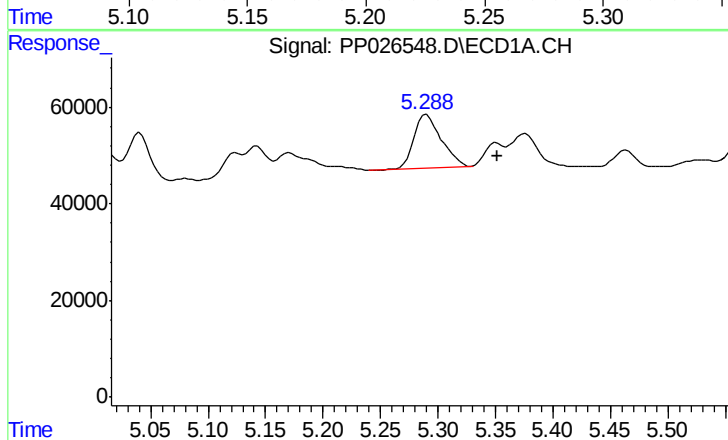


#14 Aroclor-1232-4

R.T.: 5.289 min
Delta R.T.: -0.062 min
Response: 183986
Conc: 143.03 ng/ml

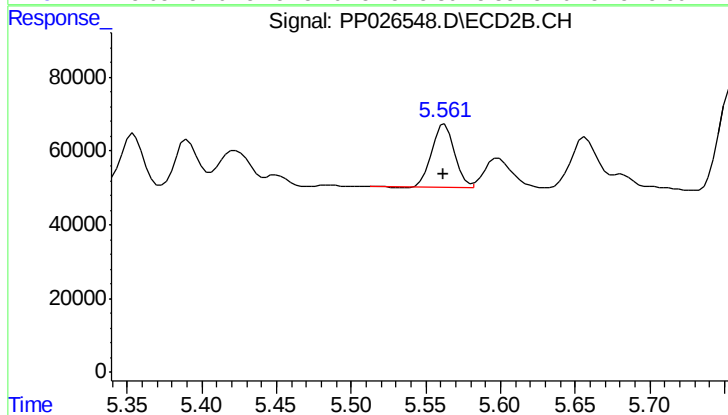

#14 Aroclor-1232-4


R.T.: 5.563 min
Delta R.T.: 0.000 min
Response: 184785
Conc: 47.34 ng/ml

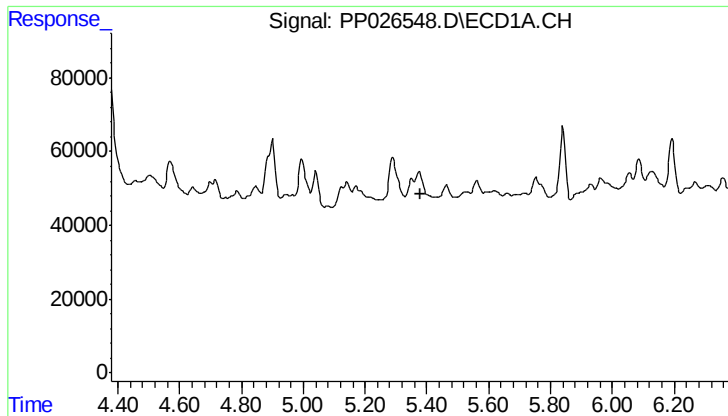

#15 Aroclor-1232-5


R.T.: 0.000 min
Exp R.T.: 5.378 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

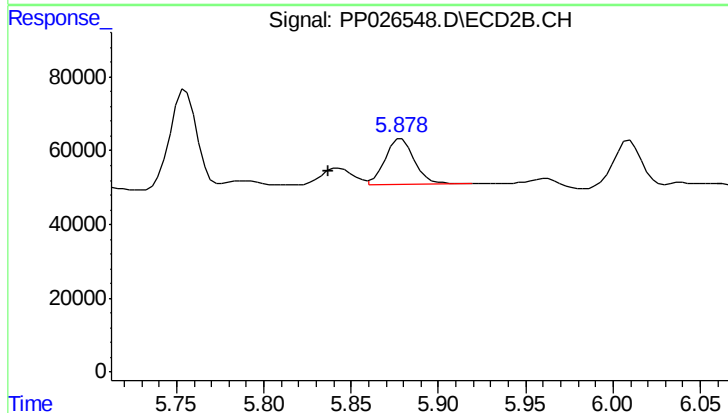


#15 Aroclor-1232-5

R.T.: 5.879 min
Delta R.T.: 0.042 min
Response: 144172
Conc: 96.20 ng/ml

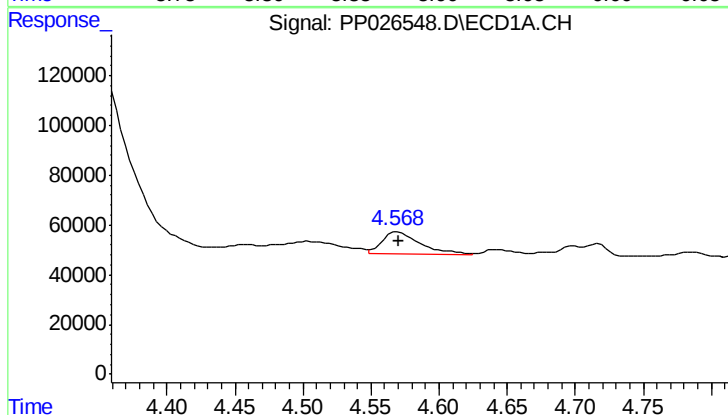


#16 Aroclor-1242-1

R.T.: 4.569 min
Delta R.T.: -0.001 min
Response: 180703
Conc: 73.57 ng/ml

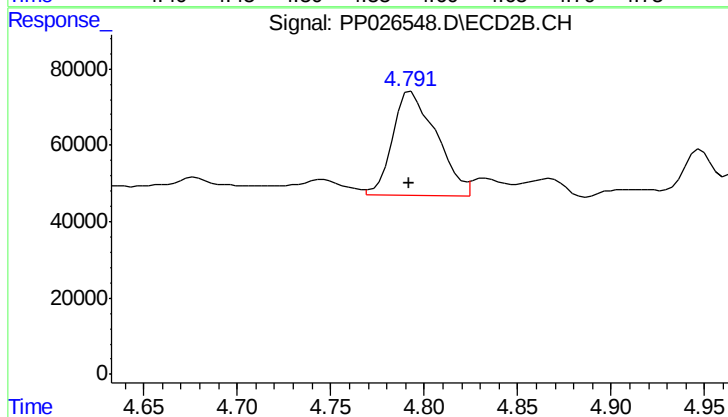

#16 Aroclor-1242-1


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 440241
Conc: 62.62 ng/ml

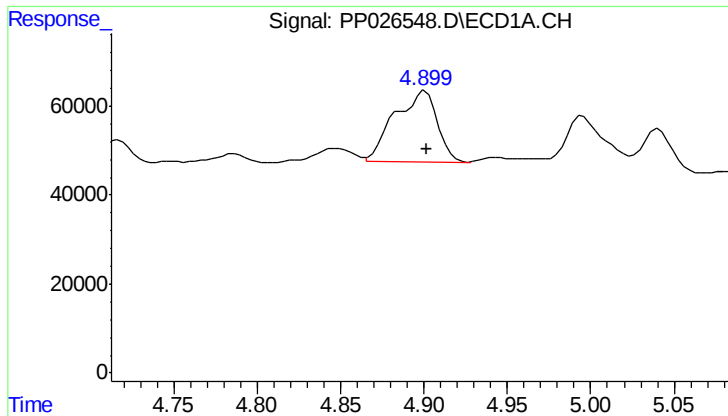

#17 Aroclor-1242-2


R.T.: 4.901 min
Delta R.T.: 0.000 min
Response: 283683
Conc: 47.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

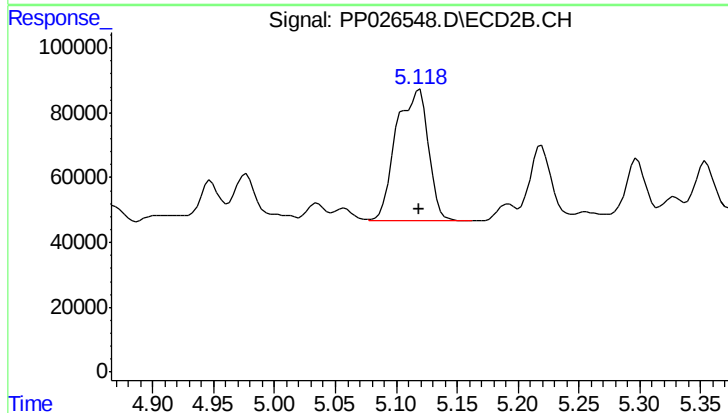


#17 Aroclor-1242-2

R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 752198
Conc: 53.61 ng/ml

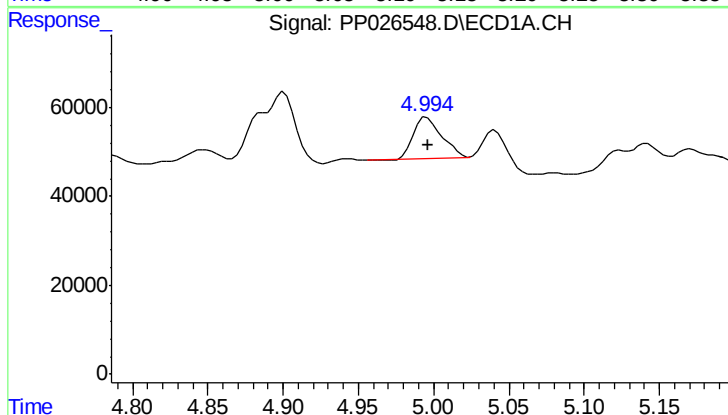


#18 Aroclor-1242-3

R.T.: 4.996 min
Delta R.T.: 0.000 min
Response: 117779
Conc: 42.86 ng/ml

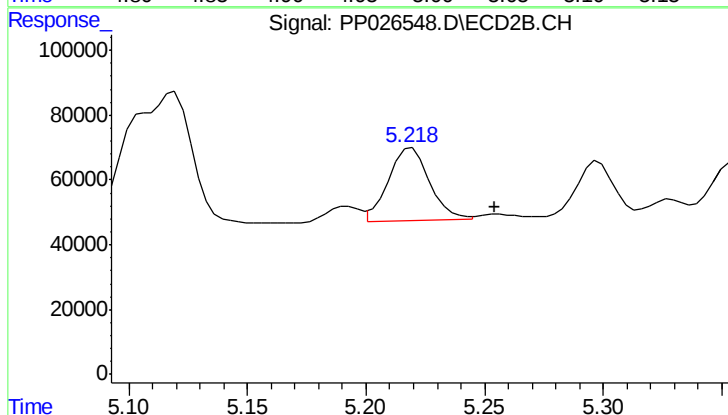

#18 Aroclor-1242-3


R.T.: 5.219 min
Delta R.T.: -0.035 min
Response: 266843
Conc: 1158.54 ng/ml

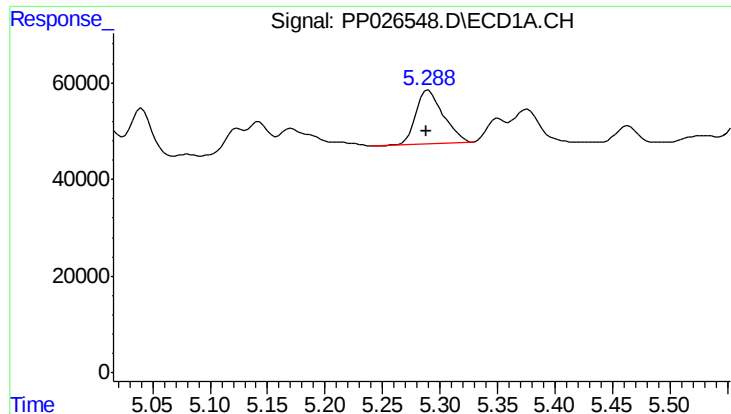

#19 Aroclor-1242-4


R.T.: 5.289 min
Delta R.T.: 0.001 min
Response: 183986
Conc: 75.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

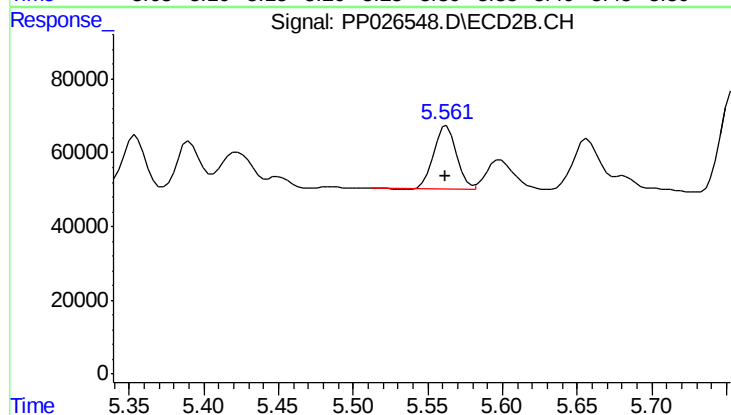


#19 Aroclor-1242-4

R.T.: 5.563 min
Delta R.T.: 0.000 min
Response: 184785
Conc: 47.34 ng/ml

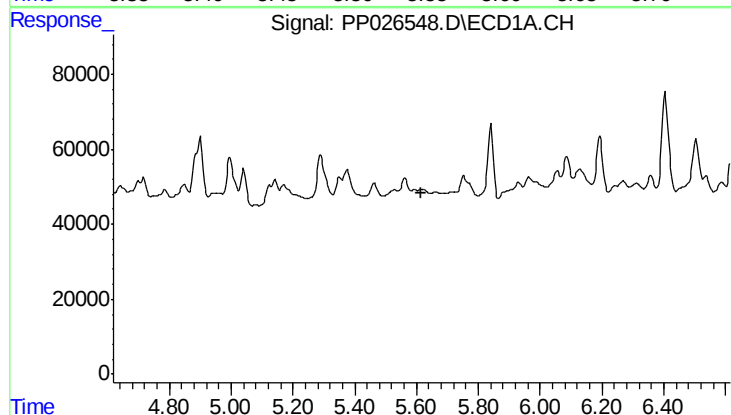


#20 Aroclor-1242-5

R.T.: 0.000 min
Exp R.T.: 5.617 min
Response: 0
Conc: N.D.

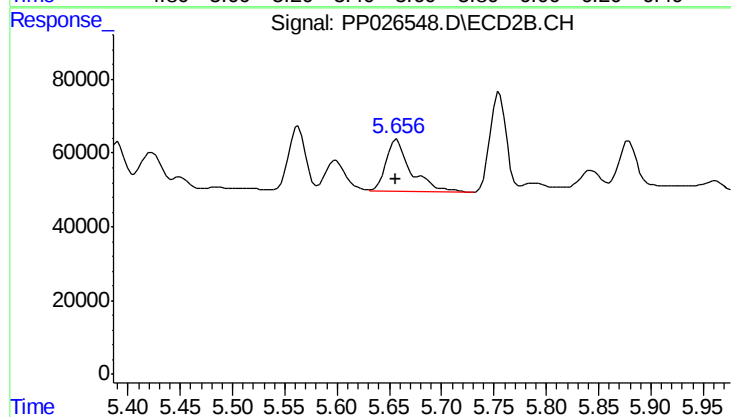

#20 Aroclor-1242-5


R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 227942
Conc: 59.24 ng/ml

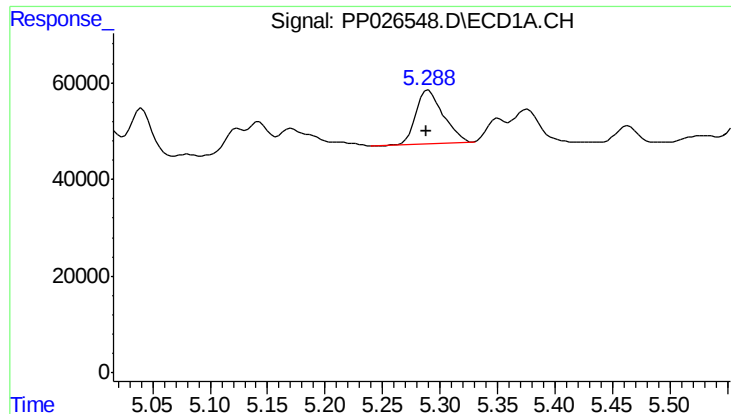

#21 Aroclor-1248-1


R.T.: 5.289 min
Delta R.T.: 0.001 min
Response: 183986
Conc: 75.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

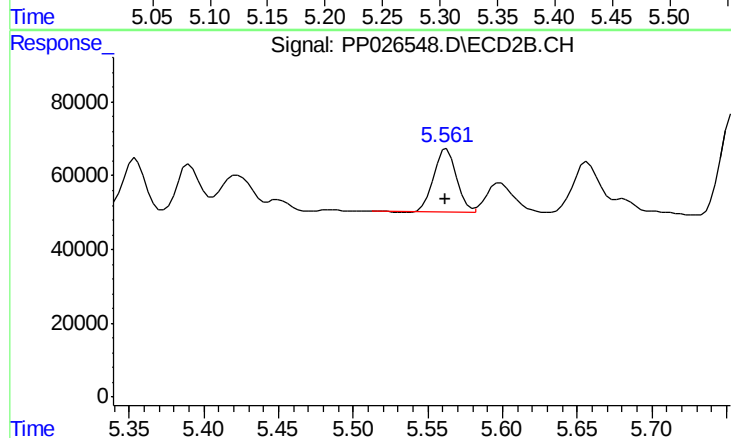


#21 Aroclor-1248-1

R.T.: 5.563 min
Delta R.T.: 0.000 min
Response: 184785
Conc: 47.34 ng/ml

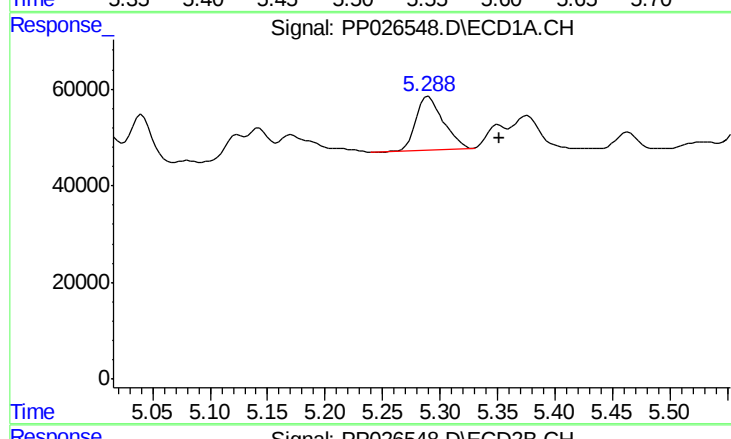


#22 Aroclor-1248-2

R.T.: 5.289 min
Delta R.T.: -0.002 min
Response: 183986
Conc: 143.03 ng/ml

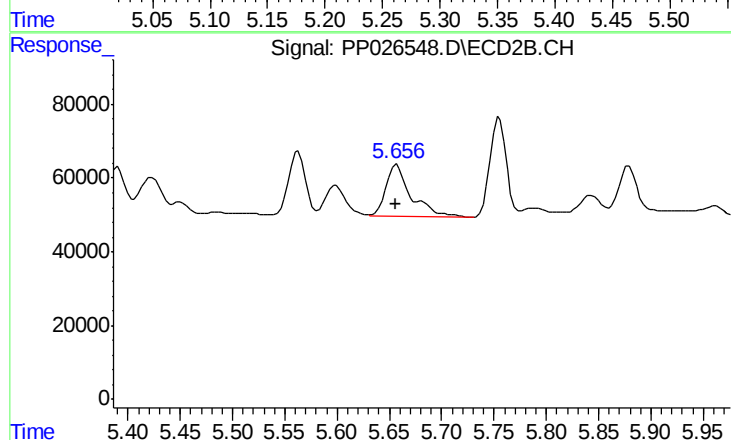

#22 Aroclor-1248-2


R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 227942
Conc: 59.24 ng/ml

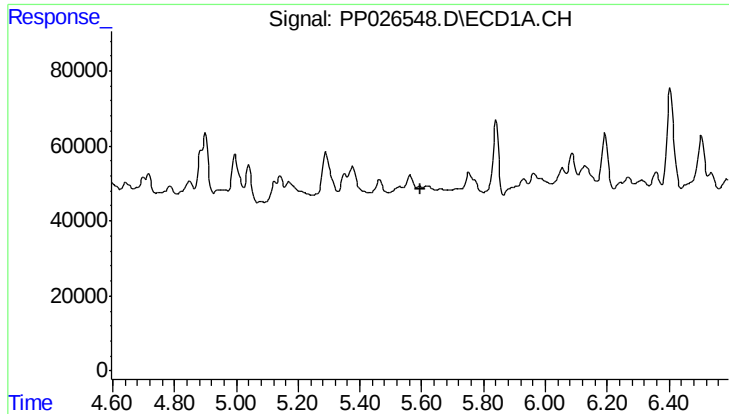

#23 Aroclor-1248-3


R.T.: 0.000 min
Exp R.T.: 5.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

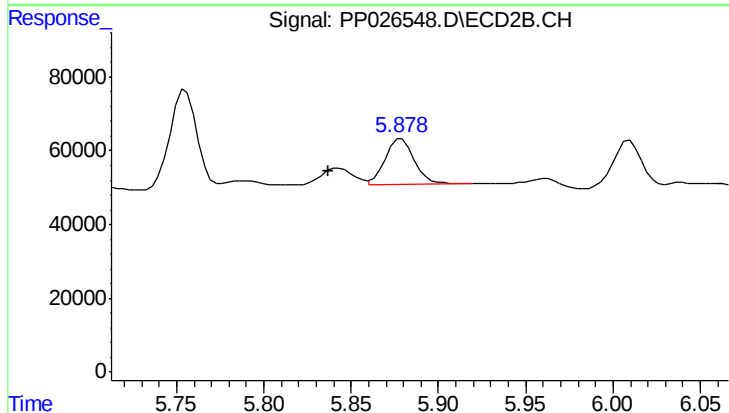


#23 Aroclor-1248-3

R.T.: 5.879 min
Delta R.T.: 0.042 min
Response: 144172
Conc: 96.20 ng/ml

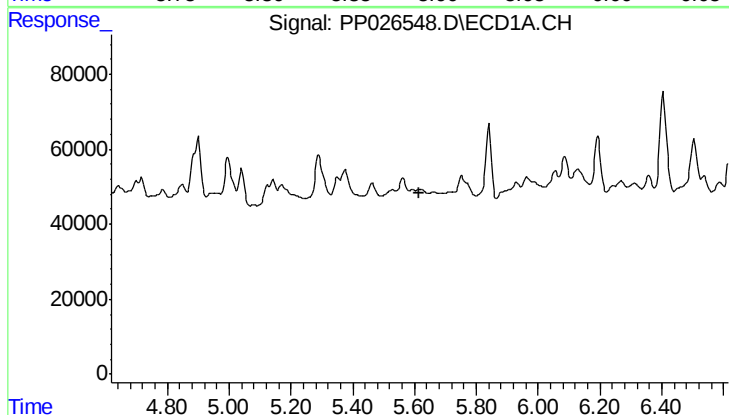


#24 Aroclor-1248-4

R.T.: 0.000 min
Exp R.T.: 5.617 min
Response: 0
Conc: N.D.

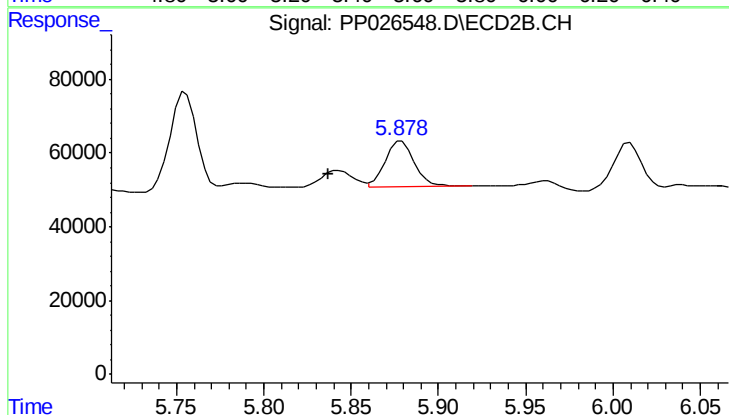

#24 Aroclor-1248-4


R.T.: 5.879 min
Delta R.T.: 0.042 min
Response: 144172
Conc: 96.20 ng/ml

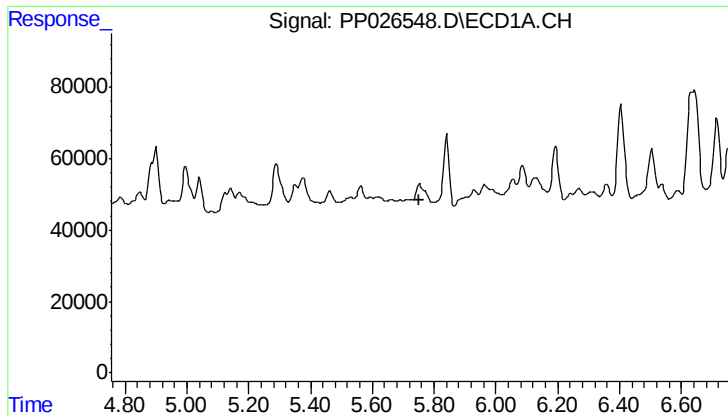

#25 Aroclor-1248-5


R.T.: 0.000 min
Exp R.T.: 5.753 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

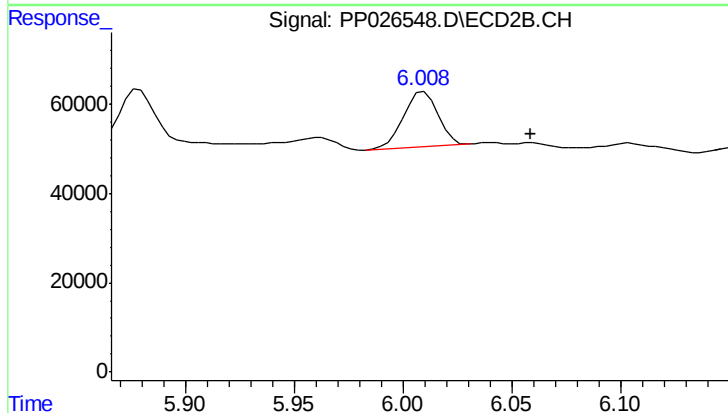


#25 Aroclor-1248-5

R.T.: 6.010 min
Delta R.T.: -0.049 min
Response: 136143
Conc: 394.86 ng/ml

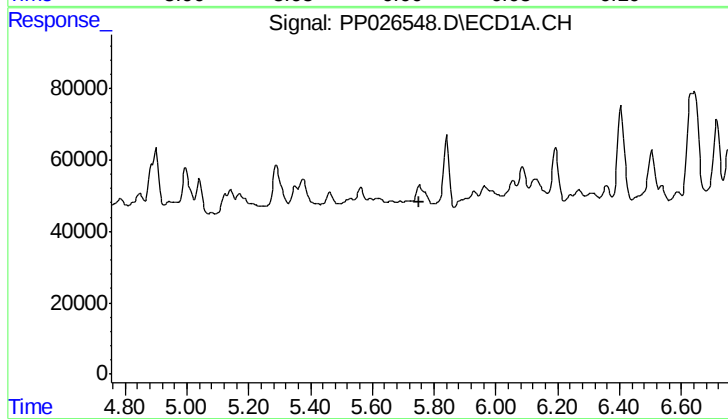


#26 Aroclor-1254-1

R.T.: 0.000 min
Exp R.T.: 5.753 min
Response: 0
Conc: N.D.

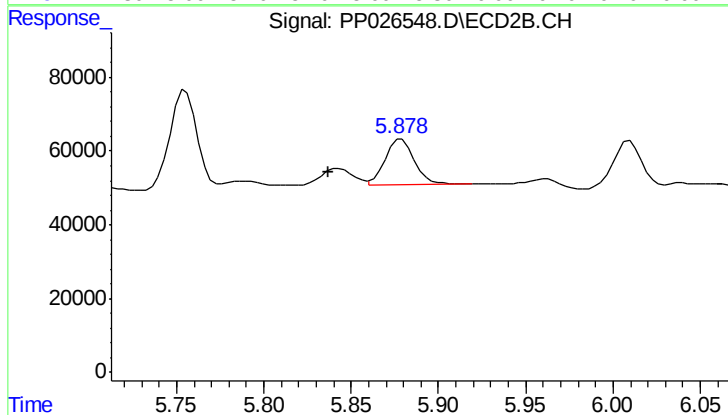

#26 Aroclor-1254-1


R.T.: 5.879 min
Delta R.T.: 0.042 min
Response: 144172
Conc: 96.20 ng/ml

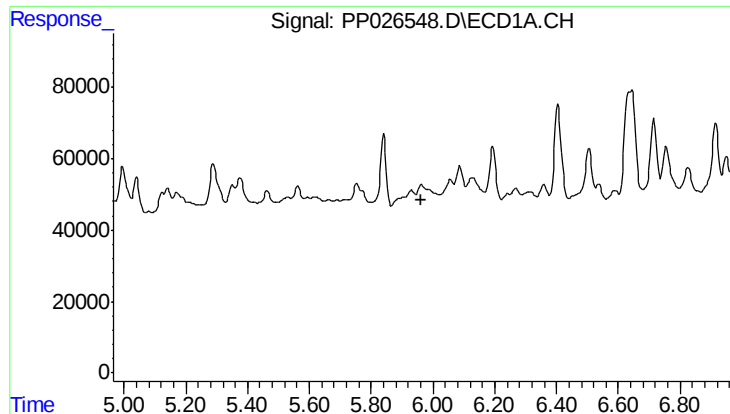

#27 Aroclor-1254-2


R.T.: 0.000 min
Exp R.T.: 5.963 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

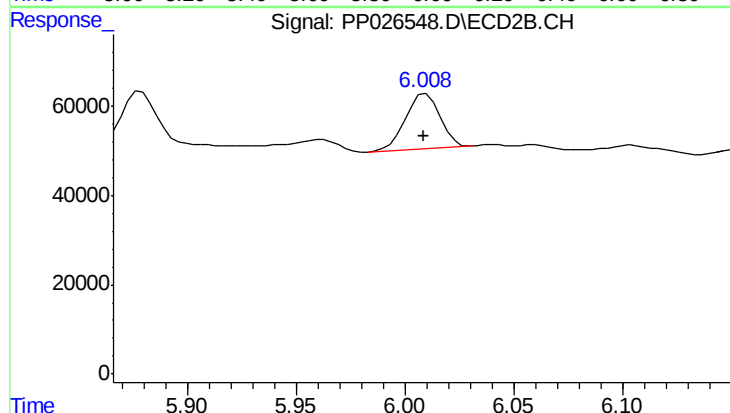


#27 Aroclor-1254-2

R.T.: 6.010 min
Delta R.T.: 0.001 min
Response: 136143
Conc: 53.43 ng/ml

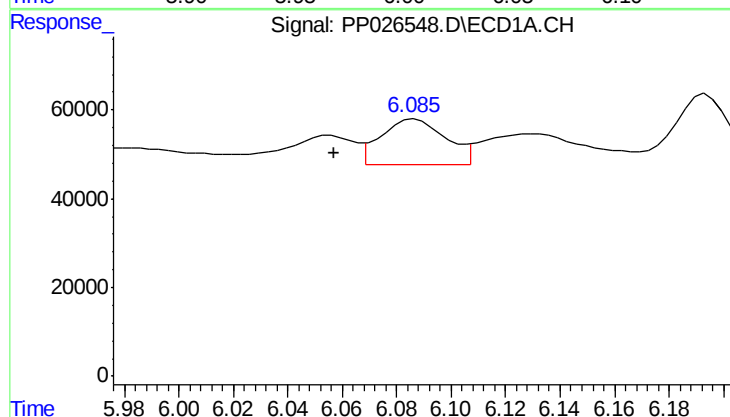


#28 Aroclor-1254-3

R.T.: 6.087 min
Delta R.T.: 0.030 min
Response: 171045
Conc: 212.47 ng/ml

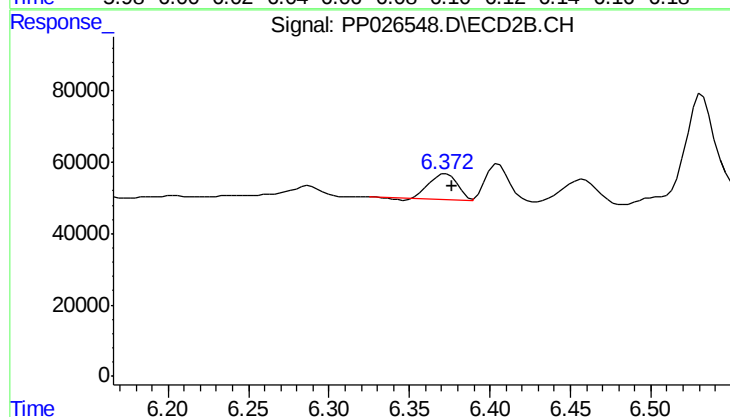

#28 Aroclor-1254-3


R.T.: 6.373 min
Delta R.T.: -0.003 min
Response: 87463
Conc: 38.54 ng/ml

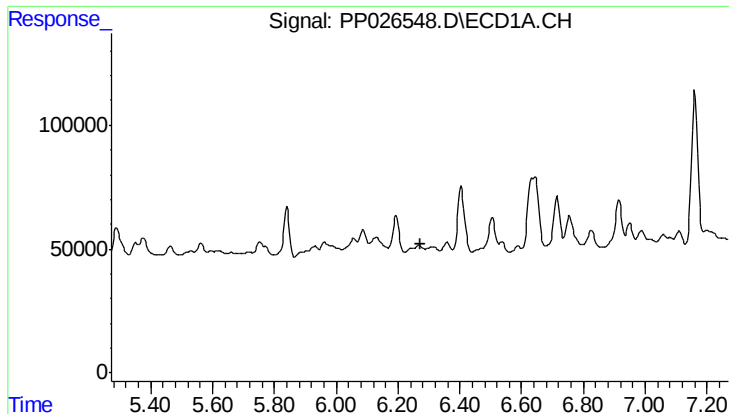

#29 Aroclor-1254-4


R.T.: 0.000 min
Exp R.T.: 6.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

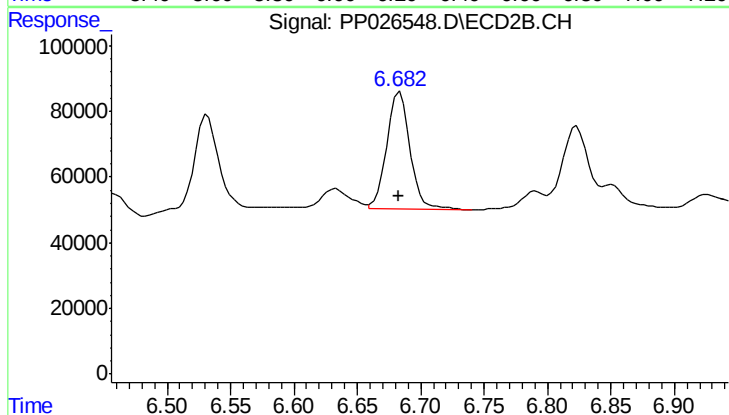


#29 Aroclor-1254-4

R.T.: 6.683 min
Delta R.T.: 0.001 min
Response: 461349
Conc: 56.35 ng/ml

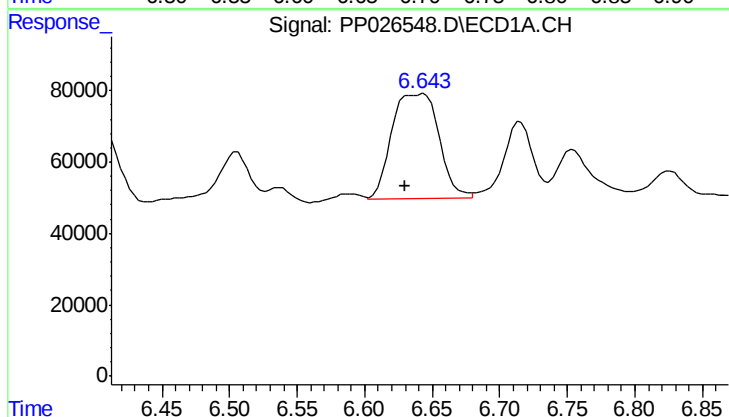


#30 Aroclor-1254-5

R.T.: 6.644 min
Delta R.T.: 0.014 min
Response: 718409
Conc: 79.04 ng/ml

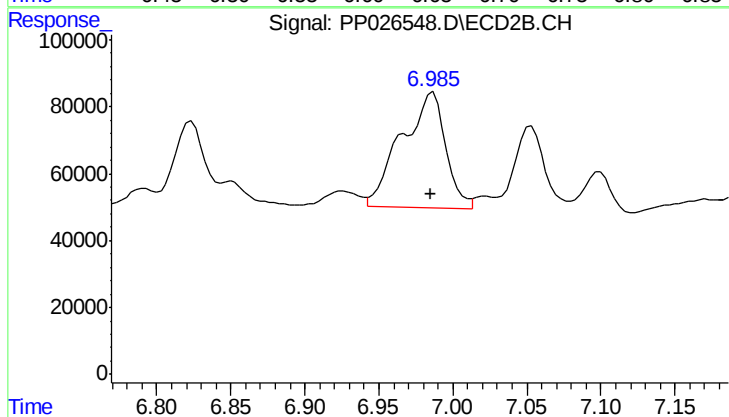

#30 Aroclor-1254-5


R.T.: 6.986 min
Delta R.T.: 0.001 min
Response: 712296
Conc: 62.41 ng/ml

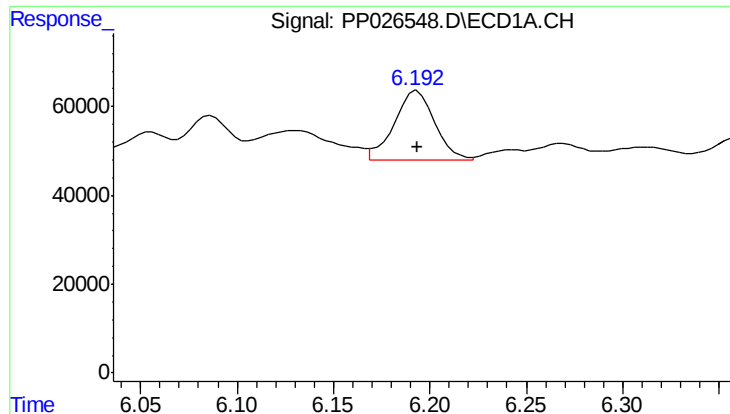

#31 Aroclor-1260-1


R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 231235
Conc: 63.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

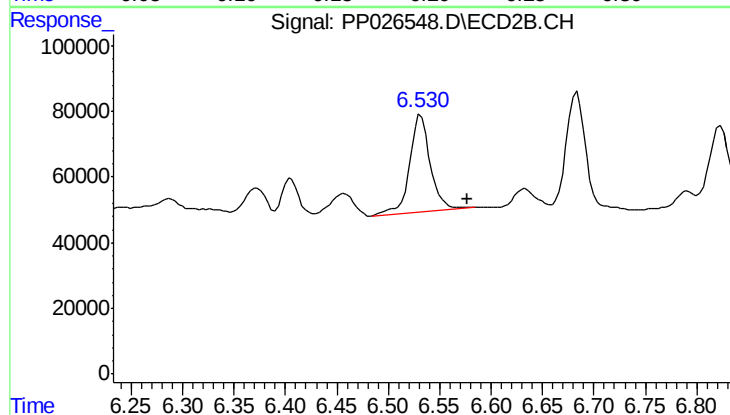


#31 Aroclor-1260-1

R.T.: 6.532 min
Delta R.T.: -0.045 min
Response: 416282
Conc: 52.07 ng/ml

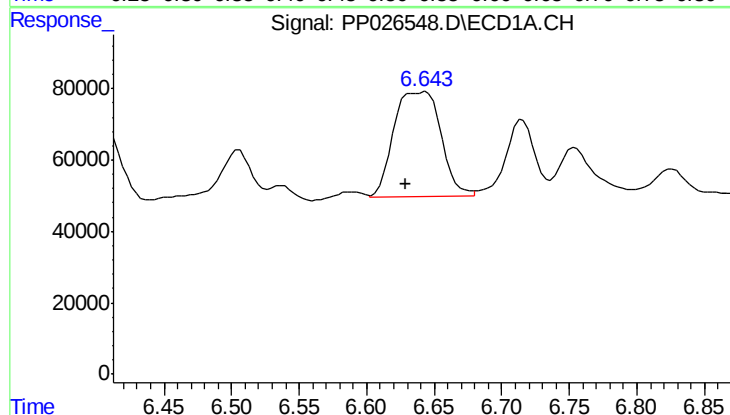


#32 Aroclor-1260-2

R.T.: 6.644 min
Delta R.T.: 0.015 min
Response: 718409
Conc: 76.42 ng/ml

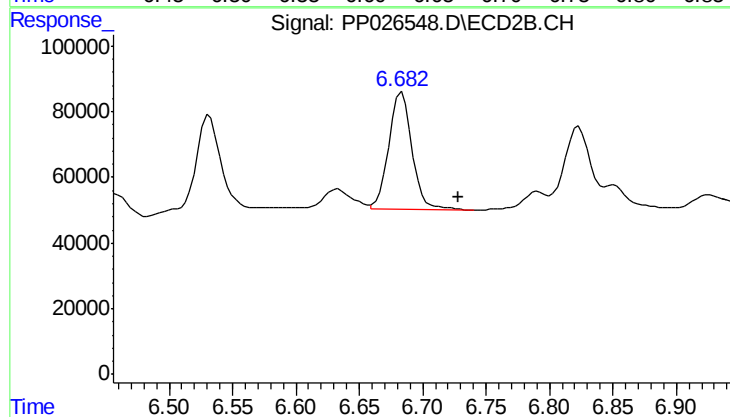

#32 Aroclor-1260-2


R.T.: 6.683 min
Delta R.T.: -0.045 min
Response: 461349
Conc: 51.02 ng/ml

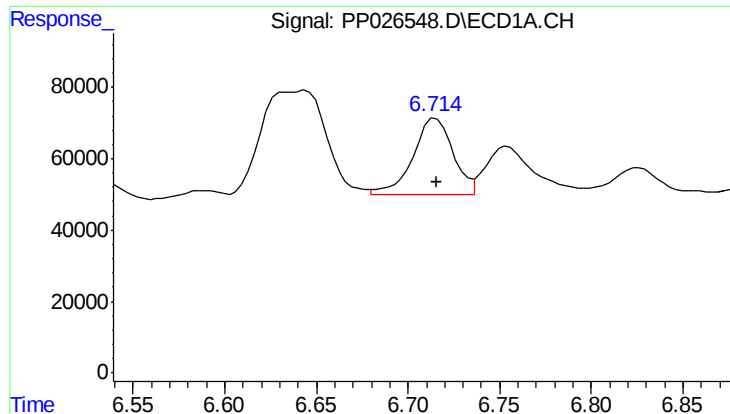

#33 Aroclor-1260-3


R.T.: 6.715 min
Delta R.T.: 0.000 min
Response: 325311
Conc: 48.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

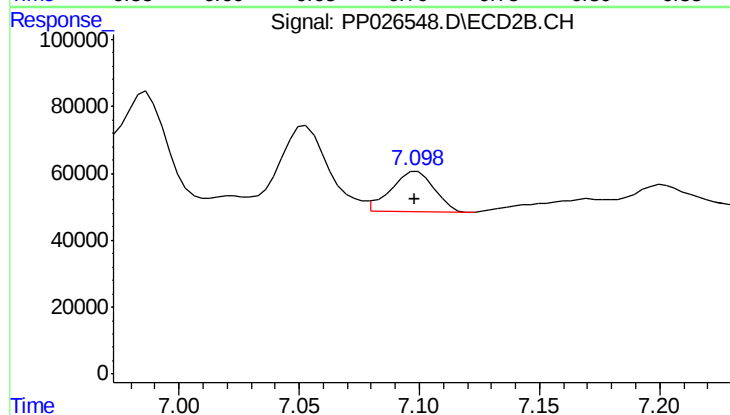


#33 Aroclor-1260-3

R.T.: 7.099 min
Delta R.T.: 0.001 min
Response: 151736
Conc: 23.74 ng/ml

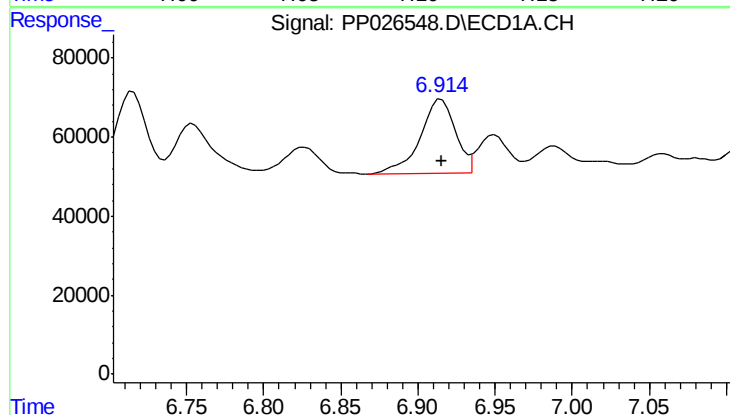


#34 Aroclor-1260-4

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 299601
Conc: 56.35 ng/ml

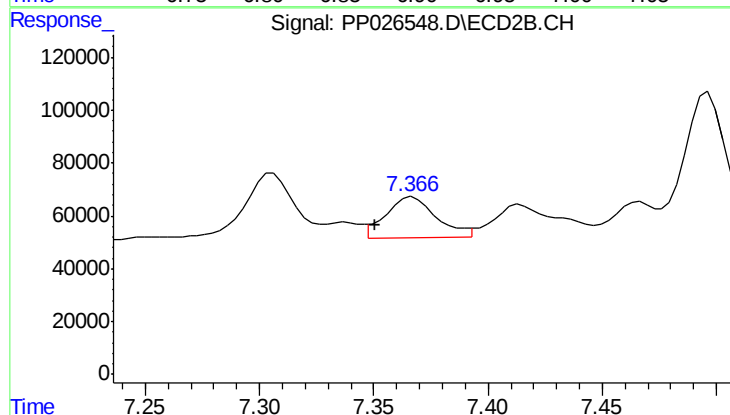

#34 Aroclor-1260-4


R.T.: 7.367 min
Delta R.T.: 0.016 min
Response: 242827
Conc: 32.77 ng/ml

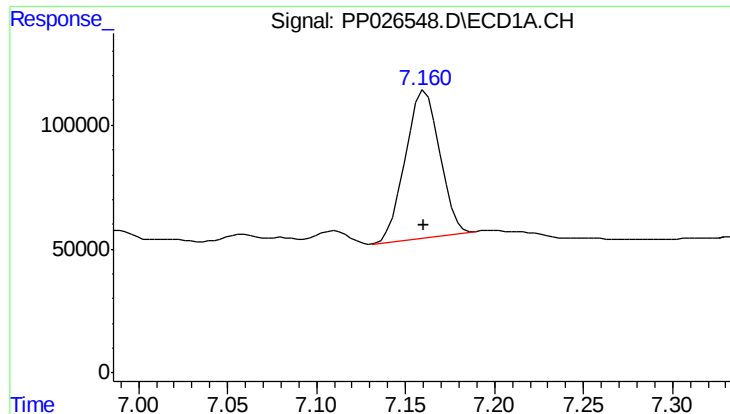

#35 Aroclor-1260-5


R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 794469
Conc: 41.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

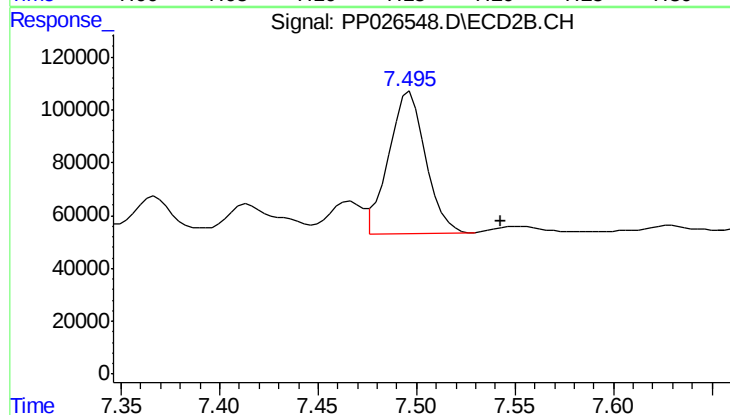


#35 Aroclor-1260-5

R.T.: 7.497 min
Delta R.T.: -0.046 min
Response: 703457
Conc: 43.74 ng/ml

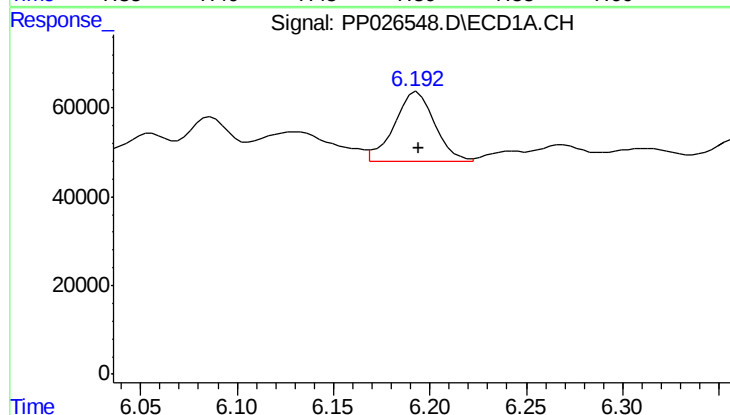


#36 Aroclor-1262-1

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 231235
Conc: 65.67 ng/ml

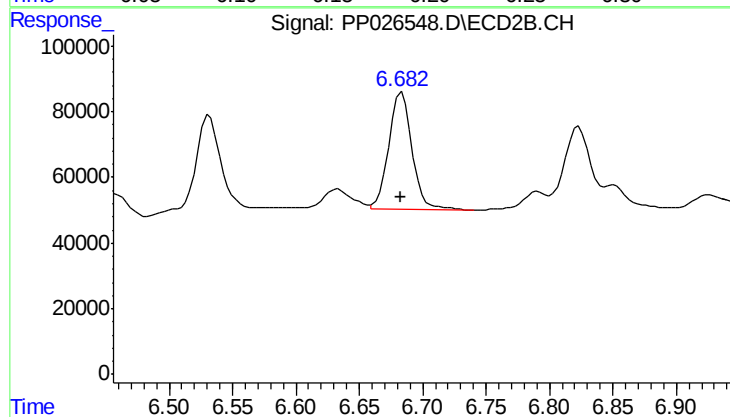

#36 Aroclor-1262-1


R.T.: 6.683 min
Delta R.T.: 0.001 min
Response: 461349
Conc: 56.35 ng/ml

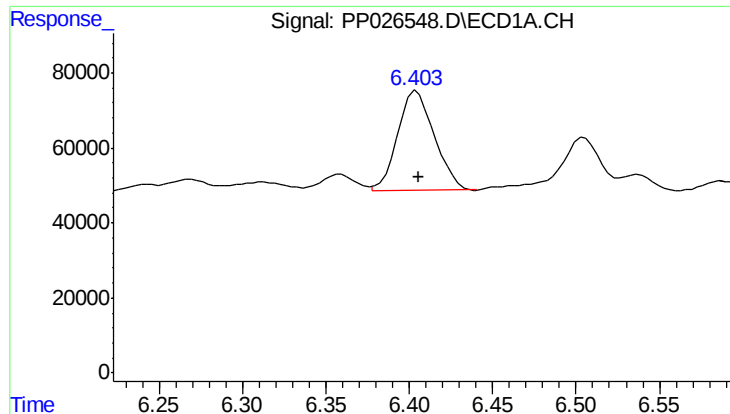

#37 Aroclor-1262-2


R.T.: 6.404 min
Delta R.T.: -0.001 min
Response: 406693
Conc: 50.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

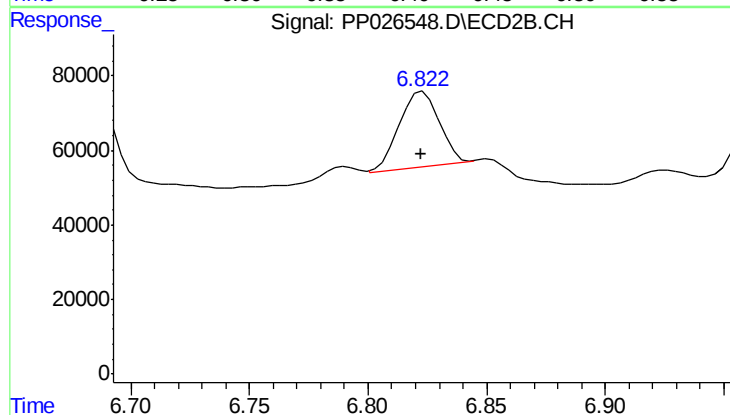


#37 Aroclor-1262-2

R.T.: 6.823 min
Delta R.T.: 0.000 min
Response: 233673
Conc: 38.64 ng/ml

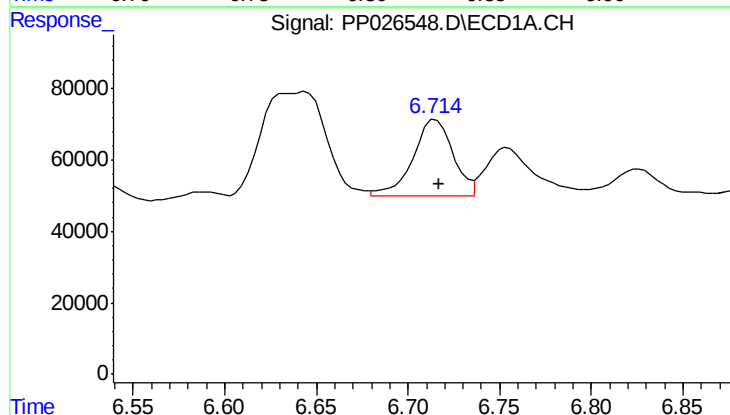


#38 Aroclor-1262-3

R.T.: 6.715 min
Delta R.T.: -0.002 min
Response: 325311
Conc: 50.56 ng/ml

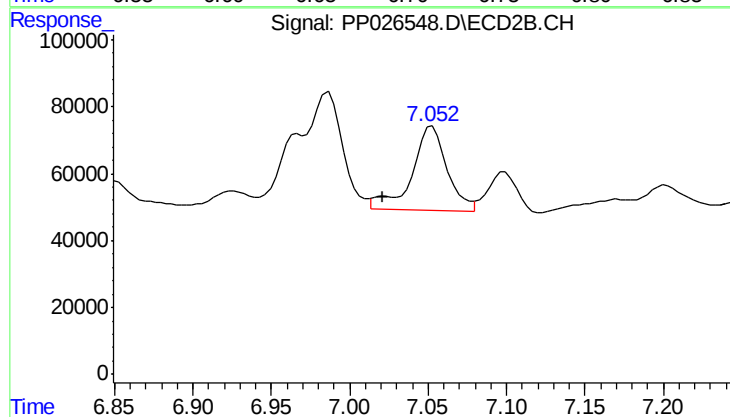

#38 Aroclor-1262-3


R.T.: 7.053 min
Delta R.T.: 0.032 min
Response: 391743
Conc: 1817.82 ng/ml

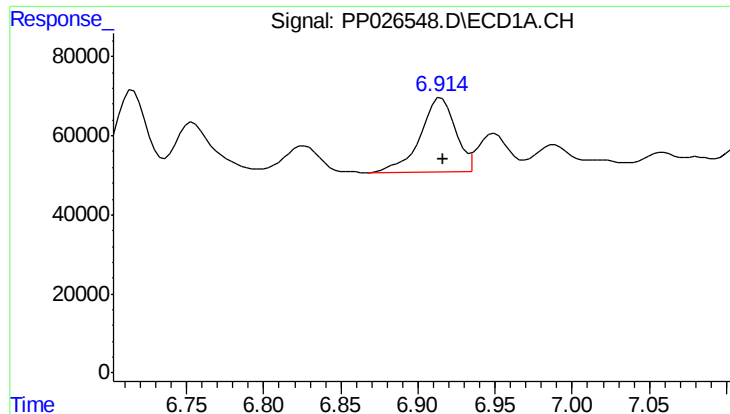

#39 Aroclor-1262-4


R.T.: 6.915 min
Delta R.T.: -0.001 min
Response: 299601
Conc: 56.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

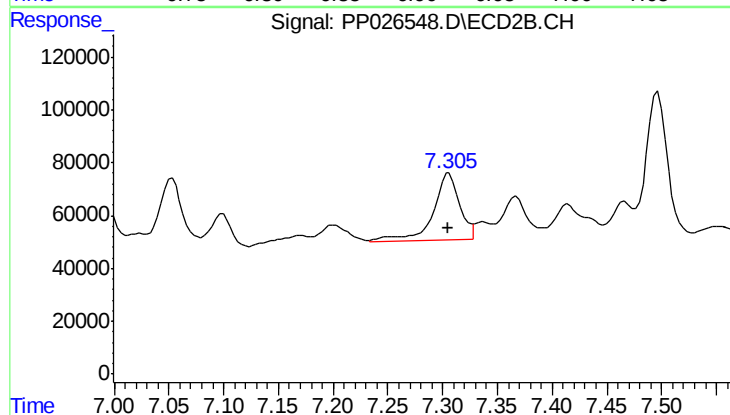


#39 Aroclor-1262-4

R.T.: 7.306 min
Delta R.T.: 0.001 min
Response: 435326
Conc: 66.22 ng/ml

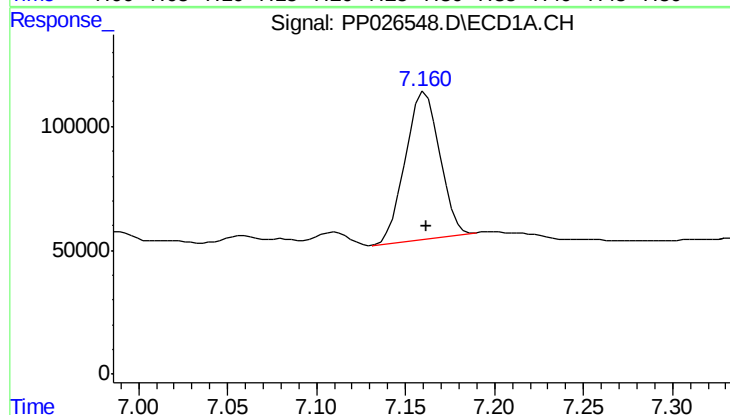


#40 Aroclor-1262-5

R.T.: 7.161 min
Delta R.T.: -0.001 min
Response: 794469
Conc: 41.25 ng/ml

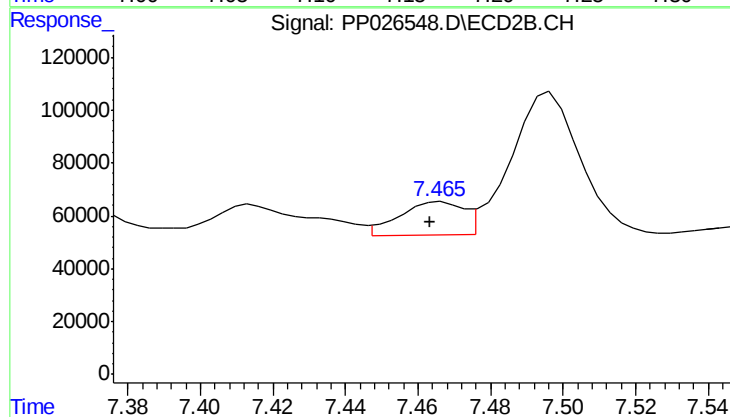

#40 Aroclor-1262-5


R.T.: 7.466 min
Delta R.T.: 0.003 min
Response: 153528
Conc: 677.52 ng/ml

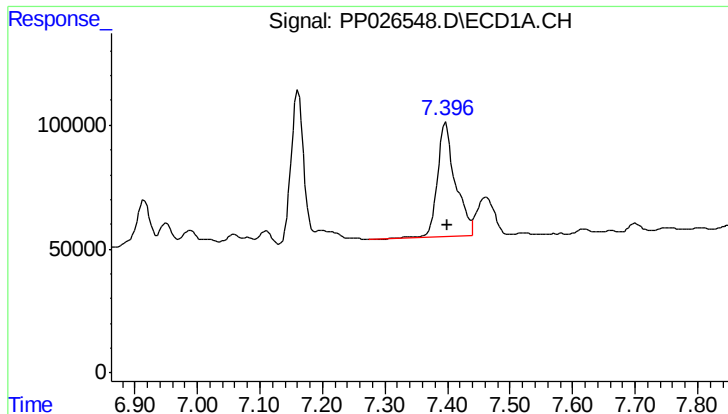

#41 Aroclor-1268-1


R.T.: 7.397 min
Delta R.T.: -0.002 min
Response: 914190
Conc: 73.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

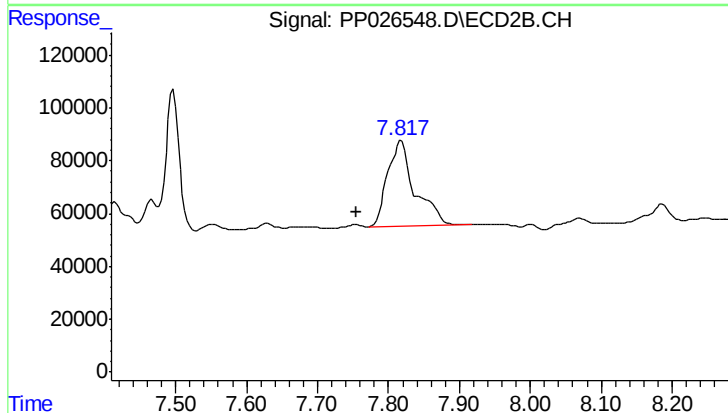


#41 Aroclor-1268-1

R.T.: 7.819 min
Delta R.T.: 0.064 min
Response: 859805
Conc: 3641.12 ng/ml

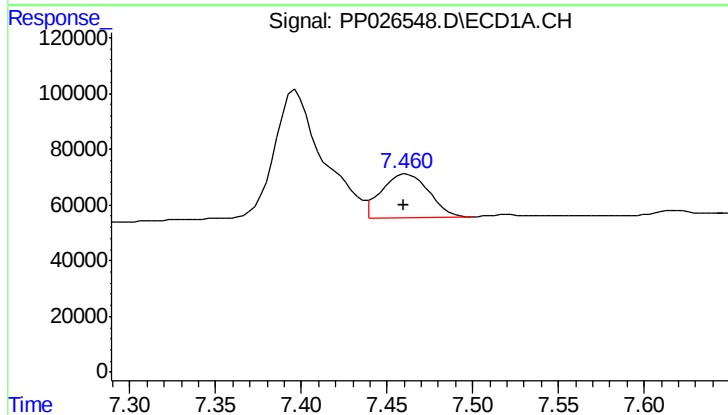


#42 Aroclor-1268-2

R.T.: 7.462 min
Delta R.T.: 0.001 min
Response: 303066
Conc: 60.41 ng/ml

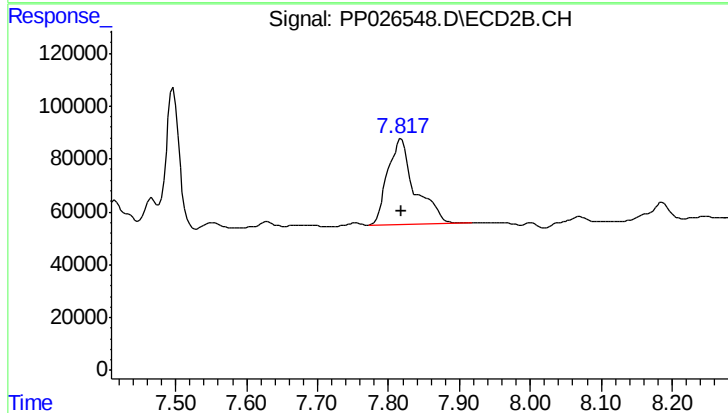

#42 Aroclor-1268-2


R.T.: 7.819 min
Delta R.T.: 0.001 min
Response: 859805
Conc: 75.41 ng/ml

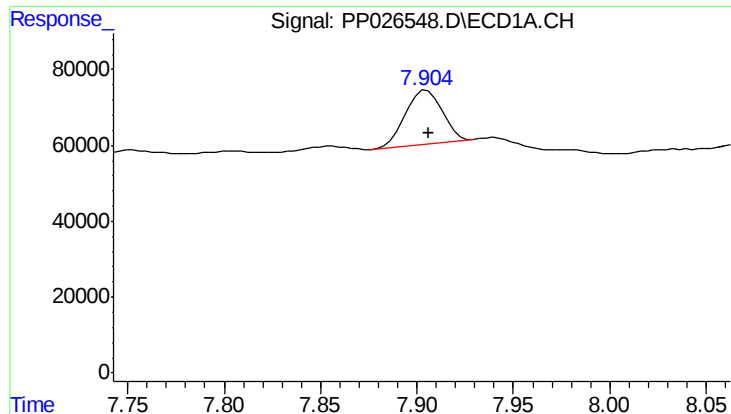

#44 Aroclor-1268-4

R.T.: 7.905 min
Delta R.T.: -0.002 min
Response: 190090
Conc: 36.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110343BSD

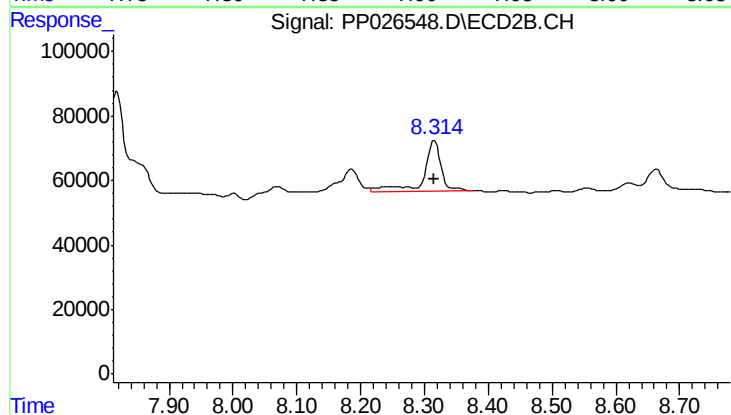

#44 Aroclor-1268-4

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 301135
Conc: 62.73 ng/ml