

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026532.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 14:58
Operator : UA/AJ
Sample : J3522-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TPTW-01

Manual Integrations
APPROVED

ugo
6/22/2018 10:42:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 15:10:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.065	4.135	1637821	2980077	17.751	12.515m#
2)	SA Decachlor...	8.339	8.953	2436299	1232129	16.793	7.809m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026532.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 14:58
Operator : UA/AJ
Sample : J3522-02
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TPTW-01


Manual Integrations
APPROVED

ugo
6/22/2018 10:42:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 15:10:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

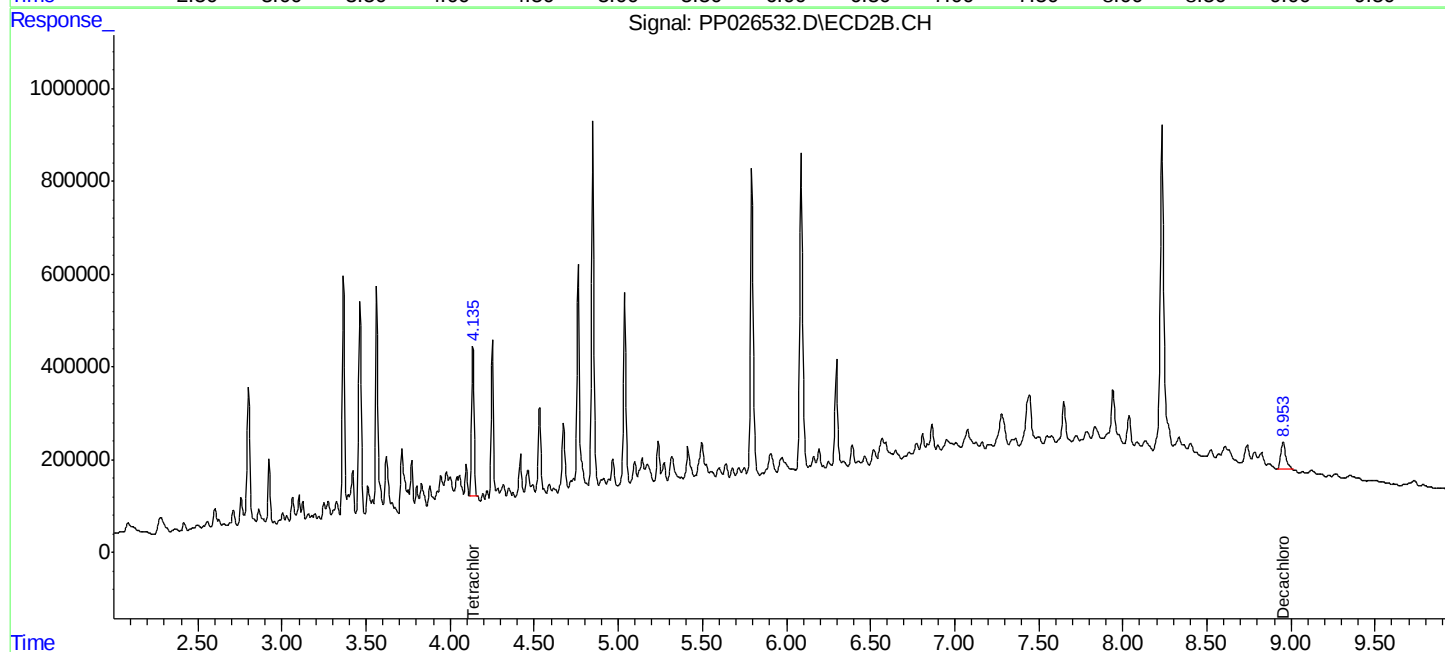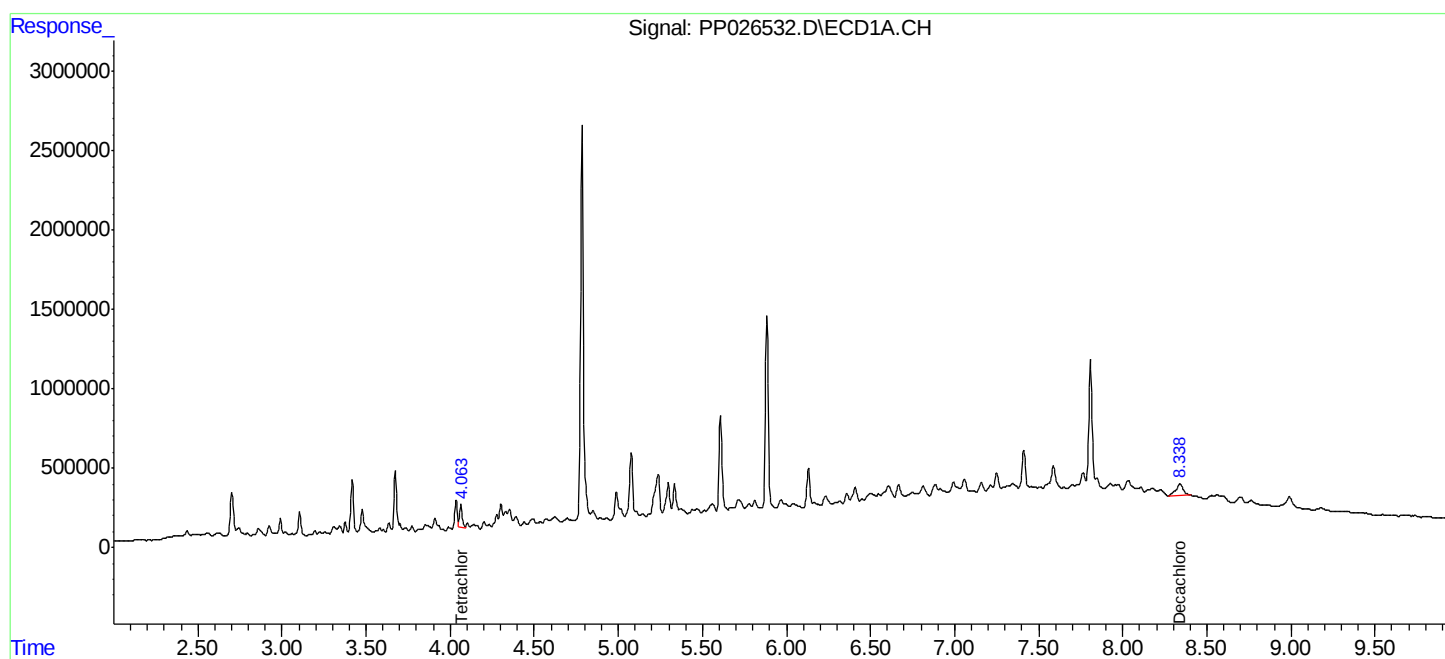

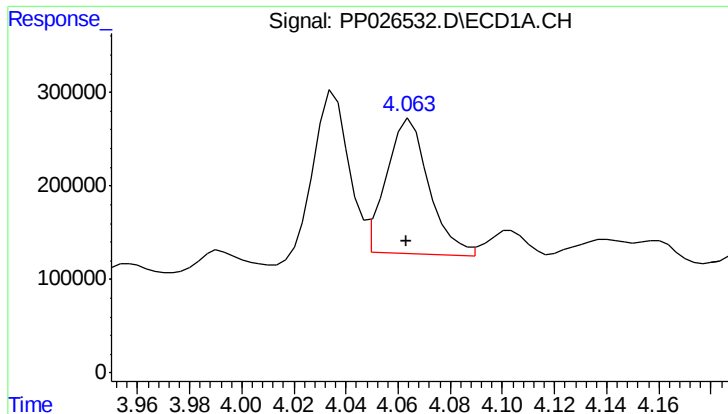


#1 Tetrachloro-m-xylene

R.T.: 4.065 min
Delta R.T.: 0.001 min
Response: 1637821
Conc: 17.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
TPTW-01


Manual Integrations
APPROVED

ugo
6/22/2018 10:42:41 AM

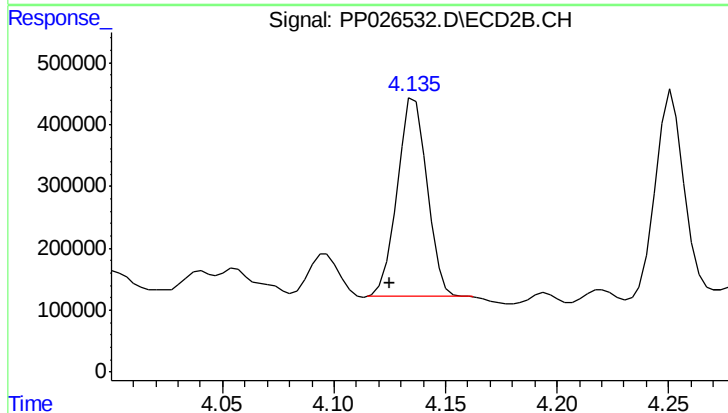


#1 Tetrachloro-m-xylene

R.T.: 4.135 min
Delta R.T.: 0.010 min
Response: 2980077
Conc: 12.51 ng/ml m

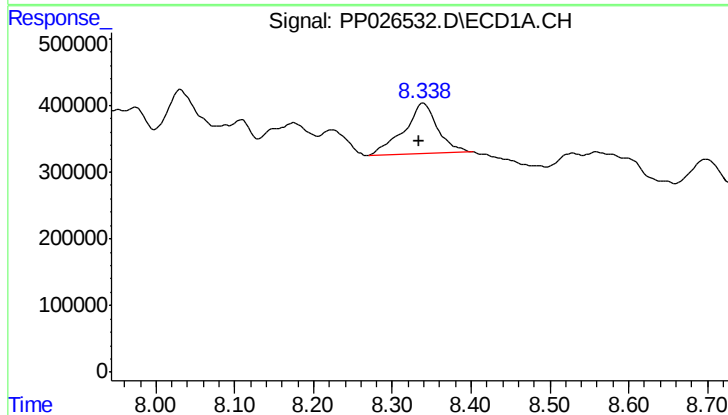

#2 Decachlorobiphenyl

R.T.: 8.339 min
Delta R.T.: 0.006 min
Response: 2436299
Conc: 16.79 ng/ml

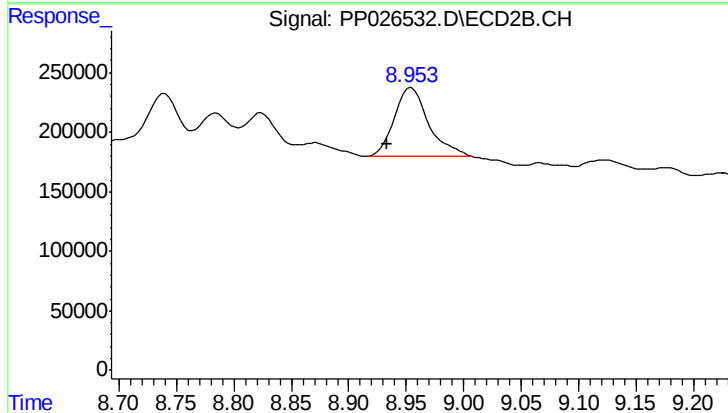

#2 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: 0.019 min
Response: 1232129
Conc: 7.81 ng/ml m