

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026537.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 16:09
Operator : UA/AJ
Sample : J3505-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-56-COMP

Manual Integrations
APPROVED

ugo
6/22/2018 10:43:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 16:20:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.064	4.139	1226823	2897770	13.296	12.169m
2) SA Decachlor...	8.335	8.959	1665640	1724102	11.481	10.927m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026537.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 16:09
Operator : UA/AJ
Sample : J3505-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-56-COMP


Manual Integrations
APPROVED

ugo
6/22/2018 10:43:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 16:20:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

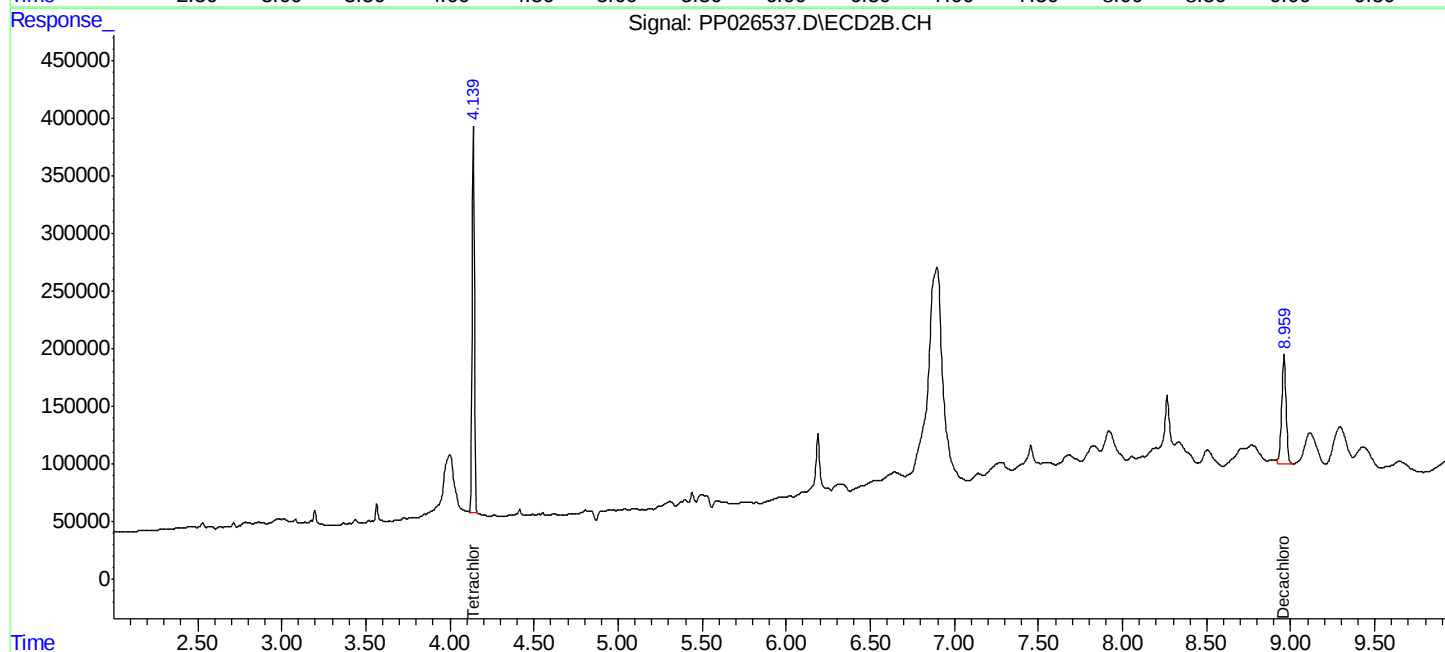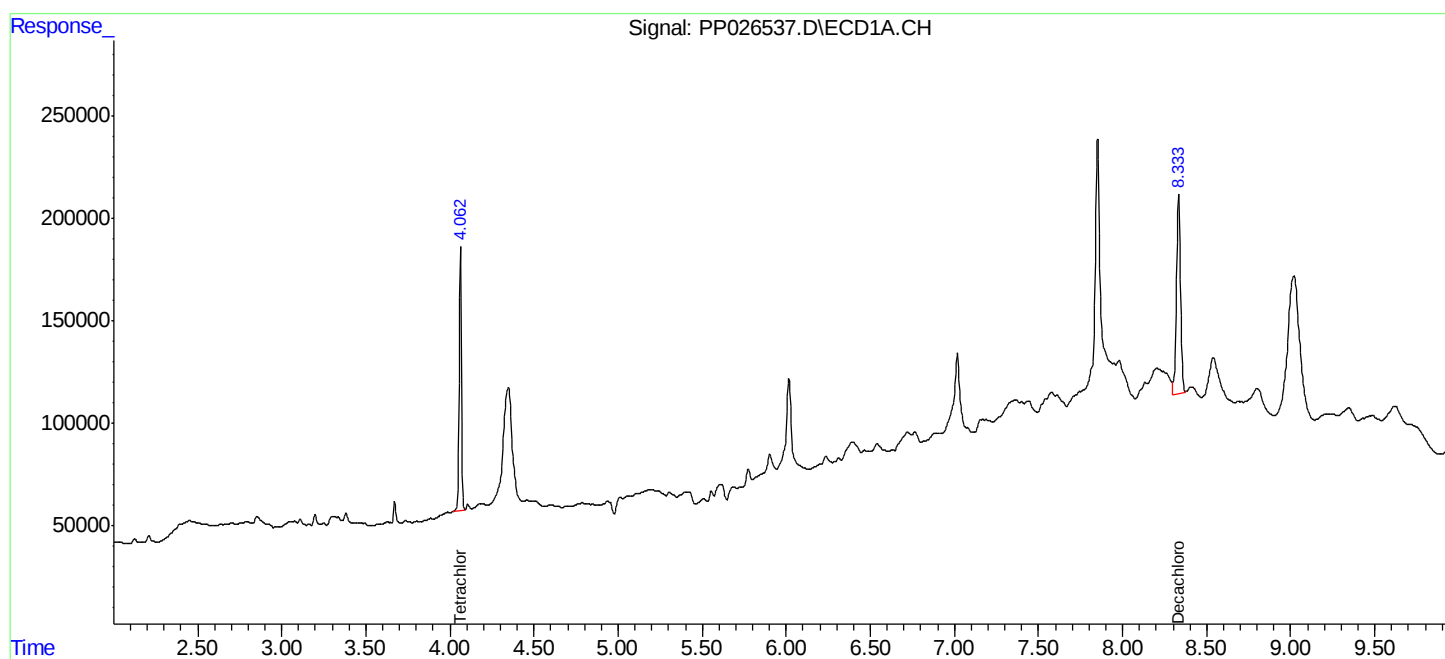

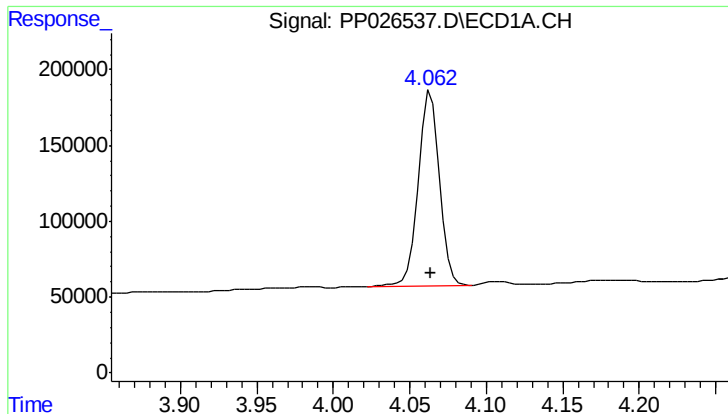


#1 Tetrachloro-m-xylene

R.T.: 4.064 min
Delta R.T.: 0.000 min
Response: 1226823
Conc: 13.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-56-COMP


Manual Integrations
APPROVED

ugo
6/22/2018 10:43:02 AM

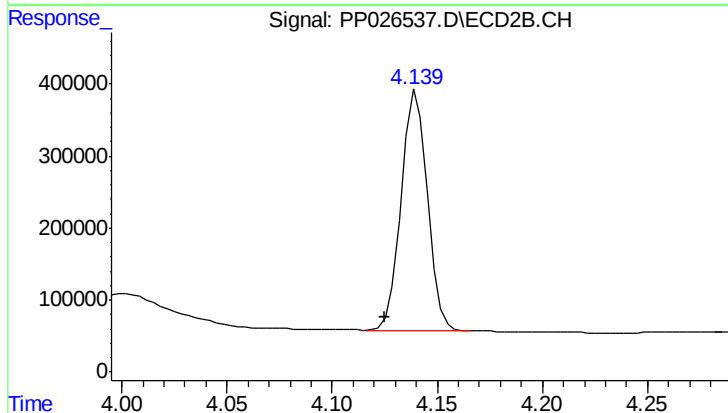


#1 Tetrachloro-m-xylene

R.T.: 4.139 min
Delta R.T.: 0.014 min
Response: 2897770
Conc: 12.17 ng/ml m

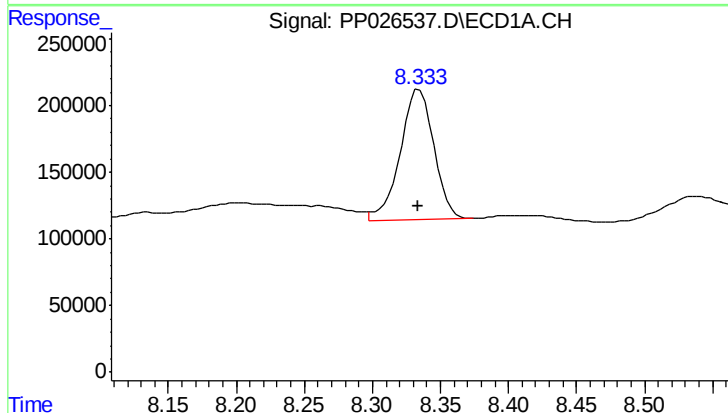

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: 0.000 min
Response: 1665640
Conc: 11.48 ng/ml

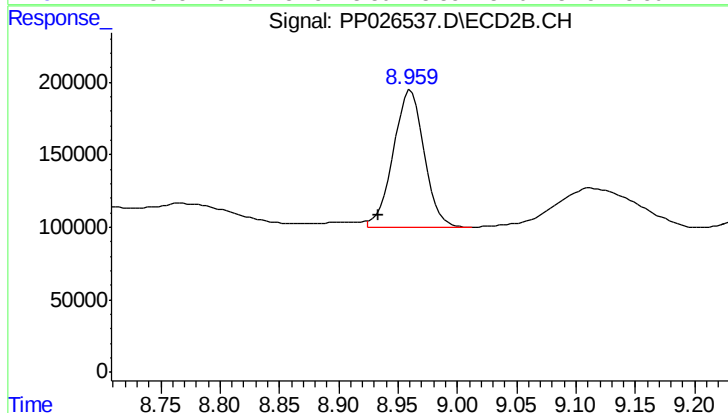

#2 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: 0.026 min
Response: 1724102
Conc: 10.93 ng/ml m