

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP026538.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 16:23
 Operator : UA/AJ
 Sample : J3532-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OILY-WATER-DRUMS-1-2

Manual Integrations
 APPROVED

ugo
 6/22/2018 10:43:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 16:38:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 14:06:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.063	4.132	1663864	821610	18.033	3.450m#
2) SA Decachlor...	8.308	8.895	3544691	241530	24.433	1.531m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026538.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 16:23
Operator : UA/AJ
Sample : J3532-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OILY-WATER-DRUMS-1-2


Manual Integrations
APPROVED

ugo
6/22/2018 10:43:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 16:38:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

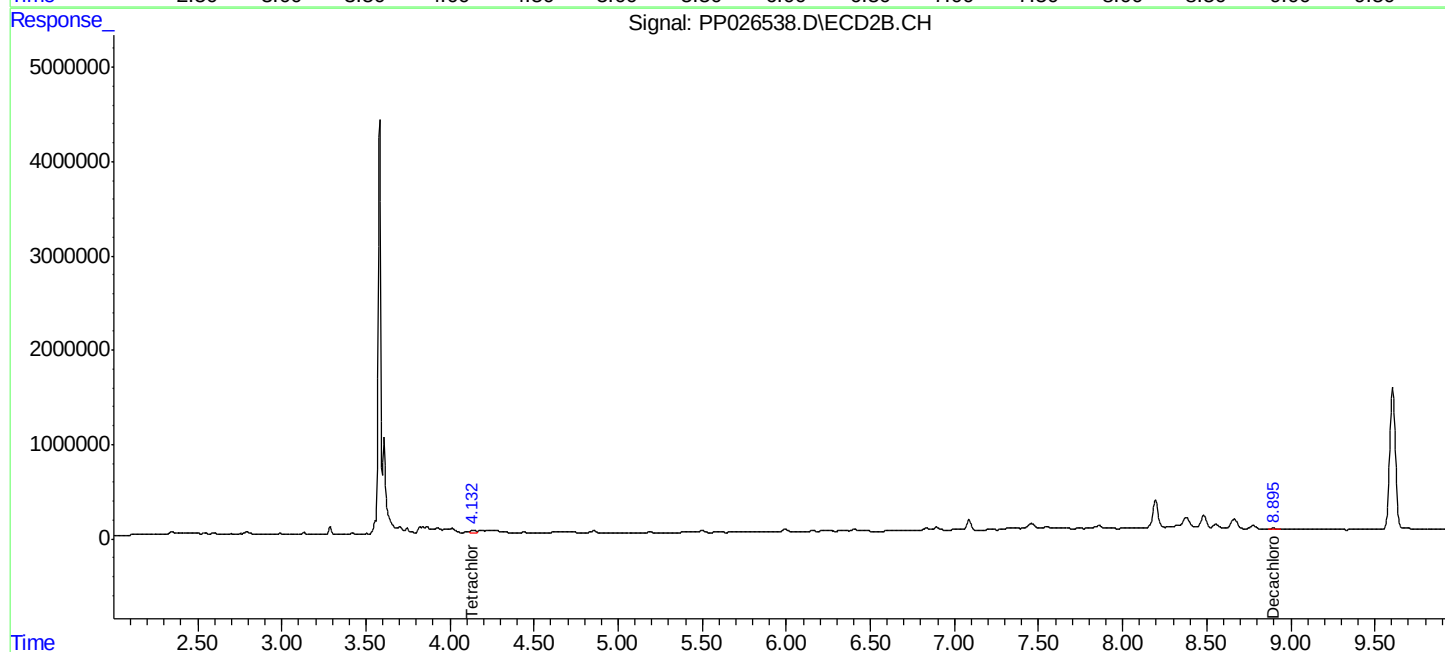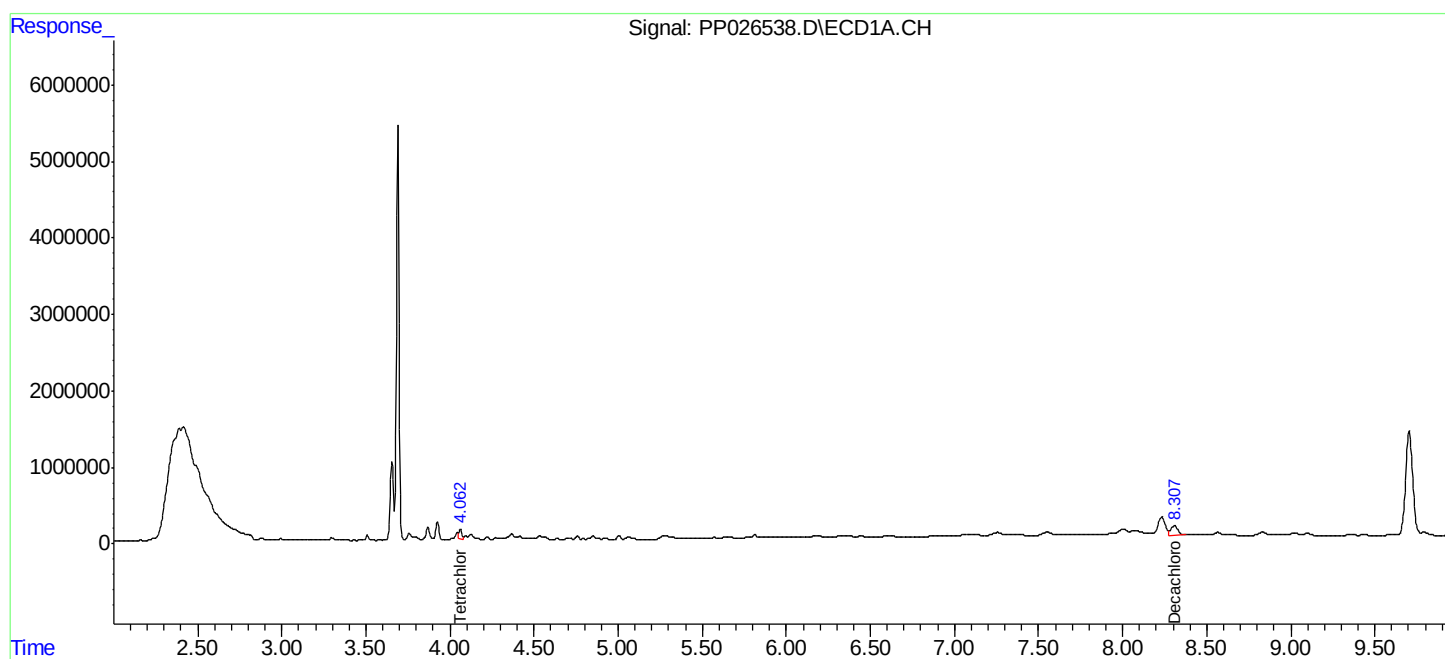

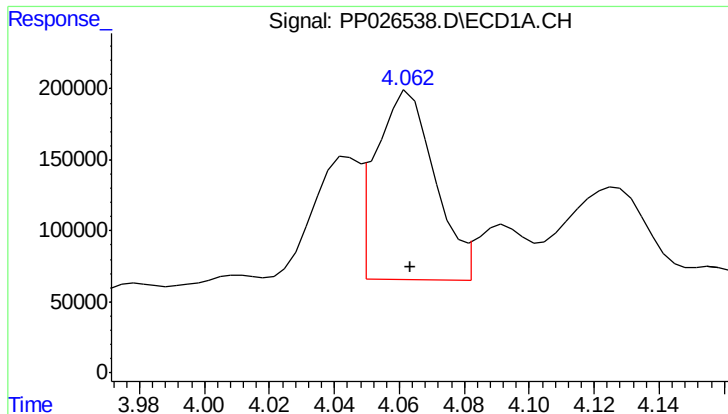


#1 Tetrachloro-m-xylene

R.T.: 4.063 min
Delta R.T.: 0.000 min
Response: 1663864
Conc: 18.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
OILY-WATER-DRUMS-1-2


Manual Integrations
APPROVED

ugo
6/22/2018 10:43:05 AM

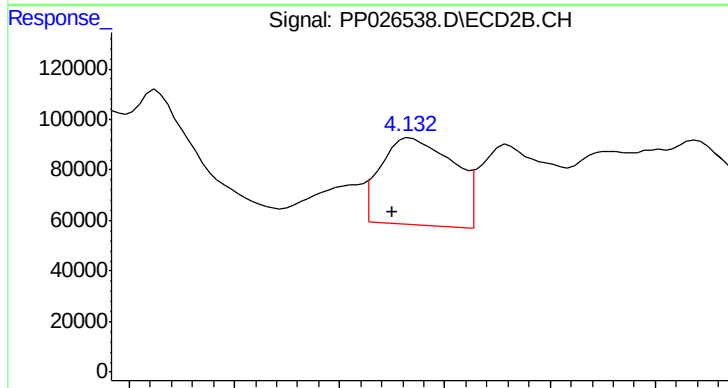


#1 Tetrachloro-m-xylene

R.T.: 4.132 min
Delta R.T.: 0.007 min
Response: 821610
Conc: 3.45 ng/ml m

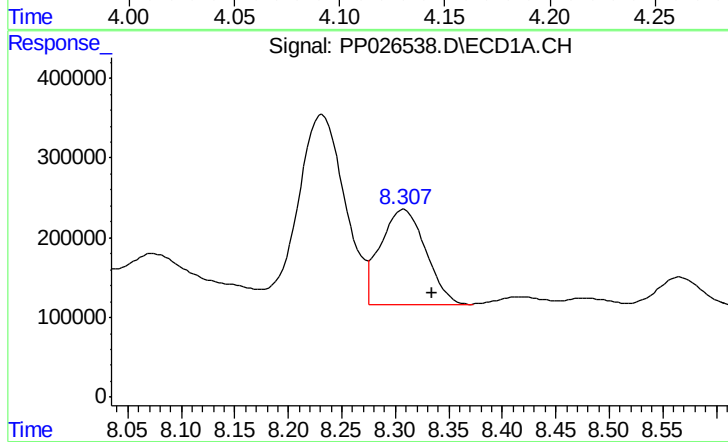

#2 Decachlorobiphenyl

R.T.: 8.308 min
Delta R.T.: -0.026 min
Response: 3544691
Conc: 24.43 ng/ml

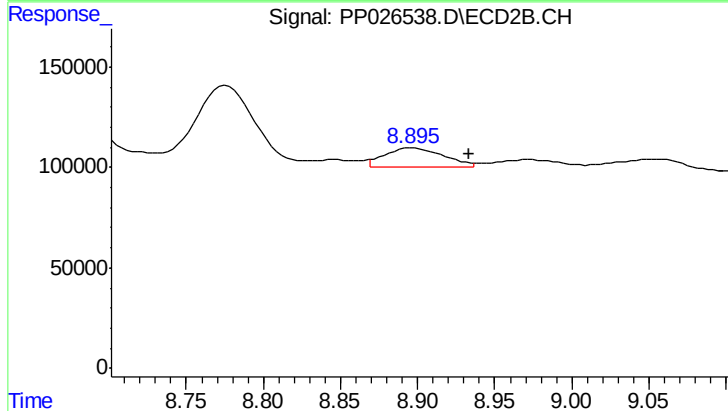

#2 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: -0.038 min
Response: 241530
Conc: 1.53 ng/ml m