

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP026540.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 16:51
 Operator : UA/AJ
 Sample : J3505-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-55-COMP

Manual Integrations
 APPROVED

Sohil
 6/23/2018 1:39:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:45:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 14:06:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.064	4.141	1569377	3604328	17.009	15.136m
2)	SA Decachlor...	8.335	8.964	1760365	1871067	12.134	11.859

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026540.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 16:51
Operator : UA/AJ
Sample : J3505-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-55-COMP


Manual Integrations
APPROVED

Sohil
6/23/2018 1:39:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:45:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

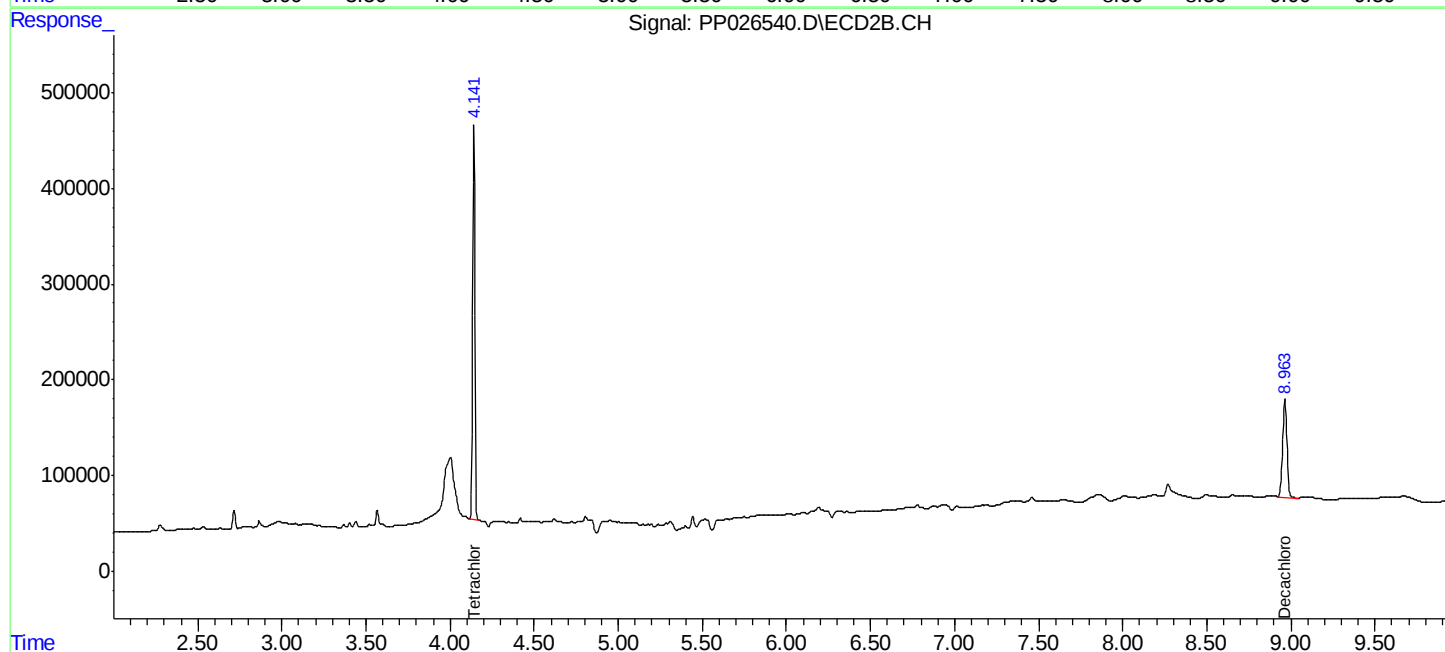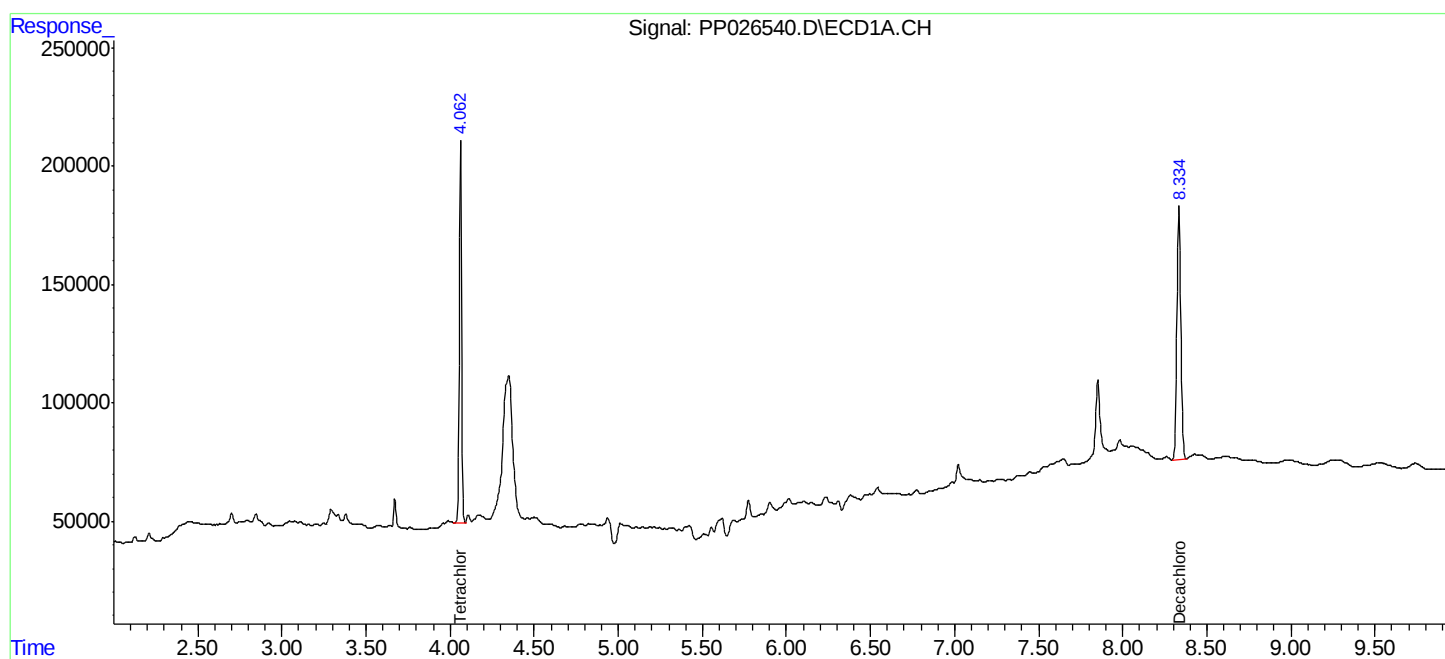

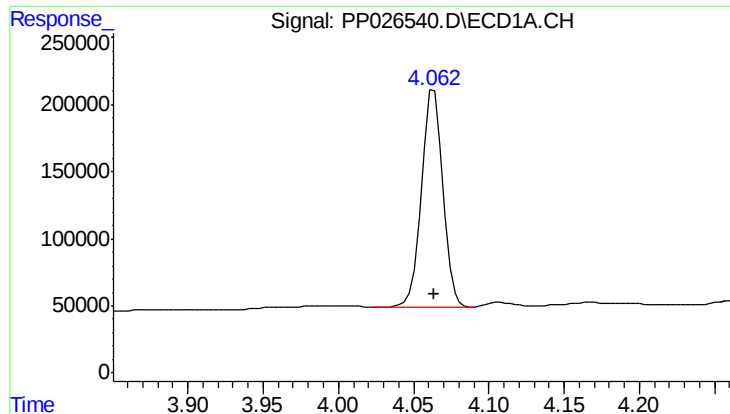


#1 Tetrachloro-m-xylene

R.T.: 4.064 min
Delta R.T.: 0.000 min
Response: 1569377
Conc: 17.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-55-COMP


Manual Integrations
APPROVED

Sohil
6/23/2018 1:39:53 AM

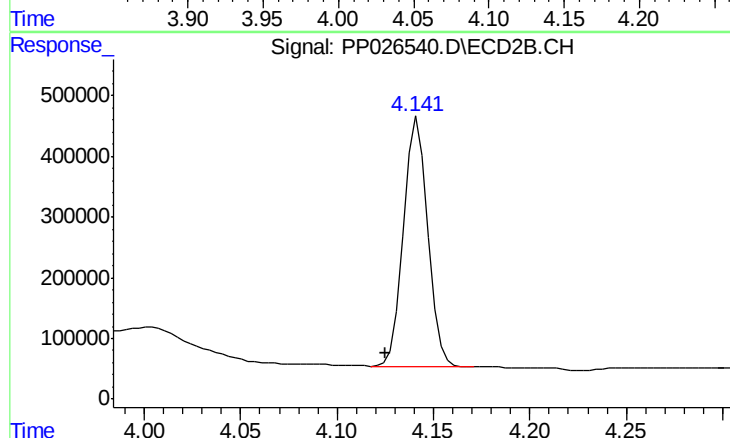


#1 Tetrachloro-m-xylene

R.T.: 4.141 min
Delta R.T.: 0.015 min
Response: 3604328
Conc: 15.14 ng/ml m

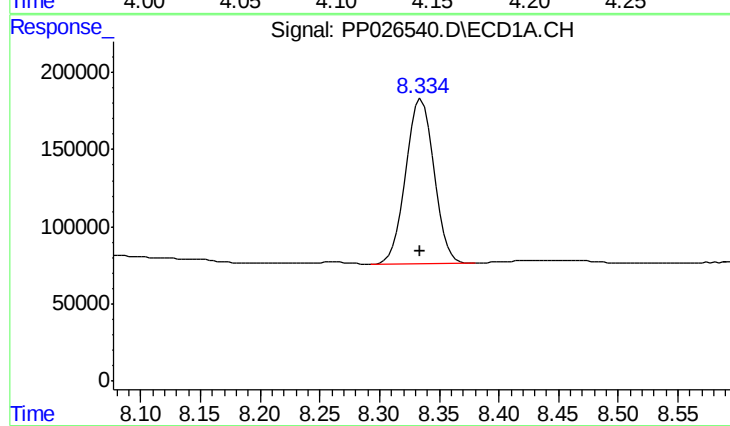

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: 0.001 min
Response: 1760365
Conc: 12.13 ng/ml

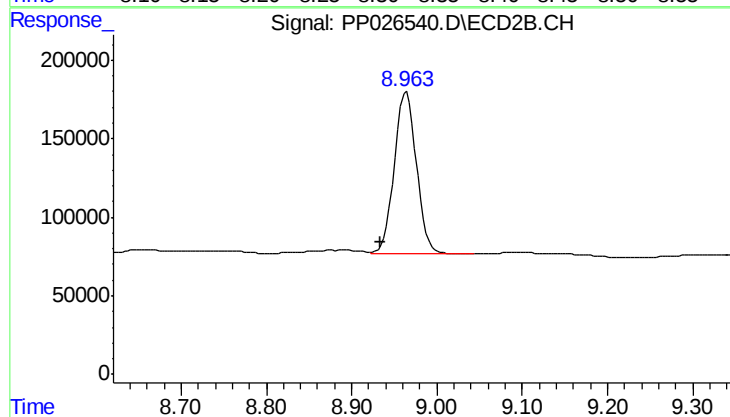

#2 Decachlorobiphenyl

R.T.: 8.964 min
Delta R.T.: 0.031 min
Response: 1871067
Conc: 11.86 ng/ml