

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026541.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 17:06
Operator : UA/AJ
Sample : J3464-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-38-COMP

Manual Integrations
APPROVED

Sohil
6/23/2018 1:40:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:51:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.062	4.143	1650848	3956485	17.892m	16.615
2)	SA Decachlor...	8.332	8.965	3370173	2053286	23.230	13.013 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026541.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 17:06
Operator : UA/AJ
Sample : J3464-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-38-COMP


Manual Integrations
APPROVED

Sohil
6/23/2018 1:40:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:51:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

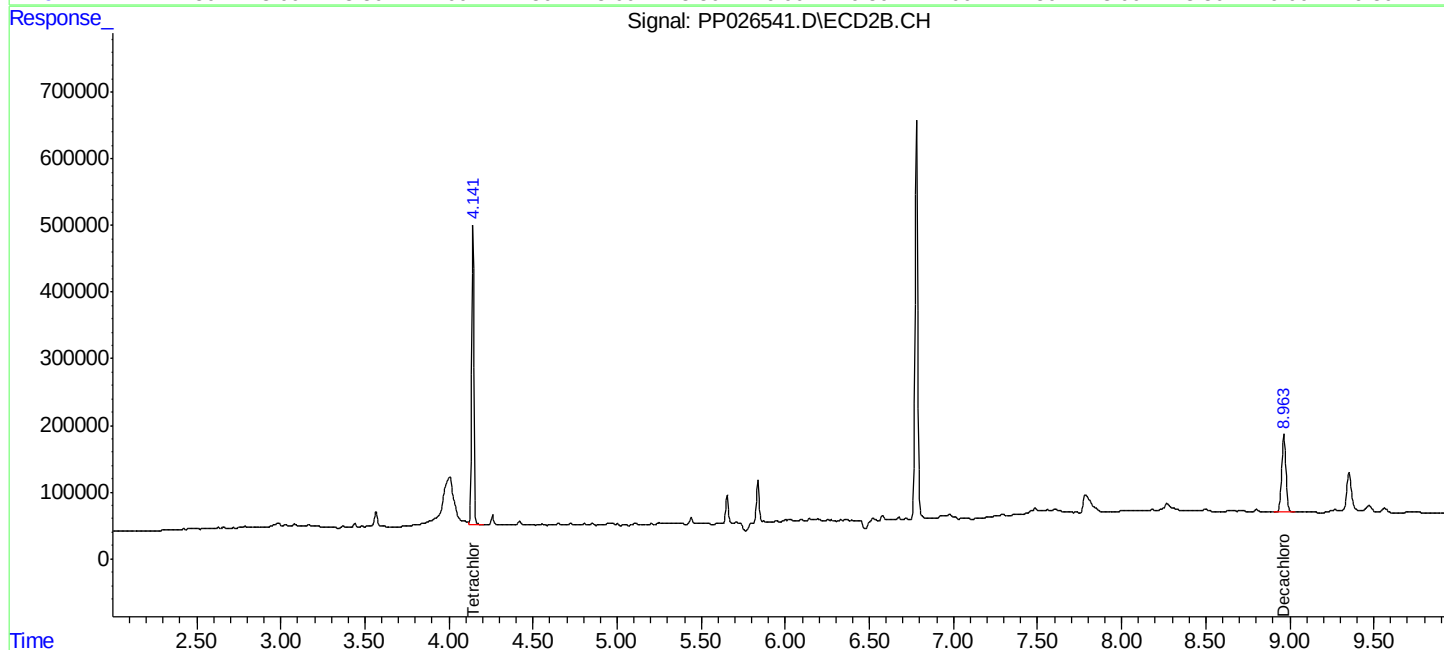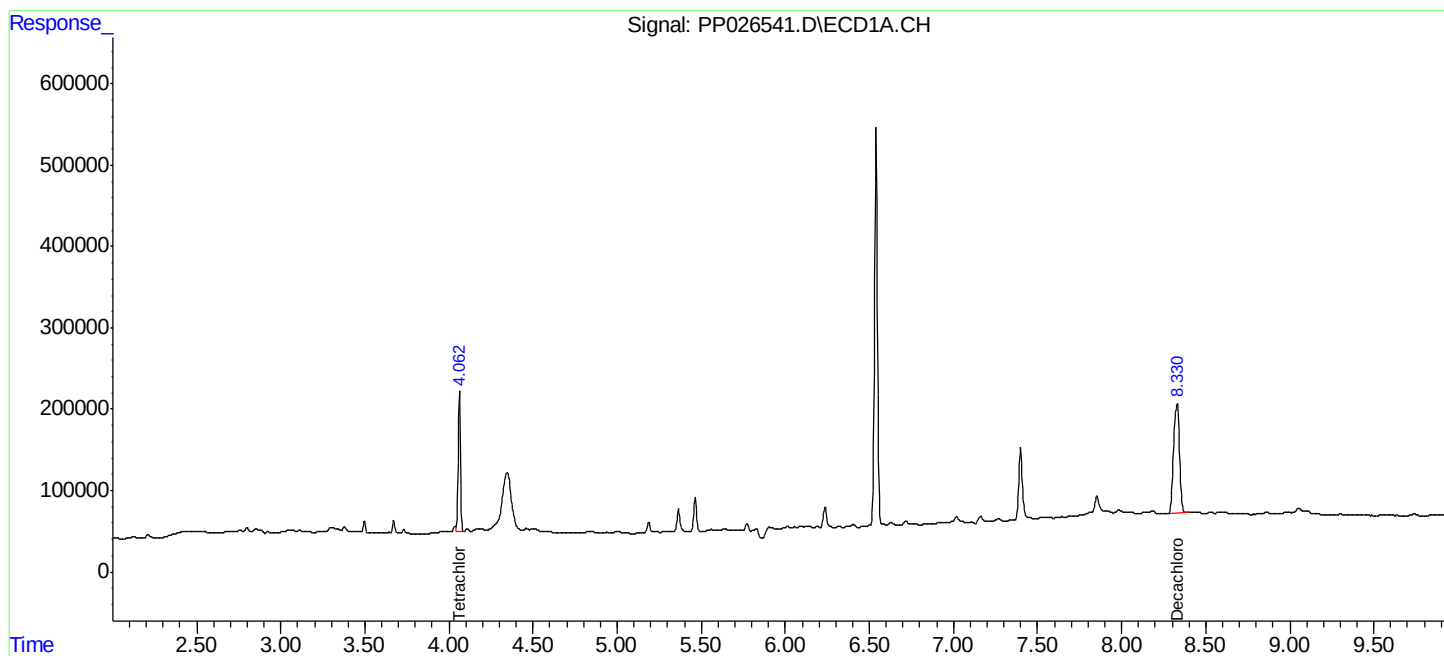

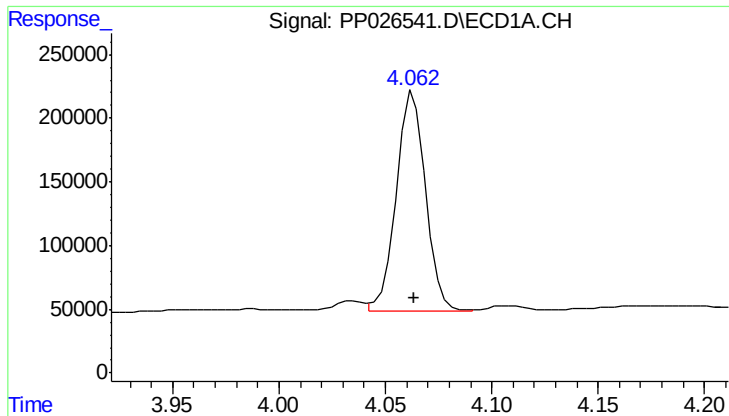


#1 Tetrachloro-m-xylene

R.T.: 4.062 min
Delta R.T.: -0.002 min
Response: 1650848
Conc: 17.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-38-COMP


Manual Integrations
APPROVED

Sohil
6/23/2018 1:40:00 AM

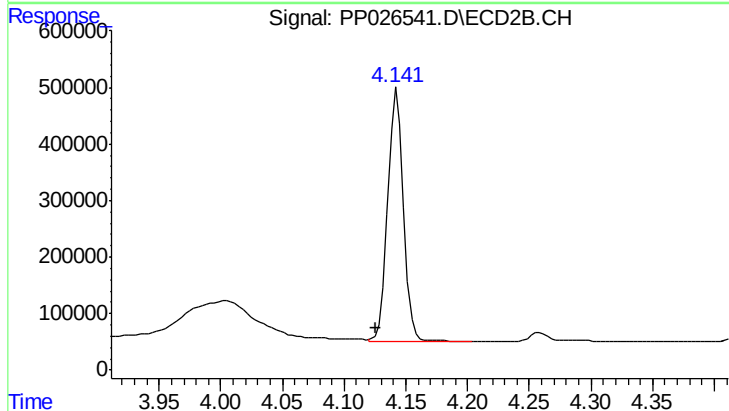


#1 Tetrachloro-m-xylene

R.T.: 4.143 min
Delta R.T.: 0.018 min
Response: 3956485
Conc: 16.62 ng/ml

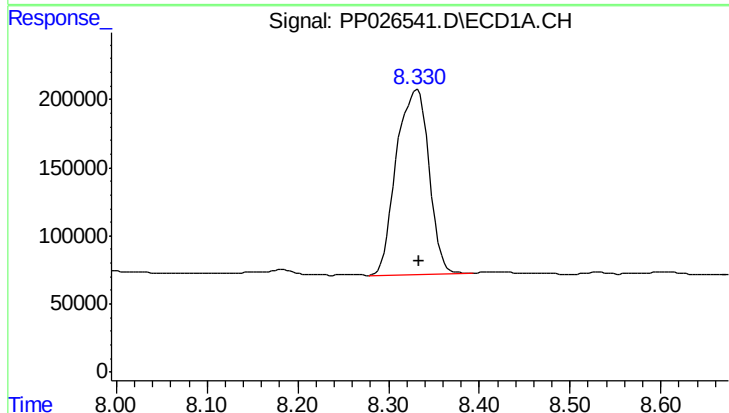

#2 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: -0.002 min
Response: 3370173
Conc: 23.23 ng/ml

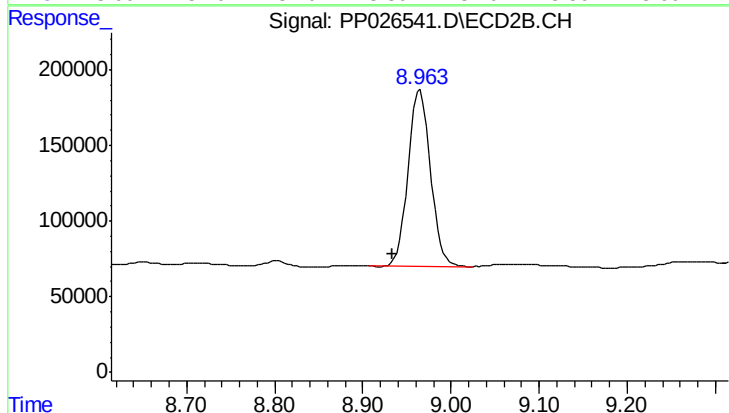

#2 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: 0.032 min
Response: 2053286
Conc: 13.01 ng/ml