

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP026556.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 20:54
 Operator : UA/AJ
 Sample : J3546-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 061418-DBRC-F-D-B

Manual Integrations
 APPROVED

ugo
 6/22/2018 10:43:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 07:52:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 14:06:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.063	4.163	1762379	2970598	19.101	12.475m#
2)	SA Decachlor...	8.335	9.002	2253450	2547390	15.533	16.145m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026556.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 20:54
Operator : UA/AJ
Sample : J3546-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
061418-DBRC-F-D-B


Manual Integrations
APPROVED

ugo
6/22/2018 10:43:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 07:52:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

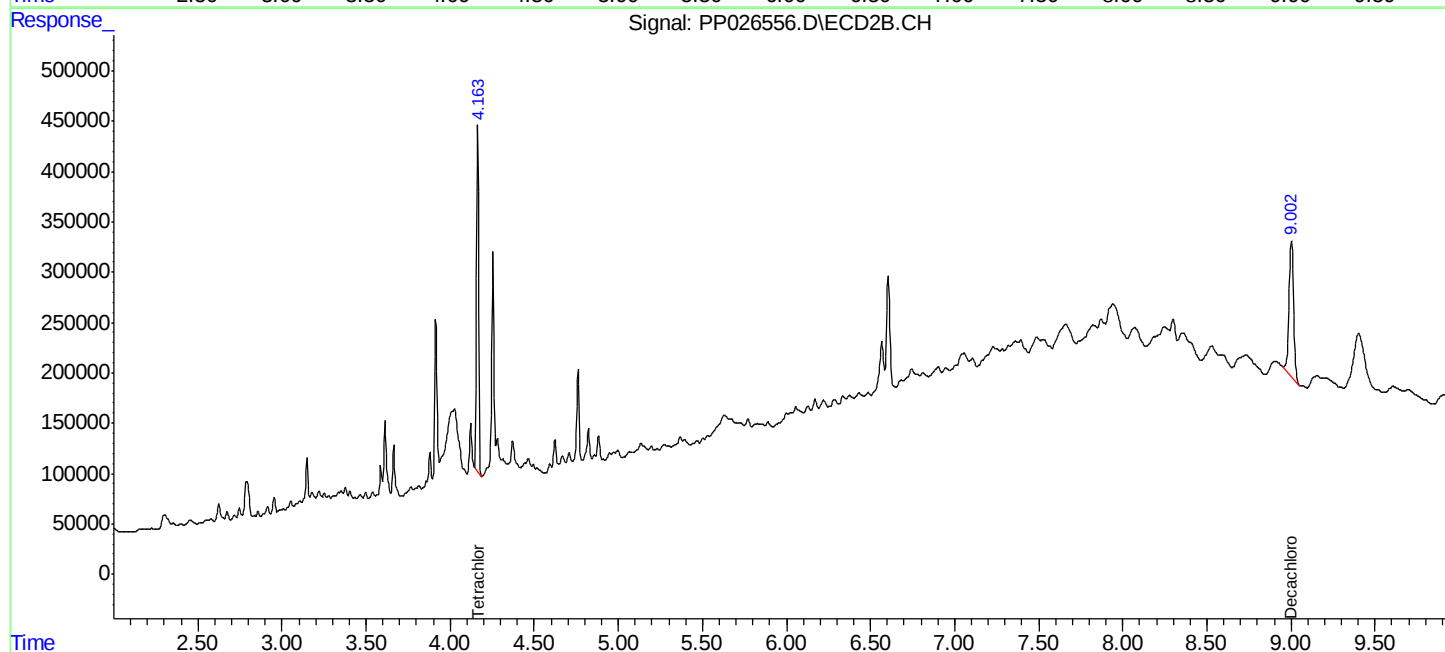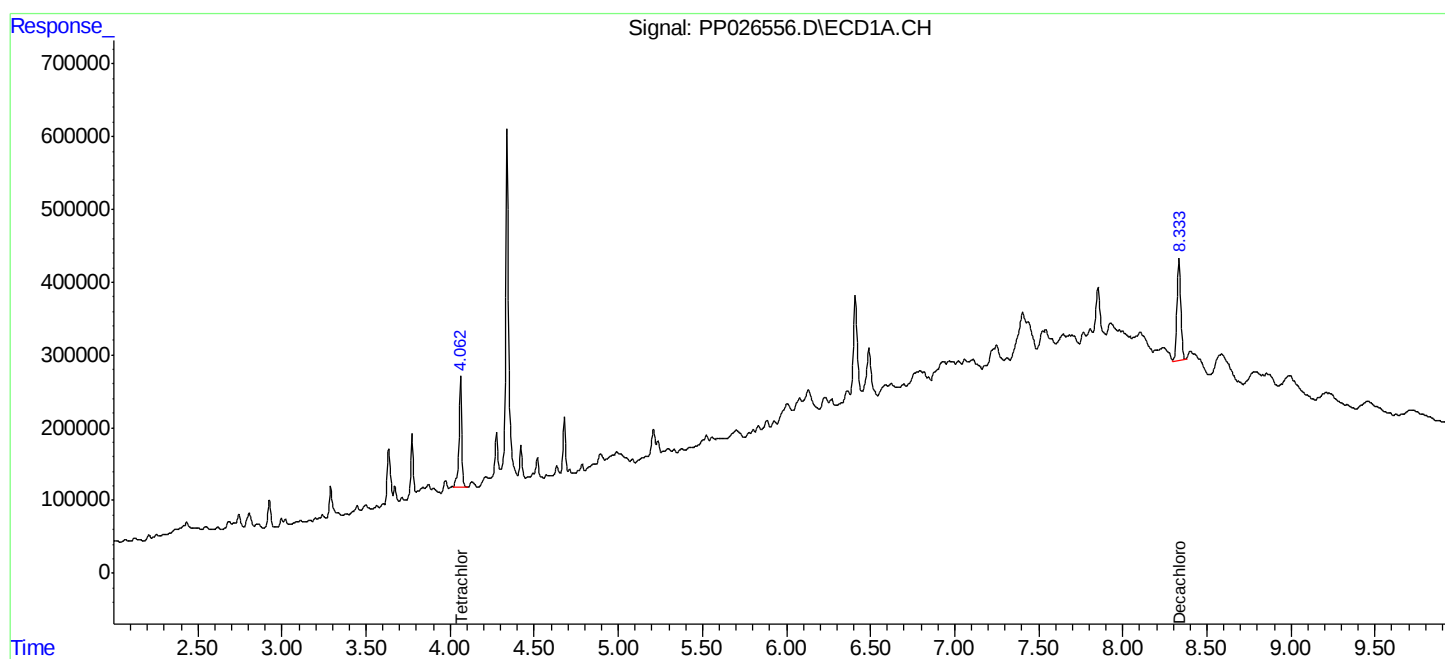

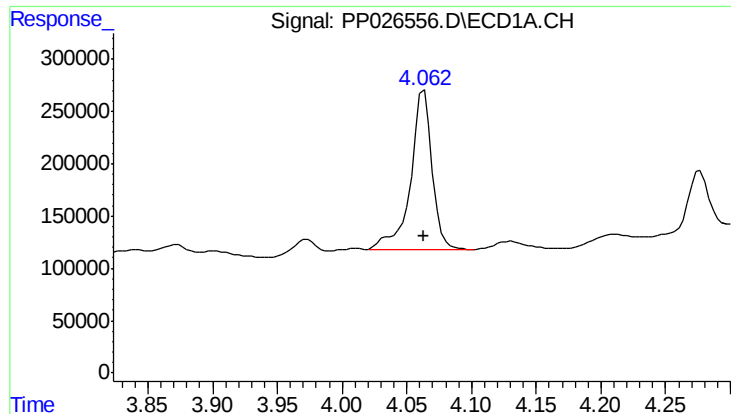


#1 Tetrachloro-m-xylene

R.T.: 4.063 min
Delta R.T.: 0.000 min
Response: 1762379
Conc: 19.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
061418-DBRC-F-D-B


Manual Integrations
APPROVED

ugo
6/22/2018 10:43:56 AM

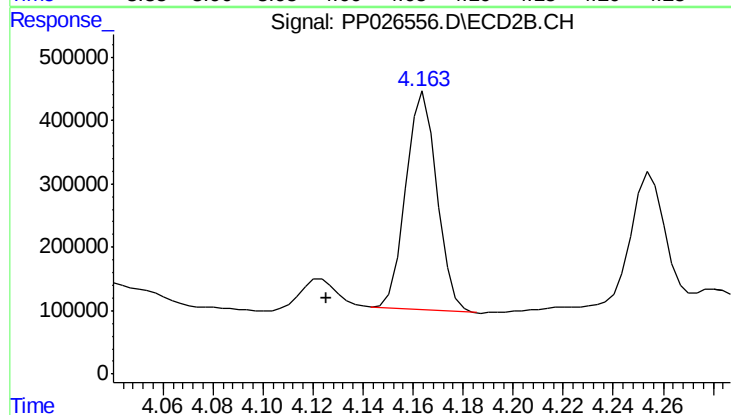


#1 Tetrachloro-m-xylene

R.T.: 4.163 min
Delta R.T.: 0.038 min
Response: 2970598
Conc: 12.48 ng/ml m

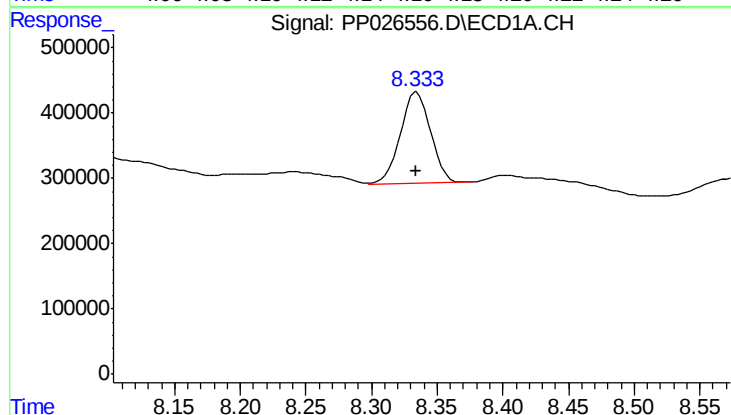

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: 0.000 min
Response: 2253450
Conc: 15.53 ng/ml

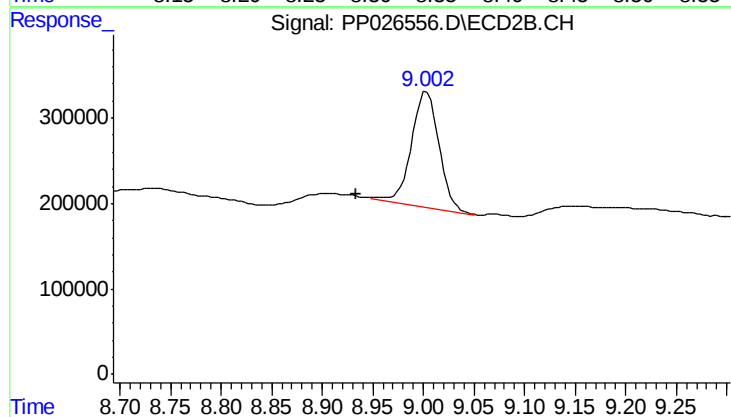

#2 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: 0.069 min
Response: 2547390
Conc: 16.14 ng/ml m