

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026557.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 21:08
Operator : UA/AJ
Sample : J3546-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
061418-DBRC-F-D-S

Manual Integrations
APPROVED

ugo
6/22/2018 10:44:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 07:53:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.063	4.164	1564105	2861405	16.952	12.017m#
2)	SA Decachlor...	8.336	9.003	2166818	2283055	14.936	14.470m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026557.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 21:08
Operator : UA/AJ
Sample : J3546-02
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
061418-DBRC-F-D-S


Manual Integrations
APPROVED

ugo
6/22/2018 10:44:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 07:53:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

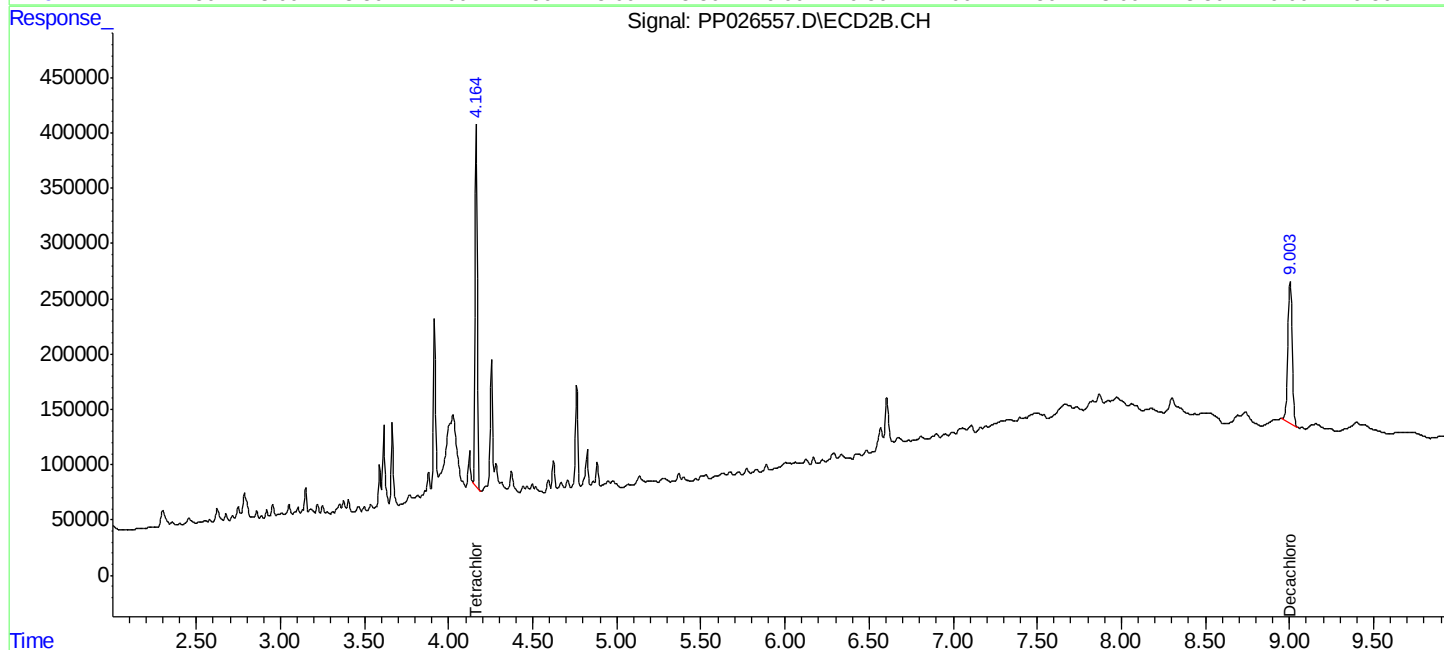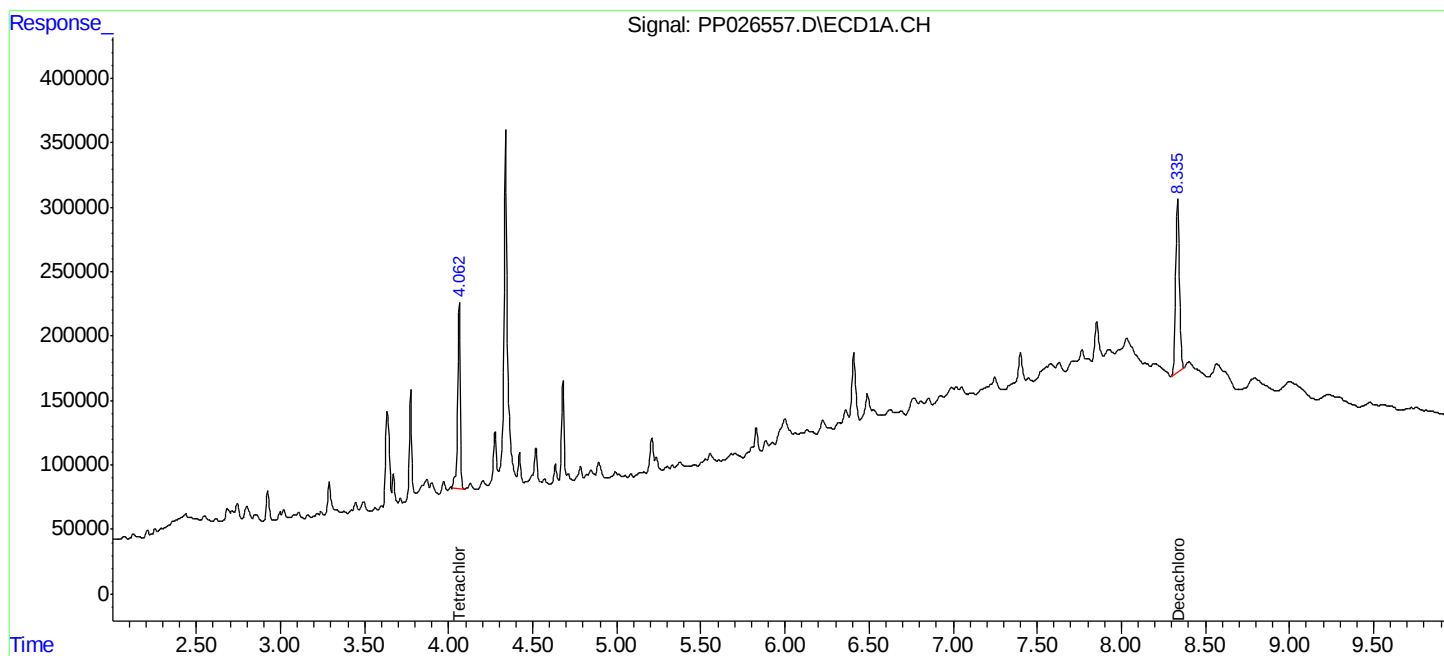

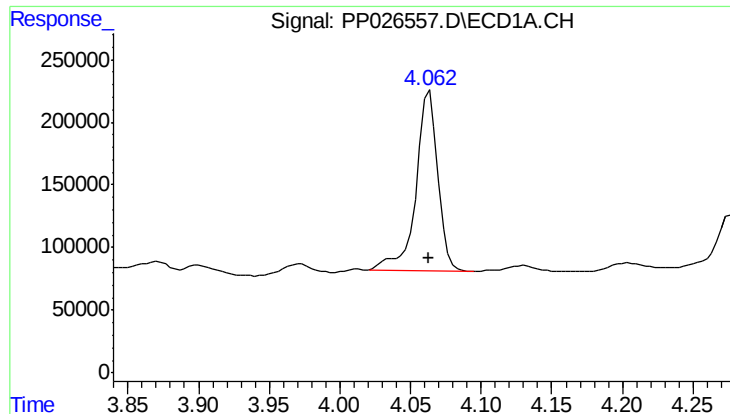


#1 Tetrachloro-m-xylene

R.T.: 4.063 min
Delta R.T.: 0.000 min
Response: 1564105
Conc: 16.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
061418-DBRC-F-D-S


Manual Integrations
APPROVED

ugo
6/22/2018 10:44:58 AM

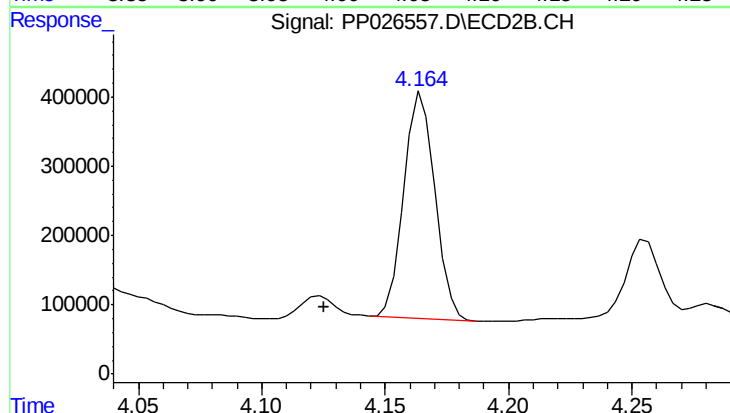


#1 Tetrachloro-m-xylene

R.T.: 4.164 min
Delta R.T.: 0.038 min
Response: 2861405
Conc: 12.02 ng/ml m

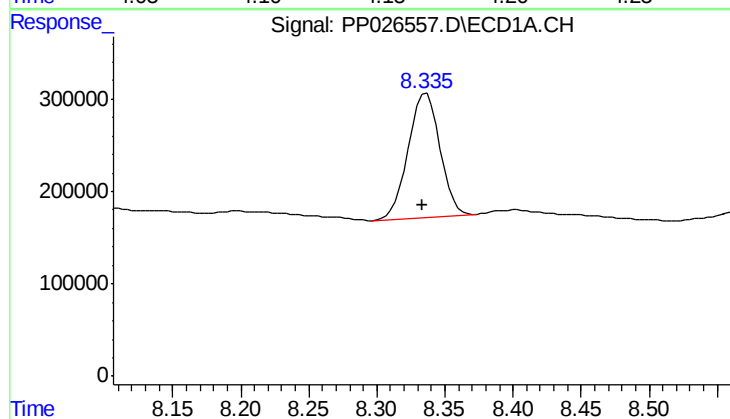

#2 Decachlorobiphenyl

R.T.: 8.336 min
Delta R.T.: 0.002 min
Response: 2166818
Conc: 14.94 ng/ml

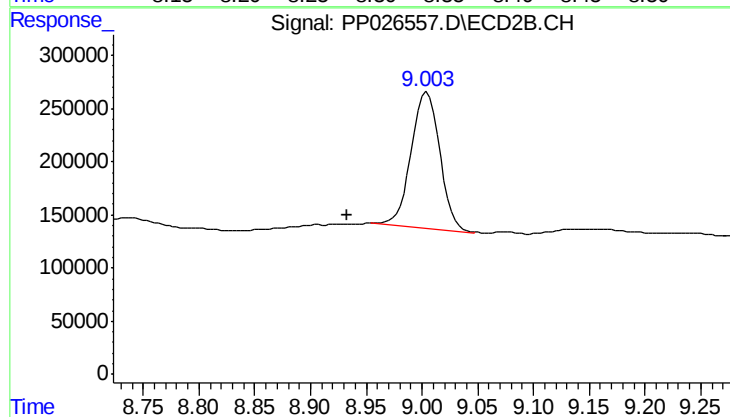

#2 Decachlorobiphenyl

R.T.: 9.003 min
Delta R.T.: 0.070 min
Response: 2283055
Conc: 14.47 ng/ml m