

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP062571.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 00:26
 Operator : UA/AJ
 Sample : PB110361BS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB110361BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 08:14:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 08:00:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.063	4.192	1787700	4057245	19.633	17.870
2) SA Decachlor...	8.335	9.050	4405557	3369971	29.482	21.171 #
Target Compounds						
3) L1 Aroclor-1...	4.569	4.549	604277	713879	266.298	182.315 #
4) L1 Aroclor-1...	4.995	4.993	633287	440573	241.660	151.837 #
5) L1 Aroclor-1...	5.041	5.266	433134	1054605	241.078	180.017 #
6) L1 Aroclor-1...	5.366	5.345	1104933	677814	915.196	179.502 #
7) L1 Aroclor-1...	5.366	5.611	1104933	805209	736.669	201.613 #
8) L2 Aroclor-1...	0.000	4.310	0	66822	N.D.	20.967 #
9) L2 Aroclor-1...	4.321	4.402	1126625	125019	931.126	62.028 #
10) L2 Aroclor-1...	4.321	4.504	1126625	171495	239.570	23.748 #
11) L3 Aroclor-1...	4.569	4.919	604277	148632	470.342	90.744 #
12) L3 Aroclor-1...	4.995	5.166	633287	1682388	431.944	535.282
13) L3 Aroclor-1...	5.041	5.266	433134	1054605	421.246	510.573
14) L3 Aroclor-1...	5.366	5.469	1104933	596320	1732.139	283.291 #
15) L3 Aroclor-1...	5.366	5.840	1104933	214708	1288.022	88.466 #
16) L4 Aroclor-1...	4.569	4.721	604277	110754	294.403	18.148 #
17) L4 Aroclor-1...	4.900	5.104	1339221	137988	291.305	18.223 #
18) L4 Aroclor-1...	4.995	5.266	633287	1054605	295.233	350.283
19) L4 Aroclor-1...	5.287	0.000	545404	0	267.162	N.D. #
20) L4 Aroclor-1...	5.564	5.648	184758	534902	103.969	111.060
21) L5 Aroclor-1...	5.287	0.000	545404	0	159.996	N.D. #
22) L5 Aroclor-1...	5.366	5.648	1104933	534902	573.843	73.494 #
23) L5 Aroclor-1...	5.564	5.840	184758	214708	61.044	30.533 #
24) L5 Aroclor-1...	5.564	5.840	184758	214708	59.896	27.109 #
25) L5 Aroclor-1...	5.752	6.059	579073	592985	196.399	80.236 #
26) L6 Aroclor-1...	5.752	5.840	579073	214708	125.556	29.471 #
27) L6 Aroclor-1...	5.962	6.011	438058	88810	131.245	11.457 #
28) L6 Aroclor-1...	6.056	6.338	408162	261882	67.269	20.185 #
29) L6 Aroclor-1...	6.269	6.638	320565	251055	54.602	48.747
30) L6 Aroclor-1...	6.629	6.975	2505911	425534	329.753	39.421 #
31) L7 Aroclor-1...	6.194	6.582	1235604	1871982	342.145	234.369 #
32) L7 Aroclor-1...	6.629	6.733	2505911	2082002	270.196	229.591
33) L7 Aroclor-1...	6.716	7.068	1525363	165946	229.958	26.159 #
34) L7 Aroclor-1...	6.915	7.356	1234767	1570072	236.428	214.107
35) L7 Aroclor-1...	7.162	7.547	4177902	3313769	220.560	206.560
36) L8 Aroclor-1...	6.194	6.638	1235604	251055	370.852	30.802 #
37) L8 Aroclor-1...	6.405	6.841	2159931	764183	321.983	162.325 #
38) L8 Aroclor-1...	6.716	7.037	1525363	2977190	131.834	270.053 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP026571.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 00:26
 Operator : UA/AJ
 Sample : PB110361BS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB110361BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 08:14:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 21 08:00:15 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39)	L8 Aroclor-1...	6.915	7.251	1234767	289362	152.710	28.954 #
40)	L8 Aroclor-1...	7.162	7.465	4177902	865656	157.975	41.086 #
41)	L9 Aroclor-1...	7.400	7.849	45128363	30586937	1662.728	1485.504
42)	L9 Aroclor-1...	7.456	7.849	1106491	30586937	53.561	1628.405 #
44)	L9 Aroclor-1...	7.906	8.241	1258308	447334	152.859	60.333 #
45)	L9 Aroclor-1...	8.155	0.000	384519	0	6.416	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 00:26
Operator : UA/AJ
Sample : PB110361BS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB110361BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 08:14:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 21 08:00:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

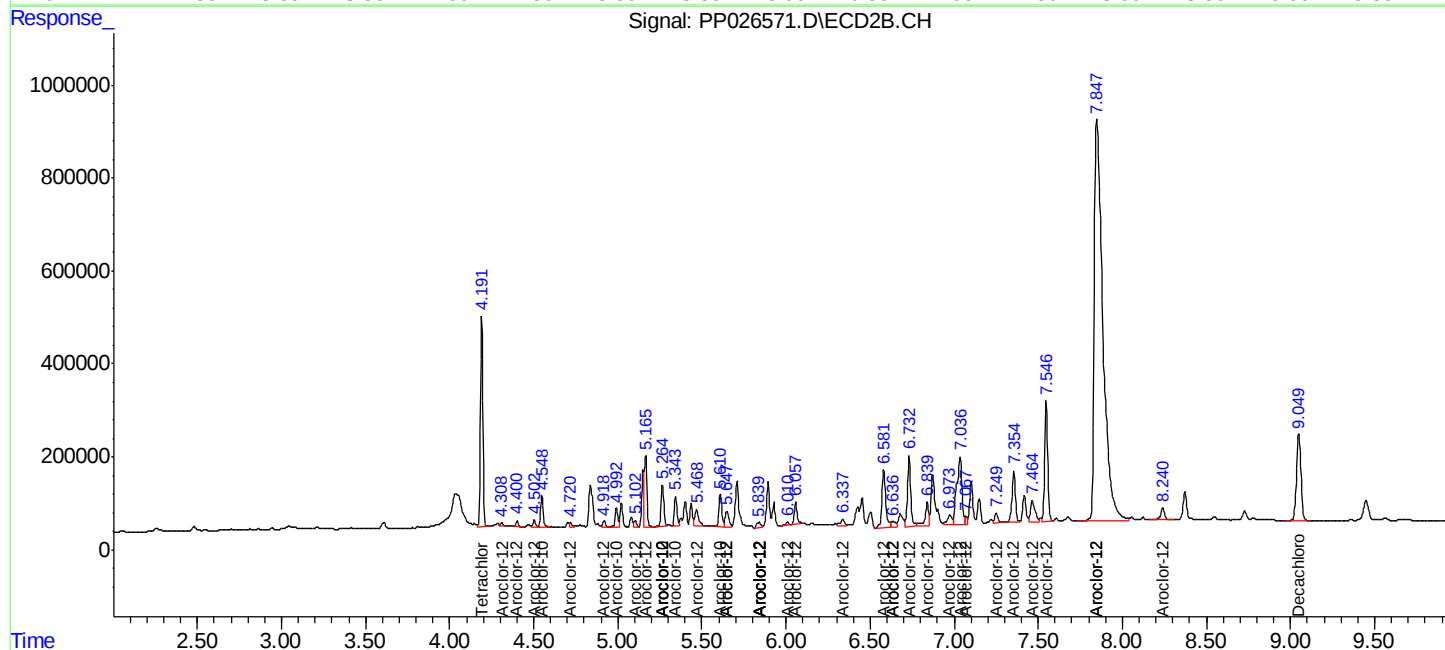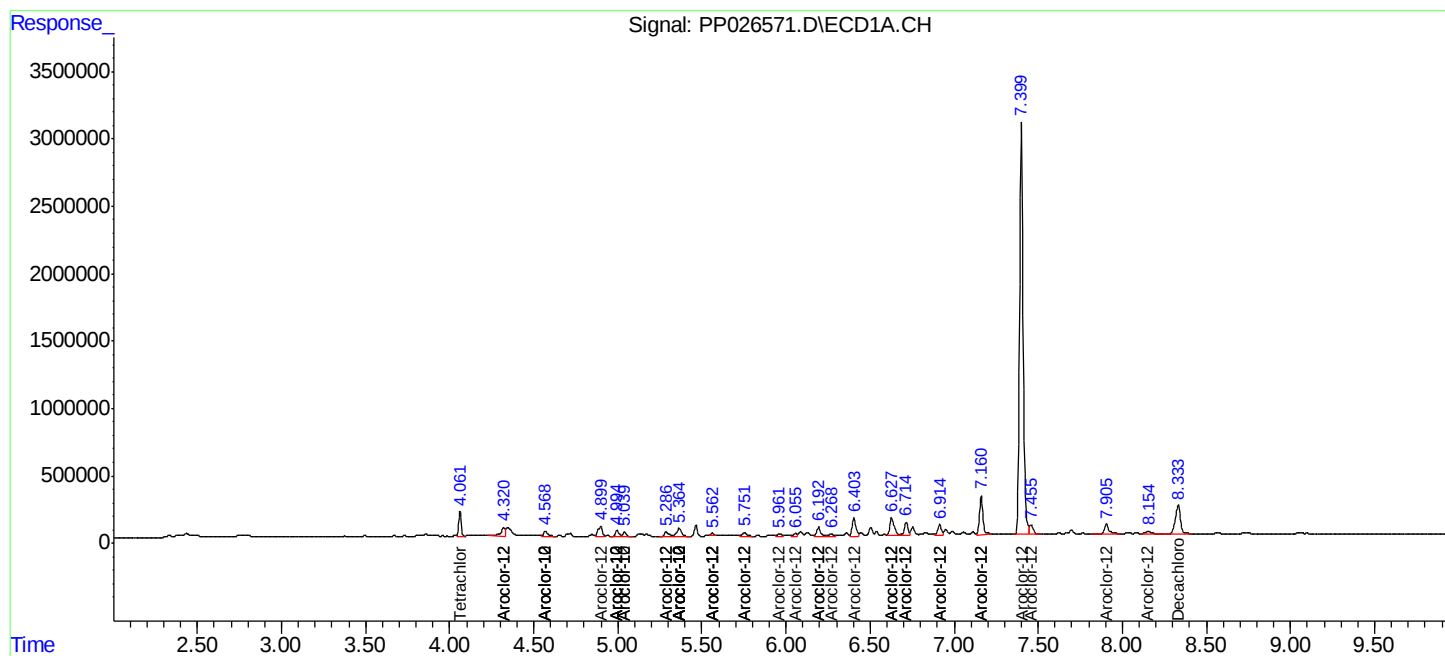


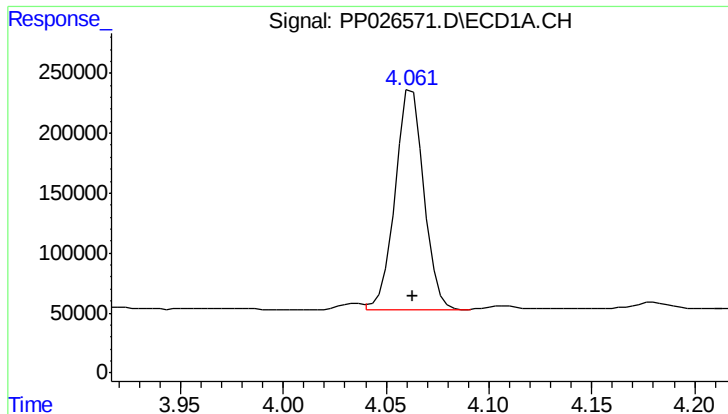

#1 Tetrachloro-m-xylene


R.T.: 4.063 min
Delta R.T.: 0.000 min
Response: 1787700
Conc: 19.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

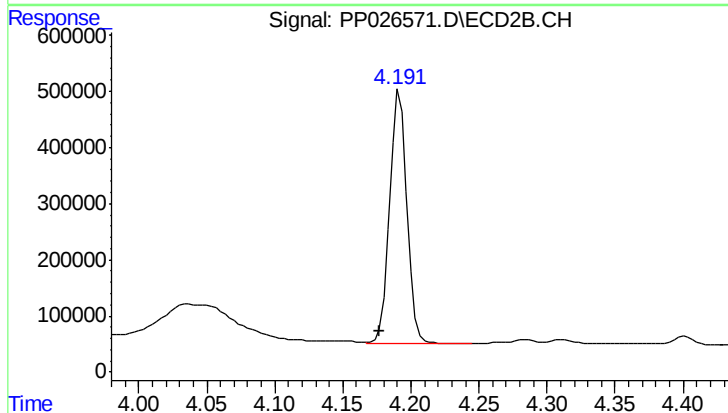


#1 Tetrachloro-m-xylene

R.T.: 4.192 min
Delta R.T.: 0.015 min
Response: 4057245
Conc: 17.87 ng/ml

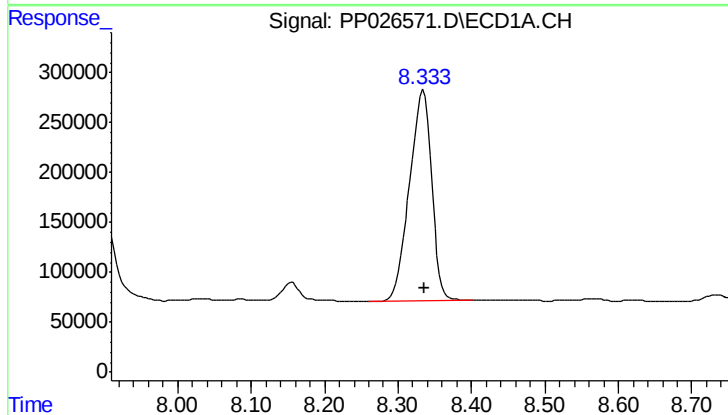


#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: 0.000 min
Response: 4405557
Conc: 29.48 ng/ml

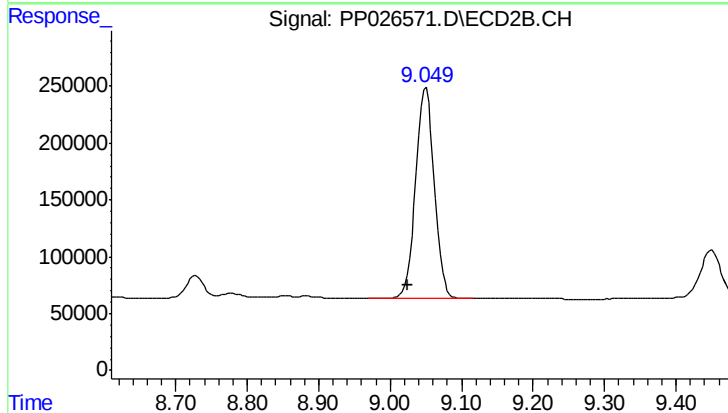

#2 Decachlorobiphenyl


R.T.: 9.050 min
Delta R.T.: 0.025 min
Response: 3369971
Conc: 21.17 ng/ml

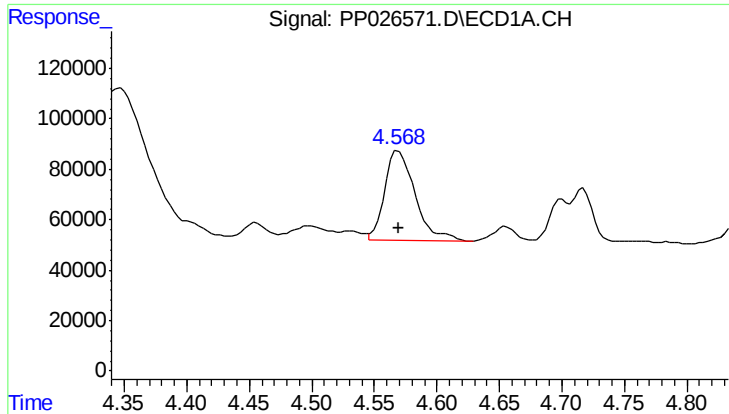

#3 Aroclor-1016-1


R.T.: 4.569 min
Delta R.T.: 0.000 min
Response: 604277
Conc: 266.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

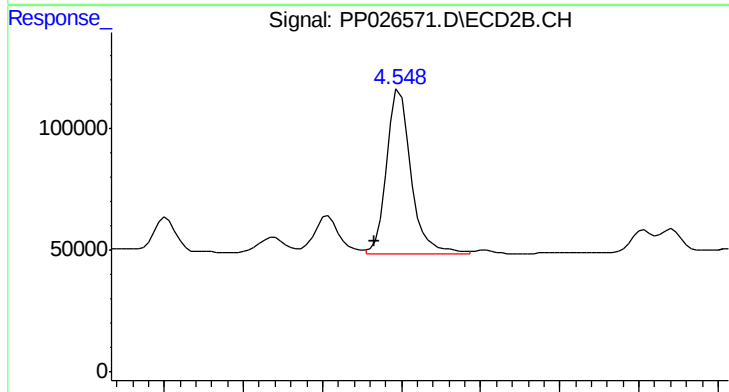


#3 Aroclor-1016-1

R.T.: 4.549 min
Delta R.T.: 0.017 min
Response: 713879
Conc: 182.32 ng/ml

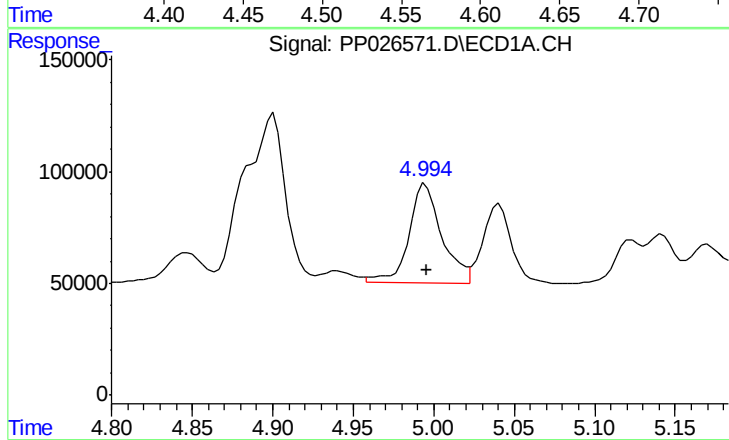


#4 Aroclor-1016-2

R.T.: 4.995 min
Delta R.T.: 0.000 min
Response: 633287
Conc: 241.66 ng/ml

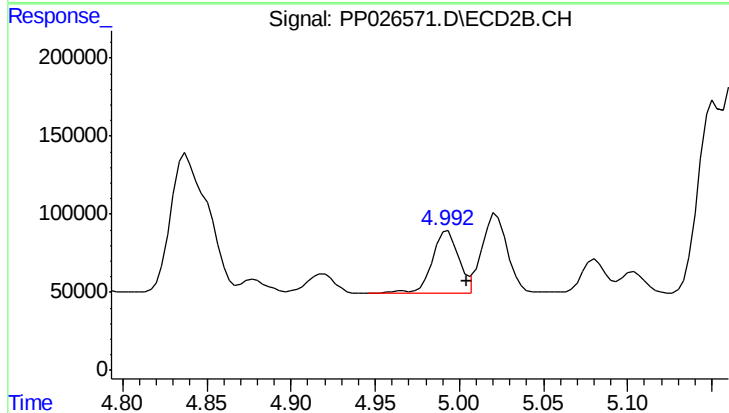

#4 Aroclor-1016-2


R.T.: 4.993 min
Delta R.T.: -0.011 min
Response: 440573
Conc: 151.84 ng/ml

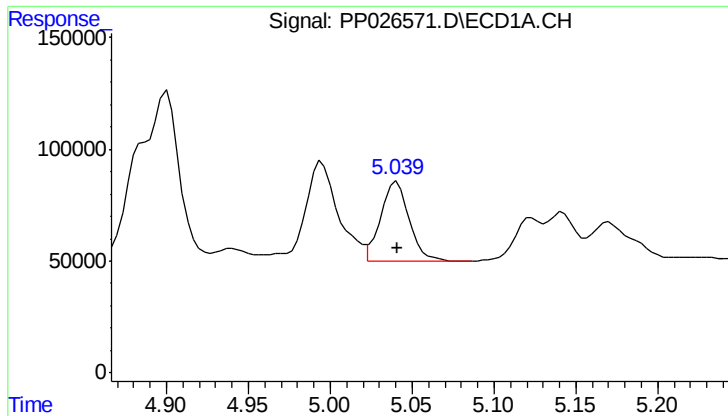

#5 Aroclor-1016-3


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 433134
Conc: 241.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

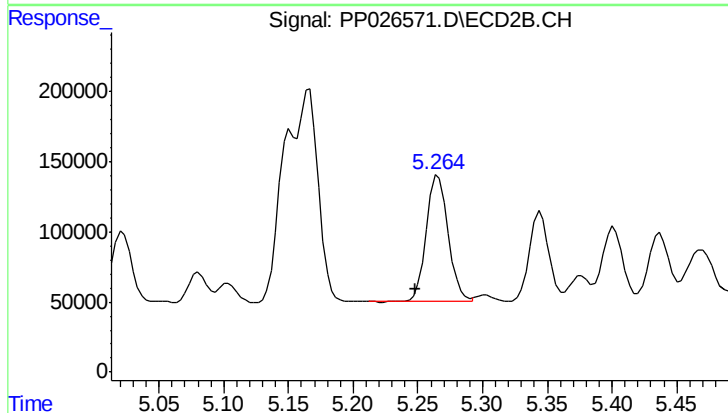


#5 Aroclor-1016-3

R.T.: 5.266 min
Delta R.T.: 0.018 min
Response: 1054605
Conc: 180.02 ng/ml

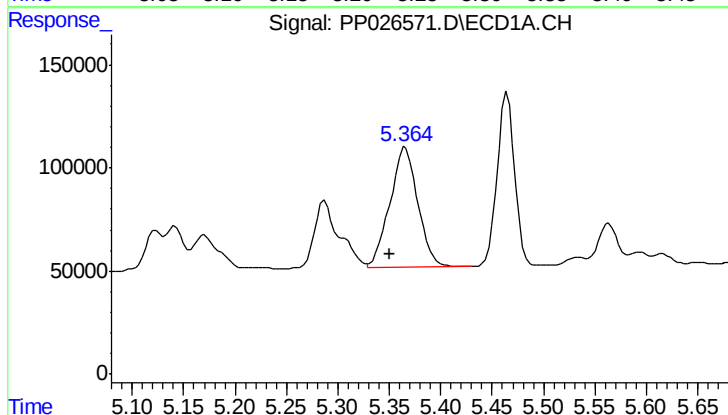


#6 Aroclor-1016-4

R.T.: 5.366 min
Delta R.T.: 0.015 min
Response: 1104933
Conc: 915.20 ng/ml

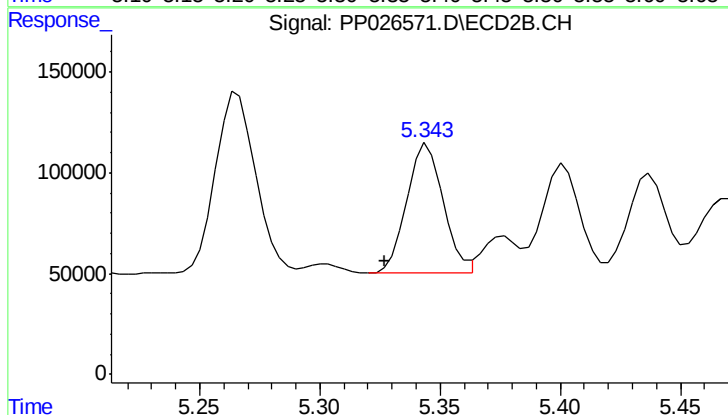

#6 Aroclor-1016-4


R.T.: 5.345 min
Delta R.T.: 0.018 min
Response: 677814
Conc: 179.50 ng/ml

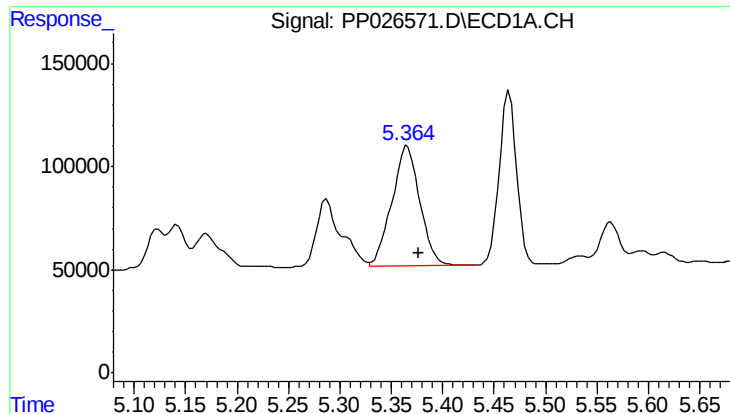

#7 Aroclor-1016-5


R.T.: 5.366 min
Delta R.T.: -0.011 min
Response: 1104933
Conc: 736.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

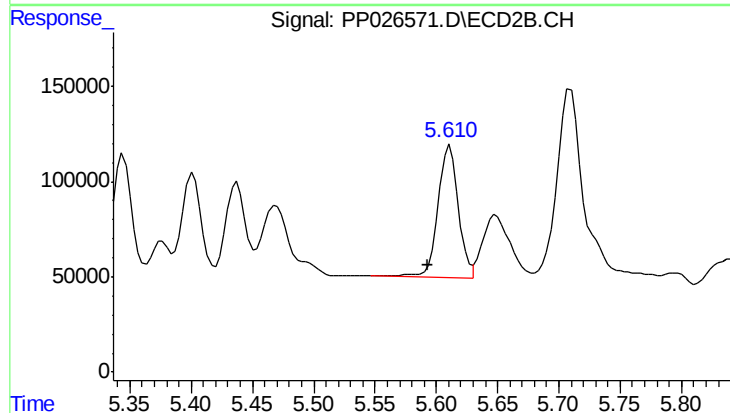


#7 Aroclor-1016-5

R.T.: 5.611 min
Delta R.T.: 0.018 min
Response: 805209
Conc: 201.61 ng/ml

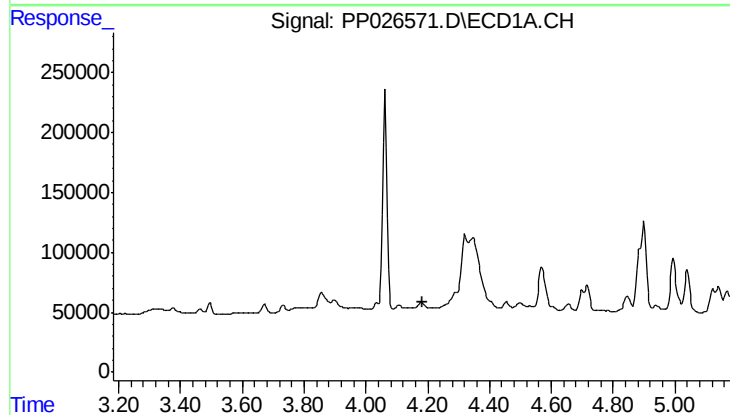


#8 Aroclor-1221-1

R.T.: 0.000 min
Exp R.T.: 4.182 min
Response: 0
Conc: N.D.

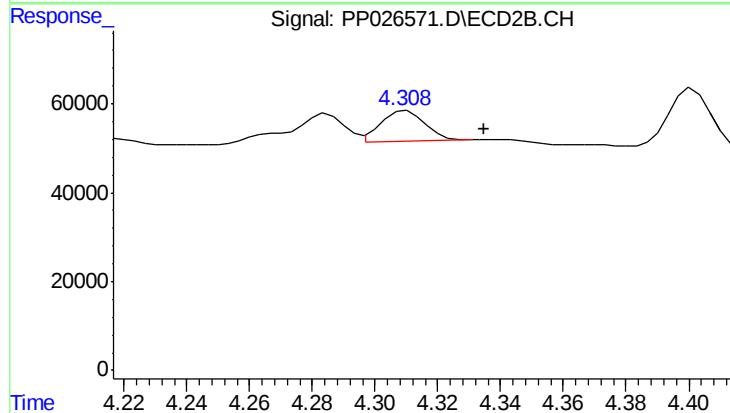

#8 Aroclor-1221-1


R.T.: 4.310 min
Delta R.T.: -0.025 min
Response: 66822
Conc: 20.97 ng/ml

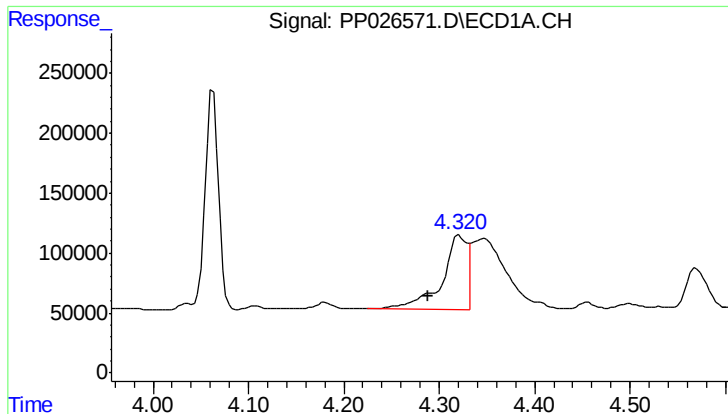

#9 Aroclor-1221-2


R.T.: 4.321 min
Delta R.T.: 0.033 min
Response: 1126625
Conc: 931.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

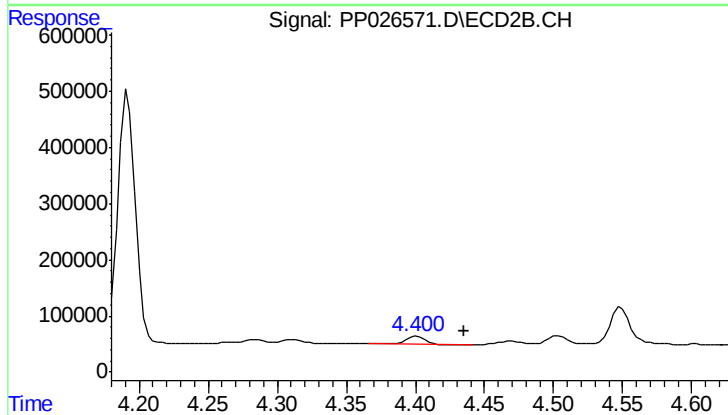


#9 Aroclor-1221-2

R.T.: 4.402 min
Delta R.T.: -0.034 min
Response: 125019
Conc: 62.03 ng/ml

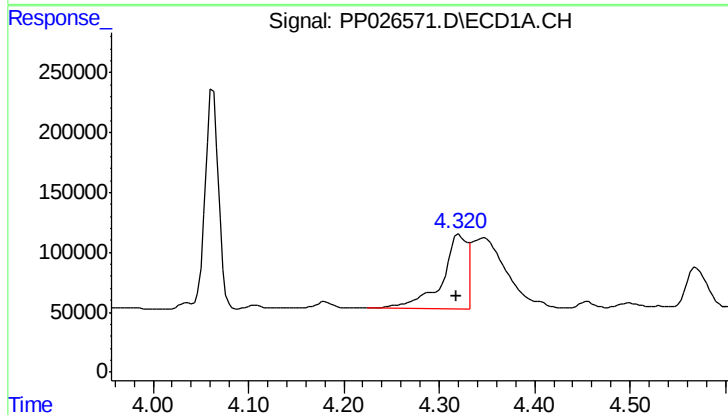


#10 Aroclor-1221-3

R.T.: 4.321 min
Delta R.T.: 0.003 min
Response: 1126625
Conc: 239.57 ng/ml

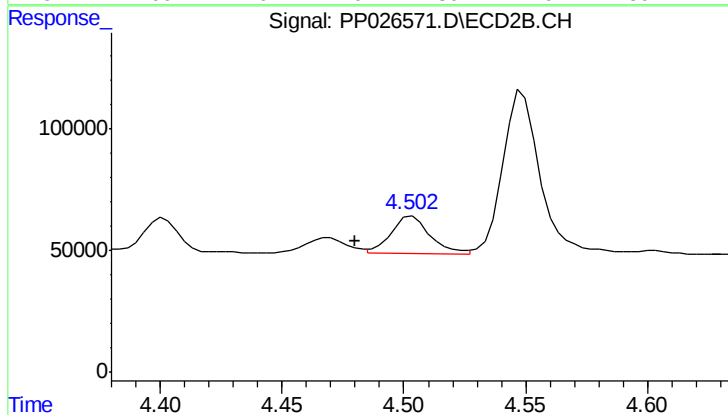

#10 Aroclor-1221-3


R.T.: 4.504 min
Delta R.T.: 0.024 min
Response: 171495
Conc: 23.75 ng/ml

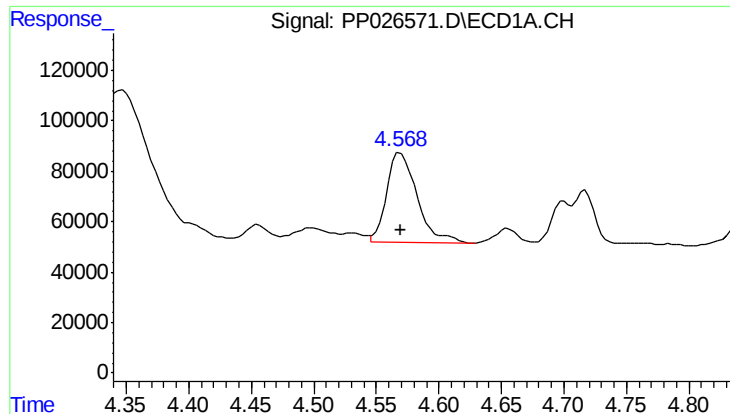

#11 Aroclor-1232-1


R.T.: 4.569 min
Delta R.T.: 0.000 min
Response: 604277
Conc: 470.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

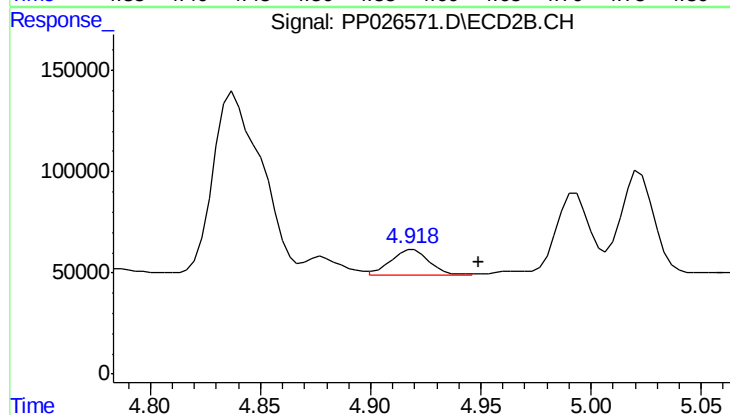


#11 Aroclor-1232-1

R.T.: 4.919 min
Delta R.T.: -0.030 min
Response: 148632
Conc: 90.74 ng/ml

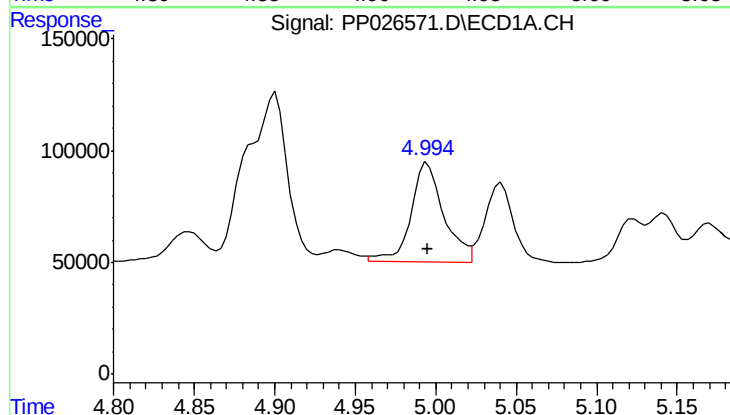


#12 Aroclor-1232-2

R.T.: 4.995 min
Delta R.T.: 0.000 min
Response: 633287
Conc: 431.94 ng/ml

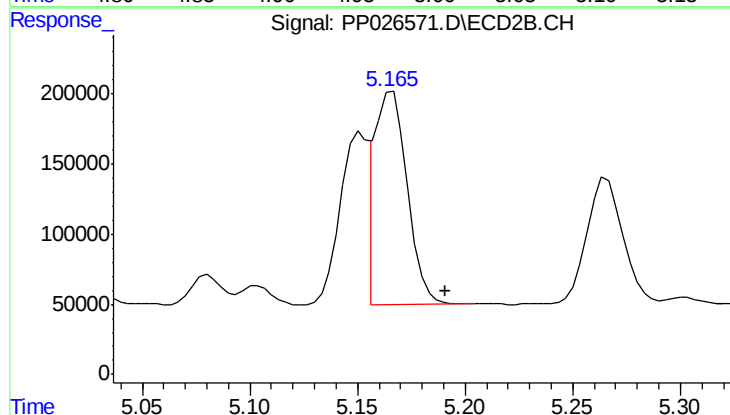

#12 Aroclor-1232-2


R.T.: 5.166 min
Delta R.T.: -0.025 min
Response: 1682388
Conc: 535.28 ng/ml

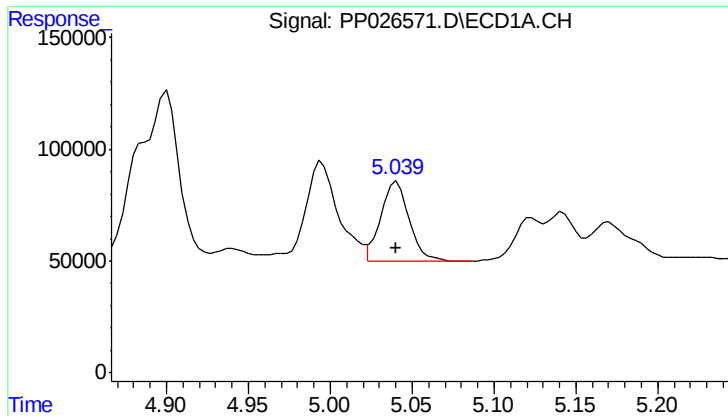

#13 Aroclor-1232-3


R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 433134
Conc: 421.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

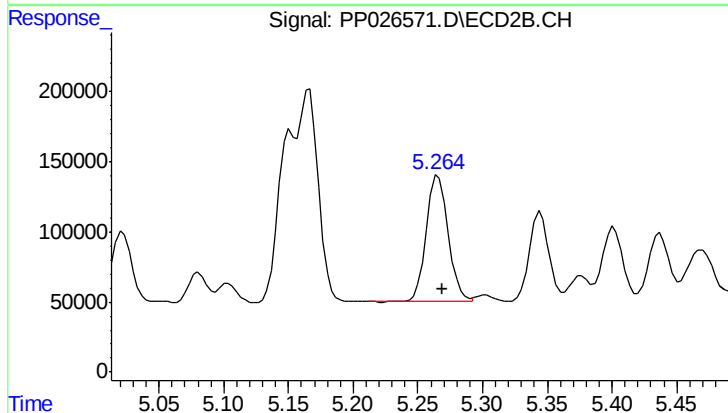


#13 Aroclor-1232-3

R.T.: 5.266 min
Delta R.T.: -0.003 min
Response: 1054605
Conc: 510.57 ng/ml

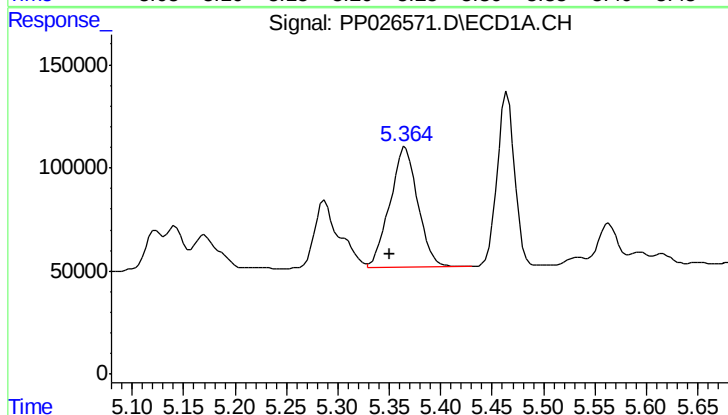


#14 Aroclor-1232-4

R.T.: 5.366 min
Delta R.T.: 0.016 min
Response: 1104933
Conc: 1732.14 ng/ml

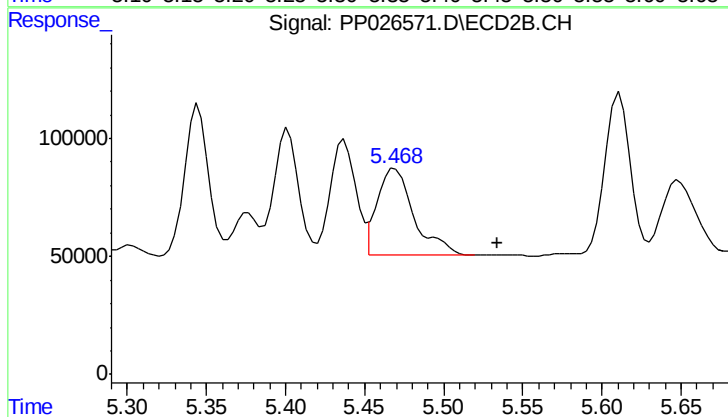

#14 Aroclor-1232-4


R.T.: 5.469 min
Delta R.T.: -0.064 min
Response: 596320
Conc: 283.29 ng/ml

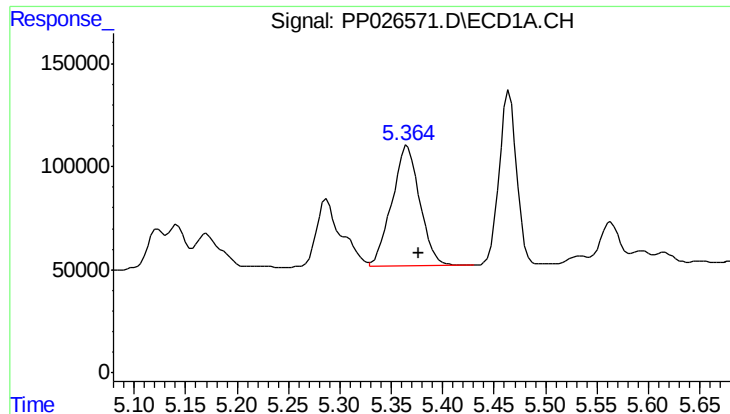

#15 Aroclor-1232-5


R.T.: 5.366 min
Delta R.T.: -0.010 min
Response: 1104933
Conc: 1288.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

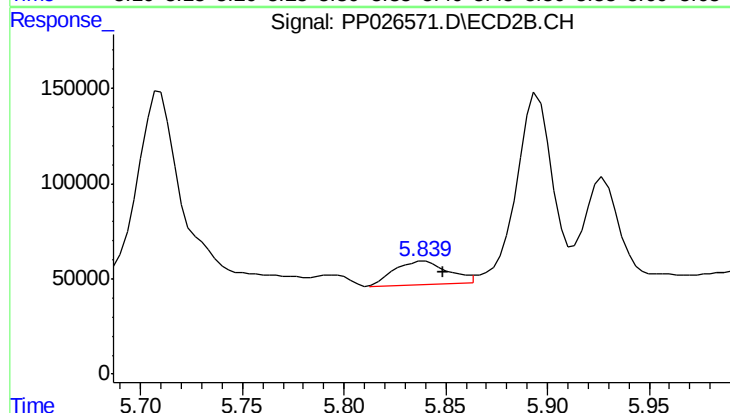


#15 Aroclor-1232-5

R.T.: 5.840 min
Delta R.T.: -0.009 min
Response: 214708
Conc: 88.47 ng/ml

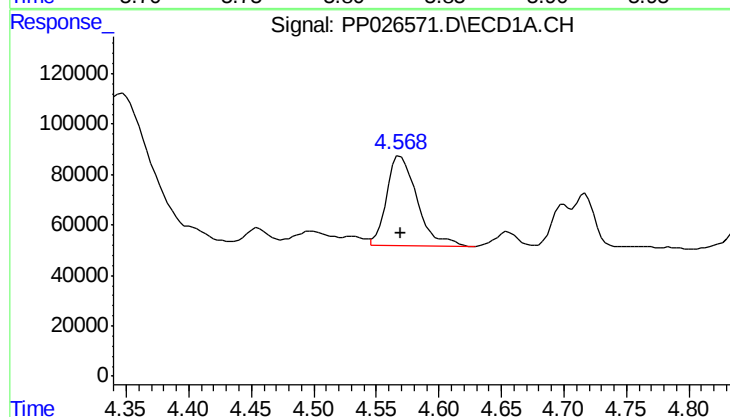


#16 Aroclor-1242-1

R.T.: 4.569 min
Delta R.T.: 0.000 min
Response: 604277
Conc: 294.40 ng/ml

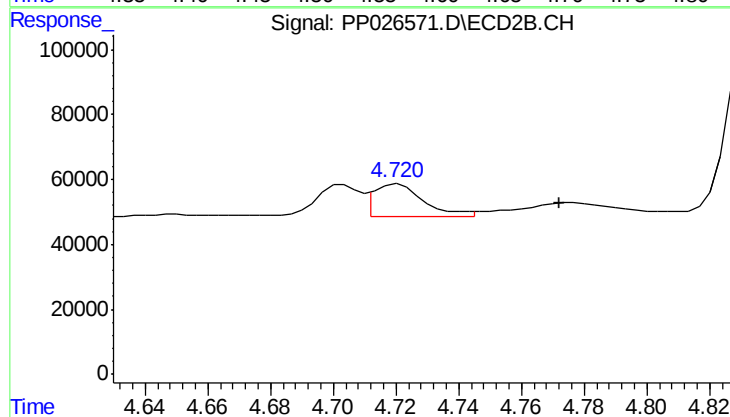

#16 Aroclor-1242-1


R.T.: 4.721 min
Delta R.T.: -0.051 min
Response: 110754
Conc: 18.15 ng/ml

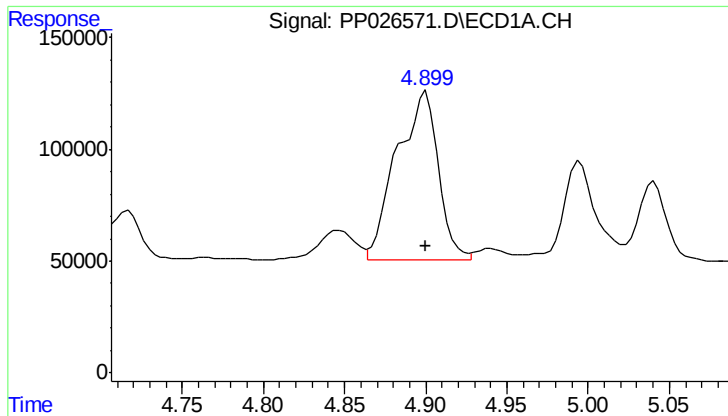

#17 Aroclor-1242-2


R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 1339221
Conc: 291.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

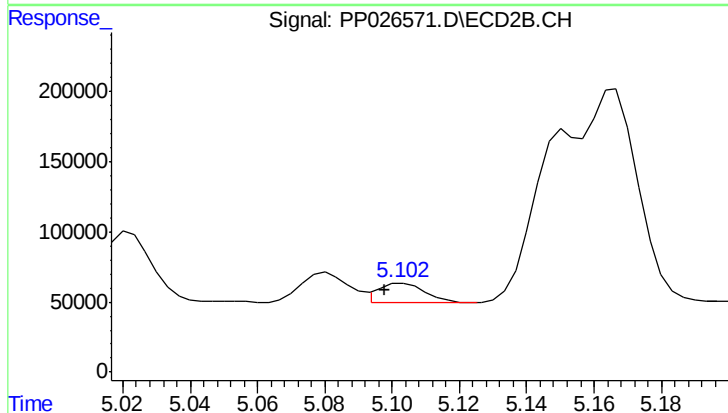


#17 Aroclor-1242-2

R.T.: 5.104 min
Delta R.T.: 0.006 min
Response: 137988
Conc: 18.22 ng/ml

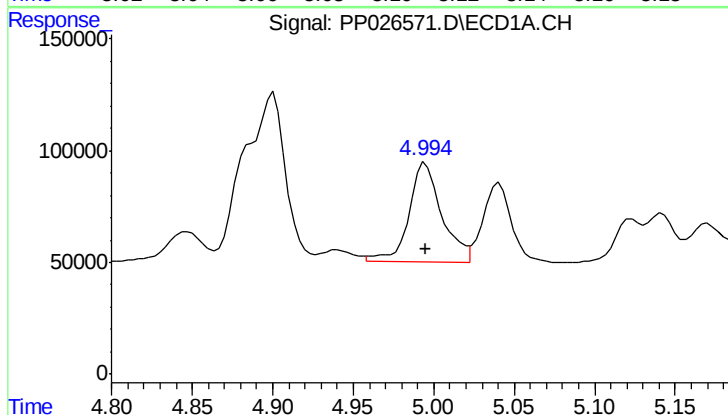


#18 Aroclor-1242-3

R.T.: 4.995 min
Delta R.T.: 0.000 min
Response: 633287
Conc: 295.23 ng/ml

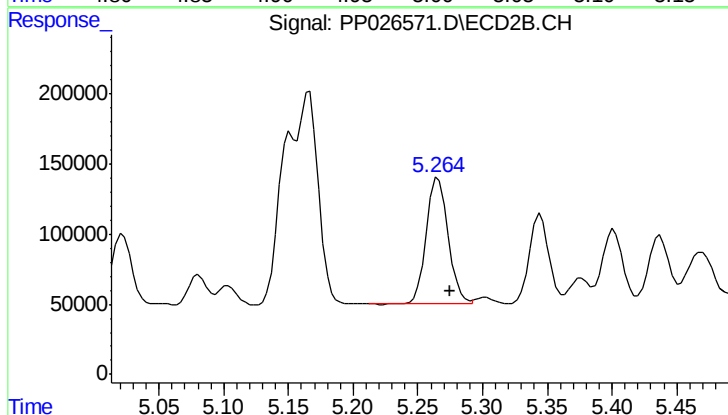

#18 Aroclor-1242-3


R.T.: 5.266 min
Delta R.T.: -0.009 min
Response: 1054605
Conc: 350.28 ng/ml

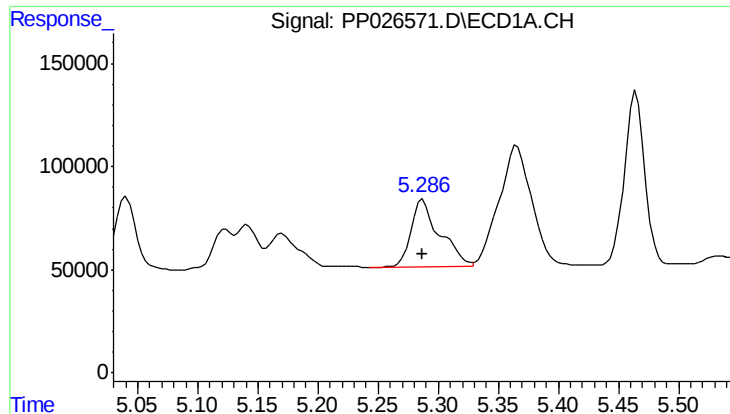

#19 Aroclor-1242-4


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 545404
Conc: 267.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

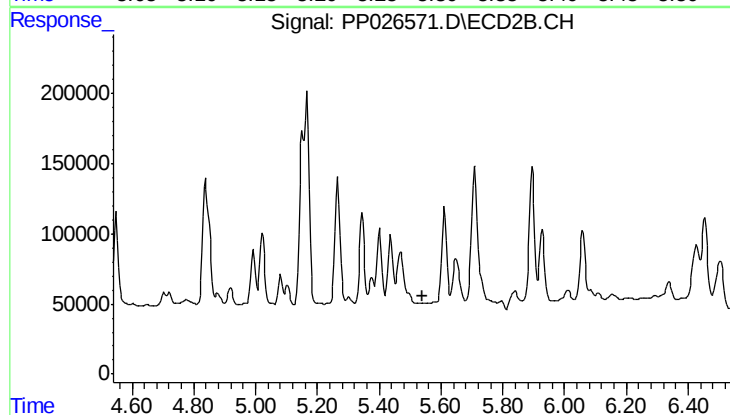


#19 Aroclor-1242-4

R.T.: 0.000 min
Exp R.T.: 5.539 min
Response: 0
Conc: N.D.

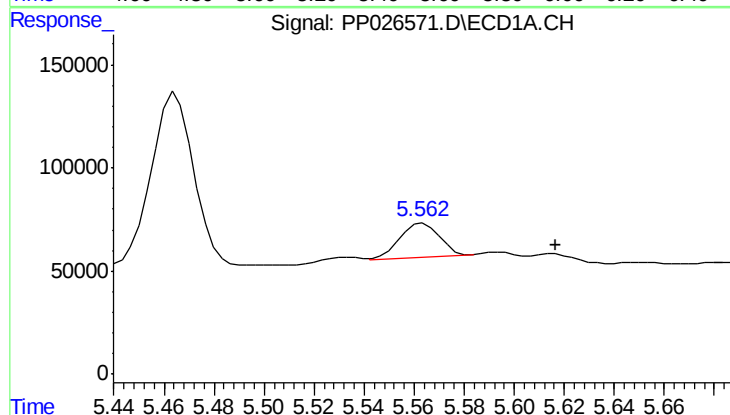


#20 Aroclor-1242-5

R.T.: 5.564 min
Delta R.T.: -0.053 min
Response: 184758
Conc: 103.97 ng/ml

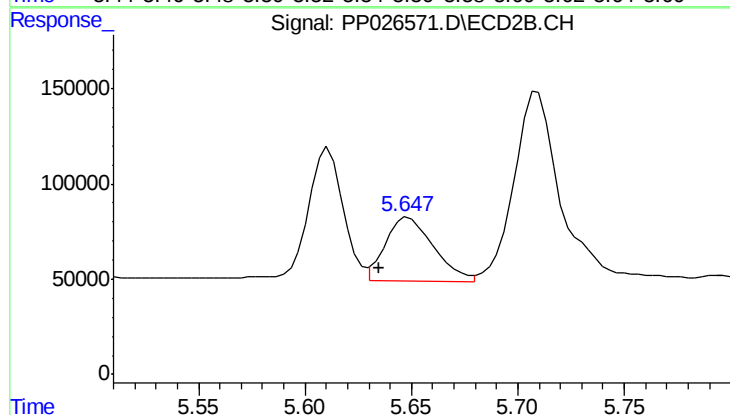

#20 Aroclor-1242-5


R.T.: 5.648 min
Delta R.T.: 0.014 min
Response: 534902
Conc: 111.06 ng/ml

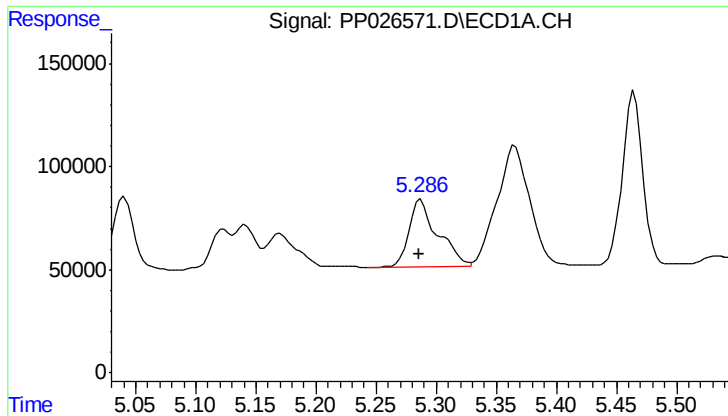

#21 Aroclor-1248-1


R.T.: 5.287 min
Delta R.T.: 0.001 min
Response: 545404
Conc: 160.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

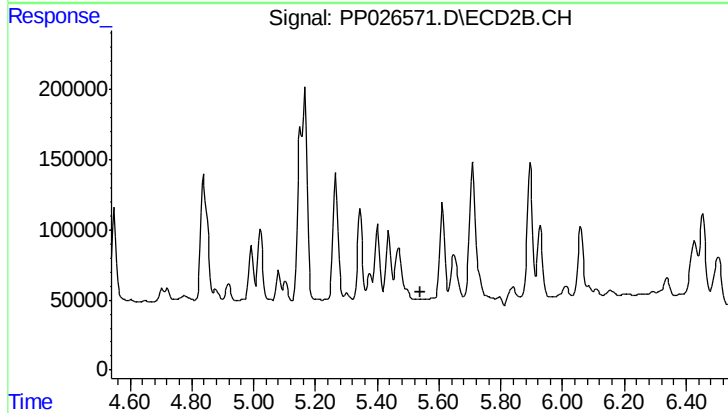


#21 Aroclor-1248-1

R.T.: 0.000 min
Exp R.T.: 5.540 min
Response: 0
Conc: N.D.

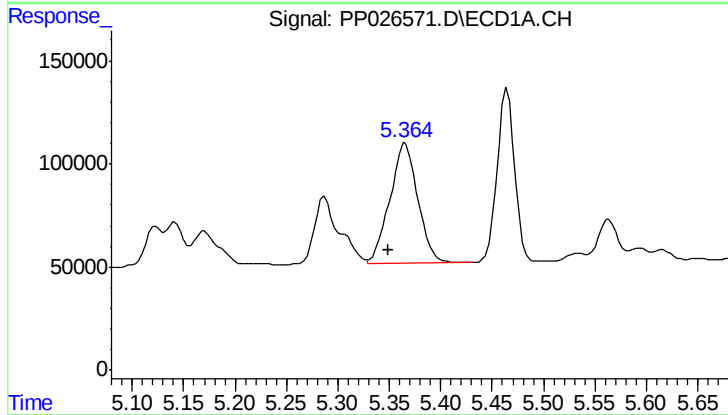


#22 Aroclor-1248-2

R.T.: 5.366 min
Delta R.T.: 0.016 min
Response: 1104933
Conc: 573.84 ng/ml

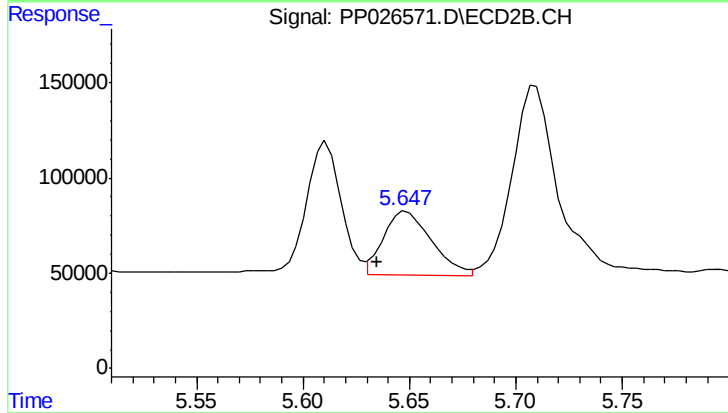

#22 Aroclor-1248-2


R.T.: 5.648 min
Delta R.T.: 0.014 min
Response: 534902
Conc: 73.49 ng/ml

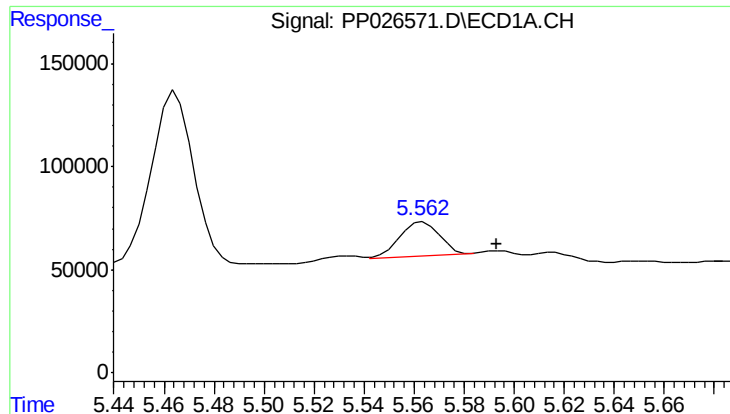

#23 Aroclor-1248-3


R.T.: 5.564 min
Delta R.T.: -0.030 min
Response: 184758
Conc: 61.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

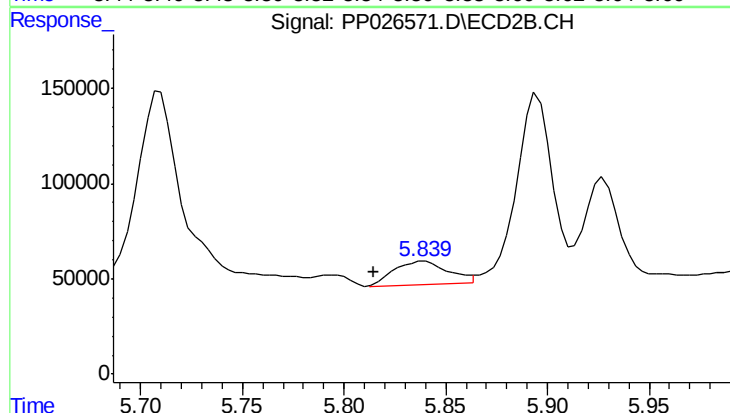


#23 Aroclor-1248-3

R.T.: 5.840 min
Delta R.T.: 0.025 min
Response: 214708
Conc: 30.53 ng/ml

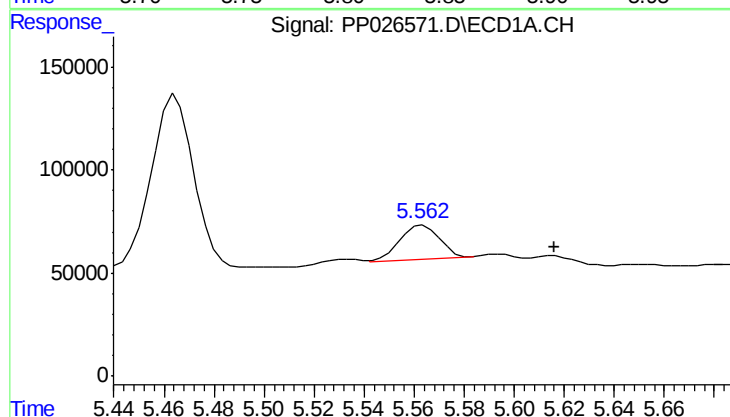


#24 Aroclor-1248-4

R.T.: 5.564 min
Delta R.T.: -0.052 min
Response: 184758
Conc: 59.90 ng/ml

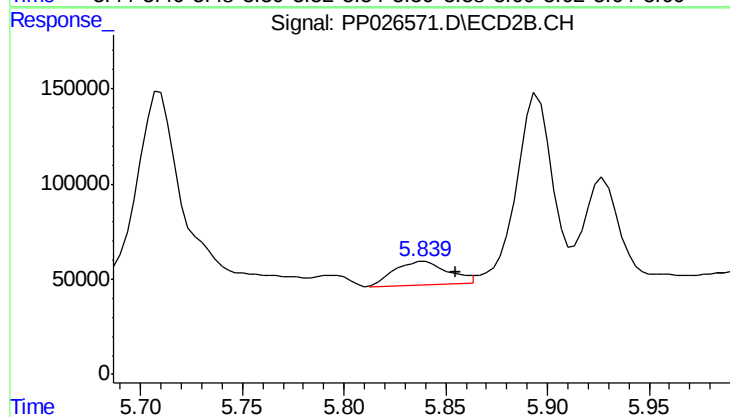

#24 Aroclor-1248-4


R.T.: 5.840 min
Delta R.T.: -0.015 min
Response: 214708
Conc: 27.11 ng/ml

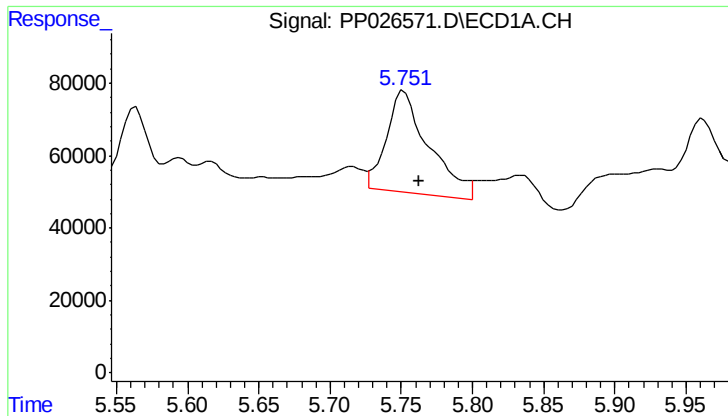

#25 Aroclor-1248-5


R.T.: 5.752 min
Delta R.T.: -0.011 min
Response: 579073
Conc: 196.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

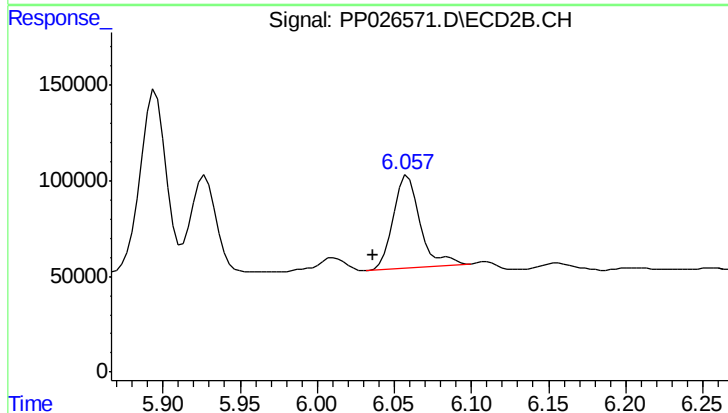


#25 Aroclor-1248-5

R.T.: 6.059 min
Delta R.T.: 0.023 min
Response: 592985
Conc: 80.24 ng/ml

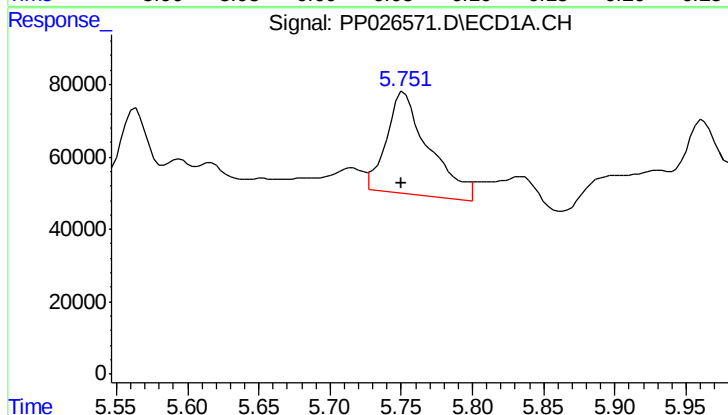


#26 Aroclor-1254-1

R.T.: 5.752 min
Delta R.T.: 0.002 min
Response: 579073
Conc: 125.56 ng/ml

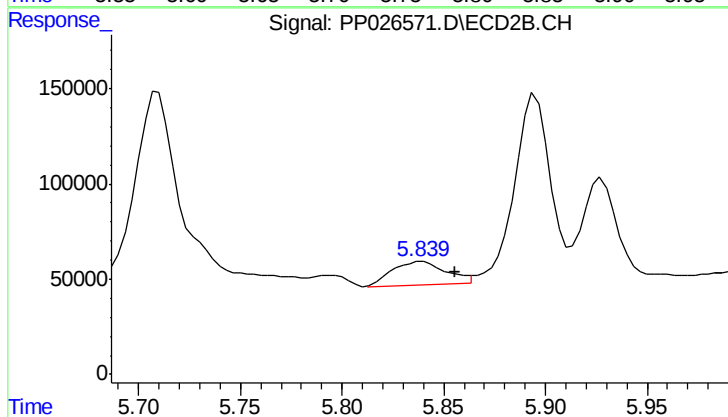

#26 Aroclor-1254-1


R.T.: 5.840 min
Delta R.T.: -0.015 min
Response: 214708
Conc: 29.47 ng/ml

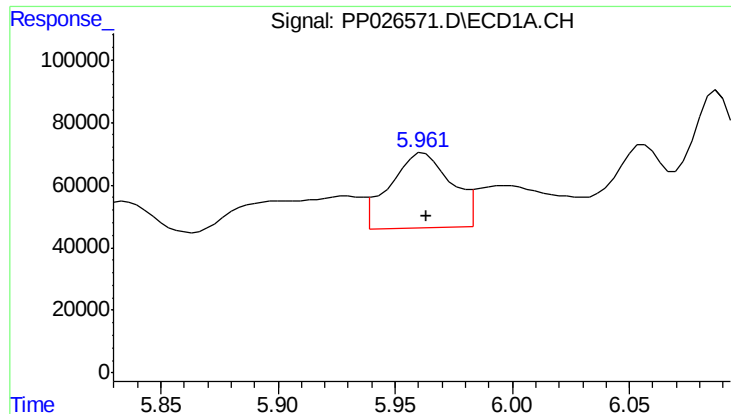

#27 Aroclor-1254-2


R.T.: 5.962 min
Delta R.T.: -0.001 min
Response: 438058
Conc: 131.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

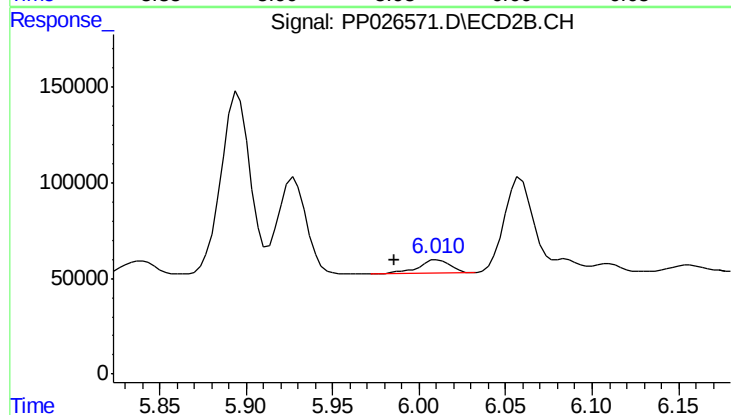


#27 Aroclor-1254-2

R.T.: 6.011 min
Delta R.T.: 0.025 min
Response: 88810
Conc: 11.46 ng/ml

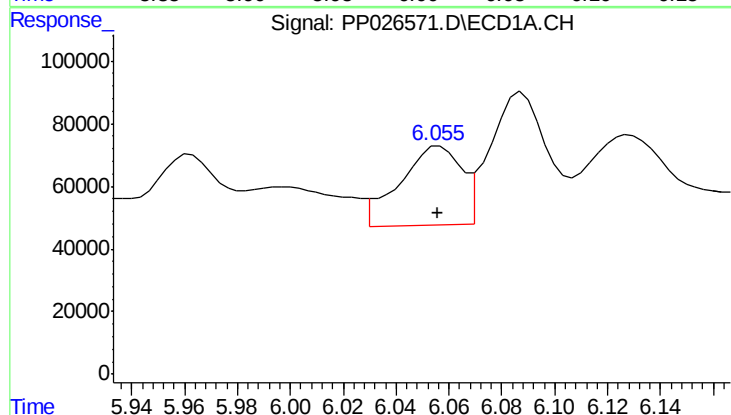


#28 Aroclor-1254-3

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 408162
Conc: 67.27 ng/ml

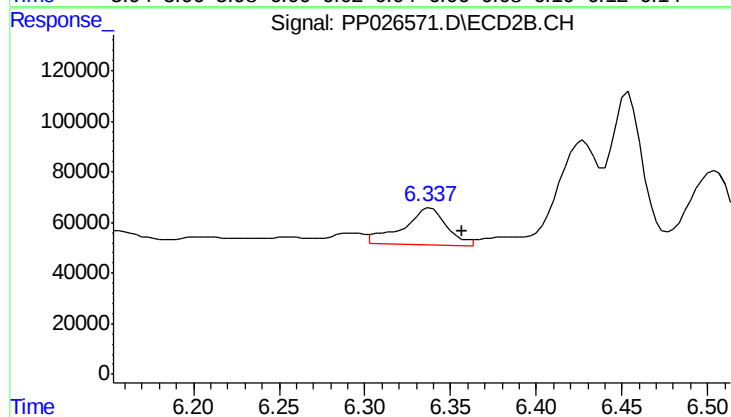

#28 Aroclor-1254-3


R.T.: 6.338 min
Delta R.T.: -0.019 min
Response: 261882
Conc: 20.18 ng/ml

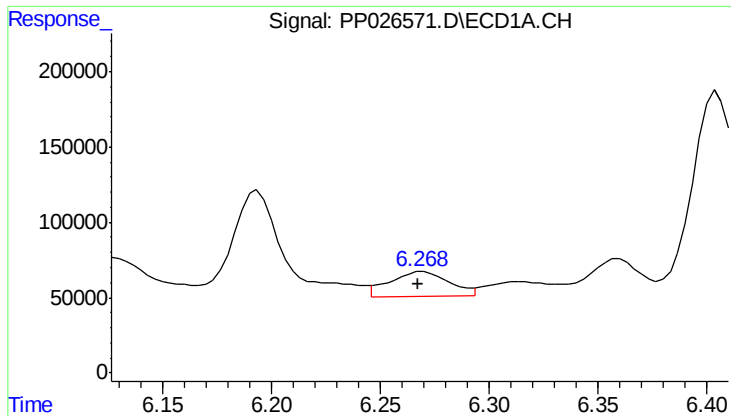

#29 Aroclor-1254-4


R.T.: 6.269 min
Delta R.T.: 0.002 min
Response: 320565
Conc: 54.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

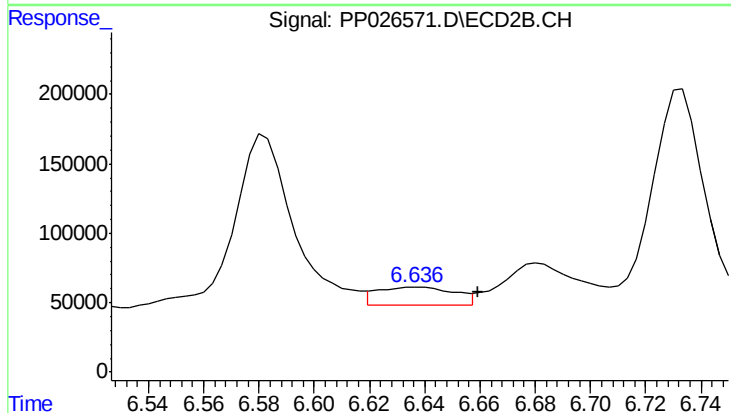


#29 Aroclor-1254-4

R.T.: 6.638 min
Delta R.T.: -0.022 min
Response: 251055
Conc: 48.75 ng/ml

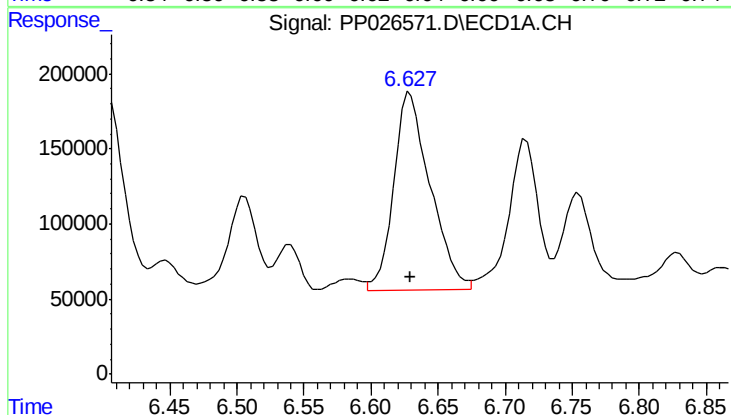


#30 Aroclor-1254-5

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 2505911
Conc: 329.75 ng/ml

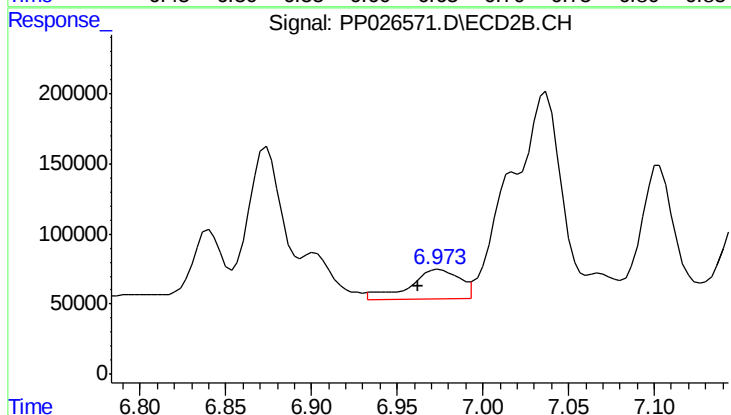

#30 Aroclor-1254-5


R.T.: 6.975 min
Delta R.T.: 0.012 min
Response: 425534
Conc: 39.42 ng/ml

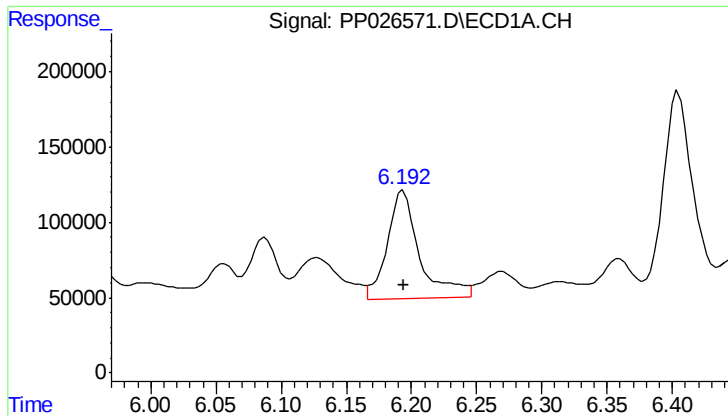

#31 Aroclor-1260-1


R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 1235604
Conc: 342.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

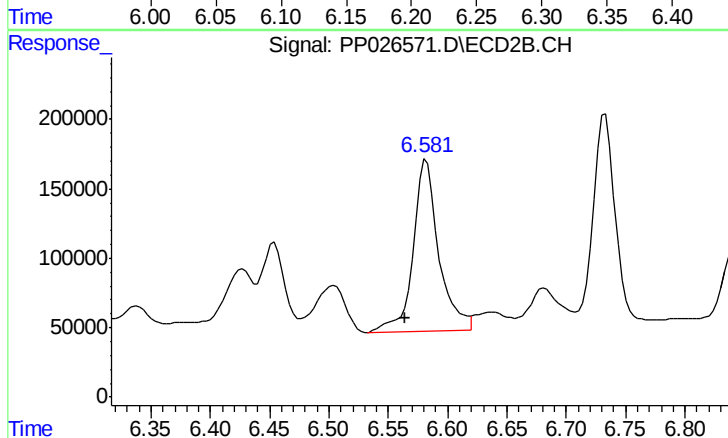


#31 Aroclor-1260-1

R.T.: 6.582 min
Delta R.T.: 0.018 min
Response: 1871982
Conc: 234.37 ng/ml

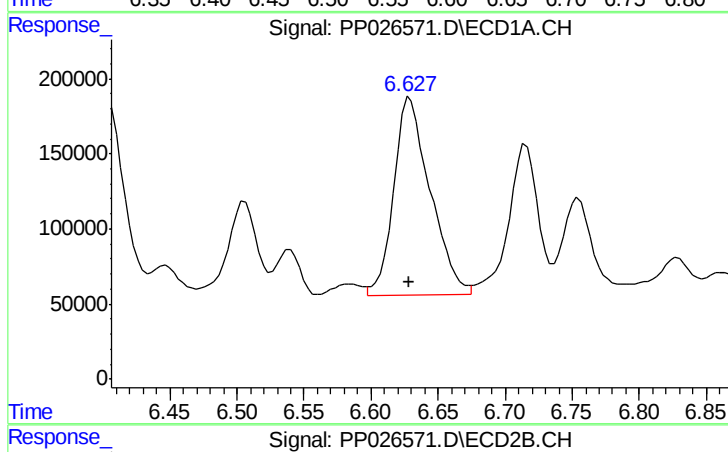


#32 Aroclor-1260-2

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 2505911
Conc: 270.20 ng/ml

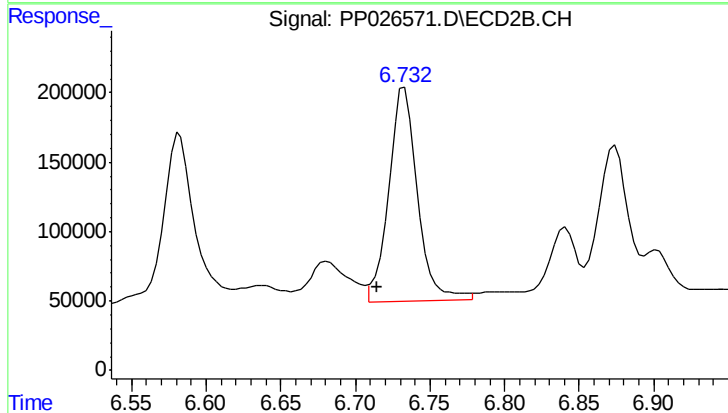

#32 Aroclor-1260-2


R.T.: 6.733 min
Delta R.T.: 0.019 min
Response: 2082002
Conc: 229.59 ng/ml

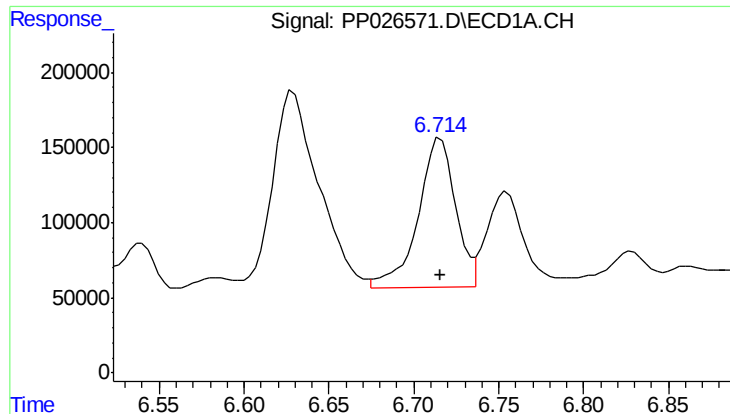

#33 Aroclor-1260-3


R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 1525363
Conc: 229.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

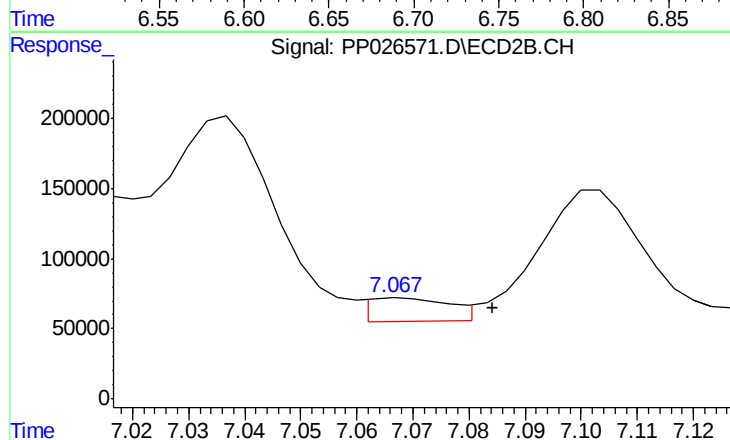


#33 Aroclor-1260-3

R.T.: 7.068 min
Delta R.T.: -0.016 min
Response: 165946
Conc: 26.16 ng/ml

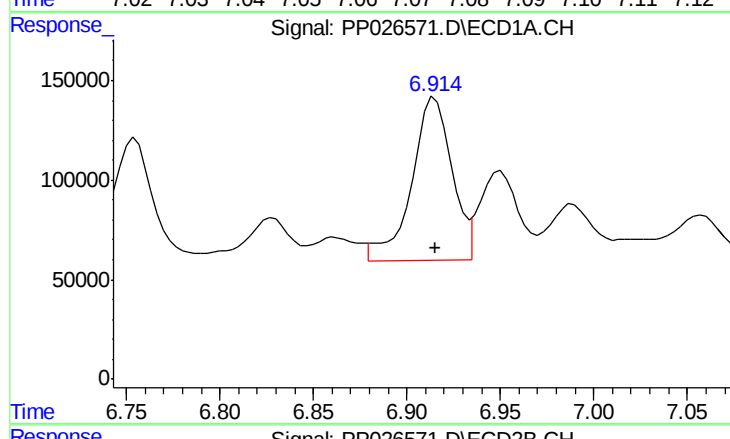


#34 Aroclor-1260-4

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 1234767
Conc: 236.43 ng/ml

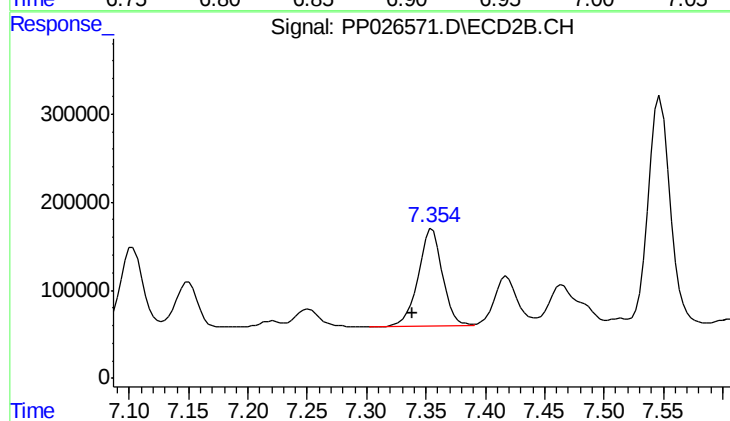

#34 Aroclor-1260-4


R.T.: 7.356 min
Delta R.T.: 0.017 min
Response: 1570072
Conc: 214.11 ng/ml

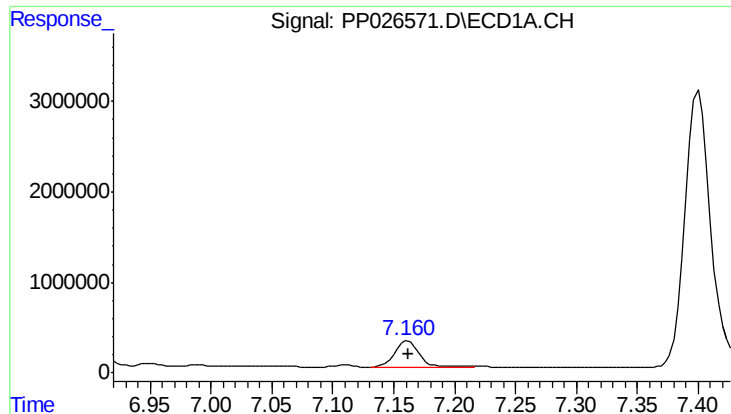

#35 Aroclor-1260-5


R.T.: 7.162 min
Delta R.T.: 0.000 min
Response: 4177902
Conc: 220.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

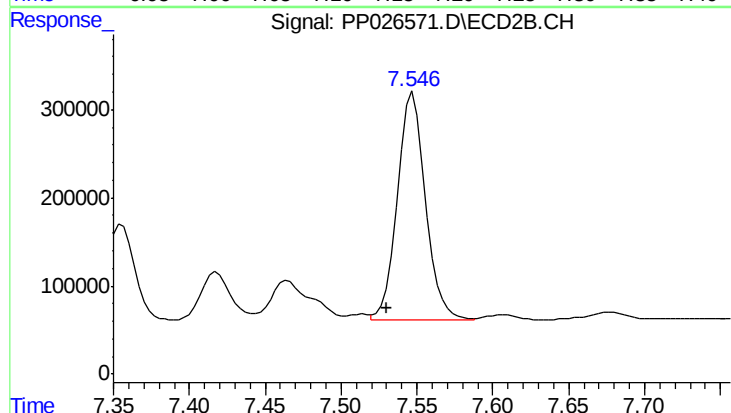


#35 Aroclor-1260-5

R.T.: 7.547 min
Delta R.T.: 0.017 min
Response: 3313769
Conc: 206.56 ng/ml

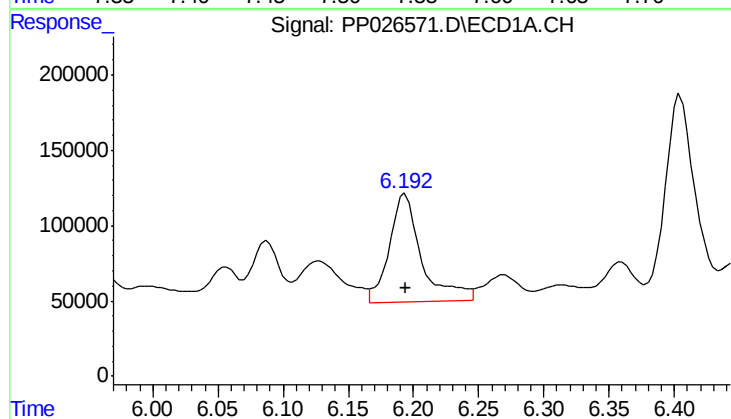


#36 Aroclor-1262-1

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 1235604
Conc: 370.85 ng/ml

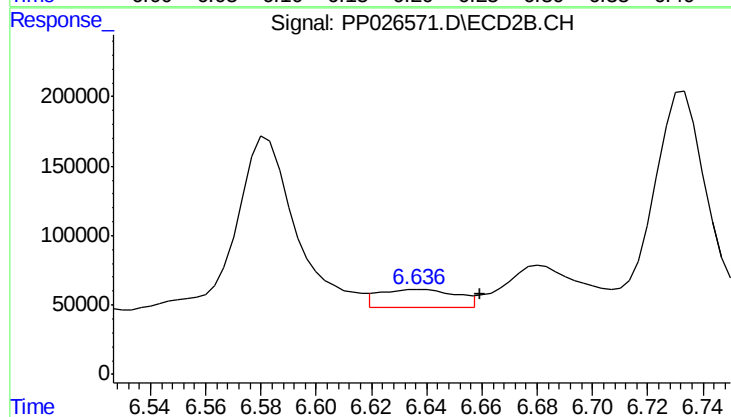

#36 Aroclor-1262-1


R.T.: 6.638 min
Delta R.T.: -0.022 min
Response: 251055
Conc: 30.80 ng/ml

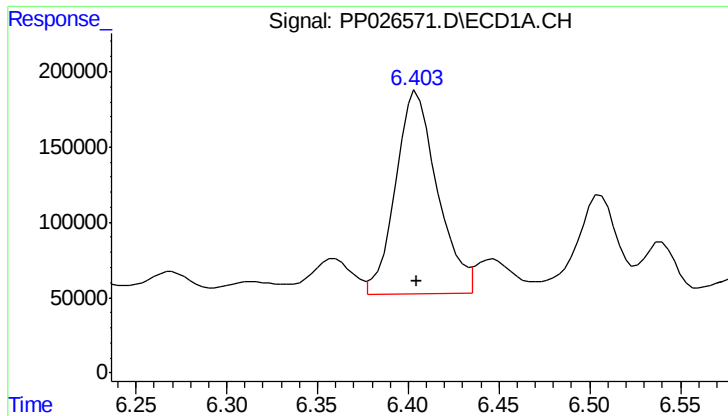

#37 Aroclor-1262-2


R.T.: 6.405 min
Delta R.T.: 0.000 min
Response: 2159931
Conc: 321.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

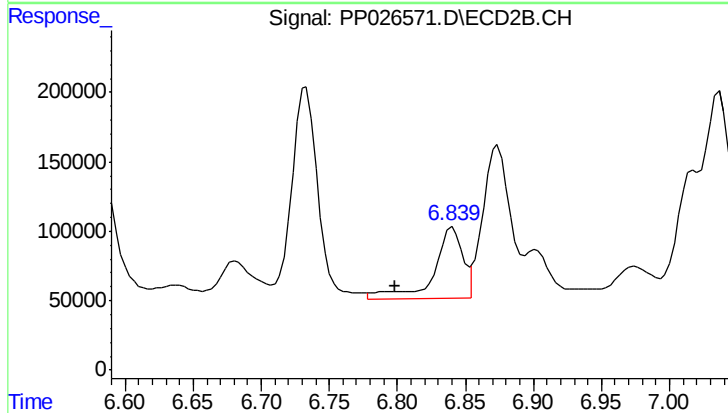


#37 Aroclor-1262-2

R.T.: 6.841 min
Delta R.T.: 0.042 min
Response: 764183
Conc: 162.32 ng/ml

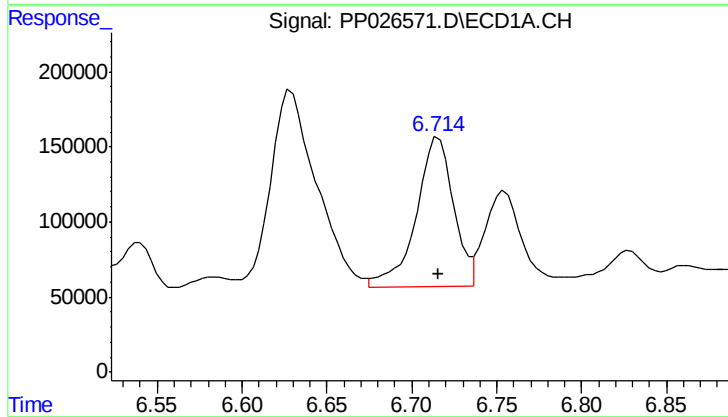


#38 Aroclor-1262-3

R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 1525363
Conc: 131.83 ng/ml

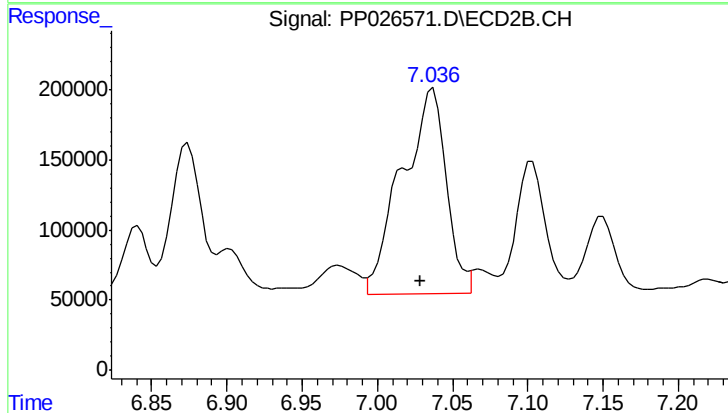

#38 Aroclor-1262-3


R.T.: 7.037 min
Delta R.T.: 0.008 min
Response: 2977190
Conc: 270.05 ng/ml

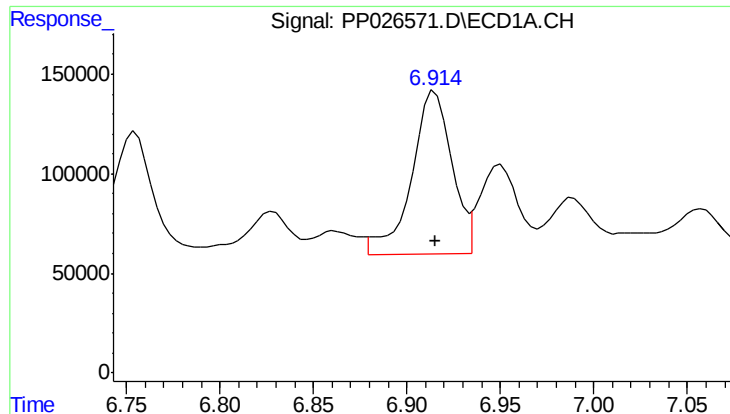

#39 Aroclor-1262-4


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 1234767
Conc: 152.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

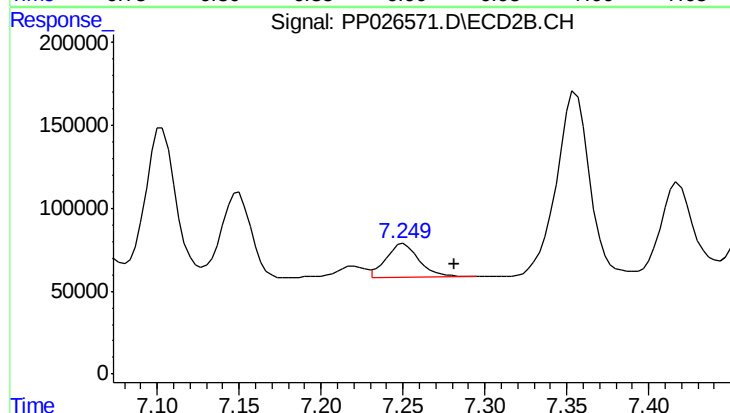


#39 Aroclor-1262-4

R.T.: 7.251 min
Delta R.T.: -0.031 min
Response: 289362
Conc: 28.95 ng/ml

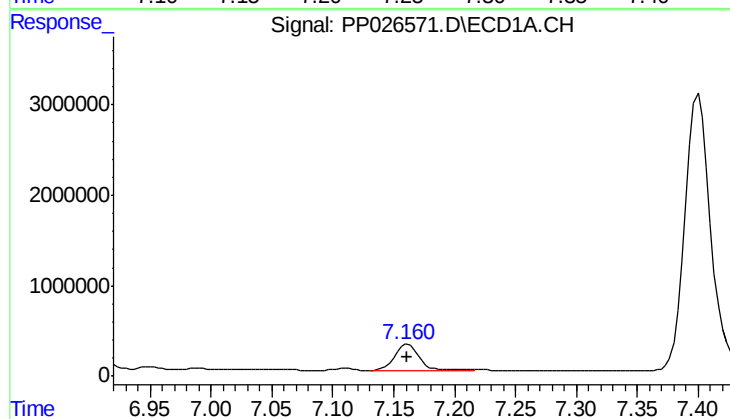


#40 Aroclor-1262-5

R.T.: 7.162 min
Delta R.T.: 0.000 min
Response: 4177902
Conc: 157.98 ng/ml

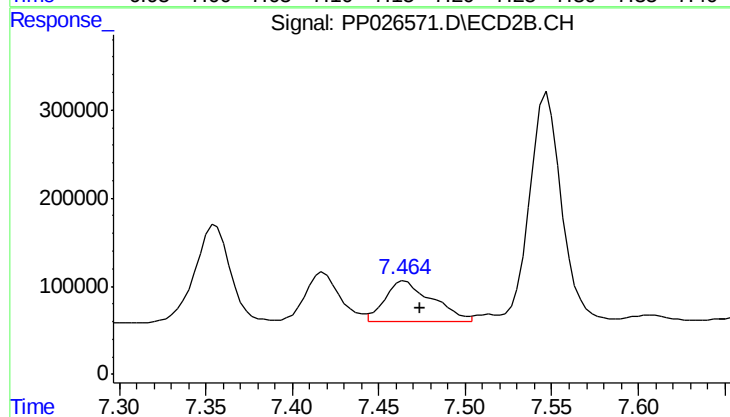

#40 Aroclor-1262-5


R.T.: 7.465 min
Delta R.T.: -0.009 min
Response: 865656
Conc: 41.09 ng/ml

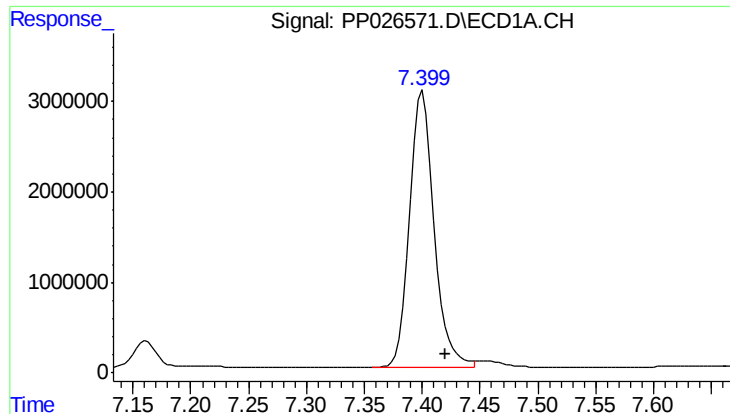

#41 Aroclor-1268-1


R.T.: 7.400 min
Delta R.T.: -0.020 min
Response: 45128363
Conc: 1662.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

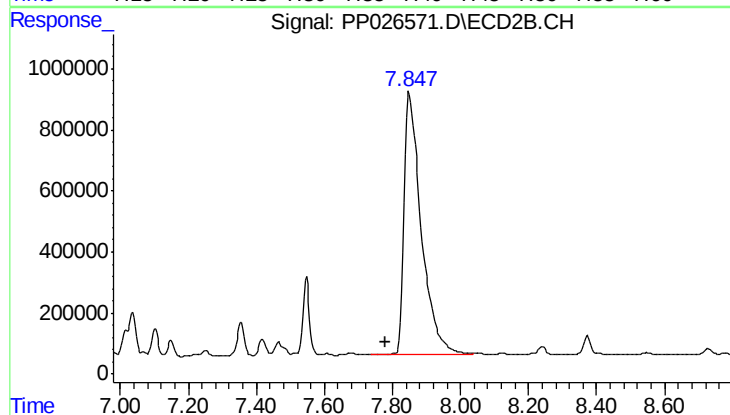


#41 Aroclor-1268-1

R.T.: 7.849 min
Delta R.T.: 0.070 min
Response: 30586937
Conc: 1485.50 ng/ml

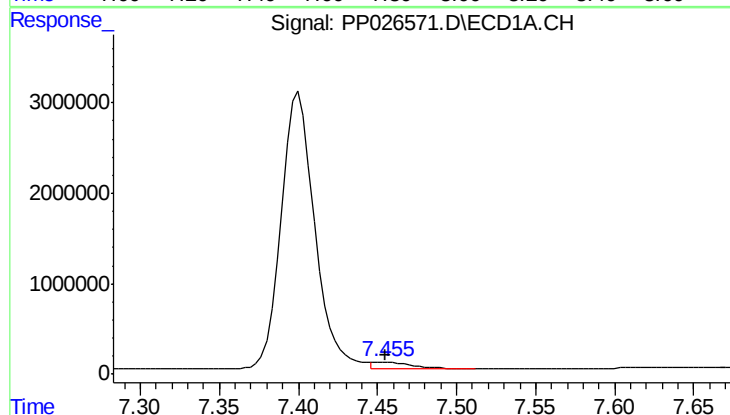


#42 Aroclor-1268-2

R.T.: 7.456 min
Delta R.T.: 0.001 min
Response: 1106491
Conc: 53.56 ng/ml

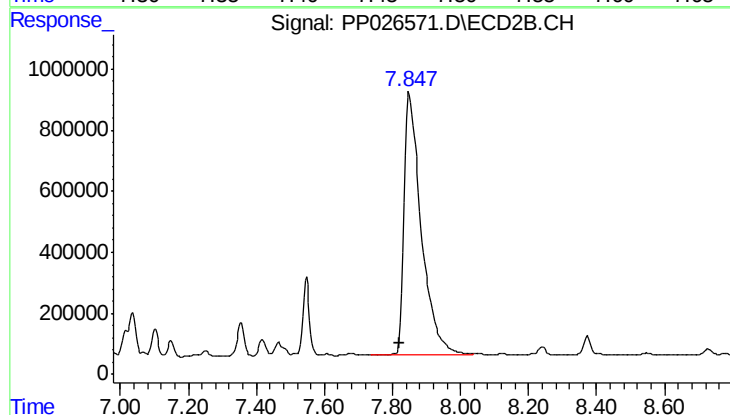

#42 Aroclor-1268-2


R.T.: 7.849 min
Delta R.T.: 0.030 min
Response: 30586937
Conc: 1628.40 ng/ml

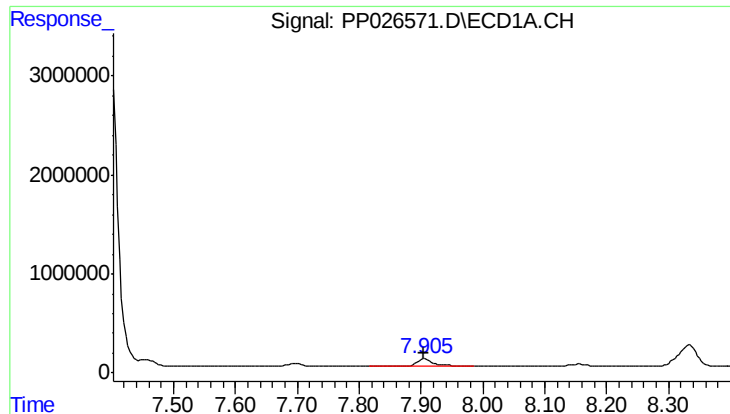

#44 Aroclor-1268-4


R.T.: 7.906 min
Delta R.T.: 0.002 min
Response: 1258308
Conc: 152.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB110361BS

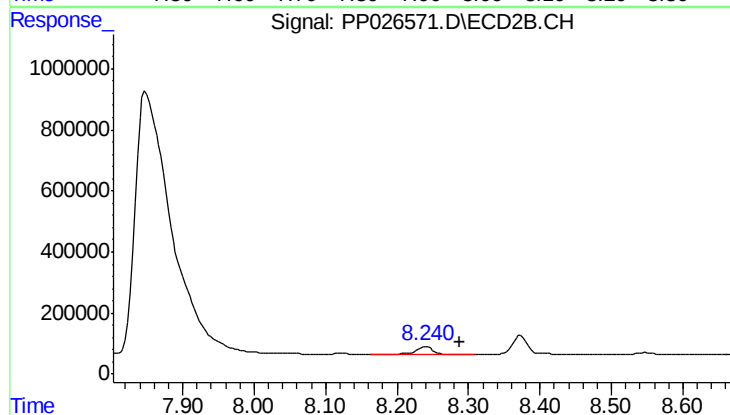


#44 Aroclor-1268-4

R.T.: 8.241 min
Delta R.T.: -0.047 min
Response: 447334
Conc: 60.33 ng/ml

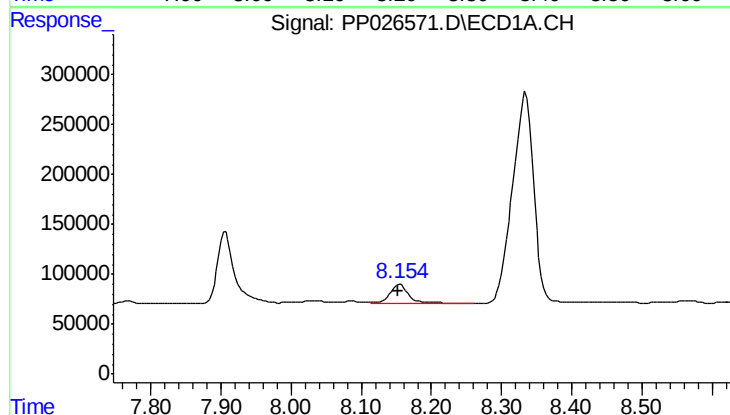

#45 Aroclor-1268-5

R.T.: 8.155 min
Delta R.T.: 0.003 min
Response: 384519
Conc: 6.42 ng/ml

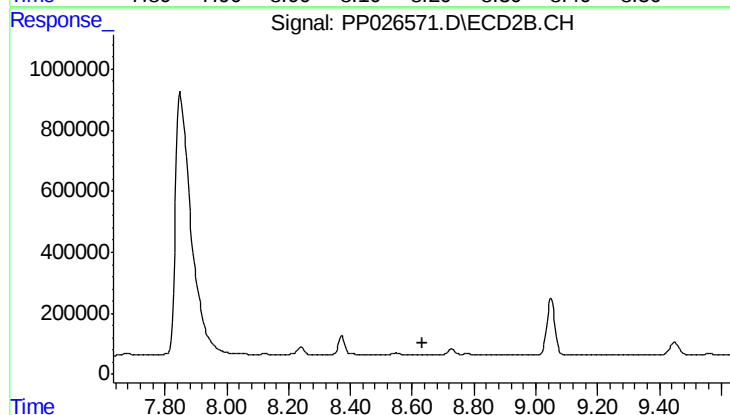

#45 Aroclor-1268-5

R.T.: 0.000 min
Exp R.T.: 8.633 min
Response: 0
Conc: N.D.